

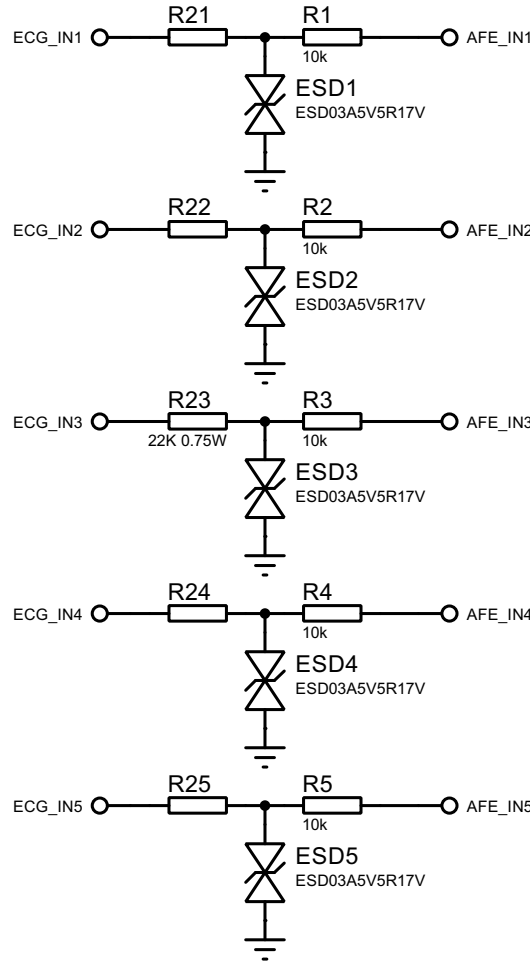
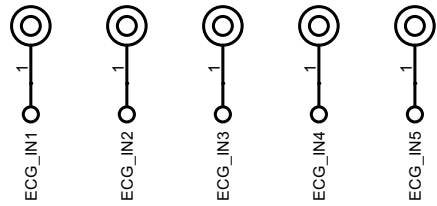
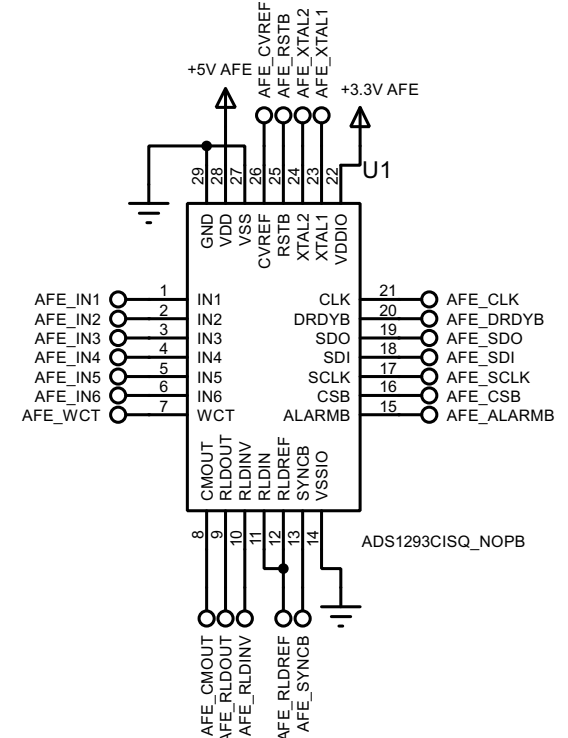
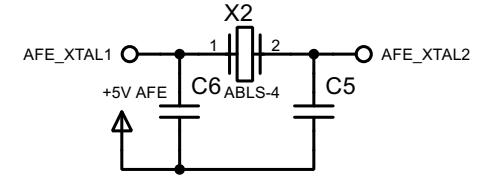




ECG1 ECG2 ECG3 ECG4 ECG5
DIN 42802-1 DIN 42802-1 DIN 42802-1 DIN 42802-1 DIN 42802-1

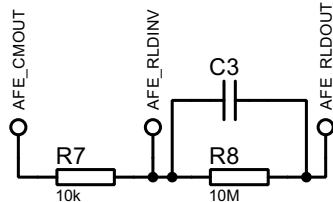


+3.3V AFE +3.3V AFE











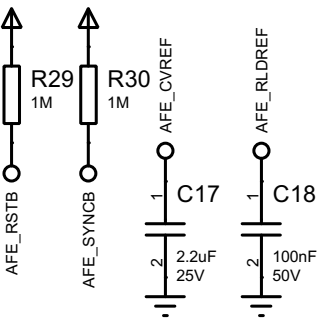


FILE NAME: ECG V1.2.pdsprj	DATE: 30.01.2024
DESIGN TITLE: EKG HOLTER	1 of 4
PATH: G:\shortcut-targets-by-id\1fucBpxm90IWcgJ4rMBWJLJuleAltK	TIME: 03:20:54
BY: Muhammed Güler	REV: 1.2
BOARD: @BOARD	

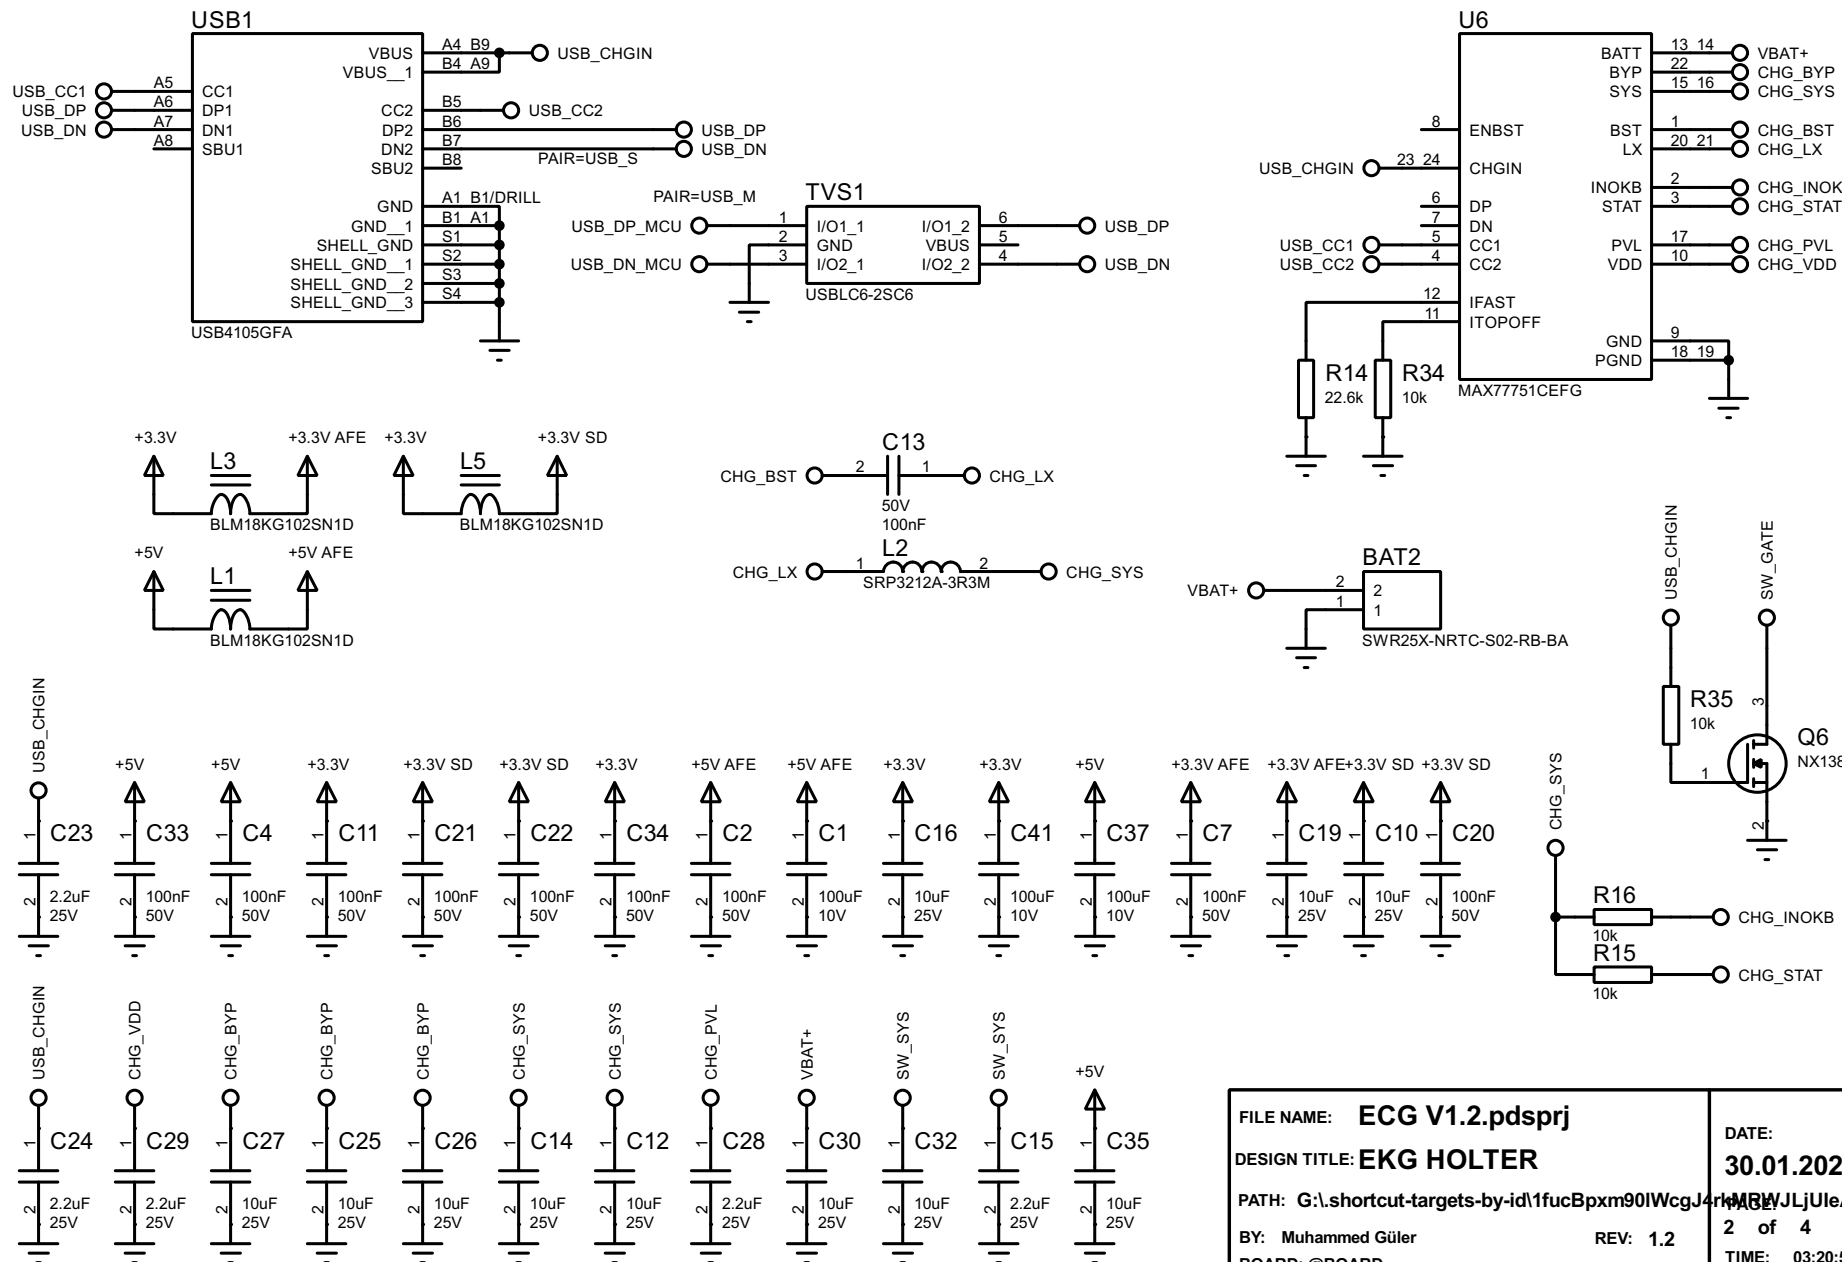

FILE NAME:	ECG V1.2.pdsprj
DESIGN TITLE:	EKG HOLTER
PATH:	G:\shortcut-targets-by-id\1fucBpxm90IWcgJ4rkMBWJLjUleAlrK
BY:	Muhammed Güler
BOARD:	@BOARD
DATE:	30.01.2024
REV:	1.2
TIME:	03:20:54

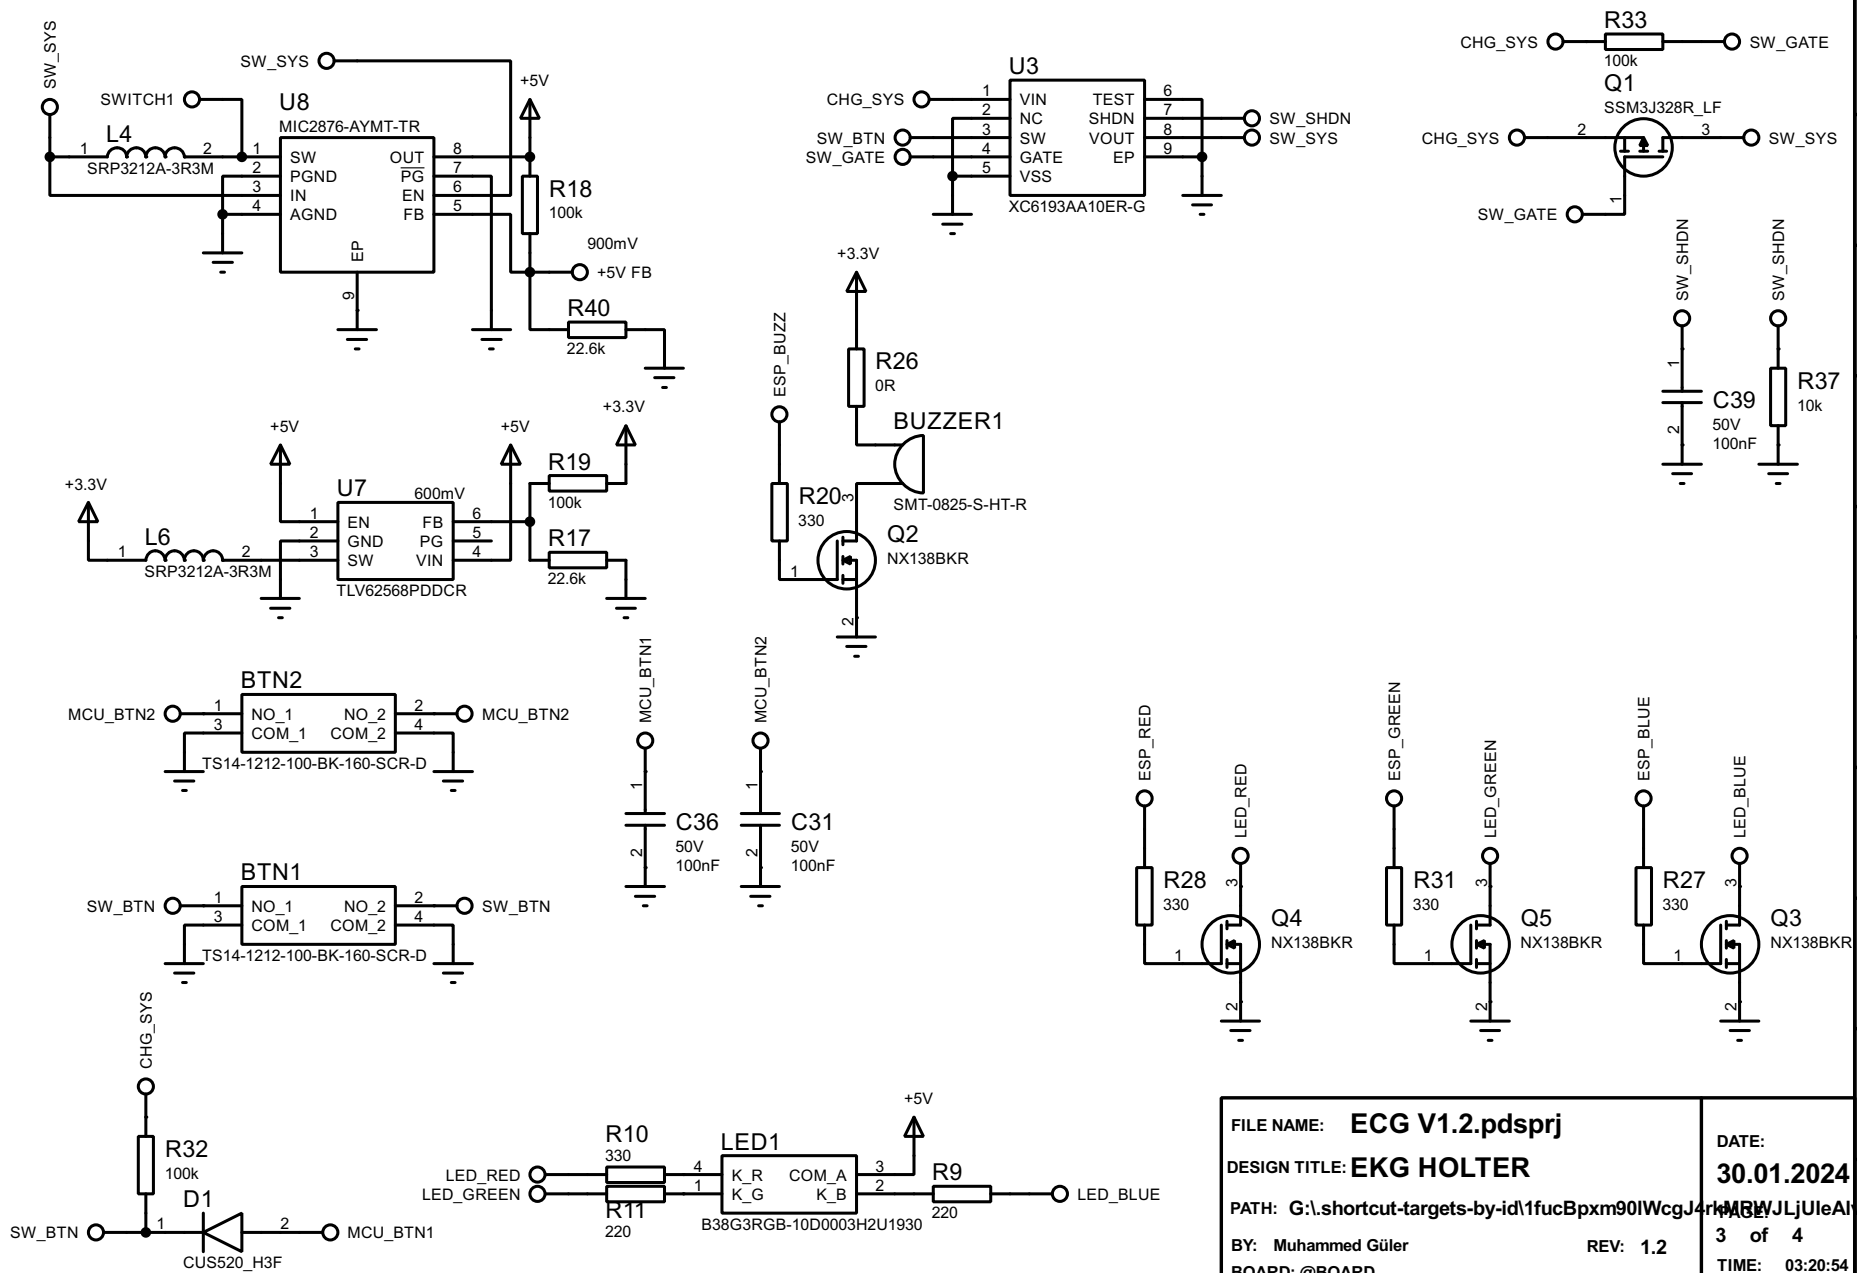

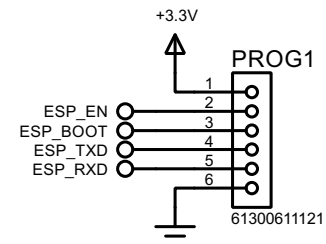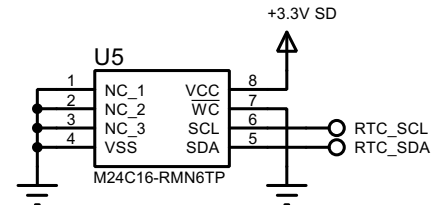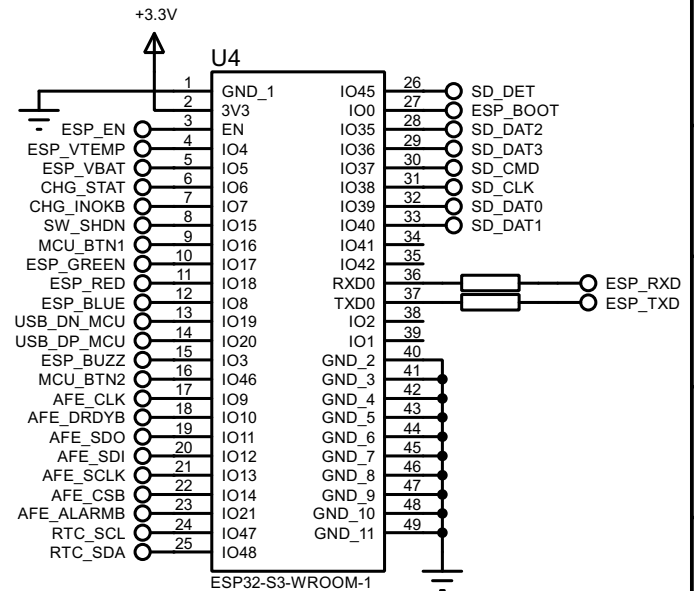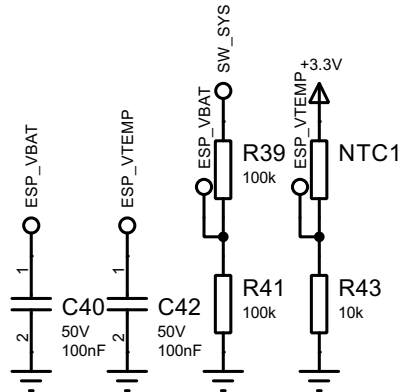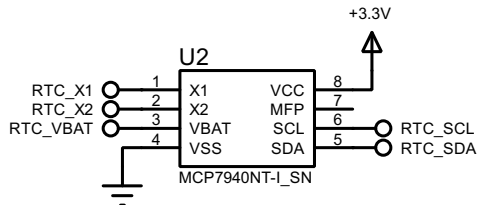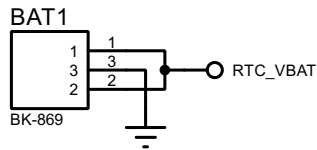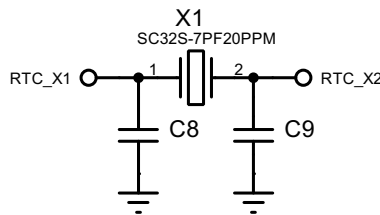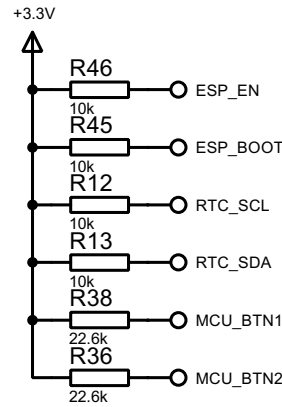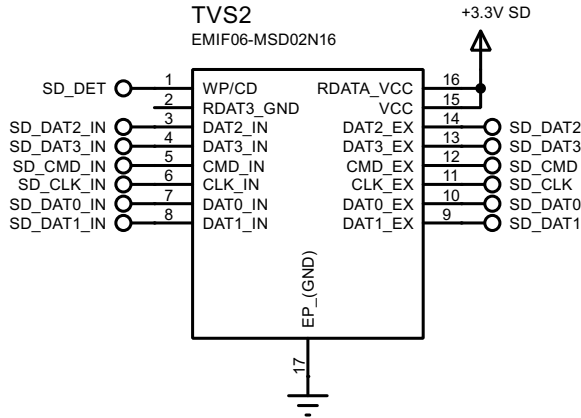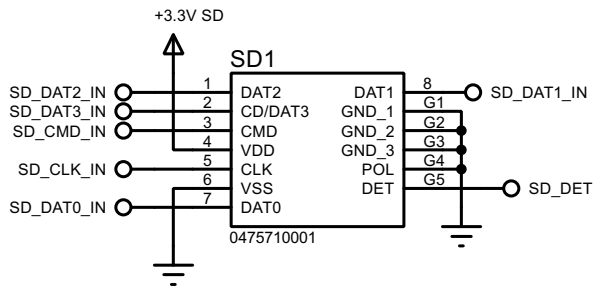

FILE NAME: ECG V1.2.pdsprj	DATE: 30.01.2024
DESIGN TITLE: EKG HOLTER	4 of 4
PATH: G:\shortcut-targets-by-id\1fucBpxm90IWcgJ4rkMBWJLjUleAlvtK	TIME: 03:20:54
BY: Muhammed Güler	REV: 1.2
BOARD: @BOARD	