



(a) Physical zero and measurement tolerance remain distinct



(b) Monthly zero-point stability

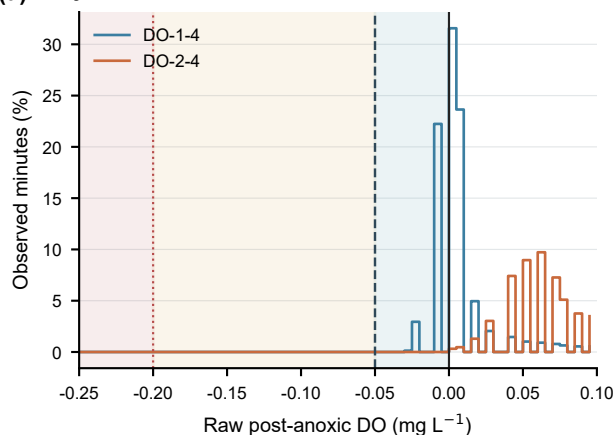

(c) Parallel post-anoxic distributions are non-exchangeable

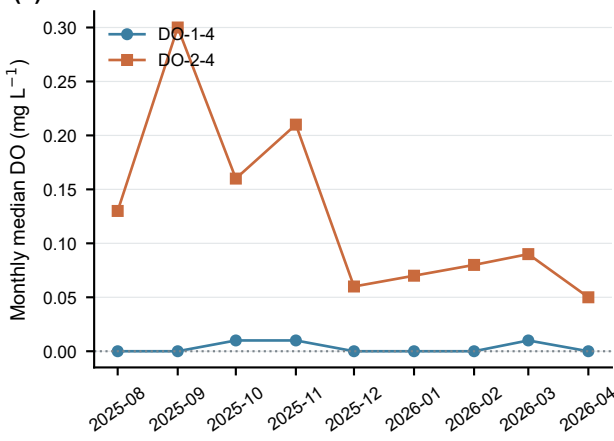

(d) Time-blocked upper-template support

