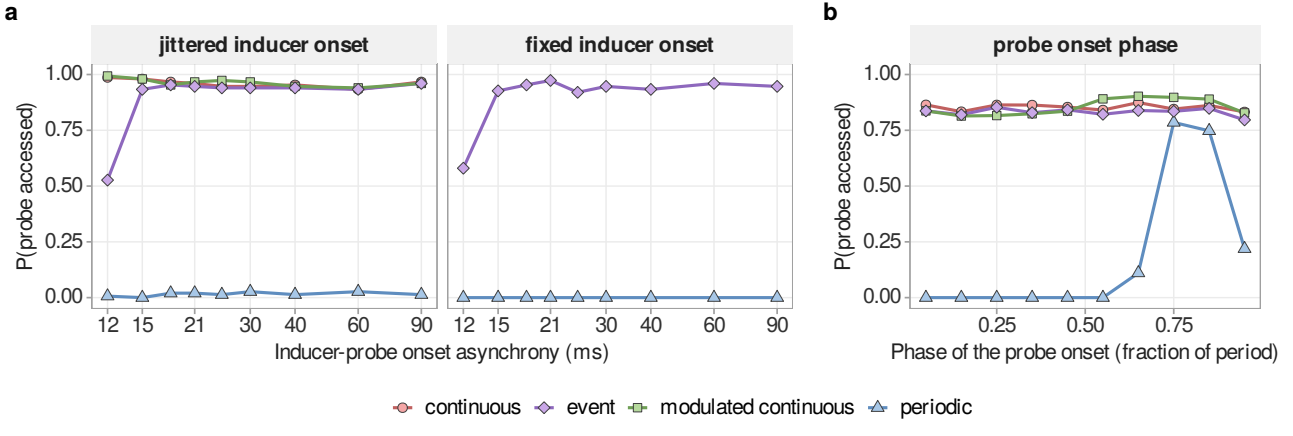
a
jittered inducer onset
fixed inducer onset
P(probe accessed)
1.00
0.75
0.50
0.25
0.00
12 15 21 30 40 60 90
12 15 21 30 40 60 90
Inducer-probe onset asynchrony (ms)
b
probe onset phase
P(probe accessed)
1.00
0.75
0.50
0.25
0.00
0.25 0.50 0.75
Phase of the probe onset (fraction of period)
continuous
event
modulated continuous
periodic