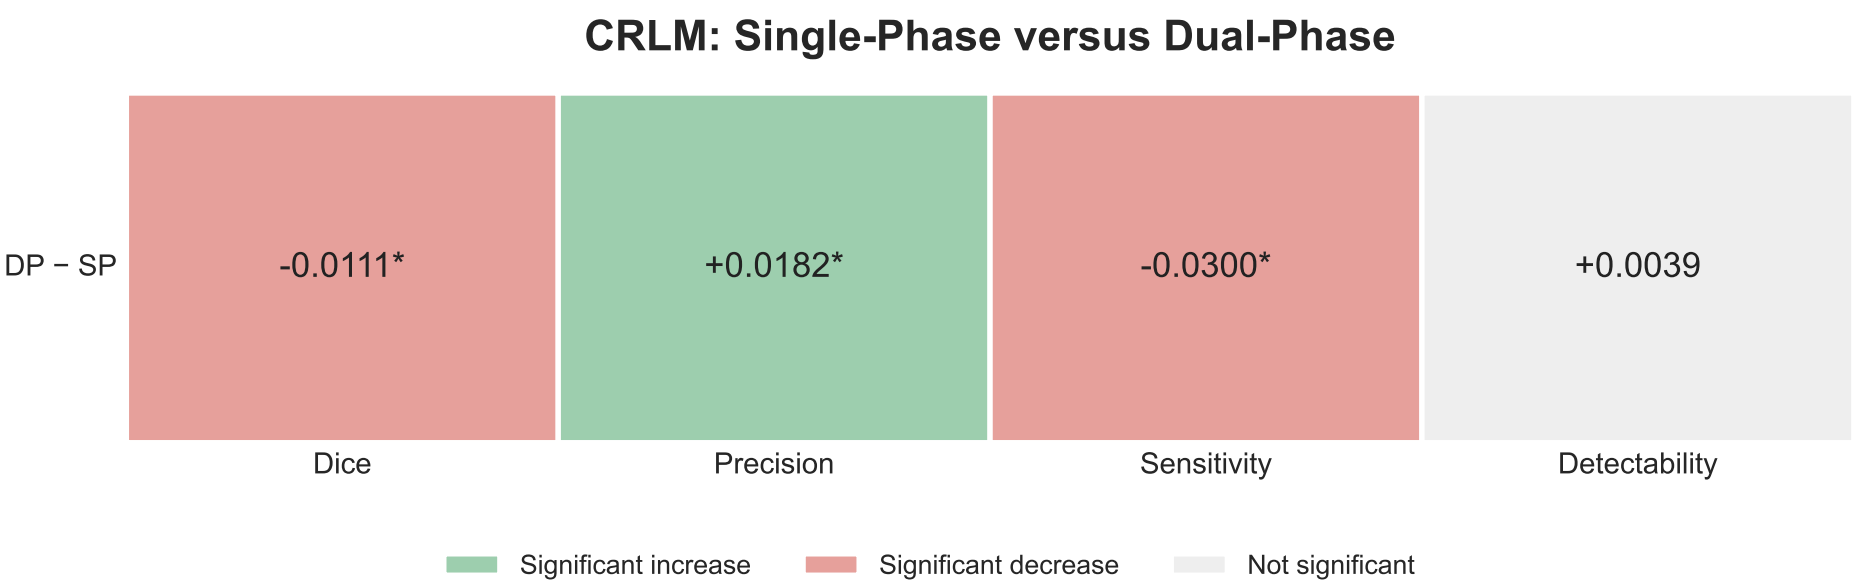
CRLM: Single-Phase versus Dual-Phase
DP − SP
-0.0111*
+0.0182*
-0.0300*
+0.0039
Dice
Precision
Sensitivity
Detectability
Significant increase
Significant decrease
Not significant
Voxel level: Dice, Precision, Sensitivity. Lesion level: Detectability (IoU ≥ 0.20).
Values: mean paired differences (named model − comparison model).
* Holm-adjusted Wilcoxon p < 0.05.