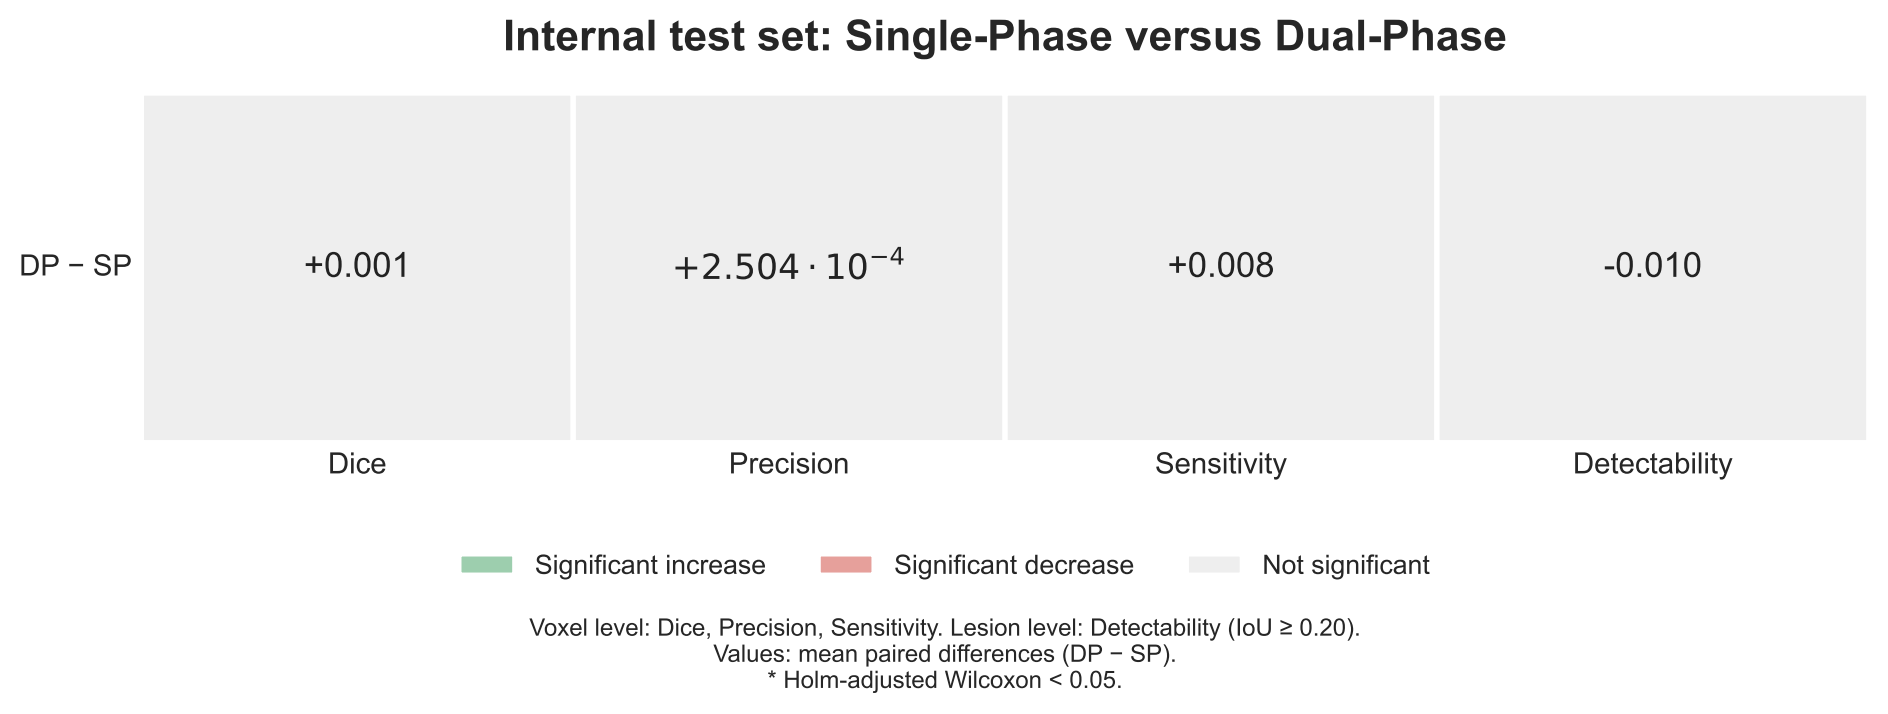
Internal test set: Single-Phase versus Dual-Phase
DP − SP
+0.001
+2.504 · 10−4
+0.008
-0.010
Dice
Precision
Sensitivity
Detectability
Significant increase
Significant decrease
Not significant
Voxel level: Dice, Precision, Sensitivity. Lesion level: Detectability (IoU ≥ 0.20).
Values: mean paired differences (DP − SP).
* Holm-adjusted Wilcoxon < 0.05.