

Access provided by:
**INSTITUTE OF COMPUTING
TECHNOLOGY CAS**
Sign Out

Browse

My Settings

Get Help

Browse Conferences > Microwave Symposium (IMS), 20...

FMCW radar fall detection based on ISAR processing utilizing the properties of RCS, range, and Doppler

View Document

1
Paper
Citation

296
Full
Text Views

Related Articles

Invertible spread-spectrum watermarking for image authentication and multilevel ...

High resolution electrophysiological activity imaging of in-vitro neuronal netwo...

View All

4
Author(s)

Zhengyu Peng ; José-María Muñoz-Ferreras ; Roberto Gómez-García ; Changzhi Li

View All Authors

Abstract	Authors	Figures	References	Citations	Keywords	Metrics	Media
----------	---------	---------	------------	-----------	----------	---------	-------

Abstract:
Falls are among the leading causes of fatal and non-fatal injuries for seniors. For long-term non-contact detection of falls in home and nursing environments, a coherent frequency-modulated continuous-wave (FMCW) radar sensor is designed and tested. The coherence property of the developed FMCW radar helps to preserve the phase history of the signal detected from human subjects, and can thus obtain Doppler information based on inverse synthetic aperture radar (ISAR) imaging. By analyzing the changes of the radar cross-section (RCS), range, and Doppler on ISAR images during the movement of a subject, falls can be distinguished from normal activities. Experiments have been carried out to demonstrate and analyze the ISAR signature of actual fall incidents, which has been compared with that of an abrupt movement. Preliminary results have confirmed the ability of an FMCW radar to successfully detect fall events using ISAR imaging.

Published in: Microwave Symposium (IMS), 2016 IEEE MTT-S International

Date of Conference: 22-27 May 2016

INSPEC Accession Number: 16213906

Date Added to IEEE Xplore: 11 August 2016

DOI: 10.1109/MWSYM.2016.7540121

ISBN Information:

Publisher: IEEE

Conference Location: San Francisco, CA, USA

Contents

Download PDF	<div>SECTION I.</div> <div>Introduction</div> <div>The health of seniors is a major concern in the society with population aging. Among various factors that threat the health of seniors, accidental fall is one of the most dangerous. Studies of fall detection based on different techniques can be found in the technical literature, including accelerometer-based solutions [1], camera-based solutions [2], [3] and Doppler-radar-based systems [4], [5]. Accelerometer-based techniques require subjects to carry or wear sensors. They also need for charging or replacing batteries frequently. Camera-based solutions implement algorithms to extract motion dynamic features, such as velocity and intensity gradient of human subjects, which require intensive computation and does not have sufficient accuracy. Though a recently-reported technique [6] tried to reduce the computational intensity and improve accuracy, camera-based solutions still suffer from several critical problems. One is that the views of cameras can be easily blocked by obstacles. Moreover, privacy concerns limit practical use of camera in seniors' daily life.</div> <div>Moving targets, such as walking persons and different parts of the body, will introduce frequency modulation to a microwave continuous-wave signal, which is commonly referred to as “Doppler</div>	
Download Citations		Full Text
View References		Abstract
Email		Authors
Print		Figures
Request Permissions		References
Export to Collabratec		Citations
		Keywords
Alerts		Back to Top

effect” and enables radars for fall detection. Unlike accelerometers, radar sensors do not need subjects to wear anything, which makes them more user-friendly. In addition, compared with camera-based solutions, radar systems can be used in all types of environments and can also penetrate obstacles. However, current radar-based fall detection systems only utilize Doppler information [5]. They may trigger false alarm because the Doppler signature produced by other life activities may be similar to that caused by a fall event. Examples of activities that may trigger a false alarm include jumping, abruptly stepping forward, or quickly moving a hand in one direction.


In this work, a custom-designed coherent FMCW radar sensor is used to mitigate the shortages of purely Doppler-based detection. In comparison with existing works, this paper utilizes multiple properties of the radar cross-section (RCS), range, and Doppler information of a subject to identify fall incidents. The coherence of an FMCW radar helps to preserve phase histories of the signal detected from human subjects. Thus, Doppler information can be derived using the inverse synthetic aperture radar (ISAR) imaging algorithm. Experiments will be carried out to demonstrate and analyze the ISAR signatures of actual fall events, as well as similar normal activities. Frames of ISAR images corresponding to different states of a fall event will be illustrated and compared with those of other motions. The obtained results will confirm the ability of an FMCW radar to properly detect and identify fall accidents with ISAR imaging.

SECTION II.

Theory of Isar-Based Fall Detection

FMCW radars can continuously track the range history of a human target [7]. Furthermore, if an FMCW radar is coherent, a series of ISAR images can be obtained by deriving the speed of a human subject and plotting it with the range information simultaneously. In this section, the theory of ISAR-based fall detection with a custom-designed FMCW radar prototype will be presented. Three different cases of body motions are illustrated in Fig. 1, along with their corresponding ISAR image evolution also depicted.

Figure 1(a) illustrates the case when the human subject falls toward the radar. The falling event is divided into four phases depending on the changes of the velocity, RCS, and range of the human subject. At time P1 the human subject starts to fall with relatively low speed, which appears as low Doppler frequency in the ISAR image. Then, at P2, the signature of the human subject has a sudden Doppler change due to the acceleration during the fall event. In the meantime, the tilt angle of the human subject is small, so that the RCS of the human subject does not change too much. Thus, the human signature is still quite strong in the ISAR evolution figure. When the human subject continues to fall, the RCS keeps decreasing as indicated by P3 in Fig. 1(a), which makes the ISAR signature to fade along the marked direction. The moving direction of the signature is affected by the changes of both the target velocity (i.e., Doppler frequency) and the target range. As soon as the human target hits the ground, the human signature disappears since both the RCS and Doppler are minimized.

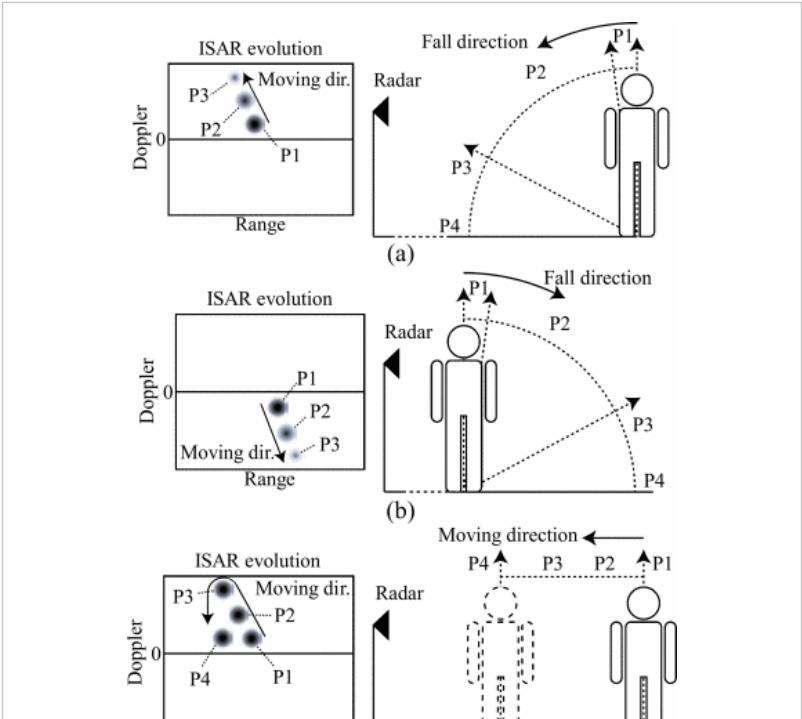




Fig. 1: Illustration of the actions of a human subject and the corresponding ISAR image evolutions. (a) The human subject falls toward the radar. (b) The human subject falls away from the radar. (c) The human subject makes an abrupt movement toward the radar.

Similar to the scenario when a subject falls toward the radar, falling away from the radar can also be divided into four phases, as shown in Fig. 1(b). At P1 the human subject starts to fall, producing a strong signature below the zero Doppler line. At P2, the human subject starts to accelerate without a significant change of the RCS. Thus, the Doppler frequency of the human signature increases while the strength does not change much. When the human subject is close to ground, indicated as P3 in Fig. 1(b), the ISAR signature fades away in the marked direction due to the decrease of the RCS. Finally, as the human subject hits the ground, its signature disappears.

A fall event can be divided into a series action of start, acceleration, and stop, based on which, one of the most similar events is an abrupt movement toward or away from the radar. Such an event can also be divided into four phases as shown in Fig. 1(c). At P1 when the human subject starts to move, the signature appears with low Doppler frequency above the zero Doppler line. During the acceleration phases P3 and P4 of Fig. 1(c), in which the Doppler frequency of the signature increases and the range slightly decreases, it can be observed that the signature moves towards the marked direction similar to the fall case in Fig. 1(a). However, as the RCS of the human subject does not change much during the abrupt movement action, the signature does not fade in P3, which is different from fall incidents. Finally, in P4, as the human subject stops, a strong signature returning to zero Doppler will be observed in the ISAR image in Fig. 1(c), which is also different from fall events.

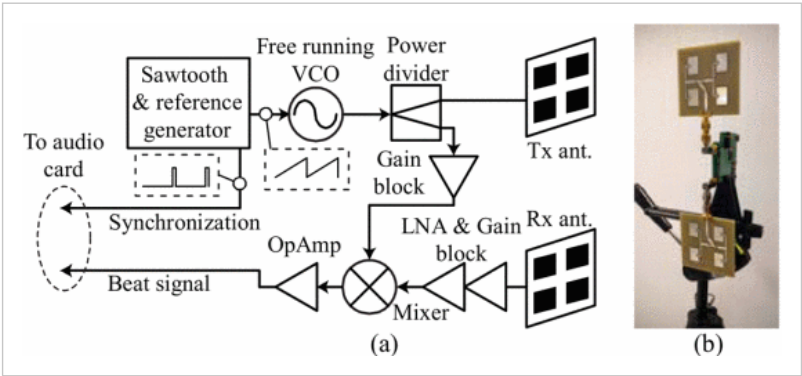


Fig. 2: (a) Schematic of the FMCW radar prototype. (b) Photograph of the FMCW radar prototype mounted on a tripod.

Table I: Parameters of the radar prototype

Center frequency f_c	5.8 GHz	Sampling frequency f_s	44.1 KHz
Transmitted bandwidth B	320 MHz	Frequency ramp repetition period T	10 ms
Average transmitted power	8 dBm		

It should be noted that for other common human activities, such as walking, sitting, and running, their actions are very different from fall incidents, so that they can be easily identified. For example, the signature of a waking person in ISAR images has a periodically-changing Doppler frequency with a continuous increase or decrease in the target range. If the person stops, the Doppler of the signature will move to zero.

SECTION III.

Radar Prototype and Experiments

The radar prototype used in the experiments was designed with a center frequency of 5.8 GHz. Fig. 2 shows the block diagram and photograph of the radar prototype. To minimize its complexity and

cost, an operational-amplifier-based circuit was implemented to generate a “sawtooth” voltage to control a free running voltage-controlled oscillator (VCO). A pair of 2×2 patch antennas were used to transmit and receive signal. The audio card of a laptop is employed for signal acquisition, facilitating real-time signal processing in the laptop. The coherence property of the system is achieved by simultaneously sampling the beat signal and the synchronization signal, which is locked to the “sawtooth” voltage signal. The phases of the beat signals are aligned to the falling edge of the synchronization signal during signal processing. The basic parameters of the radar prototype are listed in Table I.

Preliminary experiments were carried out to show the capability of the developed FMCW radar for fall detection. The ISAR images (ISAR imaging does not respect the usual convention for the sign of the Doppler frequency) shown in Fig. 3(a)–(d) correspond to the 4 different phases of the fall event in Fig. 1(a), i.e., P1 to P4. It should be noted that the ISAR signature of the human subject experienced an acceleration and a fading period, before it disappeared as the human subject hit the ground.

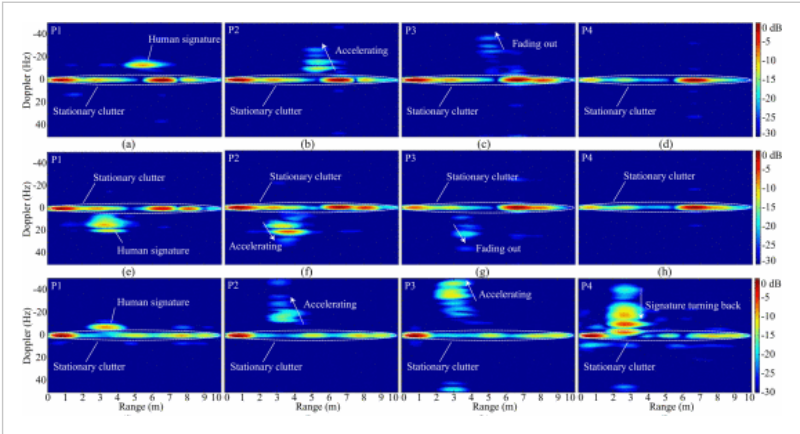


Fig. 3: Different frames of ISAR images during fall incidents and an abrupt body movement. (a)–(d): falling toward the radar; (e)–(h): falling away from the radar; (i)–(l): an abrupt movement toward the radar.

Similarly, Fig. 3(e)–(h) correspond to the fall event shown in Fig. 1(b). The phases of P1 (start), P2 (acceleration), P3 (fading), and P4 (disappearing) in the detected human signature can be clearly identified in these ISAR images, which is consistent with the theoretical analysis in Section II.

As a comparison, the results of an abrupt movement toward the radar are shown in Fig. 3(i)–(l), which also correspond to the four phases in Fig. 1(c). As discussed in Section II, P1 and P2 of the abrupt movement are similar to those of a fall event, but P3 and P4 of the abrupt movement are significantly different.

SECTION IV.

Conclusion

This work has demonstrated the ability of an FMCW radar to detect fall events based on real-time ISAR imaging. A 5.8-GHz custom-designed prototype of portable coherent FMCW radar was used in the experiments. ISAR images measured from different human motions show that with an FMCW radar, it is possible to detect falls based on Doppler frequency, range information, and the RCS. This may enable longterm remote fall detection without requiring seniors to wear any sensing device in home and nursing environments.

ACKNOWLEDGMENT

This work was supported by the NSF under grant ECCS-1254838, the University of Alcalá under Project CCG-2014/EXP-021, and the Spanish Ministry of Economy and Competitiveness under Project TEC2014-54289-R.

Keywords

INSPEC: Controlled Indexing

synthetic aperture radar, biomedical imaging, CW radar, Doppler radar, FM radar, injuries,

radar cross-sections, radar imaging, radar receivers

INSPEC: Non-Controlled Indexing

fall incident, FMCW radar fall detection, ISAR processing, RCS, range property, Doppler property, nonfatal injury, fatal injury, fall noncontact detection, home environment, nursing environment, frequency modulated continuous wave radar sensor, signal phase history, Doppler information, inverse synthetic aperture radar imaging, ISAR imaging, radar cross-section

Author Keywords

RCS, Doppler, fall detection, FMCW radar, health monitoring, ISAR

Authors

Zhengyu Peng

Dept. Electrical & Computer Engineering, Texas Tech University,
Lubbock, 79409, USA

José-María Muñoz-Ferreras

Dept. Signal Theory & Communications, University of Alcalá, Alcalá
de Henares, 28871, Madrid, Spain

Roberto Gómez-García

Dept. Signal Theory & Communications, University of Alcalá, Alcalá
de Henares, 28871, Madrid, Spain

Changzhi Li

Dept. Electrical & Computer Engineering, Texas Tech University,
Lubbock, 79409, USA

Related Articles

Invertible spread-spectrum watermarking for image authentication and multilevel access to precision-critical watermarked images

J. Domingo-Ferrer; F. Sebe

High resolution electrophysiological activity imaging of in-vitro neuronal networks

L. Berdondini; T. Overstolz; N.F. de Rooij; M. Koudelka-Hep; S. Martinoia; P. Seitz; M. Wany;
N. Blanc

277 V safety issues: recognition and prevention of lighting related electrical injuries and fatalities

H. Wolfman; M. Capelli-Schellpfeffer

Intelligent monitoring systems: smart room for patient's suffering from somnambulism

S.S. Bhattacharya

MEMS actuator array as a neuro-physiological testing tool

E.T. Enikov; K.V. Lazarov; G.R. Gonzales

Endoscopic optical coherence tomography with a micromachined mirror

Tuqiang Xie; Huikai Xie; G.K. Fedder; M. Zeidel; Yingtian Pan

A low-voltage electrostatically actuated MEMS scanner for in vivo biomedical imaging

T.W. Yeow; K.Y. Lim; B. Wilson; A.A. Goldenberg

Sequential imaging and analysis of erythrocyte aggregation

S. Jayavanth; M. Singh; K. Jagadeesan

NMR imaging of biocapsules for monitoring the performance of cell and tissue implants

S. Eroglu; B. Gimi; L. Leoni; B. Roman; G. Friedman; T. Desai; R.L. Magin

Field testing and monitoring of rolling stock under the new federal track and equipment regulations

E.J. Lombardi; E. Sherrock; D.C. Warner; B.T. Whitten

IEEE Account	Purchase Details	Profile Information	Need Help?
<div>» Change Username/Password</div> <div>» Update Address</div>	<div>» Payment Options</div> <div>» Order History</div> <div>» View Purchased Documents</div>	<div>» Communications Preferences</div> <div>» Profession and Education</div> <div>» Technical Interests</div>	<div>» US & Canada: +1 800 678 4333</div> <div>» Worldwide: +1 732 981 0060</div> <div>» Contact & Support</div>