


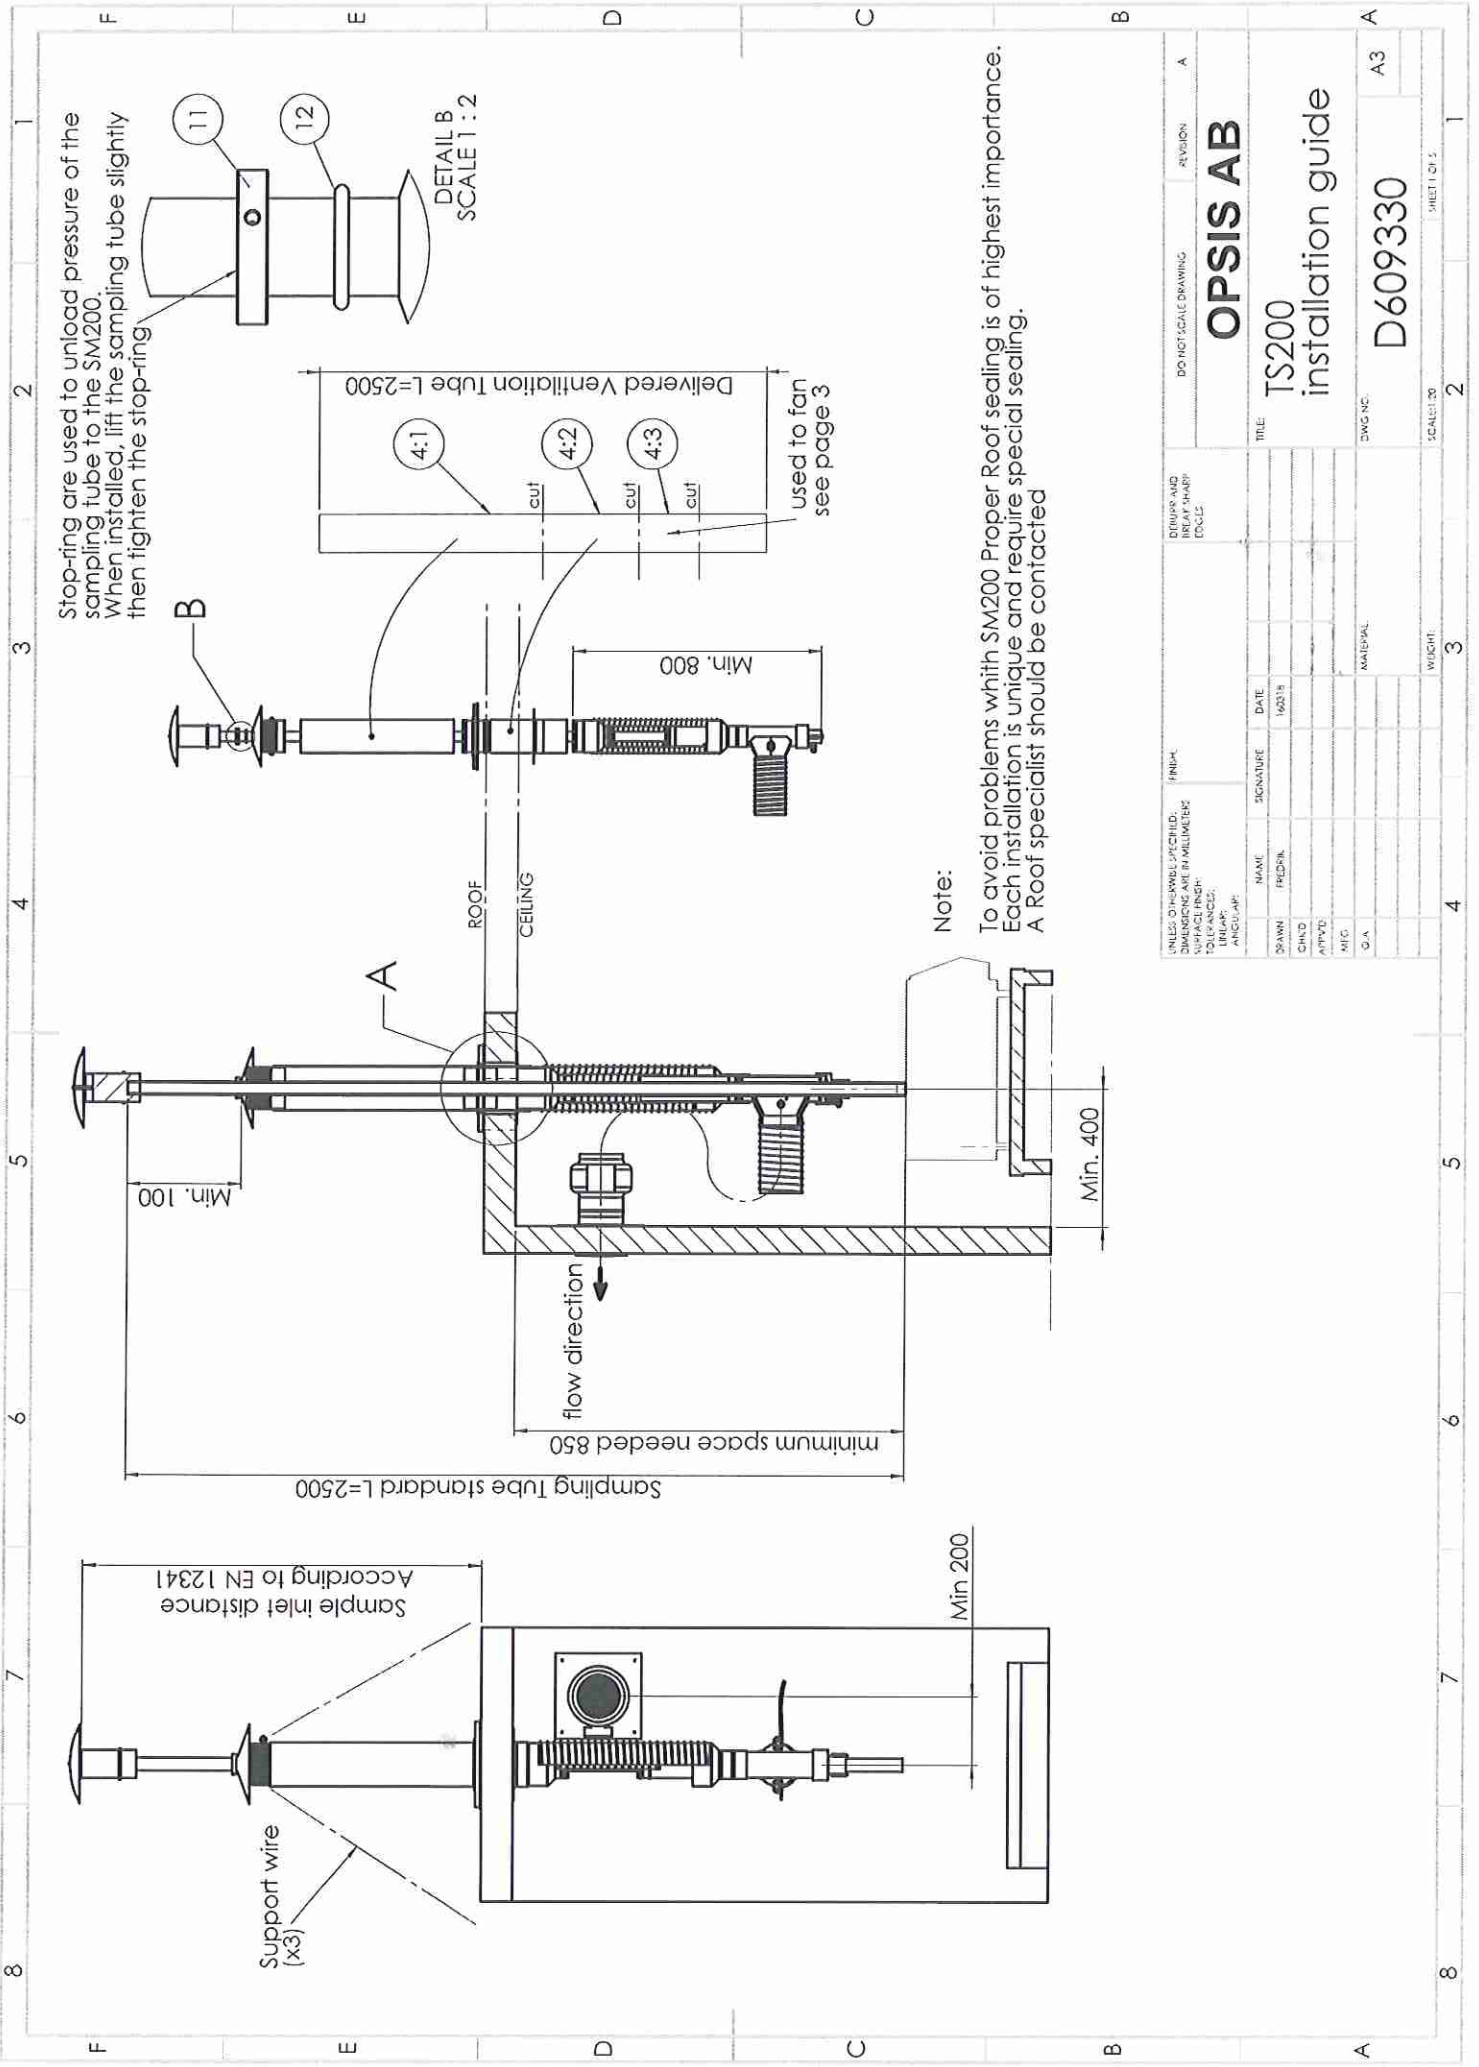


Stop-ring are used to unload pressure of the sampling tube to the SM200. When installed, lift the sampling tube slightly then tighten the stop-ring

DETAIL B
SCALE 1:2

Note:

To avoid problems with SM200 Proper Roof sealing is of highest importance. Each installation is unique and require special sealing. A Roof specialist should be contacted

UNLESS OTHERWISE SPECIFIED: DIMENSIONS ARE IN MILLIMETERS TOLERANCES: LINEAR: ANGULAR:		FINISH	DESIGNING AND CHECKING SCALE		DO NOT SCALE DRAWING		REVISION		A
DRAWN		NAME	SIGNATURE	DATE	TITLE OPSIS AB TS200 installation guide				
CHECKED									
APPROVED									
MTC									
G.A.									
MATERIAL		DWG NO.			D609330				
WIDTH		SCALE: 20			A3				
SHEET 20		2			1				

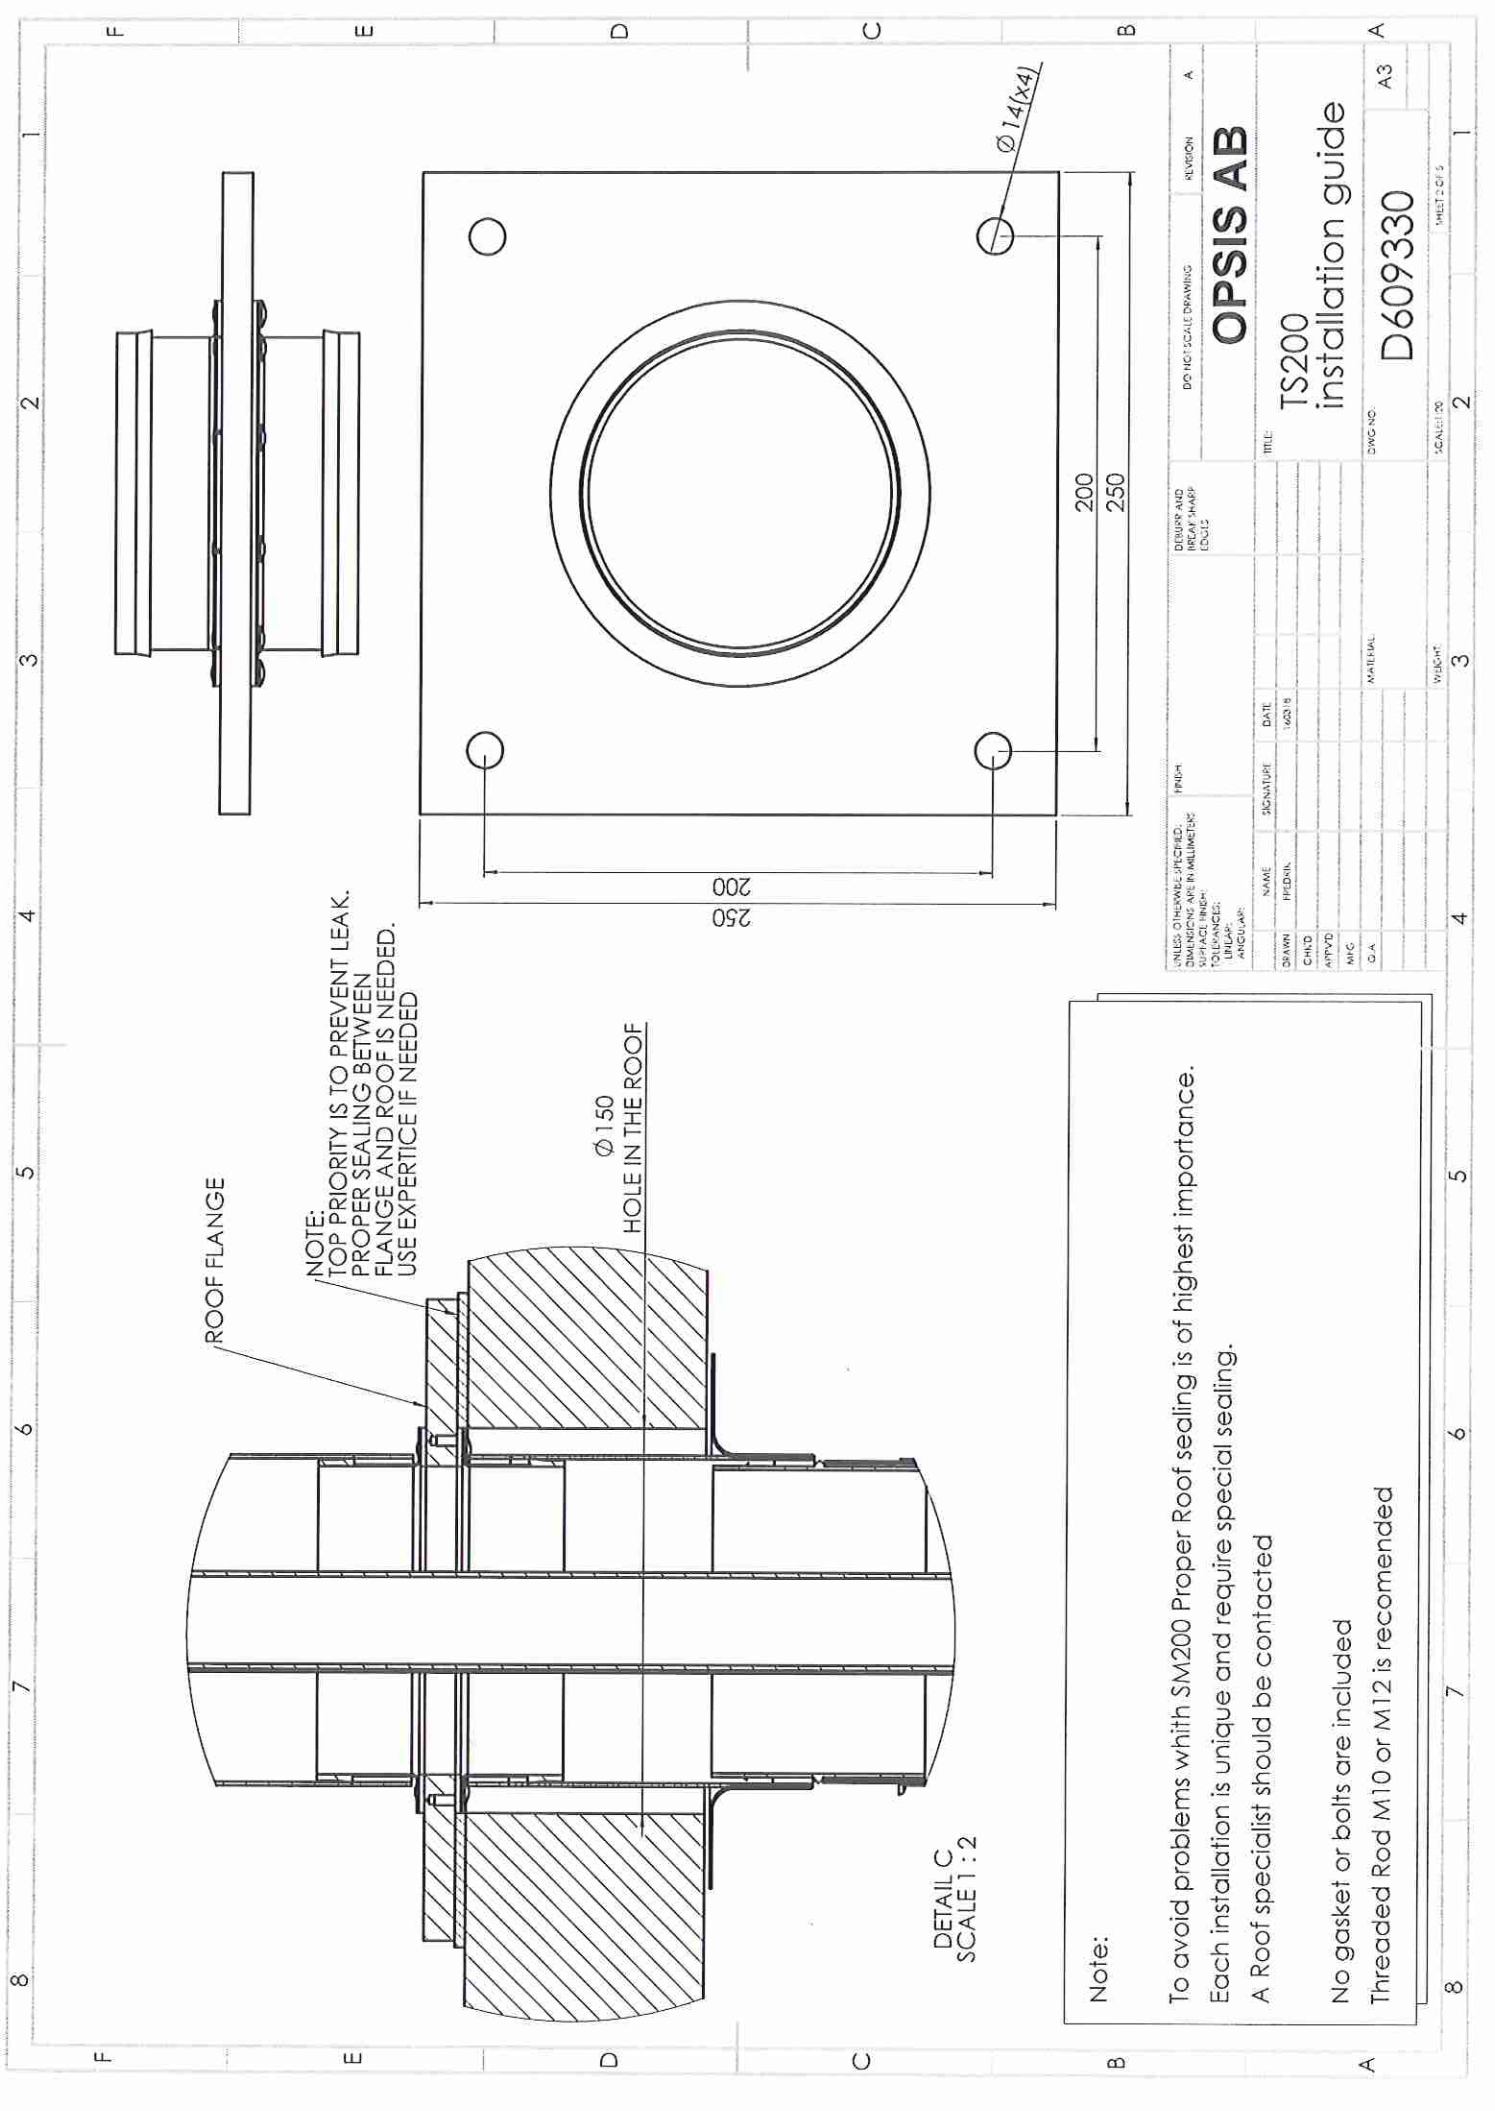

Note:

To avoid problems with SM200 Proper Roof sealing is of highest importance.
Each installation is unique and require special sealing.
A Roof specialist should be contacted


No gasket or bolts are included
Threaded Rod M10 or M12 is recommended

USE PROPER SEALING IN
OUTER WALL

CUT VENTILATION TUBE TO
SUITABLE LENGTH

SCREWS NOT INCLUDED

VENTILATION FAN
230VAC/ 115VAC
CONTACT AN ELECTRICIAN IF NEEDED

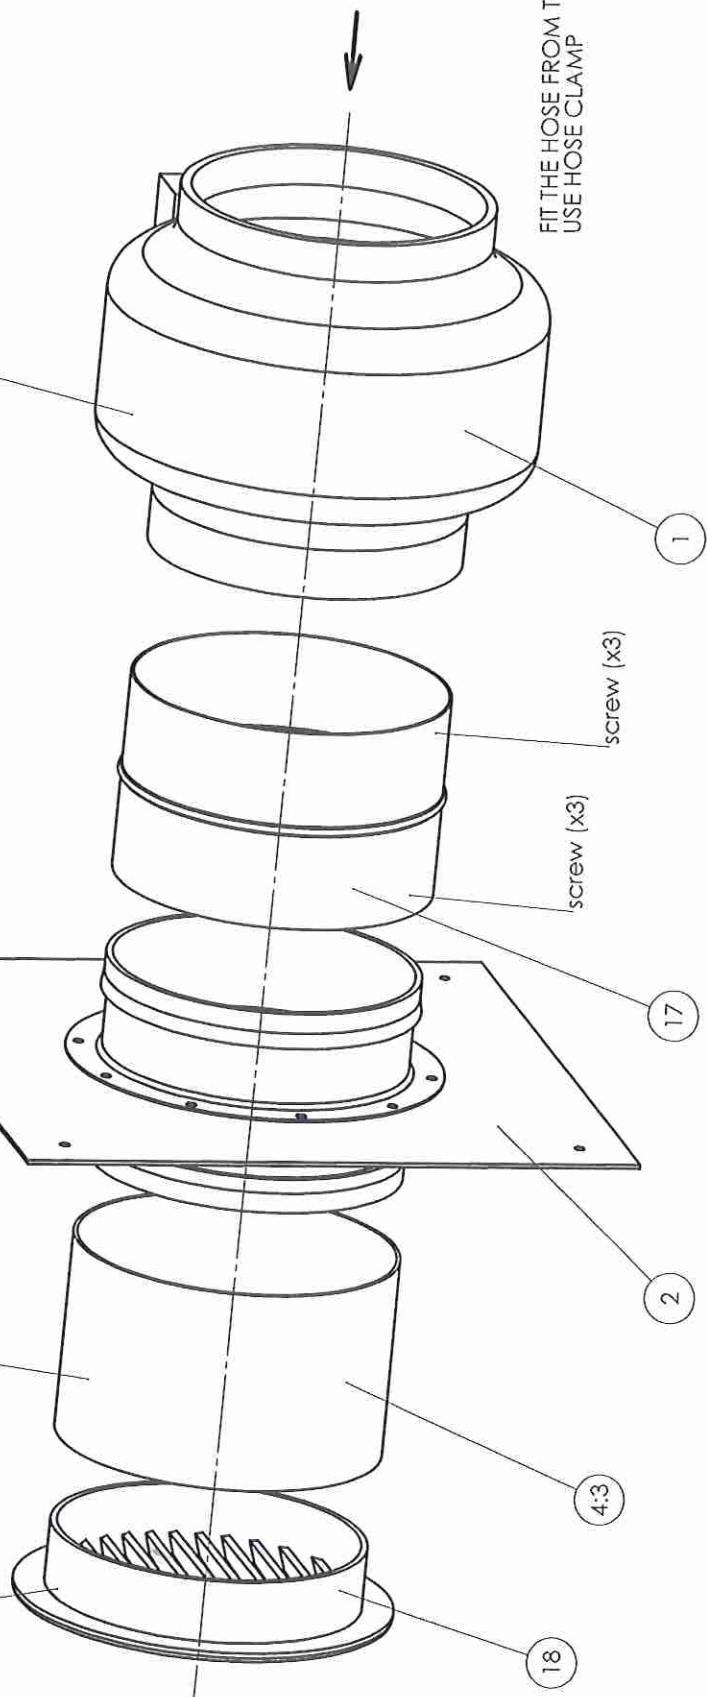

UNLESS OTHERWISE SPECIFIED
DIMENSIONS ARE IN MILLIMETERS
TOLERANCES:
FRACTIONAL
DECIMAL
ANGLES

DESIGN AND
INDICATE SHARP
EDGES

DO NOT SCALE DRAWING

REVISION

OP SIS AB

TITLE

TS200
installation guide

DWG NO.

D609330

A3


A

SCALE 1:10

2

SHEET 3 OF 5

1

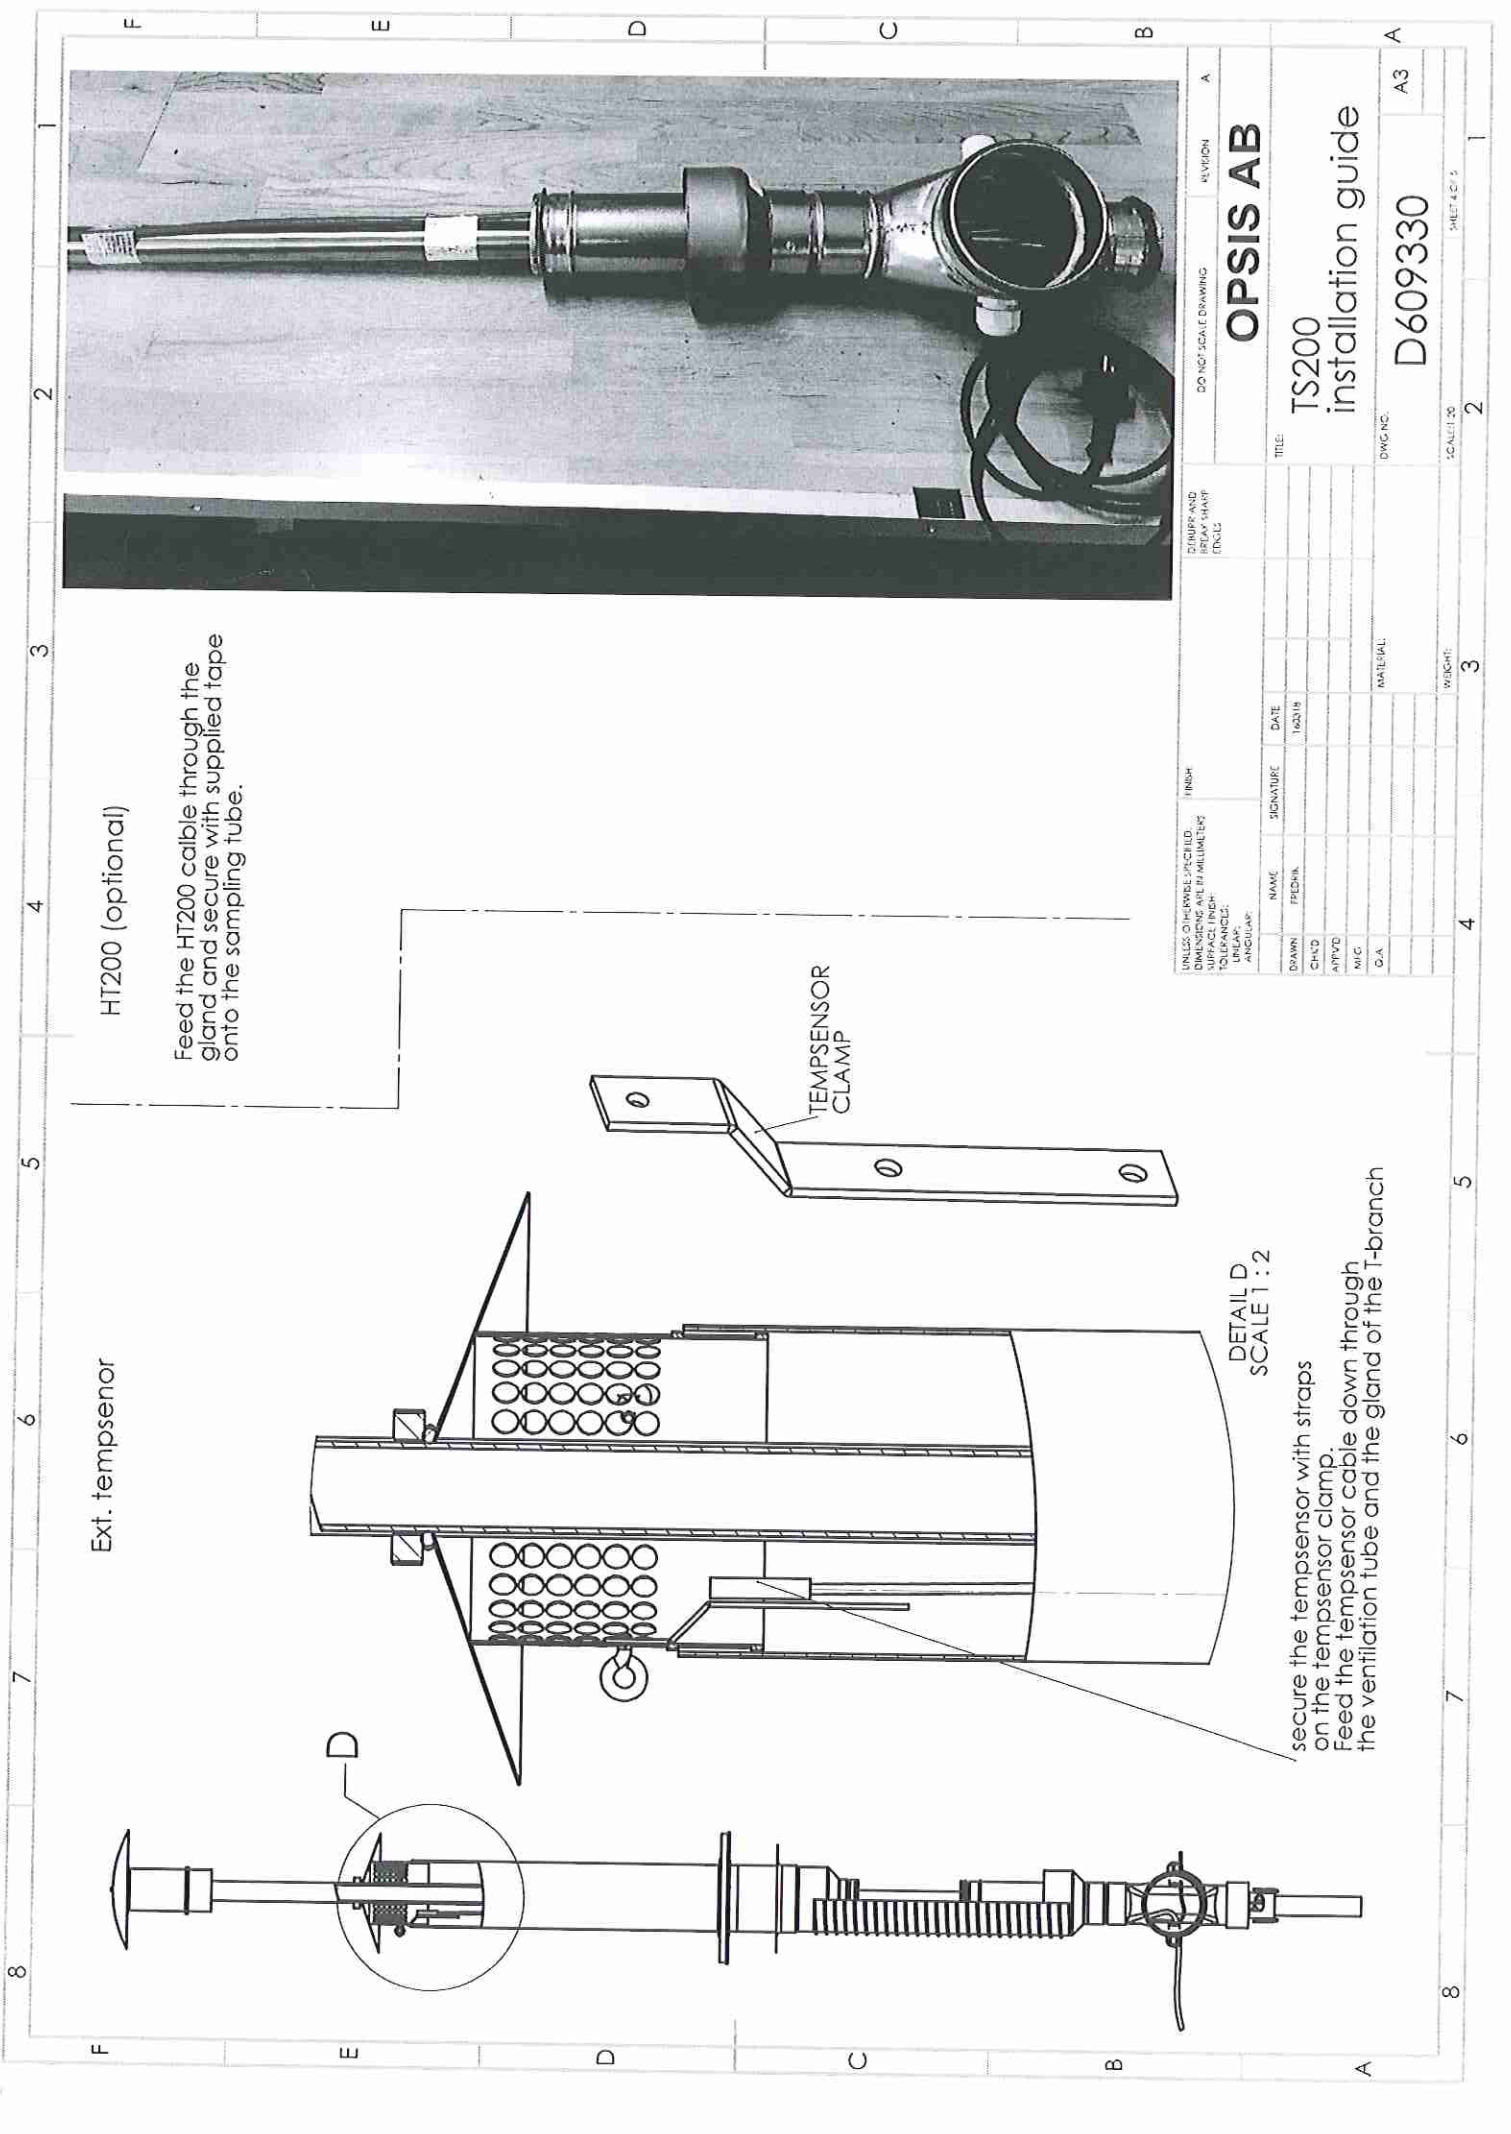

HT200 (optional)


Feed the HT200 cable through the gland and secure with supplied tape onto the sampling tube.

Ext. tempensor



TEMPSENSOR CLAMP

DETAIL D
SCALE 1:2

secure the tempensor with straps on the tempensor clamp.
Feed the tempensor cable down through the ventilation tube and the gland of the T-branch

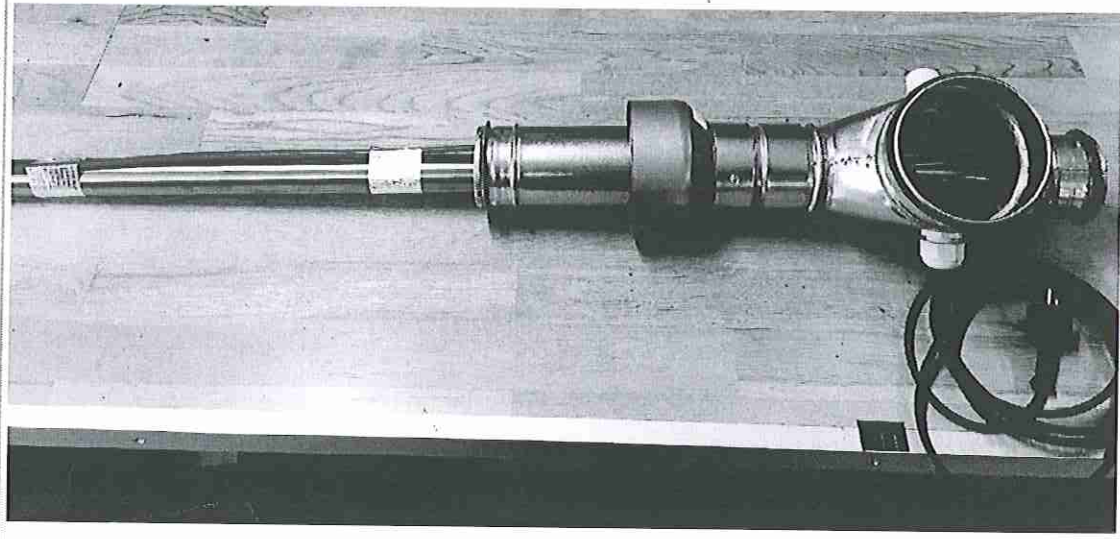

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN MILLIMETERS TOLERANCES: FRACTIONS DECIMALS ANGLES		FINISH	DO NOT SCALE DRAWING		REVISION	A
NAME		SIGNATURE	DATE	TITLE		
DRAWN		PROJEN	10/21/19	OPSIS AB		
CHKD				TS200		
APP'D				installation guide		
MFG				D609330		
Q.A.				A3		
MATERIAL				DWC-NC		
WEIGHT				SCALE 1:20		
SHEET 1 OF 5				2		

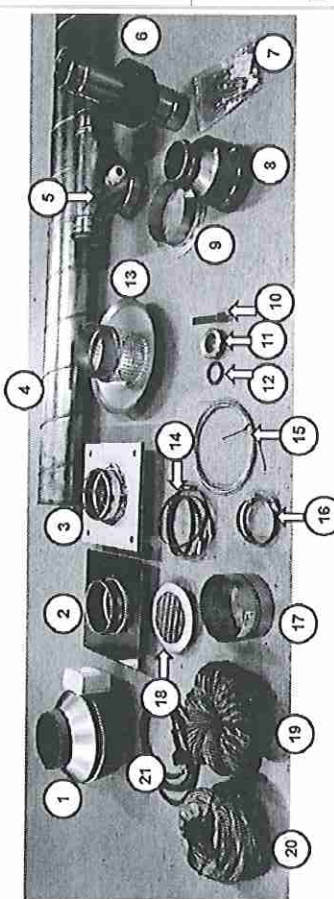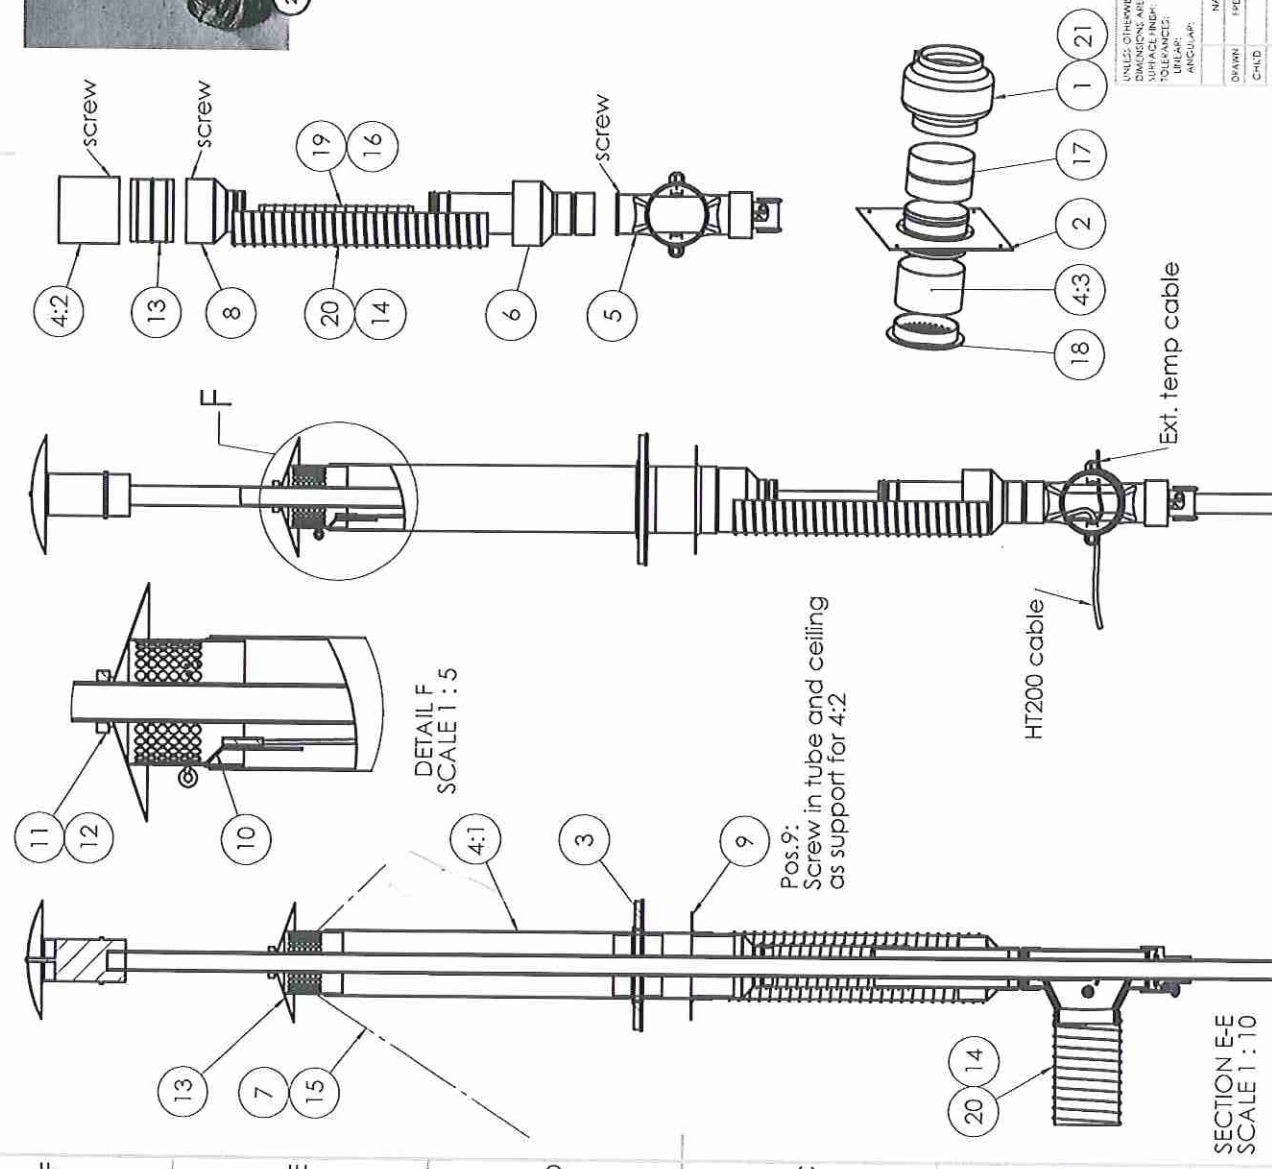

Position Artikelkod Benämning

- 1 E050110 Fan TS200
- 2 M122322 Duct-flange for fan
- 3 M102550 Roof-flange
- 4 M122315 Spiro-ducting
- 5 M122330 T-branch duct
- 6 M122368 M122359 M122325 Condensation-collector assembly
- 7 — Fasteners + wire accessories
- 8 M122325 M122352 Dimension change assembly
- 9 M122320 Wall sleeve
- 10 M102565 Tempensor holder
- 11 M122355 Stop ring for sample tube
- 12 A020363 O-ring for stop ring
- 13 M122310 Roof cowl
- 14 M000468 Hose clamp big, 104-138mm
- 15 A121196 Guy wire
- 16 M000469 Hose clamp small 68-85mm
- 17 M122369 Sleeve 125mm
- 18 M122332 Grating for outer wall
- 19 M122340 Ventilation hose small id=80mm
- 20 M122335 Ventilation hose big id=125mm
- 21 E114050 Power cable 230V/115V

UNLESS OTHERWISE SPECIFIED, DIMENSIONS ARE IN MILLIMETERS		FIRST		OTHER AND REPEAT SHAPES (COPIES)		DO NOT SCALE DRAWING		REVISION		A	
TOLERANCES:											
ANGULAR											
NAME		SIGNATURE		DATE		TITLE					
DRAWN		CHECKED		16/01/18							
CHD											
APP'D											
MTC											
G/A				MATERIAL		DWG NO.					
						SCALE 1:20					
				WEIGHT:		SHEET 5 OF 5					
				3							
				4							
				5							
				6							
				7		SECTION E-E SCALE 1:10					
				8							
				9							
				10							
				11							