

Final Test Record

Series 1405 - TEOM® Ambient Particulate Monitor

Serial #:

1405A221541209

Configuration: 1405F, Single TEOM, FDMS

This instrument was manufactured by Thermo Fisher Scientific, Environmental Instruments Division – Air Quality Instruments, located in Franklin Massachusetts, USA. The calibration and testing procedures used are in accordance with American National Standards Institute (ANSI) Z540 for calibration, including metrology equipment traceable to the National Institute of Standards and Technology (NIST) in Washington D.C., USA. The manufacturing, testing and calibration of this instrument were conducted in accordance with Thermo Fisher Scientific's certified ISO9001:2000 program for quality. This Final Test Record serves as confirmation that all the required Manufacturing and Quality Control inspections done on this instrument, are in accordance with Thermo Fisher Scientific's specifications.

Process Checks:

Assembly inspection
Passes all function tests

Voltage calibrations
Calibrate software constants
Passes required burn-in

Evaluate burn-in data
Passes leak test
Reset to user defaults

T.E. Calibration "K0":

Mass transducer **1405A125011209**

Fine - all units				
	Mass (Mg)	F0: no Filter	F1: w/filter	K0
Filter 1:	98.07	341.215	253.974	14183.891
Filter 2:	97.89	341.212	254.231	14222.611
Filter 3:	97.98	341.211	254.236	14237.051
Filter 4:	97.64	341.211	254.283	14199.446
Filter 5:	97.93	341.207	253.926	14152.469
	Std.Dev.	Coeff Variation	Average K0	
	33.16	0.23%	14199	

Coarse - dual flow only				
	Mass (Mg)	F0: no Filter	F1: w/filter	K0
	0.00	0.000	0.000	
	0.00	0.000	0.000	
	0.00	0.000	0.000	
	0.00	0.000	0.000	
	0.00	0.000	0.000	
	Std.Dev.	Coeff Variation	Average K0	


Firmware versions:

Instrument Firmware version:	1.56
Flow Controller 0 Firmware version:	0.011
Heat Controller 0 Firmware version:	0.024
User I/O Device Firmware version:	0.014

	0
	0
FDMS Device Firmware version:	0.009

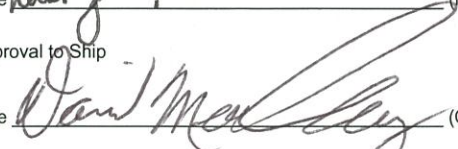
Final Test Sign off

All Process Checks listed above have been successfully completed.

Signature  (Final Test)

Date 10/17/12

Q.A. Approval to Ship

Signature  (QA or Project Leader)

Date 10-17/12

Rev: -

Final Test Record

Series 1405 - TEOM® Ambient Particulate Monitor

Serial #:

1405A221541209

Burn-in run:

from: 10/12/12 18:21

until: 10/13/12 2:22

Total: 8:01 Hrs:Mins

