



T640 / T640X PM Mass Monitor Test Data Sheet

Calibration Summary

Test Equipment: **Flow Meter:** BGI Instruments Tetracal Volumetric Airflow Calibrator
SR# EL0000819
Calibration date: 8/21/2018 **Calibration Due** 8/21/2019
Reference: T640 **SN:** 381
SpanDust: CH0000083 1.28 10.9 102
Lot No: 100128-050-014 **Valid until:** 4/1/2020

Instrument Under Test:

Model: T640 **SR#:** 626 **Sensor#:** 10030
Test Date: 1/30/2019

Pressure Check:

Test Ambient Pressure: 743 (mmHg) Value from Test Equipment
Converted Ambient Pressure: 99.0582 (kPa) Converted Value from Test Equipment
Instrument Ambient Pressure: 99.1 (kPa) Value from Test Instrument

Sample Flow Check:

Actual Flow Qa: 5.07 (LPM) Value from Test Equipment
Sample Flow: 5 (LPM) Value from Test Instrument

Bypass Flow (640X):

Actual Flow, Qa: N/A (LPM) Value from Test Equipment
Bypass Flow: N/A (LPM) Value from Test Instrument

Ambient Temp. Probe:

Actual 21.9 Deg.C Value from Test Equipment
Test Instrument 21.9 Deg.C (+/-1) Value from Test Instrument

Printed copies are UNCONTROLLED

T640 / T640X PM Mass Monitor Test Data Sheet

Downward Ramp Check:


PM10 C	PM10 R		PM2.5 C	PM2.5 R	
388	393.1	0.9870262	188	186.6	1.007503
108.7	109.4	0.99360146	55.4	55.8	0.992832
19.8	19.7	1.00507614	12.4	12.2	1.016393
Average		0.9952346	Average		1.005576

Average

1.0004052

Downward Ramp Slope Check

0.9995949

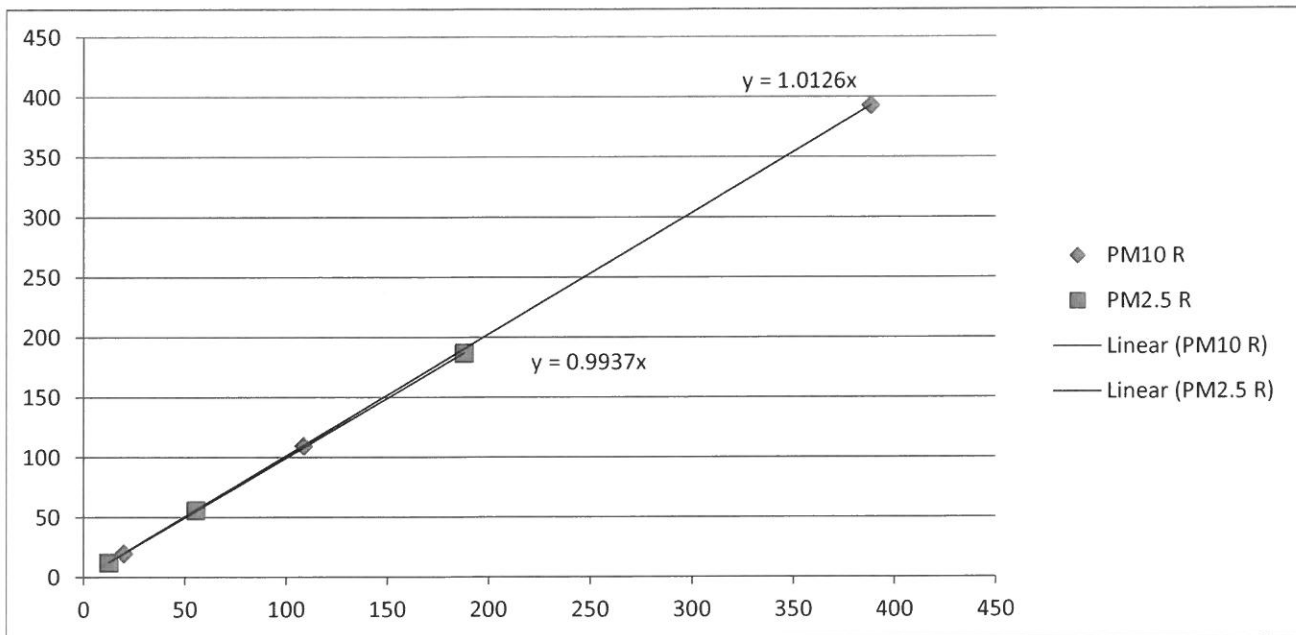

Model: T640 Serial #: 626

Technician:

Ante M. Ruelas 102
15

Test Date:

1-30-19

Final Quality Inspection by:

Inspection Date:

1/31/19

Printed copies are UNCONTROLLED