

ID Number

13-0608

Date

15-Jun-13

Service Number

N/A

Engineer Initials

BL

General Settings

Firmware Version	2.08.0004
Concentration Units	PPM
Temperature Units	°C
Pressure Units	torr

Measurement Settings

Average Period	1 Min
Filter Type	KALMAN
Background Interval	24 Hrs

Serial Communication

Main Gas ID	30
RS232 #1	RS232 #2
Baud 38400	38400
Protocol Advanced	Advanced

Analog Outputs

Output Type	Voltage
Range	50
Over-Ranging	Disabled
Offset	0.25
5.0V CAL	3142
0.5V CAL	676

Voltages

Concentration Voltage	1.34
Reference Voltage	3.86
Analog Supply	11.90
Digital Supply	4.92

Pressures

Gas Flow	1.06
Pressure Units	torr
Ambient	758.00
Cell	749.39
Cal Pressure	749.31

Temperatures

Heater set point	50
Cell	50.04
Converter	89.95
Chassis	32.38
Mirror	49.99
Cooler Voltage	1.16

Calculation Factors

Instrument Gain	0.94
P/T/F Correction	1.000
Background	0.0055
Zero Offset	0

Digital Pots

PGA Gain	64
Input Pot	195
Conc. Voltage(Raw)	1.34
Conc. Voltage	0.021
Measure Coarse Zero	195
Measure Fine Zero	141
Reference Voltage	3.86

Source	227
Cooler	0
Cooler Voltage	1.16
Test Pot	0

Notes

1. This testing result is traceable to NMI Australia via NATA or NIST laboratories.
2. Calibration gas Ecotech reference: CG-1043

ID Number

13-0608

Date

15-Jun-13

Service Number


N/A

Engineer Initials

BL

Full Scale 40.188 ppm

Calibration Point (%FS)	Expected Reading (ppm)	Actual Reading (ppm)	Error (%FS)
0.0	0.000	0.071	0.18
20.0	8.038	7.974	-0.16
40.0	16.075	15.800	-0.68
60.0	24.113	23.791	-0.80
80.0	32.150	31.925	-0.56
100.0	40.188	40.201	0.03

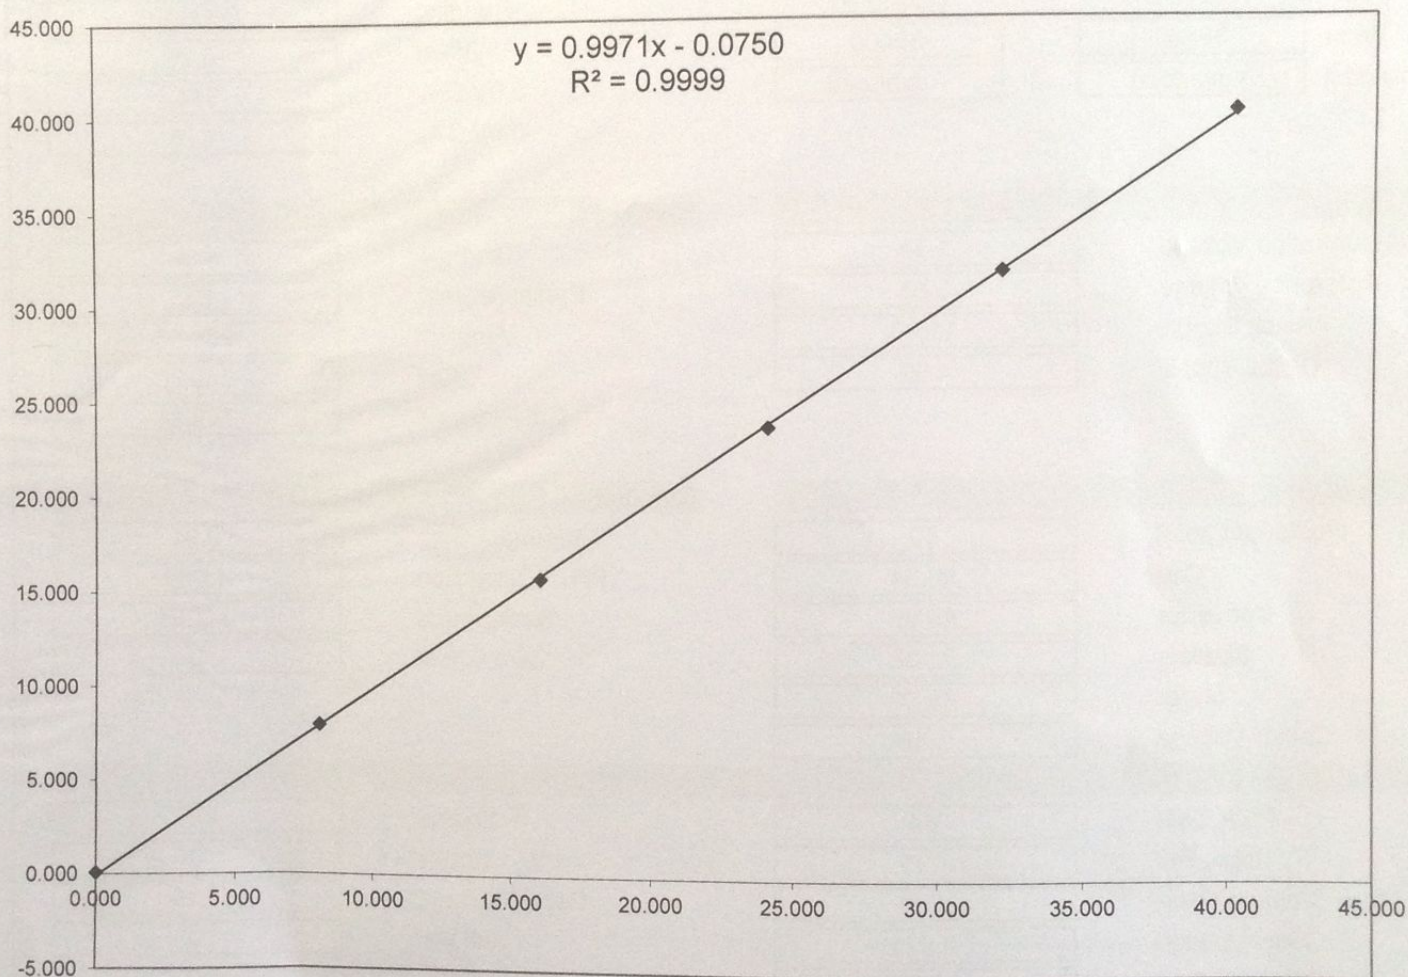

R2 0.99989

Gain 0.99708

Note: Linear line of best fit shall have a gain between 0.99 and 1.01 and a R^2 value greater than 0.998

Pass / Fail

PASS