

ID Number

13-0472

Date

26-Jun-13

Service Number

Engineer Initials

PRS

General Settings

Firmware Version	2.09.0005
Concentration Units	PPM
Temperature Units	°C
Pressure Units	torr

Measurement Settings

Average Period	1 Min
Filter Type	KALMAN
NO2 Filter	Disabled

Analog Outputs

Output Type	Voltage	NH3	NO2
Range	0.5	0.5	0.5
Over-Ranging	Disabled	Disabled	Disabled
Offset	0.25	0.25	0.25
5.0V CAL	3117	3089	3096
0.5V CAL	611	603	624

Calculation Factors

	<u>NO</u>
Instrument Gain	0.87
P/T/F Correction	1.01
Background	0.1236
Zero Offset	0.00

	<u>NH3</u>	
NH3 Efficiency		98.90
	<u>NO2</u>	
Zero Offset		0.00
Converter Efficiency		99.10

Voltages

Conc Voltage (RAW)	1.50
Analog Supply	11.90
Digital Supply	4.95
High Voltage	656.84

Pressures

Gas Flow	0.93
Pressure Units	torr
Ambient	761.52
Cell	108.90
Manifold Pressure	736.43
Cal. Pressure	736.48
Cal. Pressure 2	732.11

Temperatures

Heater set point	50
Cell	49.99
Converter	325.00
Chassis	38.34
Cooler	13.00
Manifold	50.04

Serial Communication

Main Gas ID	40	
AUX Gas ID	0	
RS232 #1	RS232 #2	
Baud	38400	38400
Protocol	Advanced	Advanced

Digital Pots

High Voltage Adjust	141
High Voltage	656.84
Input Pot	104
Conc Voltage (RAW)	1.50
Conc Voltage	0.0234

PGA Gain	64
Test Measure	0

Notes

NH3 Converter ID	13-0113
------------------	---------

Serinus 44 NOx Multipoint Linearity

ID Number

13-0472

Date

26-Jun-13

Service Number

0


Engineer Initials

PRS

Full Scale

0.2034 ppm

Calibration Point (%FS)	Expected Reading (ppm)	Actual Reading (ppm)	Error (%FS)
0.0	0.0000	0.0009	0.45
20.0	0.0407	0.0398	-0.43
40.0	0.0814	0.0794	-0.94
60.0	0.1220	0.1201	-0.94
80.0	0.1627	0.1611	-0.77
100.0	0.2034	0.2033	-0.07

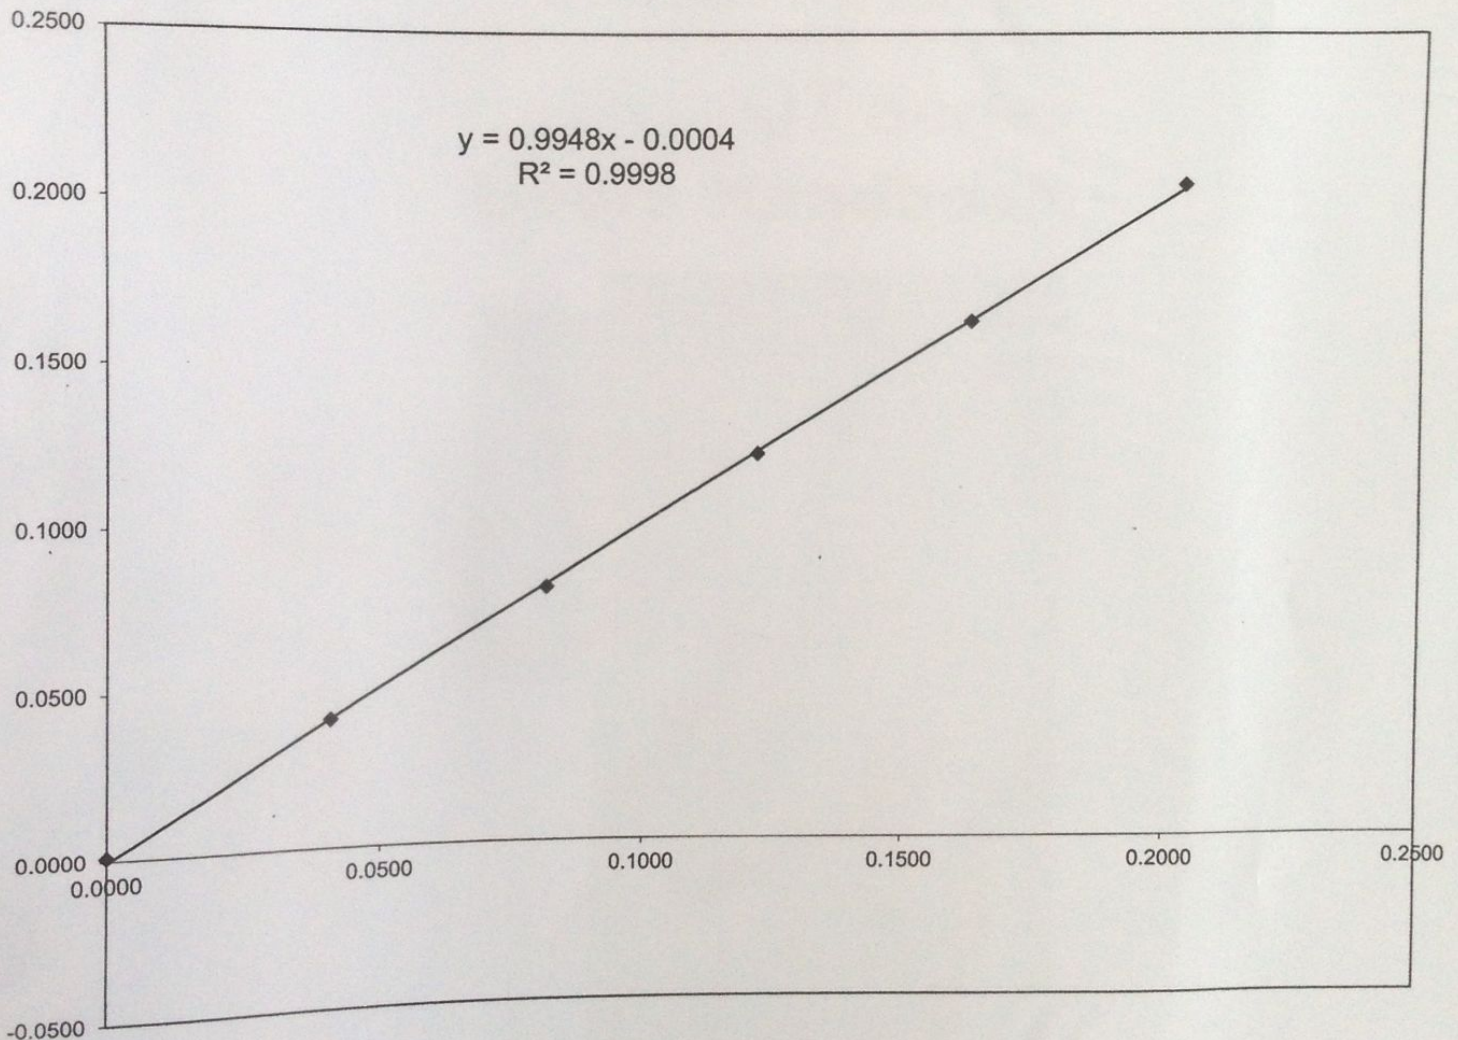

R2 0.99981

Gain 0.99481

Note: Linear line of best fit shall have a gain between 0.99 and 1.01 and a R^2 value greater than 0.998

Pass / Fail

PASS