Allergan eMVA Design Summary

2.00



Allergan

Document prepared by

indegene

Table of Contents

Allergan eMVA Design Summary

Vertical Screen Grid.....4
Horizontal screen Grid.....5
Logo.....6
Standard Icons.....7
Main Icon.....8
Key Message Buttons.....9
Menu Screen.....10
Key Message Titles.....11
Heading.....12
Sub-heading.....13
Body Copy.....14
Important Safety Information.....15
Boxed Warning Button.....16
Boxed Warning Pop-up.....17
Zoom Icon.....18
Pop-up (Big).....19
Pop-up (Small).....20
Close Button.....21
Video Screen.....22
Video Pop-up (Small).....23
Full Screen Video.....24
Patients Screen.....25
Individual Patient's Screen.....26
Internal Toggle Button.....27
Toggle Button.....28

Vertical Screen Grid

The screen is divided into 16 parts vertically.



Horizontal Screen Grid

The screen is divided into 12 parts horizontally.




Logo

The logo shall fit into the 8 boxes on the top-right most corner.




Standard Icons

The left-most column holds the Standard Icons. Each icon resides in a grid with overall dimensions of 128 x 128 px.

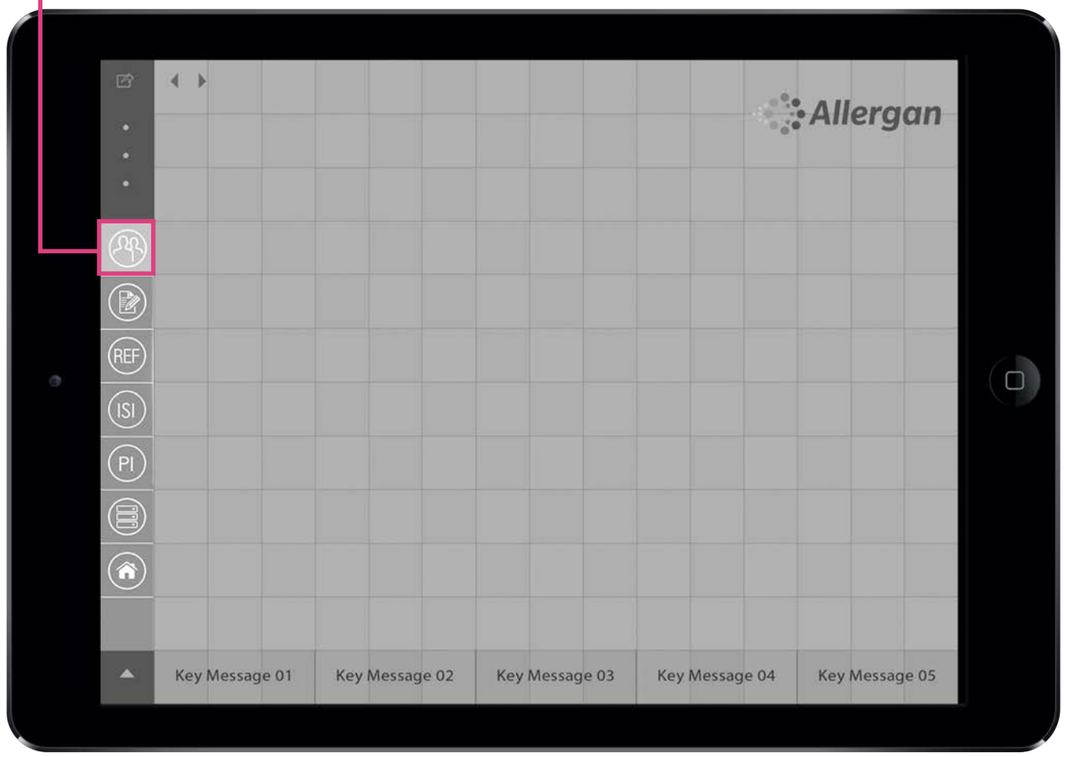

Main Icon

The icon is depicted within a circle of dimensions 96 px diameter (~80% of the grid).

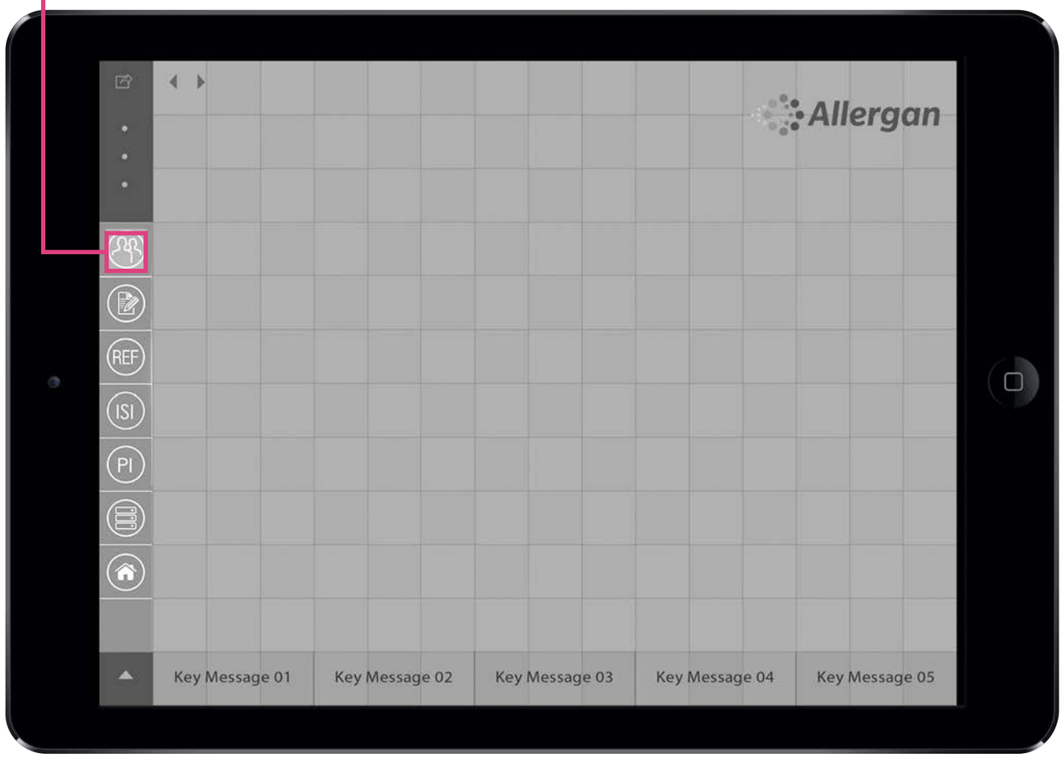


Key Message Buttons



The top 5 key messages are shown in the bottom-most row in their order of priority from left to right.
While the height must always remain the same, the width of the buttons can be altered according to their number.

Menu Screen

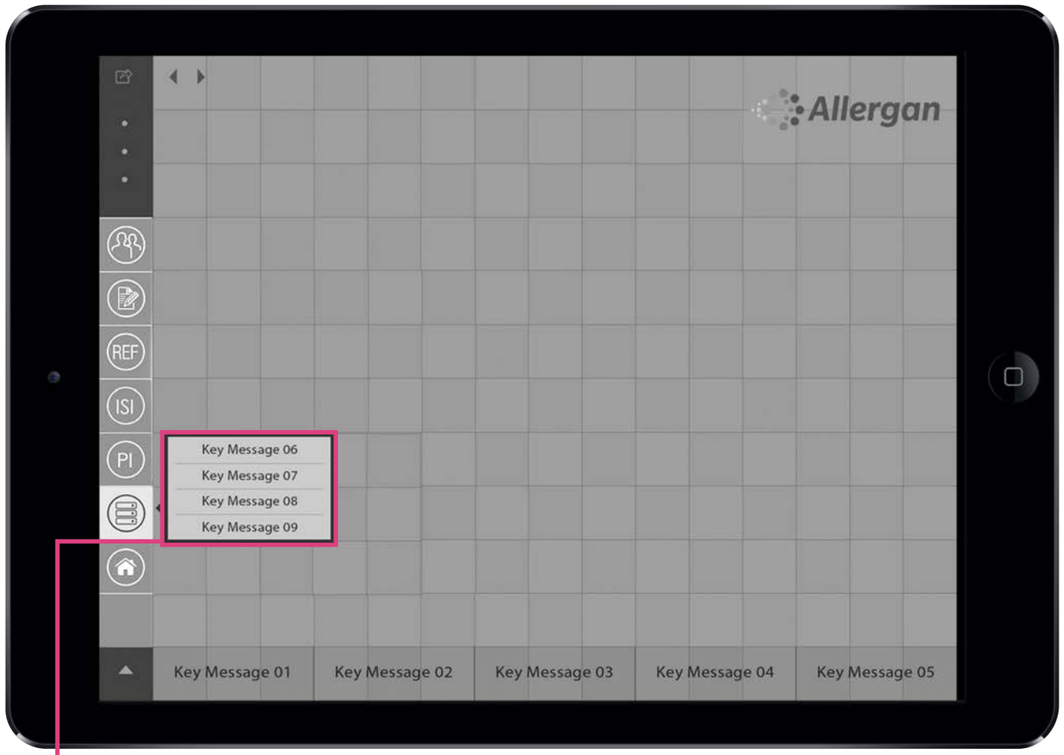

The remaining key messages will appear as a dropdown from the menu icon.


Key Message Titles



The title of the key message will be centre aligned and will occupy 1/3rd the size of the button.


Heading

The heading will be placed in the top-most row with a font size of 24pt.

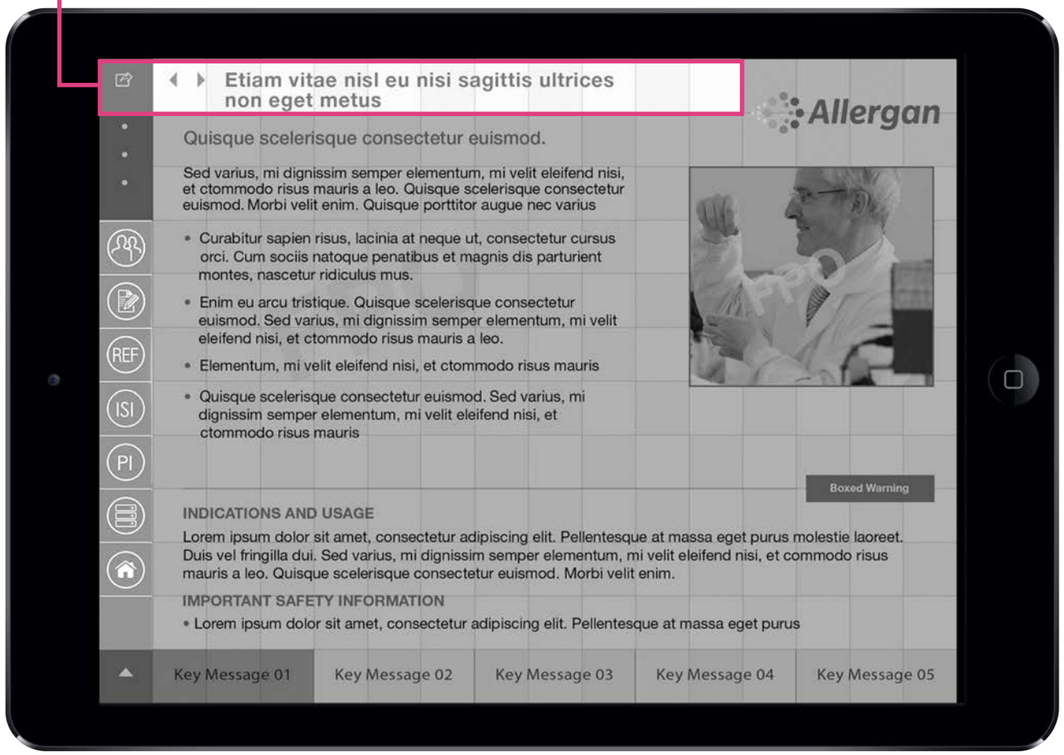


Sub-heading

The second row will be for the sub-heading with a font size of 20pt.

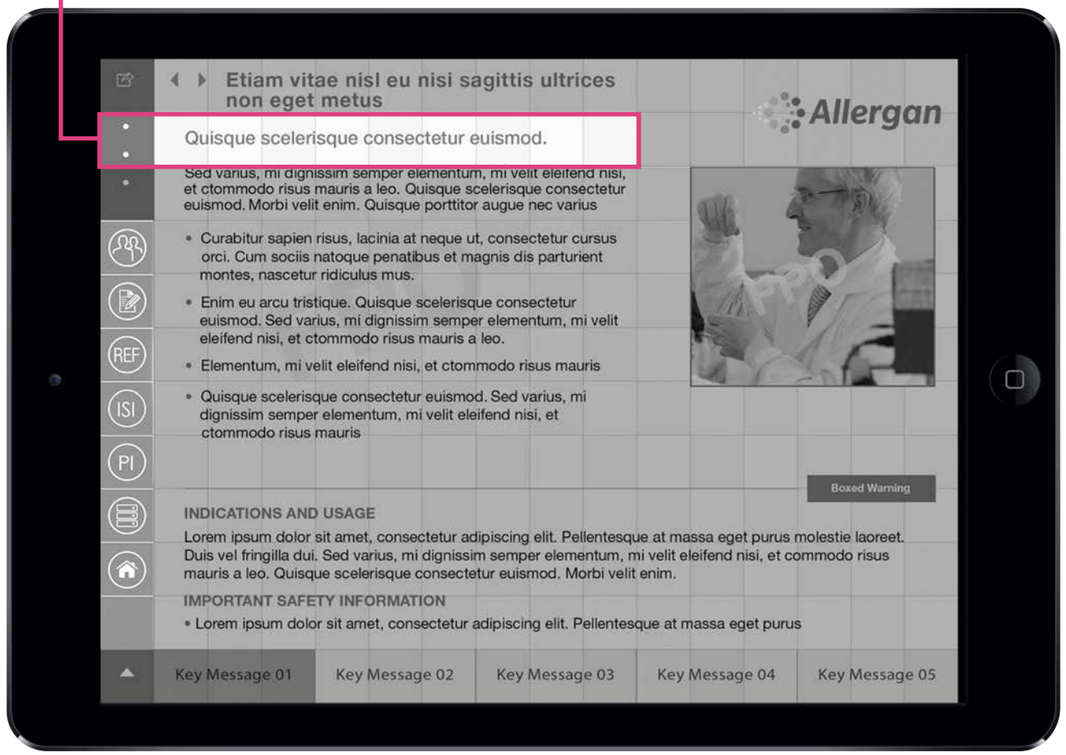


Body Copy

The body copy starts from the third row and the font size will be 18pt.

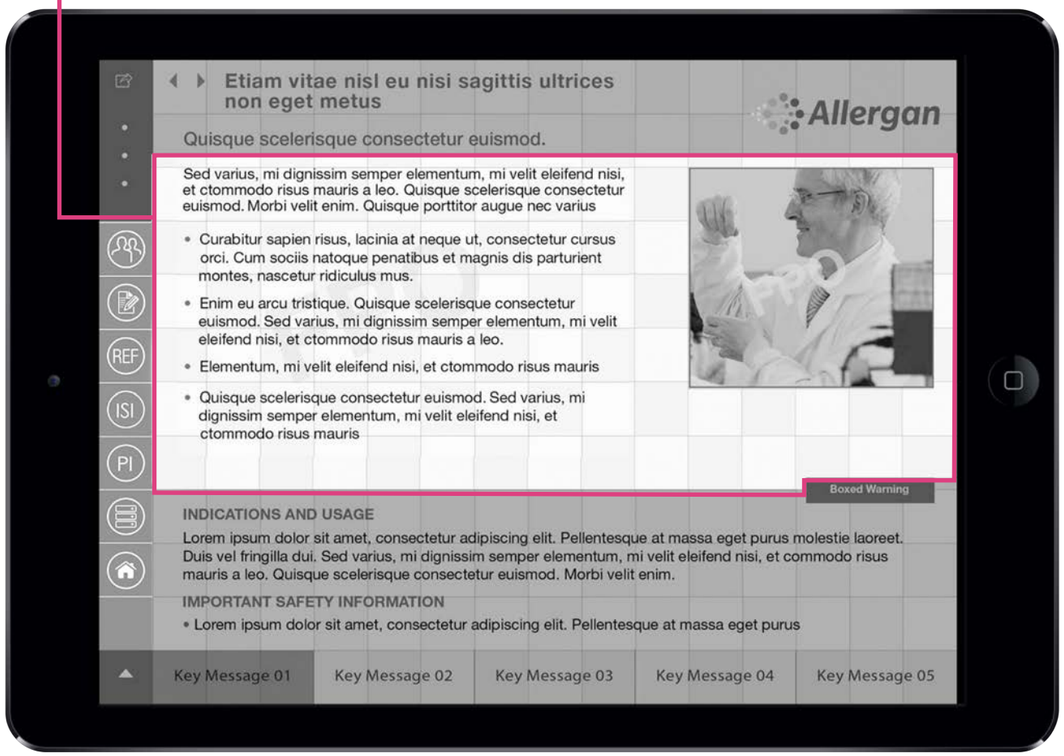


Important Safety Information

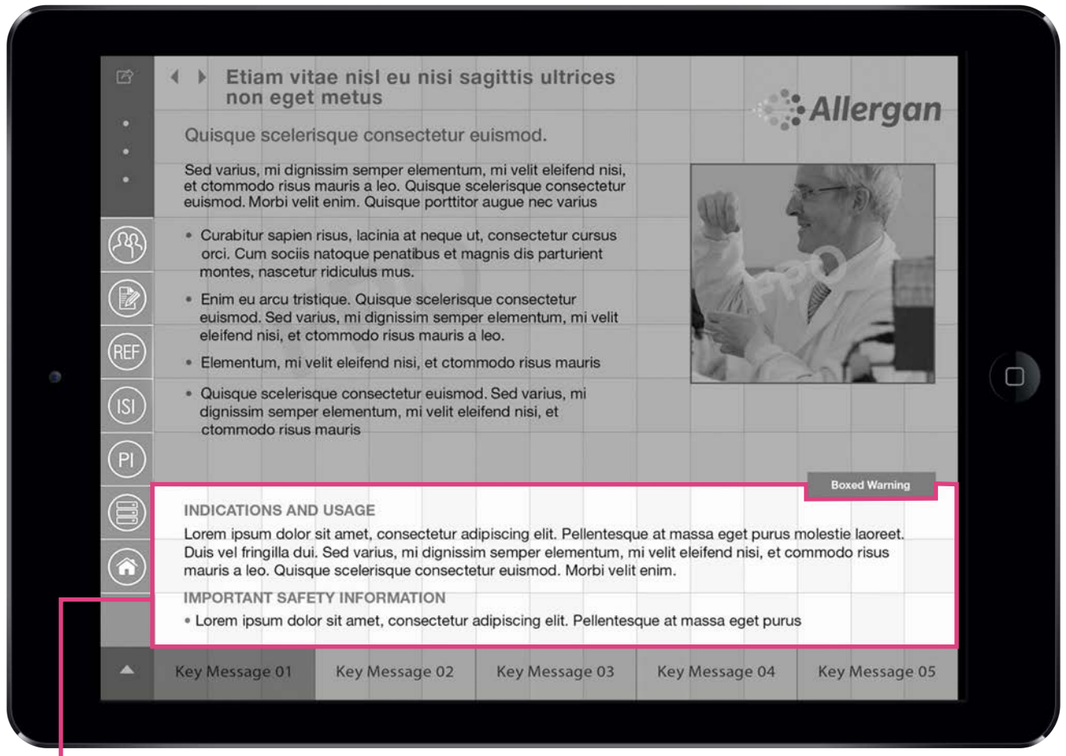


The ISI information will occupy three rows horizontally above the key message buttons.

Boxed Warning Button

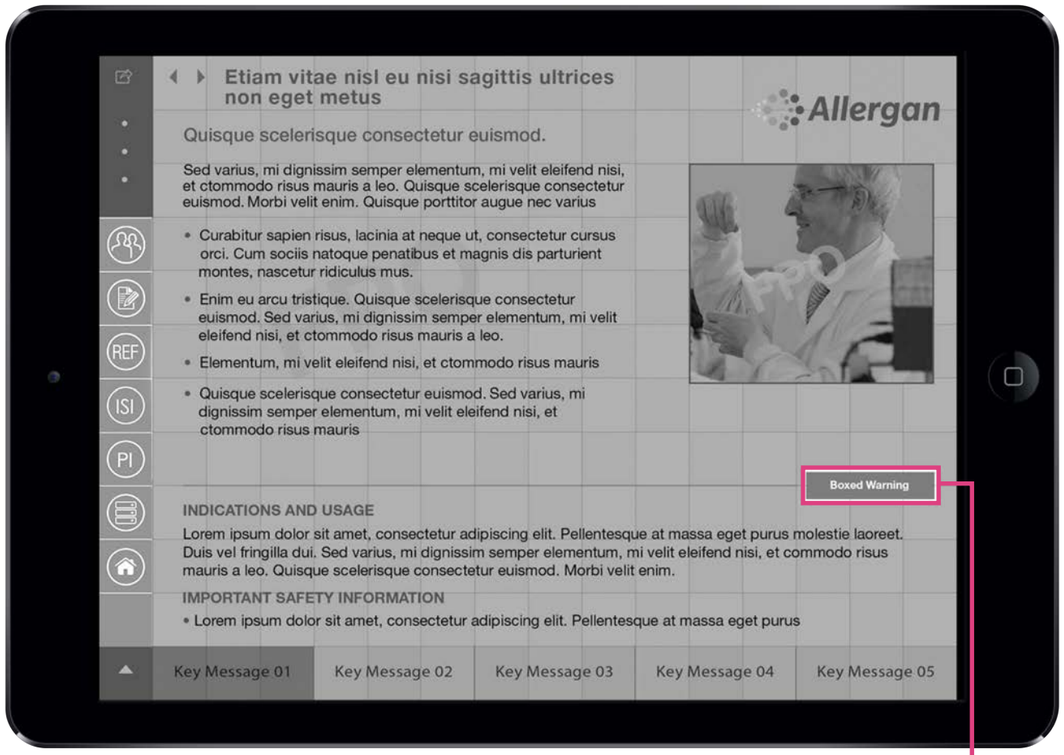

The boxed warning button (when present) is placed to the right of the screen as shown in the image.


Boxed Warning Pop-up

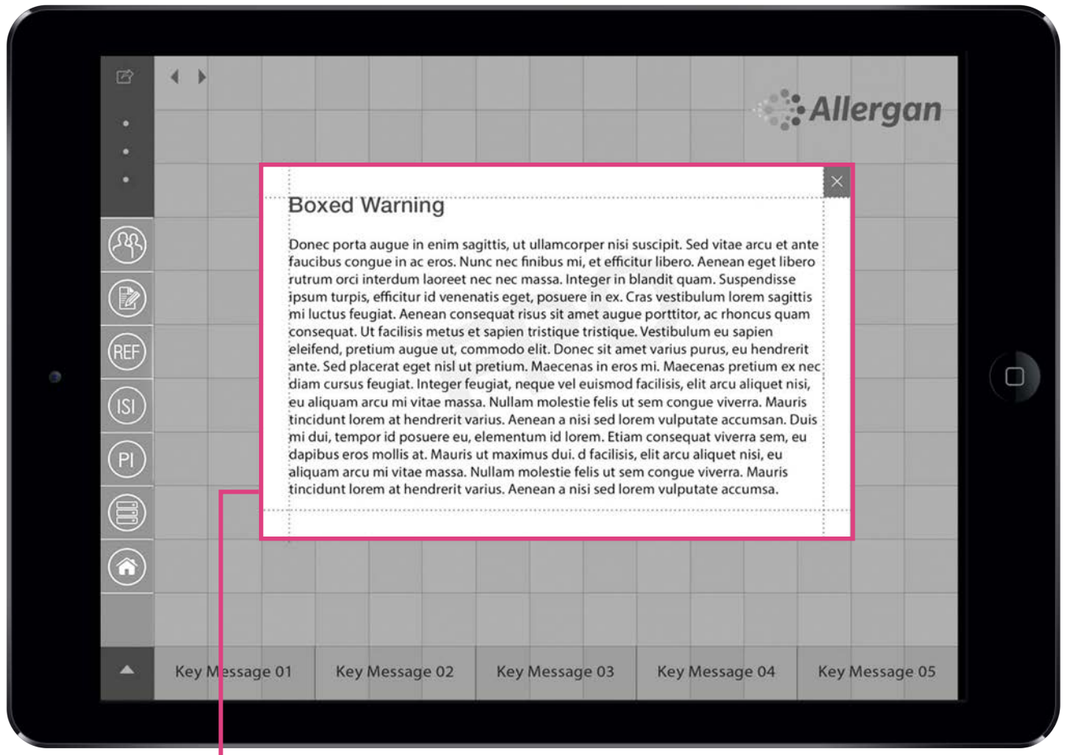

The boxed warning pop–up can occupy 20, 40, 60 or 80% of the screen area.


Zoom Icon

The Zoom icon is placed in a circle which is of the same size as the main icon (96x96px).

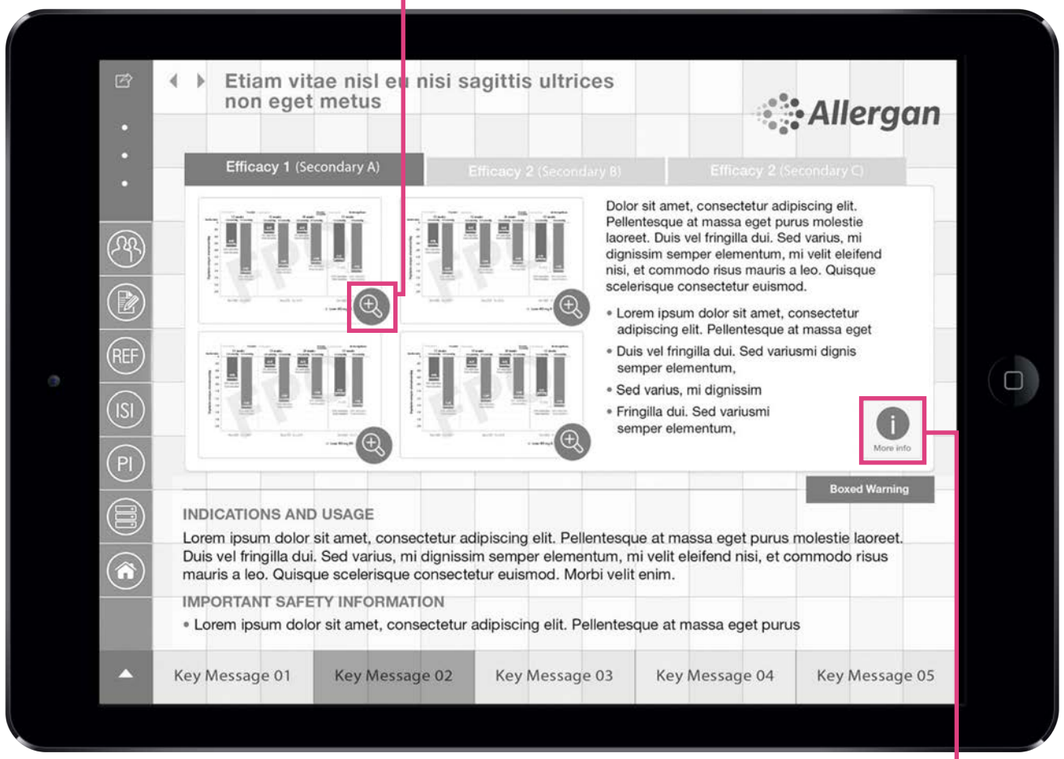

The icon for more information (size 96x96px).


Pop-up (Big)

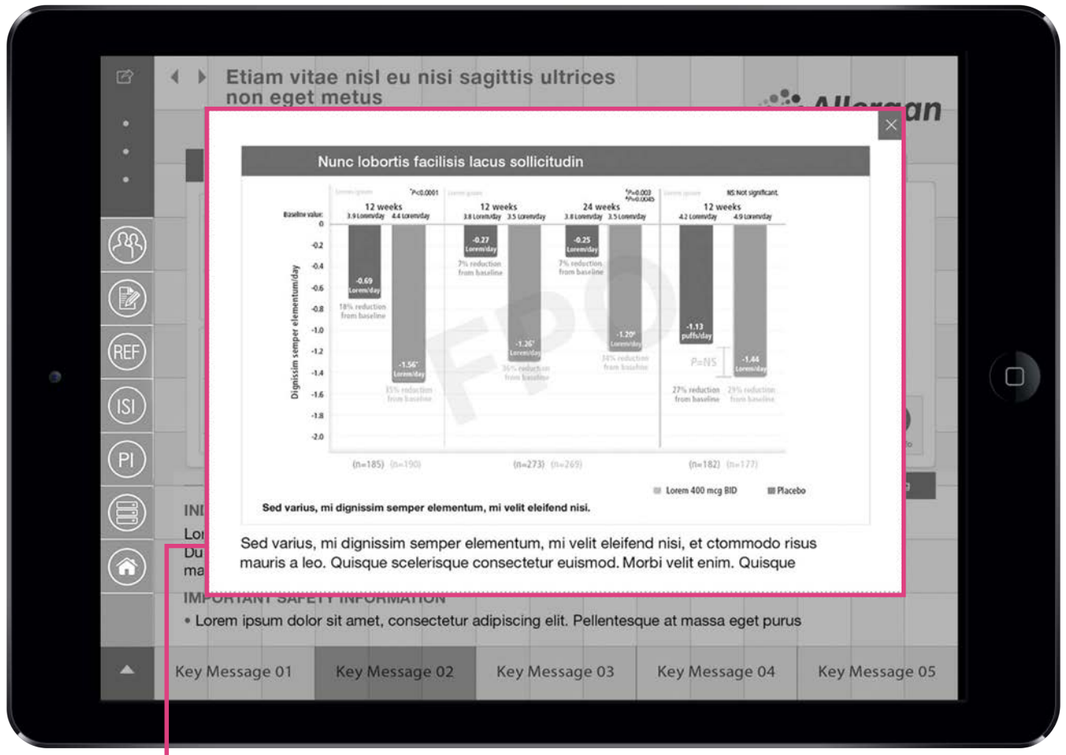


The pop–up window (variation 01) will cover 80% of the screen size.

Pop-up (Small)

The pop up window (variation 02) will cover 60% of the screen size.

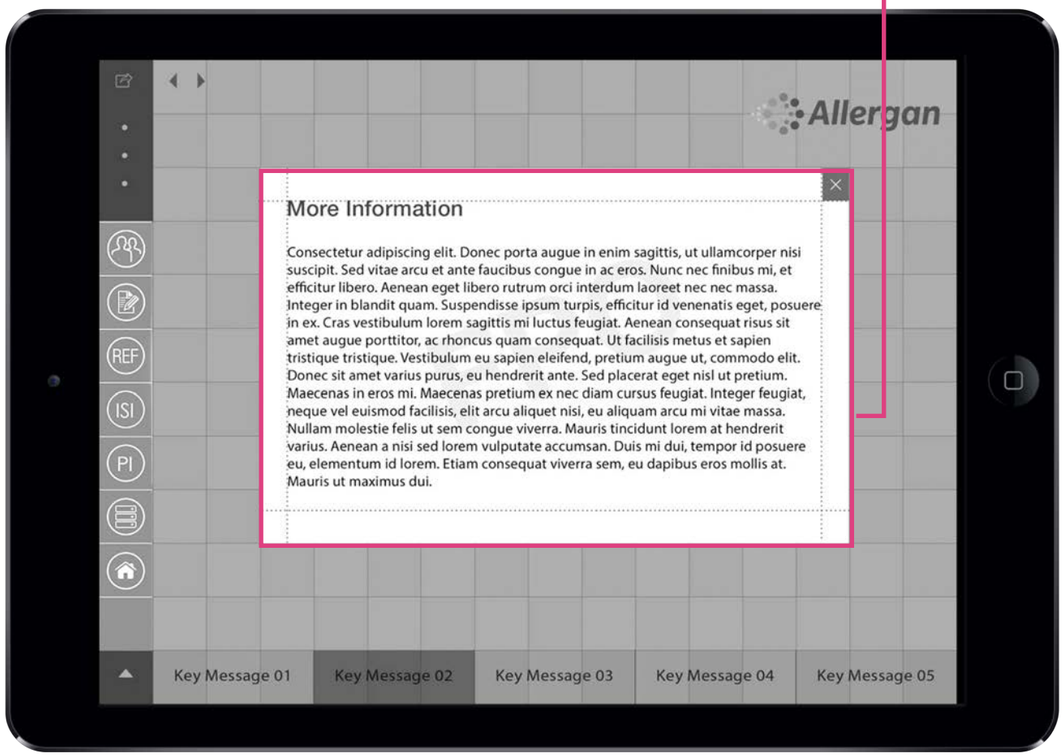


Close Button

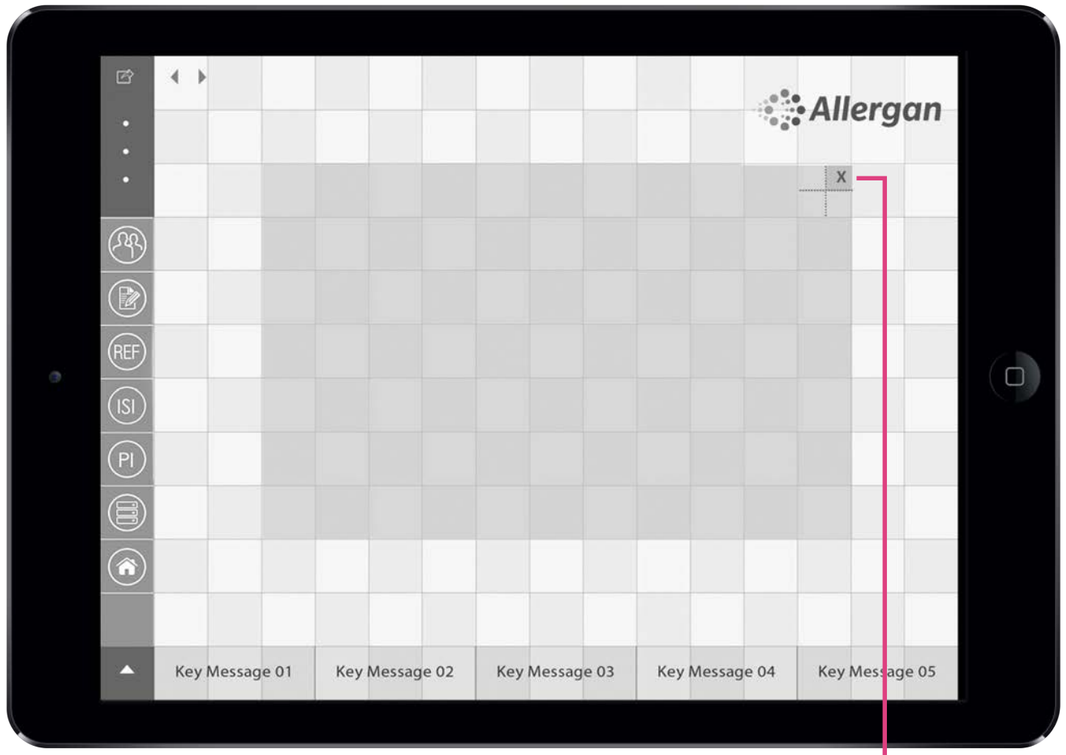

The close button will be 1/4th of the size of the grid.
It will be placed in the top-right corner of the pop-up area.


Video Screen

Video size 6x5 (row & columns)

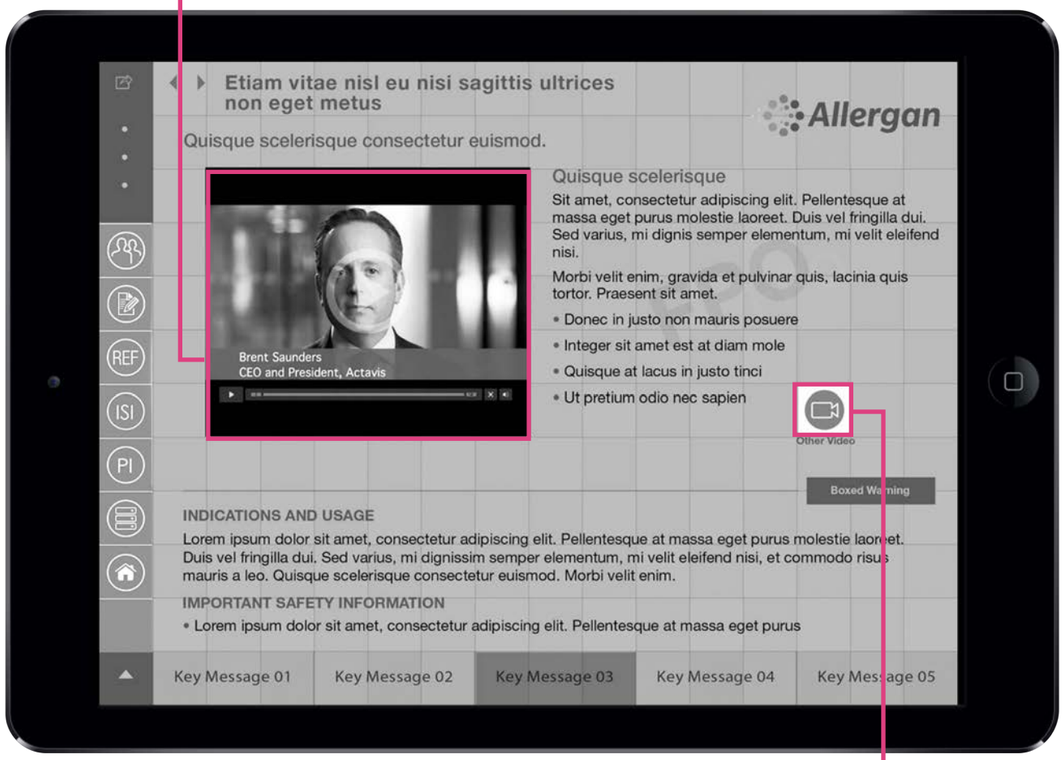

Icon for more videos.

Video Pop-up (Small)

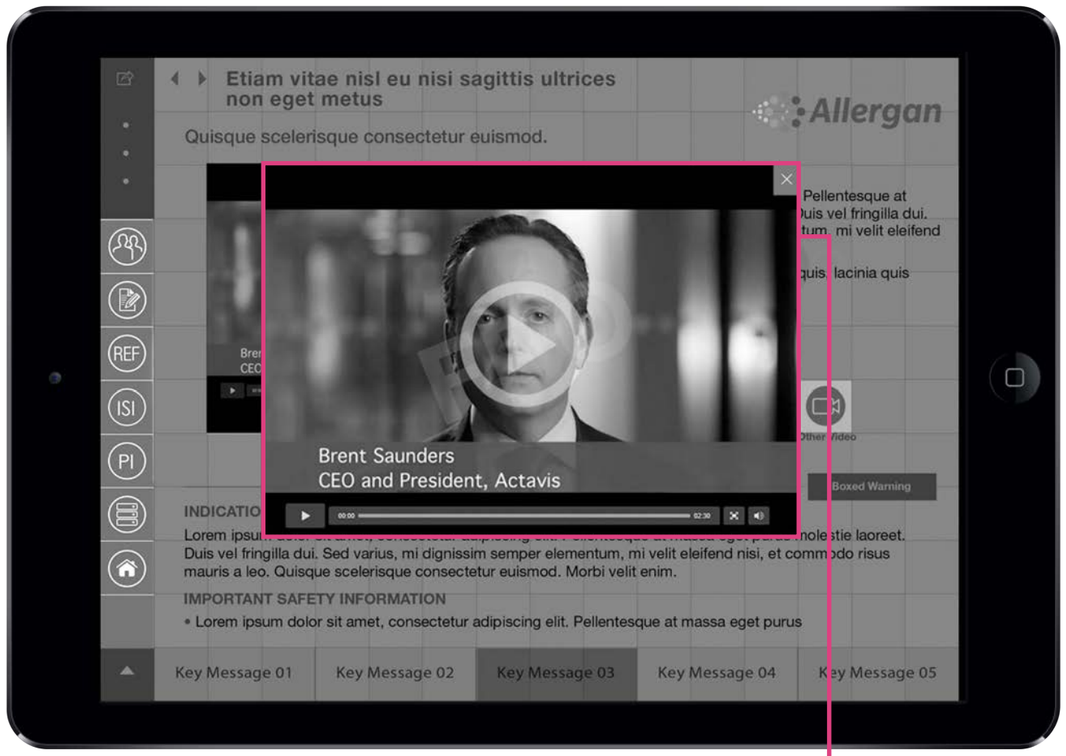

The size of the video pop-up will be 10 x 7 grids.

Full Screen Video




Patients Screen




Individual Patient's Screen

Individual Patient profile will pop-up, occupying 60% of the screen space.

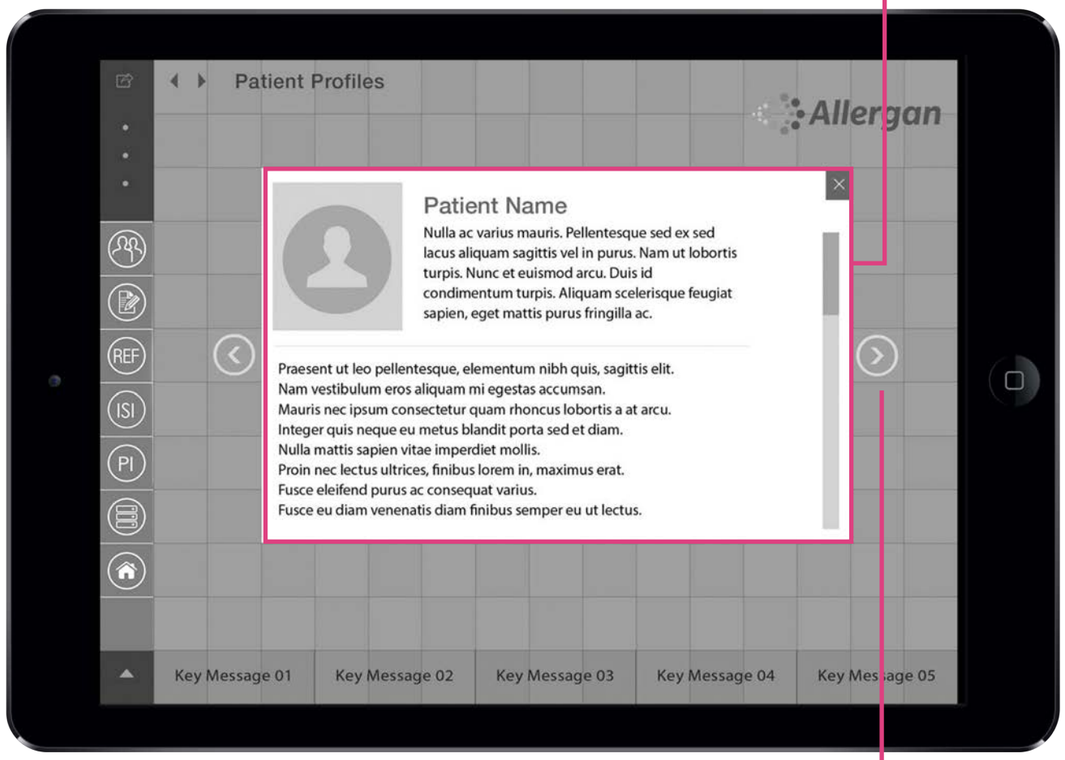

The next & back buttons are in the same size as the icons (96 x 96px).


Internal Toggle Button

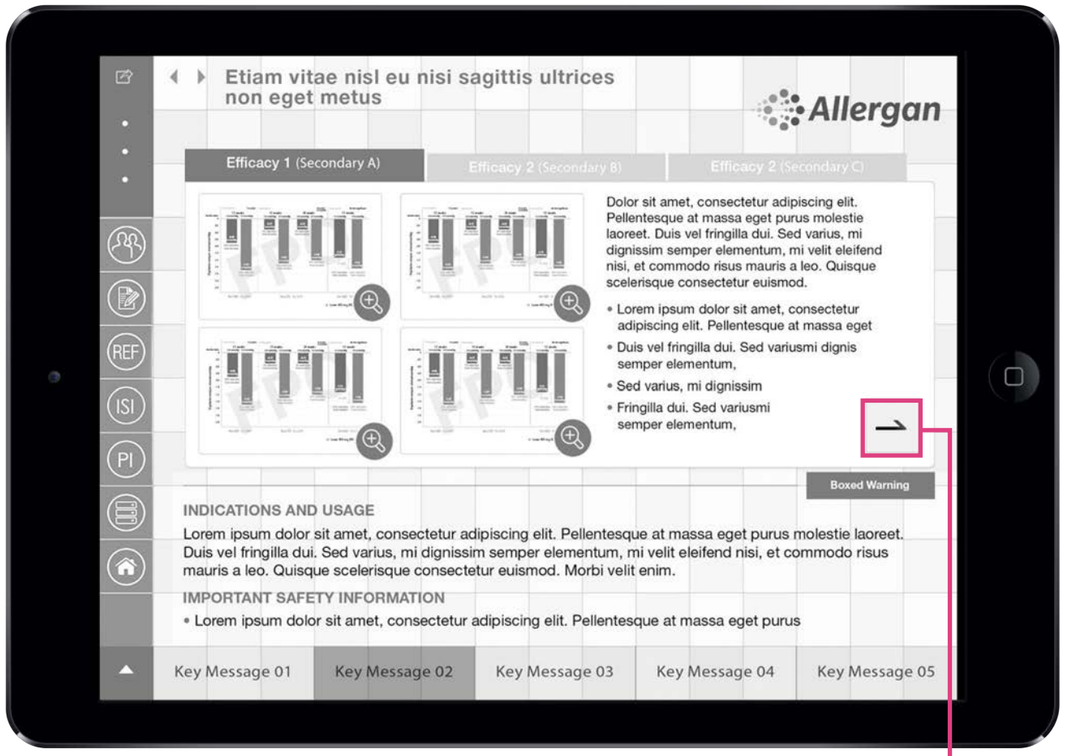

Internal toggle button links to other key messages within the existing eMVA.

VEEVA eMVA DESIGN GUIDE 2.00

Toggle Button

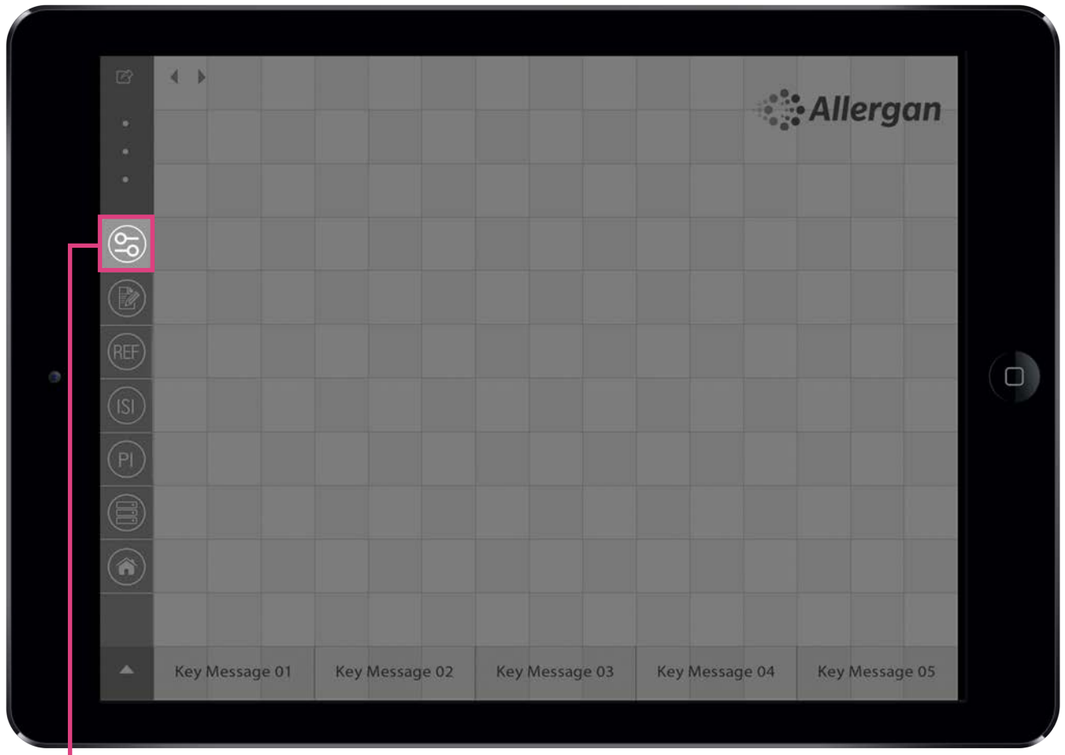

Toggle button links to a similar key message in a different eMVA.