

SPC Analysis Report

Item:	All	AirGauge ID:	All / CH: All	Drawing:	All
Operator:	All	Machine ID:	All	Customer:	

DATA COLLECTION FROM 01/01/2020 TO 22/06/2026

UCL (X)	27.1200819	LCL (X)	27.1193181	UCL (R)	0.0022035	LCL (R)	0.0000000		
σ	0.0004029	CPK_I	20.4351783	CPK_u	4.3848763	CP	12.4100273	CPK	4.3848763
Std Dev	0.0005814	PPK_I	14.1612200	PPK_u	3.0386424	PP	8.5999312	PPK	3.0386424

RESULT: PROCESS IS EXCELLENT


Data Collection (10xN)

S.No	C1	C2	C3	C4	C5	C6	C7	C8	C9	C10
1	27.12000	27.12000	27.11920	27.11880	27.11880					
2	27.11960	27.11880	27.12200	27.12000	27.11960					
3	27.11960	27.12000	27.12000	27.11920	27.12000					
4	27.11960	27.12080	27.12000	27.11960	27.12000					
5	27.12000	27.11960	27.12080	27.11960	27.12040					
6	27.11960	27.11960	27.12040	27.11960	27.11960					
7	27.12040	27.11920	27.12000	27.11960	27.12000					
8	27.11960	27.12000	27.11880	27.11920	27.12000					
9	27.12000	27.11960	27.11960	27.11880	27.11960					
10	27.12000	27.11960	27.11880	27.11960	27.12000					

Column Statistics


Xlarge	27.1204000	27.1208000	27.1220000	27.1200000	27.1204000	X Max=	27.1220000
Xsmall	27.1196000	27.1188000	27.1188000	27.1188000	27.1188000	X Min=	27.1188000
Range	0.0008000	0.0020000	0.0032000	0.0012000	0.0016000	R-Bar=	0.0017600
Avg	27.1198400	27.1197200	27.1199600	27.1194000	27.1198000	X-Bar=	27.1197440

X-Bar Chart

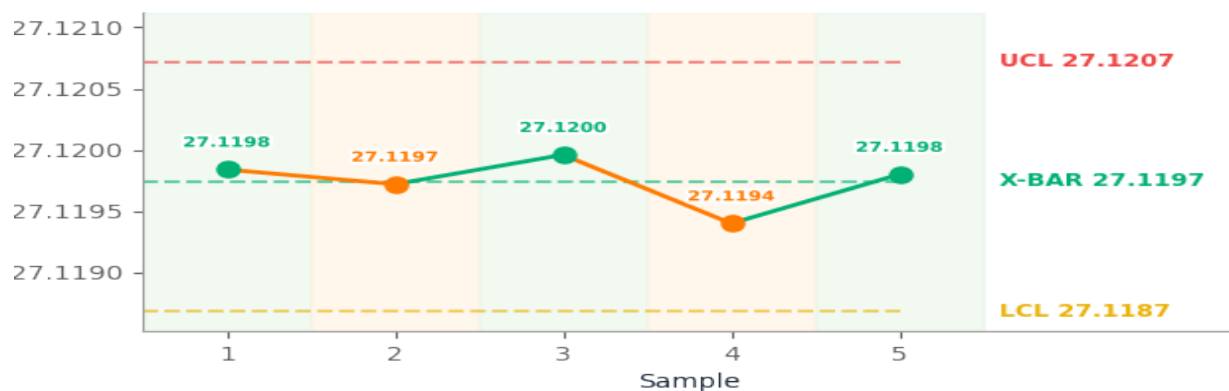


Sample	X-Bar
1	27.11984
2	27.11972
3	27.11996
4	27.11940
5	27.11980

R-Bar Chart

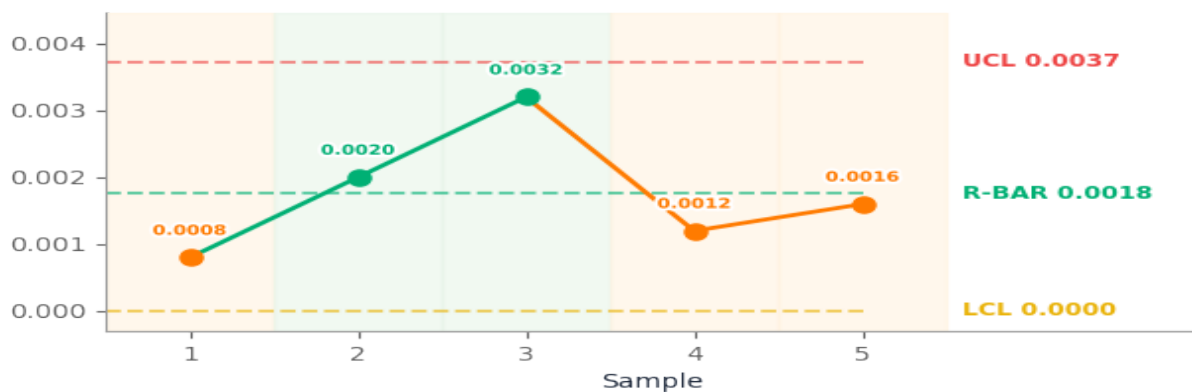

Sample	R-Bar
1	0.00080
2	0.00200
3	0.00320
4	0.00120
5	0.00160

Histogram

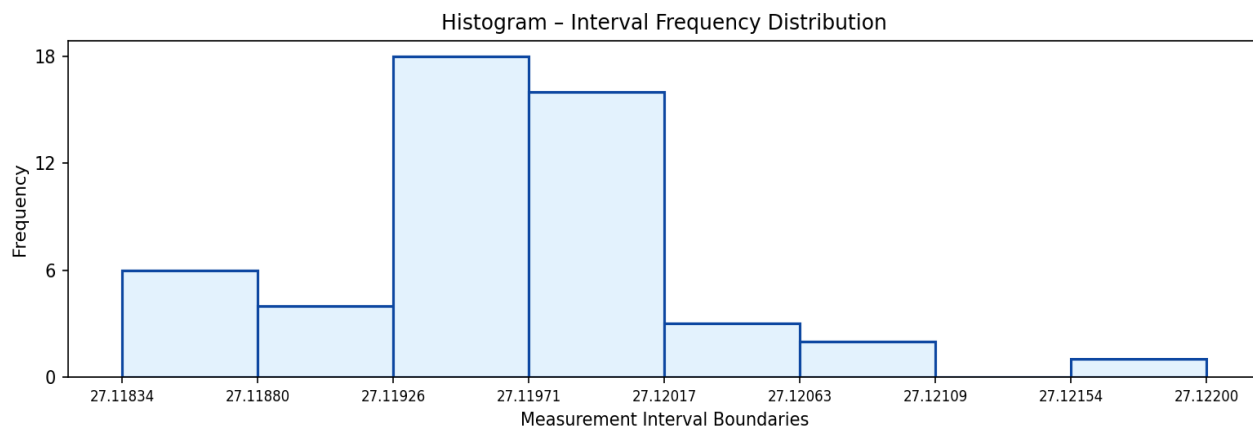

Frequency Distribution

Interval From	Interval To	Cumulative	Frequency
27.11834	27.11880	6	6
27.11880	27.11926	10	4
27.11926	27.11971	28	18
27.11971	27.12017	44	16
27.12017	27.12063	47	3
27.12063	27.12109	49	2
27.12109	27.12154	49	0
27.12154	27.12200	50	1