


Separating measurement, dose and panel as causes of the Tahoe/LINCS disagreement

A Does any restriction reconcile Tahoe with LINCS?



B How stable is the index to panel choice?

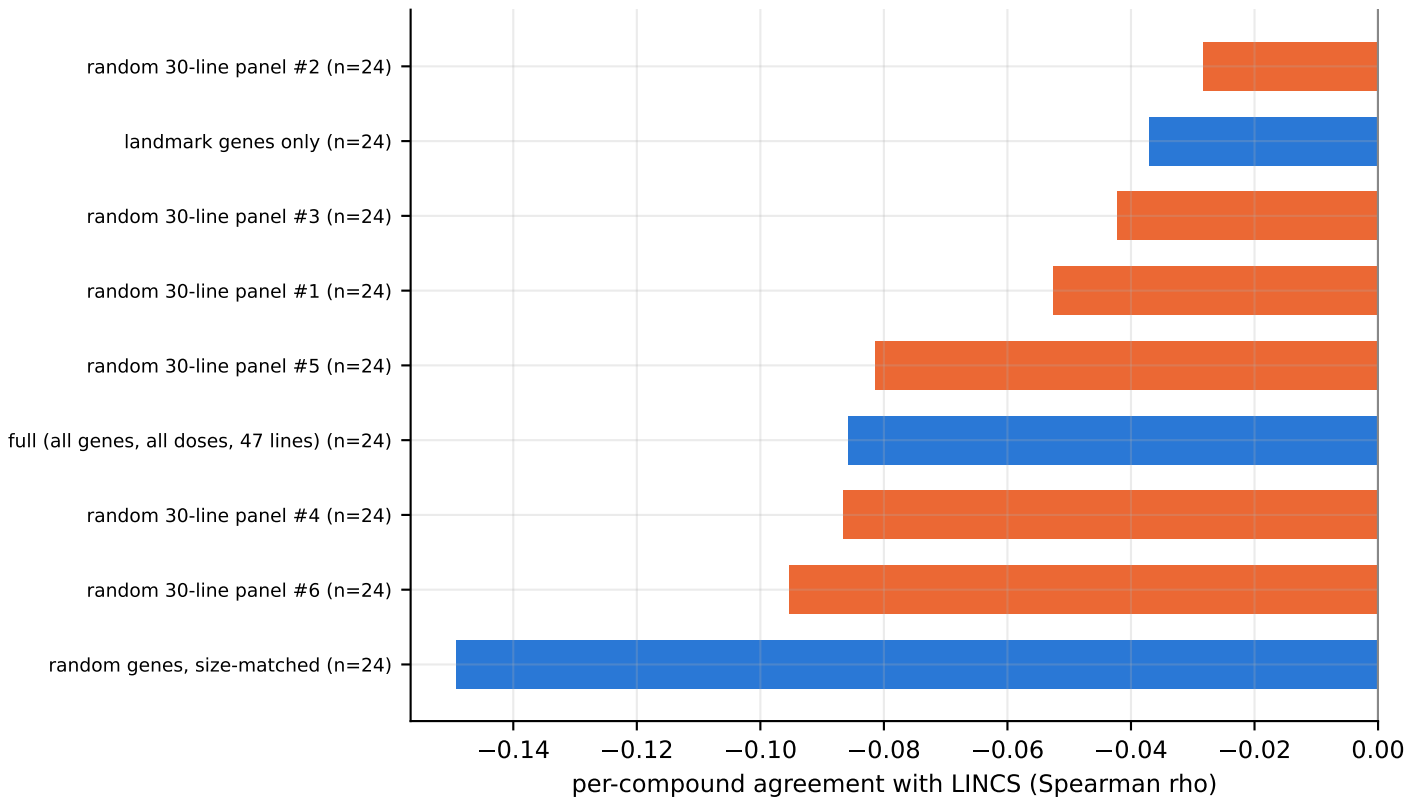