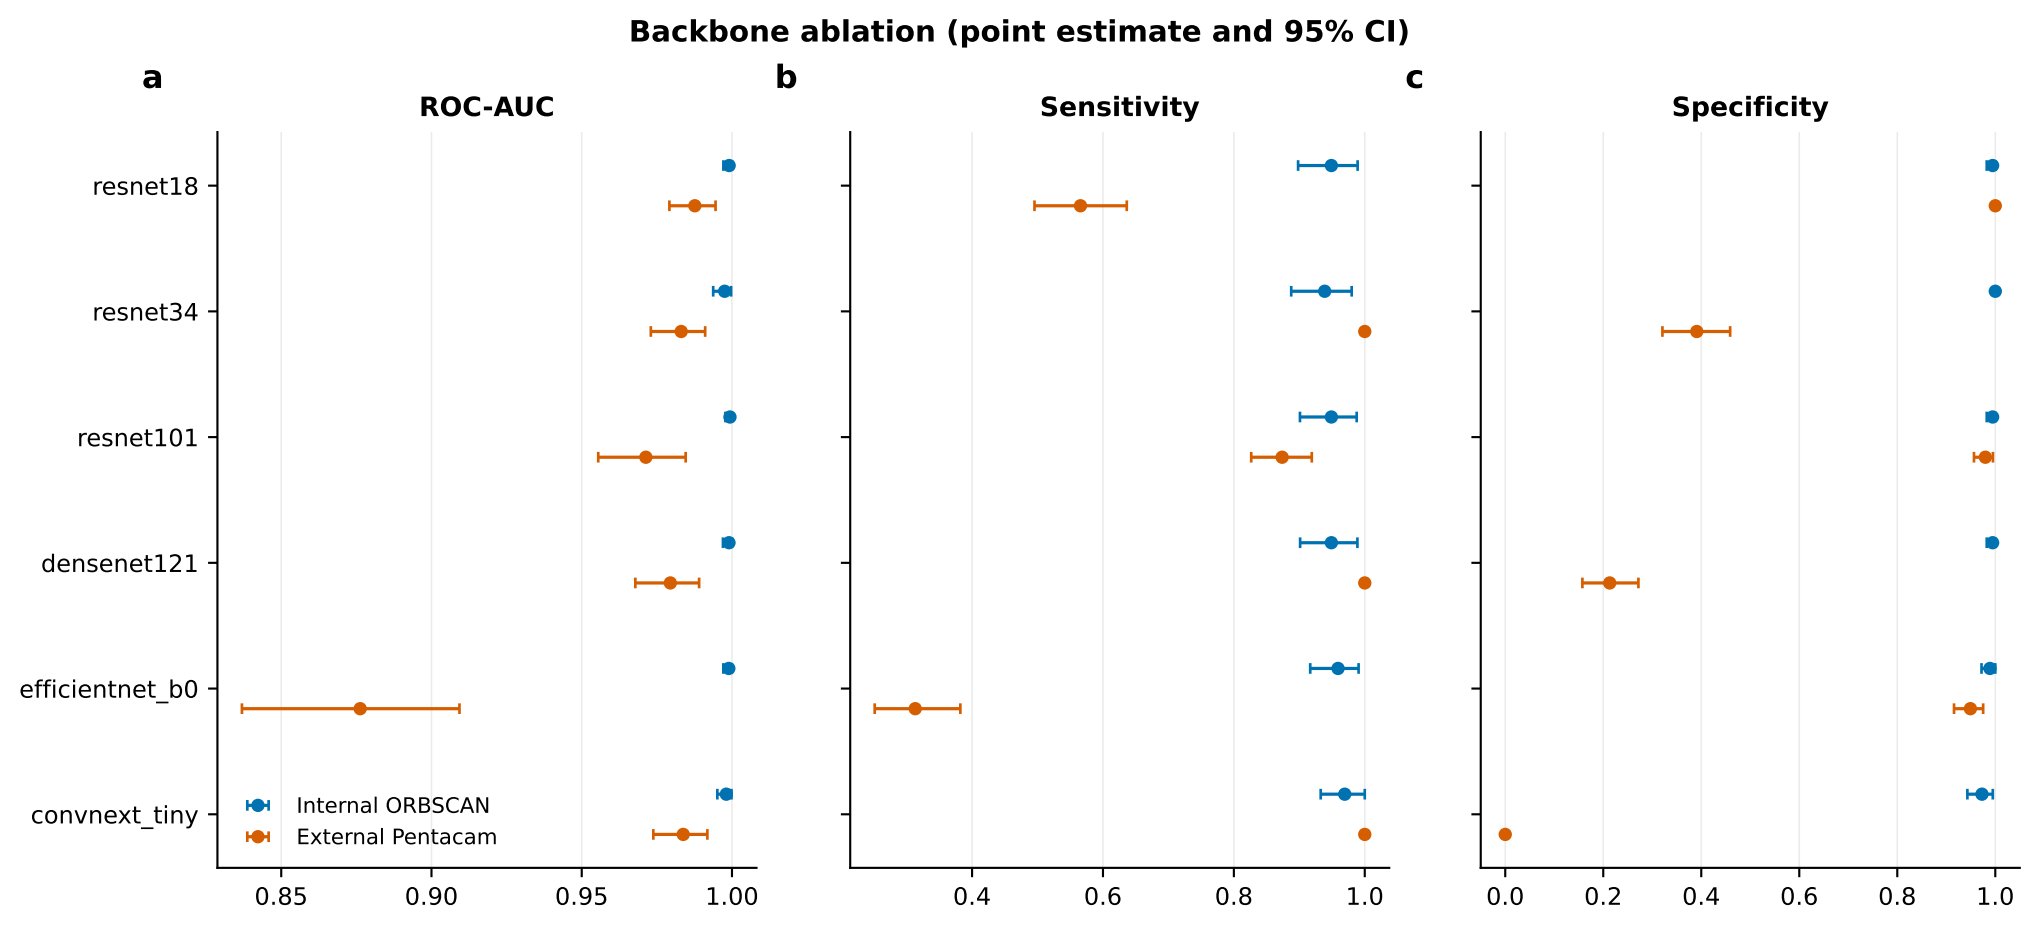
Backbone ablation (point estimate and 95% CI)
a
ROC-AUC
b
Sensitivity
c
Specificity
resnet18
resnet34
resnet101
densenet121
efficientnet_b0
convnext_tiny
Internal ORBSCAN
External Pentacam
0.85
0.90
0.95
1.00
0.4
0.6
0.8
1.0
0.0
0.2
0.4
0.6
0.8
1.0