FOR REFERENCE ONLY

Maximum load and torque requirements for this system have been acknowledged and it is confirmed by signing this document, that proper provisions at the constructions site have been made or will be implemented

△ Measurements to be checked by Dräger on site.

separate preinstallation material:

1 × G25210 ceiling fixture set

Cable and hose length outside of ceiling bearing 1000mm.

minimum concrete thickness 200mm
concrete grade C20/25

brakes:
F = Friction brake
E = Electromagnetic brake

(1) 4x OP75579 Shelf 1,5B/480 with US rails(GG16040 (1320)) Powder-coated aluminum shelf for the column of a supply unit with an usable surface of 630x480 mm and side plastic caps with integrated Fairfield rails, which have a maximum load of 10kg in each case.

(2) G95048 remote control double arm lift

(3) G39800 Handle with sensoric lift

(4) G39960 Handle with sensoric

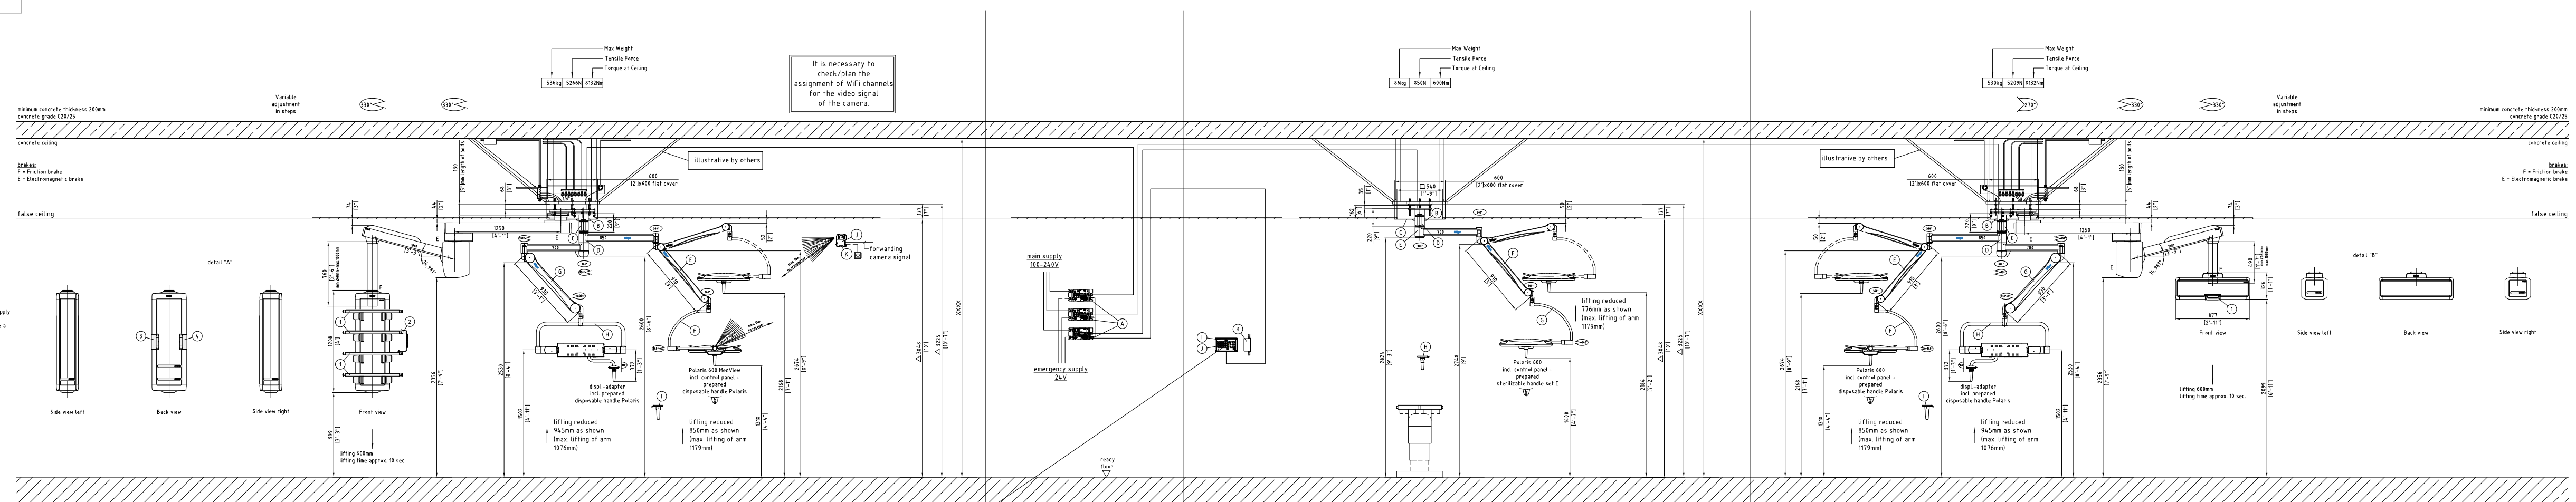

Pos.	No/pc	Order-no.	Description	
A	1	G36402	PSU 100-240V Polaris 600	pre installation
B	1	GG10153	clamp ring ∅110, outside diamenter 160mm	pre installation
C	1	G94400	suspension tube ∅110x220mm	pre installation
D	1	G97958	axis 2-fold MOX/L1	
E	1	G36699	spring load arm Polaris 100/200/600 incl. cabling	
F	1	OP75085	Polaris 600 MedView/prepared disposable handle Polaris	
G	1	G28374	spring arm display 17-26 MOX SD/HD incl. cabling	
H	1	G35462	1 displ.-adap. 24-32" Disp.	
I	60	MP05700	disposable handle Polaris, dual	
J	1	G36478	wireless video receiver HDMI NALA	
K	1	G37030	wireless video receiver box wall	

Pos.	No/pc	Order-no.	Description	
A	1	G36402	PSU 100-240V Polaris 600	pre installation
B	1	G19756	flat cover ∅144	pre installation
C	1	G15796	clamp ring ∅110	pre installation
D	1	G94400	suspension tube ∅110x220mm	pre installation
E	1	G97955	axis 1-fold L1 700	
F	1	G36699	spring load arm Polaris 100/200/600 incl. cabling	
G	1	OP75084	Polaris 600/prepared sterilizable handle set E	
H	1	G36993	sterilizable handle set E (2 pcs)	
I	1	G33880	front cover WCU P6+P6+P6+camera	
J	1	G36708	WCU lights + camera P600	
K	1	G50741	wall box FM 250	pre installation

Pos.	No/pc	Order-no.	Description	
A	1	G36402	PSU 100-240V Polaris 600	pre installation
B	1	GG10153	clamp ring ∅110, outside diamenter 160mm	pre installation
C	1	G94400	suspension tube ∅110x220mm	pre installation
D	1	G97958	axis 2-fold MOX/L1	
E	1	G36699	spring load arm Polaris 100/200/600 incl. cabling	
F	1	OP75084	Polaris 600/prepared disposable handle Polaris	
G	1	G28374	spring arm display 17-26 MOX SD/HD incl. cabling	
H	1	G35462	1 displ.-adap. 24-32" Disp.	
I	60	MP05700	disposable handle Polaris, dual	

detail "assembly"
M. 1:10

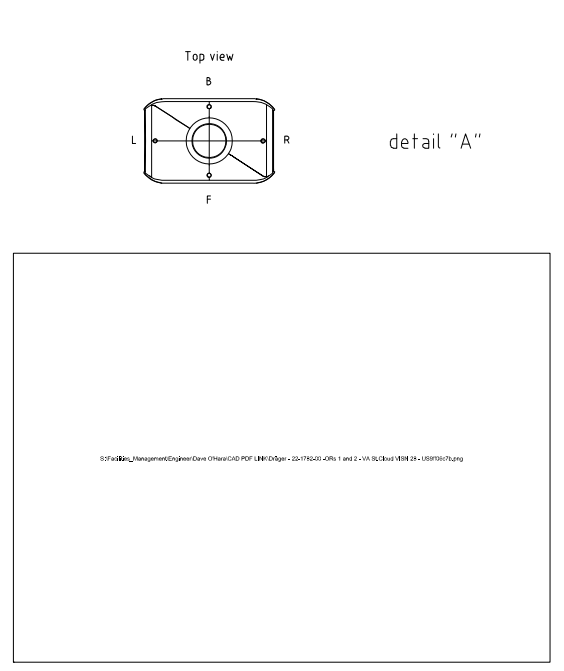

Electrical outlets:

Ambia - Hubbell E socket Hospital Grade (NFPA-70)

Position	Text	circuit
F -55/246	Duplex Receptacle, 125V, 20A, red, backbox	2
F -55/408	Duplex Receptacle, 125V, 20A, red, backbox	2
F -55/576	Duplex Receptacle, 125V, 20A, red, backbox	3
F -55/747	Duplex Receptacle, 125V, 20A, red, backbox	3
F -55/911	Duplex Receptacle, 125V, 20A, red, backbox	4
B -55/154	Duplex Receptacle, 125V, 20A, red, backbox	5
B 55/154	Duplex Receptacle, 125V, 20A, red, backbox	6

Gas outlets:

DISS gas terminal unit Beacon Medaes - US

Position	Text
R 0/607	AIR_1
L 0/531	AIR_2
R 0/180	CO2_1
L 0/400	CO2_2
B 55/500	N2_1
R 0/450	O2_1
R 0/800	VAC_1
L 0/850	VAC_2

Other outlets:

AK Cutouts

Position	Text
B 0/650	1362 - Cut out „N2-Control Panel US"

Ambia - Hubbell (NFPA-70)

Position	Text	comment
B 55/300	Blind plate 1-gang, backbox without conduit	Maximum short-circuit power over 10 VA: yes
B -55/300	Blind plate 1-gang, backbox without conduit	Maximum short-circuit power over 10 VA: yes
F 55/408	Blind plate 1-gang, backbox without conduit	Maximum short-circuit power over 10 VA: yes
F 55/576	Blind plate 1-gang, backbox without conduit	Maximum short-circuit power over 10 VA: yes
F 55/911	Blind plate 1-gang, backbox without conduit	Maximum short-circuit power over 10 VA: yes
L 0/220	Blind plate 1-gang, backbox without conduit	Maximum short-circuit power over 10 VA: yes
F 55/246	4x RJ45, white, backbox without conduit	Power over Ethernet (PoE) available: yes

Ambia controls

Position	Text
R 0/283	Touchpanel brake/lift 2arm
R -20/353	Service socket
R 22,5/356	Switch lift stop

Ambia rails

Position	Text
B 0/800	Fairfield rail 280
B 0/950	Fairfield rail 280
L 0/950	Fairfield rail 180
R 0/950	Fairfield rail 180



Electrical outlets:

Ambia - Hubbell E socket Hospital Grade (NFPA-70)

Position	Text	circuit
F 0/580	Duplex Receptacle, 125V, 20A, red, backbox	2
F 0/670	Duplex Receptacle, 125V, 20A, red, backbox	2
B 0/70	Duplex Receptacle, 125V, 20A, red, backbox	3
F 0/760	Duplex Receptacle, 125V, 20A, red, backbox	3
U 0/670	Duplex Receptacle, 125V, 20A, red, backbox	4
U 0/760	Duplex Receptacle, 125V, 20A, red, backbox	4

Gas outlets:

DISS gas terminal unit Beacon Medaes - US

Position	Text
B 0/180	AIR_1
F 0/460	AIR_2
B 0/320	N2O_1
B 0/740	O2_1
B 0/600	O2_2
L 0/160	VAC_1
L 0/50	VAC_2
B 0/460	WAGD_1

Other outlets:

Ambia - Hubbell (NFPA-70)

Position	Text	comment
F 0/160	Blind plate 1-gang, backbox without conduit	phillips Maximum short-circuit power over 10 VA: yes
F 0/70	Blind plate 1-gang, backbox without conduit	Easyport Maximum short-circuit power over 10 VA: yes
F 0/250	6x RJ45, white, backbox without conduit	Power over Ethernet (PoE) available: yes
F 0/340	4x RJ45, white, backbox without conduit	Power over Ethernet (PoE) available: yes

Ambia controls

Position	Text
R 0/60	Touchpanel brake/lift 2arm
R 20/140	Switch lift stop
R -20/140	Service socket

Ambia rails

Position	Text
L -68,5/111	Fairfield rail 180
R -68,5/111	Fairfield rail 180

top view M. 1:20

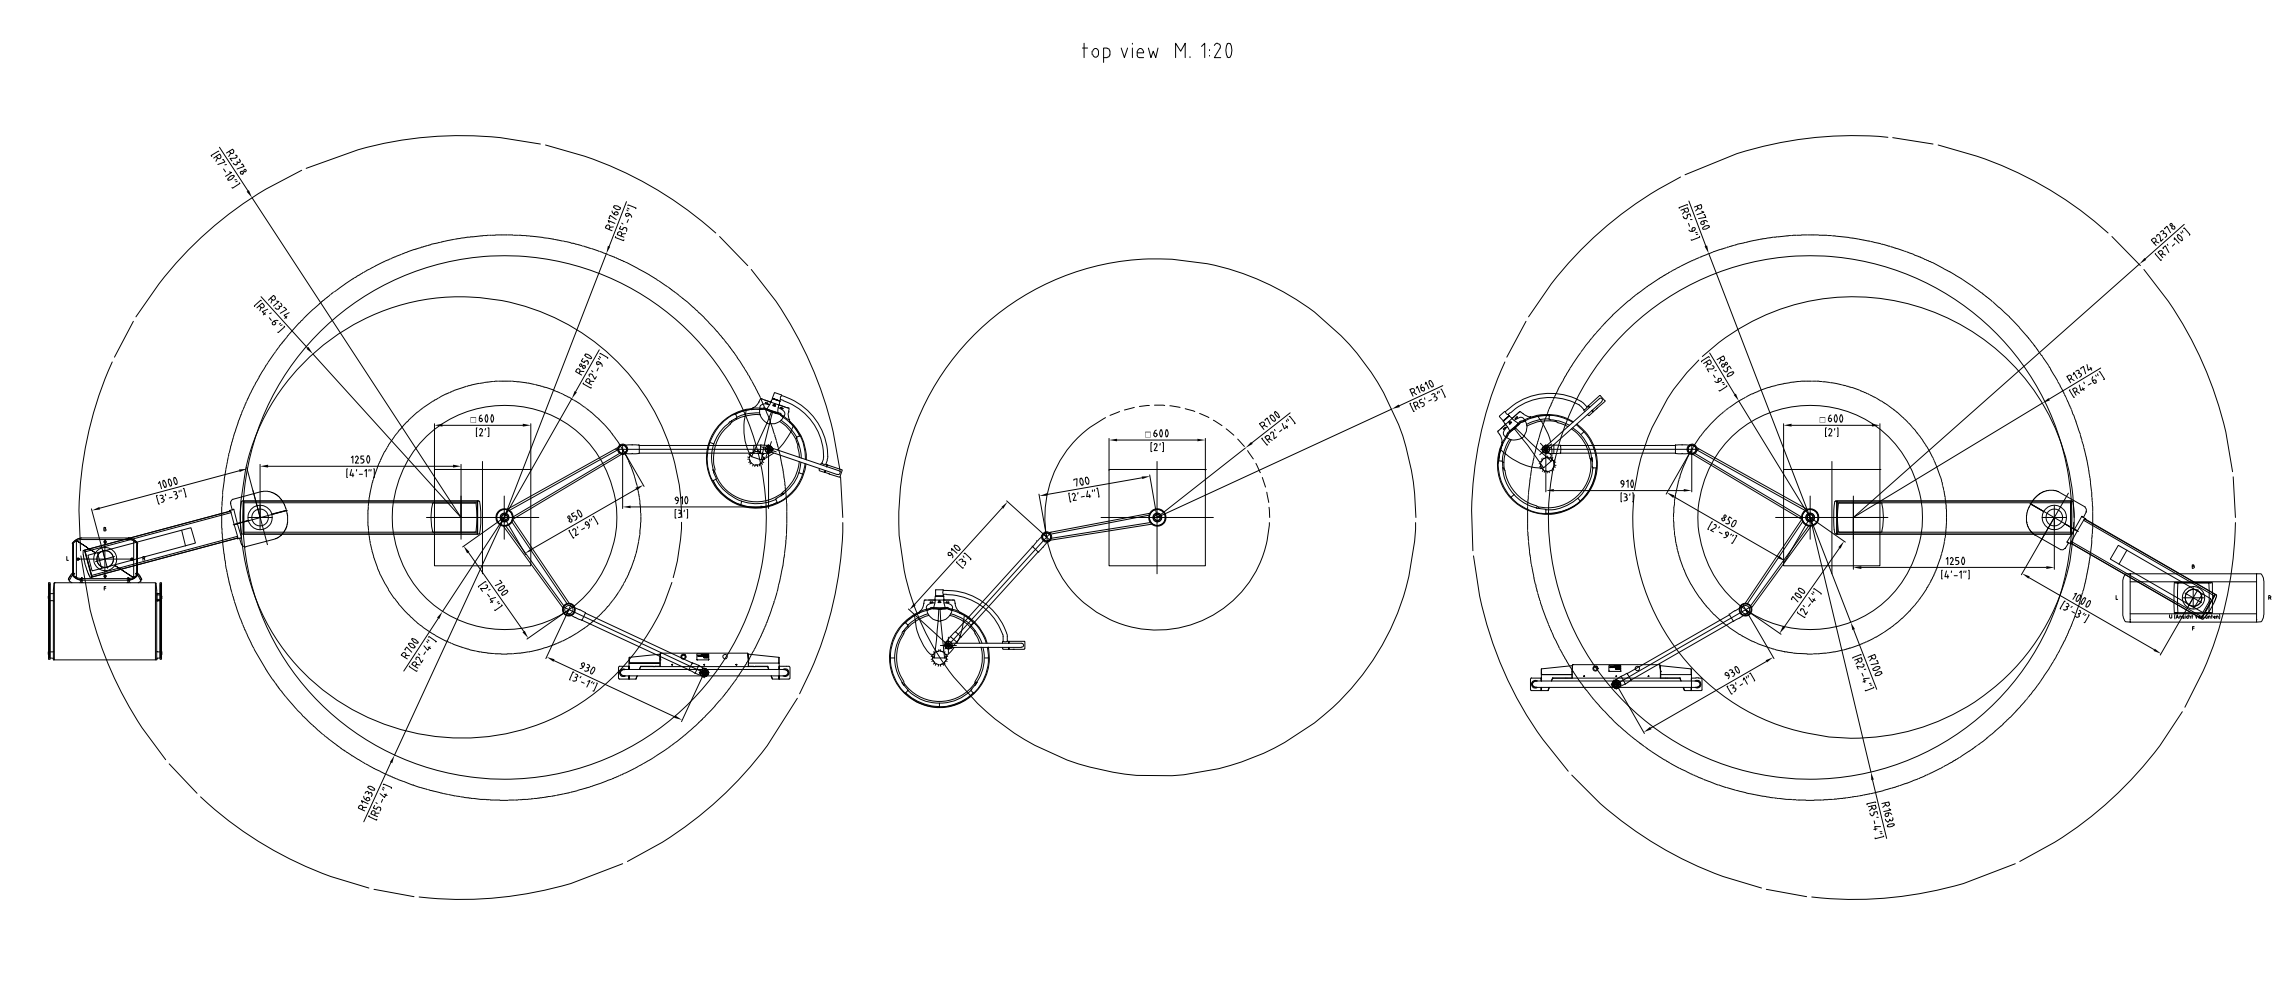

Regulatory information

The safety distance from empty installations shall be 200mm if it is intended to use them with electrical installations and medical gas outlets for oxidizing gases.

The safety distance of 200mm to oxidizing gases can be undercut if the electrical installations do not reach a power >10VA in the first fault case (e.g. short circuit).

Dräger Medical Supply Units shall not be installed in rooms, where combustible or explosive gases can occur.

Dräger Medical Supply Units shall not be installed in MRI rooms with high Tesla levels.

If installations or devices are installed, which have not been approved by Dräger, these installation or devices needs an on-site approval.

date:	author:	revision text:	index:

projectname + department: VA St. Cloud VISN 23

Dräger-country code: US | voltage (V): 120/240 | frequency (Hz): 60 | target country: United States

LV-Pos.: --

room-no. + roomname: OR 1 + 2

quantity of units: 2 pcs.



(1) equipment color: Medical White W1100/S-0500-N
(2) service plate: anodized
(3) Color frame: Medical White W1100/S-0500-N

scale: view: 1:20, rest: see details

author: date: 2022-08-10 name: RÜHMANN
approved: date: 2011-08-12 name: BRINKER/JANACK

title:
Ceiling supply unit
type: Polaris 600 (article-number: G16720)

Ceiling supply unit
type left: Ambia (article-number: GG16010)
type right: Polaris 600 (article-number: G16720)

Ceiling supply unit
type left: Ambia (article-number: GG16010)
type right: Polaris 600 (article-number: G16720)

Dräger

revision index: 00 | number: 22-1732

size A0+630