
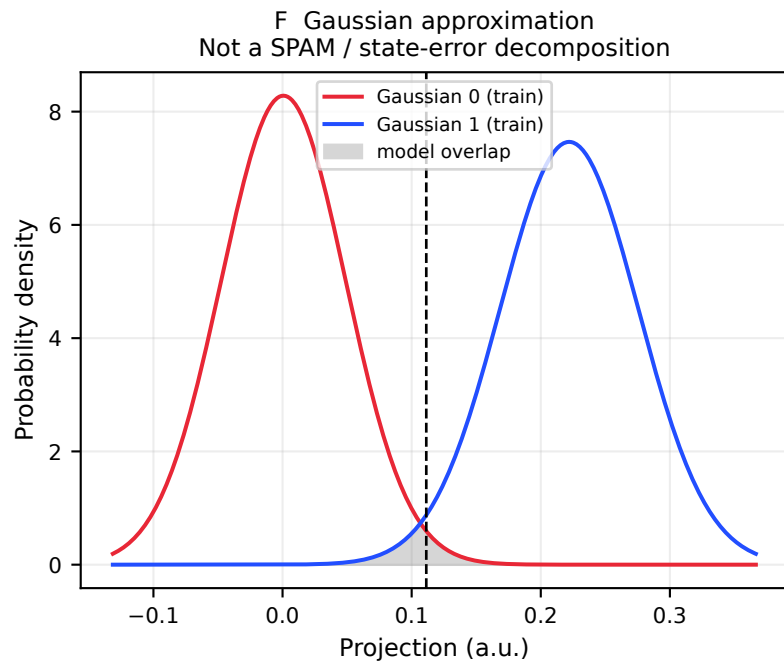
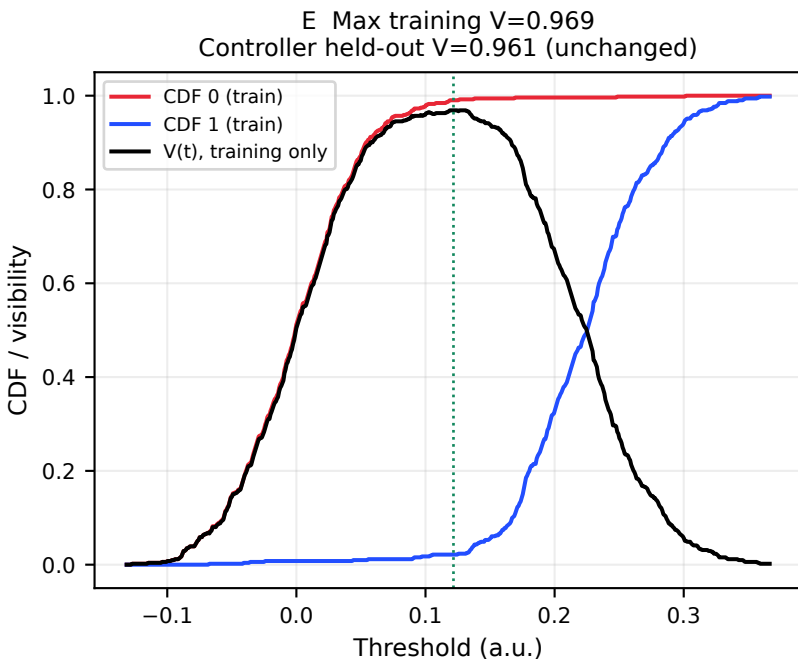
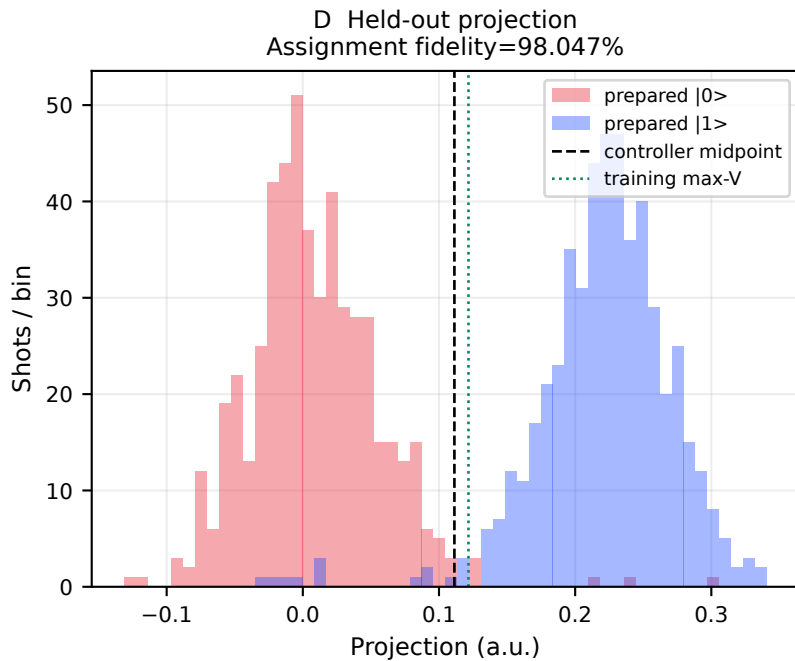
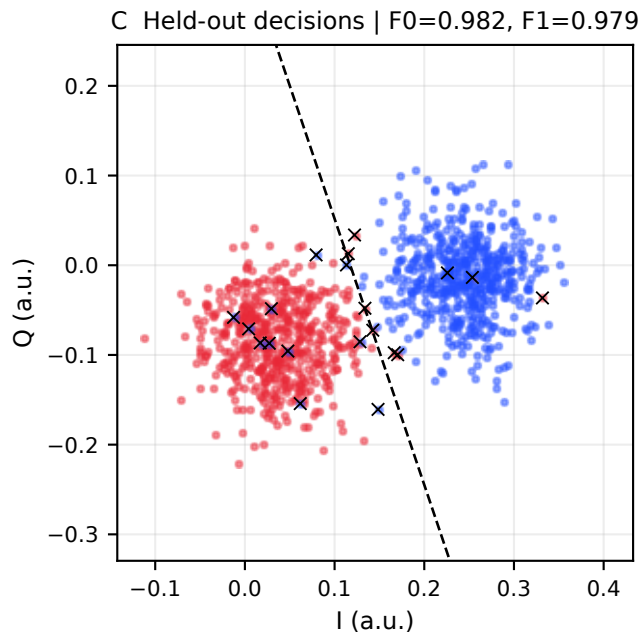
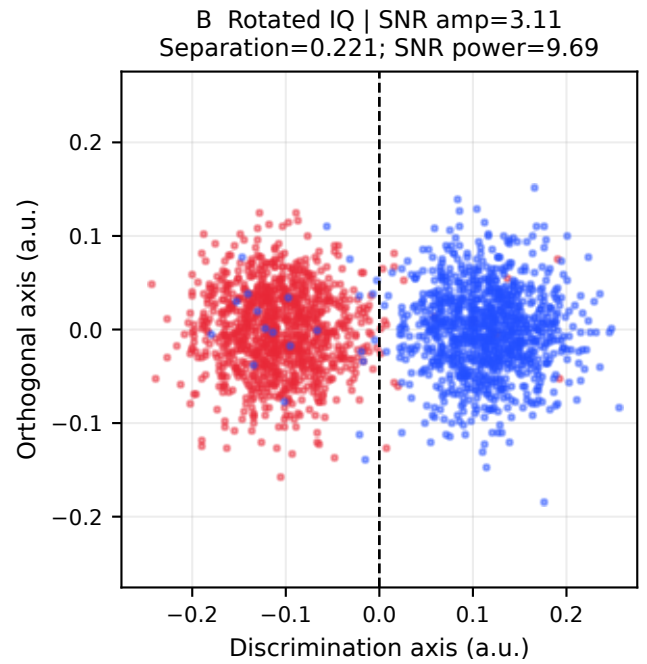


IQ discrimination | SIMULATED | HF + LORA

Controller: accepted | step 13 | consecutive IQ passes 2/2

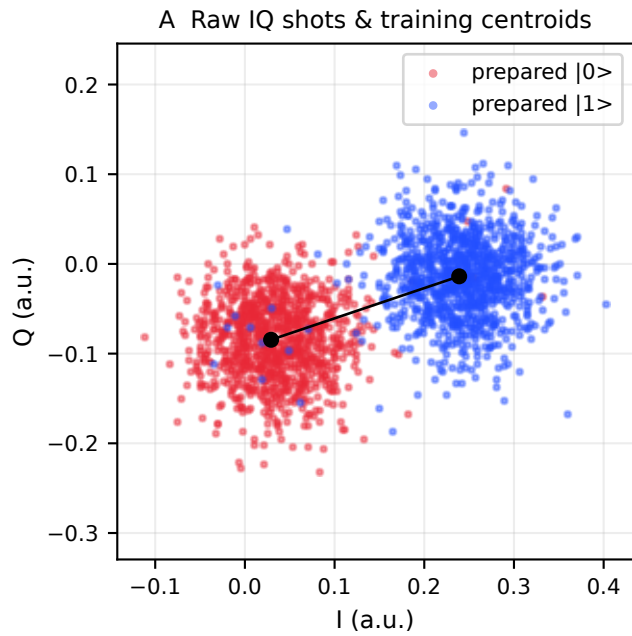

Even shots train; odd shots evaluate. Max-V is diagnostic only.
Model-policy simulation. All points come from the saved measurement.