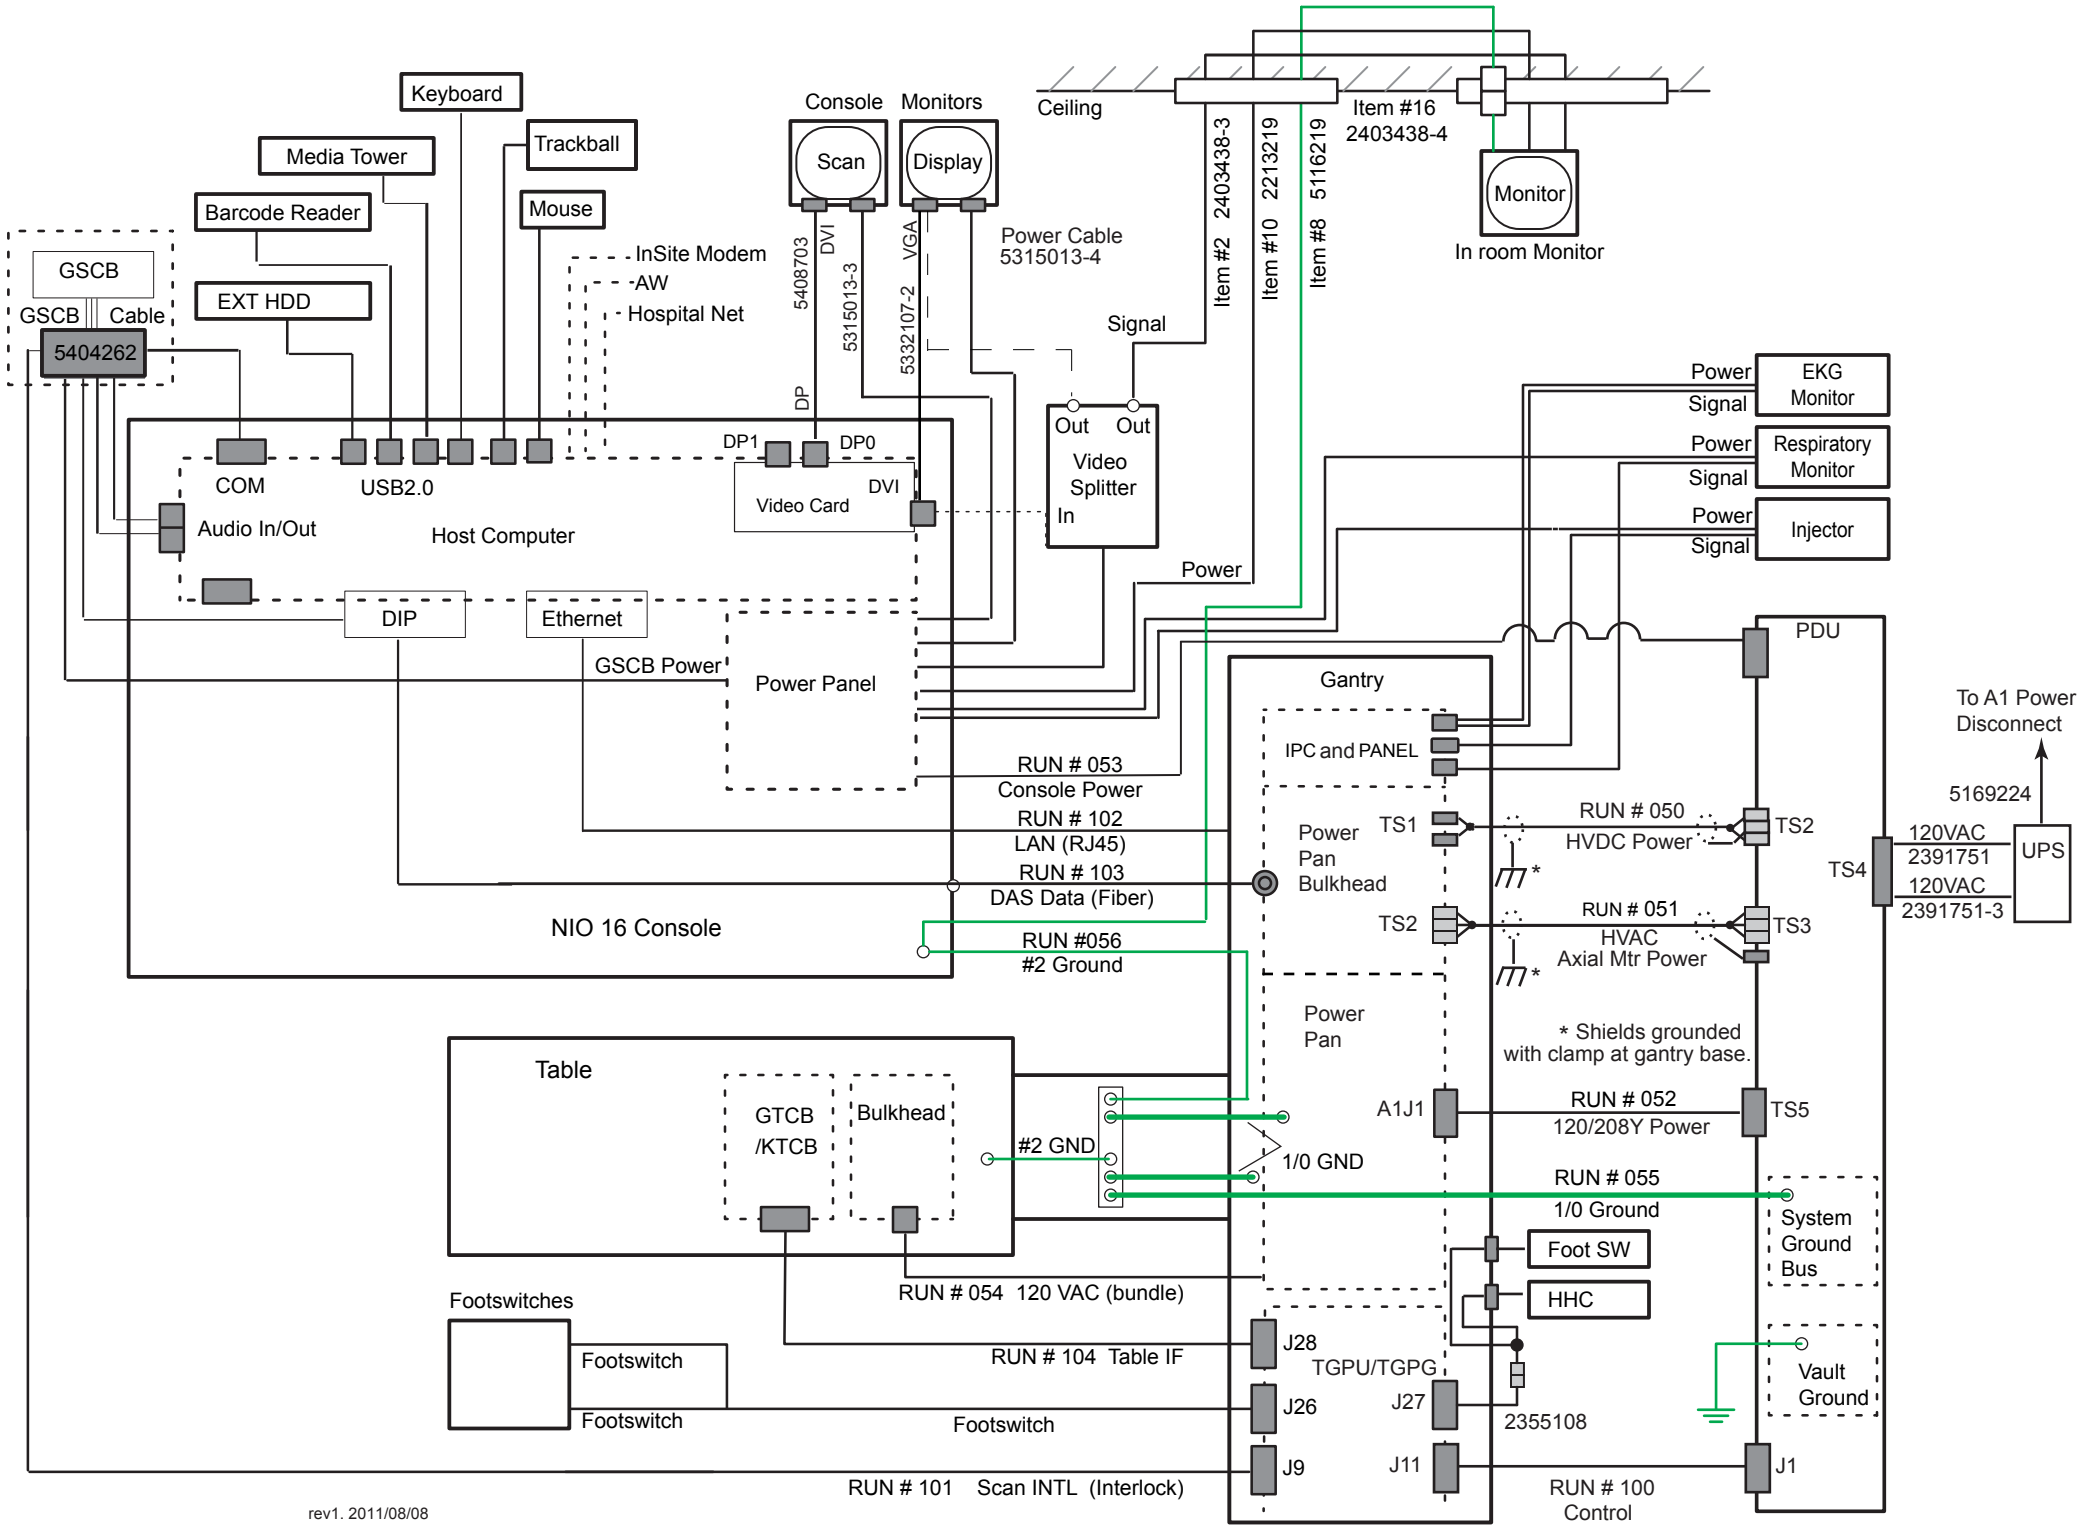

Keyboard
Media Tower
Trackball
Barcode Reader
Mouse
InSite Modem
AW
Hospital Net
GSCB
GSCB Cable
5404262
EXT HDD
Console
Monitors
Scan
Display
5408703
DVI
5315013-3
VGA
5332107-2
DP
Power Cable
5315013-4
Ceiling
Item #16
2403438-4
Monitor
In room Monitor
Item #2 2403438-3
Item #10 2213219
Item #8 5116219
Signal
Power
Signal
EKG Monitor
Power
Signal
Respiratory Monitor
Power
Signal
Injector
Out
Out
Video Splitter
In
DP1
DP0
DVI
Video Card
COM
USB2.0
Audio In/Out
Host Computer
DIP
Ethernet
GSCB Power
Power Panel
NIO 16 Console
PDU
Gantry
IPC and PANEL
RUN # 053
Console Power
RUN # 102
LAN (RJ45)
RUN # 103
DAS Data (Fiber)
RUN #056
#2 Ground
Power
Pan
Bulkhead
TS1
RUN # 050
HVDC Power
TS2
TS4
To A1 Power Disconnect
5169224
120VAC
2391751
120VAC
2391751-3
UPS
TS2
RUN # 051
HVAC
Axial Mtr Power
TS3
* Shields grounded with clamp at gantry base.
Power
Pan
A1J1
RUN # 052
120/208Y Power
TS5
RUN # 055
1/0 Ground
System Ground Bus
Table
GTCB
/KTCB
Bulkhead
#2 GND
1/0 GND
Foot SW
HHC
Footswitches
Footswitch
Footswitch
RUN # 054 120 VAC (bundle)
RUN # 104 Table IF
J28
TGPU/TGPG
J27
2355108
Vault Ground
J26
Footswitch
J9
J11
J1
RUN # 101 Scan INTL (Interlock)
RUN # 100
Control
rev1. 2011/08/08