



synthesized electrode locations

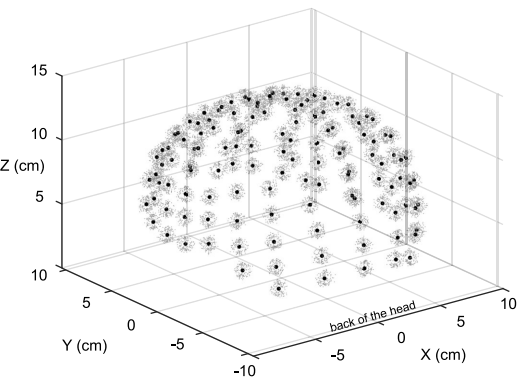


minimum volume enclosing ellipsoids


motion capture probe

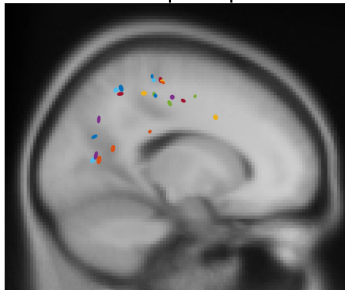

infrared 3D scan

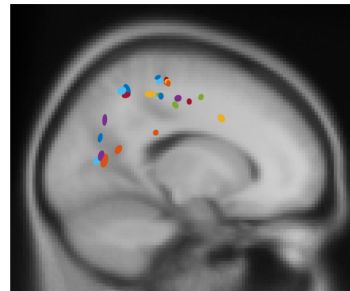

structured-light 3D scan

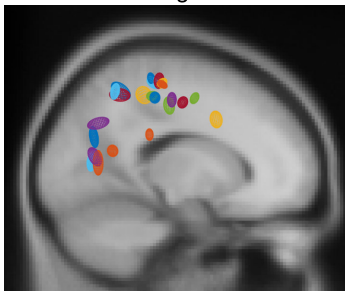

ultrasound

