



Agilent Technologies

Sample ID: Vinay sample PAO_ 100 mms

Method

Name: C:\Users\Public\Documents\Agilent\MicroLab\Methods\Amir V.a2m

User: Admin

Sample Scans: 64

Background Scans: 100

Date/Time: 07/18/2024 3:36:22 PM

Resolution: 4


Range: 4000 - 400

System Status: Good

Apodization: Happ-Genzel

File Location: C:\Users\Public\Documents\Agilent\MicroLab\Results\Amir V\NaOH Washed\Vinay sample

PAO_ 100 mms_0000.a2r

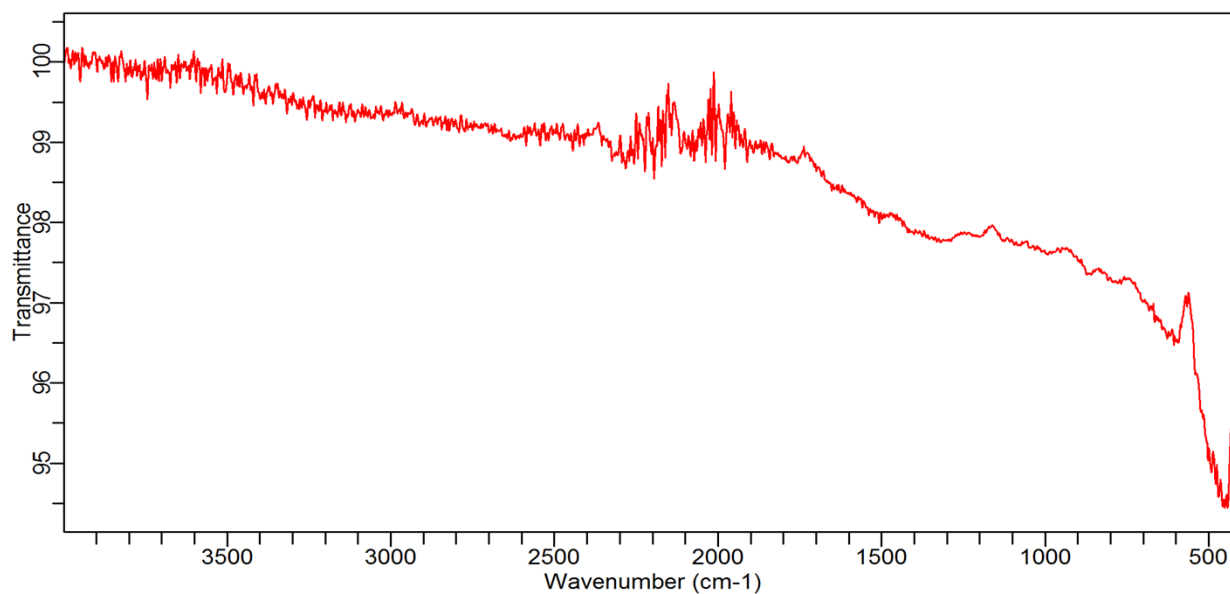

Peak Number	Wavenumber (cm ⁻¹)	Intensity
-------------	--------------------------------	-----------