



Agilent Technologies

Sample ID: Vinay sample PAO_ 100 mms

Method

Name: C:\Users\Public\Documents\Agilent\MicroLa
b\Methods\Amir V.a2m

User: Admin

Sample Scans: 64

Date/Time: 07/18/2024 3:39:14 PM

Background Scans: 100

Range: 4000 - 400


Resolution: 4

Apodization: Happ-Genzel

System Status: Good

File Location: C:\Users\Public\Documents\Agilent\MicroLab\Results\Amir V\NaOH Washed\Vinay sample

PAO_ 100 mms_0001.a2r

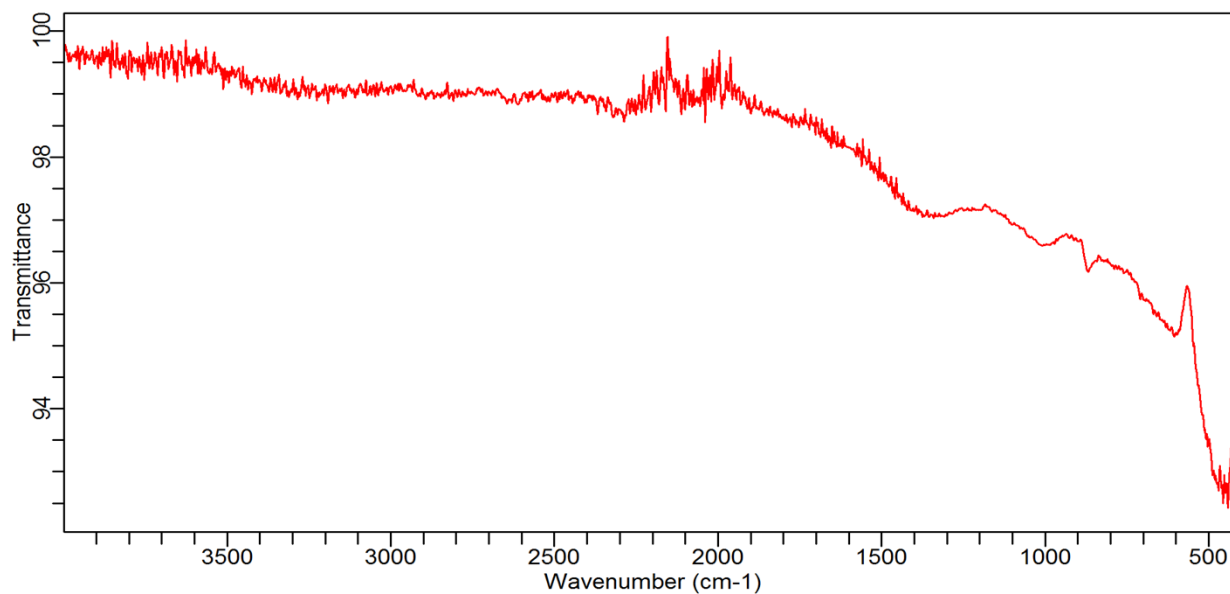

Peak Number	Wavenumber (cm ⁻¹)	Intensity
-------------	--------------------------------	-----------