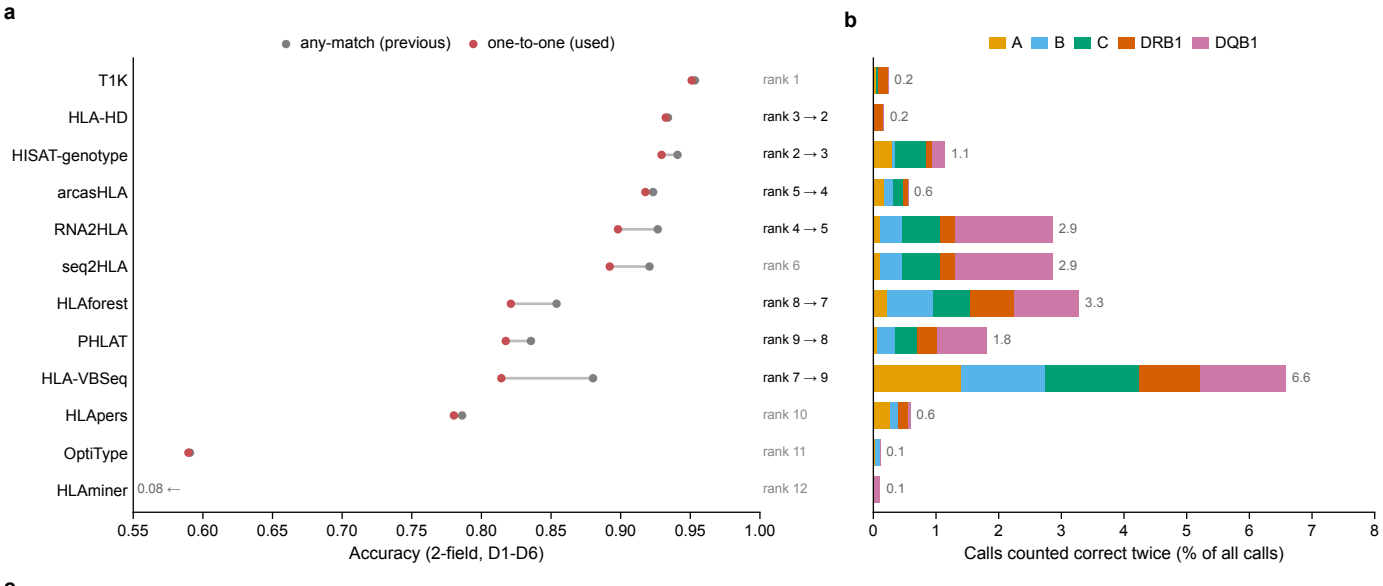

c

Example: HLA-VBSeq, D1 sample ERR188025, HLA-DRB1

```
Gold standard:   DRB1*16:01 / DRB1*13:01
Reported:        DRB1*13:01  DRB1*13:01
Any-match:       2 / 2 correct  (both calls match DRB1*13:01)
One-to-one:      1 / 2 correct  (DRB1*16:01 is missed)
```