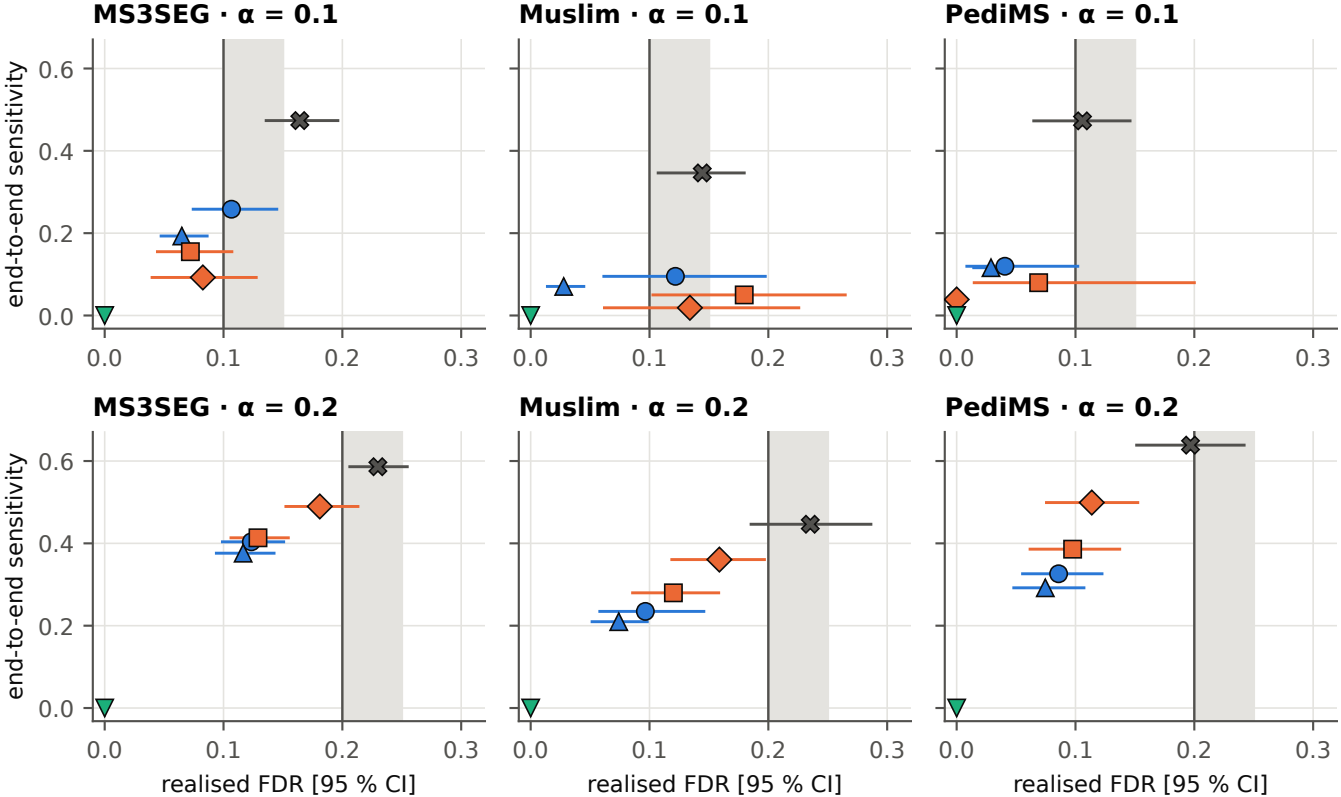

Calibration on the 1-mm-grid sites, test on each thick-slice site (D3). Hierarchical e-values selected nothing in every D3 cell (sensitivity 0). Grey band: nominal α to α + 0.05.