Automated Image Alignment

Automated Subtraction Maps

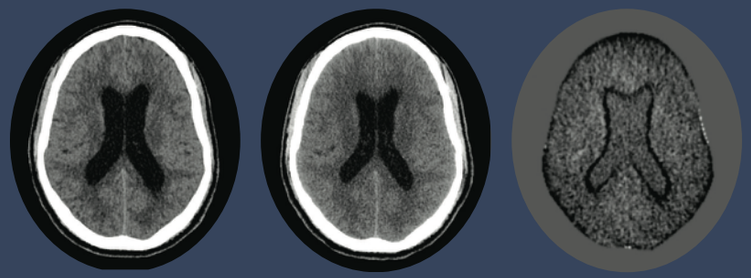

Current → Prior → Current–Prior

FAST, ACCURATE, & PROVEN

cortechs.ai

www.cortechs.ai | +1 858.459.9700

Distributed by Cortechs.ai
Copyright © 2020 CorTechs Labs, Inc.

cortechs.ai

CT CoPilot

Head CT Scans, Quantified.

Fast & Accurate Automated Quantitative Head CT Analysis

- ✓ Automatically registers head CT images to an anatomical atlas and generates aligned reformatted images for standard viewing
- ✓ Quantifies lateral ventricle volume and calculates a midline shift index to improve measurement accuracy and aid in clinical assessment
- ✓ Co-registers current and prior exams and generates a subtraction series
- ✓ FDA cleared for clinical use

19% **IMPROVEMENT** in radiologist certainty when determining a change in ventricular volume.1

73% **IMPROVEMENT** in radiologist reading efficiency when assessing a change in ventricular volume.2

[1] Farid, N., Goel, G., Sung, A., Yamin, G. (2017, April).

[2] Chang, Y.H.A., Farid, N., Li, C.Q., Sung, A, J., (2017, Oct).

CT CoPilot® Quantitative Report

Light Background Report

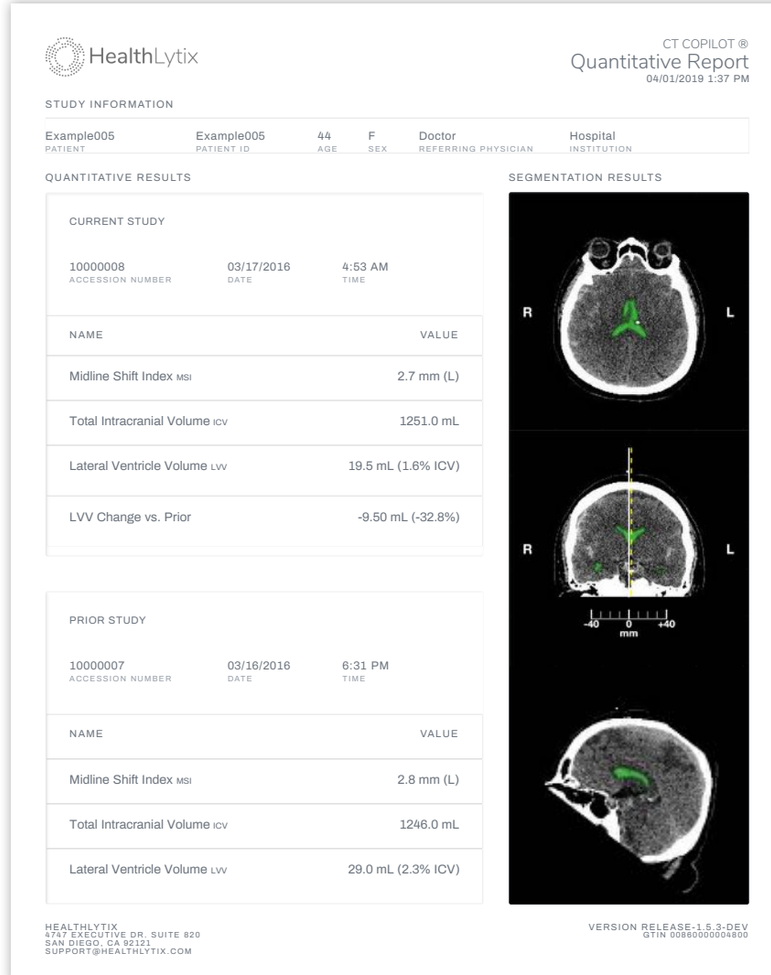

HealthLytix

CT COPILOT ®
Quantitative Report
04/01/2019 1:37 PM

STUDY INFORMATION

Example005	Example005	44	F	Doctor	Hospital
PATIENT	PATIENT ID	AGE	SEX	REFERRING PHYSICIAN	INSTITUTION

QUANTITATIVE RESULTS

CURRENT STUDY

10000008	03/17/2016	4:53 AM
ACCESSION NUMBER	DATE	TIME

NAME	VALUE
Midline Shift Index MSI	2.7 mm (L)
Total Intracranial Volume ICV	1251.0 mL
Lateral Ventricle Volume LVV	19.5 mL (1.6% ICV)
LVV Change vs. Prior	-9.50 mL (-32.8%)

PRIOR STUDY

10000007	03/16/2016	6:31 PM
ACCESSION NUMBER	DATE	TIME

NAME	VALUE
Midline Shift Index MSI	2.8 mm (L)
Total Intracranial Volume ICV	1246.0 mL
Lateral Ventricle Volume LVV	29.0 mL (2.3% ICV)

SEGMENTATION RESULTS

HEALTHLYTIX
4747 EXECUTIVE DR. SUITE 820
SAN DIEGO, CA 92121
SUPPORT@HEALTHLYTIX.COM

VERSION RELEASE-1.5.3-DEV
GTIN 00860000004800

- ✓ Midline shift index
- ✓ Total intracranial volume
- ✓ Lateral ventricle volume (LVV)
- ✓ LVV change between current and prior study

Dark Background Report

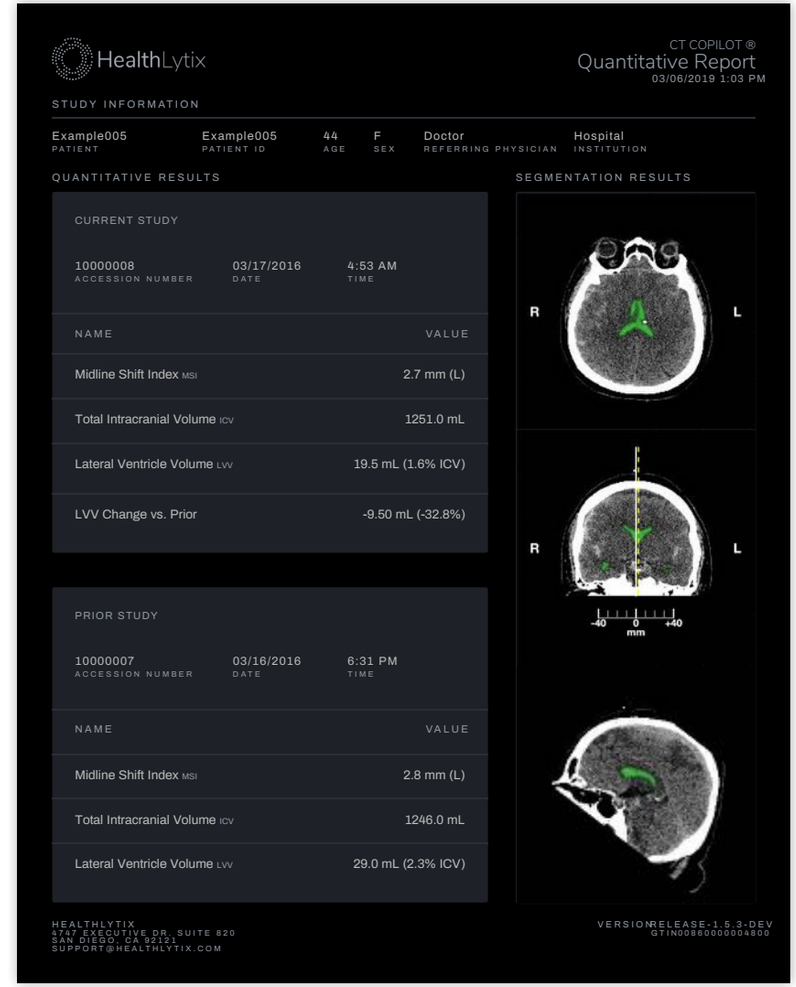

HealthLytix

CT COPILOT ®
Quantitative Report
03/06/2019 1:03 PM

STUDY INFORMATION

Example005	Example005	44	F	Doctor	Hospital
PATIENT	PATIENT ID	AGE	SEX	REFERRING PHYSICIAN	INSTITUTION

QUANTITATIVE RESULTS

CURRENT STUDY

10000008	03/17/2016	4:53 AM
ACCESSION NUMBER	DATE	TIME

NAME	VALUE
Midline Shift Index MSI	2.7 mm (L)
Total Intracranial Volume ICV	1251.0 mL
Lateral Ventricle Volume LVV	19.5 mL (1.6% ICV)
LVV Change vs. Prior	-9.50 mL (-32.8%)

PRIOR STUDY

10000007	03/16/2016	6:31 PM
ACCESSION NUMBER	DATE	TIME

NAME	VALUE
Midline Shift Index MSI	2.8 mm (L)
Total Intracranial Volume ICV	1246.0 mL
Lateral Ventricle Volume LVV	29.0 mL (2.3% ICV)

SEGMENTATION RESULTS

HEALTHLYTIX
4747 EXECUTIVE DR. SUITE 820
SAN DIEGO, CA 92121
SUPPORT@HEALTHLYTIX.COM

VERSIONRELEASE-1.5.3-DEV
GTIN00860000004800

- ✓ Dark background report option for comfortable review in radiology reading rooms