
BENCH CONFIGURATION ONLY

Existing LOGIC_SEL = 5 V (continuity checked). Uno R3 uses 5 V logic.

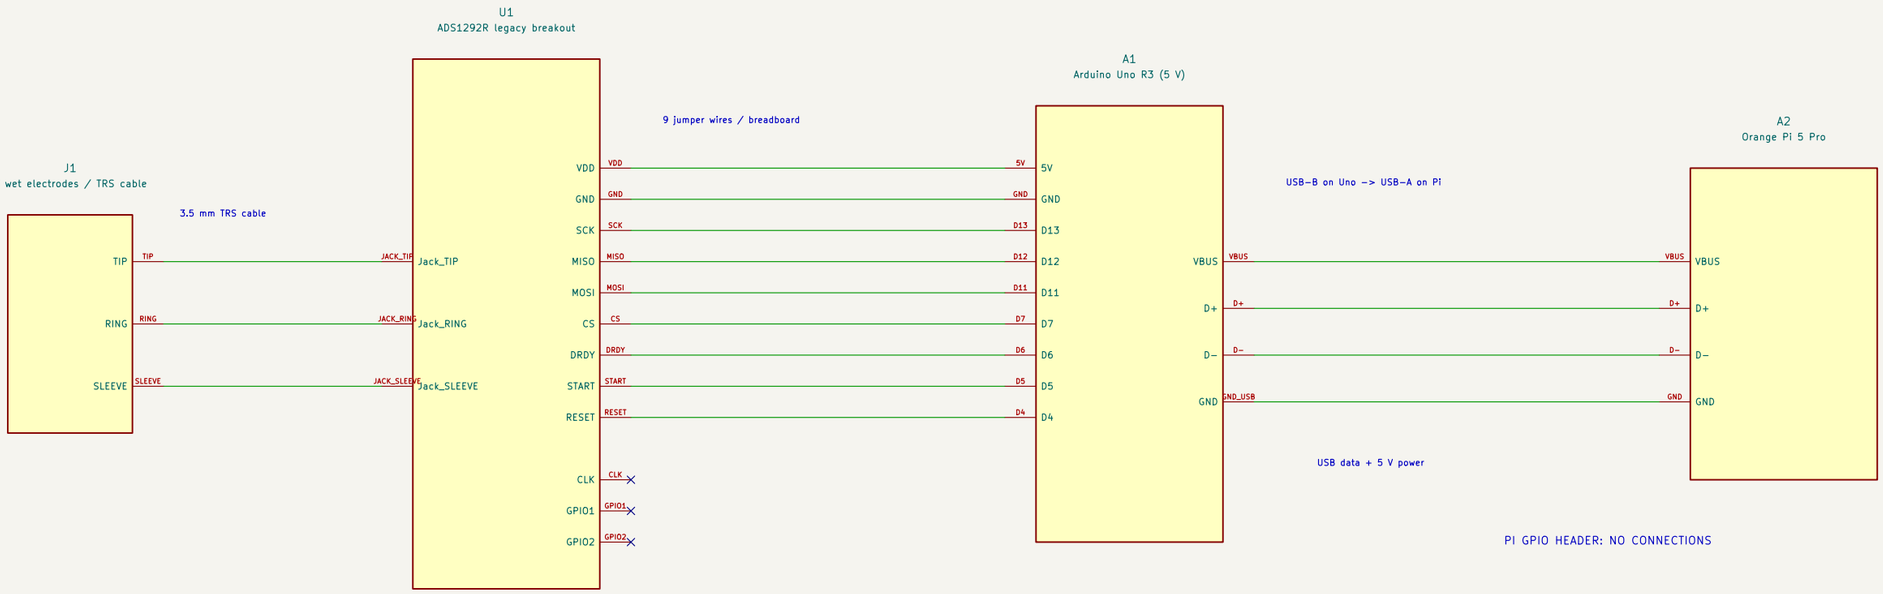

ELECTRODES: LEAVE DISCONNECTED during USB/mains bench tests.

Cable contact names shown only. Lead colors and skin placements are UNVERIFIED.

The ADS1292R board is sold for ECG/respiration; EEG suitability is not yet validated.

Before body use: isolated battery acquisition and a reviewed wireless data path are required.

Do not treat a battery-powered Pi connected to mains USB/HDMI peripherals as isolated.

No extra Uno barrel-jack / VIN supply in this USB-powered bench configuration.

CHECK BEFORE POWER: each header pin has its own breadboard strip; no adjacent-pin shorts.

Firmware: CS=D7, DRDY=D6, START=D5, RESET=D4. Keep Uno D10 configured as OUTPUT for SPI master.

NOT IMPLEMENTED: isolated body-use supply, wireless uplink, electrode placement, EEG validation.

No robot arm or heart-rate hardware in this MVP. Quest/WebXR receives the network intensity stream.

Module wiring reference; not a medical device or body-use approval

MOLTEN hackathon prototype

Sheet: /
File: adaptive-horror.kicad_sch

Title: Adaptive Horror | Biosignal Bench Wiring

Size: A3	Date: 2026-10-17	**Rev: A**
KiCad E.D.A. 10.0.6		Id: 1/1