

The ULTRASPEAKER PROJECTOR LAB

USER GUIDE

The projector right before you speak

Projector Lab guides you through 10 steps to set the projector's format, focus, black, white and colour, with test patterns made for your presentation.

VERSION 1.2 · NOVEMBER 2026

CONTENTS

In this guide

01 Before you start
What Projector Lab does, where to find it, PowerPoint and web version

02 The interface
The parts of the screen, one by one

03 Before the talk: the 10-step procedure
What to look at on each pattern and which menu to adjust

04 Screen Test
Full-screen patterns and the .pptx file for PowerPoint and Keynote

05 Saved venues, timer and report
Warm-up, settings to reuse and a report to share

06 Speaker tips
Arriving early, what to ask the AV desk, 4:3 and 3:1 screens

07 Frequently asked questions
Common problems and support

01 Before you start

Every room has a different projector. Projector Lab has you show a test pattern, tells you what to look at and which projector menu to adjust. In 10–15 minutes your slides and clinical photos look as they do on your monitor.


IN POWERPOINT

Home tab — **The Ultraspeaker** group — **Projector Lab**. The pane opens on the right. **Insert the test slides** adds 15 test slides to the presentation in its format, with the instructions in the speaker notes.

IN THE BROWSER

niki977.github.io/ultraspeaker-projector-lab, with nothing to install. Show the patterns full screen on the projector or download the Screen Test as .pptx for PowerPoint and Keynote. On your phone the procedure stays at hand.

> **WHAT STAYS ON THE DEVICE**
>
> Language, procedure in progress, timer and saved venues stay in the browser or PowerPoint storage. No data is sent to any server.

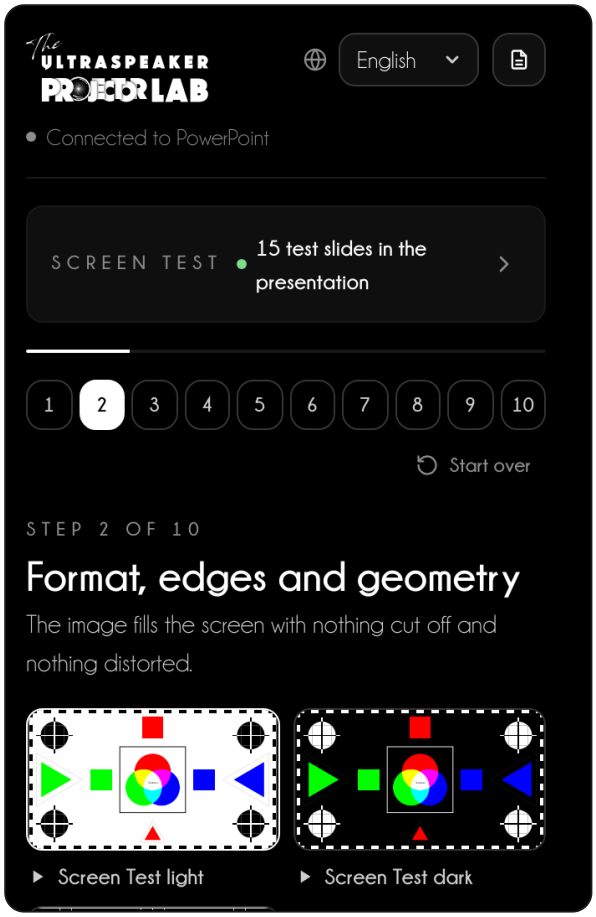


POWERPOINT PANE

FEATURE	POWERPOINT	WEB VERSION
Test slides in the presentation	Yes	—
Full-screen patterns	In a window	Yes
Screen Test .pptx to download	—	Yes
Clinical photo	In the test slide	In the full-screen pattern
“Reset everything”	—	Yes

02 The interface

The same page in the web version and in the pane: the Screen Test at the top, the 10 steps below.

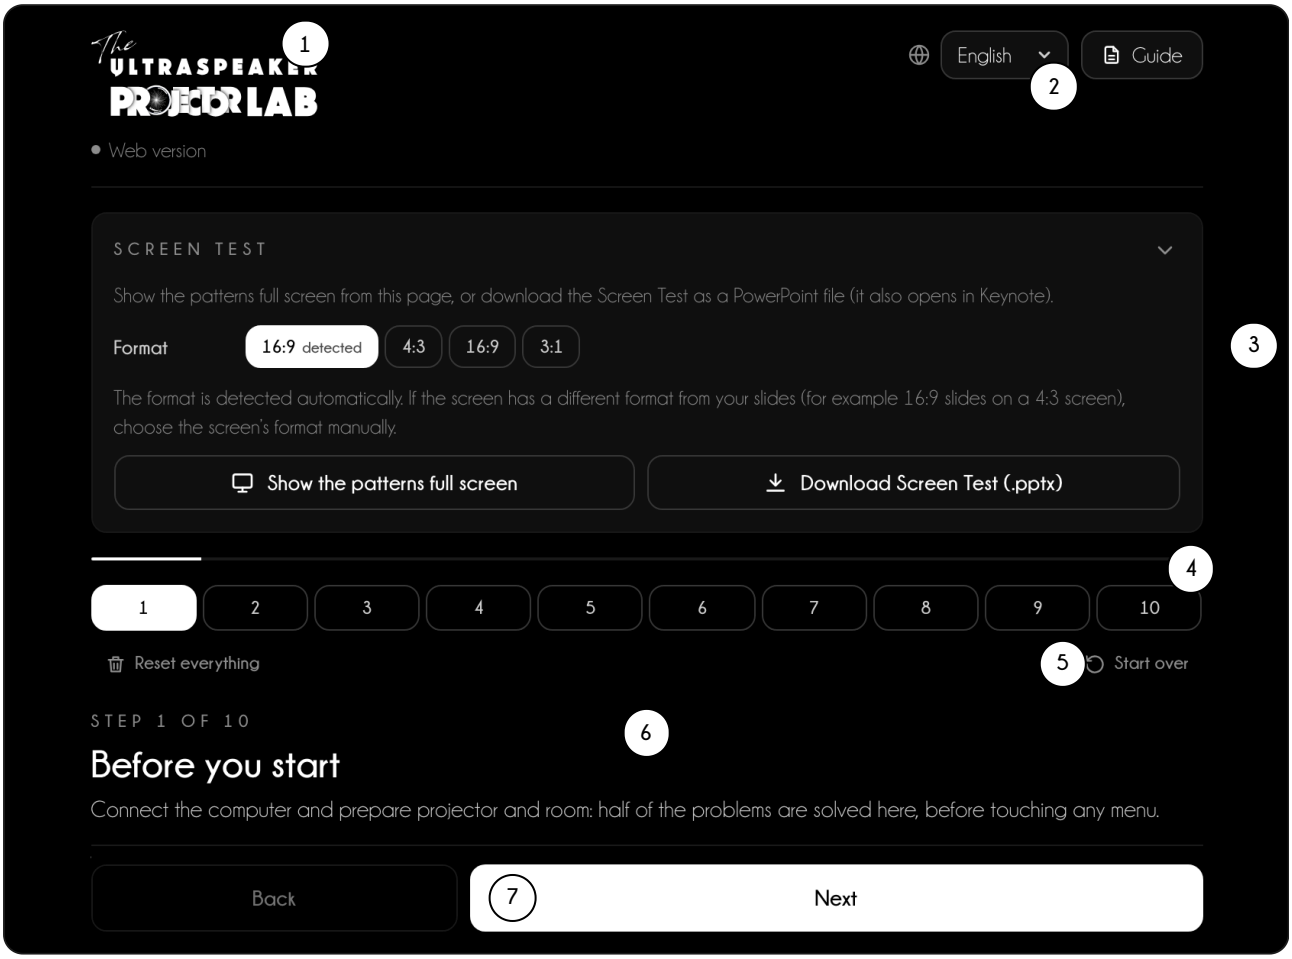

WEB VERSION · COMPUTER

1. **Logo.** opens theultraspeaker.com. Below it, the status line: "Web version" or "Connected to PowerPoint".
2. **Guide and language.** opens this PDF guide; the menu changes the language of the interface, patterns and notes.
3. **Screen Test.** format (detected automatically, or 4:3, 16:9, 3:1), pattern window, download or insertion.
4. **Steps.** 1 to 10; the dot shows the result: green fine, amber needs work, grey skipped.
5. **Start over.** "Start over" clears results and answers; in the web version "Reset everything" also deletes the venues.
6. **The step.** what to look at, the "What do you see?" question, what to adjust, the settings used and the result.
7. **Back / Next.** always at the bottom; on the last step "Download the report (PDF)".

03 Before the talk: the 10-step procedure


Every step has the same structure. Show the pattern, look from the back of the room, answer the question and the Lab tells you which menu to adjust, in which direction and by how much.

THE "WHAT DO YOU SEE?" QUESTION


In steps 4–8 you tap what you see: for example the first patch you can tell from black. The answer gives the correction, and the step result updates on its own.

COLOUR CAST

In step 6 choose, in each group, the grey that looks most neutral. If it is not number 5 in the centre, the Lab recognises the cast and points to colour temperature, tint or RGB gain.

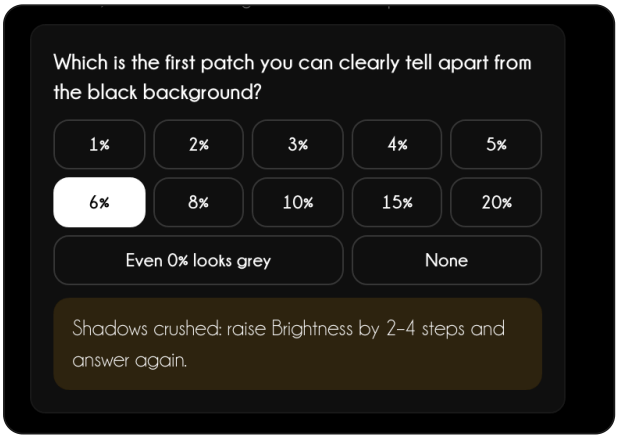

STEP 4 · BLACK LEVEL

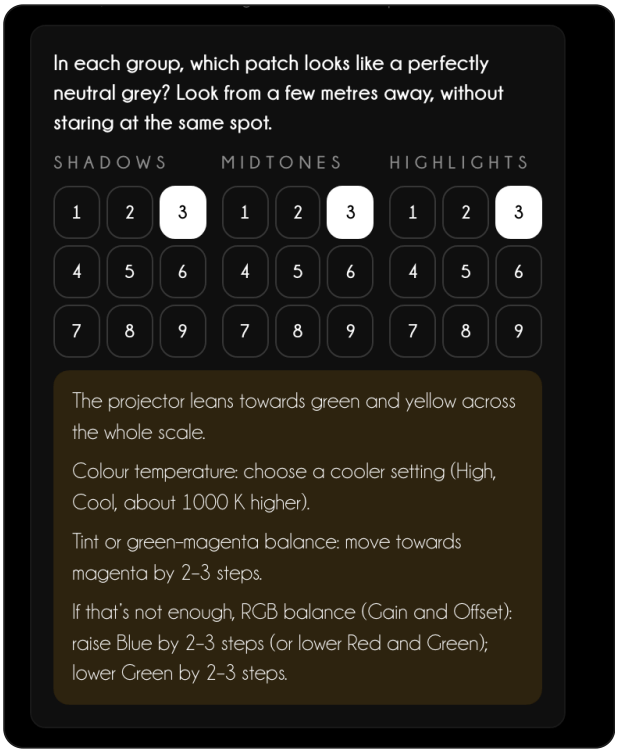

STEP 6 · GREY COMPARISON

SETTINGS USED

Note the projector settings before and after adjusting: they go into the report and the saved venues.



SETTINGS BEFORE AND AFTER

1 · Before you start

Connect the computer and prepare projector and room: half of the problems are solved here, before touching any menu.

- Switch the projector on early: with a lamp at least 15 minutes, ideally 30, because brightness and colour only settle once warm; laser or LED models need 5–10.
- Laptop on mains power; screen saver and power saving off.

2 · Format, edges and geometry

The image fills the screen with nothing cut off and nothing distorted.

- **Look at:** The chequered border is complete on all four sides. If part of it is missing, the image is cropped (overscan).
- **Adjust:** First place the projector square to the screen and centred: it is the best correction there is.

3 · Focus and legibility

Sharp stars in the centre and corners, and the minimum text size readable from the back of the room.

- **Look at:** In the big star the spokes stay separate almost to the centre, with no wide grey blur.
- **Adjust:** Focus ring or control: focus the centre, then check the corners and find the best compromise.

4 · Brightness: black level

Detail in the shadows without a greyish black.

- **Look at:** 0% is as black as the background.
- **Adjust:** Brightness menu: it sets the black level, not the lamp power.

5 · Contrast: white level

Full whites that don't clip: light details stay visible.

- **Look at:** Patches up to 97–98% still stand out from the white background.
- **Adjust:** Contrast menu: lower it until 97 and 98% reappear, then stop.

6 · Greyscale and colour temperature

Neutral greys and even steps: the foundation for correct colour.

- **Look at:** All 11 steps are distinct, from 0 to 100%.
- **Adjust:** Colour temperature: Normal / Medium / 6500 K (D65). High = bluish, Low = yellowish.

7 · Colour and saturation

Rich but faithful colours, no shifted hues and no clumped areas.

- **Look at:** In the bars yellow is yellow (not green), cyan is not blue, magenta is not red.
- **Adjust:** Saturation / Colour: lower it if the last ramp steps merge; raise it if everything looks dull.

8 · Clinical references

Your clinical photos must show enamel, margins and tissue as you see them on your monitor.

To see one of your clinical photos, use "Try one of your clinical photos" ("Insert one of your clinical photos" in PowerPoint), or drag the photo, JPG or PNG, into the dashed box: it appears in the "Your photo" pattern.

- **Look at:** All enamel whites are distinct, even the second one from pure white: otherwise characterisations and light shades disappear.
- **Adjust:** Whites merging: lower Contrast (step 5).

9 · Uniformity and cleanliness

No blotches, coloured zones or fixed dots in the image.

- **Look at:** White: no dark or coloured blotches; corners not much darker than the centre.
- **Adjust:** Clean the lens with a microfibre cloth.


10 · Final check

Check a real slide, note the settings and remove the test slides.

- Show your most demanding slide: a clinical photo, the smallest text, a chart.
- Look at it from the back row and from one side of the room.

04 Screen Test

15 patterns, in the same order as the steps. They adapt to the real shape of the screen: the edges of the pattern match those of the projector.

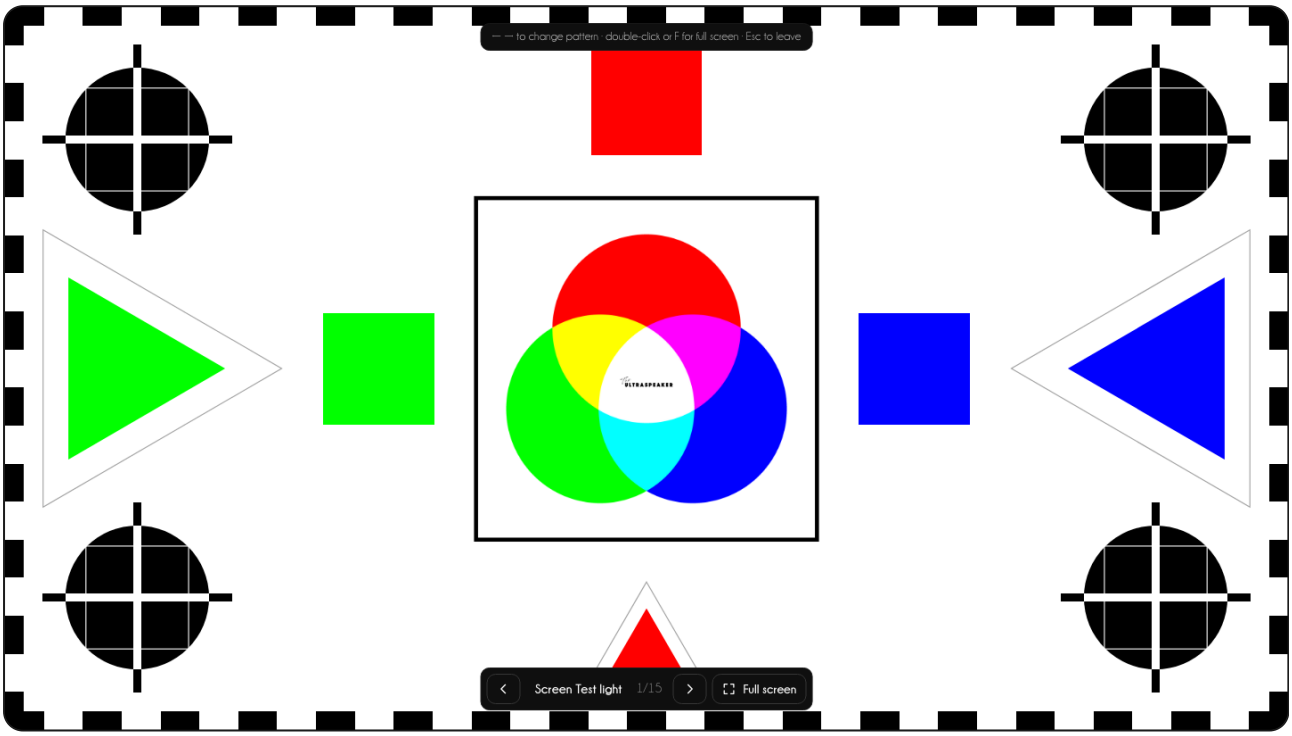

LIGHT SCREEN TEST, FULL SCREEN

Three ways to show them


1. **In the presentation** (PowerPoint): **Insert the test slides**, connect the projector in **Extend** mode and start the slide show from the first test slide. The instructions are in the speaker notes.

2. **In a window** (PowerPoint): **Open the patterns in a window**, drag the window onto the projector screen and double-click. The pane changes pattern at every step.

3. **In the browser**: **Show the patterns full screen**. Arrows ← → change pattern, F for full screen, Esc to leave.

The .pptx file for PowerPoint and Keynote

In the web version choose the screen format and press **Download Screen Test (.pptx)**. The file contains the 15 slides with notes; Keynote opens it with **File → Open**.

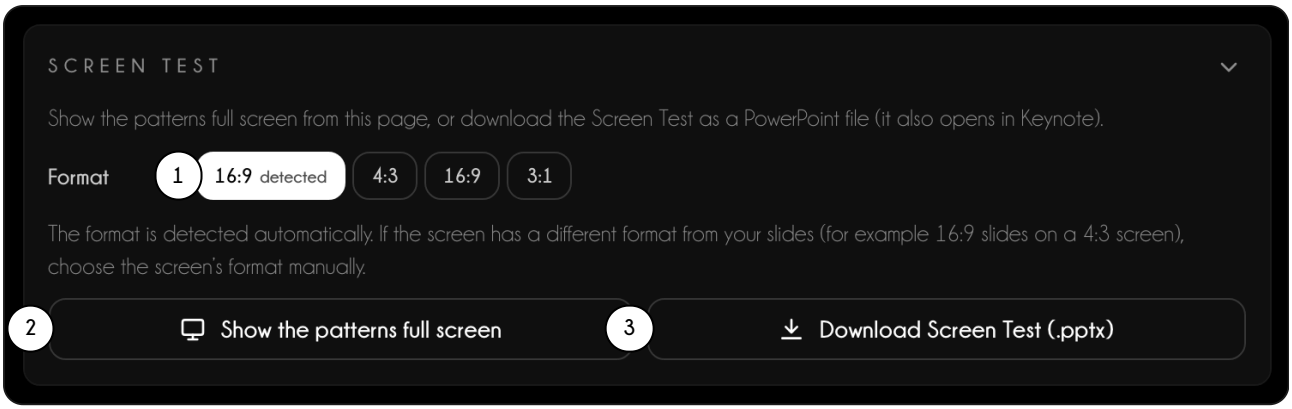

SCREEN TEST CARD · WEB VERSION

(1) **Format.** detected automatically; choose the screen's format by hand if it differs from your slides.

(2) **Full-screen patterns.** on the projector, without touching your presentation.

(3) **Download.** Screen Test .pptx in the chosen format.

STEP	PATTERNS
2 · Format, edges and geometry	Screen Test light, Screen Test dark, Grid
3 · Focus and legibility	Focus
4 · Brightness: black level	Black
5 · Contrast: white level	White
6 · Greyscale and colour temperature	Greys, Grey comparison
7 · Colour and saturation	SMPTE bars, Colour ramps
8 · Clinical references	Clinical, Your photo
9 · Uniformity and cleanliness	Full white, Full grey, Full black

05 Saved venues, timer and report


Three tools so you do not start from scratch in every room.

Warm-up timer

In step 1 press **Start warm-up timer (15 min)**. A lamp needs at least 15 minutes, ideally 30; laser and LED settle in 5–10.

Saved venues

1. Write the venue name in step 1.
2. Note the projector settings during the steps.
3. In step 10 press **Save this venue**.
4. Next time choose the venue in step 1 and press **Use these settings as a starting point**.

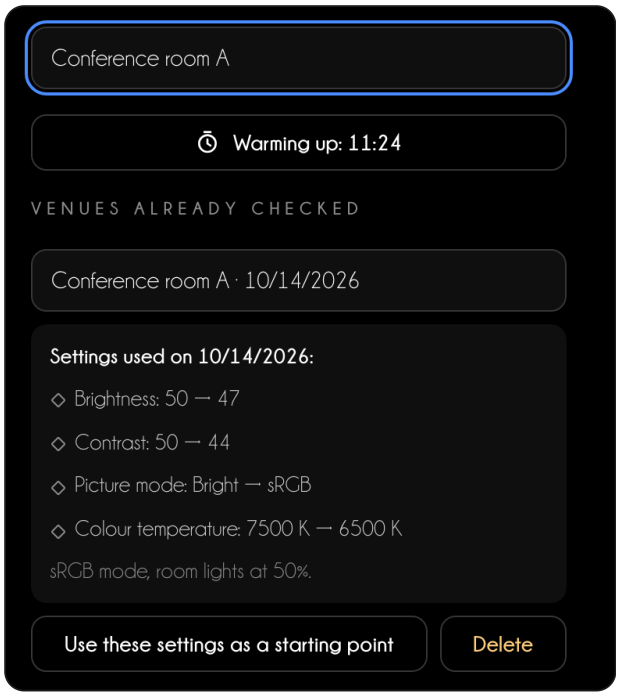


STEP 1 · SAVED VENUE AND TIMER

Report

In step 10 the report sums up date, format, results, answers and settings. Add a note and press **Download the report (PDF)**: you get a PDF to send to the AV desk (in the panel it opens in your browser).

> **Start over** clears results, answers and settings but keeps the saved venues. In the web version **Reset everything** also deletes venues and format.

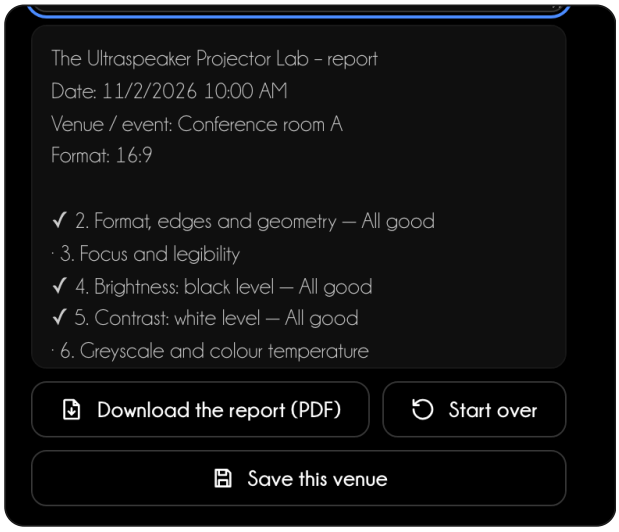

STEP 10 · REPORT

06 Speaker tips

The best adjustment does not replace preparation.

SPEAKER TIP

Arrive 30 minutes early. Switch the projector on straight away, run the procedure while it warms up and finish with your most demanding slide: a clinical photo, the smallest text, a chart.

IF THE AV DESK WILL NOT LET YOU TOUCH THE PROJECTOR

Ask for three precise things: **sRGB** or **Presentation** mode, **overscan** off, keystone at minimum. Do the rest from your computer: native resolution, RGB Full colour format, Night Shift and Night light off.

SCREEN	WHAT HAPPENS	WHAT TO DO
4:3 with 16:9 slides	Black bars above and below	Accept the bars; choose 4:3 in the Screen Test to check the screen edges
16:9 with 4:3 slides	Black bars at the sides	Do not stretch the image: circles would turn oval
3:1 (panoramic screens)	Small slides in the centre, or cropped	Ask for the format beforehand; test with the 3:1 Screen Test and the largest text

07 Frequently asked questions

I cannot see Projector Lab on the Home tab.

Reinstall the add-in following the "Installation" page of the site, then close and reopen PowerPoint.

The detected format is wrong.

Choose 4:3, 16:9 or 3:1 by hand in the Screen Test card. If it differs from your slides, the Screen Test opens in a new presentation in that format.

I do not want to change my presentation.

Use **Open the patterns in a window**: the patterns stay in a separate window. Before the talk, **Remove the test slides** deletes all the test slides anyway.

My projector's menus have different names.

Every brand uses its own names: the Lab gives the most common ones (Brightness, Contrast, Aspect, Overscan). If in doubt, ask the venue technician.

Where does my data go?

Nowhere: it stays on the device. In the web version **Reset everything** deletes it.

SUPPORT

Write to info@theultraspeaker.com with your computer and PowerPoint version.



Knowledge is not enough.
From expert to Ultraspeaker.

ASK FOR ADVICE

THEULTRASPEAKER.COM · INFO@THEULTRASPEAKER.COM