

See discussions, stats, and author profiles for this publication at: <https://www.researchgate.net/publication/352145516>

Efficient Approach for Measuring Heart Pulse from Real Time Facial RGB Color Videos

Conference Paper · April 2021

DOI: 10.1109/ICIEM51511.2021.9445283

CITATIONS

0

READS

56

3 authors, including:



[Mamoon Rashid](#)

Vishwakarma University

116 PUBLICATIONS 588 CITATIONS

[SEE PROFILE](#)

Some of the authors of this publication are also working on these related projects:



Cloud Storage Security in Healthcare Systems [View project](#)



Privacy of Data in Hybrid Clouds [View project](#)

Efficient Approach for Measuring Heart Pulse from Real Time Facial RGB Color Videos

P.V.P. Sai Kiran
Bachelor of Technology
Computer Science & Engineering,
Lovely Professional
University, India
saikiran660@gmail.com

Sujith Reddy Vangala
Bachelor of Technology
Computer Science & Engineering,
Lovely Professional
University, India
sujithreddyvangala@gmail.com

Mamoon Rashid
Assistant Professor, School of
Computer Science & Engineering,
Lovely Professional
University, India
mamoon873@gmail.com

Abstract— The heart, the vital organ of the human body, needs to function with proper care, and therefore it is important to monitor. Detecting Heart Rate (HR) often requires costly equipment which is complex especially with sensors. Various methods are defined over the years to measure heart rate. One of them being a non-contact method of measuring heart rate using remote photoplethysmography (rPPG). This paper presents a working solution on the live video i.e., in real-time. A set of rectangles are established around the face for detection along with object detection, which is later used in the pipeline of color variations. The mean of the colors (RGB-red, green, blue) in the Region of Interest (ROI) selected on the face (forehead region). Thus, the signal is obtained from the heart rate frequency by the signal processing method. This paper discusses the reimplementation of one such approach that uses Fast Fourier Transform (FFT). Researchers can now refer to the reviewed and classified algorithms as a starting point to improve and increase the robustness of the experiment.

Keywords— Heart Rate, non-contact, Fast Fourier Transform, camera-based, photoplethysmography.

I. INTRODUCTION

The heart, being the vital organ in a human body is subjected to many risks. A person's heart rate (HR) can be a result of their lifestyles such as health, physical exercises, anxiety, stress, and more. The above-mentioned factors differ for each person. General circumstances to measure heart rate would be in a hospital environment. At the beginning of monitoring of heart rate, physical touch was required for equipment to work and precisely generate results of the patients [1].

The cardiac pulse is typically measured in clinical settings using an electrocardiogram (ECG), which required them to wear on their bodies which proved too abrasive and uncomfortable. Later years, the method to measure or monitor heart rate measurement has changed, which resulted in using sensors that may be worn on the fingertip or earlobe. Hence, after moving to the adaptation of sensors, one of the inferences to note is that they were discomfoting to the wearer. Furthermore, in acknowledging such situations over the past few decades, a non-contact means of detecting heart rate was developed. Such a method would be very beneficial. Noncontact heart rate measure through a simple camera either on a laptop, computer, or phone. Interest in maintaining the fitness of the body has made people health-conscious and resulting technology trends and growth led to such experiments [2-3].

Few earlier studies have shown that heart rate can be calculated using a person's face in a video. So, our research can be simple stated as a reimplementation of one such approach that uses Fast Fourier Transform on mean pixels

within a region of interest (ROI). Then, we explore the head movement of the subject and bound their face and forehead region in a box, to measure the heart rate more accurately [4-5].

A measured heart rate is obtained from the number of contractions per minute as a volumetric measurement (plethysmogram). Moreover, the photoplethysmogram (PPG) application which exists in smartwatches today and other fitness tracking products proven to have some sought of physical touch on a wearer which is discomfoting. Many researchers have been trying to perfect the application by any means necessary [6]. The studied technique uses a color-based model RGB imaging to receive a signal by placing the subject a few meters from the camera. Later, it was slowly taking the shape and named remote photoplethysmography (rPPG). The main aim of our research is to observe, study and lend a hand in such important applications which makes life easier and helps to continue in the growing years. And heart rate monitoring based on periodic head movements is another observable phenomenon affected by the cardiac cycle and thus allowing practitioners to obtain HR through monitoring from an estimated rPPG signal [7-8].

Such application was put forward in 2008 [7], nearly more than two decades and still, the observation finds to attract attention and constantly trying to perfect the application. To my dismay, earlier research papers did not discuss every aspect in detail. The basic pipeline which was used for the execution is the same. As stated earlier, our contribution to this topic-

1. Is to provide an outline of previously organized research in medical sciences.
2. Is to label studies by preferred algorithm and contributions to the field. We chose to use this method- rPPG because it is the most frequently used (~50%) and more approachable to novice accomplices.

The reviewed research relating to rPPG that used a low-cost process was only targeted because much of the work is related to the thought or idea we had earlier. Recording equipment is of commercial grade. Included only those in regard whose goal was to obtain HRM using videos or live capture of subject faces. And from that standpoint, proceeding towards the details regarding the implementation of our research.

The remaining paper is split into various sections which briefly describe the pipeline of our project. As the research is mostly based on few prior papers. Extensive developments are not listed but considered and will surely be acknowledged in the development of the paper later. Section II details the methodology, section III deals with the approach, section IV

discusses the setup and equipment used. Finally, section V is dealt with the conclusion of the paper.

II. METHODOLOGY

The method exploited in the research regarding the rPPG is related to the cardiac cycle very closely. Each cycle being periodic will show effects both on the facial skin and mechanical head movement, which enables researchers to calculate HR.

The connection between the light and human tissue on the forehead of a person's head is complex. When the application is all about low-cost and easy accessibility, certain aspects of the experiment should hold viable for the proper conduct of the research. This has shown the reflection of light is dependent on many factors present in the environment and among them, change in blood volume and blood vessel [9-10] movement. Present-day research has shown that ambient light is sufficient to acquire a plethysmographic signal [11]. All the above-mentioned changes in the region of the face, are not easy to track and difficult to be visible by a naked human eye. So, to detect such phenomena the implementation of image processing algorithms is necessary. These are used for selecting the region of interest and observing the change in intensities of the pixels located in the region. By calculating the mean of the intensities of the pixel and extracting the frequencies using FFT would provide us with a clear peak of values that represent the heartbeats. To achieve the primary goal of this project, the implementation of the ROI was carried in Jupyter notebook and other related python libraries- mainly OpenCV.

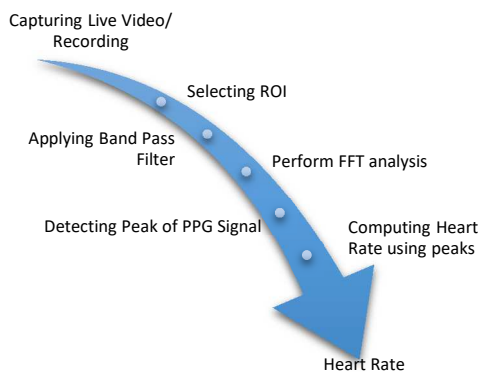


Figure 1. Determining Heart Rate – Each step in the process helps in understanding the approach and provide insight on different methods used.

A. Detecting Faces

Face detection is not the important aspect of the research, so we are not choosing the best method available but one that is readily available and is implemented on the hardware and mobile devices for convenience's sake. The method for face detection is using Haar cascades, which has been proven effective and proposed by Michael Jones and Paul Viola in their paper [12]. Creating a haar cascade filter is complex but effective in the latter end. Various objects can be focused and detected by training the machine learning model with two sets of images- positive and negative images. The positive set contains the features we want our filter to detect and focus while the negative contains all the unwanted data which makes the model distinguishable and helps in identifying the object. Viola-Jones proposal has stated several key features, such as:

1. *Integral Images* are used as an alternative to the pixel values the haar feature captures.

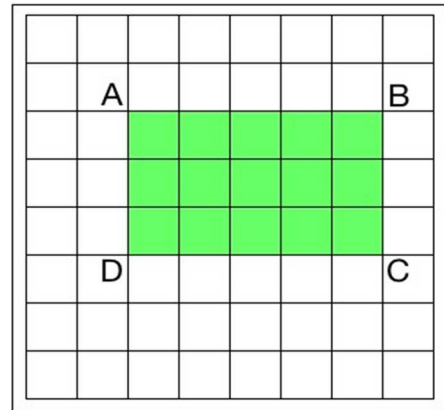


Fig. 2. Integral Images – Mainly used for calculating the average intensity within a given image (grayscale).

2. *Haar Features*: Different rectangular sections within the image of the subject.

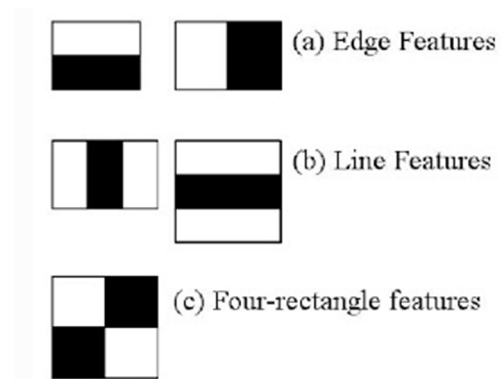


Fig. 3. Haar Cascade Features – to simply understand, white and black regions are positive and negative features of the image.

3. *AdaBoost Algorithm*: optimum characteristics are selected, as this algorithm excels in binary classification.

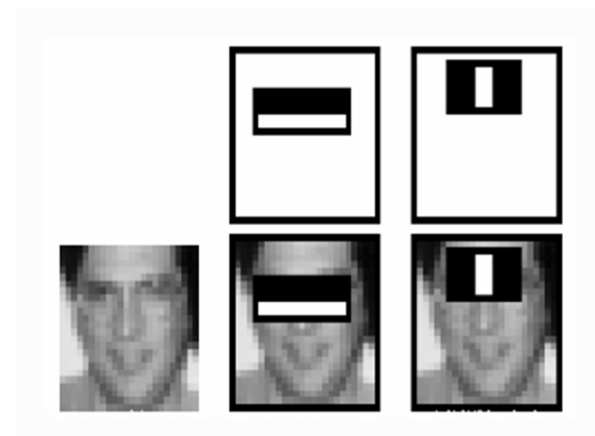


Fig. 4. Achieved through AdaBoost – this is the working of haar features on an actual image where only white or positive region are taken into consideration.

4. *Cascade Filter*: to focus on the computing process of many positive ones possible, the filter negates the images which does not match the intended results.

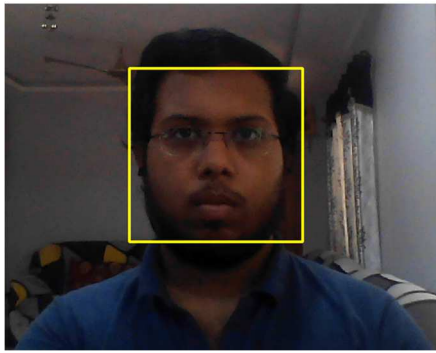


Fig. 5. Detecting Faces – OpenCV has different extensions for the figure enclosing the face, rectangle gives proper sense of understanding the procedure.

B. Selecting ROI

The intermediary part of the process of determining heart rate. The portion (ROI) of the main image, to be used during the computational process, is selected on a specific criterion. As discussed earlier, the skin color variation observed on the forehead is the best and optimal region to observe this phenomenon. Thus, a rectangular box enclosing the ROI adapts to the changes depending on the distance between the camera and the subject. ROI is applied only to the frames where the haar cascade filter detects the face of the subject. The enclosing is a significant way of making the observers understand the working of the process. Now, evaluating the mean of the pixels in the forehead portion and select the maximum or peak of generated values to obtain a clear signal.




Fig. 6. Phenomenon explained in rPPG – the most prominent region to measure heartrate would be the forehead. Blood flow variation in a and b helps in determining the heart rate.[13]

C. Tracking Objects in Image

Two options can be implemented to detect a face,

1. Detecting face for the respective frame.
2. Face Tracking for individual frames using face detection algorithm.

The Applied first procedure for the subject's face. Turns out there is another way that is quite [14] faster. The reason being, at the time of implementation, the method followed was not quite influenced in many studies and experimented with the best of abilities.

D. Heart Rate Measurement

The most vital process of the research is studying heart rate. According to the information gathered from the above sections, start by implementing the Fast Fourier Transform (FFT) for the last 150 frames of the signal acquired from the preceding frame. Heartbeats are in the range of 35 to 195 beats

per minute. The heart rate measurement translates this to a frequency between 1-3 Hertz.

Frequency filtering is applied to the false readings. The filter specifically used is a bandpass filter, used to transmit signals in a certain band of frequencies and block signals of lower and higher range. The same is observed in a television or radio by tuning for a desired frequency. The desired band is centered around a frequency. And finally, narrow it down to finding out the heart rate of the subject.

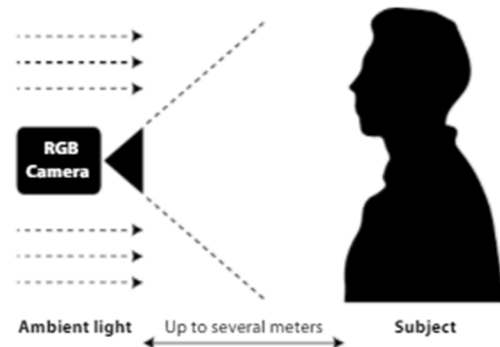


Fig. 7. Setup during rPPG application in HR measurement – camera captures the face using haar features. Only frontal area of the head should be used and heartrate is measured. [13]

III. APPROACH

A lot of various sources define the process of calculating the heart rate. After studying different opinions on such study has opened many possibilities and areas to explore. To start with, the programming mainly involved building a gaussian-like surface around the frame, just like in physics where different surfaces are built around objects. Every picture, live video, or recordings is all read in the form of arrays in python.

1. During the gaussian phase, the frames are reduced in dimension and stored away for later use.
2. Define the parameters for the dimensions of the frame.
3. Define color magnification parameters.
4. Now, we define the parameters such as the thickness, font color, font scale, and few others.
5. Initialize this gaussian frame we have built for the specified frequencies we are targeting.
6. The bandpass filter is applied to the frequencies that are targeted.
7. The most important parameters are the heart rate for determining the frequency.
8. Reconstructing the frame by increasing the dimension of the frame, is mainly done to aid with the computational process of the research.
9. Another helping hand function in this process would be to detect faces using haar cascade.

The above mentioned are to clarify the process we established for the research. Profound knowledge of different areas of interest will surely make all the changes. In addition to the points above, keeping in mind that it is a low-cost and homemade computational process, we are very much limited by the equipment. But, to the best of our abilities, we were

able to design a process which soon is developed and adapted in industries.

It is fascinating to know from the previous studies that provide many ideas, methods to execute such experiments. By focusing on the idea, we had at the beginning, we're able to learn and maintain the integrity for which the research stands.

Then, as stated earlier, convert the color image to grayscale mainly to decrease the computational process for various reasons and select the ROI based on the rectangle enclosing our face. Remember the ROI is less and based on the position of our forehead. Somewhat live to track the motion of the face to aid us in determining the signal.

The function (FFT) commonly used for frequency analysis converts the time into the frequency of the obtained signal. Being a better version of Discrete Fourier Transform (DFT), it can be applied when the number of specimens is of power two [15-16].

$$x_n = \frac{1}{N} \sum_{k=1}^{N-1} X_k \cdot e^{2i\pi kn/N}, n \in Z$$

x_n is the discrete-time varying signal with a period N. For the PPG signal determination, FFT is computed and analyzed. Once the frequency of the signal is obtained from the spectrum, heart rate measurement is given by,

$$\text{Heart Rate} = \text{frequency } (f_h) * 60$$

A. Peak Detection

Individual peaks in the spectrum are used for extracting more information such as heart rate variability. To obtain a refined signal from peak detection, we use a cubic spline interpolation [17-19]. This is often used when the time frame or the data we have or generated is small. The points can then be recognized using a moving section, as they represent the maxima.

$$\text{Heart Rate} = f_h * [(\text{Number of peaks/Time})] \text{ bpm}$$

The more elaborated formula for the understanding of measuring heart rate. This approach is selected to provide quality in determining the signal.

IV. SETUP

During development, the process and trials were performed on the hardware mentioned:

- Processor: Intel^R CoreTM i5 7200U CPU @2.50GHz
- RAM: 16.00 GB
- 720p laptop-camera FHD

Now, computing the average pixels present only in ROI. By juxtaposing the results acquired for different subjects having a slightly visible difference between skin tone. All the observations are noted in the morning and in a well-lit environment for better results. None of the subjects suffered from any skin conditions.

Table I. Experiment Details

| Subject | Features | | |
|---------|----------|--------------|--------|
| | Age | Skin Tone | Gender |
| 1 | 21 | Brown Medium | Male |

| Subject | Features | | |
|---------|----------|--------------|--------|
| | Age | Skin Tone | Gender |
| 2 | 21 | Brown Medium | Male |

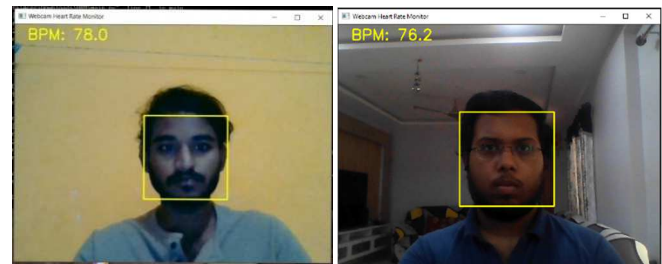


Fig. 8. Shows subject 1 & 2 during the test.

Figure Labels: Performing tests on Subject 1 and Subject 2 having similar skin tones.

While calculating the HR, tests are done later in parallel with another application to certify the accuracy of the measurement. Error variation detected from 1.0 – 5.0 %, but it is hard to detect errors in this process, as these can be a result of the intrinsic ones. The tests performed on the subjects belong to the Indian subcontinent. One more study suggests that the heart rate can be affected by fitness. The more obese a person is, the higher the chances of heart rate rising. Because the cardiac cycle maintained by the veins in our forehead upholds more stress in flowing the blood. When the mean is observed between the two subjects, they vary. And this variation is to be noted on the fitness levels and no other factors.

Table II. Heart Rate Tests

| Number | Experiment Results | | |
|--------|--------------------|------------------|-----------|
| | Subject | Observations (5) | Error (%) |
| 1 | Person A | 76.2 | ~ 1.2 |
| | | 75.6 | |
| | | 73.8 | |
| | | 77.4 | |
| | | 78.0 | |
| 2 | Person B | 85.2 | ~ 4.2 |
| | | 77.4 | |
| | | 85.8 | |
| | | 80.4 | |
| | | 76.2 | |

V. CONCLUSION

A real-time noncontact-based heart rate method is described in this paper using facial video of a subject, which is easy to implement, cost-effective, and comfortable in real-time applications. The main idea is to determine heart rate using the color variation in the foreskin of a subject who is completely still or slightly moving, though any of those factors will not affect the process. With sufficient ambient light, the experiment works. Comparison of our experiment is done with other applications to strengthen our case of using

rPPG. Though many variations were observed in the procedure, the results are similar, precise, and notable. The noncontact technology in the last two decades has been noted by many scholars and many improvements had taken place. The most promising sector for such applications to work would be medical, road safety, security. Also, increasing the accuracy of the application would involve only making more observations in different scenarios and other verifying systems. Creating a real-time, multi-parameter application with different technological improvements will be the subject of future work.

ACKNOWLEDGMENT

We are thankful to our supervisor Mamoon Rashid, Assistant Professor, School of Computer Science and Engineering for providing technological suggestions, study work, and mainly for moral support throughout the experiment, and without such understanding and guidance, our research would not have been possible.

REFERENCES

- [1] Zhang, Y., Dong, Z., Zhang, K., Shu, S., Lu, F., & Chen, J. (2021). Illumination variation-resistant video-based heart rate monitoring using LAB color space. *Optics and Lasers in Engineering*, 136, 106328.
- [2] Chen, Q., Jiang, X., Liu, X., Lu, C., Wang, L., & Chen, W. (2020, July). Non-Contact Heart Rate Monitoring in Neonatal Intensive Care Unit using RGB Camera. In 2020 42nd Annual International Conference of the IEEE Engineering in Medicine & Biology Society (EMBC) (pp. 5822-5825). IEEE.
- [3] Shah, A. A., Parah, S. A., Rashid, M., & Elhoseny, M. (2020). Efficient image encryption scheme based on the generalized logistic map for real-time image processing. *Journal of Real-Time Image Processing*, 17(6), 2139-2151.
- [4] Le, D. Q., Lie, W. N., Nhu, Q. N. Q., & Nguyen, T. T. (2020, November). Heart Rate Estimation Based on Facial Image Sequence. In 2020 5th International Conference on Green Technology and Sustainable Development (GTSD) (pp. 449-453). IEEE.
- [5] Demirezen, H., & Erdem, C. E. (2021). Heart rate estimation from facial videos using nonlinear mode decomposition and improved consistency check. *Signal, Image and Video Processing*, 1-9.
- [6] Rashid, M., Singh, H., & Goyal, V. (2020). The use of machine learning and deep learning algorithms in functional magnetic resonance imaging—A systematic review. *Expert Systems*, 37(6), e12644.
- [7] Saluja, J., Casanova, J., & Lin, J. (2019). A supervised machine learning algorithm for heart-rate detection using doppler motion-sensing radar. *IEEE Journal of Electromagnetics, RF and Microwaves in Medicine and Biology*, 4(1), 45-51.
- [8] Rashid, M., Singh, H., & Goyal, V. (2021, January). Efficient Feature Selection Technique based on Fast Fourier Transform with PSO-GA for Functional Magnetic Resonance Imaging. In 2021 2nd International Conference on Computation, Automation and Knowledge Management (ICCAKM) (pp. 238-242). IEEE.
- [9] Allen J. Photoplethysmography and its application in clinical physiological measurement. *Physiological measurement*, 2007, 28(3): R1-R39.
- [10] Lindberg L-G, Öberg PA. Optical properties of blood in motion. *Optical Engineering*, 1993, 32(2): 253-257.
- [11] Verkruysse W, Svaasan d LO, Nelson J S. Remote plethysmographic imaging using ambient light. *Optics Express*, 2008, 16(26): 21434-21445.
- [12] P. Viola and M. Jones, "Rapid object detection using a boosted cascade of simple features," *Proceedings of the 2001 IEEE Computer Society Conference on Computer Vision and Pattern Recognition*, vol.1. pp. 511-518, 2001.
- [13] Rouast, Philipp & Adam, Marc & Chiong, Raymond & Cornforth, David & Lux, Ewa. (2018). Remote heart rate measurement using low-cost RGB face video: A technical literature review. *Frontiers of Computer Science (electronic)*. 12. 858-872. 10.1007/s11704-016-6243-6.
- [14] Poenaru, Carmen & Poenaru, Vlad & Suciuc, George. (2018). Heart Rate Measurement Using Face Detection in Video. 131-134. 10.1109/ICComm.2018.8430116.
- [15] Sani, N. & Mansor, Wahidah & Lee, Yoot Khuan & Zainudin, N. & Mahrim, Syamsul Adlan. (2015). Determination of heart rate from photoplethysmogram using Fast Fourier Transform. 168-170. 10.1109/ICBAPS.2015.7292239.
- [16] Kang, M., Jung, J., Shin, S., Kang, K. H., & Kim, Y. T. (2020, January). Multi bio-signal-based algorithm using EMD and FFT for stress analysis. In 2020 IEEE International Conference on Consumer Electronics (ICCE) (pp. 1-4). IEEE.
- [17] Rahman, Hamidur & Ahmed, Mobyen & Begum, Shahina & Funk, Peter. (2016). Real Time Heart Rate Monitoring from Facial RGB Color Video Using Webcam.
- [18] Poh M-Z, McDuff DJ, Picard RW. Advancements in non-contact, multiparameter physiological measurements using a webcam. *IEEE Transactions on Biomedical Engineering*, 2011, 58(1): 1-4.
- [19] McDuff DJ, Gontarek S, Picard RW. Remote detection of photoplethysmographic systolic and diastolic peaks using a digital camera. *IEEE Transactions on Biomedical Engineering*, 2014, 61(12): 2948-2954.