

# SPIRou Data Reduction Software

## User Guide

0.3.003

For DRS SPIRou 0.2.056 (alpha pre-release)

N. Cook, F. Bouchy, E. Artigau, , M. Hobson, C. Moutou, I. Boisse, E. Martioli

2018-06-29



### Abstract

This is the guide to installing, running, and using the SPIRou DRS.

# Contents

<b>1</b>	<b>Introduction</b>	<b>1</b>
<b>2</b>	<b>Quick Install Guide</b>	<b>3</b>
2.1	Linux . . . . .	3
2.2	Mac . . . . .	4
2.3	Windows . . . . .	5
<b>3</b>	<b>Installation</b>	<b>6</b>
3.1	Introduction . . . . .	6
3.2	Download . . . . .	6
3.3	Prerequisites . . . . .	7
3.3.1	Anaconda python distribution . . . . .	7
3.3.2	Separate python installation . . . . .	7
3.4	Installation Linux and macOS . . . . .	8
3.4.1	Extraction . . . . .	8
3.4.2	Modify environmental settings . . . . .	8
3.4.3	Make recipes executable . . . . .	9
3.5	Setting up the DRS on Linux and macOS . . . . .	10
3.5.1	Other configuration parameters . . . . .	10
3.6	Validating Installation on Linux and macOS . . . . .	12
3.7	Installation Windows . . . . .	13
3.7.1	How to modify environmental settings in windows . . . . .	13
3.8	Setting up the DRS (Windows) . . . . .	15
3.8.1	Other configuration parameters . . . . .	15
3.9	Validating Installation on Windows . . . . .	17
3.10	Setting up custom constant files . . . . .	18
<b>4</b>	<b>Data Architecture</b>	<b>20</b>
4.1	Installed file structure . . . . .	20
4.2	The Installation root directory . . . . .	21
4.2.1	The bin directory . . . . .	21
4.3	The data root directory . . . . .	22
4.3.1	The raw and reduced data directories . . . . .	22
4.4	The calibration database directory . . . . .	23
<b>5</b>	<b>Using the DRS</b>	<b>24</b>
5.1	Running the DRS recipes directly . . . . .	24
5.2	Running the DRS recipes from a python script . . . . .	24
5.3	Working example of the code for SPIRou . . . . .	25
5.3.1	Overview . . . . .	25
5.3.2	Run through from command line/python shell (Linux and macOS) . . . . .	25
5.3.3	Run through python script . . . . .	28
<b>6</b>	<b>Required input header keywords</b>	<b>29</b>
6.1	Required keywords . . . . .	29
<b>7</b>	<b>User modifiable variables</b>	<b>31</b>
7.1	Variable file locations . . . . .	31
7.2	Global variables . . . . .	31
7.3	Directory variables . . . . .	33

7.4	Observatory variables . . . . .	35
7.5	Image variables . . . . .	36
7.6	Fiber variables . . . . .	38
7.7	Pre-processing variables . . . . .	41
7.8	Dark calibration variables . . . . .	43
7.9	Localization calibration variables . . . . .	45
7.10	Slit calibration variables . . . . .	53
7.11	Flat fielding calibration variables . . . . .	54
7.12	Extraction calibration variables . . . . .	58
7.13	Drift calibration variables . . . . .	61
7.14	Drift-Peak calibration variables . . . . .	65
7.15	Bad pixel calibration variables . . . . .	69
7.16	Wavelength solution variables . . . . .	71
7.17	CCF calibration variables . . . . .	79
7.18	Exposure-meter variables . . . . .	81
7.19	Quality control variables . . . . .	84
7.20	Calibration database variables . . . . .	88
7.21	Logging and printing variables . . . . .	89
<b>8</b>	<b>The Recipes</b>	<b>90</b>
8.1	The cal_DARK recipe . . . . .	90
8.1.1	The inputs . . . . .	90
8.1.2	The outputs . . . . .	90
8.1.3	Summary of procedure . . . . .	91
8.1.4	Quality Control . . . . .	91
8.1.5	Example working run . . . . .	92
8.1.6	Interactive mode . . . . .	93
8.2	The cal_BADPIX recipe . . . . .	94
8.2.1	The inputs . . . . .	94
8.2.2	The outputs . . . . .	94
8.2.3	Summary of procedure . . . . .	94
8.2.4	Quality Control . . . . .	95
8.2.5	Example working run . . . . .	96
8.3	The cal_loc recipe . . . . .	97
8.3.1	The inputs . . . . .	97
8.3.2	The outputs . . . . .	97
8.3.3	Summary of procedure . . . . .	98
8.3.4	Quality Control . . . . .	98
8.3.5	Example working run . . . . .	99
8.3.6	Interactive mode . . . . .	102
8.4	The cal_SLIT recipe . . . . .	103
8.4.1	The inputs . . . . .	103
8.4.2	The outputs . . . . .	103
8.4.3	Summary of procedure . . . . .	103
8.4.4	Quality Control . . . . .	104
8.4.5	Example working run . . . . .	104
8.4.6	Interactive mode . . . . .	106
8.5	The cal_FF recipe . . . . .	107
8.5.1	The inputs . . . . .	107
8.5.2	The outputs . . . . .	107
8.5.3	Summary of procedure . . . . .	108
8.5.4	Quality Control . . . . .	108
8.5.5	Example working run . . . . .	109

8.5.6	Interactive mode . . . . .	111
8.6	The cal_extract recipes . . . . .	112
8.6.1	The inputs . . . . .	112
8.6.2	The outputs . . . . .	114
8.6.3	Summary of procedure . . . . .	115
8.6.4	Quality Control . . . . .	116
8.6.5	Example working run . . . . .	116
8.7	The cal_DRIFT recipes . . . . .	118
8.7.1	The inputs . . . . .	118
8.7.2	The outputs . . . . .	119
8.7.3	Summary of procedure . . . . .	120
8.7.4	Example working run . . . . .	121
8.7.5	Interactive mode . . . . .	126
8.8	The cal_CCF recipe . . . . .	129
8.8.1	The inputs . . . . .	129
8.8.2	The outputs . . . . .	129
8.8.3	Summary of procedure . . . . .	130
8.8.4	Example working run . . . . .	131
8.8.5	Interactive mode . . . . .	132
8.9	The validation recipe . . . . .	133
8.9.1	The inputs . . . . .	133
8.9.2	The outputs . . . . .	133
8.9.3	Summary of procedure . . . . .	133
8.9.4	Example working run . . . . .	135
8.10	The cal_HC recipe . . . . .	136
8.11	The cal_WAVE recipe . . . . .	136
8.12	The pol_spirou recipe . . . . .	136

# Chapter 1

## Introduction

This documentation will cover the installation, data architecture, , using the DRS (with a working example), descriptions of the variables , and the recipes .

Variables are defined in detail in section 7 and will be defined throughout via the following syntax: **VARIABLE**. When referred to, one should take it as using the value set in section 7 by default or in the file described in the variables description 'Defined in' section. Clicking these variables will go to the appropriate variable description.

Certain sections will be written in code blocks, these imply text that is written into a text editor, the command shell console, or a python terminal/script. Below explains how one can distinguish these in this document.

The following denotes a line of text (or lines of text) that are to be edited in a text editor.

```
Generic text file

# A variable name that can be changes to a specific value
VARIABLE_NAME = "Variable Value"
```

These can also be shell scripts in a certain language:

```
For example in ~/.bashrc

#!/usr/bin/bash
# Find out which console you are using
echo $0
# Set environment Hello
export Hello="Hello"
```

```
For example in ~/.tcshrc

#!/usr/bin/tcsh
# Find out which console you are using
echo $0
# Set environment Hello
setenv Hello "Hello"
```

The following denotes a command to run in the command shell console

```
>> cd ~/Downloads
```

The following denotes a command line print out

```
This is a print out in the command line
produced by using the echo command
```

The following denotes a python terminal or python script

Python/Ipynb

```
import numpy as np
print("Hello world")
print("{0} seconds".format(np.sqrt(25)))
```

## Chapter 2

# Quick Install Guide

## 2.1 Linux

This is a quick guide to installation, for a more full description please see Chapter 3 . This assumes you have the latest version of Anaconda for python 3 (or python 2) and are using BASH.

1. Get the latest version of the DRS (for SPIROU version 0.2.056 (alpha pre-release)). from here: [https://github.com/njcuk9999/spirou\\_py3](https://github.com/njcuk9999/spirou_py3)
2. Download the test data from here: [http://genesis.astro.umontreal.ca/neil/spirou\\_test\\_data\\_alpha0.1.003.zip](http://genesis.astro.umontreal.ca/neil/spirou_test_data_alpha0.1.003.zip) (if required).
3. Extract the DRS (make a note of the path, hereinafter `DRS_ROOT` )
4. Add the following paths to your PATH and PYTHON PATH environmental variables

e.g. in `~/.bashrc`

```
export PATH="$DRS_ROOT/bin/:${PATH}"
export PYTHONPATH="$DRS_ROOT:$DRS_ROOT/bin/:${PYTHONPATH}"
```

5. make sure your paths are set

```
>> source ~/.bashrc
>> echo $PATH
```

6. Make recipes executable (found in the `DRS_ROOT/bin` folder) - to use from the command line.
7. Setup the DRS paths (edit the file: `'../config /config.py'`):

<code>TDATA</code>	<code>= /drs/data/</code>	/	Define the DATA directory
<code>DRS_ROOT</code>	<code>= /drs/INTROOT/</code>	/	Define the installation directory
<code>DRS_DATA_RAW</code>	<code>= /drs/data/raw</code>	/	Define the folder with the raw data files in
<code>DRS_DATA_REDUC</code>	<code>= /drs/data/reduced</code>	/	Define the directory that the reduced data should be saved to/read from
<code>DRS_CALIB_DB</code>	<code>= /drs/data/calibDB</code>	/	Define the directory that the calibration files should be saved to/read from
<code>DRS_DATA_MSG</code>	<code>= /drs/data/msg</code>	/	Define the directory that the log messages are stored in
<code>DRS_DATA_WORKING</code>	<code>= /drs/data/tmp/</code>	/	Define the working directory

8. Make sure `USER_CONFIG` and `DRS_DEBUG` are set to a value of 0 (or False) and that `ICDP_NAME` is set to `'constants_SPIROU.py'`.
9. validate the DRS installation:

```
>> cal_validate_spirou.py
```

or

```
>> python cal_validate_spirou
```

The DRS is now installed and set-up. To run see section 5 .

## 2.2 Mac

This is a quick guide to installation, for a more full description please see Chapter 3 . This assumes you have the latest version of Anaconda for python 3 (or python 2) and are using **BASH**.

1. Get the latest version of the DRS (for SPIROU version 0.2.056 (alpha pre-release)). from here: [https://github.com/njcuk9999/spirou\\_py3](https://github.com/njcuk9999/spirou_py3)
2. Download the test data from here: [http://genesis.astro.umontreal.ca/neil/spirou\\_test\\_data\\_alpha0.1.003.zip](http://genesis.astro.umontreal.ca/neil/spirou_test_data_alpha0.1.003.zip) (if required).
3. Extract the DRS (make a note of the path, hereinafter **DRS\_ROOT**)
4. Add the following paths to your PATH and PYTHON PATH environmental variables

e.g. in ~/.bashrc or ~/.bash\_profile

```
export PATH=".:DRS_ROOT/bin/:${PATH}"
export PYTHONPATH=".:DRS_ROOT:DRS_ROOT/bin/:${PYTHONPATH}"
```

5. make sure your paths are set

```
>> source ~/.bashrc
>> echo $PATH
```

6. Make recipes executable (found in the **DRS\_ROOT** /bin folder) - to use from the command line.
7. Setup the DRS paths (edit the file: './config /config.py'):

<b>TDATA</b>	= /drs/data/	/ Define the DATA directory
<b>DRS_ROOT</b>	= /drs/INTROOT/	/ Define the installation directory
<b>DRS_DATA_RAW</b>	= /drs/data/raw	/ Define the folder with the raw data files in
<b>DRS_DATA_REDUC</b>	= /drs/data/reduced	/ Define the directory that the reduced data should be saved to/read from
<b>DRS_CALIB_DB</b>	= /drs/data/calibDB	/ Define the directory that the calibration files should be saved to/read from
<b>DRS_DATA_MSG</b>	= /drs/data/msg	/ Define the directory that the log messages are stored in
<b>DRS_DATA_WORKING</b>	= /drs/data/tmp/	/ Define the working directory

8. Make sure **USER\_CONFIG** and **DRS\_DEBUG** are set to a value of 0 (or False) and that **ICDP\_NAME** is set to 'constants\_SPIROU.py'.
9. validate the DRS installation:

```
>> cal_validate_spirou.py
```

or

```
>> python cal_validate_spirou
```

The DRS is now installed and set-up. To run see section 5 .



## 2.3 Windows

This is a quick guide to installation, for a more full description please see Chapter 3 . This assumes you have the latest version of Anaconda for python 3 (or python 2)

1. Get the latest version of the DRS (for SPIROU version 0.2.056 (alpha pre-release)). from here: [https://github.com/njcuk9999/spirou\\_py3](https://github.com/njcuk9999/spirou_py3)
2. Download the test data from here: [http://genesis.astro.umontreal.ca/neil/spirou\\_test\\_data\\_alpha0.1.003.zip](http://genesis.astro.umontreal.ca/neil/spirou_test_data_alpha0.1.003.zip) (if required).
3. Extract the DRS (make a note of the path, hereinafter `DRS_ROOT` )
4. Add the following paths to your PATH environmental variable

In "Environmental Variables"

```
DRS_ROOT\bin\;
```

5. Add the following paths to your PYTHONPATH environmental variable

In "Environmental Variables"

```
%PYTHONPATH%;DRS_ROOT;DRS_ROOT\bin\;
```

6. Setup the DRS paths (edit the file: ‘../config /config.py’):

```

TDATA          = C:\\Users\\User\\          / Define the DATA directory
                \\Documents\\drs\\data
DRS_ROOT        = C:\\Users\\User\\          / Define the installation directory
                \\Documents\\drs\\INTRROOT
DRS_DATA_RAW    = C:\\Users\\User\\          / Define the folder with the raw data files
                \\Documents\\drs\\data\\raw    in
DRS_DATA_REduc  = C:\\Users\\User\\          / Define the directory that the reduced
                \\Documents\\drs\\data\\      data should be saved to/read from
                \\reduced
DRS_CALIB_DB     = C:\\Users\\User\\          / Define the directory that the calibra-
                \\Documents\\drs\\data\\      tion files should be saved to/read from
                \\calibDB
DRS_DATA_MSG     = C:\\Users\\User\\          / Define the directory that the log mes-
                \\Documents\\drs\\data\\msg    sages are stored in
DRS_DATA_WORKING= C:\\Users\\User\\          / Define the working directory
                \\Documents\\drs\\data\\tmp

```

**Note:** Note paths in windows must have a ‘\\’ also the python files must be open with a valid editor such as Sublime Text, Notepad++, Spyder or Pycharm for example

7. Make sure `USER_CONFIG` and `DRS_DEBUG` are set to a value of 0 (or False) and that `ICDP_NAME` is set to ‘constants\_SPIROU.py’.
8. validate the DRS installation:

```
>> python cal_validate_spirou
```

The DRS is now installed and set-up. To run see section 5 .

## Chapter 3

# Installation

### 3.1 Introduction

Once finalized the installation should just be a download, run set-up.py and configure the DRS directories, however, during development the following stages are required.

### 3.2 Download

Get the latest version of the DRS (for SPIROU version 0.2.056 (alpha pre-release)). Use any of the following ways:

- manually download from here: [https://github.com/njcuk9999/spirou\\_py3\protect\kern+.1667em\relax](https://github.com/njcuk9999/spirou_py3\protect\kern+.1667em\relax)

- use Git:

```
>> git checkout https://github.com/njcuk9999/spirou_py3.git
```

- use SVN:

```
>> svn checkout https://github.com/njcuk9999/spirou_py3.git
```

- use ssh:

```
>> scp -r git@github.com:njcuk9999/spirou_py3.git
```

## 3.3 Prerequisites

It is recommended to install the latest version of Anaconda python distribution, available for Windows, macOS and Linux (here: <https://www.anaconda.com/download/>). However one can run the DRS on a native python installation.

We recommend python 3 over python 2 for long term continued support (however the latest version of the DRS supports the newest versions of python 2.7).

**Note:** Before installing the DRS you must have one of the following:

- Latest version of Anaconda (for python 2 or python 3) — RECOMMENDED
- An Up-to-date version of python (python 2 or python 3)

### 3.3.1 Anaconda python distribution

A valid version of the Anaconda python distribution (for python 2 or python 3) Currently tested version of python are:

- Python 2.7.13 and Anaconda 4.4.0
- Python 3.6.3 and Anaconda 5.0.1 — RECOMMENDED

### 3.3.2 Separate python installation

An up-to-date version of python (either python 2 or python 3) and the following python modules (with version of python they were tested with).

- Python 3.6.4
  - ASTROPY (tested with version 2.0.3)
  - MATPLOTLIB (tested with version 2.1.2)
  - NUMPY (tested with version 1.14.0)
  - SCIPY (tested with version 1.0.0)
  - and the following built-in modules (comes with python): `__FUTURE__`, `CALENDER`, `CODE`, `COLLECTIONS`, `DATETIME`, `FILECMP`, `GLOB`, `OS`, `PDB`, `PKG_RESOURCES`, `SHUTIL`, `STRING`, `SYS`, `TIME`, `WARNINGS`.
- Python 2.7.14
  - astropy (tested with version 2.0.3)
  - matplotlib (tested with version 2.1.2)
  - numpy (tested with version 1.14.0)
  - scipy (tested with version 1.0.0)
  - and the following built-in modules (comes with python): `__FUTURE__`, `CALENDER`, `CODE`, `COLLECTIONS`, `DATETIME`, `FILECMP`, `GLOB`, `OS`, `PDB`, `PKG_RESOURCES`, `SHUTIL`, `STRING`, `SYS`, `TIME`, `WARNINGS`.

## 3.4 Installation Linux and macOS

Currently the DRS has to be installed manually. This involves the following steps:

1. Extraction (Section 3.4.1)
2. Modify environmental settings (Section 3.4.2)
3. Make recipes executable (Section 3.4.3)

### 3.4.1 Extraction

The first step is to extract the DRS into a folder (the `DRS_ROOT`). Do this by using the following commands:

```
>> cd DRS_ROOT
>> unzip DRS.zip
```

### 3.4.2 Modify environmental settings

The next step is to modify your `PATH` and `PYTHONPATH` environmental variables (to include the `DRS_ROOT`). This depends which shell you are using (type `echo $0` to find out which).

- In bash open the `‘.bashrc’` or `‘.bash_profile’` text file in your home (`~`) directory (or create it if it doesn't exist)

e.g. in `~/ .bashrc` or `~/ .bash_profile`

```
export PATH=".:DRS_ROOT/bin/:${PATH}"
export PYTHONPATH=".:DRS_ROOT:DRS_ROOT/bin/:${PYTHONPATH}"
```

- In csh/tcsh open the `‘.cshrc’` or `‘.tcshrc’` text file in your home (`~`) directory (or create it if it doesn't exist).

e.g. in `~/ .tcshrc`

```
setenv PATH ".:DRS_ROOT/bin/:${PATH}"
```

In csh/tcsh one has to check whether `‘$PYTHONPATH’` exists before adding to the `PYTHONPATH`. To check type:

```
>> echo $PYTHONPATH
```

If the response is:

```
PYTHONPATH: Undefined variable.
```

Then in the `‘.cshrc’` or `‘.tcshrc’` add:

e.g. in `~/ .tcshrc`

```
setenv PYTHONPATH ".:DRS_ROOT:DRS_ROOT/bin/"
```

If the response is some paths, then in the '.cshrc' or '.tcshrc' add:

e.g. in ~/.tcshrc

```
setenv PYTHONPATH ".:DRS_ROOT:DRS_ROOT/bin/${PYTHONPATH}"
```

### 3.4.3 Make recipes executable

To run the recipes from the command line (without starting python) one must make them executable. Do this by using the following command:

```
>> chmod +x DRS_ROOT/bin/*.py
```

## 3.5 Setting up the DRS on Linux and macOS

Before running the DRS one must set the data paths.

The ‘../config /config.py’ file is located in the [DRS\\_ROOT](#) in the config folder.

i.e. at [DRS\\_ROOT](#) /config/./config /config.py

The following keywords **must** be changed (and must be a valid path):

<a href="#">TDATA</a>	=	/drs/data/	/	Define the DATA directory
<a href="#">DRS_ROOT</a>	=	/drs/INTROOT/	/	Define the installation directory
<a href="#">DRS_DATA_RAW</a>	=	/drs/data/raw	/	Define the folder with the raw data files in
<a href="#">DRS_DATA_REDUC</a>	=	/drs/data/reduced	/	Define the directory that the reduced data should be saved to/read from
<a href="#">DRS_CALIB_DB</a>	=	/drs/data/calibDB	/	Define the directory that the calibration files should be saved to/read from
<a href="#">DRS_DATA_MSG</a>	=	/drs/data/msg	/	Define the directory that the log messages are stored in
<a href="#">DRS_DATA_WORKING</a>	=	/drs/data/tmp/	/	Define the working directory

**Note:** Some text editors (such as TextEdit on macOS) use ‘smart speech-marks’ these characters are invalid for python and thus care must be taken when editing the configuration files. The [cal\\_validate\\_spirou](#) recipe (Section 3.6) will check for invalid characters and show the lines which do not have valid characters (valid characters are ASCII letters, digits, punctuation and white spaces as defined by python’s ‘STRING’ module). We suggest using text editors such as [SUBLIME-TEXT](#) or a python IDE such as [PYCHARM](#).

### 3.5.1 Other configuration parameters

If one is using the DRS in the default setup one needs to make sure the following parameters are set correctly:

- [USER\\_CONFIG](#) is set to a value of 0 (or False)
- [DRS\\_DEBUG](#) is set to a value of 0 (or False)
- [ICDP\\_NAME](#) is set to ‘constants\_SPIROU.py’

The following keywords can be changed:

```
DRS_PLOT      =      1    /   Whether to show plots
PRINT_LEVEL   =   "all"   /   Level at which to print
LOG_LEVEL     =   "all"   /   Level at which to log in log file
```

For the ‘`PRINT_LEVEL`’ and ‘`LOG_LEVEL`’ keywords the values are set as follows:

- "all" – prints all events
- "info" – prints info, warning and error events
- "warning" – prints warning and error events
- "error" – print only error events

## 3.6 Validating Installation on Linux and macOS

**Note:** One must install the DRS (Section 3.4) AND set up the DRS (Section 3.5) before validation will be successful.

There are four ways to run the DRS in Linux and macOS (thus four ways to verify installation was correct).

- To validate running from command line type:

```
>> cal_validate_spirou.py
```

- To validate running from python/ipython from the command line type:

```
>> python cal_validate_spirou
>> ipython cal_validate_spirou
```

- To validate running from ipython, open ipython and type:

Python/Ipython

```
run cal_validate_spirou.py
```

- To validate running from import from python/ipython, open python/ipython and type:

Python/Ipython

```
import cal_validate_spirou
cal_validate_spirou.main()
```

If validation is successful the following should appear:

```
HH:MM:SS.S - || *****
HH:MM:SS.S - || * SPIROU Q(#) Geneva Observatory (0.0.1)
HH:MM:SS.S - || *****
HH:MM:SS.S - ||(dir_data_raw)      DRS_DATA_RAW=/drs/data/raw
HH:MM:SS.S - ||(dir_data_reduc)    DRS_DATA_REDUCE=/drs/data/reduced
HH:MM:SS.S - ||(dir_calib_db)      DRS_CALIB_DB=/drs/data/calibDB
HH:MM:SS.S - ||(dir_data_msg)      DRS_DATA_MSG=/drs/data/msg
HH:MM:SS.S - ||(print_level)       PRINT_LEVEL=all          %(error/warning/info/all)
HH:MM:SS.S - ||(log_level)         LOG_LEVEL=all             %(error/warning/info/all)
HH:MM:SS.S - ||(plot_graph)        DRS_PLOT=1                %(def/undef/trigger)
HH:MM:SS.S - ||(used_date)         DRS_USED_DATE=undefined
HH:MM:SS.S - ||(working_dir)       DRS_DATA_WORKING=/drs/data/tmp/
HH:MM:SS.S - ||                   DRS_INTERACTIVE is not set, running on-line mode
HH:MM:SS.S - ||
HH:MM:SS.S - ||Validation successful. DRS installed corrected.
```



## 3.7 Installation Windows


This is very similar currently to the Linux/macOS installation (in the future a '.exe' file will be given).

1. Extract to `DRS_ROOT` with your favourite unzipping software.
2. Add `DRS_ROOT` to your PYTHONPATH (Section 3.7.1)

### 3.7.1 How to modify environmental settings in windows


This process is a little more convoluted than on Linux or macOS system.

1. Go to 'My computer > Properties > Advanced System Settings > Environmental Variables'. Note in windows 10 you can also click the windows icon and type 'Advanced System Settings' then click 'Environment Variables'.
2. under system variable 'Path' click edit and add:




```
DRS_ROOT ; DRS_ROOT \bin;
```

3. if under system variable 'PYTHONPATH' exists click edit and add '`DRS_ROOT`;' to the end.  
i.e.




```
DRS_ROOT ; DRS_ROOT \bin;
```

4. if under system variables 'PYTHONPATH' does not exist create a new variable called 'PYTHONPATH' and add:



```
%PYTHONPATH%; DRS_ROOT ; DRS_ROOT \bin\;
```

Figure 3.1 shows screen-grabs of the various steps above to aid in updating PATH and PYTHONPATH. For problems/troubleshooting see here: <https://stackoverflow.com/questions/3701646>.



**Figure 3.1** (a) Once in “Advanced system properties” click “Environment Variables” (b) Click “Path” and click “Edit...” to edit the “Path” environmental variable (c) Once in the “Path” environmental variable click “New” to add a new path (d) Type in the new line to add variable and click “OK” (e) Once back in the Environmental variable page click “New” to add ‘PYTHONPATH’ (f) Set the variable name to “PYTHONPATH” and edit the variable value accordingly.

## 3.8 Setting up the DRS (Windows)

Before running the DRS one must set the data paths.

The ‘./config /config.py’ file is located in the `DRS_ROOT` in the config folder.  
i.e. at `DRS_ROOT\\config\\config.txtfile`

The following keywords **must** be changed (and must be a valid path):

<code>TDATA</code>	<code>= C:\\Users\\User\\ \\Documents\\drs\\ \\data</code>	/ Define the DATA directory
<code>DRS_ROOT</code>	<code>= C:\\Users\\User\\ \\Documents\\drs\\ \\INTROOT</code>	/ Define the installation directory
<code>DRS_DATA_RAW</code>	<code>= C:\\Users\\User\\ \\Documents\\drs\\ \\data\\raw</code>	/ Define the folder with the raw data files in
<code>DRS_DATA_REDUC</code>	<code>= C:\\Users\\User\\ \\Documents\\drs\\ \\data\\reduced</code>	/ Define the directory that the reduced data should be saved to/read from
<code>DRS_CALIB_DB</code>	<code>= C:\\Users\\User\\ \\Documents\\drs\\ \\data\\calibDB</code>	/ Define the directory that the calibration files should be saved to/read from
<code>DRS_DATA_MSG</code>	<code>= C:\\Users\\User\\ \\Documents\\drs\\ \\data\\msg</code>	/ Define the directory that the log messages are stored in
<code>DRS_DATA_WORKING</code>	<code>= C:\\Users\\User\\ \\Documents\\drs\\ \\data\\tmp</code>	/ Define the working directory

**Note:** Note: On windows paths in windows must have a ‘\\’ also the python files must be open with a valid editor such as Sublime Text, Notepad++, Spyder or Pycharm for example

### 3.8.1 Other configuration parameters

If one is using the DRS in the default setup one needs to make sure the following parameters are set correctly:

- `USER_CONFIG` is set to a value of 0 (or False)
- `DRS_DEBUG` is set to a value of 0 (or False)
- `ICDP_NAME` is set to ‘constants\_SPIROU.py’

The following keywords can be changed:

```
DRS_PLOT      =      1    /   Whether to show plots
PRINT_LEVEL   =   "all"   /   Level at which to print
LOG_LEVEL     =   "all"   /   Level at which to log in log file
```

For the 'PRINT\_LEVEL and LOG\_LEVEL keywords the values are set as follows:

- "all" – prints all events
- "info" – prints info, warning and error events
- "warning" – prints warning and error events
- "error" – print only error events

## 3.9 Validating Installation on Windows

**Note:** One must install the DRS (Section 3.7) AND set up the DRS (Section 3.5) before validation will be successful.

In windows there are currently 3 ways to run the RS (running in python/ipython).

- To validate running from python/ipython from the command line type:

```
>> python cal_validate_spirou
>> ipython cal_validate_spirou
```

- To validate running from ipython, open ipython and type:

```
Python/Ipython
run cal_validate_spirou.py
```

- To validate running from import from python/ipython, open python/ipython and type:

```
Python/Ipython
import cal_validate_spirou
cal_validate_spirou.main()
```

If validation is successful the following should appear:

```
17:34:19.0 - || *****
17:34:19.0 - || * SPIROU @(#) Geneva Observatory (0.1.016)
17:34:19.0 - || *****
17:34:19.0 - ||(dir_data_raw)      DRS_DATA_RAW=C:\\Users\\User\\Documents\\drs\\data\\raw
17:34:19.0 - ||(dir_data_reduc)    DRS_DATA_REduc=C:\\Users\\User\\Documents\\drs\\data\\reduced
17:34:19.0 - ||(dir_calib_db)      DRS_CALIB_DB=C:\\Users\\User\\Documents\\drs\\data\\calibDB
17:34:19.0 - ||(dir_data_msg)      DRS_DATA_MSG=C:\\Users\\User\\Documents\\drs\\data\\msg
17:34:19.0 - ||(print_level)      PRINT_LEVEL=all          %(error/warning/info/all)
17:34:19.0 - ||(log_level)         LOG_LEVEL=all          %(error/warning/info/all)
17:34:19.0 - ||(plot_graph)        DRS_PLOT=1            %(def/undef/trigger)
17:34:19.0 - ||(used_date)         DRS_USED_DATE=undefined
17:34:19.0 - ||(working_dir)       DRS_DATA_WORKING=C:\\Users\\User\\Documents\\drs\\data\\tmp
17:34:19.0 - ||                   DRS_INTERACTIVE is not set, running on-line mode
17:34:19.0 - ||                   DRS_DEBUG is set, debug mode level:1
17:34:19.0 - ||
17:34:19.0 - ||Validation successful. DRS installed corrected.
```

## 3.10 Setting up custom constant files

It is also possible to set up custom constant files (in a folder separate from the DRS).

To do this one need to change the `USER_CONFIG` parameter to 1 (or True). This tells the DRS to look for `DRS_UCONFIG` parameter either in the master config file (`../config /config.py`) and in the system environment (for the variable `'DRS_UCONFIG'`).

**Note:** The path set in the system environment takes precedence over the path set in the master config file (`../config /config.py`).

All constants are loaded initial from the master file and then any parameter in the configuration file at the custom location overwrites the value in the master file.

For example:

In `".../INTROOT/config/config.py"`

```
USER_CONFIG = 1
DRS_ROOT = '/drs/spirou/INTROOT/'
DRS_DATA_RAW = '/drs/spirou/data/raw'
DRS_DATA_REduc = '/drs/spirou/data/reduced'
DRS_UCONFIG = '/home/user/spirou/config.py'
```

In `" /home/user/spirou/config.py"`

```
DRS_DATA_RAW = '/DATA/RAW'
DRS_DATA_REDIC = '/DATA/RED'
```

OR

e.g. in `~/.bashrc` or `~/.bash_profile`

```
export DRS_UCONFIG=/home/user/spirou/config.py
```

In `".../INTROOT/config/config.py"`

```
USER_CONFIG = 1
DRS_ROOT = '/drs/spirou/INTROOT/'
DRS_DATA_RAW = '/drs/spirou/data/raw'
DRS_DATA_REduc = '/drs/spirou/data/reduced'
```

In `" /home/user/spirou/config.py"`

```
DRS_DATA_RAW = '/DATA/RAW'
DRS_DATA_REDIC = '/DATA/RED'
```

Then once the DRS runs, `DRS_ROOT` is set from `/INTROOT/config/config.py` and `DRS_DATA_RAW` and `DRS_DATA_REduc` are set from `/home/user/spirou/config.py` and thus the variables set will be:

```
DRS_ROOT = '/drs/spirou/INTROOT/'
DRS_DATA_RAW = '/DATA/RAW'
DRS_DATA_REDIC = '/DATA/RED'
```

**Note:** Constants/variables set in the custom constant files **always** take precedence over the master files.

**Note:** Any constant/variable not set in a custom constant file is taken from the master files.

**Note:** For other configuration files (i.e. `ICDP_NAME`) the name can be changed in the master configuration file (`../config /config.py`) thus allowing an easy switch between constant files. The custom path will always use `ICDP_NAME` to locate the file.

This also works for other configuration files (i.e. `ICDP_NAME`). Thus one can have a completely separate set of configuration files and switch between folders in the master configuration file (`../config /config.py`) or by editing the environmental variables.

e.g. in `~/.bashrc` or `~/.bash_profile`

```
export DRS_UCONFIG=/home/user/spirou/config.py
```

e.g. in `~/.tcshrc`

```
setenv DRS_UCONFIG /home/user/spirou/config.py
```

See the config folder (`../config/`) for example `DRS_UCONFIG` directories and files.

## Chapter 4

## Data Architecture

Described below is the file structure, after correct installation (Chapter 3).


## 4.1 Installed file structure

The file structure should look as follows:



\* This is the recommended file structure and raw, reduced, calibDB, msg and tmp can be changed using the `DRS_DATA_RAW`, `DRS_DATA_REDUCE`, `DRS_CALIB_DB`, `DRS_DATA_MSG`, and `DRS_DATA_WORKING` variables in Section 3.5.

i.e. for the paths given in Section 3.5 this would be:





## 4.2 The Installation root directory

The `DRS_ROOT` contains all the installed recipes, modules functions, documentation and configuration files needed to run the DRS. The file structure is set up as below:

```
{dir}
├── {DRS_ROOT}
│   ├── bin .....Recipes
│   ├── config .....Configuration files
│   ├── documentation .....Documentation files
│   └── SpirouDRS .....The DRS Module
```

### 4.2.1 The bin directory

The bin directory is located in the `DRS_ROOT` directory. This contains all the recipes that can be used. A detailed description of all recipes can be found in Chapter 8 but are listed here for completeness.

```
{dir}
├── {DRS_ROOT}
│   ├── bin .....Recipes
│   │   ├── cal_BADPIX_spirou .....See Section 8.2
│   │   ├── cal_CCF_E2DS_spirou .....See Section 8.8
│   │   ├── cal_DARK_spirou .....See Section 8.1
│   │   ├── cal_DRIFT_RAW_spirou .....See Section 8.7
│   │   ├── cal_DRIFT_E2DS_spirou .....See Section 8.7
│   │   ├── cal_DRIFTPEAK_E2DS_spirou .....See Section 8.7
│   │   ├── cal_extract_RAW_spirou .....See Section 8.6
│   │   ├── cal_extract_RAW_spirouAB .....See Section 8.6
│   │   ├── cal_extract_RAW_spirouC .....See Section 8.6
│   │   ├── cal_FF_RAW_spirou .....See Section 8.5
│   │   ├── cal_HC_E2DS_spirou .....See Section 8.10
│   │   ├── cal_loc_RAW_spirou .....See Section 8.3
│   │   ├── cal_SLIT_spirou .....See Section 8.4
│   │   ├── cal_validate_spirou .....See Section 8.9
│   │   └── cal_WAVE_E2DS_spirou .....See Section 8.11
```

### 4.3 The data root directory

This is the directory where all the data should be stored. The default and recommended design is to have `DRS_DATA_RAW`, `DRS_DATA_REDUCE`, `DRS_CALIB_DB`, `DRS_DATA_MSG`, and `DRS_DATA_WORKING` as sub-directories of `DRS_ROOT`. However as in Section 3.5. these sub-directories can be defined elsewhere.

#### 4.3.1 The raw and reduced data directories

The raw observed data is stored under the `DRS_DATA_RAW` path, the files are stored by night in the form `YYYYMMDD`.

The file structure can be seen below:

```
{DRS_DATA_RAW}
├── YYYYMMDD .....night_repository
│   ├── .....Raw observation files
│   ├── dark_dark{name}.fits
│   ├── dark_flat{name}.fits
│   ├── flat_dark{name}.fits
│   └── fp_fp{name}.fits
```

## 4.4 The calibration database directory

```
{TDATA}
├─ calibDB or {DRS_CALIB_DB}
│   └─ master_calib_SPIROU.txt
│       └─ .....The calibration fits files
```

The calibDB contains all the calibration files that pass the quality tests and a test file `ic_calibDB_filename`. It is located at `DRS_CALIB_DB` or if this is not defined is located by default at the `TDATA` directory. Each line in this file is a unique calibration file and lines are formatted in the following manner:

In calibration database file

```
{key} {night_repository} {filename} {human readable date} {unix time}
```

where

- **key** is a code assigned for each type of calibration file. Currently accepted keys are:
  - DARK - Created from `cal_DARK_spirou`
  - ORDER\_PROFIL\_fiber - Created in `cal_loc_RAW_spirou`
  - LOC\_C - Created in `cal_loc_RAW_spirou`
  - TILT - Created in `cal_SLIT_spirou`
  - FLAT\_fiber - Created in `cal_FF_RAW_spirou`
  - WAVE - Currently manually added
- **night\_repository** is the raw data observation directory (in `DRS_DATA_RAW`) normally in the form YYYYMMDD.
- **filename** is the filename of the calibration file (located in the calibDB).
- **human readable date** is the date in DD/MM/YY/HH:MM:SS.ss format taken from the header keyword 'ACQTIME1' of the file that created the calibration file.
- **unix time** is the time (as in **human readable date**) but in unix time (in seconds).

An example working `ic_calibDB_filename` is shown below (assuming the listed files are present in `DRS_CALIB_DB`)

In calibration database file

```
DARK 20170710 dark_dark02d406.fits 07/10/17/16:37:48 1499704668.0
ORDER_PROFIL_C 20170710 dark_flat02f10_order_profil_C.fits 07/10/17/17:03:50 1499706230.0
LOC_C 20170710 dark_flat02f10_loco_C.fits 07/10/17/17:03:50 1499706230.0
ORDER_PROFIL_AB 20170710 flat_dark02f10_order_profil_AB.fits 07/10/17/17:07:08 1499706428.0
LOC_AB 20170710 flat_dark02f10_loco_AB.fits 07/10/17/17:07:08 1499706428.0
TILT 20170710 fp_fp02a203_tilt.fits 07/10/17/17:25:15 1499705515.0
FLAT_C 20170710 dark_flat02f10_flat_C.fits 07/10/17/17:03:50 1499706230.0
WAVE 20170710 spirou_wave_ini3.fits 07/10/17/17:03:50 1499706230.0
```

## Chapter 5

# Using the DRS

There are two ways to run the DRS recipes. The first (described in Section 5.1) directly calls the code and inputs arguments (either from the command line or from python), the second way is to import the recipes in a python script and define arguments in a call to a function (see Section 5.2).

## 5.1 Running the DRS recipes directly

As in Chapter 3, using Linux or macOS one can run DRS recipes from the command line or from python, in windows one is required to be in python before running the scripts. Below we use `cal_DARK_spirou` as an example:

- To run from command line type:

```
>> cal_DARK_spirou YYMMDD Filenames
```

- To run from python/ipython from the command line type:

```
>> python cal_DARK_spirou YYMMDD Filenames
>> ipython cal_DARK_spirou YYMMDD Filenames
```

- To run from ipython, open ipython and type:

Python/Ipypthon

```
run cal_DARK_spirou YYMMDD Filenames
```

## 5.2 Running the DRS recipes from a python script

In any operating system one can also import a recipe and call a function to run the code. This is useful in batch operations, timing tests and unit tests for example. Below we use `cal_DARK_spirou` as an example:

Python/Ipypthon

```
# import the recipe
import cal_DARK_spirou
# define the night folder name
night_name = "20170710"
# define the file(s) to run through the code
files = ['dark_dark02d406.fits']
# run code
cal_validate_spirou.main(night_name=night_name, files=files)
```

## 5.3 Working example of the code for SPIRou

### 5.3.1 Overview

For this example all files are from:

```
>> spirou@10.102.14.81:/data/RawImages/H2RG-AT4/AT4-04/2017-07-10_15-36-18/ramps/
```

following our example data architecture (from Section 3.5 and shown explicitly in Section 4.1) all files should be places in the [DRS\\_DATA\\_RAW](#) ([/drs/data/raw](#) in our case).

and we will also need the current WAVE file from here:

```
>> spirou@10.102.14.81:/data/reduced/DATA-CALIB/spirou_wave_ini3.fits
```

which needs to be placed in the [DRS\\_CALIB\\_DB](#) directory ([/drs/data/calibDB](#) in our case).

Starting with RAMP files and ending with extracted orders and calculated drifts we need to run six codes:

1. [cal\\_DARK\\_spirou](#) (See Section 8.1)
2. [cal\\_loc\\_RAW\\_spirou](#) ( $\times 2$ ) (See Section 8.3)
3. [cal\\_SLIT\\_spirou](#) (See Section 8.4)
4. [cal\\_FF\\_RAW\\_spirou](#) ( $\times 2$ ) (See Section 8.5)
5. (add [spirou\\_wave\\_ini3.fits](#) to [calibDB](#))
6. [cal\\_extract\\_RAW\\_spirouAB](#) and [cal\\_extract\\_RAW\\_spirouC](#) (many times) (See Section 8.6)
7. [cal\\_DRIFT\\_RAW\\_spirou](#) (See Section 8.7)

### 5.3.2 Run through from command line/python shell (Linux and macOS)

As long as all codes are executable (see Section 3.4.3) one can run all codes from the command line or if not executable or one has a preference for python one can run the following with ‘python {command}’, ‘ipython {command}’ or indeed through an interactive ipython session using ‘run {command}’.

1. run the dark extraction on the ‘dark\_dark’ file:

```
>> cal_DARK_spirou.py 20170710 dark_dark02d406.fits
```

2. run the order localisation on the ‘dark\_flat’ files:

```
>> cal_loc_RAW_spirou.py 20170710 dark_flat02f10.fits dark_flat03f10.fits dark_flat04f10.fits
    dark_flat05f10.fits dark_flat06f10.fits
```

3. run the order localisation on the ‘flat\_dark’ files:

```
>> cal_loc_RAW_spirou.py 20170710 flat_dark02f10.fits flat_dark03f10.fits flat_dark04f10.fits
    flat_dark05f10.fits flat_dark06f10.fits
```

4. run the slit calibration on the ‘fp\_fp’ files.

```
>> cal_SLIT_spirou.py 20170710 fp_fp02a203.fits fp_fp03a203.fits fp_fp04a203.fits
```

5. run the flat field creation on the 'dark\_flat' files:

**Note:** if using same files as above AND `calib_db_match="older"` you will get an error message when running the file (the tilt file is newer than input data) to solve this change `calib_db_match="closest"`.

```
>> cal_FF_RAW_spirou.py 20170710 dark_flat02f10.fits dark_flat03f10.fits dark_flat04f10.fits
dark_flat05f10.fits dark_flat06f10.fits
```

6. Currently we do not create a new wavelength calibration file for this run.

Therefore we need one (as stated in the above section). We use the ones from here:

```
>> spirou@10.102.14.81:/data/reduced/DATA-CALIB/spirou_wave_ini3.fits
>> spirou@10.102.14.81:/data/.../AT4-04/2017-10-11_21-32-17 2017
-10-11_21-32-17_hcone_hcone02c406_wave_AB.fits
>> spirou@10.102.14.81:/data/.../AT4-04/2017-10-11_21-32-17 2017
-10-11_21-32-17_hcone_hcone02c406_wave_C.fits
```

then place it in the `DRS_CALIB_DB` folder. You will also need to edit the '`ic_calibDB_filename`' file located in `DRS_CALIB_DB`.

Add the following line to '`ic_calibDB_filename`'

In calibration database file

```
WAVE_AB AT4-04/2017-10-11_21-32-17 2017-10-11_21-32-17_hcone_hcone02c406_wave_AB.fits
2014-08-11-03:42:12.000000 1407728532
WAVE_A 20170710 spirou_wave_ini3.fits 2000-01-01-00:00:00.00 946684800
WAVE_B 20170710 spirou_wave_ini3.fits 2000-01-01-00:00:00.00 946684800
WAVE_C AT4-04/2017-10-11_21-32-17 2017-10-11_21-32-17_hcone_hcone02c406_wave_C.fits
```

and the '`master_calib_SPIROU.txt`' should look like this:

In calibration database file

```
WAVE_AB AT4-04/2017-10-11_21-32-17 2017-10-11_21-32-17_hcone_hcone02c406_wave_AB.fits
2014-08-11-03:42:12.000000 1407728532
WAVE_A 20170710 spirou_wave_ini3.fits 2000-01-01-00:00:00.00 946684800
WAVE_B 20170710 spirou_wave_ini3.fits 2000-01-01-00:00:00.00 946684800
WAVE_C AT4-04/2017-10-11_21-32-17 2017-10-11_21-32-17_hcone_hcone02c406_wave_C.fits
DARK 20170710 dark_dark02d406.fits 07/10/17/16:37:48 1499704668.0
ORDER_PROFIL_C 20170710 dark_flat02f10_order_profil_C.fits 07/10/17/17:03:50 1499706230.0
LOC_C 20170710 dark_flat02f10_loco_C.fits 07/10/17/17:03:50 1499706230.0
ORDER_PROFIL_AB 20170710 flat_dark02f10_order_profil_AB.fits 07/10/17/17:07:08 1499706428.0
LOC_AB 20170710 flat_dark02f10_loco_AB.fits 07/10/17/17:07:08 1499706428.0
TILT 20170710 fp_fp02a203_tilt.fits 07/10/17/17:07:08 1499706428.0
```

7. run the extraction files on the 'hcone\_dark', 'dark\_hcone', 'hcone\_hcone', 'dark\_dark\_AHC1', 'hctwo\_dark', 'dark\_hctwo', 'hctwo-hctwo', 'dark\_dark\_AHC2' and 'fp\_fp' files. For example for the 'fp\_fp' files:

```
>> cal_extract_RAW_spirouAB.py 20170710 fp_fp02a203.fits fp_fp03a203.fits fp_fp04a203.fits
>> cal_extract_RAW_spirouC.py 20170710 fp_fp02a203.fits fp_fp03a203.fits fp_fp04a203.fits
```

8. run the drift calculation on the 'fp\_fp' files:

```
>> @cal_DRIFT_RAW_spirou.py 20170710 @fp_fp02a203.fits fp_fp03a203.fits fp_fp04a203.fits
```

### 5.3.3 Run through python script

The process is in the same order as Section 5.3.2, including adding the ‘WAVE’ lines to the calibDB folder).

Python/Ipython

```
import cal_DARK_spirou, cal_loc_RAW_spirou
import cal_SLIT_spirou, cal_FF_RAW_spirou
import cal_extract_RAW_spirou, cal_DRIFT_RAW_spirou
import matplotlib.pyplot as plt

# define constants
NIGHT_NAME = '20170710'

# cal_dark_spirou
files = ['dark_dark02d406.fits']          # set up files
cal_DARK_spirou.main(NIGHT_NAME, files)  # run cal_dark_spirou
plt.close('all')                         # close graphs

# cal_loc_RAW_spirou - flat_dark
files = ['flat_dark02f10.fits', 'flat_dark03f10.fits', 'flat_dark04f10.fits',
        'flat_dark05f10.fits', 'flat_dark06f10.fits']
cal_loc_RAW_spirou.main(NIGHT_NAME, files)
plt.close('all')

# cal_loc_RAW_spirou - dark_flat
files = ['dark_flat02f10.fits', 'dark_flat03f10.fits', 'dark_flat04f10.fits',
        'dark_flat05f10.fits', 'dark_flat06f10.fits']
cal_loc_RAW_spirou.main(NIGHT_NAME, files)
plt.close('all')

# cal_SLIT_spirou
files = ['fp_fp02a203.fits', 'fp_fp03a203.fits', 'fp_fp04a203.fits']
cal_SLIT_spirou.main(NIGHT_NAME, files)
plt.close('all')

# cal_FF_RAW_spirou - flat_dark
files = ['flat_dark02f10.fits', 'flat_dark03f10.fits', 'flat_dark04f10.fits',
        'flat_dark05f10.fits', 'flat_dark06f10.fits']
cal_FF_RAW_spirou.main(NIGHT_NAME, files)
plt.close('all')

# cal_FF_RAW_spirou - dark_flat
files = ['dark_flat02f10.fits', 'dark_flat03f10.fits', 'dark_flat04f10.fits',
        'dark_flat05f10.fits', 'dark_flat06f10.fits']
cal_FF_RAW_spirou.main(NIGHT_NAME, files)
plt.close('all')

# cal_extract_RAW_spirou - fp_fp AB
files = ['fp_fp02a203.fits', 'fp_fp03a203.fits', 'fp_fp04a203.fits']
cal_extract_RAW_spirou.main(NIGHT_NAME, files, 'AB')
plt.close('all')

# cal_extract_RAW_spirou - fp_fp C
files = ['fp_fp02a203.fits', 'fp_fp03a203.fits', 'fp_fp04a203.fits']
cal_extract_RAW_spirou.main(NIGHT_NAME, files, 'C')
plt.close('all')

# test cal_DRIFT_RAW_spirou
files = ['fp_fp02a203.fits', 'fp_fp03a203.fits', 'fp_fp04a203.fits']
cal_DRIFT_RAW_spirou.main(NIGHT_NAME, files)
plt.close('all')
```



## Chapter 6

## Required input header keywords

## 6.1 Required keywords

The following keywords are required by the current recipes to run.

- **Data fits file type (`kw_DPRTYPE`)**

The data fits file type (template Name)

```
kw_DPRTYPE = ["TPL_NAME", "DATA", "template Name"]
```

HEADER file entry:

```
TPL_NAME = "DATA" \ template Name
```

Used in: All Recipes

Defined in: SpirouDRS.spirouConfig.spirouKeywords

- **Acquisition time (human readable) (`kw_ACQTIME_KEY`)**

The acquisition time in format YYYY-mm-dd-HH-MM-SS.ss

```
kw_ACQTIME_KEY = ["ACQTIME1", "YYYY-mm-dd-HH-MM-SS.ss", "Date at start of observation"]
```

HEADER file entry:

```
ACQTIME1 = YYYY-mm-dd-HH-MM-SS.ss \ Date at start of observation
```

Used in: All Recipes

Defined in: SpirouDRS.spirouConfig.spirouKeywords

- **Acquisition time (unix time format) (`kw_ACQTIME_KEY_UNIX`)**

The acquisition time in in unix time format (time since 1970-01-01-00-00-00)

```
kw_ACQTIME_KEY_UNIX = ["ACQTIME", "000000000.00", "Date in unix time at start of observation"]
```

HEADER file entry:

```
ACQTIME = 000000000.00 \ Date in unix time at start of observation
```

Used in: All Recipes

Defined in: SpirouDRS.spirouConfig.spirouKeywords

- **Read noise (`kw_RDNOISE`)**

The read noise (used for sigdet) [e-]

```
kw_RDNOISE = ["RDNOISE", "0.0", "read noise (electrons)"]
```

HEADER file entry:

```
RDNOISE    = 0.0 \ read noise (electrons)
```

Used in: All Recipes

Defined in: SpirouDRS.spirouConfig.spirouKeywords

- **Gain (`kw_GAIN`)**

The gain [e-/ADU]

```
kw_GAIN = ["GAIN", "0.0", "gain (electrons/ADU)"]
```

HEADER file entry:

```
GAIN       = 0.0 \ gain (electrons/ADU)
```

Used in: All Recipes

Defined in: SpirouDRS.spirouConfig.spirouKeywords

- **Exposure time (`kw_EXPTIME`)**

The integration time in seconds

```
kw_EXPTIME = ["EXPTIME", "0.0", "Integration time (seconds)"]
```

HEADER file entry:

```
EXPTIME    = 0.0 \ Integration time (seconds)
```

Used in: All Recipes

Defined in: SpirouDRS.spirouConfig.spirouKeywords

## Chapter 7

# User modifiable variables

To better understand the variables in the DRS we have laid out each variable in the following way:

- **Variable title (`VARIABLE_NAME`)**

Description of the variable

`VARIABLE_NAME` = Default Value

Used in: The recipe used the variable is used in.

Defined in: The place where the variable is defined.

## 7.1 Variable file locations

The variables are currently stored in two places. The first (`../config /config.py`) contains constants that deal with initial set up. These were mentioned in Section 3.5 and are located in `DRS_ROOT /config /../config /config.py`.

The other variables modify how the DRS runs. These are located in `constants_SPIROU_H4RG.py` (located at `DRS_ROOT /config /constants_SPIROU_H4RG.py`).

## 7.2 Global variables

- **DRS Detector Type (`IC_IMAGE_TYPE`)**

Defines the detector. Value must be a valid string. Currently supported values are: “H2RG” or “H4RG”.

`IC_IMAGE_TYPE` = H4RG

Used in: All Recipes

Defined in: `constants_SPIROU_H4RG.py`

- **Plotting switch (`DRS_PLOT`)**

Defines whether to show plots (A value of 1 to show plots, a value of 0 to not show plots). Value must be an integer (0 or 1) or boolean (True or False)

`DRS_PLOT` = 1

Used in: All Recipes

Defined in: `../config /config.py`

- **Interactive switch (`DRS_INTERACTIVE`)**

Defines whether to run in interactive mode. If False or 0 will be set to non-interactive mode (i.e. `DRS_PLOT` will be set to 0). Will stop any user input at the end of recipes if set to 0.

`DRS_INTERACTIVE` = 1

Used in: All Recipes

Defined in: ../config /config.py

- **Debug mode (`DRS_DEBUG`)**

Defines whether we should run the DRS in debug mode. Certain print/log statements and certain graphs only plot in debug mode. On an error the option to enter the python debugger is asked (allows user to look into functions/current memory and see what variables are currently defined. Value must be an integer. Value must be an integer where:

- 0 = No debug
- 1 = basic debugging on errors (prompted to enter python debugger)
- 2 = Same as 1 and recipes specific (plots and some code runs)

`DRS_DEBUG` = 0

Used in: All Recipes

Defined in: ../config /config.py

- **Enable use of custom configuration files (`DRS_DEBUG`)**

Controls whether the DRS searches for custom configuration files (all configuration files). Value can be 1 (True) or 0 (False), True turns on the use of custom configuration files. Constants/variables set in the custom constant files **always** take precedence over the master files. Any constant/variable not set in a custom constant file is taken from the master files. Value must be 1 or True to switch on or 0 or False to switch off.

`DRS_DEBUG` = 0

Used in: All Recipes

Defined in: ../config /config.py

- **Plot interval (`constants_SPIROU.py`)**

Defines the main constants file for the DRS (not the directory just the file name). The directory is controlled internally or if `USER_CONFIG` is set by `DRS_UCONFIG`

`constants_SPIROU.py` = All Recipes

Used in: ../config /config.py

Defined in: All Recipes

- Plot interval (**special\_config\_SPIROU.py**)

Defines the a special constants file for the DRS (not the directory just the file name). The directory is controlled internally or if **USER\_CONFIG** is set by **DRS\_UCONFIG**

**special\_config\_SPIROU.py** = All Recipes

Used in: ../config /config.py

Defined in: All Recipes

This file does not currently exist.

- Plot interval (**ic\_display\_timeout**)

Set the interval between plots in seconds (for certain interactive graphs). Value must be a valid float larger than zero.

**ic\_display\_timeout** = 0.5

Used in: cal\_loc\_RAW\_spirou

Defined in: constants\_SPIROU\_H4RG.py

## 7.3 Directory variables

- The data directory (**TDATA**)

Defines the path to the data directory. Value must be a string containing a valid file location.

**TDATA** = /drs/data/

Used in: All Recipes

Defined in: ../config /config.py

- The installation directory (**DRS\_ROOT**)

Defines the installation directory (**DRS\_ROOT**). Value must be a string containing a valid file location.

**DRS\_ROOT** = /drs/INTROOT/

Used in: All Recipes

Defined in: ../config /config.py

- The raw data directory (**DRS\_DATA\_RAW**)

Defines the directory that the reduced data will be saved to/read from. Value must be a string containing a valid file location.

**DRS\_DATA\_RAW** = /drs/data/raw

Used in: All Recipes

Defined in: ../config /config.py

- The reduced data directory (**DRS\_DATA\_REduc**)

Defines the directory that the reduced data will be saved to/read from. Value must be a string containing a valid file location.

**DRS\_DATA\_REduc** = /drs/data/reduced

Used in: All Recipes

Defined in: ../config /config.py

- The calibration database and calibration file directory (**DRS\_CALIB\_DB**)

Defines the directory that the calibration files and database will be saved to/read from. Value must be a string containing a valid file location.

**DRS\_CALIB\_DB** = /drs/data/calibDB

Used in: All Recipes

Defined in: ../config /config.py

- The log directory (**DRS\_DATA\_MSG**)

Defines the directory that the log messages are stored in. Value must be a string containing a valid file location.

**DRS\_DATA\_MSG** = /drs/data/msg

Used in: All Recipes

Defined in: ../config /config.py

- The working directory (**DRS\_DATA\_WORKING**)

Defines the working directory. Value must be a string containing a valid file location.

**DRS\_DATA\_WORKING** = /drs/data/tmp/

Used in: All Recipes

Defined in: ../config /config.py

- The custom configuration directory (**DRS\_UCONFIG**)

Defines the custom configuration directory. Value must be a string containing a valid file location.

**DRS\_UCONFIG** = ~/spirou\_config/

Used in: All Recipes

Defined in: ../config /config.py

## 7.4 Observatory variables

- CFHT Longitude (**IC\_LONGIT\_OBS**)

Defines the CFHT longitude West (in degrees)

**IC\_LONGIT\_OBS** = 155.468876

Used in: cal\_CCF\_E2DS\_spirou

Defined in: constants\_SPIROU\_H4RG.py

- CFHT Longitude (**IC\_LATIT\_OBS**)

Defines the CFHT latitude North (in degrees)

**IC\_LATIT\_OBS** = 19.825252

Used in: cal\_CCF\_E2DS\_spirou

Defined in: constants\_SPIROU\_H4RG.py

- CFHT Longitude (**IC\_ALTIT\_OBS**)

Defines the CFHT altitude (in km)

**IC\_ALTIT\_OBS** = 4.204

Used in: cal\_CCF\_E2DS\_spirou

Defined in: constants\_SPIROU\_H4RG.py

## 7.5 Image variables

- Resizing blue window (**ic\_ccd{x/y}\_blue\_{low/high}**)

The blue window used in `cal_DARK_spirou`. Each value must be a integer between 0 and the maximum array size in each dimension.

```
ic_ccdx_blue_low    = 2048-200
ic_ccdx_blue_high   = 2048-1500
ic_ccdy_blue_low    = 2048-20
ic_ccdy_blue_high   = 2048-350
```

```
Used in:             cal_DARK_spirou
Defined in:          constants_SPIROU_H4RG.py
```

- Resizing red window (**ic\_ccd{x/y}\_red\_{low/high}**)

The blue window used in `cal_DARK_spirou`. Each value must be a integer between 0 and the maximum array size in each dimension.

```
ic_ccdx_red_low     = 2048-20
ic_ccdx_red_high    = 2048-1750
ic_ccdy_red_low     = 2048-1570
ic_ccdy_red_high    = 2048-1910
```

```
Used in:             cal_DARK_spirou
Defined in:          constants_SPIROU_H4RG.py
```

- Resizing red window (**ic\_ccd{x/y}\_{low/high}**)

The blue window used in `cal_DARK_spirou`. Each value must be a integer between 0 and the maximum array size in each dimension.

```
ic_ccdx_low         = 5
ic_ccdx_high        = 2040
ic_ccdy_low         = 5
ic_ccdy_high        = 1935
```

```
Used in:             cal_loc_RAW_spirou,           cal_SLIT_spirou,
                    cal_FF_RAW_spirou,           cal_extract_RAW_spirou,
                    cal_DRIFT_RAW_spirou
Defined in:          constants_SPIROU_H4RG.py
```



- Available fiber types (**fiber\_types**)

Defines the type of fiber we have (used in various codes). These are define in a python list of string, where the earlier a fiber is in the list the more it takes priority in searches (i.e. AB over A or B if AB is first)

```
fiber_types = ['AB', 'A', 'B', 'C']
```

Used in: `cal_extract_RAW_spirou`, `cal_DRIFT_E2DS_spirou`

Defined in: `constants_SPIROU_H4RG.py`

## 7.6 Fiber variables

These variables are defined for each type of fiber and thus are defined as a python dictionary of values . As such they all must contain the same dictionary keys (currently 'AB', 'A', 'B' and 'C').

- **Number of fibers (nbfib\_fpall)**

This describes the number of fibers of a given type. Must be a python dictionary with identical keys to all other fiber parameters (each value must be an integer).

```
nbfib_fpall = {'AB':2, 'A':1, 'B':1, 'C':1}
```

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Order skip number (ic\_first\_order\_jump\_fpall)**

Describes the number of orders to skip at the start of an image. Must be a python dictionary with identical keys to all other fiber parameters (each value must be an integer).

```
ic_first_order_jump_fpall = {'AB':2, 'A':0, 'B':0, 'C':0}
```

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Maximum order numbers (ic\_locnbmaxo\_fpall)**

Describes the maximum allowed number of orders. Must be a python dictionary with identical keys to all other fiber parameters (each value must be an integer).

```
ic_locnbmaxo_fpall = {'AB':72, 'A':36, 'B':36, 'C':36}
```

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Number of orders to fit (QC) (qc\_loc\_nbo\_fpall)**

Quality control parameter for the number of orders on fiber to fit. Must be a python dictionary with identical keys to all other fiber parameters (each value must be an integer).

```
qc_loc_nbo_fpall = {'AB':72, 'A':36, 'B':36, 'C':36}
```

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Fiber types for this fiber (`fib_type_fpall`)**

The fiber type(s) – as a list – for this fiber. Must be a python dictionary with identical keys to all other fiber parameters (each value must be a list of strings).

```
fib_type_fpall = {'AB':["AB"], 'A':["A"], 'B':["B"], 'C':["C"]}
```

Used in: `cal_FF_RAW_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Half-zone extraction width (left/top) (`ic_ext_range1_fpall`)**

The pixels are extracted from the center of the order out to the edges in the row direction (y-axis), i.e. defines the illuminated part of the order - this number defines the **top** side (if one requires a symmetric extraction around the order fit both range 1 and range 2 – below – should be the same). This can also be used to extract A and B separately (where the fit order is defined at the centre of the AB pair). Must be a python dictionary with identical keys to all other fiber parameters.

```
ic_ext_range1_fpall = {'AB':14.5, 'A':0.0, 'B':14.5, 'C':7.5}
```

Used in: `cal_FF_RAW_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Half-zone extraction width (right/bottom) (`ic_ext_range2_fpall`)**

The pixels are extracted from the center of the order out to the edges in the row direction (y-axis), i.e. defines the illuminated part of the order - this number defines the **bottom** side (if one requires a symmetric extraction around the order fit both range 1 and range 2 – below – should be the same). This can also be used to extract A and B separately (where the fit order is defined at the centre of the AB pair). Must be a python dictionary with identical keys to all other fiber parameters.

```
ic_ext_range2_fpall = {'AB':14.5, 'A':14.5, 'B':0.0, 'C':7.5}
```

Used in: `cal_FF_RAW_spirou`, `cal_extract_RAW_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Half-zone extraction width for full extraction (`ic_ext_range_fpall`)**

The pixels are extracted from the centre of the order out to the edges in the row direction (y-axis), i.e. defines the illuminated part of the order. In `cal_extract_RAW_spirou` both sides of the fit order are extracted at with the same width (symmetric). Must be a python dictionary with identical keys to all other fiber parameters.

```
ic_ext_range_fpall = {'AB':14.5, 'A':14.5, 'B':14.5, 'C':7.5}
```

Used in: `cal_extract_RAW_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Localization fiber for extraction** (**loc\_file\_fpall**)

Defines the localization fiber to use for each fiber type. This is the file in calibDB that is used i.e. the keyword `ic_calibDB_filename` used will be `LOC_{loc_file_fpall}` (e.g. for fiber='AB' use 'LOC\_AB'). Must be a python dictionary with identical keys to all other fiber parameters.

```
loc_file_fpall = {'AB':'AB', 'A':'AB', 'B':'AB', 'C':'C'}
```

Used in: `cal_extract_RAW_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Order profile fiber for extraction** (**orderp\_file\_fpall**)

Defines the order profile fiber to use for each fiber type. This is the file in calibDB that is used i.e. the keyword `ic_calibDB_filename` used will be `ORDER_PROFILE_{orderp_file_fpall}` (e.g. for fiber='AB' use 'ORDER\_PROFILE\_AB'). Must be a python dictionary with identical keys to all other fiber parameters.

```
orderp_file_fpall = {'AB':'AB', 'A':'AB', 'B':'AB', 'C':'C'}
```

Used in: `cal_extract_RAW_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Half-zone extract width** `cal_DRIFT_RAW_spirou` (**ic\_ext\_d\_range\_fpall**)

The size in pixels of the extraction away from the order localization fit (to the top and bottom) - defines the illuminated area of the order for extraction. Must be a python dictionary with identical keys to all other fiber parameters.

```
ic_ext_d_range_fpall = {'AB':14.0, 'A':14.0, 'B':14.0, 'C':7.0}
```

Used in: `cal_DRIFT_RAW_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

## 7.7 Pre-processing variables

- **Force Pre-processing (`IC_FORCE_PREPROCESS`)**

Defines whether the DRS should force pre-processed files only. If True (or 1) only files that are pre-processed will be allowed to be used in the DRS (an error will be generated on un-preprocessed files). If False (or 0) any file will be accepted (but un-preprocessed files will be assumed to be raw and hence rotated, as in pre-processing).

`IC_FORCE_PREPROCESS` = 1

Used in: All Recipes  
Defined in: constants\_SPIROU\_H4RG.py

- **Pre-processing suffix (`PROCESSED_SUFFIX`)**

Defines the suffix to apply to the pre-processed files. If "None" then no suffix is added (or checked for).

`PROCESSED_SUFFIX` = "\_pp.fits"

Used in: All Recipes  
Defined in: constants\_SPIROU\_H4RG.py

- **Number of dark amplifiers (`NUMBER_DARK_AMP`)**

Defines the number of dark amplifiers on the detector

`NUMBER_DARK_AMP` = 5

Used in: cal\_preprocess\_spirou  
Defined in: constants\_SPIROU\_H4RG.py

- **Total number of amplifiers (`TOTAL_AMP_NUM`)**

Defines the total number of amplifiers on the detector

`TOTAL_AMP_NUM` = 32

Used in: cal\_preprocess\_spirou  
Defined in: constants\_SPIROU\_H4RG.py

- **Number of top reference pixels (`NUMBER_REF_TOP`)**

Defines the number of un-illuminated reference pixels at the top of the image.

`NUMBER_REF_TOP` = 4

Used in: cal\_preprocess\_spirou  
Defined in: constants\_SPIROU\_H4RG.py

- Number of bottom reference pixels (**NUMBER\_REF\_BOTTOM**)

Defines the number of un-illuminated reference pixels at the bottom of the image.

**NUMBER\_REF\_BOTTOM** = 4

Used in: `cal_preprocess_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- Number of bins in dark median process (**DARK\_MED\_BINNUM**)

Define the number of bins used in the dark media process.

**DARK\_MED\_BINNUM** = 32

Used in: `cal_preprocess_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- Raw to Pre-processed rotation (**RAW\_TO\_PP\_ROTATION**)

Defines the rotation angle of the raw images compared to that expected by the DRS. Value must be multiple of 90 degrees (in degrees counter-clockwise direction).

**RAW\_TO\_PP\_ROTATION** = -90

Used in: All Recipes

Defined in: `constants_SPIROU_H4RG.py`

## 7.8 Dark calibration variables

- Lower percentile for dead pixel stats (**dark\_qmin**)

This defines the lower percentile to be logged for the fraction of dead pixels statistics. Value must be an integer between 0 and 100 (1 sigma below the mean is  $\sim 16$ ).

**dark\_qmin** = 5

Used in: `cal_DARK_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- Upper percentile for dead pixel stats (**dark\_qmax**)

This defines the upper percentile to be logged for the fraction of dead pixels statistics. Value must be an integer between 0 and 100 (1 sigma above the mean is  $\sim 84$ ).

**dark\_qmax** = 95

Used in: `cal_DARK_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- Dark stat histogram bins (**histo\_bins**)

Defines the number of bins to use in the dark histogram plot. Value must be a positive integer.

**histo\_bins** = 200

Used in: `cal_DARK_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- Lower bound for the Dark stat histogram (**histo\_range\_low**)

Defines the lower bound for the dark statistic histogram. Value must be a float less than (not equal to) the value of 'histo\_range\_high'

**histo\_range\_low** = -0.5

Used in: `cal_DARK_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- Upper bound for the Dark stat histogram (**histo\_range\_high**)

Defines the upper bound for the dark statistic histogram. Value must be a float greater than (not equal to) the value of 'histo\_range\_low'

**histo\_range\_high** = 5

Used in: `cal_DARK_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Bad pixel cut limit (`dark_cutlimit`)**

Defines the bad pixel cut limit in ADU/s.

$$badpixels = (image > dark\_cut\_limit) \text{ OR (non-finite)} \quad (7.1)$$

`dark_cutlimit` = 100.0

Used in: `cal_DARK_spirou`

Defined in: `constants_SPIROU_H4RG.py`



## 7.9 Localization calibration variables

- Order profile smoothed box size (**loc\_box\_size**)

Defines the size of the order profile smoothing box (from the central pixel minus size to the central pixel plus size). Value must be an integer larger than zero.

**loc\_box\_size** = 10

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- Image row offset (**ic\_offset**)

The row number (y axis) of the image to start localization at (below this row orders will not be fit). Value must be an integer equal to or larger than zero.

**ic\_offset** = 40

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- Central column of the image (**ic\_cent\_col**)

The column which is to be used as the central column (x-axis), this is the column that is initially used to find the order locations. Value must be an integer between 0 and the number of columns (x-axis dimension).

**ic\_cent\_col** = 1000

Used in: `cal_loc_RAW_spirou`, `cal_FF_RAW_spirou`,  
`cal_extract_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- Localization window row size (**ic\_ext\_window**)

Defines the size of the localization window in rows (y-axis). Value must be an integer larger than zero and less than the number of rows (y-axis dimension).

**ic\_ext\_window** = 12

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Localization window column step (`ic_locstepc`)**

For the initial localization procedure interval points along the order (x-axis) are defined and the centers are found, this is used as the first estimate of the order shape. This parameter defines that interval step in columns (x-axis). Value must be an integer larger than zero and less than the number of columns (x-axis dimension).

`ic_locstepc` = 12

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Image gap index (`ic_image_gap`)**

Defines the image gap index. The order is skipped if the top of the row (row number - `ic_ext_window`) or bottom of the row (row number + `ic_ext_window`) is inside this image gap index. i.e. a order is skipped if:

$$(\text{top of the row} < \text{ic\_image\_gap}) \text{ OR } (\text{bottom of the row} > \text{ic\_image\_gap}) \quad (7.2)$$

Value must be an integer between zero and the number of rows (y-axis dimension).

`ic_image_gap` = 0

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Minimum order row size (`ic_widthmin`)**

Defines the minimum row width (width in y-axis) to accept an order as valid. If below this threshold order is not recorded. Value must be an integer between zero and the number of rows (y-axis dimension).

`ic_widthmin` = 5

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Center noise multiplier threshold (`ic_noise_mult_thres`)**

Defines the noise multiplier threshold in order to accept an order center as usable such that:

$$\max(\text{value}) - \min(\text{value}) > \text{ic\_noise\_mult\_thres} * \text{sigdet} \quad (7.3)$$

where the value is row center pixel value and sigdet is the image's read out noise. Values must be a float.

`ic_noise_mult_thres` = 100

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Polynomial fit coefficients for bad region interp. (`bad_region_fit`)**

Defines the polynomial fit parameters for interpolating over the bad regions (holes) before the localization is done. Must be a python list of floats. The coefficient list should be in the following order:

$$p[0] * x^{(N-1)} + p[1] * x^{(N-2)} + \dots + p[N-2] * x + p[N-1] \quad (7.4)$$

`bad_region_fit` = [3.19884964e-05, -1.08289228e-01, 2.16643659e+03]

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Median filter box size 1 for bad region interp. (`bad_region_med_size`)**

Defines the median filter box size used in interpolating over the bad regions (holes) before the localization is done. Value must be a positive integer.

`bad_region_med_size` = 101

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Threshold for bad pixels for bad region interp. (`bad_region_threshold`)**

Defines the threshold below which the image (normalised between 0 and 1) should be regarded as bad. Used in interpolating over the bad regions (holes) before localization is done. Value must be a float between 0 and 1.

`bad_region_threshold` = 0.2

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Box size (kernel) for convolve in bad region interp. (`bad_region_kernel_size`)**

Defines the box size (kernel) for the convolution. Used in interpolating over the bad regions (holes) before localization is done. Value must be a positive integer.

`bad_region_kernel_size` = 51

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Median filter box size 2 for bad region interp. (`bad_region_med_size2`)**

Defines the median filter box size used (during the convolution) in interpolating over the bad regions (holes) before the localization is done. Value must be a positive integer.

`bad_region_med_size2` = 11

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Threshold for good ratio for bad region interp. (`bad_region_good_value`)**

Defines the threshold (of the ratio between original image and the interpolated image) where pixels are deemed "good". For use in interpolating over the bad regions (holes) before the localization is done.

`bad_region_good_value` = 0.5

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Threshold for bad ratio for bad region interp. (`bad_region_bad_value`)**

Defines the threshold (of the ratio between original image and the interpolated image) where pixels are deemed "bad". For use in interpolating over the bad regions (holes) before the localization is done.

`bad_region_bad_value` = 0.25

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Min/Max smoothing box size (`ic_locnbpix`)**

Defines the half-size of the rows to use when smoothing the image to work out the minimum and maximum pixel values. This defines the half-spacing between orders and is used to estimate background and the maximum signal. Value must be greater than zero and less than the number of rows (y-axis dimension).

`ic_locnbpix` = 45

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Minimum signal amplitude (`ic_min_amplitude`)**

Defines a cut off (in e-) where below this point the central pixel values will be set to zero. Value must be a float greater than zero.

`ic_min_amplitude` = 100.0

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Normalized background amplitude threshold (`ic_locseuil`)**

Defines the normalized amplitude threshold to accept pixels for background calculation (pixels below this normalized value will be used for the background calculation). Value must be a float between zero and one.

`ic_locseuil` = 0.2

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Saturation threshold on the order profile plot (`ic_satseuil`)**

Defines the saturation threshold on the order profile plot, pixels above this value will be set this value (`ic_satseuil`). Value must be a float greater than zero.

`ic_satseuil` = 64536

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Degree of the fitting polynomial for localization position (`ic_locdfitc`)**

Defines the degree of the fitting polynomial for locating the positions of each order i.e. if value is 1 is a linear fit, if the value is 2 is a quadratic fit. The value must be a positive integer equal to or greater than zero (zero would lead to a constant fit along the column direction (x-axis direction)).

`ic_locdfitc` = 5

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- Degree of the fitting polynomial for localization width (**ic\_locdfitw**)

Defines the degree of the fitting polynomial for measuring the width of each order i.e. if value is 1 is a linear fit, if the value is 2 is a quadratic fit. The value must be a positive integer equal to or greater than zero (zero would lead to a constant fit along the row direction (y-axis direction)).

**ic\_locdfitw** = 5

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- Degree of the fitting polynomial for localization position error (**ic\_locdfitp**)

Defines the degree of the fitting polynomial for locating the positions error of each order i.e. if value is 1 is a linear fit, if the value is 2 is a quadratic fit. The value must be a positive integer equal to or greater than zero (zero would lead to a constant fit along the column direction (x-axis direction)).

**ic\_locdfitp** = 3

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- Maximum RMS for sigma-clipping order fit (positions) (**ic\_max\_rms\_center**)

Defines the maximum RMS allowed for an order, if RMS is above this value the position with the highest residual is removed and the fit is recalculated without that position (sigma-clipped). Value must be a positive float. i.e. position fit is recalculated if:

$$\max(RMS) > \text{ic\_max\_rms\_center} \quad (7.5)$$

**ic\_max\_rms\_center** = 0.2

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Maximum peak-to-peak for sigma-clipping order fit (positions) (`ic_max_ptp_center`)**

Defines the maximum peak-to-peak value allowed for an order, if the peak to peak is above this value the position with the highest residual is removed and the fit is recalculated without that position (sigma-clipped). Value must be a positive float. i.e. position fit is recalculated if:

$$\max(|\text{residuals}|) > \text{ic\_max\_ptp\_center} \quad (7.6)$$

`ic_max_ptp_center` = 0.2

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Maximum peak-to-peak-RMS ratio for sigma-clipping order fit(positions) (`ic_ptporms_center`)**

Defines the maximum ratio of peak-to-peak residuals and RMS value allowed for an order, if the ratio is above this value the position with the highest residual is removed and the fit is recalculated without that position (sigma-clipped). Value must be a positive float. i.e. position

fit is recalculated if:

$$\max(|\text{residuals}|)/\text{RMS} > \text{ic\_ptporms\_center} \quad (7.7)$$

`ic_ptporms_center` = 8.0

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Maximum RMS for sigma-clipping order fit (width) (`ic_max_rms_fwhm`)**

Defines the maximum RMS allowed for an order, if RMS is above this value the width with the highest residual is removed and the fit is recalculated without that width (sigma-clipped). Value must be a positive float. i.e. width fit is recalculated if:

$$\max(RMS) > \text{ic\_max\_rms\_width} \quad (7.8)$$

`ic_max_rms_fwhm` = 1.0

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Maximum peak-to-peak for sigma-clipping order fit (widths) (`ic_max_ptp_fracfwhm`)**

Defines the maximum peak-to-peak value allowed for an order, if the peak to peak is above this value the width with the highest residual is removed and the fit is recalculated without that width (sigma-clipped). Value must be a positive float. i.e. width fit is recalculated if:

$$\max(|\text{residuals}/\text{data}|) \times 100 > \text{ic\_max\_ptp\_fracfwhm} \quad (7.9)$$

`ic_max_ptp_fracfwhm` = 1.0

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Delta width 3 convolve shape model (`ic_loc_delta_width`)**

Defines the delta width in pixels for the 3 convolve shape model - currently not used. Value must be a positive float.

`ic_loc_delta_width` = 1.85

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Localization archiving option (`ic_locopt1`)**

Whether we save the location image with the superposition of the fit (zeros). If this option is 1 or True it will save the file to ‘\_with-order\_`fiber`.fits’ if 0 or False it will not save this file. Value must be 1, 0, True or False.

`ic_locopt1` = 1

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`



## 7.10 Slit calibration variables

- **Tilt oversampling factor (`ic_tilt_coi`)**

Defines the oversampling factor used to work out the tilt of the slit. Value must be an integer value larger than zero.

`ic_tilt_coi` = 10

Used in: `cal_SLIT_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Slit fit order plot offset factor (`ic_facdec`)**

Defines an offset of the position fit to show the edges of the illuminated area. (Final offset is  $\pm \times 2$  of this offset away from the order fit. Value must be a positive float.)

`ic_facdec` = 1.6

Used in: `cal_SLIT_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Degree of the fitting polynomial for the tilt (`ic_tilt_fit`)**

Defines the degree of the fitting polynomial for determining the tilt i.e. i.e. if value is 1 is a linear fit, if the value is 2 is a quadratic fit. The value must be a positive integer equal to or greater than zero (zero would lead to a constant fit).

`ic_tilt_fit` = 4

Used in: `cal_SLIT_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Selected order in Slit fit order plot (`ic_slit_order_plot`)**

Defines the selected order to plot the fit for in the Slit fir order plot. Value must be between zero and the maximum number of orders.

`ic_slit_order_plot` = 10

Used in: `cal_SLIT_spirou`

Defined in: `constants_SPIROU_H4RG.py`

## 7.11 Flat fielding calibration variables

- Measure background (**ic\_do\_bkgr\_subtraction**)

Define whether to measure the background and do a background subtraction. Value must be True or 1 to do the background measurement and subtraction or be False or 0 to not do the background measurement and subtraction.

**ic\_do\_bkgr\_subtraction** = 0

Used in: `cal_FF_RAW_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- Half-size of background window (**ic\_bkgr\_window**)

Defines the half-size (in pixels) of the background window to create a sub-frame to find the minimum  $2 \times \text{ic\_bkgr\_window}$  pixels for which to calculate the background from. Size is used in both row and column (y and x) direction. Value must be an integer between zero and the minimum(row number, column number) (minimum(x-axis dimension, y-axis dimension)).

**ic\_bkgr\_window** = 100

Used in: `cal_FF_RAW_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- Number of orders in tilt measurement (**ic\_tilt\_nbo**)

Defines the number of orders in the tilt measurement file (TILT key in the `ic_calibDB_filename`). This is the number of tilts that will be extracted. Value must be an integer larger than zero and smaller than or equal to the total number of orders present in the TILT file.

**ic\_tilt\_nbo** = 36

Used in: `cal_FF_RAW_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- Flat extraction start order (**ff\_start\_order**)

Start order of the extract for the flat finding recipe. If value is "None" uses start order = 0, else must be a positive order number less than the total number of orders.

**ff\_start\_order** = None

Used in: `cal_FF_RAW_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- Flat extraction end order (**ff\_end\_order**)

End order of the extract for the flat finding recipe. If value is "None" uses last order, else must be a positive order number less than the total number of orders.

**ff\_end\_order** = None

Used in: `cal_FF_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- The manually set sigdet for flat fielding. (**ic\_ff\_sigdet**)

This defines the sigdet to use in the weighted tilt extraction. Set to -1 to use from the input file ('fitsfilename') HEADER. Value must be either -1 or a positive float.

**ic\_ff\_sigdet** = 100.0

Used in: `cal_FF_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- Half size blaze window (**ic\_extfblaz**)

Defines the distance from the central column that should be used to measure the blaze for each order. Value must be an integer greater than zero and less than half the number of columns (x-axis dimension).

**ic\_extfblaz** = 50

Used in: `cal_FF_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- Fit degree for the blaze polynomial fit (**ic\_blaze\_fitn**)

Defines the degree of the fitting polynomial for fitting the blaze function of each order i.e. if value is 1 is a linear fit, if the value is 2 is a quadratic fit. The value must be a positive integer equal to or greater than zero (zero would lead to a constant fit along the column direction (x-axis direction)).

**ic\_blaze\_fitn** = 5

Used in: `cal_FF_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Selected order for flat fielding plot (`ic_ff_order_plot`)**

Defines the selected order to plot on the flat fielding image plot. Value must be a integer between zero and the number of orders.

`ic_ff_order_plot` = 5

Used in: `cal_FF_RAW_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Plot all order fits for flat fielding plot (`ic_ff_plot_all_orders`)**

If True or 1, instead of plotting the selected order from `ic_ff_order_plot` will plot the order fits (and edges) for all orders. This is slower than just plotting one. Value must be True or 1 or False or 0.

`ic_ff_plot_all_orders` = 0

Used in: `cal_FF_RAW_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Flat-field plot skip orders (`FF_RMS_PLOT_SKIP_ORDERS`)**

Define the orders not to plot on the RMS flat-field plot. Should be a valid python list of integers (with each value being an integer between 0 and the maximum number of orders)

`FF_RMS_PLOT_SKIP_ORDERS` = [22, 23, 24, 25, 48]

Used in: `cal_FF_RAW_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Flat-field extraction type (`IC_FF_EXTRACT_TYPE`)**

Defines the extraction type for the flat-fielding. Must be one of the following:

- "0" - Simple extraction (function = `SpirouDRS.spirouEXTOR.spirouEXTOR.extract_const_range`)
- "1" - Wiegthed extraction (function = `SpirouDRS.spirouEXTOR.spirouEXTOR.extract_weight`)
- "2" - tilt extraction (function = `SpirouDRS.spirouEXTOR.spirouEXTOR.extract_tilt`)
- "3a" - tilt weight extraction - old (function = `SpirouDRS.spirouEXTOR.spirouEXTOR.extract_tilt_weight`)
- "3b" - tilt weight extraction 2 - old (function = `SpirouDRS.spirouEXTOR.spirouEXTOR.extract_tilt_weight_old2`)
- "3c" - tilt weight extraction 2 (function = `SpirouDRS.spirouEXTOR.spirouEXTOR.extract_tilt_weight2`)
- "3d" - tilt weight extraction 2 - with cosmic correction (function = `SpirouDRS.spirouEXTOR.spirouEXTOR.extract_tilt_weight2cosm`)

`IC_FF_EXTRACT_TYPE` = "3c"

Used in: `cal_FF_RAW_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

## 7.12 Extraction calibration variables

- **Extraction option - rough extraction (`ic_extopt`)**

Extraction option for rough extraction:

- if 0 extraction by summation over a constant range
- if 1 extraction by summation over constants sigma (not currently available)
- if 2 Horne extraction without cosmic elimination (not currently available)
- if 3 Horne extraction with cosmic elimination (not currently available)

Used for estimating the slit tilt and in calculating the blaze/flat fielding. Value must be a integer between 0 and 3.

`ic_extopt` = 0

Used in: `cal_SLIT_spirou`, `cal_FF_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Extraction start order (`ff_start_order`)**

Start order of the extract for the extraction. If value is "None" uses start order = 0, else must be a positive order number less than the total number of orders.

`ff_start_order` = None

Used in: `cal_extract_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Extraction end order (`ff_end_order`)**

End order of the extract for the extraction. If value is "None" uses last order, else must be a positive order number less than the total number of orders.

`ff_end_order` = None

Used in: `cal_extract_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Extraction distance - rough extraction (`ic_extnbsig`)**

The pixels are extracted from the centre of the order out to the edges in the row direction (y-axis), i.e. defines the illuminated part of the order). Used for estimating the slit tilt and in calculating the blaze/flat fielding. Value must be a positive float between 0 and the total number of rows (y-axis dimension).

`ic_extnbsig` = 2.5

Used in: `cal_SLIT_spirou`, `cal_FF_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Extraction type (`ic_extract_type`)**

Defines the extraction type for the `cal_extract_RAW_spirou`. Must be one of the following:

- "0" - Simple extraction (function = `SpirouDRS.spirouEXTOR.spirouEXTOR.extract_const_range`)
- "1" - Wiegthed extraction (function = `SpirouDRS.spirouEXTOR.spirouEXTOR.extract_weight`)
- "2" - tilt extraction (function = `SpirouDRS.spirouEXTOR.spirouEXTOR.extract_tilt`)
- "3a" - tilt weight extraction - old (function = `SpirouDRS.spirouEXTOR.spirouEXTOR.extract_tilt_weight`)
- "3b" - tilt weight extraction 2 - old (function = `SpirouDRS.spirouEXTOR.spirouEXTOR.extract_tilt_weight_old2`)
- "3c" - tilt weight extraction 2 (function = `SpirouDRS.spirouEXTOR.spirouEXTOR.extract_tilt_weight2`)
- "3d" - tilt weight extraction 2 - with cosmic correction (function = `SpirouDRS.spirouEXTOR.spirouEXTOR.extract_tilt_weight2cosm`)

`ic_extract_type` = "3d"

Used in: `cal_extract_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Tilt border (`ic_ext_tilt_bord`)**

Set the number of pixels to set as the border (needed to allow for tilt to not go off edge of image). Value must be a positive integer, smaller than half the number of x pixels.

`ic_ext_tilt_bord` = 2

Used in: `cal_extract_RAW_spirou`, `cal_FF_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Manually set the extraction sigdet (`ic_ext_sigdet`)**

Set the sigdet used in the extraction process instead of using the sigdet in the FITS rec HEADER file. If the value is set to -1 the sigdet from the HEADER is used instead.

```
ic_ext_sigdet = 100
```

Used in: `cal_extract_RAW_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Selected order in extract fit order plot (`ic_ext_order_plot`)**

Defines the selected order to plot the fit for in the extract fit order plot. Value must be between zero and the maximum number of orders.

```
ic_ext_order_plot = 20
```

Used in: `cal_extract_RAW_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Cosmic Sig Cut (`IC_COSMIC_SIGCUT`)**

Defines the percentage of (normalized) flux above which we detect as cosmsics.

```
IC_COSMIC_SIGCUT = 0.25
```

Used in: `cal_FF_RAW_spirou`, `cal_extract_RAW_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Max Cosmic Threshold (`IC_COSMIC_THRES`)**

Defines the maximum number of iterations to check for cosmsics (for each pixel).

```
IC_COSMIC_THRES = 5
```

Used in: `cal_FF_RAW_spirou`, `cal_extract_RAW_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`



## 7.13 Drift calibration variables

- Noise value for SNR drift calculation (**ic\_drift\_noise**)

Define the noise value for the signal to noise ratio in the drift calculation.

$$snr = flux / \sqrt{(flux + noise^2)} \quad (7.10)$$

Value must be a float larger than zero.

**ic\_drift\_noise** = 100.0

Used in: `cal_DRIFT_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- Do background correction (**IC\_DRIFT\_BACK\_CORR**)

Defines whether the background correction is done.

**IC\_DRIFT\_BACK\_CORR** = 1

Used in: `cal_DRIFT_E2DS_spirou`, `cal_DRIFTPEAK_E2DS_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- The maximum flux for a good (unsaturated) pixel (**ic\_drift\_maxflux**)

Defines the maximum flux to define a good pixel. This pixels and those that surround it will not be used in determining the RV parameters. Value must be a float greater than zero.

**ic\_drift\_maxflux** = 1.e9

Used in: `cal_DRIFT_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- Saturated pixel flag size (**ic\_drift\_boxsize**)

Defines the number of pixels around a saturated pixel to flag as unusable (and hence not used in determining the RV parameters). Value must be an integer larger than zero.

**ic\_drift\_boxsize** = 12

Used in: `cal_DRIFT_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- Large number of files for skip (**drift\_nlarge**)

Defines the number of files that is large enough to require the 'drift\_file\_skip' parameter (only uses one file in every 'drift\_file\_skip' files). This is done to speed up the code and avoid a bug. Value must be an integer larger than zero.

**drift\_nlarge** = 300

Used in: `cal_DRIFT_RAW_spirou`, `cal_DRIFT_E2DS_spirou`,  
`cal_DRIFTPEAK_E2DS_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- Large number of files skip parameter (**cal\_DRIFT\_RAW\_spirou**) (**drift\_file\_skip**)

Defines how many files we skip. This is done by selecting one file every 'drift\_file\_skip' files. i.e. if skip is 3 the code uses every 3rd file to calculate the drift. Value must be an integer larger than zero. A value of 1 is equivalent to no skipping of files regardless of the file number.

**drift\_file\_skip** = 3

Used in: `cal_DRIFT_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- Large number of files skip parameter (**cal\_DRIFT\_E2DS\_spirou**) (**drift\_e2ds\_file\_skip**)

Defines how many files we skip. This is done by selecting one file every 'drift\_file\_skip' files. i.e. if skip is 3 the code uses every 3rd file to calculate the drift. Value must be an integer larger than zero. A value of 1 is equivalent to no skipping of files regardless of the file number.

**drift\_e2ds\_file\_skip** = 1

Used in: `cal_DRIFT_E2DS_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- Number of sigmas to cut in cosmic re-normalization (**cal\_DRIFT\_RAW\_spirou**) (**ic\_drift\_cut\_raw**)

Defines the number of standard deviations to remove fluxes at (and replace with the reference flux) for `cal_DRIFT_RAW_spirou`. Value must be a float larger than zero.

**ic\_drift\_cut\_raw** = 3

Used in: `cal_DRIFT_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- Number of sigmas to cut in cosmic re-normalization (`cal_DRIFT_E2DS_spirou`) (`ic_drift_cut_e2ds`)

Defines the number of standard deviations to remove fluxes at (and replace with the reference flux) for `cal_DRIFT_E2DS_spirou`. Value must be a float larger than zero.

`ic_drift_cut_e2ds` = 4.5

Used in: `cal_DRIFT_E2DS_spirou`  
Defined in: `constants_SPIROU_H4RG.py`

- Number of orders to use in drift (`ic_drift_n_order_max`)

Defines the number of orders to use (starting from zero to maximum number). This is used to get the median drift. Value must be an integer between 0 and the maximum number of orders.

`ic_drift_n_order_max` = 28

Used in: `cal_DRIFT_RAW_spirou`  
Defined in: `constants_SPIROU_H4RG.py`

- Define the way to combine orders for drift (for `cal_DRIFT_RAW_spirou`) (`drift_type_raw`)

Defines the way to calculate the combine order drifts (to one drift per image) should either be 'weighted mean' (Equation 7.11) or 'median' (Equation 7.12) for `cal_DRIFT_RAW_spirou`.

$$\text{drift} = \frac{\sum (\text{drift}_i * w_i)}{\sum w_i} \quad (7.11)$$

where  $w_i$  is  $1/\Delta v_{rms}$

$$\text{drift} = \text{median}(\text{drift}_i) \quad (7.12)$$

Value should be a valid python string either 'median' or 'weighted mean'.

`drift_type_raw` = median

Used in: `cal_DRIFT_RAW_spirou`  
Defined in: `constants_SPIROU_H4RG.py`

- Define the way to combine orders for drift `cal_DRIFT_E2DS_spirou` (`drift_type_e2ds`)

Defines the way to calculate the combine order drifts (to one drift per image) should either be 'weighted mean' (Equation 7.13) or 'median' (Equation 7.14) for `cal_DRIFT_E2DS_spirou`.

$$\text{drift} = \frac{\sum (\text{drift}_i * w_i)}{\sum w_i} \quad (7.13)$$

where  $w_i$  is  $1/\Delta v_{rms}$

$$\text{drift} = \text{median}(\text{drift}_i) \quad (7.14)$$

Value should be a valid python string either 'median' or 'weighted mean'.

`drift_type_e2ds` = weighted mean

Used in: `cal_DRIFT_E2DS_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- Selected order in drift fit order plot (`ic_drift_order_plot`)

Defines the selected order to plot the fit for in the drift fit order plot. Value must be between zero and the maximum number of orders.

`ic_drift_order_plot` = 20

Used in: `cal_DRIFT_RAW_spirou`, `cal_DRIFT_E2DS_spirou`

Defined in: `constants_SPIROU_H4RG.py`

## 7.14 Drift-Peak calibration variables

- First order to use in drift-peak (**ic\_drift\_peak\_n\_order\_min**)

Defines the first order to use (from this to **ic\_drift\_peak\_n\_order\_max**). This is used to get the median drift. Value must be an integer greater than or equal to 0 and less than **ic\_drift\_peak\_n\_order\_max**.

**ic\_drift\_peak\_n\_order\_min** = 2

Used in: **cal\_DRIFTPEAK\_E2DS\_spirou**  
Defined in: **constants\_SPIROU\_H4RG.py**

- Last order to use in drift-peak (**ic\_drift\_peak\_n\_order\_max**)

Defines the last order to use (from **ic\_drift\_peak\_n\_order\_min** to this). This is used to get the median drift. Value must be an integer greater than **ic\_drift\_peak\_n\_order\_min** and less than or equal to the maximum number of orders.

**ic\_drift\_peak\_n\_order\_max** = 30

Used in: **cal\_DRIFTPEAK\_E2DS\_spirou**  
Defined in: **constants\_SPIROU\_H4RG.py**

- Large number of files skip parameter (**cal\_DRIFT\_E2DS\_spirou**) (**drift\_e2ds\_file\_skip**)

Defines how many files we skip. This is done by selecting one file every 'drift\_file\_skip' files. i.e. if skip is 3 the code uses every 3rd file to calculate the drift. Value must be an integer larger than zero. A value of 1 is equivalent to no skipping of files regardless of the file number.

**drift\_e2ds\_file\_skip** = 1

Used in: **cal\_DRIFTPEAK\_E2DS\_spirou**  
Defined in: **constants\_SPIROU\_H4RG.py**

- Minimum box size for min max smoothing (**drift\_peak\_minmax\_boxsize**)

Defines the minimum size of the box used to get the minimum and maximum pixel values (specifically minimum pixel values). Each box (defined as the pixel position  $\pm$  box size) is used to work out the background value for that pixel. Value must be an integer larger than zero and less than half the number of columns (x-dimension).

**drift\_peak\_minmax\_boxsize** = 6

Used in: **cal\_DRIFTPEAK\_E2DS\_spirou**  
Defined in: **constants\_SPIROU\_H4RG.py**

- **Image column (x-dim) border size (`drift_peak_border_size`)**

Defines the number of pixels on either side of an image that should not be used to find FP peaks. This size must be larger to or equal to `drift_peak_fpbox_size`, therefore the fit to an individual FP does not go off the edge of the image. Value must be an integer larger to or equal to `drift_peak_fpbox_size` and less than and less than half the number of columns (x-dimension).

`drift_peak_border_size` = 3

Used in: `cal_DRIFTPEAK_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Box size for fitting individual FP peak. (`drift_peak_fpbox_size`)**

Defines the half-box size (i.e. central position  $\pm$  box size) of the box used to fit an individual FP peak. This size must be large enough to fit a peak but not too large as to encompass multiple FP peaks. The value must be an integer larger than zero and smaller than or equal to `drift_peak_border_size` (to avoid fitting off the edges of the image).

`drift_peak_fpbox_size` = 3

Used in: `cal_DRIFTPEAK_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Minimum sigma above median for valid peak (`drift_peak_peak_sig_lim`)**

Defines the flux a valid peak must have in order to be recognized as a valid peak (before the peak fitting is done). If a peaks maximum is below this threshold it will not be used as a valid peak in finding the drifts. Value is a dictionary containing keys equivalent to the lamp types (currently this is 'fp' and 'hc'). The values of each must be a float greater than 1 for above the median and, between zero and 1 for below the median).

`drift_peak_peak_sig_lim` = `fp':1.0, 'hc':7.0'fp':1.0, 'hc':7.0`

Used in: `cal_DRIFTPEAK_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Minimum spacing between valid peaks (`drift_peak_inter_peak_spacing`)**

Defines the minimum spacing peaks must have (between neighbouring peaks) in order to recognized as valid peaks (before the peak fitting is done). If peak is closer than this separation to a previous peak the peak will not be used as a valid peak in finding the drifts. Value must be an integer greater than zero.

`drift_peak_inter_peak_spacing` = 5

Used in: `cal_DRIFTPEAK_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- Expected width of FP peaks (**drift\_peak\_exp\_width**)

Defines the expected width of the FP peaks. Parameter is used to ‘normalise’ the peaks which are then subsequently removed if:

$$\text{normalized FP FWHM} > \text{drift\_peak\_norm\_width\_cut} \quad (7.15)$$

this is equivalent to:

$$\text{FP FWHM} > (\text{drift\_peak\_exp\_width} + \text{drift\_peak\_norm\_width\_cut}) \quad (7.16)$$

Value must be a float larger than zero and less than the number of columns (x-dimension).

$$\text{drift\_peak\_exp\_width} = 0.8$$

Used in: `cal_DRIFTPEAK_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- Normalized FP width threshold (**drift\_peak\_norm\_width\_cut**)

Defines the maximum ‘normalized’ width of FP peaks that is acceptable for a valid FP peak. i.e. widths above this threshold are rejected as valid FP peaks. This works as follows:

$$\text{normalized FP FWHM} > \text{drift\_peak\_norm\_width\_cut} \quad (7.17)$$

this is equivalent to:

$$\text{FP FWHM} > (\text{drift\_peak\_exp\_width} + \text{drift\_peak\_norm\_width\_cut}) \quad (7.18)$$

Value must be a float larger than zero and less than the number of columns (x-dimension) but if `drift_peak_exp_width` is defined sensibly then this number should be small.

$$\text{drift\_peak\_norm\_width\_cut} = 0.2$$

Used in: `cal_DRIFTPEAK_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- Get drift via a Gaussian fitting process (**drift\_peak\_getdrift\_gaussfit**)

Defines whether the drift is calculated via a Gaussian fitting process (fitting the targeted order with a Gaussian) –  $\sim \times 10$  slower, or adjusts a barycentre to get the drift. Value must be True or 1 to do the Gaussian fit, or False or 0 to use the barycentre adjustment.

$$\text{drift\_peak\_getdrift\_gaussfit} = \text{False}$$

Used in: `cal_DRIFTPEAK_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Pearson R coefficient (between reference and image) (`drift_peak_pearsonr_cut`)**

Defines the threshold below which a image is deemed to dissimilar from the reference image to be used. A Pearson R test is performed between the reference image (E2DS file) and the current iteration image (E2DS file), the minimum of all usable orders is then tested. If any order does not pass the criteria:

$$\text{coefficient}_{\text{order}} > \text{drift\_peak\_pearsonr\_cut} \quad (7.19)$$

then the whole image (E2DS file) is rejected. Value must be a float larger than zero and less than 1.0, values should be close to unity for a good fit i.e. 0.97.

`drift_peak_pearsonr_cut` = 0.9

Used in: `cal_DRIFTPEAK_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Sigma clip for found FP peaks (`drift_peak_sigmaclip`)**

Defines the number of sigmas above the median that is used to remove bad FP peaks from the drift calculation process. Value must be a float larger than zero.

`drift_peak_sigmaclip` = 1.0

Used in: `cal_DRIFTPEAK_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Plot linelist vs log Amplitude (`drift_peak_plot_line_log_amp`)**

Defines whether we plot the line list against log amplitude. Value must be 1 or True to plot, or 0 or False to not plot

`drift_peak_plot_line_log_amp` = False

Used in: `cal_DRIFTPEAK_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Selected order for line-list vs log Amplitude plot (`drift_peak_selected_order`)**

Defines the selected order to plot the wave vs extracted spectrum for over-plotting on the line list against log amplitude plot. Value must be an integer between 0 and the number of orders

`drift_peak_selected_order` = 30

Used in: `cal_DRIFTPEAK_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`



## 7.15 Bad pixel calibration variables

- Bad pixel median image box width (**badpix\_flat\_med\_wid**)

A similar flat is produced by taking the running median of the flat in the column direction (x-dimension) over a boxcar width of **badpix\_flat\_med\_wid**. This assumes that the flux level varies only by a small amount over **badpix\_flat\_med\_wid** pixels and that the bad pixels are isolated enough that the median along that box will be representative of the flux they should have if they were not bad. Value should be an integer larger than zero and less than the number of columns (x-axis dimension).

**badpix\_flat\_med\_wid** = 7

Used in: `cal_BADPIX_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- Bad pixel illumination cut parameter (**badpix\_illum\_cut**)

Threshold below which a pixel is considered unilluminated. As we cut the pixels that fractionally deviate by more than a certain amount (**badpix\_flat\_cut\_ratio**) this would lead to lots of bad pixels in unilluminated regions of the array. This parameter stops this, as the pixels are normalised this value must be a float greater than zero and less than 1.

**badpix\_illum\_cut** = 0.05

Used in: `cal_BADPIX_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- Bad pixel maximum differential pixel cut ratio (**badpix\_flat\_cut\_ratio**)

This sets the maximum differential pixel response relative to the expected value. Value must be a float larger than zero.

**badpix\_flat\_cut\_ratio** = 0.5

Used in: `cal_BADPIX_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- Bad pixel maximum flux to considered too hot (**badpix\_max\_hotpix**)

Defines the maximum flux value to be considered too hot to user.

**badpix\_max\_hotpix** = 100.0

Used in: `cal_BADPIX_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Bad pixel normalisation percentile (`badpix_norm_percentile`)**

Defines the percentile at which the bad pixels are normalised to in order to locate bad and dead pixels.

`badpix_norm_percentile` = 90.0

Used in: `cal_BADPIX_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Full detector flat file (`badpix_full_flat`)**

Defines the full detector flat file (located in the data folder)

`badpix_full_flat` = 'detector\_flat\_full.fits'

Used in: `cal_BADPIX_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Full detector good threshold (`badpix_full_threshold`)**

Defines the threshold on the full detector flat file to deem pixels as good

`badpix_full_threshold` = 0.3

Used in: `cal_BADPIX_spirou`

Defined in: `constants_SPIROU_H4RG.py`

## 7.16 Wavelength solution variables

- **Lamp types (IC\_LAMPS)**

Define the lamp types. These must be present in `IC_LL_LINE_FILE_ALL` and `IC_CAT_TYPE_ALL` to be used. Each dictionary entry must be a list of strings (to look for in the header).

```
IC_LAMPS = dict(UNe=['hcne', 'hc1'], TH=['hctwo', 'hc2'])
```

Used in: `cal_HC_E2DS_spirou`, `cal_WAVE_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Catalogue line list files (IC\_LL\_LINE\_FILE\_ALL)**

Define the lamp types. These must be present in `IC_LAMPS` and `IC_CAT_TYPE_ALL` to be used.

```
IC_LL_LINE_FILE_ALL = dict(UNe='catalogue_UNe.dat', TH='catalogue_ThAr.dat')
```

Used in: `cal_HC_E2DS_spirou`, `cal_WAVE_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Type of line list catalogue (IC\_CAT\_TYPE\_ALL)**

Define the lamp types. These must be present in `IC_LAMPS` and `IC_LL_LINE_FILE_ALL` to be used.

```
IC_CAT_TYPE_ALL = dict(UNe='fullcat', TH='thcat')
```

Used in: `cal_HC_E2DS_spirou`, `cal_WAVE_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Resolution of the detector (IC\_RESOL)**

Define the resolution of the detector

```
IC_RESOL = 65000
```

Used in: `cal_HC_E2DS_spirou`, `cal_WAVE_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Wavelength free-span (IC\_LL\_FREE\_SPAN)**

Define the wavelength free span parameter in find lines. Must be a list of line widths (in pixels). Ordered from largest to smallest.

```
IC_LL_FREE_SPAN = [6.0, 3.5]
```

Used in: `cal_HC_E2DS_spirou`, `cal_WAVE_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Minimum wavelength - find lines (IC\_LL\_SP\_MIN)**

Define the minimum wavelength of the detector to use in find lines (in nm).

**IC\_LL\_SP\_MIN** = 900

Used in: cal\_HC\_E2DS\_spirou, cal\_WAVE\_E2DS\_spirou  
 Defined in: constants\_SPIROU\_H4RG.py

- **Maximum wavelength - find lines (IC\_LL\_SP\_MAX)**

Define the maximum wavelength of the detector to use in find lines (in nm).

**IC\_LL\_SP\_MAX** = 2400

Used in: cal\_HC\_E2DS\_spirou, cal\_WAVE\_E2DS\_spirou  
 Defined in: constants\_SPIROU\_H4RG.py

- **Readout noise - find lines (IC\_HC\_NOISE)**

Define the read out noise to use in find lines

**IC\_HC\_NOISE** = 60

Used in: cal\_HC\_E2DS\_spirou, cal\_WAVE\_E2DS\_spirou  
 Defined in: constants\_SPIROU\_H4RG.py

- **Maximum sig-fit of guess lines (IC\_MAX\_SIGLL\_CAL\_LINES)**

Define the maximum sigma fit of the guessed lines (FWHM/2.35 of the lines). Used to filter out bad lines after a guess on the lines.

**IC\_MAX\_SIGLL\_CAL\_LINES** = 4

Used in: cal\_HC\_E2DS\_spirou, cal\_WAVE\_E2DS\_spirou  
 Defined in: constants\_SPIROU\_H4RG.py

- **Maximum error on guess lines (IC\_MAX\_ERRW\_ONFIT)**

Define the maximum error on the guess of the lines. Used to filter out bad lines after a guess on the lines.

**IC\_MAX\_ERRW\_ONFIT** = 1

Used in: cal\_HC\_E2DS\_spirou, cal\_WAVE\_E2DS\_spirou  
 Defined in: constants\_SPIROU\_H4RG.py

- **Maximum amplitude on guess lines (`IC_MAX_AMPL_LINE`)**

Define the maximum amplitude on the guess of the lines. Used to filter out bad lines after a guess on the lines.

`IC_MAX_AMPL_LINE` = 1.0e8

Used in: `cal_HC_E2DS_spirou`, `cal_WAVE_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Wave solution first order (`IC_HC_N_ORD_START`)**

Defines the first order to at which the wave solution is calculated.

`IC_HC_N_ORD_START` = 13

Used in: `cal_HC_E2DS_spirou`, `cal_WAVE_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Wave solution last order (`IC_HC_N_ORD_START`)**

Defines the last order to at which the wave solution is calculated.

`IC_HC_N_ORD_START` = 40

Used in: `cal_HC_E2DS_spirou`, `cal_WAVE_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **First echelle order number (`IC_HC_T_ORDER_START`)**

Defines the first echelle order number extracted.

`IC_HC_T_ORDER_START` = 79

Used in: `cal_HC_E2DS_spirou`, `cal_WAVE_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Minimum x error in 1D fit (`IC_ERRX_MIN`)**

Define the maximum weight given to a line via defining the minimum instrumental error, such that:

$$\text{max\_weight} = 1.0/(\text{IC\_ERRX\_MIN})^2 \quad (7.20)$$

`IC_ERRX_MIN` = 0.01

Used in: `cal_HC_E2DS_spirou`, `cal_WAVE_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- Wavelength solution poly-fit degree (**IC\_LL\_DEGR\_FIT**)

Define the wavelength fit polynomial order

**IC\_LL\_DEGR\_FIT** = 4

Used in: cal\_HC\_E2DS\_spirou, cal\_WAVE\_E2DS\_spirou  
Defined in: constants\_SPIROU\_H4RG.py

- Maximum RMS for wave solution sigma-clip fit (**IC\_MAX\_LLFIT\_RMS**)

Define the maximum RMS for the wavelength sigma-clip fitting process

**IC\_MAX\_LLFIT\_RMS** = 3.0

Used in: cal\_HC\_E2DS\_spirou, cal\_WAVE\_E2DS\_spirou  
Defined in: constants\_SPIROU\_H4RG.py

- Littrow poly-fit degree 1 (**IC\_LITTROW\_FIT\_DEG\_1**)

Define the polynomial fit degree for the Littrow fit (iteration 1)

**IC\_LITTROW\_FIT\_DEG\_1** = 5

Used in: cal\_HC\_E2DS\_spirou, cal\_WAVE\_E2DS\_spirou  
Defined in: constants\_SPIROU\_H4RG.py

- Littrow poly-fit degree 2 (**IC\_LITTROW\_FIT\_DEG\_2**)

Define the polynomial fit degree for the Littrow fit (iteration 2)

**IC\_LITTROW\_FIT\_DEG\_2** = 7

Used in: cal\_HC\_E2DS\_spirou, cal\_WAVE\_E2DS\_spirou  
Defined in: constants\_SPIROU\_H4RG.py

- Littrow cut steps (**IC\_LITTROW\_CUT\_STEP\_1**)

Define the x-pixel interval between positions to measure the Littrow at (iteration 1) i.e.:

$$x_{cutpoints} = [1 * step, 2 * step, 3 * step, \dots, (N - 1) * step] \quad (7.21)$$

where 'step' = IC\_LITTROW\_CUT\_STEP\_1 and 'N' = length of x-dimension divided by 'step'.

**IC\_LITTROW\_CUT\_STEP\_1** = 250

Used in: cal\_HC\_E2DS\_spirou, cal\_WAVE\_E2DS\_spirou  
Defined in: constants\_SPIROU\_H4RG.py

- **Littrow cut steps (IC\_LITTROW\_CUT\_STEP\_2)**

Define the x-pixel interval between positions to measure the Littrow at (iteration 2) i.e.:

$$x_{cutpoints} = [1 * step, 2 * step, 3 * step, \dots, (N - 1) * step] \quad (7.22)$$

where 'step' = IC\_LITTROW\_CUT\_STEP\_2 and 'N' = length of x-dimension divided by 'step'.

IC\_LITTROW\_CUT\_STEP\_2 = 500

Used in: cal\_HC\_E2DS\_spirou, cal\_WAVE\_E2DS\_spirou

Defined in: constants\_SPIROU\_H4RG.py

- **Littrow fit - first order (IC\_LITTROW\_ORDER\_INIT)**

Defines the first order to start the Littrow fit from

IC\_LITTROW\_ORDER\_INIT = 0

Used in: cal\_HC\_E2DS\_spirou, cal\_WAVE\_E2DS\_spirou

Defined in: constants\_SPIROU\_H4RG.py

- **Littrow fit - remove orders (IC\_LITTROW\_REMOVE\_ORDERS)**

Define the orders to ignore to ignore in the Littrow fit. Must be a valid python list of integers where each integer is a number between zero and the maximum number of orders.

IC\_LITTROW\_REMOVE\_ORDERS = []

Used in: cal\_HC\_E2DS\_spirou, cal\_WAVE\_E2DS\_spirou

Defined in: constants\_SPIROU\_H4RG.py

- **Littrow-Wavelength solution poly-fit degree (IC\_LITTROW\_ORDER\_FIT\_DEG)**

Define the wavelength fit polynomial order

IC\_LITTROW\_ORDER\_FIT\_DEG = 4

Used in: cal\_HC\_E2DS\_spirou, cal\_WAVE\_E2DS\_spirou

Defined in: constants\_SPIROU\_H4RG.py

- **Wavelength free-span 2 (IC\_LL\_FREE\_SPAN\_2)**

Define the wavelength free span parameter in find lines used after Littrow fit. Must be a list of line widths (in pixels). Ordered from largest to smallest.

IC\_LL\_FREE\_SPAN\_2 = [4.25, 3.0]

Used in: cal\_HC\_E2DS\_spirou, cal\_WAVE\_E2DS\_spirou

Defined in: constants\_SPIROU\_H4RG.py

- **Wave solution first order 2 (IC\_HC\_N\_ORD\_START\_2)**

Defines the first order to at which the wave solution is calculated used after Littrow fit.

**IC\_HC\_N\_ORD\_START\_2** = 0

Used in: `cal_HC_E2DS_spirou`, `cal_WAVE_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Wave solution last order 2 (IC\_HC\_N\_ORD\_START\_2)**

Defines the last order to at which the wave solution is calculated used after Littrow fit.

**IC\_HC\_N\_ORD\_START\_2** = 46

Used in: `cal_HC_E2DS_spirou`, `cal_WAVE_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Find lines mode (HC\_FIND\_LINES\_MODE)**

Defines the mode to find lines. Currently allowed modes are:

- 0: Fortran `fitgaus.f` routine
- 1: Python fit using `scipy.optimize.curve_fit`
- 2: Python fit using `lmfit.models` (Model, GaussianModel)
- 3: Python conversion of Fortran ‘fitgaus’ - direct translation
- 4: Python conversion of Fortran ‘fitgaus’ - gaussj improvement MH
- 5: Python conversion of Fortran ‘fitgaus’ - gaussj improvement NJC

where value must be an integer between 0 and 5.

**HC\_FIND\_LINES\_MODE** = 0

Used in: `cal_HC_E2DS_spirou`, `cal_WAVE_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **FP solution - first order (IC\_FP\_N\_ORD\_START)**

Defines the first order to start the FP solution fitting at.

**IC\_FP\_N\_ORD\_START** = 0

Used in: `cal_WAVE_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`



- **FP solution - last order (`IC_FP_N_ORD_FINAL`)**

Defines the last order to stop the FP solution fitting at.

`IC_FP_N_ORD_FINAL` = 24

Used in: `cal_WAVE_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **FP solution - region size (`IC_FP_SIZE`)**

Region size (in pixels) that each FP peak is fitted to

`IC_FP_SIZE` = 3

Used in: `cal_WAVE_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **FP solution - position threshold (`IC_FP_THRESHOLD`)**

Defines the threshold used in detecting the positions of the FP peaks.

`IC_FP_THRESHOLD` = 0.2

Used in: `cal_WAVE_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **FP solution - cavity width (`IC_FP_DOPD0`)**

Defines the initial value of the FP effective cavity width (in nm). For SPIROu this is:

$$2 \times d = 24.5mm = 24.5 \times 10^6 nm \quad (7.23)$$

`IC_FP_DOPD0` = 2.45e7

Used in: `cal_WAVE_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **FP solution - poly-fit degree (`IC_FP_FIT_DEGREE`)**

Defines the polynomial fit degree between FP line numbers and the measured cavity width for each line.

`IC_FP_FIT_DEGREE` = 9

Used in: `cal_WAVE_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **FP solution - large jump size (IC\_FP\_LARGE\_JUMP)**

Defines the “jump” value (in pixels) that is considered too large between the current and previous FP peaks.

**IC\_FP\_LARGE\_JUMP** = 0.7

Used in: [cal\\_WAVE\\_E2DS\\_spirou](#)

Defined in: [constants\\_SPIROU\\_H4RG.py](#)

## 7.17 CCF calibration variables

- CCF Width (**ic\_ccf\_width**)

Define the width of the CCF range. Value must be a positive integer.

**ic\_ccf\_width** = 30.0

Used in: `cal_CCF_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- CCF Step (**ic\_ccf\_step**)

Define the computations steps of the CCF

**ic\_ccf\_step** = 0.5

Used in: `cal_CCF_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- CCF mask weight (**ic\_w\_mask\_min**)

Define the weight of the CCF mask (if 1 force all weights equal)

**ic\_w\_mask\_min** = 0.0

Used in: `cal_CCF_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- Template line width (**ic\_mask\_width**)

Define the width of the template line (if 0 use natural)

**ic\_mask\_width** = 1.7

Used in: `cal_CCF_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- Barycentric Earth RV (**ccf\_berv**)

Define the barycentric Earth RV (berv)

**ccf\_berv** = 0.0

Used in: `cal_CCF_E2DS_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Maximum barycentric Earth RV (`ccf_berv_max`)**

Define the maximum barycentric Earth RV

`ccf_berv_max` = 0.0

Used in: `cal_CCF_E2DS_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Detector CCF noise (`ccf_det_noise`)**

Define the detector noise to use in the CCF.

`ccf_det_noise` = 100.0

Used in: `cal_CCF_E2DS_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **CCF Fit type (`ccf_fit_type`)**

Define the type of fit for the CCF fit.

`ccf_fit_type` = 0

Used in: `cal_CCF_E2DS_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **CCF end order number. (`ccf_num_orders_max`)**

Define the number of orders (from zero to `ccf_num_orders_max`) to use to calculate the CCF and RV

`ccf_num_orders_max` = 25

Used in: `cal_CCF_E2DS_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Earth velocity calculation mode (`CCF_BERVMODE`)**

Define the mode to work out the Earth velocity correction calculation. Options are:

- "off" - `berv` is set to zero
- "old" - `berv` is calculated with FORTRAN `newbervmain.f`
- "new" - `berv` is calculated using `barycorrpy`

`CCF_BERVMODE` = "new"

Used in: `cal_CCF_E2DS_spirou`

Defined in: `constants_SPIROU_H4RG.py`

## 7.18 Exposure-meter variables

- **Exposure-meter Fiber Type (`EM_FIB_TYPE`)**

Define which fiber to extract. Must be either AB or A or B or C.

`EM_FIB_TYPE` = "AB"

Used in: `cal_exposure_meter`

Defined in: `constants_SPIROU_H4RG.py`

- **Telluric threshold (`EM_TELL_THRESHOLD`)**

Define the telluric threshold (transmission) level to mask at.

`EM_TELL_THRESHOLD` = 0.95

Used in: `cal_exposure_meter`

Defined in: `constants_SPIROU_H4RG.py`

- **Minimum wavelength for exposure-meter (`EM_MIN_LAMBDA`)**

Define the minimum wavelength (in nm) to mask at.

`EM_MIN_LAMBDA` = 1478.7

Used in: `cal_exposure_meter`

Defined in: `constants_SPIROU_H4RG.py`

- **Maximum wavelength for exposure-meter (`EM_MAX_LAMBDA`)**

Define the maximum wavelength (in nm) to mask at.

`EM_MAX_LAMBDA` = 1823.1

Used in: `cal_exposure_meter`

Defined in: `constants_SPIROU_H4RG.py`

- **Exposure-meter file output type (EM\_OUTPUT\_TYPE)**

Define what shape/properties we want the output mask to be. Options are:

- "raw" - shape and rotation as in the raw input files
- "drs" - shape and rotation as in the DRS files
- "preprocess" - shape and rotation as in the pre-processed files
- "all" - produces all of the above

**EM\_OUTPUT\_TYPE** = "all"

Used in: `cal_exposure_meter`

Defined in: `constants_SPIROU_H4RG.py`

- **Exposure-meter - include bad pixel mask (EM\_COMBINED\_BADPIX)**

Define whether to combine exposure meter mask with the bad pixel mask. If True bad pixel mask is combined if False it is not.

**EM\_COMBINED\_BADPIX** = True

Used in: `cal_exposure_meter`

Defined in: `constants_SPIROU_H4RG.py`

- **Exposure-meter - save wave map (EM\_SAVE\_WAVE\_MAP)**

Define whether to save the 2D wavelength map. If True saves map if False does not save the map.

**EM\_SAVE\_WAVE\_MAP** = True

Used in: `cal_exposure_meter`

Defined in: `constants_SPIROU_H4RG.py`

- **Exposure-meter - save telluric spectrum (EM\_SAVE\_TELL\_SPEC)**

Define whether to save the telluric spectrum mapped on to the 2D wavelength map. If True saves map if False does not save the map.

**EM\_SAVE\_TELL\_SPEC** = True

Used in: `cal_exposure_meter`

Defined in: `constants_SPIROU_H4RG.py`

- **Exposure-meter - save mask (EM\_SAVE\_MASK\_MAP)**

Define whether to save the mask mapped on to the 2D wavelength map. If True saves map if False does not save the map.

**EM\_SAVE\_MASK\_MAP** = True

Used in: `cal_exposure_meter`

Defined in: `constants_SPIROU_H4RG.py`

## 7.19 Quality control variables

- **Maximum dark median level (`qc_max_darklevel`)**

Defines the maximum dark median level in ADU/s. If this is greater than median flux it does not pass the quality control criteria:

$$\text{Median Flux} < \text{qc\_max\_darklevel} \quad (7.24)$$

Value must be a float equal to or larger than zero.

`qc_max_darklevel` = 0.5

Used in: `cal_DARK_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Maximum percentage of dead pixels (`qc_max_dead`)**

Defines the maximum allowed percentage of dead pixels in a dark image. If the number of dead pixels is greater than this it does not pass the quality control criteria:

$$\text{dead pixels} = (\text{pixel value} > \text{dark\_cutlimit}) \text{ and } (\text{pixel value} \neq \text{NaN}) \quad (7.25)$$

$$\text{Percentage of dead pixels} < \text{qc\_max\_dead} \quad (7.26)$$

`qc_max_dead` = 20.0

Used in: `cal_DARK_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`

- **Maximum percentage of bad dark pixels (`qc_max_dark`)**

Defines the maximum allowed percentage of bad dark pixels in a dark image. If the number of dead pixels is greater than this it does not pass the quality control criteria:

$$\text{bad dark pixels} = \text{pixel value} > \text{dark\_cutlimit} \quad (7.27)$$

$$\text{Percentage of bad dark pixels} < \text{qc\_max\_dark} \quad (7.28)$$

`qc_max_dark` = 6.0

Used in: `cal_DARK_spirou`  
 Defined in: `constants_SPIROU_H4RG.py`



- **Minimum dark exposure time (`qc_dark_time`)**

Defines the minimum dark exposure time. If exposure time (from FITS rec HEADER) is below this the code will exit with ‘Dark exposure time too short’ message. Value must be a float greater than zero.

`qc_dark_time` = 599.0

Used in: `cal_DARK_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Maximum points removed in localization position fit (`qc_loc_maxlocfit_removed_ctr`)**

Defines the maximum allowed number of points removed in the position fitting process (during localization). If number is more than this it does not pass the quality control criteria:

$$\text{Number of rejected orders in center fit} > \text{qc\_loc\_maxlocfit\_removed\_ctr} \quad (7.29)$$

Value must be a integer greater than zero.

`qc_loc_maxlocfit_removed_ctr` = 1500

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Maximum points removed in localization width fit (`qc_loc_maxlocfit_removed_wid`)**

Defines the maximum allowed number of points removed in the width fitting process (during localization). If number is more than this it does not pass the quality control criteria:

$$\text{Number of rejected orders in width fit} > \text{qc\_loc\_maxlocfit\_removed\_width} \quad (7.30)$$

Value must be a integer greater than zero.

`qc_loc_maxlocfit_removed_wid` = 105

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Maximum allowed RMS in fitting in localization position fit (`qc_loc_rmsmax_center`)**

Defines the maximum RMS allowed in the position fitting process (during localization). If the RMS is higher than this value it does not pass the quality control criteria:

$$\text{Mean rms center fit} > \text{qc\_loc\_rmsmax\_center} \quad (7.31)$$

Value must be a float greater than zero.

`qc_loc_rmsmax_center` = 100

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Maximum allowed RMS in fitting in localization width fit (`qc_loc_rmsmax_fwhm`)**

Defines the maximum RMS allowed in the width fitting process (during localization). If the RMS is higher than this value it does not pass the quality control criteria:

$$\text{Mean rms width fit} > \text{qc\_loc\_rmsmax\_fwhm} \quad (7.32)$$

Value must be a float greater than zero.

`qc_loc_rmsmax_fwhm` = 500

Used in: `cal_loc_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Maximum allowed RMS (`qc_ff_rms`)**

Defines the maximum RMS allowed to accept a flat-field for calibration. Value must be a float greater than zero.

`qc_ff_rms` = 0.12

Used in: `cal_FF_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Saturation level reached warning (`qc_loc_flumax`)**

Defines the level above which a warning is generated in the form ‘SATURATION LEVEL REACHED on Fiber `fiber`’. Value must be a float greater than zero.

`qc_loc_flumax` = 64500

Used in: `cal_FF_RAW_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- **Maximum RMS allowed for slit TILT (`qc_slit_rms`)**

Defines the maximum allowed RMS in the calculated TILT to add TILT profile to the `calibration database`. Value must be a float larger than zero.

`qc_slit_rms` = 0.1

Used in: `cal_SLIT_spirou`

Defined in: `constants_SPIROU_H4RG.py`

- Minimum angle allowed for slit TILT (**qc\_slit\_min**)

Defines the minimum tilt angle allowed to add TILT profile to the calibration database. Value must be a float and must be less than **qc\_slit\_max**

**qc\_slit\_min** = -8.0

Used in: **cal\_SLIT\_spirou**

Defined in: **constants\_SPIROU\_H4RG.py**

- Maximum angle allowed for slit TILT (**qc\_slit\_max**)

Defines the maximum tilt angle allowed to add TILT profile to the calibration database. Value must be a float and must be greater than **qc\_slit\_min**

**qc\_slit\_max** = 0.0

Used in: **cal\_SLIT\_spirou**

Defined in: **constants\_SPIROU\_H4RG.py**

- Saturation point (**qc\_max\_signal**)

Defines the maximum signal allowed (when defining saturation limit). Currently this does not contribute to failing the quality test. Value must be a float greater than zero.

**qc\_max\_signal** = 65500

Used in: **cal\_extract\_RAW\_spirou**

Defined in: **constants\_SPIROU\_H4RG.py**

## 7.20 Calibration database variables

- The calibration database master filename (**ic\_calibDB\_filename**)

Defines the name of the master calibration database text file for use in all calibration database operation.

**ic\_calibDB\_filename** = master\_calib\_SPIROU.txt

Used in: All Recipes

Defined in: constants\_SPIROU\_H4RG.py

- Maximum wait time for locked calibration database (**calib\_max\_wait**)

Defines the maximum time the code waits for the calibration database when it is locked. A locked file is created every time the calibration database is open (and subsequently closed when reading of the database was successful). If a lock file is present the code will wait a maximum of this many seconds and keep checking whether the lock file has been removed. After which time the code will exit with an error. Value must be a positive float greater than zero. Measured in seconds.

**calib\_max\_wait** = 3600

Used in: All Recipes

Defined in: constants\_SPIROU\_H4RG.py

- Calibration database duplicate key handler (**calib\_db\_match**)

Defines the mechanism to use in deciding between duplicate keys in the calibration database file. Value must be a string and must be either 'older' or 'closest'. If 'older' the calibration database will only use keys that are older than the timestamp in the input fits file (first argument) using the key kw\_ACQTIME\_KEY

**calib\_db\_match** = 'closest'

Used in: All Recipes

Defined in: constants\_SPIROU\_H4RG.py

## 7.21 Logging and printing variables

- **Print message level (`PRINT_LEVEL`)**

The level of messages to print, values can be as follows:

- "all" – prints all events
- "info" – prints info, warning and error events
- "warning" – prints warning and error events
- "error" – print only error events

Value must be a valid string.

`PRINT_LEVEL` = all

Used in: All Recipes  
Defined in: ../config /config.py

- **Log message level (`LOG_LEVEL`)**

The level of messages to print, values can be as follows:

- "all" – prints all events
- "info" – prints info, warning and error events
- "warning" – prints warning and error events
- "error" – print only error events

Value must be a valid string.

`LOG_LEVEL` = all

Used in: All Recipes  
Defined in: ../config /config.py

- **Toggle coloured log (`COLOURED_LOG`)**

Defines whether the log (printed to the standard output) is coloured . Value must be True or 1 to colour the log or False or 0 to use the default console colour throughout.

`COLOURED_LOG` = True

Used in: All Recipes  
Defined in: ../config /config.py

## Chapter 8

# The Recipes

## 8.1 The cal\_DARK recipe

Dark with short exposure time ( 5min, to be defined during AT-4) to check if read-out noise, dark current and hot pixel mask are consistent with the ones obtained during technical night. Quality control is done automatically by the pipeline

### 8.1.1 The inputs

The input of `cal_DARK_spirou` is as follows:

```
>> cal_DARK_spirou.py night_repository filenames
```

for example:

```
example
>> cal_DARK_spirou.py 20170710 dark_dark02d406.fits
```

or

```
Python/Ipython
import cal_DARK_spirou
night_repository = '20170710'
filenames = ['dark_dark02d406.fits']
cal_DARK_spirou.main(night_repository, files=filenames)
```

where 'night\_repository' defines arg\_night\_name and 'filenames' define the list of files in arg\_file\_names. All files in filenames must be valid python strings separated by a space (command line) or in a line (python).

Filename prefixes allowed are:

- dark\_dark

### 8.1.2 The outputs

The outputs of `cal_DARK_spirou` are as follows:

- darkfile in form:

```
{reduced_dir}/{date prefix}_{file}.fits
```

- darkbadpixfile in form:

```
{reduced_dir}/{date prefix}_{file}_badpixel.fits
```

where 'date prefix' is constructed from arg\_night\_name and the file name is the first file in arg\_file\_names.

For example for `reduced_dir='/drs/data/reduced/20170710'` and `arg_file_names=['dark_dark02d406.fits']` the output files would be:

- /drs/data/reduced/20170710/20170710\_dark\_dark02d406.fits
- /drs/data/reduced/20170710/20170710\_dark\_dark02d406\_badpixel.fits

### 8.1.3 Summary of procedure

1. adds defined 'dark\_dark' files together
2. resizes the image
3. calculates the fraction of dead pixels [full, blue part, red part]
4. calculates median dark level [full, blue part, red part]
5. calculates threshold of dark level to retain
6. removes dead pixels by setting them to 0
7. does some quality control
8. updates calibDB with key "DARK"

### 8.1.4 Quality Control

There are currently three quality control checks for `cal_DARK_spirou`

- Unexpected median dark level if:

$$\text{Median Flux} > \text{qc\_max\_darklevel} \quad (8.1)$$

- Unexpected fraction of dead pixels if:

$$\text{Number of dead pixels} > \text{qc\_max\_dead} \quad (8.2)$$

- Unexpected fraction of dark pixels if:

$$\text{Number of bad dark pixels} > \text{qc\_max\_dark} \quad (8.3)$$

If none of these quality control criteria are valid then the output file is passed into the `calibration database` with key 'DARK' for the 'darkfile' and 'BADPIX' for the 'darkbadpixfile'.

For example the following lines are added to the `calibration database` for `arg_night_name = "20170710"` and `arg_file_names = "dark_dark02d406.fits"`.

In calibration database file

```
DARK 20170710 20170710_dark_dark02d406.fits 2017-07-10-12:37:48.260000 1499690268.26
BADPIX 20170710 20170710_dark_dark02d406_badpixel.fits 2017-07-10-12:37:48.260000 1499690268.26
```

## 8.1.5 Example working run

An example run where everything worked is below:

example


```
>> cal_DARK_spirou.py 20170710 dark_dark02d406.fits
```

```
HH:MM:SS.S - || *****
HH:MM:SS.S - || * SPIROU @(#) Geneva Observatory (VERSION)
HH:MM:SS.S - || *****
HH:MM:SS.S - ||(dir_data_raw)      DRS_DATA_RAW=/drs/data/raw
HH:MM:SS.S - ||(dir_data_reduc)    DRS_DATA_REduc=/drs/data/reduced
HH:MM:SS.S - ||(dir_calib_db)    DRS_CALIB_DB=/drs/data/calibDB
HH:MM:SS.S - ||(dir_data_msg)    DRS_DATA_MSG=/drs/data/msg
HH:MM:SS.S - ||(print_level)    PRINT_LEVEL=all          %(error/warning/info/all)
HH:MM:SS.S - ||(log_level)      LOG_LEVEL=all           %(error/warning/info/all)
HH:MM:SS.S - ||(plot_graph)     DRS_PLOT=1              %(def/undef/trigger)
HH:MM:SS.S - ||(used_date)      DRS_USED_DATE=undefined
HH:MM:SS.S - ||(working_dir)    DRS_DATA_WORKING=/drs/data/tmp/
HH:MM:SS.S - ||
HH:MM:SS.S - ||      DRS_INTERACTIVE is not set, running on-line mode
HH:MM:SS.S - ||
HH:MM:SS.S - ||      DRS_DEBUG is set, debug mode level:1
HH:MM:SS.S - |ipython:2d406|Now running : ipython on file(s): dark_dark02d406.fits
HH:MM:SS.S - |ipython:2d406|On directory /drs/data/raw/20170710
HH:MM:SS.S - |ipython:2d406|ICDP_NAME loaded from: /drs/INTROOT/config/constants_SPIROU.py
HH:MM:SS.S - * |ipython:2d406|Correct type of image for dark (dark_dark)
HH:MM:SS.S - * |ipython:2d406|Now processing Image TYPE UNKNOWN with ipython recipe
HH:MM:SS.S - |ipython:2d406|Reading Image /drs/data/raw/20170710/dark_dark02d406.fits
HH:MM:SS.S - |ipython:2d406|Image 2048 x 2048 loaded
HH:MM:SS.S - * |ipython:2d406|Dark Time = 597.489 s
HH:MM:SS.S - |ipython:2d406|Doing Dark measurement
HH:MM:SS.S - * |ipython:2d406|In Whole det: Frac dead pixels= 14.7 % - Median= 0.35 ADU/s - Percent
HH:MM:SS.S - | [5:95]= 0.08-99.57 ADU/s
HH:MM:SS.S - * |ipython:2d406|In Blue part: Frac dead pixels= 1.0 % - Median= 0.15 ADU/s - Percent
HH:MM:SS.S - | [5:95]= 0.09-0.53 ADU/s
HH:MM:SS.S - * |ipython:2d406|In Red part : Frac dead pixels= 20.5 % - Median= 2.11 ADU/s - Percent
HH:MM:SS.S - | [5:95]= 0.18-232.09 ADU/s
HH:MM:SS.S - * |ipython:2d406|Frac pixels with DARK > 100.0 ADU/s = 4.3 %
HH:MM:SS.S - @ |python warning|Line 138 warning reads: invalid value encountered in greater
HH:MM:SS.S - * |ipython:2d406|Total Frac dead pixels (N.A.N) + DARK > 100.0 ADU/s = 18.9 %
HH:MM:SS.S - * |ipython:2d406|QUALITY CONTROL SUCCESSFUL - Well Done -
HH:MM:SS.S - |ipython:2d406|Saving Dark frame in 20170710_dark_dark02d406.fits
HH:MM:SS.S - @ |python warning|Line 980 warning reads: Card is too long, comment will be truncated.
HH:MM:SS.S - |ipython:2d406|Saving Bad Pixel Map in 20170710_dark_dark02d406_badpixel.fits
HH:MM:SS.S - @ |python warning|Line 980 warning reads: Card is too long, comment will be truncated.
HH:MM:SS.S - * |ipython:2d406|Updating Calib Data Base with DARK
HH:MM:SS.S - * |ipython:2d406|Updating Calib Data Base with BADPIX
HH:MM:SS.S - * |ipython:2d406|Recipe ipython has been succesfully completed
```



### 8.1.6 Interactive mode

In interactive mode (`DRS_PLOT = 1`) three figures will also appear (see Figure 8.1).

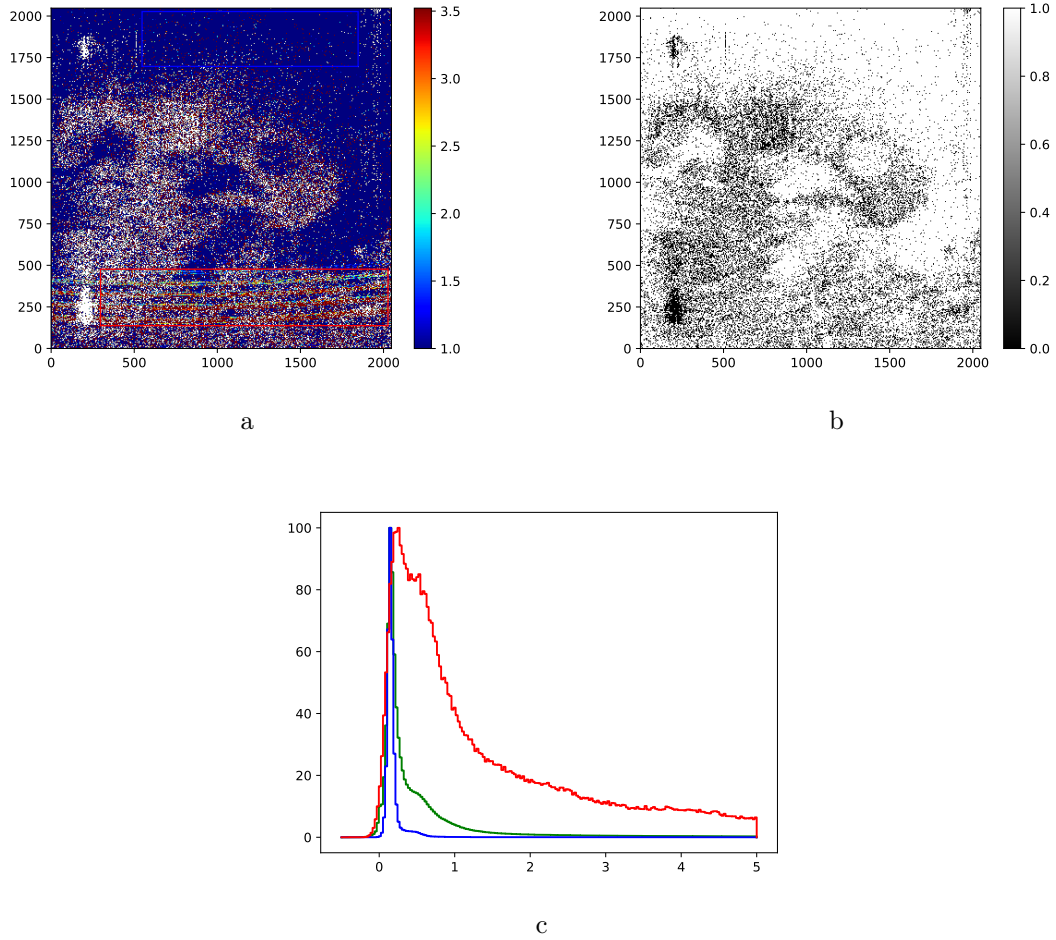

**Figure 8.1** (a) The image with over-plot red and blue regions (red/blue rectangles). (b) The bad pixel mask, bad pixels have a value=1 (in black) and good pixels have a value=0 (in white). (c) Histograms of the image regions, the full image (in green), the blue section (in blue) and the red section (in red).

## 8.2 The cal\_BADPIX recipe

Recipe to generate the bad pixel map.

### 8.2.1 The inputs

The input of `cal_BADPIX_spirou` is as follows:

```
>> cal_BADPIX_spirou.py night_repository flatfile darkfile
```

for example:

example

```
>> cal_BADPIX_spirou.py 20170710 flat_flat02f10.fits dark_dark02d406.fits
```

or

Python/Ipypthon

```
import cal_DARK_spirou
night_repository = '20170710'
darkfile = 'dark_dark02d406.fits'
flatfile = 'flat_flat02f10.fits'
cal_DARK_spirou.main(night_repository, flatfile=flatfile, darkfile=darkfile)
```

where 'night\_repository' defines `arg_night_name` and 'filenames' define the list of files in `arg_file_names`. All files in filenames must be valid python strings separated by a space (command line) or in a line (python) and must have the following prefixes: File prefixes allowed:

- flat\_flat (flatfile)
- dark\_dark (darkfile)

### 8.2.2 The outputs

The outputs of `badpixelfits` are as follows:

- `badpixelfits` in form:

```
{reduced_dir}/{date prefix}_{file}_badpixelfits.fits
```

where 'date prefix' is constructed from `arg_night_name` and the file name is the flatfile name.

for example for `reduced_dir='/drs/data/reduced/20170710'` and `flatfile='flat_flat02f10.fits'` the output file would be:

- `/drs/data/reduced/20170710/20170710_flat_flat02f10_badpixelfits.fits`

### 8.2.3 Summary of procedure

1. Normalise the flats
2. Look for isolated hot pixels
3. Calculate how much pixels deviate compared to expected values

4. Select hot pixels compared to neighbours
5. Combine bad pixel map
6. Save bad pixel mask to file

#### 8.2.4 Quality Control

There are no quality control parameters for `cal_BADPIX_spirou`.

The output file is passed into the `calibration database` with key 'BADPIX' for the 'badpixfile'.

For example the following lines are added to the `calibration database` for `arg_night_name = "20170710"` ,  
`flatfile = "flat_flat02f10.fits"` and `darkfile = "dark_dark02d406.fits"` .

In calibration database file

```
BADPIX 20170710 20170710_flat_flat02f10_badpixel.fits 2017-07-10-13:07:49.470000 1499692069.47
```

## 8.2.5 Example working run

An example run where everything worked is below:

example

```
>> cal_BADPIX_spirou.py 20170710 flat_flat02f10.fits dark_dark02d406.fits
```

```
HH:MM:SS.S - || *****
HH:MM:SS.S - || * SPIROU @(#) Geneva Observatory (VERSION)
HH:MM:SS.S - || *****
HH:MM:SS.S - ||(dir_data_raw)      DRS_DATA_RAW=/drs/data/raw
HH:MM:SS.S - ||(dir_data_reduc)     DRS_DATA_REduc=/drs/data/reduced
HH:MM:SS.S - ||(dir_calib_db)      DRS_CALIB_DB=/drs/data/calibDB
HH:MM:SS.S - ||(dir_data_msg)     DRS_DATA_MSG=/drs/data/msg
HH:MM:SS.S - ||(print_level)     PRINT_LEVEL=all          %(error/warning/info/all)
HH:MM:SS.S - ||(log_level)       LOG_LEVEL=all           %(error/warning/info/all)
HH:MM:SS.S - ||(plot_graph)      DRS_PLOT=1             %(def/undef/trigger)
HH:MM:SS.S - ||(used_date)       DRS_USED_DATE=undefined
HH:MM:SS.S - ||(working_dir)     DRS_DATA_WORKING=/drs/data/tmp
HH:MM:SS.S - ||
HH:MM:SS.S - || DRS_INTERACTIVE is not set, running on-line mode
HH:MM:SS.S - || DRS_DEBUG is set, debug mode level:1
HH:MM:SS.S - |cal_BADPIX_spirou|Now running : cal_BADPIX_spirou with:
HH:MM:SS.S - |cal_BADPIX_spirou|      -- flatfile=flat_flat02f10.fits
HH:MM:SS.S - |cal_BADPIX_spirou|      -- darkfile=dark_dark02d406.fits
HH:MM:SS.S - |cal_BADPIX_spirou|Config Error: ICDP_NAME loaded from: /drs/spirou_py3/INTROOT/config/
              constants_SPIROU.py
HH:MM:SS.S - * |cal_BADPIX_spirou|Now processing Image TYPE FLAT with cal_BADPIX_spirou recipe
HH:MM:SS.S - * |cal_BADPIX_spirou|Now processing Image TYPE DARK with cal_BADPIX_spirou recipe
HH:MM:SS.S - |cal_BADPIX_spirou|Reading FLAT Image /drs/data/raw/20170710/flat_flat02f10.fits
HH:MM:SS.S - |cal_BADPIX_spirou|FLAT Image 2048 x 2048 loaded
HH:MM:SS.S - |cal_BADPIX_spirou|Reading DARK Image /drs/data/raw/20170710/dark_dark02d406.fits
HH:MM:SS.S - |cal_BADPIX_spirou|DARK Image 2048 x 2048 loaded
HH:MM:SS.S - |cal_BADPIX_spirou|Normalising the flat
HH:MM:SS.S - |cal_BADPIX_spirou|Looking for bad pixels
HH:MM:SS.S - |cal_BADPIX_spirou|Fraction of hot pixels from dark: 3.01 %
HH:MM:SS.S - |cal_BADPIX_spirou|Fraction of bad pixels from flat: 1.66 %
HH:MM:SS.S - |cal_BADPIX_spirou|Fraction of non-finite pixels in dark: 20.76 %
HH:MM:SS.S - |cal_BADPIX_spirou|Fraction of non-finite pixels in flat: 14.66 %
HH:MM:SS.S - |cal_BADPIX_spirou|Fraction of bad pixels with all criteria: 24.87 %
HH:MM:SS.S - * |cal_BADPIX_spirou|QUALITY CONTROL SUCCESSFUL - Well Done -
HH:MM:SS.S - |cal_BADPIX_spirou|Saving Bad Pixel Map in 20170710_flat_flat02f10_badpixel.fits
HH:MM:SS.S - @ |python warning Line 980 warning reads: Card is too long, comment will be truncated.|
HH:MM:SS.S - * |cal_BADPIX_spirou|Updating Calib Data Base with BADPIX
HH:MM:SS.S - * |cal_BADPIX_spirou|Recipe cal_BADPIX_spirou has been successfully completed
```

## 8.3 The cal\_loc recipe

Locates the orders on the ‘dark\_flat’ or ‘flat\_dark’ images.

### 8.3.1 The inputs

The input of `cal_loc_RAW_spirou` is as follows:

```
>> cal_loc_RAW_spirou.py night_repository filenames
```

for example:

example

```
>> cal_loc_RAW_spirou.py 20170710 flat_dark02f10.fits flat_dark03f10.fits flat_dark04f10.fits
    flat_dark05f10.fits flat_dark06f10.fits
```

or

Python/Ipypthon

```
import cal_loc_RAW_spirou
night_repository = '20170710'
filenames = ['flat_dark02f10.fits', 'flat_dark03f10.fits', 'flat_dark04f10.fits',
             'flat_dark05f10.fits', 'flat_dark06f10.fits']
cal_loc_RAW_spirou.main(night_repository, files=filenames)
```

where ‘night\_repository’ defines `arg_night_name` and ‘filenames’ define the list of files in `arg_file_names`. All files in filenames must be valid python strings separated by a space (command line) or in a line (python) and must have the following prefixes: File prefixes allowed:

- dark\_flat
- flat\_dark

### 8.3.2 The outputs

The outputs of `cal_loc_RAW_spirou` are as follows:

- order\_profile in form:

```
{reduced_dir}/{date prefix}_{file}_order_profile_{fiber}.fits
```

- locofitsfile in form:

```
{reduced_dir}/{date prefix}_{file}_loco_{fiber}.fits
```

- locofitsfile2 in form:

```
{reduced_dir}/{date prefix}_{file}_fwhm-order_{fiber}.fits
```

- locofitsfile3 in form:

```
{reduced_dir}/{date prefix}_{file}_with-order_{fiber}.fits
```

where ‘date prefix’ is constructed from `arg_night_name` and the file name is the first file in `arg_file_names`.

For example for `reduced_dir='/drs/data/reduced/20170710'` and `arg_file_names=['flat_dark02f10.fits']` the output files would be:

- `/drs/data/reduced/20170710/20170710_flat_dark02f10_order_profile_{fiber}.fits`
- `/drs/data/reduced/20170710/20170710_flat_dark02f10_loco_{fiber}.fits`
- `/drs/data/reduced/20170710/20170710_flat_dark02f10_fwhm-order_{fiber}.fits`
- `/drs/data/reduced/20170710/20170710_flat_dark02f10_with-order_{fiber}.fits`

### 8.3.3 Summary of procedure

1. adds all defined 'dark\_flat' or 'flat\_dark' files together
2. corrects for darks
3. resizes the image
4. constructs 'order\_profile' image
5. locates the central pixel of each order
6. steps out in large steps along the order (toward beginning and end)
7. fits the position of each order (using a small 2D box around each fit point)
  - includes a rejection of bad points (while loop)
8. fits the width of each order (using a small 2D box around each fit point)
  - includes a rejection of bad points (while loop)
9. saves the 'order\_profile' image (with a superposition of the fit orders as zero values)
10. does some quality control
11. updates calibDB with keys "ORDER\_PROFILE\_{fiber}" "LOC\_{fiber}" where {fiber} = [AB, C] etc

### 8.3.4 Quality Control

There are currently five quality control checks for `cal_loc_RAW_spirou`

- Too many rejected orders in centre position fit:

$$\text{Number of rejected orders in centre fit} > \text{qc\_loc\_maxlocfit\_removed\_ctr} \quad (8.4)$$

- Too many rejected orders in width fit:

$$\text{Number of rejected orders in width fit} > \text{qc\_loc\_maxlocfit\_removed\_wid} \quad (8.5)$$

- RMS on centre fit too high:

$$\text{Mean rms centre fit} > \text{qc\_loc\_rmsmax\_center} \quad (8.6)$$

- RMS on width fit too high:

$$\text{Mean rms width fit} > \text{qc\_loc\_rmsmax\_fwhm} \quad (8.7)$$

- Abnormal number of identified orders:

$$\text{Number of orders found} \neq \text{qc\_loc\_nbo} \quad (8.8)$$

If none of these quality control criteria are valid then the output file is passed into the [calibration database](#) with keys 'ORDER\_PROFILE\_{fiber}' for the 'order\_profile' file and 'LOC\_{fiber}' for the 'locfitsname' file.

For example the following lines are added to the [calibration database](#) for `arg_night_name = "20170710"` and `arg_file_names = ["flat_dark02f10.fits"]`.

In calibration database file

```
ORDER_PROFILE_AB 20170710 20170710_flat_dark02f10_order_profile_AB.fits 2017-07-10-13:04:34.440000
1499691874.44
LOC_AB 20170710 20170710_flat_dark02f10_loco_AB.fits 2017-07-10-13:04:34.440000 1499691874.44
```

### 8.3.5 Example working run

An example run where everything worked is below:

example

```
>> cal_loc_RAW_spirou.py 20170710 flat_dark02f10.fits flat_dark03f10.fits flat_dark04f10.fits
flat_dark05f10.fits flat_dark06f10.fits
```

```
HH:MM:SS.S - || *****
HH:MM:SS.S - || * SPIROU @(#) Geneva Observatory (VERSION)
HH:MM:SS.S - || *****
HH:MM:SS.S - ||(dir_data_raw)      DRS_DATA_RAW=/drs/data/raw
HH:MM:SS.S - ||(dir_data_reduc)    DRS_DATA_REDUCE=/drs/data/reduced
HH:MM:SS.S - ||(dir_calib_db)     DRS_CALIB_DB=/drs/data/calibDB
HH:MM:SS.S - ||(dir_data_msg)    DRS_DATA_MSG=/drs/data/msg
HH:MM:SS.S - ||(print_level)    PRINT_LEVEL=all          %(error/warning/info/all)
HH:MM:SS.S - ||(log_level)      LOG_LEVEL=all           %(error/warning/info/all)
HH:MM:SS.S - ||(plot_graph)     DRS_PLOT=1              %(def/undef/trigger)
HH:MM:SS.S - ||(used_date)      DRS_USED_DATE=undefined
HH:MM:SS.S - ||(working_dir)    DRS_DATA_WORKING=/drs/data/tmp
HH:MM:SS.S - ||                  DRS_INTERACTIVE is not set, running on-line mode
HH:MM:SS.S - ||                  DRS_DEBUG is set, debug mode level:1
HH:MM:SS.S - |cal_loc_RAW_spirou|Now running : ipython on file(s):
HH:MM:SS.S - |cal_loc_RAW_spirou|On directory /drs/data/raw/20170710
HH:MM:SS.S - |cal_loc_RAW_spirou|ICDP_NAME loaded from: /drs/spirou_py3/INTROOT/config/
constants_SPIROU.py
HH:MM:SS.S - * |cal_loc_RAW_spirou|Correct type of image for localisation (dark_flat or flat_dark)
HH:MM:SS.S - |cal_loc_RAW_spirou|Calibration file: 20170710_flat_flat02f10_badpixel.fits already
exists - not copied
HH:MM:SS.S - |cal_loc_RAW_spirou|Calibration file: 20170710_flat_dark02f10_blaze_AB.fits already
exists - not copied
```

```

...
HH:MM:SS.S - |cal_loc_RAW_spirou|Calibration file: spirou_wave_ini3.fits already exists - not copied
HH:MM:SS.S - |cal_loc_RAW_spirou|Calibration file: 2017-10-11_21-32-17_hcone_hcone02c406_wave_C.fits
              already exists - not copied
HH:MM:SS.S - * |cal_loc_RAW_spirou|Now processing Image TYPE UNKNOWN with ipython recipe
HH:MM:SS.S - |cal_loc_RAW_spirou|Reading Image /drs/data/raw/20170710/flat_dark02f10.fits
HH:MM:SS.S - |cal_loc_RAW_spirou|Image 2048 x 2048 loaded
HH:MM:SS.S - * |cal_loc_RAW_spirou|Adding 4 frame(s)
HH:MM:SS.S - |cal_loc_RAW_spirou|Reading File: /drs/data/raw/20170710/flat_dark03f10.fits
HH:MM:SS.S - |cal_loc_RAW_spirou|Reading File: /drs/data/raw/20170710/flat_dark04f10.fits
HH:MM:SS.S - |cal_loc_RAW_spirou|Reading File: /drs/data/raw/20170710/flat_dark05f10.fits
HH:MM:SS.S - |cal_loc_RAW_spirou|Reading File: /drs/data/raw/20170710/flat_dark06f10.fits
HH:MM:SS.S - |cal_loc_RAW_spirou|Doing Dark Correction using /drs/data/calibDB/20170710
              _dark_dark02d406.fits
HH:MM:SS.S - |cal_loc_RAW_spirou|Image format changed to 1930x2035
HH:MM:SS.S - |cal_loc_RAW_spirou|Saving processed raw frame in 20170710
              _flat_dark02f10_order_profile_AB.fits
HH:MM:SS.S - @ |python warning Line 980  warning reads: Card is too long, comment will be truncated.|
HH:MM:SS.S - * |cal_loc_RAW_spirou|Updating Calib Data Base with ORDER_PROFILE_AB
HH:MM:SS.S - * |cal_loc_RAW_spirou|Maximum flux/pixel in the spectrum: 412475.3 [e-]
HH:MM:SS.S - * |cal_loc_RAW_spirou|Average background level: 1.36 [%]
HH:MM:SS.S - |cal_loc_RAW_spirou|Searching order center on central column
HH:MM:SS.S - * |cal_loc_RAW_spirou|On fiber AB 36 orders have been detected on 2 fiber(s)
HH:MM:SS.S - |cal_loc_RAW_spirou|ORDER: 0 center at pixel 102.5 width 11.6 rms 0.047
HH:MM:SS.S - |cal_loc_RAW_spirou| - center fit rms/ptp/sigrms: 0.047/0.108/2.305 with 0 rejected
              points
HH:MM:SS.S - |cal_loc_RAW_spirou| - width fit rms/ptp/ptp%: 0.442/0.814/6.951 with 0 rejected
              points
HH:MM:SS.S - |cal_loc_RAW_spirou|ORDER: 1 center at pixel 116.9 width 11.4 rms 0.072
HH:MM:SS.S - |cal_loc_RAW_spirou| - center fit rms/ptp/sigrms: 0.072/0.167/2.331 with 0 rejected
              points
HH:MM:SS.S - |cal_loc_RAW_spirou| - width fit rms/ptp/ptp%: 0.457/0.875/7.295 with 0 rejected
              points
...
HH:MM:SS.S - |cal_loc_RAW_spirou|ORDER: 71 center at pixel 1881.0 width 10.8 rms 0.414
HH:MM:SS.S - |cal_loc_RAW_spirou|      center fit converging with rms/ptp/sigrms: 0.414/2.989/7.215
...
HH:MM:SS.S - |cal_loc_RAW_spirou|      center fit converging with rms/ptp/sigrms: 0.100/0.203/2.026
HH:MM:SS.S - |cal_loc_RAW_spirou| - center fit rms/ptp/sigrms: 0.098/0.193/1.973 with 21 rejected
              points
HH:MM:SS.S - |cal_loc_RAW_spirou|      fwhm fit converging with rms/ptp/ptp%: 0.970/5.272/87.869
...
HH:MM:SS.S - |cal_loc_RAW_spirou|      fwhm fit converging with rms/ptp/ptp%: 0.478/1.258/10.480
HH:MM:SS.S - |cal_loc_RAW_spirou| - width fit rms/ptp/ptp%: 0.459/1.199/9.993 with 12 rejected
              points
HH:MM:SS.S - * |cal_loc_RAW_spirou|On fiber AB 72 orders geometry have been measured
HH:MM:SS.S - * |cal_loc_RAW_spirou|Average uncertainty on position: 65.96 [mpix]
HH:MM:SS.S - * |cal_loc_RAW_spirou|Average uncertainty on width: 388.67 [mpix]
HH:MM:SS.S - * |cal_loc_RAW_spirou|QUALITY CONTROL SUCCESSFUL - Well Done -
HH:MM:SS.S - |cal_loc_RAW_spirou|Saving localization information in file: 20170710
              _flat_dark02f10_loco_AB.fits
HH:MM:SS.S - @ |python warning Line 980  warning reads: Card is too long, comment will be truncated.|
HH:MM:SS.S - |cal_loc_RAW_spirou|Saving FWHM information in file: 20170710_flat_dark02f10_fwhm-
              order_AB.fits


```



```
HH:MM:SS.S - @ |python warning Line 980 warning reads: Card is too long, comment will be truncated.|
HH:MM:SS.S - |cal_loc_RAW_spirou|Saving localization image with superposition of orders in
HH:MM:SS.S - |cal_loc_RAW_spirou|file: 20170710_flat_dark02f10_with-order_AB.fits
HH:MM:SS.S - * |cal_loc_RAW_spirou|Updating Calib Data Base with LOC_AB
HH:MM:SS.S - * |cal_loc_RAW_spirou|Recipe ipython has been successfully completed
```

8.3.6 Interactive mode

In interactive mode three figures will also appear (see Figure 8.2).

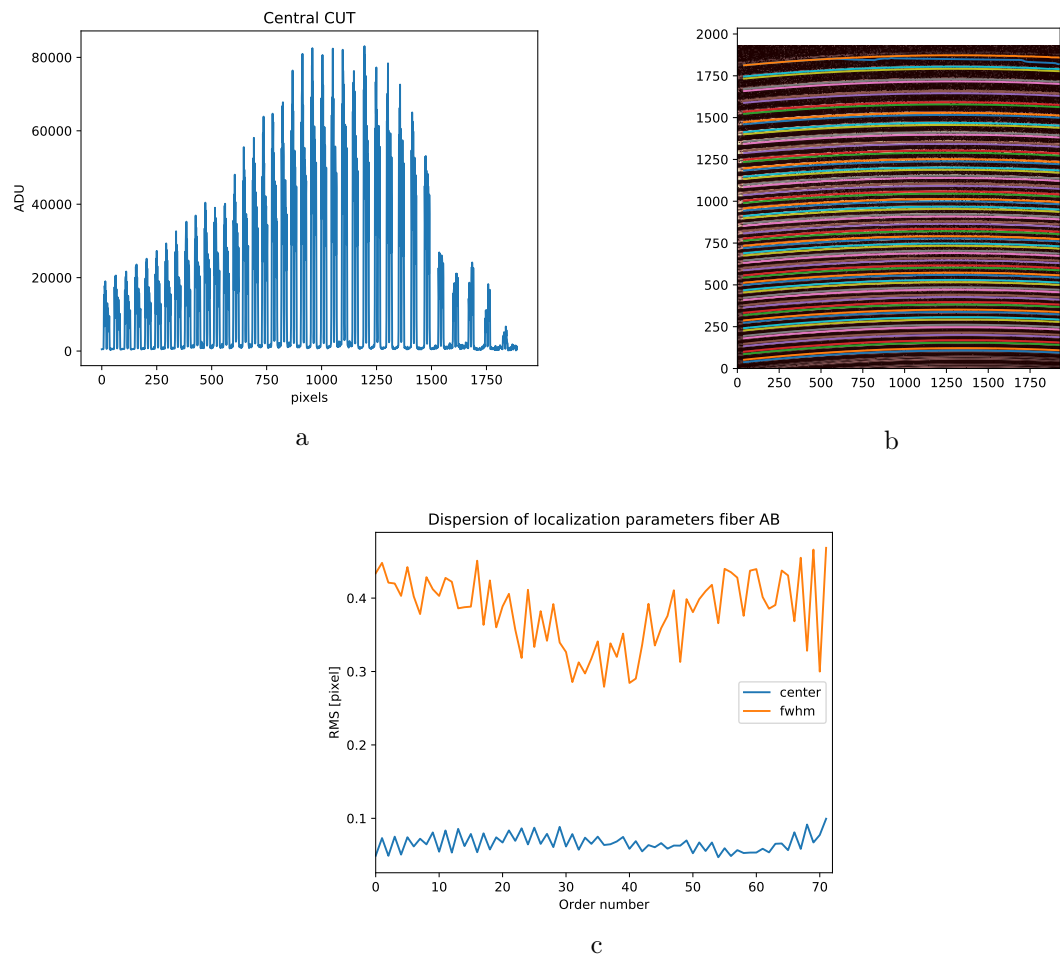

**Figure 8.2** (a) Pixel number (across order) against flux value of central pixel. (b) Image with fits to each order. (c) The dispersion of localization parameters.

## 8.4 The cal\_SLIT recipe

Fabry-Perot exposures in which the three fibres are simultaneously fed by light from the Fabry-Perot filter. Each exposure is used to build the slit orientation. Finds the tilt of the orders.

### 8.4.1 The inputs

The input of `cal_SLIT_spirou` is as follows:

```
>> cal_SLIT_spirou.py night_repository filenames
```

for example:

```
>> cal_SLIT_spirou.py 20170710 fp_fp02a203.fits fp_fp03a203.fits fp_fp04a203.fits
```

or

Python/Ipypthon

```
import cal_SLIT_spirou
night_repository = '20170710'
filenames = ['fp_fp02a203.fits', 'fp_fp03a203.fits', 'fp_fp04a203.fits']
cal_SLIT_spirou.main(night_repository, files=filenames)
```

where 'night\_repository' defines arg\_night\_name and 'filenames' define the list of files in arg\_file\_names. All files in filenames must be valid python strings separated by a space (command line) or in a line (python) and must have the following prefixes:

- fp\_fp

### 8.4.2 The outputs

The outputs of `cal_SLIT_spirou` are as follows:

- tiltfits in form:

```
{reduced_dir}/{date prefix}_{file}_tilt.fits
```

where 'date prefix' is constructed from arg\_night\_name and the file name is the first file in arg\_file\_names. for example for reduced\_dir='/drs/data/reduced/20170710' and arg\_file\_names=['fp\_fp02a203.fits', 'fp\_fp03a203.fits', 'fp\_fp04a203.fits'] the output files would be:

- /drs/data/reduced/20170710/20170710\_fp\_fp02a203\_tilt.fits

### 8.4.3 Summary of procedure

1. adds all fp\_fp files together
2. corrects for dark
3. resizes the image
4. extracts the orders (no weight no tilt)
5. works out the tilt for each order using the location and width

6. saves the tilt to file
7. should do some quality control
8. updates calibDB with key “TILT”

#### 8.4.4 Quality Control

There are currently two quality control checks for `cal_SLIT_spirou`

- Abnormal RMS of SLIT angle if:

$$\text{RMS}_{\text{tilt}} > \text{qc\_slit\_rms} \quad (8.9)$$

- Abnormal SLIT angle if:

$$\max(\text{tilt}) > \text{qc\_slit\_max} \quad (8.10)$$

or

$$\min(\text{tilt}) < \text{qc\_slit\_min} \quad (8.11)$$

If none of these quality control criteria are valid then the output file is passed into the `calibration database` with key ‘TILT’.

For example the following lines are added to the `calibration database` for `arg_night_name = "20170710"` and `arg_file_names = ['fp_fp02a203.fits', 'fp_fp03a203.fits', 'fp_fp04a203.fits']`.

In calibration database file

```
TILT 20170710 20170710_fp_fp02a203_tilt.fits 2017-07-10-13:25:15.590000 1499693115.59
```

#### 8.4.5 Example working run

An example run where everything worked is below:

```
>> cal_SLIT_spirou.py 20170710 fp_fp02a203.fits fp_fp03a203.fits fp_fp04a203.fits
```

```
HH:MM:SS.S - || *****
HH:MM:SS.S - || * SPIROU @(#) Geneva Observatory (VERSION)
HH:MM:SS.S - || *****
HH:MM:SS.S - ||(dir_data_raw)      DRS_DATA_RAW=/drs/data/raw
HH:MM:SS.S - ||(dir_data_reduc)    DRS_DATA_REDUCE=/drs/data/reduced
HH:MM:SS.S - ||(dir_calib_db)     DRS_CALIB_DB=/drs/data/calibDB
HH:MM:SS.S - ||(dir_data_msg)    DRS_DATA_MSG=/drs/data/msg
HH:MM:SS.S - ||(print_level)     PRINT_LEVEL=all          %(error/warning/info/all)
HH:MM:SS.S - ||(log_level)      LOG_LEVEL=all          %(error/warning/info/all)
HH:MM:SS.S - ||(plot_graph)     DRS_PLOT=1            %(def/undef/trigger)
HH:MM:SS.S - ||(used_date)      DRS_USED_DATE=undefined
HH:MM:SS.S - ||(working_dir)    DRS_DATA_WORKING=/drs/data/tmp
HH:MM:SS.S - ||                DRS_INTERACTIVE is not set, running on-line mode
HH:MM:SS.S - ||                DRS_DEBUG is set, debug mode level:1
HH:MM:SS.S - |cal_SLIT_spirou:2a203+[...]|Now running : cal_SLIT_spirou on file(s): fp_fp02a203.fits
, fp_fp03a203.fits, fp_fp04a203.fits
HH:MM:SS.S - |cal_SLIT_spirou:2a203+[...]|On directory /drs/data/raw/20170710
```


```

HH:MM:SS.S - |cal_SLIT_spirou:2a203+...|ICDP_NAME loaded from: /scratch/Projects/spirou_py3/
               spirou_py3/INTROOT/config/constants_SPIROU.py
HH:MM:SS.S - * |cal_SLIT_spirou:2a203+...|Correct type of image for slit (f or p or _ or f or p)
HH:MM:SS.S - |cal_SLIT_spirou:2a203+...|Calibration file: 20170710_flat_flat02f10_badpixel.fits
               already exists - not copied
...
HH:MM:SS.S - |cal_SLIT_spirou:2a203+...|Calibration file: spirou_wave_ini3.fits already exists -
               not copied
HH:MM:SS.S - |cal_SLIT_spirou:2a203+...|Calibration file: 2017-10-11_21-32-17
               _hcone_hcone02c406_wave_AB.fits already exists - not copied
HH:MM:SS.S - |cal_SLIT_spirou:2a203+...|Calibration file: spirou_wave_ini3.fits already exists -
               not copied
HH:MM:SS.S - |cal_SLIT_spirou:2a203+...|Calibration file: 2017-10-11_21-32-17
               _hcone_hcone02c406_wave_C.fits already exists - not copied
HH:MM:SS.S - * |cal_SLIT_spirou:2a203+...|Now processing Image TYPE UNKNOWN with cal_SLIT_spirou
               recipe
HH:MM:SS.S - |cal_SLIT_spirou:2a203+...|Reading Image /drs/data/raw/20170710/fp_fp02a203.fits
HH:MM:SS.S - |cal_SLIT_spirou:2a203+...|Image 2048 x 2048 loaded
HH:MM:SS.S - * |cal_SLIT_spirou:2a203+...|Adding 2 frame(s)
HH:MM:SS.S - |cal_SLIT_spirou:2a203+...|Reading File: /drs/data/raw/20170710/fp_fp03a203.fits
HH:MM:SS.S - |cal_SLIT_spirou:2a203+...|Reading File: /drs/data/raw/20170710/fp_fp04a203.fits
HH:MM:SS.S - |cal_SLIT_spirou:2a203+...|Doing Dark Correction using /drs/data/calibDB/20170710
               _dark_dark02d406.fits
HH:MM:SS.S - |cal_SLIT_spirou:2a203+...|Image format changed to 1930x2035
HH:MM:SS.S - * |cal_SLIT_spirou:2a203+...|Nb dead pixels = 611716 / 15.58 %
HH:MM:SS.S - |cal_SLIT_spirou:2a203+...|Reading localization parameters of Fiber AB
HH:MM:SS.S - |cal_SLIT_spirou:2a203+...|Order 0.0: Tilt = 4.70 on pixel 37.0 = -7.23 deg
HH:MM:SS.S - |cal_SLIT_spirou:2a203+...|Order 1.0: Tilt = 4.60 on pixel 37.4 = -7.02 deg
HH:MM:SS.S - |cal_SLIT_spirou:2a203+...|Order 2.0: Tilt = 4.50 on pixel 36.8 = -6.97 deg
HH:MM:SS.S - |cal_SLIT_spirou:2a203+...|Order 3.0: Tilt = 4.30 on pixel 36.3 = -6.75 deg
...
HH:MM:SS.S - |cal_SLIT_spirou:2a203+...|Order 32.0: Tilt = 1.40 on pixel 33.3 = -2.41 deg
HH:MM:SS.S - |cal_SLIT_spirou:2a203+...|Order 33.0: Tilt = 1.10 on pixel 32.3 = -1.95 deg
HH:MM:SS.S - |cal_SLIT_spirou:2a203+...|Order 34.0: Tilt = 1.00 on pixel 32.1 = -1.79 deg
HH:MM:SS.S - |cal_SLIT_spirou:2a203+...|Order 35.0: Tilt = 0.30 on pixel 17.1 = -1.01 deg
HH:MM:SS.S - * |cal_SLIT_spirou:2a203+...|AB|Tilt dispersion = 0.091 deg
HH:MM:SS.S - |cal_SLIT_spirou:2a203+...|Saving tilt information in file: 20170710
               _fp_fp02a203_tilt.fits
HH:MM:SS.S - @ |python warning Line 980 warning reads: Card is too long, comment will be truncated.|
HH:MM:SS.S - * |cal_SLIT_spirou:2a203+...|QUALITY CONTROL SUCCESSFUL - Well Done -
HH:MM:SS.S - * |cal_SLIT_spirou:2a203+...|Updating Calib Data Base with TILT
HH:MM:SS.S - * |cal_SLIT_spirou:2a203+...|Recipe cal_SLIT_spirou has been successfully completed
HHMSSS

```

## 8.4.6 Interactive mode

In interactive mode three figures will also appear (see Figure 8.3).

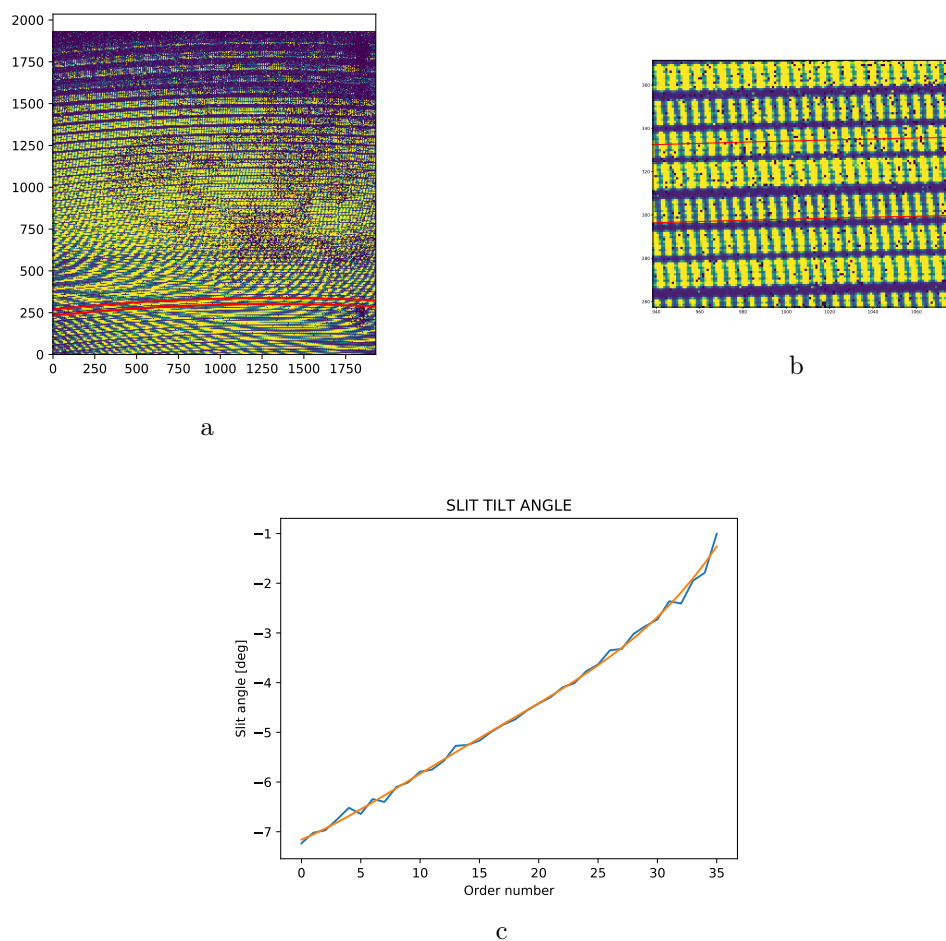

**Figure 8.3** (a) The full 'fp\_fp' image with one orders fit plotted. (b) Zoom in on a section of the 'fp\_fp' image showing the tilt. (c) Slit angle as a function of order number with the fit to the tilt also show.

## 8.5 The cal\_FF recipe

Creates the flat fields.

### 8.5.1 The inputs

The input of `cal_FF_RAW_spirou` is as follows:

```
>> cal_FF_RAW_spirou.py night_repository filenames
```

for example

example

```
>> cal_FF_RAW_spirou.py 20170710 dark_flat02f10.fits dark_flat03f10.fits dark_flat04f10.fits
    dark_flat05f10.fits dark_flat06f10.fits
```

or

Python/Ipython

```
import cal_FF_RAW_spirou
night_repository = '20170710'
filenames = ['dark_flat02f10.fits', 'dark_flat03f10.fits', 'dark_flat04f10.fits',
             'dark_flat05f10.fits', 'dark_flat06f10.fits']
cal_FF_RAW_spirou.main()
```

where 'night\_repository' defines arg\_night\_name and 'filenames' define the list of files in arg\_file\_names. All files in filenames must be valid python strings separated by a space (command line) or in a line (python) and must have the following prefixes:

- dark\_flat
- flat\_dark

### 8.5.2 The outputs

The outputs of `cal_FF_RAW_spirou` are as follows:

- blazefits in form:

```
{reduced_dir}/{date prefix}_{file}_blaze_{fiber}.fits
```

- flatfits in form:

```
{reduced_dir}/{date prefix}_{file}_flat_{fiber}.fits
```

where 'date prefix' is constructed from arg\_night\_name and the file name is the first file in arg\_file\_names. for example for reduced\_dir='/drs/data/reduced/20170710' and arg\_file\_names=['dark\_flat02f10.fits', 'dark\_flat03f10.fits', 'dark\_flat04f10.fits', 'dark\_flat05f10.fits', 'dark\_flat06f10.fits'] the output files would be:

- /drs/data/reduced/20170710/20170710\_flat\_dark02f10\_blaze\_AB.fits
- /drs/data/reduced/20170710/20170710\_flat\_dark02f10\_flat\_AB.fits

### 8.5.3 Summary of procedure

1. adds all 'dark\_flat' or 'flat\_dark' files together
2. corrects for darks
3. resizes the image
4. possible background subtraction?
5. extracts the orders using tilt and weight
6. calculates the blaze
7. calculates the flat field, (flat = extraction / blaze)
8. stores the flat fields
9. does some quality control
10. updates calibDB with key "FLAT\_{fiber}" where {fiber} = [AB, C] etc.

### 8.5.4 Quality Control

There is currently one quality control check for `cal_FF_RAW_spirou`

- Too much flux in the image:

$$\text{maximum signal} > \text{qc\_max\_signal} * \text{nbframes} \quad (8.12)$$

**Note:** This check does not currently lead to a failed run and all files are processed as passing quality checks

The output file is passed into the `calibration database` with key 'FLAT\_{fiber}' for the 'flatfits' file.

For example the following lines are added to the `calibration database` for `arg_night_name = "20170710"` and `arg_file_names=['dark_flat02f10.fits', 'dark_flat03f10.fits', 'dark_flat04f10.fits', 'dark_flat05f10.fits', 'dark_flat06f10.fits']`.

In calibration database file

```
FLAT_C 20170710 20170710_dark_flat02f10_flat_C.fits 2017-07-10-13:03:50.440000 1499691830.44
BLAZE_C 20170710 20170710_dark_flat02f10_blaze_C.fits 2017-07-10-13:03:50.440000 1499691830.44
```



### 8.5.5 Example working run

An example run where everything worked is below:

example

```
>> cal_FF_RAW_spirou.py 20170710 dark_flat02f10.fits dark_flat03f10.fits dark_flat04f10.fits
    dark_flat05f10.fits dark_flat06f10.fits
```

```
HH:MM:SS.S - || *****
HH:MM:SS.S - || * SPIROU @(#) Geneva Observatory (VERSION)
HH:MM:SS.S - || *****
HH:MM:SS.S - ||(dir_data_raw)      DRS_DATA_RAW=/drs/data/raw
HH:MM:SS.S - ||(dir_data_reduc)    DRS_DATA_REDUCE=/drs/data/reduced
HH:MM:SS.S - ||(dir_calib_db)     DRS_CALIB_DB=/drs/data/calibDB
HH:MM:SS.S - ||(dir_data_msg)    DRS_DATA_MSG=/drs/data/msg
HH:MM:SS.S - ||(print_level)     PRINT_LEVEL=all          %(error/warning/info/all)
HH:MM:SS.S - ||(log_level)      LOG_LEVEL=all           %(error/warning/info/all)
HH:MM:SS.S - ||(plot_graph)     DRS_PLOT=1              %(def/undef/trigger)
HH:MM:SS.S - ||(used_date)      DRS_USED_DATE=undefined
HH:MM:SS.S - ||(working_dir)    DRS_DATA_WORKING=/drs/data/tmp
HH:MM:SS.S - ||
HH:MM:SS.S - ||      DRS_INTERACTIVE is not set, running on-line mode
HH:MM:SS.S - ||      DRS_DEBUG is set, debug mode level:1
HH:MM:SS.S - |cal_FF_RAW_spirou:02f10+[...]|Now running : cal_FF_RAW_spirou on file(s):
    dark_flat02f10.fits, dark_flat03f10.fits, dark_flat04f10.fits, dark_flat05f10.fits,
    dark_flat06f10.fits
HH:MM:SS.S - |cal_FF_RAW_spirou:02f10+[...]|On directory /drs/data/raw/20170710
HH:MM:SS.S - |cal_FF_RAW_spirou:02f10+[...]|ICDP_NAME loaded from: /scratch/Projects/spirou_py3/
    spirou_py3/INTRROOT/config/constants_SPIROU.py
HH:MM:SS.S - * |cal_FF_RAW_spirou:02f10+[...]|Correct type of image for Flat-field (dark_flat or
    flat_dark)
HH:MM:SS.S - |cal_FF_RAW_spirou:02f10+[...]|Calibration file: 20170710_flat_flat02f10_badpixel.fits
    already exists - not copied
HH:MM:SS.S - |cal_FF_RAW_spirou:02f10+[...]|Calibration file: 20170710_dark_dark02d406.fits already
    exists - not copied
...
HH:MM:SS.S - |cal_FF_RAW_spirou:02f10+[...]|Calibration file: 20170710
    _flat_dark02f10_order_profile_AB.fits already exists - not copied
HH:MM:SS.S - |cal_FF_RAW_spirou:02f10+[...]|Calibration file: 20170710
    _dark_flat02f10_order_profile_C.fits already exists - not copied
HH:MM:SS.S - |cal_FF_RAW_spirou:02f10+[...]|Calibration file: 20170710_fp_fp02a203_tilt.fits already
    exists - not copied
HH:MM:SS.S - |cal_FF_RAW_spirou:02f10+[...]|Calibration file: spirou_wave_ini3.fits already exists -
    not copied
HH:MM:SS.S - |cal_FF_RAW_spirou:02f10+[...]|Calibration file: 2017-10-11_21-32-17
    _hcone_hcone02c406_wave_AB.fits already exists - not copied
HH:MM:SS.S - |cal_FF_RAW_spirou:02f10+[...]|Calibration file: spirou_wave_ini3.fits already exists -
    not copied
HH:MM:SS.S - |cal_FF_RAW_spirou:02f10+[...]|Calibration file: 2017-10-11_21-32-17
    _hcone_hcone02c406_wave_C.fits already exists - not copied
HH:MM:SS.S - * |cal_FF_RAW_spirou:02f10+[...]|Now processing Image TYPE UNKNOWN with cal_FF_RAW_spirou
    recipe
HH:MM:SS.S - |cal_FF_RAW_spirou:02f10+[...]|Reading Image /drs/data/raw/20170710/dark_flat02f10.fits
HH:MM:SS.S - |cal_FF_RAW_spirou:02f10+[...]|Image 2048 x 2048 loaded
HH:MM:SS.S - * |cal_FF_RAW_spirou:02f10+[...]|Adding 4 frame(s)
```


```

HH:MM:SS.S - |cal_FF_RAW_spirou:02f10+[...]|Reading File: /drs/data/raw/20170710/dark_flat03f10.fits
HH:MM:SS.S - |cal_FF_RAW_spirou:02f10+[...]|Reading File: /drs/data/raw/20170710/dark_flat04f10.fits
HH:MM:SS.S - |cal_FF_RAW_spirou:02f10+[...]|Reading File: /drs/data/raw/20170710/dark_flat05f10.fits
HH:MM:SS.S - |cal_FF_RAW_spirou:02f10+[...]|Reading File: /drs/data/raw/20170710/dark_flat06f10.fits
HH:MM:SS.S - |cal_FF_RAW_spirou:02f10+[...]|Doing Dark Correction using /drs/data/calibDB/20170710
               _dark_dark02d406.fits
HH:MM:SS.S - |cal_FF_RAW_spirou:02f10+[...]|Image format changed to 2035x1930
HH:MM:SS.S - * |cal_FF_RAW_spirou:02f10+[...]|Nb dead pixels = 568541 / 14.48 %
HH:MM:SS.S - * |cal_FF_RAW_spirou:02f10+[...]|Maximum average flux/pixel in the spectrum: 73636.3 [ADU
               ]
HH:MM:SS.S - |cal_FF_RAW_spirou:02f10+[...]|Reading localization parameters of Fiber C
HH:MM:SS.S - |cal_FF_RAW_spirou:02f10+[...]|C|Reading order profile of Fiber C
HH:MM:SS.S - |cal_FF_RAW_spirou:02f10+[...]|On fiber C order 0: S/N= 1158.4 - FF rms=4.68 %
HH:MM:SS.S - |cal_FF_RAW_spirou:02f10+[...]|On fiber C order 1: S/N= 1193.9 - FF rms=4.80 %
HH:MM:SS.S - |cal_FF_RAW_spirou:02f10+[...]|On fiber C order 2: S/N= 1232.6 - FF rms=4.76 %
...
HH:MM:SS.S - |cal_FF_RAW_spirou:02f10+[...]|On fiber C order 33: S/N= 1686.9 - FF rms=5.67 %
HH:MM:SS.S - |cal_FF_RAW_spirou:02f10+[...]|On fiber C order 34: S/N= 1574.5 - FF rms=8.17 %
HH:MM:SS.S - |cal_FF_RAW_spirou:02f10+[...]|On fiber C order 35: S/N= 1260.6 - FF rms=8.10 %
HH:MM:SS.S - |cal_FF_RAW_spirou:02f10+[...]|C|Saving blaze spectrum for fiber: C in 20170710
               _dark_flat02f10_blaze_C.fits
HH:MM:SS.S - @ |python warning Line 980 warning reads: Card is too long, comment will be truncated.|
HH:MM:SS.S - |cal_FF_RAW_spirou:02f10+[...]|C|Saving FF spectrum for fiber: C in 20170710
               _dark_flat02f10_flat_C.fits
HH:MM:SS.S - @ |python warning Line 980 warning reads: Card is too long, comment will be truncated.|
HH:MM:SS.S - * |cal_FF_RAW_spirou:02f10+[...]|QUALITY CONTROL SUCCESSFUL - Well Done -
HH:MM:SS.S - * |cal_FF_RAW_spirou:02f10+[...]|Updating Calib Data Base with FLAT_C
HH:MM:SS.S - * |cal_FF_RAW_spirou:02f10+[...]|Updating Calib Data Base with BLAZE_C
HH:MM:SS.S - * |cal_FF_RAW_spirou:02f10+[...]|Recipe cal_FF_RAW_spirou has been successfully completed

```

### 8.5.6 Interactive mode

In interactive mode three figures will also appear (see Figure 8.4).



**Figure 8.4** (a) the full processed image with one order fit highlighted. (b) An extracted over-plotted with the blaze fit. (c) A flattened order.

## 8.6 The `cal_extract` recipes

Extracts orders for specific fibers and files. There are currently three extraction recipes. There is the main extraction recipe (`cal_extract_RAW_spirou`) and two wrapper recipes (`cal_extract_RAW_spirouAB` and `cal_extract_RAW_spirouC`), which push certain options into `cal_extract_RAW_spirou`.

### 8.6.1 The inputs

The input of `cal_extract_RAW_spirou` is as follows:

```
>> cal_extract_RAW_spirou.py night_repository filenames
```

for example

example

```
>> cal_extract_RAW_spirou.py 20170710 fp_fp02a203.fits
```

or

Python/Ipython

```
import cal_extract_RAW_spirou
night_repository = '20170710'
filenames = ['fp_fp02a203.fits']
cal_extract_RAW_spirou.main(night_repository, files=filenames)
```

where 'night\_repository' defines `arg_night_name` and 'filenames' define the list of files in `arg_file_names`. In addition to this one can add optional arguments (and this is the case for the wrapper recipes of `cal_extract_RAW_spirouAB` and `cal_extract_RAW_spirouC`).

All files in filenames must be valid python strings separated by a space (command line) or in a line (python) and should have the following prefixes:

- fp\_fp
- hcne\_dark
- dark\_hcne
- hcne\_hcne
- dark\_dark\_AHC1
- dark\_hctwo
- hctwo\_hctwo
- dark\_dark\_AHC2

#### 8.6.1.1 Optional arguments

By default `cal_extract_RAW_spirou` will extract all fibers defined in `fiber_types` (i.e. 'AB', 'A', 'B' and 'C'). It may be the case that one wishes to extract only one fiber, this can be done by setting the 'fiber\_type' option (when run from python). For example:

Python/Ipypthon

```
import cal_extract_RAW_spirou
night_repository = '20170710'
filenames = ['fp_fp02a203.fits']
cal_DARK_spirou.main(night_repository, filenames, fiber_type='A')
```

where 'fiber\_type' must be a valid python string and defined in [fiber\\_types](#). One can also overwrite any other variable that is (or even is not) defined in any of the constant files (or run time) by simply adding it as an optional argument in the python function call:

Python/Ipypthon

```
import cal_extract_RAW_spirou
night_repository = '20170710'
filenames = ['fp_fp02a203.fits', 'fp_fp03a203.fits', 'fp_fp04a203.fits']
kwargs = dict(parameter1='This', parameter2='That')
cal_DARK_spirou.main(night_repository, filenames, fiber_type='A', **kwargs)
```

**Note:** This will extract fiber 'A' and also set the values `parameter1='This'` and `parameter2='That'` in the main constant parameter dictionary.

This is the case for the two wrapper recipes ([cal\\_extract\\_RAW\\_spirouAB](#) and [cal\\_extract\\_RAW\\_spirouC](#)) which add some specific keywords that are used to individually extract fibers 'AB' and 'C' respectively. The two calls to the main extraction code are shown below but can be called from the console or python as with all other recipes.

```
>> cal_extract_RAW_spirouAB.py night_repository filenames
>> cal_extract_RAW_spirouC.py night_repository filenames
```

for example

example

```
>> cal_extract_RAW_spirouAB.py 20170710 fp_fp02a203.fits fp_fp03a203.fits fp_fp04a203.fits
>> cal_extract_RAW_spirouC.py 20170710 fp_fp02a203.fits fp_fp03a203.fits fp_fp04a203.fits
```

or

Python/Ipypthon

```
import cal_extract_RAW_spirouAB
import cal_extract_RAW_spirouC
night_repository = '20170710'
filenames = ['fp_fp02a203.fits']
# extract fiber AB
cal_extract_RAW_spirouAB.main(night_repository, files=filenames)
# extract fiber C
cal_extract_RAW_spirouC.main(night_repository, files=filenames)
```

as mentioned above this can also be done in python just by adding additional arguments to [cal\\_extract\\_RAW\\_spirou](#):

Python/Ipynb

```
import cal_extract_RAW_spirou
night_repository = '20170710'
filenames = ['fp_fp02a203.fits', 'fp_fp03a203.fits', 'fp_fp04a203.fits']
# extract fiber AB (for all extraction types)
cal_extract_RAW_spirou.main(night_repository, files=filenames, fiber_type='AB',
                             ic_extract_type='all', ic_ext_sigdet=-1)
# extract fiber C (for all extraction types)
cal_extract_RAW_spirou.main(night_repository, files=filenames, fiber_type='C',
                             ic_extract_type='all', ic_ext_sigdet=-1)
```

**Note:** Here we set the optional arguments `ic_extract_type='all'`, `ic_ext_sigdet=-1`. `ic_extract_type` defines which type of extraction should be used (simple, tilt, weigh, tiltweight, all) and `ic_ext_sigdet` manually sets the extraction sigdet (-1 sets it to the value from the HEADER else it is defined in `constants_SPIROU_H4RG.py`).

The above python code is exactly what `cal_extract_RAW_spirouAB` and `cal_extract_RAW_spirouC` do by default.

### 8.6.2 The outputs

The outputs of `cal_extract_RAW_spirou` depend on the extraction type (`ic_extract_type`).

- e2ds in form:

```
{reduced_dir}/{date prefix}_{file}_e2ds_{fiber}.fits
```

- simple in form:

```
{reduced_dir}/{date prefix}_{file}_e2ds_{fiber}_simple.fits
```

**Note:** Only if `ic_extract_type` is 'all'

- tilt in form:

```
{reduced_dir}/{date prefix}_{file}_e2ds_{fiber}_tilt.fits
```

**Note:** Only if `ic_extract_type` is 'all'

- tiltweight in form:

```
{reduced_dir}/{date prefix}_{file}_e2ds_{fiber}_tiltweight.fits
```

**Note:** Only if `ic_extract_type` is 'all'

- tiltweight2 in form:

```
{reduced_dir}/{date prefix}_{file}_e2ds_{fiber}_tiltweight2.fits
```

**Note:** Only if `ic_extract_type` is 'all'

- weight in form:

```
{reduced_dir}/{date prefix}_{file}_e2ds_{fiber}_weight.fits
```

**Note:** Only if `ic_extract_type` is 'all'

where 'date prefix' is constructed from `arg_night_name` and the file name is the first file in `arg_file_names`. for example for `reduced_dir='/drs/data/reduced/20170710'` and `arg_file_names=['fp_fp02a203.fits']` and, `fiber_type='all'` the output files would be:

- `/drs/data/reduced/20170710/fp_fp02a203_e2ds_AB.fits`
- `/drs/data/reduced/20170710/fp_fp02a203_e2ds_A.fits`
- `/drs/data/reduced/20170710/fp_fp02a203_e2ds_B.fits`
- `/drs/data/reduced/20170710/fp_fp02a203_e2ds_C.fits`

or if `ic_extract_type='all'` and `fiber_type='AB'` the output files would be:

- `/drs/data/reduced/20170710/fp_fp02a203_e2ds_AB.fits`
- `/drs/data/reduced/20170710/fp_fp02a203_e2ds_AB_simple.fits`
- `/drs/data/reduced/20170710/fp_fp02a203_e2ds_AB_tilt.fits`
- `/drs/data/reduced/20170710/fp_fp02a203_e2ds_AB_tiltweight.fits`
- `/drs/data/reduced/20170710/fp_fp02a203_e2ds_AB_tiltweight2.fits`
- `/drs/data/reduced/20170710/fp_fp02a203_e2ds_AB_weight.fits`

### 8.6.3 Summary of procedure

1. adds all files together (if more than one)
2. corrects for darks
3. resizes the image
4. checks for saturation
5. possible background subtraction?
6. extracts orders (depending on `ic_extract_type`)
  - without tilt/weight Fortran
  - without tilt/weight python
  - with tilt (no weight)

- with tilt and weight
- with weight (no tilt)

7. saves extraction to e2ds file(s)

### 8.6.4 Quality Control

There is currently one quality control check for `cal_extract_RAW_spirou`

- Too much flux in the image:

$$\text{maximum signal} > \text{qc\_max\_signal} * \text{nbframes} \quad (8.13)$$

**Note:** This check does not currently lead to a failed run and all files are processed as passing quality checks

### 8.6.5 Example working run

An example run where everything worked is below:

example

```
>> cal_extract_RAW_spirou.py 20170710 fp_fp02a203.fits
```

```
HH:MM:SS.S - || *****
HH:MM:SS.S - || * SPIROU @(#) Geneva Observatory (VERSION)
HH:MM:SS.S - || *****
HH:MM:SS.S - ||(dir_data_raw)      DRS_DATA_RAW=/drs/data/raw
HH:MM:SS.S - ||(dir_data_reduc)    DRS_DATA_REduc=/drs/data/reduced
HH:MM:SS.S - ||(dir_calib_db)     DRS_CALIB_DB=/drs/data/calibDB
HH:MM:SS.S - ||(dir_data_msg)    DRS_DATA_MSG=/drs/data/msg
HH:MM:SS.S - ||(print_level)     PRINT_LEVEL=all          %(error/warning/info/all)
HH:MM:SS.S - ||(log_level)       LOG_LEVEL=all            %(error/warning/info/all)
HH:MM:SS.S - ||(plot_graph)      DRS_PLOT=1              %(def/undef/trigger)
HH:MM:SS.S - ||(used_date)       DRS_USED_DATE=undefined
HH:MM:SS.S - ||(working_dir)     DRS_DATA_WORKING=/drs/data/tmp
HH:MM:SS.S - ||                  DRS_INTERACTIVE is not set, running on-line mode
HH:MM:SS.S - ||                  DRS_DEBUG is set, debug mode level:1
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|Now running : cal_extract_RAW_spirou on file(s):
              fp_fp02a203.fits
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|On directory /drs/data/raw/20170710
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|ICDP_NAME loaded from: /scratch/Projects/spirou_py3/
              spirou_py3/INTRoot/config/constants_SPIROU.py
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|Calibration file: 20170710_flat_flat02f10_badpixel.fits
              already exists - not copied
...
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|Calibration file: 2017-10-11_21-32-17
              _hcone_hcone02c406_wave_C.fits already exists - not copied
HH:MM:SS.S - * |cal_extract_RAW_spirou:2a203|Now processing Image TYPE UNKNOWN with
              cal_extract_RAW_spirou recipe
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|Reading Image /drs/data/raw/20170710/fp_fp02a203.fits
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|Image 2048 x 2048 loaded
```



```

HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|Doing Dark Correction using /drs/data/calibDB/20170710
               _dark_dark02d406.fits
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|Image format changed to 2035x1930
HH:MM:SS.S - * |cal_extract_RAW_spirou:2a203|Nb dead pixels = 568485 / 14.47 %
HH:MM:SS.S - * |cal_extract_RAW_spirou:2a203|Maximum average flux/pixel in the spectrum: 109726.7 [ADU
               ]
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|Reading localization parameters of Fiber AB
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203AB|Reading order profile of Fiber AB
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|On fiber AB order 0: S/N= 352.4
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|On fiber AB order 1: S/N= 398.4
...
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|On fiber AB order 34: S/N= 138.8
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|On fiber AB order 35: S/N= 47.8
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|Saving E2DS spectrum of Fiber AB in fp_fp02a203_e2ds_AB.
               fits
HH:MM:SS.S - @ |python warning Line 980  warning reads: Card is too long, comment will be truncated.|
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|Reading localization parameters of Fiber A
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203A|Reading order profile of Fiber A
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|On fiber A order 0: S/N= 210.2
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|On fiber A order 1: S/N= 237.4
...
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|On fiber A order 34: S/N= 114.3
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|On fiber A order 35: S/N= 33.8
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|Saving E2DS spectrum of Fiber A in fp_fp02a203_e2ds_A.
               fits
HH:MM:SS.S - @ |python warning Line 980  warning reads: Card is too long, comment will be truncated.|
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|Reading localization parameters of Fiber B
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203B|Reading order profile of Fiber B
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|On fiber B order 0: S/N= 286.8
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|On fiber B order 1: S/N= 324.4
...
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|On fiber B order 34: S/N= 87.2
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|On fiber B order 35: S/N= 36.1
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|Saving E2DS spectrum of Fiber B in fp_fp02a203_e2ds_B.
               fits
HH:MM:SS.S - @ |python warning Line 980  warning reads: Card is too long, comment will be truncated.|
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|Reading localization parameters of Fiber C
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203C|Reading order profile of Fiber C
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|On fiber C order 0: S/N= 376.6
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|On fiber C order 1: S/N= 424.3
...
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|On fiber C order 34: S/N= 252.7
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|On fiber C order 35: S/N= 130.0
HH:MM:SS.S - |cal_extract_RAW_spirou:2a203|Saving E2DS spectrum of Fiber C in fp_fp02a203_e2ds_C.
               fits
HH:MM:SS.S - @ |python warning Line 980  warning reads: Card is too long, comment will be truncated.|
HH:MM:SS.S - * |cal_extract_RAW_spirou:2a203|Too much flux in the image (max authorized=65500)
HH:MM:SS.S - * |cal_extract_RAW_spirou:2a203|QUALITY CONTROL SUCCESSFUL - Well Done -
HH:MM:SS.S - * |cal_extract_RAW_spirou:2a203|Recipe cal_extract_RAW_spirou has been successfully
               complited

```

## 8.7 The cal\_DRIFT recipes

There are currently three different drift recipes: `cal_DRIFT_RAW_spirou`, `cal_DRIFT_E2DS_spirou` and `cal_DRIFTPEAK_E2DS_spirou`. The `cal_DRIFT_E2DS_spirou` and `cal_DRIFTPEAK_E2DS_spirou` recipes are the primary drift code recipes and `cal_DRIFT_RAW_spirou` is an older version where spectra are re-extracted.

### 8.7.1 The inputs

#### 8.7.1.1 cal\_DRIFT\_E2DS\_spirou and cal\_DRIFTPEAK\_E2DS\_spirou

The input of `cal_DRIFT_E2DS_spirou` and `cal_DRIFTPEAK_E2DS_spirou` are as follows:

```
>> cal_DRIFT_E2DS_spirou.py night_repository referencece_file
>> cal_DRIFTPEAK_E2DS_spirou.py night_repository referencece_file
```

for example

```
example
>> cal_DRIFT_E2DS_spirou.py 20170710 fp_fp02a203_e2ds_AB.fits
>> cal_DRIFTPEAK_E2DS_spirou.py 20170710 fp_fp02a203_e2ds_AB.fits
```

or

```
Python/Ipypthon
import cal_DRIFT_E2DS_spirou
import cal_DRIFTPEAK_E2DS_Spirou
night_repository = '20170710'
reffilename = 'fp_fp02a203_e2ds_AB.fits'
cal_DRIFT_E2DS_spirou.main(night_repository, reffile=reffilename)
cal_DRIFTPEAK_E2DS_spirou.main(night_repository, reffile=reffilename)
```

where 'night\_repository' defines arg\_night\_name and 'reffilename' define the file to use as the reference spectrum. The reference file must be a valid python string and must have the following prefixes:

- fp\_fp

and must contain the fiber type (i.e. 'AB' or 'A' or 'C').

#### 8.7.1.2 cal\_DRIFT\_RAW\_spirou

The input of `cal_DRIFT_RAW_spirou` is as follows:

```
>> cal_DRIFT_RAW_spirou.py night_repository files
```

for example

```
example
>> cal_DRIFT_RAW_spirou.py 20170710 fp_fp02a203.fits
```

or

Python/Ipypthon

```
import cal_DRIFT_RAW_spirou
night_repository = '20170710'
filenames = ['fp_fp02a203.fits']
cal_DRIFT_RAW_spirou.main(night_repository, files=filenames)
```

where 'night\_repository' defines arg\_night\_name and 'filenames' define the list of files in arg\_file\_names. All files in filenames must be valid python strings separated by a space (command line) or in a line (python) and must have the following prefixes:

- fp\_fp

**Note:** `cal_DRIFT_RAW_spirou` can also take an addition argument. By default it will extract fiber 'AB', but this can be changed if using python by specifying the 'fiber' keyword, for example:

Python/Ipypthon

```
import cal_DRIFT_RAW_spirou
night_repository = '20170710'
filenames = ['fp_fp02a203.fits']
cal_DRIFT_RAW_spirou.main(night_repository, files=filenames, fiber='A')
```

## 8.7.2 The outputs

### 8.7.2.1 cal\_DRIFT\_E2DS\_spirou

The outputs of `cal_DRIFT_E2DS_spirou` is as follows:

- driftfits\_e2ds in form:

```
{reduced_dir}/{date prefix}_{file}_drift_{fiber}.fits
```

- drifttblfilename\_e2ds in form:

```
{reduced_dir}/{date prefix}_{file}_drift_{fiber}.tbl
```

where 'date prefix' is constructed from arg\_night\_name and the file name is the 'reference filename'. for example for reduced\_dir = '/drs/data/reduced/20170710', reffile = 'fp\_fp02a203\_e2ds\_AB.fits' and fiber='AB' the output files would be:

- /drs/data/reduced/20170710/fp\_fp02a203\_e2ds\_AB\_drift\_AB.fits
- /drs/data/reduced/20170710/fp\_fp02a203\_e2ds\_AB\_drift\_AB.tbl

### 8.7.2.2 cal\_DRIFTPEAK\_E2DS\_spirou

The outputs of `cal_DRIFTPEAK_E2DS_spirou` is as follows:

- driftfits\_peak\_e2ds in form:

```
{reduced_dir}/{date prefix}_{file}_driftnew_{fiber}.fits
```

- `drifttblfilename_peak_e2ds` in form:

```
{reduced_dir}/{date prefix}_{file}_driftnew_{fiber}.tbl
```

where ‘date prefix’ is constructed from `arg_night_name` and the file name is the ‘reference filename’. for example for `reduced_dir = '/drs/data/reduced/20170710'`, `reffile = 'fp_fp02a203_e2ds_AB.fits'` and `fiber='AB'` the output files would be:

- `/drs/data/reduced/20170710/fp_fp02a203_e2ds_AB_driftnew_AB.fits`
- `/drs/data/reduced/20170710/fp_fp02a203_e2ds_AB_driftnew_AB.tbl`

### 8.7.2.3 cal\_DRIFT\_RAW\_spirou

The outputs of `cal_DRIFT_RAW_spirou` are as follows:

- `driftfits_raw` in form:

```
{reduced_dir}/{date prefix}_{file}_drift_{fiber}.fits
```

where ‘date prefix’ is constructed from `arg_night_name` and the file name is the first file in `arg_file_names`. for example for `reduced_dir = '/drs/data/reduced/20170710'`, `arg_file_names = ['fp_fp02a203.fits']` and `fiber='AB'` the output files would be:

- `/drs/data/reduced/20170710/fp_fp02a203_e2ds_AB_drift_AB.fits`

## 8.7.3 Summary of procedure

### 8.7.3.1 cal\_DRIFT\_E2DS\_spirou

1. first file is reference image (must be an E2DS file) extracted using one of the `cal_extract_RAW` recipes
2. loops around all other ‘\*\_e2ds\_{fiber}.fits’ files in directory
3. calculates photon noise uncertainty and estimated RV uncertainty on spectrum
  - uses wave file
4. calculates RV drift and mean RV drift between reference (mean of files) and other ‘fp\_fp’ files
5. saves drift values to file

### 8.7.3.2 cal\_DRIFTPEAK\_E2DS\_spirou

1. first file is reference image
2. resizes the image
3. background correction
4. Identifies FP peaks in reference file
5. Creates a reference ASCII file that contains the positions of the FP peaks
6. Removes lines with suspicious widths
7. loops around all other ‘\*\_e2ds\_{fiber}.fits’ files

8. Gets the centroid of all peaks using Gaussian fitting
9. Performs a Pearson R test to look for issues with extraction and/or illumination
10. Performs sigma clipping on measured drift
11. Saves drifts to file

### 8.7.3.3 cal\_DRIFT\_RAW\_spirou

1. first file is reference image
2. resizes the image
3. extracts with weight (no tilt)
4. loops around all other 'fp\_fp' files in directory
5. calculates photon noise uncertainty and estimated RV uncertainty on spectrum
  - uses wave file
6. calculates RV drift and mean RV drift between reference (mean of files) and other 'fp\_fp' files
7. saves drift values to file

## 8.7.4 Example working run

### 8.7.4.1 cal\_DRIFT\_E2DS\_spirou

An example run where everything worked is below:

example

```
>> cal_DRIFT_E2DS_spirou.py 20170710 fp_fp02a203_e2ds_AB.fits
```

```
HH:MM:SS.S - || *****
HH:MM:SS.S - || * SPIROU /Q(##) Geneva Observatory (0.1.022)
HH:MM:SS.S - || *****
HH:MM:SS.S - ||(dir_data_raw)      DRS_DATA_RAW=/drs/data/raw
HH:MM:SS.S - ||(dir_data_reduc)    DRS_DATA_REduc=/drs/data/reduced
HH:MM:SS.S - ||(dir_calib_db)     DRS_CALIB_DB=/drs/data/calibDB
HH:MM:SS.S - ||(dir_data_msg)    DRS_DATA_MSG=/drs/data/msg
HH:MM:SS.S - ||(print_level)     PRINT_LEVEL=all          %(error/warning/info/all)
HH:MM:SS.S - ||(log_level)       LOG_LEVEL=all            %(error/warning/info/all)
HH:MM:SS.S - ||(plot_graph)      DRS_PLOT=1              %(def/undef/trigger)
HH:MM:SS.S - ||(used_date)       DRS_USED_DATE=undefined
HH:MM:SS.S - ||(working_dir)     DRS_DATA_WORKING=/drs/data/tmp
HH:MM:SS.S - ||                  DRS_INTERACTIVE is not set, running on-line mode
HH:MM:SS.S - ||                  DRS_DEBUG is set, debug mode level:1
HH:MM:SS.S - |cal_DRIFT_E2DS_spirou|Now running : cal_DRIFT_E2DS_spirou with:
HH:MM:SS.S - |cal_DRIFT_E2DS_spirou|      -- reffile=fp_fp02a203_e2ds_AB.fits
HH:MM:SS.S - |cal_DRIFT_E2DS_spirou|ICDP_NAME loaded from: /scratch/Projects/spirou_py3/spirou_py3/
          INTROOT/config/constants_SPIROU.py
HH:MM:SS.S - |cal_DRIFT_E2DS_spirou|Calibration file: 20170710_flat_flat02f10_badpixel.fits already
          exists - not copied
HH:MM:SS.S - |cal_DRIFT_E2DS_spirou|Calibration file: 20170710_flat_dark02f10_blaze_AB.fits already
          exists - not copied
```

```

HH:MM:SS.S - |cal_DRIFT_E2DS_spirou|Calibration file: 20170710_dark_flat02f10_blaze_C.fits already
exists - not copied
HH:MM:SS.S - |cal_DRIFT_E2DS_spirou|Calibration file: 20170710_dark_dark02d406.fits already exists -
not copied
HH:MM:SS.S - |cal_DRIFT_E2DS_spirou|Calibration file: 20170710_flat_dark02f10_flat_AB.fits already
exists - not copied
HH:MM:SS.S - |cal_DRIFT_E2DS_spirou|Calibration file: 20170710_dark_flat02f10_flat_C.fits already
exists - not copied
HH:MM:SS.S - |cal_DRIFT_E2DS_spirou|Calibration file: 20170710_flat_dark02f10_loco_AB.fits already
exists - not copied
HH:MM:SS.S - |cal_DRIFT_E2DS_spirou|Calibration file: 20170710_dark_flat02f10_loco_C.fits already
exists - not copied
HH:MM:SS.S - |cal_DRIFT_E2DS_spirou|Calibration file: 20170710_flat_dark02f10_order_profile_AB.fits
already exists - not copied
HH:MM:SS.S - |cal_DRIFT_E2DS_spirou|Calibration file: 20170710_dark_flat02f10_order_profile_C.fits
already exists - not copied
HH:MM:SS.S - |cal_DRIFT_E2DS_spirou|Calibration file: 20170710_fp_fp02a203_tilt.fits already exists
- not copied
HH:MM:SS.S - |cal_DRIFT_E2DS_spirou|Calibration file: spirou_wave_ini3.fits already exists - not
copied
HH:MM:SS.S - |cal_DRIFT_E2DS_spirou|Calibration file: 2017-10-11_21-32-17_hcone_hcone02c406_wave_AB.
fits already exists - not copied
HH:MM:SS.S - |cal_DRIFT_E2DS_spirou|Calibration file: spirou_wave_ini3.fits already exists - not
copied
HH:MM:SS.S - |cal_DRIFT_E2DS_spirou|Calibration file: 2017-10-11_21-32-17_hcone_hcone02c406_wave_C.
fits already exists - not copied
HH:MM:SS.S - * |cal_DRIFT_E2DS_spirou|Now processing Image TYPE DRIFT with cal_DRIFT_E2DS_spirou
recipe
HH:MM:SS.S - |cal_DRIFT_E2DS_spirou|Reading File: /drs/data/reduced/20170710/fp_fp02a203_e2ds_AB.
fits
HH:MM:SS.S - * |cal_DRIFT_E2DS_spirou|On fiber AB estimated RV uncertainty on spectrum is 0.025 m/s
HH:MM:SS.S - * |cal_DRIFT_E2DS_spirou|Number of fp_fp files found on directory = 2
HH:MM:SS.S - |cal_DRIFT_E2DS_spirou|Reading file fp_fp03a203_e2ds_AB.fits
HH:MM:SS.S - |cal_DRIFT_E2DS_spirou|Time from ref=0.09 h - Drift mean= -2.92 +- 0.036 m/s - Flux
ratio= 0.99 - Nb Cmsic= 391
HH:MM:SS.S - |cal_DRIFT_E2DS_spirou|Reading file fp_fp04a203_e2ds_AB.fits
HH:MM:SS.S - |cal_DRIFT_E2DS_spirou|Time from ref=0.18 h - Drift mean= 10.22 +- 0.036 m/s - Flux
ratio= 0.98 - Nb Cmsic= 346
HH:MM:SS.S - |cal_DRIFT_E2DS_spirou|Total drift Peak-to-Peak=13.142 m/s RMS=6.571 m/s in 0.18 hour
HH:MM:SS.S - |cal_DRIFT_E2DS_spirou|Saving drift values of Fiber AB in fp_fp02a203_e2ds_AB_drift_AB.
fits
HH:MM:SS.S - |cal_DRIFT_E2DS_spirou|AB|Average Drift saved in fp_fp02a203_e2ds_AB_drift_AB.tbl Saved
HH:MM:SS.S - * |cal_DRIFT_E2DS_spirou|Recipe cal_DRIFT_E2DS_spirou has been successfully completed

```

#### 8.7.4.2 cal\_DRIFTPEAK\_E2DS\_spirou

An example run where everything worked is below:

example

```
>> cal_DRIFTPEAK_E2DS_spirou.py 20170710 fp_fp02a203_e2ds_AB.fits
```

```

HH:MM:SS.S - || *****
HH:MM:SS.S - || * SPIROU @(#) Geneva Observatory (VERSION)

```

```

HH:MM:SS.S - || *****
HH:MM:SS.S - ||(dir_data_raw)      DRS_DATA_RAW=/drs/data/raw
HH:MM:SS.S - ||(dir_data_reduc)   DRS_DATA_REDUC=/drs/data/reduced
HH:MM:SS.S - ||(dir_calib_db)    DRS_CALIB_DB=/drs/data/calibDB
HH:MM:SS.S - ||(dir_data_msg)    DRS_DATA_MSG=/drs/data/msg
HH:MM:SS.S - ||(print_level)     PRINT_LEVEL=all          %(error/warning/info/all)
HH:MM:SS.S - ||(log_level)       LOG_LEVEL=all           %(error/warning/info/all)
HH:MM:SS.S - ||(plot_graph)      DRS_PLOT=1              %(def/undef/trigger)
HH:MM:SS.S - ||(used_date)       DRS_USED_DATE=undefined
HH:MM:SS.S - ||(working_dir)     DRS_DATA_WORKING=/drs/data/tmp
HH:MM:SS.S - ||                  DRS_INTERACTIVE is not set, running on-line mode
HH:MM:SS.S - ||                  DRS_DEBUG is set, debug mode level:1
HH:MM:SS.S - |cal_DRIFTPEAK_E2DS_spirou|Now running : cal_DRIFTPEAK_E2DS_spirou with:
HH:MM:SS.S - |cal_DRIFTPEAK_E2DS_spirou|          -- reffile=fp_fp02a203_e2ds_AB.fits
HH:MM:SS.S - |cal_DRIFTPEAK_E2DS_spirou|ICDP_NAME loaded from: /scratch/Projects/spirou_py3/
              spirou_py3/INTROOT/config/constants_SPIROU.py
HH:MM:SS.S - |cal_DRIFTPEAK_E2DS_spirou|Calibration file: 20170710_flat_flat02f10_badpixel.fits
              already exists - not copied
HH:MM:SS.S - |cal_DRIFTPEAK_E2DS_spirou|Calibration file: 20170710_flat_dark02f10_blaze_AB.fits
              already exists - not copied
...
HH:MM:SS.S - |cal_DRIFTPEAK_E2DS_spirou|Calibration file: spirou_wave_ini3.fits already exists - not
              copied
HH:MM:SS.S - |cal_DRIFTPEAK_E2DS_spirou|Calibration file: 2017-10-11_21-32-17
              _hcone_hcone02c406_wave_C.fits already exists - not copied
HH:MM:SS.S - * |cal_DRIFTPEAK_E2DS_spirou|Now processing Image TYPE DRIFT with
              cal_DRIFTPEAK_E2DS_spirou recipe
HH:MM:SS.S - |cal_DRIFTPEAK_E2DS_spirou|Reading File: /drs/data/reduced/20170710/fp_fp02a203_e2ds_AB
              .fits
HH:MM:SS.S - |cal_DRIFTPEAK_E2DS_spirou|Perform background correction
HH:MM:SS.S - |cal_DRIFTPEAK_E2DS_spirou|Identification of lines in reference file:
              fp_fp02a203_e2ds_AB.fits
HH:MM:SS.S - |cal_DRIFTPEAK_E2DS_spirou|Order 0 : 389 peaks found, 0 peaks rejected
...
HH:MM:SS.S - |cal_DRIFTPEAK_E2DS_spirou|Order 28 : 235 peaks found, 0 peaks rejected
HH:MM:SS.S - @ |python warning Line 779  warning reads: Covariance of the parameters could not be
              estimated|
HH:MM:SS.S - @ |python warning Line 779  warning reads: Covariance of the parameters could not be
              estimated|
HH:MM:SS.S - |cal_DRIFTPEAK_E2DS_spirou|Order 29 : 231 peaks found, 1 peaks rejected
...
HH:MM:SS.S - |cal_DRIFTPEAK_E2DS_spirou|Order 33 : 311 peaks found, 28 peaks rejected
HH:MM:SS.S - @ |python warning Line 779  warning reads: Covariance of the parameters could not be
              estimated|
...
HH:MM:SS.S - @ |python warning Line 779  warning reads: Covariance of the parameters could not be
              estimated|
HH:MM:SS.S - |cal_DRIFTPEAK_E2DS_spirou|Order 34 : 348 peaks found, 24 peaks rejected
HH:MM:SS.S - @ |python warning Line 779  warning reads: Covariance of the parameters could not be
              estimated|
...
HH:MM:SS.S - @ |python warning Line 779  warning reads: Covariance of the parameters could not be
              estimated|
HH:MM:SS.S - |cal_DRIFTPEAK_E2DS_spirou|Order 35 : 483 peaks found, 77 peaks rejected

```

```

HH:MM:SS.S - * |cal_DRIFTPEAK_E2DS_spirou|Total Nb of FP lines found = 11054
HH:MM:SS.S - * |cal_DRIFTPEAK_E2DS_spirou|Nb of lines removed due to suspicious width = 1245
HH:MM:SS.S - * |cal_DRIFTPEAK_E2DS_spirou|Nb of lines removed with no width measurement = 0
HH:MM:SS.S - * |cal_DRIFTPEAK_E2DS_spirou|Number of files found on directory = 2
HH:MM:SS.S - |cal_DRIFTPEAK_E2DS_spirou|Reading file fp_fp03a203_e2ds_AB.fits
HH:MM:SS.S - * |cal_DRIFTPEAK_E2DS_spirou|Time from ref= 0.09 h - Flux Ratio= 1.01 - Drift mean= -2.31
               +- 0.24 m/s
HH:MM:SS.S - |cal_DRIFTPEAK_E2DS_spirou|Reading file fp_fp04a203_e2ds_AB.fits
HH:MM:SS.S - * |cal_DRIFTPEAK_E2DS_spirou|Time from ref= 0.18 h - Flux Ratio= 1.01 - Drift mean= 9.41
               +- 0.26 m/s
HH:MM:SS.S - |cal_DRIFTPEAK_E2DS_spirou|Total drift Peak-to-Peak=11.718 m/s RMS=5.859 m/s in 0.18
               hour
HH:MM:SS.S - |cal_DRIFTPEAK_E2DS_spirou|Saving drift values of Fiber AB in
               fp_fp02a203_e2ds_AB_driftnew_AB.fits
HH:MM:SS.S - |cal_DRIFTPEAK_E2DS_spirouAB|Average Drift saved in fp_fp02a203_e2ds_AB_driftnew_AB.tbl
               Saved
HH:MM:SS.S - * |cal_DRIFTPEAK_E2DS_spirou|Recipe cal_DRIFTPEAK_E2DS_spirou has been successfully
               completed

```

#### 8.7.4.3 cal\_DRIFT\_RAW\_spirou

example

```
>> cal_DRIFT_RAW_spirou.py 20170710 fp_fp02a203.fits
```

```

HH:MM:SS.S - || *****
HH:MM:SS.S - || * SPIROU @(#) Geneva Observatory (VERSION)
HH:MM:SS.S - || *****
HH:MM:SS.S - ||(dir_data_raw)      DRS_DATA_RAW=/drs/data/raw
HH:MM:SS.S - ||(dir_data_reduc)    DRS_DATA_REDUC=/drs/data/reduced
HH:MM:SS.S - ||(dir_calib_db)     DRS_CALIB_DB=/drs/data/calibDB
HH:MM:SS.S - ||(dir_data_msg)    DRS_DATA_MSG=/drs/data/msg
HH:MM:SS.S - ||(print_level)     PRINT_LEVEL=all          %(error/warning/info/all)
HH:MM:SS.S - ||(log_level)      LOG_LEVEL=all           %(error/warning/info/all)
HH:MM:SS.S - ||(plot_graph)     DRS_PLOT=1              %(def/undef/trigger)
HH:MM:SS.S - ||(used_date)      DRS_USED_DATE=undefined
HH:MM:SS.S - ||(working_dir)    DRS_DATA_WORKING=/drs/data/tmp
HH:MM:SS.S - ||                  DRS_INTERACTIVE is not set, running on-line mode
HH:MM:SS.S - ||                  DRS_DEBUG is set, debug mode level:1
HH:MM:SS.S - |cal_DRIFT_RAW_spirou:2a203|Now running : cal_DRIFT_RAW_spirou on file(s): fp_fp02a203.
               fits
HH:MM:SS.S - |cal_DRIFT_RAW_spirou:2a203|On directory /drs/data/raw/20170710
HH:MM:SS.S - |cal_DRIFT_RAW_spirou:2a203|ICDP_NAME loaded from: /scratch/Projects/spirou_py3/
               spirou_py3/INTRoot/config/constants_SPIROU.py
HH:MM:SS.S - * |cal_DRIFT_RAW_spirou:2a203|Correct type of image for Drift (f or p or _ or f or p)
HH:MM:SS.S - |cal_DRIFT_RAW_spirou:2a203|Calibration file: 20170710_flat_flat02f10_badpixel.fits
               already exists - not copied
HH:MM:SS.S - |cal_DRIFT_RAW_spirou:2a203|Calibration file: 20170710_flat_dark02f10_blaze_AB.fits
               already exists - not copied
...
HH:MM:SS.S - |cal_DRIFT_RAW_spirou:2a203|Calibration file: 2017-10-11_21-32-17
               _hcone_hcone02c406_wave_C.fits already exists - not copied

```



```


HH:MM:SS.S - * |cal_DRIFT_RAW_spirou:2a203|Now processing Image TYPE UNKNOWN with cal_DRIFT_RAW_spirou
recipe
HH:MM:SS.S - |cal_DRIFT_RAW_spirou:2a203|Reading Image /drs/data/raw/20170710/fp_fp02a203.fits
HH:MM:SS.S - |cal_DRIFT_RAW_spirou:2a203|Image 2048 x 2048 loaded
HH:MM:SS.S - |cal_DRIFT_RAW_spirou:2a203|Doing Dark Correction using /drs/data/calibDB/20170710/
_dark_dark02d406.fits
HH:MM:SS.S - |cal_DRIFT_RAW_spirou:2a203|Image format changed to 2035x1930
HH:MM:SS.S - * |cal_DRIFT_RAW_spirou:2a203|Nb dead pixels = 568485 / 14.47 %
HH:MM:SS.S - |cal_DRIFT_RAW_spirou:2a203|Reading localization parameters of Fiber AB
HH:MM:SS.S - |cal_DRIFT_RAW_spirou:2a203AB|Reading order profile of Fiber AB
HH:MM:SS.S - |cal_DRIFT_RAW_spirou:2a203|Extraction Reference file /drs/data/raw/20170710/
fp_fp02a203.fits
HH:MM:SS.S - |cal_DRIFT_RAW_spirou:2a203|On fiber AB order 0: S/N= 513.5
HH:MM:SS.S - |cal_DRIFT_RAW_spirou:2a203|On fiber AB order 1: S/N= 561.6
...
HH:MM:SS.S - |cal_DRIFT_RAW_spirou:2a203|On fiber AB order 34: S/N= 283.3
HH:MM:SS.S - |cal_DRIFT_RAW_spirou:2a203|On fiber AB order 35: S/N= 149.9
HH:MM:SS.S - * |cal_DRIFT_RAW_spirou:2a203|On fiber AB estimated RV uncertainty on spectrum is 0.028 m
/s
HH:MM:SS.S - * |cal_DRIFT_RAW_spirou:2a203|Number of fp_fp files found on directory = 2
HH:MM:SS.S - |cal_DRIFT_RAW_spirou:2a203|Reading file fp_fp03a203.fits
HH:MM:SS.S - |cal_DRIFT_RAW_spirou:2a203|Time from ref=0.09 h - Drift mean=2.53 m/s - Flux ratio
=0.99 = Nb Cmsic=1218
HH:MM:SS.S - |cal_DRIFT_RAW_spirou:2a203|Reading file fp_fp04a203.fits
HH:MM:SS.S - |cal_DRIFT_RAW_spirou:2a203|Time from ref=0.18 h - Drift mean=-10.13 m/s - Flux ratio
=0.98 = Nb Cmsic=1246
HH:MM:SS.S - |cal_DRIFT_RAW_spirou:2a203|Total drift Peak-to-Peak=12.596 m/s RMS=6.298 m/s in 0.18
hour
HH:MM:SS.S - |cal_DRIFT_RAW_spirou:2a203|Saving drift values of Fiber AB in fp_fp02a203_drift_AB.
fits
HH:MM:SS.S - @ |python warning Line 980 warning reads: Card is too long, comment will be truncated.|
HH:MM:SS.S - * |cal_DRIFT_RAW_spirou:2a203|Recipe cal_DRIFT_RAW_spirou has been successfully completed

```

### 8.7.5 Interactive mode

#### 8.7.5.1 cal\_DRIFT\_E2DS\_spirou


In interactive mode three figures will also appear (see Figure 8.5).



**Figure 8.5** (a) The extract FP orders for spectral order 20, x-axis is wavelength and y-axis is extract flux. (b) Photon noise uncertainty versus spectral order. (c) Mean drift in m/s against the time from the reference extraction.

### 8.7.5.2 cal\_DRIFTPEAK\_E2DS\_spirou


In interactive mode three figures will also appear (see Figure 8.6).



**Figure 8.6** (a) The extract FP orders for spectral order 20, x-axis is wavelength and y-axis is extract flux. (b) Mean drift in m/s against the time from the reference extraction for the left side of the orders, the right side of the orders and the whole image.

8.7.5.3 cal\_DRIFT\_RAW\_spirou

In interactive mode three figures will also appear (see Figure 8.7).



**Figure 8.7** (a) The extract FP orders for spectral order 20, x-axis is wavelength and y-axis is extract flux. (b) Photon noise uncertainty versus spectral order. (c) Mean drift in m/s against the time from the reference extraction.

## 8.8 The cal\_CCF recipe

Computes the CCF for a specific file using a CCF mask, target RV, CCF width and CCF step.

### 8.8.1 The inputs

The input of `cal_CCF_E2DS_spirou` is as follows:

```
>> cal_CCF_E2DS_spirou.py night_repository e2dsfile mask rv width step
```

for example

example

```
>> cal_CCF_E2DS_spirou.py 20170710 fp_fp02a203_e2ds_AB.fits UrNe.mas 0 10 0.1
```

or

Python/Ipypthon

```
import cal_CCF_E2DS_spirou
filename = 'fp_fp02a203_e2ds_AB.fits'
ccf_mask = 'UrNe.mas'
target_rv = 0.0
ccf_width = 10
ccf_step = 0.1
cal_CCF_E2DS_spirou.main(night_repository, filename=e2dsfile, mask=ccfmask,
                          rv=target_rv, width=ccf_width, step=ccf_step)
```

where:

- 'night\_repository' defines arg\_night\_name
- 'e2dsfile' is the E2DS file to calculate the CCF for
- 'mask' is the name (or full path) of the CCF mask file.
- 'rv' is the target radial velocity (central velocity) in km/s
- 'width' is the CCF width (half range in velocity) in km/s
- 'step' is the CCF step in km/s

Filename suffixes allowed are:

- \*e2ds\_{fiber}.fits

where {fiber} is the fiber type (i.e. 'AB', 'A', 'B' or 'C').

### 8.8.2 The outputs

The outputs of `cal_CCF_E2DS_spirou` are as follows:

- corfile in form:

```
{reduced_dir}/{date prefix}_{file}_ccf_{ccf_mask}.fits
```

- `ccf_table_file` in form:

```
{reduced_dir}/{date prefix}_{file}_ccf_{ccf_mask}.tbl
```

where ‘date prefix’ is constructed from `arg_night_name`, the file name the ‘e2dsfile’, and `{ccf_mask}` is ‘mask’ from the inputs.

for example for `reduced_dir='/drs/data/reduced/20170710'`, `e2dsfile=fp_fp02a203_e2ds_AB.fits`, and `"UrNe.mas"` the output files would be:

- `/drs/data/reduced/20170710/fp_fp02a203_ccf_UrNe_AB.fits`
- `/drs/data/reduced/20170710/fp_fp02a203_ccf_UrNe_AB.tbl`

### 8.8.3 Summary of procedure

1. reads the E2DS file
2. reads the wavelength solution and the flat file
3. corrects for the flat
4. computes photon noise uncertainty
5. gets the CCF mask
6. calculates the CCF for each order
7. fits the CCF for each each
8. averages the CCFs over all orders
9. fits the average CCF over all orders
10. archives the ccf to .fits and .tbl format

### 8.8.4 Example working run

An example run where everything worked is below:


example

```
>> cal_CCF_E2DS_spirou.py 20170710 fp_fp02a203_e2ds_AB.fits UrNe.mas 0 10 0.1
```

```
HH:MM:SS.S - || *****
HH:MM:SS.S - || * SPIROU @(#) Geneva Observatory (VERSION)
HH:MM:SS.S - || *****
HH:MM:SS.S - ||(dir_data_raw)      DRS_DATA_RAW=/drs/data/raw
HH:MM:SS.S - ||(dir_data_reduc)    DRS_DATA_REduc=/drs/data/reduced
HH:MM:SS.S - ||(dir_calib_db)     DRS_CALIB_DB=/drs/data/calibDB
HH:MM:SS.S - ||(dir_data_msg)    DRS_DATA_MSG=/drs/data/msg
HH:MM:SS.S - ||(print_level)    PRINT_LEVEL=all          %(error/warning/info/all)
HH:MM:SS.S - ||(log_level)      LOG_LEVEL=all           %(error/warning/info/all)
HH:MM:SS.S - ||(plot_graph)     DRS_PLOT=1             %(def/undef/trigger)
HH:MM:SS.S - ||(used_date)      DRS_USED_DATE=undefined
HH:MM:SS.S - ||(working_dir)    DRS_DATA_WORKING=/drs/data/tmp
HH:MM:SS.S - ||
HH:MM:SS.S - ||      DRS_INTERACTIVE is not set, running on-line mode
HH:MM:SS.S - ||      DRS_DEBUG is set, debug mode level:1
HH:MM:SS.S - |cal_CCF_E2DS_spirou|Now running : cal_CCF_E2DS_spirou with:
HH:MM:SS.S - |cal_CCF_E2DS_spirou|      -- e2dsfile=fp_fp02a203_e2ds_AB.fits
HH:MM:SS.S - |cal_CCF_E2DS_spirou|      -- ccf_mask=UrNe.mas
HH:MM:SS.S - |cal_CCF_E2DS_spirou|      -- target_rv=0.0
HH:MM:SS.S - |cal_CCF_E2DS_spirou|      -- ccf_width=10.0
HH:MM:SS.S - |cal_CCF_E2DS_spirou|      -- ccf_step=0.1
HH:MM:SS.S - |cal_CCF_E2DS_spirou|ICDP_NAME loaded from: /drs/INTROOT/config/constants_SPIROU.py
HH:MM:SS.S - |cal_CCF_E2DS_spirou|Calibration file: 20170710_flat_flat02f10_badpixel.fits already
exists - not copied
HH:MM:SS.S - |cal_CCF_E2DS_spirou|Calibration file: 20170710_flat_dark02f10_blaze_AB.fits already
exists - not copied
...
HH:MM:SS.S - |cal_CCF_E2DS_spirou|Calibration file: spirou_wave_ini3.fits already exists - not
copied
HH:MM:SS.S - |cal_CCF_E2DS_spirou|Calibration file: 2017-10-11_21-32-17_hcone_hcone02c406_wave_C.
fits already exists - not copied
HH:MM:SS.S - * |cal_CCF_E2DS_spirou|Now processing Image TYPE DRIFT with cal_CCF_E2DS_spirou recipe
HH:MM:SS.S - |cal_CCF_E2DS_spirou|Reading File: /drs/data/reduced/20170710/fp_fp02a203_e2ds_AB.fits
HH:MM:SS.S - |cal_CCF_E2DS_spirou|Reading wavelength solution
HH:MM:SS.S - |cal_CCF_E2DS_spirou|Reading Flat-Field
HH:MM:SS.S - * |cal_CCF_E2DS_spirou|On fiber AB estimated RV uncertainty on spectrum is 0.025 m/s
HH:MM:SS.S - * |cal_CCF_E2DS_spirou|Template used for CCF computation: /drs/INTROOT/SpirouDRS/data/
UrNe.mas
HH:MM:SS.S - |cal_CCF_E2DS_spirou|Using RV template: UrNe.mas (2052 rows)
HH:MM:SS.S - |cal_CCF_E2DS_spirou|Computing CCF at RV= 0.0 [km/s]
HH:MM:SS.S - * |cal_CCF_E2DS_spirou|Correlation: C=2.8[%] RV=-0.55305[km/s] FWHM=4.2613[km/s] maxcpp
=422345.0
HH:MM:SS.S - |cal_CCF_E2DS_spirou|Archiving CCF on file /drs/data/reduced/20170710/
fp_fp02a203_ccf_UrNe_AB.tbl
HH:MM:SS.S - |cal_CCF_E2DS_spirou|Archiving CCF on file fp_fp02a203_ccf_UrNe_AB.fits
HH:MM:SS.S - * |cal_CCF_E2DS_spirou|Recipe cal_CCF_E2DS_spirou has been successfully completed
```

## 8.8.5 Interactive mode

In interactive mode three figures will also appear (see Figure 8.8).



**Figure 8.8** (a) The extract FP orders for spectral order 20, x-axis is wavelength and y-axis is extract flux. (b) Photon noise uncertainty versus spectral order. (c) The normalised CCF averaged across all orders, in red the fit to this CCF.



## 8.9 The validation recipe

This recipe validates that the DRS has been installed correctly and insures that all recipes should run. This is mentioned in Section 3.6.

**Note:** The validation recipe does not protect against incorrect or missing constants and keywords. If all constants are defined as they were when installed and if all paths were set up correctly, then running the validation recipe should be enough to confirm that the DRS installed correctly. Again this does not protect against invalid files and other user inputs.

### 8.9.1 The inputs

The `cal_validate_spirou` recipe requires no input. Thus run the validation as follows:

```
>> cal_validate_spirou.py
```

or

Python/Ipypthon

```
import cal_validate_spirou
cal_validate_spirou.main()
```

One can also define an optional argument to put the validation recipe into debug mode with:

Python/Ipypthon

```
import cal_validate_spirou
cal_validate_spirou.main(DEBUG=1)
```

where a value of True or 1 runs the validation script in debugging mode. This lists all sub-module tests that are performed during the validation and thus allows problems to be identified more easily.

### 8.9.2 The outputs

There are no outputs to `cal_validate_spirou` other than printing to screen and the log file (see Section 8.9.4).

### 8.9.3 Summary of procedure

1. checks core module imports:
  - SpirouDRS
  - SpirouDRS.spirouConfig.spirouConfig
  - SpirouDRS.spirouCore.spirouCore
2. checks that configuration files can be read
3. checks recipe modules
  - SpirouDRS.spirouBACK.spirouBACK
  - SpirouDRS.spirouCDB.spirouCDB
  - SpirouDRS.spirouEXTOR.spirouEXTOR
  - SpirouDRS.spirouFLAT.spirouFLAT

- SpirouDRS.spirouImage.spirouImage
- SpirouDRS.spirouLOCOR.spirouLOCOR
- SpirouDRS.spirouRV.spirouRV
- SpirouDRS.spirouStartup.spirouStartup
- SpirouDRS.spirouTHORCA.spirouTHORCA

4. displays and prints the configuration file paths
5. confirms validation of the DRS installation

### 8.9.4 Example working run

An example run where everything worked is below:

```
>> cal_validate_spirou.py
```

```
*****
*      VALIDATING DRS
*****

1) Running core module tests

2) Running config test

    Testing /drs/INTROOT/config/config.py

        Congratulations all paths in /drs/INTROOT/config/config.py set up correctly.

2) Running sub-module tests

4) Running recipe test

HH:MM:SS.S - || *****
HH:MM:SS.S - || * SPIROU @(#) Geneva Observatory (VERSION)
HH:MM:SS.S - || *****
HH:MM:SS.S - ||(dir_data_raw)      DRS_DATA_RAW=/drs/data/raw
HH:MM:SS.S - ||(dir_data_reduc)    DRS_DATA_REduc=/drs/data/reduced
HH:MM:SS.S - ||(dir_calib_db)     DRS_CALIB_DB=/drs/data/calibDB
HH:MM:SS.S - ||(dir_data_msg)    DRS_DATA_MSG=/drs/data/msg
HH:MM:SS.S - ||(print_level)    PRINT_LEVEL=all          %(error/warning/info/all)
HH:MM:SS.S - ||(log_level)      LOG_LEVEL=all           %(error/warning/info/all)
HH:MM:SS.S - ||(plot_graph)     DRS_PLOT=1              %(def/undef/trigger)
HH:MM:SS.S - ||(used_date)      DRS_USED_DATE=undefined
HH:MM:SS.S - ||(working_dir)    DRS_DATA_WORKING=/drs/data/tmp
HH:MM:SS.S - ||                DRS_INTERACTIVE is not set, running on-line mode
HH:MM:SS.S - ||                DRS_DEBUG is set, debug mode level:1
HH:MM:SS.S - ||
HH:MM:SS.S - ||Validation successful. DRS installed corrected.
```

## 8.10 The cal\_HC recipe

Recipe not yet updated.

## 8.11 The cal\_WAVE recipe

Recipe not yet updated.

## 8.12 The pol\_spirou recipe

Recipe not yet updated.