

**SIEMENS**



[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

A Tim+Dot System  
Data sheet based on **syngo MR E11**

Answers for life.



# MAGNETOM Skyra

Maximize 3T. Every case. Every day.

- Deliver exceptional quality and speed in 3T MRI.
- Go for consistent results, efficiently.
- Expand your MRI services.

MAGNETOM® Skyra is designed to maximize the total power of 3T MRI. To deliver robust image quality and increase productivity by up to 50%<sup>1)</sup>. Consistently. To reach new patient populations and radically improve return on investment. From clinical routine to advanced research, you can count on the latest advances in MRI – MAGNETOM Skyra will transform every part of your day. In every case, the benefits will be nothing less than profound. Maximize 3T. Every case. Every day.

<sup>1)</sup> Data on file; results may vary

# DirectRF® Technology

## General

Tim's new and unique all digital-in/digital-out design integrates all RF transmit and receive components at the magnet

- Optical RF system improves SNR by reducing electrical noise and increasing signal detection
- Digital-in and digital-out design – optical links between magnet and equipment room to achieve high RF stability
- Transmit path is integrated in the magnet housing
- Receive path is integrated in the magnet housing
- Dual-Density Signal Transfer technology enables ultra-high density coil designs by integrating key RF components into the local coil.
- Receiver with high dynamic range without adjustments

## Direct Transmit Technology

Frequency stability (5 min)	$\pm 2 \times 10^{-10}$
Frequency control	32 bits (0.03 Hz)
Phase control	16 bits (0.006 degrees)
Body coil	Integrated whole body no tune transmit/receive coil with 32 rungs Optimized RF efficiency and signal-to-noise ratio (SNR)
Transmitter path	Real-time Feedback loop for unmatched RF stabilization Transmit amplitude 16 bit control 25 ns resolution Gain stability (after first minute) <0.05 dB (1 s) <0.2 dB (5 min)
Transmit amplifier	Extremely compact, water-cooled solid state amplifier, fully integrated at the magnet as part of DirectRF technology Transmit amplifier bandwidth 800 kHz Peak power 37.5 kW

### **TimTX TrueForm**

TimTX TrueForm includes innovative techniques in the RF excitation hardware as well as new application and processing features enabling uniform RF distribution in all body regions. TimTX TrueForm for MAGNETOM Skyra consists of TrueForm excitation, which uses amplitude and phase transmission settings optimized for dedicated body regions. Feeding the 2 ports of the integrated body coil with an optimized weighting yields a homogeneous B1 distribution

TimTX TrueForm is supported by:

- a-SPACE, which is a version of the SPACE sequence. a-SPACE uses composite adiabatic excitation pulses, which are insensitive to B1 spatial variations.
- B1 Filter, which is an adaptive inline image filter that reduces any remnant B1 effects without affecting image contrast.

### **RF Receiver Technology**

The revolutionary Total imaging matrix optimizes coil positioning and virtually eliminates coil changing times. It also features Dual-Density Signal Transfer technology in the local receive coils, which enables the high density design. All local coils are no tune coils. Further Tim 4G features are AutoCoilSelect for dynamic, automatic, or interactive selection of the coil elements within the FoV.

Receive path	Number of coil elements	Up to 204
	Number of independent receiver channels	24 <sup>1)</sup> , 48, 64 <sup>1)</sup> , 128 <sup>1)</sup>
	Quadrature demodulation and filtering	Digital
	Receiver bandwidth	500 Hz – 1 MHz (for each channel)
	Receiver signal resolution	32 bit
	ADC sampling rate	80 MHz
	Preamplifier noise figure	<0.5 dB
	Dynamic range at coil connector (referred to 1 Hz resolution bandwidth)	164 dB instantaneous at receiver 169 dB with automatic gain control at local coil connector

<sup>1)</sup> Optional

# Patient Handling

## General

Tim 4G and DotGO help increase patient comfort and improve workflow efficiency.

- Set up the patient once, no repositioning, no changing of coils needed
- Scan range of 205 cm<sup>1)</sup> allows for whole body examinations with full usage of the surface coils, without the need for patient repositioning
- Ultra-light weight coils
- Imaging with optimized high element surface coil
- Remote table move
- Feet-first examinations for many applications (e.g. cardiac, liver, upper abdomen, pelvis, colonography, body angio) reduces the level of anxiety experienced by highly claustrophobic patients
- AutoPosition for selected exams
- In-room Dot Display: Patient preparation is smooth with all patient data displayed right at the scanner. Dot gives the user advice during the positioning process – very helpful in the case of ECG, for example

## Patient Positioning Aids

Standard set of cushions for comfortable and stable patient positioning together with safety straps.

Additional positioning supports (optional):  
Set of vacuum cushions (large, medium, small)  
with vacuum pump

## Tim Table

Comfortable patient table solution which fits the needs for patients up to 250 kg supporting full weight capacity in vertical and horizontal movement. Integrated coils for fast patient preparation and enhanced user comfort. Scan range up to 205 cm<sup>1)</sup>. Integrated infusion stand.

Max. patient weight for vertical and horizontal table movement	250 kg (550 lbs)
--	------------------

Max. scan range	140 cm, opt. 205 cm <sup>1)</sup>
-----------------	--------------------------------------

User can adjust the table speed with two pre-defined speed mode buttons or accelerate continuously with the wheel on the Dot Control Centers

Vertical table movement	Range	52–102 cm <sup>2)</sup> +13 mm <sup>3)</sup>
----------------------------	-------	---

Speed	60 mm/s; one click table up
-------	--------------------------------

Horizontal table movement	Max. range	2750 mm
---------------------------------	------------	---------

Max. speed	200 mm/s
------------	----------

Position accuracy	±0.5 mm
----------------------	---------

Continuous table movement during scan capable

<sup>1)</sup> Optional with Tim Whole Body Suite

<sup>2)</sup> Including Heightening Kit, if necessary

<sup>3)</sup> Depending on the floor conditions

### **Dot Control Centers**

Two ergonomically designed control units integrated into the front cover on each side of the patient tunnel. Optional 3<sup>rd</sup> Dot Control Center including a Dot Display is available at the rear-end of the system.

- Continuous table movement or two speed predefined levels
- Automatic transfer from any vertical position to home position
- Automatic transfer to isocenter
- Automatic transfer from any horizontal position to home position
- In-bore ventilation (6-step regulation)
- In-bore lighting (6-step regulation)
- Headphone volume adjustment (6-step regulation)
- In room loudspeaker adjustment (6-step regulation)
- Laser light localization
- Start scan
- Alarm off
- Horizontal table movement, lighting adjustments, and ventilation are also possible from the console

### **Dot Display**

Dot Display with user guidance for fast and efficient exam preparation and start of measurement at the scanner. Display of physiological curves and guidance for patient set up of triggering device.

Color LCD Monitor	13.3"; 16 : 10
Horizontal frequency	15.0–80.0 kHz
Vertical frequency	50.0–85.1 kHz
Screen Matrix	1280×800 pixels

## **Physiological Measurement Unit (PMU) – Wireless Physio Control**

Synchronizes the measurement with the physiological cycles (triggering to minimize motion artifacts caused by cardiac and respiratory movements). The physiological curves are visualized at the Dot Display.

Wireless Sensors	Wireless Vector ECG/respiration and pulse sensors for physiologically synchronized imaging, rechargeable battery-powered – for optimized patient handling
Physiological Signals	<ul style="list-style-type: none"><li>• ECG (3 channels)</li><li>• Pulse</li><li>• Respiration</li></ul>
	<b>ECG Triggering:</b> <ul style="list-style-type: none"><li>• Acquisition of multiple slices, e.g. of the heart, at different phases of the cardiac cycle</li><li>• Excellent image quality by synchronizing data acquisition with cardiac motion</li></ul>
	<b>Peripheral PulseTriggering:</b> <ul style="list-style-type: none"><li>• Reduces flow artifacts caused by pulsatile blood flow</li><li>• Excellent image quality by synchronizing data acquisition to the pulsatile blood flow</li></ul>
	<b>Respiratory Triggering:</b> <ul style="list-style-type: none"><li>• Excellent image quality by synchronizing data acquisition with the respiratory motion</li></ul>
	<b>External Triggering :</b> <ul style="list-style-type: none"><li>• Interface for trigger input from external sources (e.g. Patient Monitoring System) inside the examination room</li><li>• Interface for trigger input from external sources (e.g. pulse generator, trigger sources for fMRI) outside the examination room</li><li>• Optical trigger output for fMRI</li></ul>
	Retrospective gating for ECG, peripheral pulse and external trigger input

## **Patient Communication**

Ergonomically designed patient communication unit – may be placed at any convenient location on the workplace table.

- Intercom system incorporating active noise cancellation for improved patient communication
  - Assistance call via squeeze-bulb for the patient
  - Response to the patient's activation of the squeeze-bulb via communication unit
  - Table stop
  - Sequence stop
  - Volume of speaker in control room
  - Volume of speaker and headphones in examination room for voice commands
  - Connection to external audio system
  - Independent volume control of voice and music
  - Pneumatic system of ergonomically designed headphones
  - Loudspeaker
  - Microphone
  - Automatic and freely programmable voice commands for breath-hold examinations
-

# Noise Reduction Features

## General Features

- Acoustically optimized mountings for all components including gradient coil and body coil
- Minimized structure-borne noise transfer to building
- Noise attenuating foam between gradient coil and cover, and between magnet and cover
- Encapsulation of noise producing components

## Gradient

- Special epoxy resin and casting technology for damping vibrations
- Reduction of gradient stray field to decrease eddy currents
- Noise-optimization of the MR system with an acoustically soft but mechanically rigid mounting of the gradient coil inside the magnet
- Force compensation for all axes

## Magnet

- Encapsulation of the entire magnet
- Efficient floor decoupling for reduction of noise transferred to the building
- Noise-optimized cold head

## Body Coil

Material of supporting tube of the body coil is optimized for low vibration and noise

- In order to achieve maximum noise reduction, the body coil tube was extended beyond the gradient coil
- Copper structures are slotted and glued to the tube to reduce high frequency noise
- The Body coil is acoustically decoupled by special suspensions

## "Whisper Mode"

The "Whisper Mode" is a user selectable mode that reduces the max. slew rate and max. amplitude of the gradients and enables very quiet imaging techniques.

## Quiet Suite

A family of sequences for extremely quiet neuro and orthopedic imaging, with up to 97% reduction in sound pressure<sup>1)</sup>:

- QuietX TSE, SE and GRE sequences for T1, T2, DarkFluid and SWI contrasts
- PETRA, a 3D T1-weighted UTE sequence

Quiet Suite sequences employ optimized gradient waveforms to achieve significant noise reductions and smoother, more tolerable sounds with no loss in image quality or substantial increases in scan times. Optimized protocols for the imaging of the brain and large joints are provided.

<sup>1)</sup> Data on file

# Acquisition Parameters

Acquisition Parameters <sup>1)</sup>		
2D	Number of slices	1–128 (steps of 1)
	Slice order	Sequential or interleaved
3D Slabs/Partitions	Number of 3D partitions for matrix 256×256	4–512
	Number of 3D Slabs (3D volumes)	1–128 (steps of 1)
Acquisition Matrix	Frequency encoding (true imaging matrix without interpolation or oversampling)	64–1024 (in steps of 2; sequence dependent)
	Phase encoding	32–1024 (in steps of 1)
Reduced Matrix	Phase resolution (rectangular matrix)	32×n ... n×n (steps of 1)
	Slice resolution (3D volumes)	50–100%
Partial Fourier Imaging	Phase partial Fourier (Half Fourier)	4/8–1 (steps of 1/8)
	Read partial Fourier (asymmetric echo)	Selectable
	Slice partial Fourier (3D volumes)	5/8–1 (steps of 1/8)
Rectangular Field of View	In phase encoding direction	3–100%
Averaging	Number of data acquisitions	1–32 (steps of 1)
	Averaging mode	Short term, Long term (LOTA)
Oversampling	Read oversampling	100% standard
	Phase oversampling	0–100% (steps of 12.5%)
	Slice oversampling (3D volumes)	0–100% (steps of 12.5%)
Interpolation	In plane interpolation	Selectable (factor of 2)
	3D interpolation (3D volumes)	Selectable (up to factor of 2)
Serial Acquisitions	Number of repeated scans	With constant delay times 1–4096  With different delay times 1–65
Swap	Exchange of read-out and phase-encoding direction	Yes
Slice orientation	Slice orientation for 2D and 3D scans	Transverse, sagittal, coronal, oblique, double oblique (steps of 0.1°)
	Multi-slice multi-angle (simultaneously)	Yes

<sup>1)</sup> Combinations of the parameters stated are not always possible; some parameters may depend on optional application packages

# Standard Acquisition and Reconstruction Techniques

## Standard techniques

- True Inversion Recovery to obtain strong T1-weighted contrast
- Dark Blood inversion recovery technique that nulls fluid blood signal
- Saturation Recovery for 2D TurboFLASH, gradient echo, and T1-weighted 3D TurboFLASH with short scan time (e.g. MPRAGE)
- Freely adjustable receiver bandwidth, permitting studies with increased signal-to-noise ratio
- Freely adjustable flip angle. Optimized RF pulses for image contrast enhancement and increased signal-to-noise ratio
- MTC (Magnetization Transfer Contrast). Off-resonance RF pulses to suppress signal from certain tissues, thus enhancing the contrast. Used e.g. in MRA
- Argus viewer for reviewing cine studies
- Report Viewer for DICOM structured reports including report editing
- Dynamic Analysis for addition, subtraction, division, standard deviation, calculations of ADC maps, T1 and T2 values, TTP, t-Test, etc.
- Image Filter
- 3D post-processing MPR, MIP, MinIP, SSD
- Flexible film formats and paper print
- Data storage of images and cine AVI files on CD/DVD with DICOM viewer as the viewing tool
- Selectable centric elliptical phase reordering via the user interface
- Inversion Recovery to nullify the signal of fat, fluid or any other tissue
- Multiple Direction Diffusion Weighting (MDDW) – diffusion tensor imaging measurements can be done with multiple diffusion-weightings and up to 12 directions for generating data sets for diffusion tensor imaging
- WARP – 2D TSE sequence combining optimized high-bandwidth protocols and View Angle Tilting (VAT), tailored to reduce susceptibility artifacts caused by orthopedic MR-Conditional<sup>1)</sup> metal implants.

## Sequences

- |                                  |  |
|----------------------------------|--|
| Spin Echo family<br>of sequences | <ul style="list-style-type: none"><li>• Spin Echo (SE) – Single, Double, and Multi Echo (up to 32 echoes); Inversion Recovery (IR)</li><li>• 2D/3D Turbo Spin Echo (TSE) – Restore technique for shorter TR times while maintaining excellent T2 contrast; TurboIR: Inversion Recovery for STIR, DarkFluid T1 and T2, TrueIR</li><li>• 2D TSE with multiple averages – it is possible to acquire T2-weighted TSE images during shallow breathing in a time efficient manner</li><li>• 2D/3D HASTE (Half-Fourier Acquisition with Single Shot Turbo Spin Echo) – Inversion Recovery for STIR and DarkFluid contrast</li><li>• SPACE for 3D imaging with high isotropic resolution with T1, T2, PD, and DarkFluid Contrast</li><li>• 2D/ Optimized high bandwidth TSE (T1, T2, and PD weighted and STIR) with WARP for the reduction of susceptibility artifacts caused by MR-Conditional metal<sup>1)</sup> implants.</li></ul> |
|----------------------------------|--|

<sup>1)</sup> MR imaging of patients with metallic implants brings specific risks. However, certain implants are approved by the governing regulatory bodies to be MR conditionally safe. For such implants, the previously mentioned warning may not be applicable. Please contact the implant manufacturer for the specific conditional information. The conditions for MR safety are the responsibility of the implant manufacturer, not of Siemens.

### **Sequences (Continued)**

Gradient Echo family of sequences	<ul style="list-style-type: none"><li>• 2D/3D FLASH (spoiled GRE) – dual echo for in-/opposed phase imaging 3D VIBE (Volume Interpolated Breathhold Examination) – quick fat saturation; double echo for in-phase/opposed phase 3D imaging; DynaVIBE: Inline 3D elastic motion correction for multi phase data sets of the abdomen; Inline Breast Evaluation</li><li>• 2D/3D MEDIC (Multi Echo Data Image Combination) for high resolution T2 weighted orthopedic imaging and excellent contrast</li><li>• 2D/3D TurboFLASH – 3D MPRAGE; single shot T1 weighted imaging e.g. for abdominal imaging during free breathing</li><li>• 3D GRE for field mapping</li><li>• 2D/3D FISP (Fast Imaging with Steady State Precession)</li><li>• 2D/3D PSIF – PSIF Diffusion</li><li>• Echo Planar Imaging (EPI) – diffusion-weighted; single shot SE and FID e.g. for BOLD imaging and Perfusion-weighted imaging; 2D/3D Segmented EPI (SE and FID)</li><li>• ce-MRA sequence with Inline subtraction and Inline MIP</li><li>• 2D/3D Time-of-Flight (ToF) Angiography – single slab and multi slab; triggered and segmented</li><li>• 2D/3D Phase Contrast Angiography</li><li>• BEAT Tool – TrueFISP segmented; 2D FLASH segmented; Magnetization-prepared TrueFISP (IR, SR, FS); IR TI scout; Retrogating</li></ul>
TGSE (Turbo Gradient Spin Echo)	Hybrid Turbo Spin Echo / Gradient Echo used primarily for T2-weighted imaging <ul style="list-style-type: none"><li>• Shorter measurement time</li><li>• Decreased RF power deposition</li><li>• Improved visualization of hemorrhage, due to magnetic susceptibility differences</li><li>• High resolution imaging of brain and spine</li></ul>

### **Standard Fat/Water Imaging**

- Fat and Water Saturation. Additional frequency selective RF pulses used to suppress bright signal from fatty tissue. Two selectable modes: weak, strong
- Quick FatSat
- SPAIR: robust fat suppression for body imaging using a frequency selective inversion pulse
- Fat/Water Excitation. Spectral selective RF pulses for exclusive fat/water excitation
- Dixon technique for fat and water separation – available on VIBE and Turbo Spin Echo sequence

### **Standard Flow Artifact Reduction**

- LOTA (Long Term Data Averaging) technique to reduce motion and flow artifact
- Pre-saturation technique. RF saturation pulses to suppress flow and motion artifacts
- Tracking SAT bands maintain constant saturation of venous and/or arterial blood flow, e.g. for 2D/3D sequential MRA
- TONE (Tilted Optimized Non-saturating Excitation). Variable excitation flip angle to compensate inflow saturation effects in 3D MRA. TONE pulse selectable depending on the desired flow direction and speed
- GMR (Gradient Motion Rephasing). Sequences with additional bipolar gradient pulses, permitting effective reduction of flow artifacts

## Standard Scan Time Reduction

Elliptical scanning reduces scan time for 3D imaging

iPAT – integrated Parallel Acquisition Technique high-performance and flexible Parallel Imaging with integrated AutoCalibration

Two algorithms – mSENSE and GRAPPA – for maximum quality for all applications

iPAT is compatible with all relevant sequence techniques (e.g. SE, TSE, SPACE, MEDIC, TIRM DarkFluid, HASTE, EPI, MPRAGE, 3D VIBE, FLASH, TrueFISP, TurboFLASH, FLASH Phase Contrast, etc)

iPAT is compatible with all multi-element coils, as well as coil combinations

Tim Assistant facilitates optimized iPAT settings. Higher speed and temporal resolution can be used for:

- Improved image resolution
- Improved image quality due to reduced artifacts

T-PAT with mSENSE and GRAPPA for advanced parallel imaging provides fast high-resolution dynamic imaging

3 different calibration techniques can be used:

- AutoCalibration with an integrated reference (calibration) scan to additionally save on total scan time
- TurboCalibration uses a separate measurement directly before the actual measurement. Images measured using TurboCalibration are characterized by reduced PAT artifacts.
- T-PAT and PAT averaging for motion artifact suppression using Self-Calibration

iPAT<sup>2</sup>

Multidirectional parallel imaging for faster 3D imaging

The effective PAT factor can be maximized, and PAT applications are extended. Typical clinical applications is ultrafast isotropic T1-weighted 3D imaging of the head

A new iPAT<sup>2</sup> sequence technique named CAIPIRINHA (Controlled Aliasing In Parallel Imaging Results IN Higher Acceleration) has been added. It can be applied to volumetric 3D imaging e.g. in the abdominal region.

### **Standard Motion Correction**

BLADE	<ul style="list-style-type: none"><li>• Improves image quality by minimizing and correcting for the effects of motion during an MR sequence acquisition. e.g. head, spine, orthopedic imaging and the abdomen</li><li>• Motion insensitive Turbo Spin Echo sequence</li><li>• Can be used with all coils and in all planes</li><li>• Supports T2-weighted, T1-weighted, STIR, and DarkFluid protocols</li><li>• Simultaneous in-plane motion correction for arbitrary slice orientations</li><li>• Versatile sequence e.g. supporting iPAT with GRAPPA, Restore pulses and supports respiratory triggered imaging of the abdomen using 2D PACE</li></ul>
1D PACE (Prospective Acquisition CorREction)	<ul style="list-style-type: none"><li>• Quick and easy acquisition control for free breathing examinations, e.g. for cardiac imaging</li></ul>
2D PACE Precise Motion Correction	<ul style="list-style-type: none"><li>• Detects and corrects respiratory motion of the heart, liver, etc. for free breathing high resolution 2D and 3D examinations</li><li>• Increased image quality</li><li>• Improved security in the diagnosis of diseases in moving organs and precise slice registration for multi breath-hold studies</li><li>• Data acquisition during free breathing for high resolution 2D and 3D examinations</li><li>• Eliminates the need for respiratory belt</li><li>• PAT averaging for motion artifact suppression using Self-Calibration</li></ul>

### **Standard Susceptibility Artifact Reduction**

WARP	<ul style="list-style-type: none"><li>• 2D TSE sequence combining optimized high-bandwidth protocols and View Angle Tilting (VAT), tailored to reduce susceptibility artifacts caused by orthopedic MR-Conditional<sup>1)</sup> metal implants.</li><li>• This helps in the evaluation of soft tissue in proximity of the implant</li><li>• Available protocols include T1-weighted, T2-weighted, proton density and STIR contrast</li></ul>
------	--

### **Standard Workflow Enhancements**

AutoCoilDetect	Detects the position and orientation of coils automatically. Shows coils in the user interface right within the graphical slice positioning.
AutoCoilSelect	Automatic detection and selection of all coil elements in the active Field-of-View.
syngo Scan Assistant	Shows parameter constraints and provides possible solutions.
scan@center	Automated movement of table so that the scan is performed in the magnet isocenter – can be activated or deactivated by the user.

<sup>1)</sup> MR imaging of patients with metallic implants brings specific risks. However, certain implants are approved by the governing regulatory bodies to be MR conditionally safe. For such implants, the previously mentioned warning may not be applicable. Please contact the implant manufacturer for the specific conditional information. The conditions for MR safety are the responsibility of the implant manufacturer, not of Siemens.

### **Standard Workflow Enhancements (Continued)**

AutoVoiceCommands	These multi-language automatic voice commands during the scan assist the user in providing optimal timing of breathing, scanning, and contrast media injection.
Phoenix and PhoenixZIP	Exchange of protocol data (e.g. via Internet) by drag & drop clinical images. PhoenixZIP allows transfer of whole measurement programs.
Online Help Functions	Context sensitive and quick resource for questions about software operation or MR physics.
DirectConnect	Cable-less direct connection for Head/Neck 20, Spine 32, Foot/Ankle 16 <sup>1)</sup> .
SlideConnect	SlideConnect cable connectors can be securely plugged-in with one hand only.
Inline Technology – Processing Instead of Post-processing	Inline Technology helps to streamline the clinical workflow by automating common post-processing steps before image viewing. See the clinical results immediately. Inline functionality is user-configurable. Examples: <ul style="list-style-type: none"><li>• Automatic subtraction of images, e.g. pre- and post-contrast enhancements</li><li>• MIP on-the-fly, automatic image subtraction and following MIP in three orthogonal planes</li><li>• Prospective motion correction (1D and 2D PACE) on-the-fly</li><li>• Automatic perfusion<sup>1)</sup> and diffusion maps</li><li>• Automatic composing of multi-step images<sup>1)</sup></li><li>• Automatic on-the-fly calculation of standard deviation, for better differentiation of arterial and venous phases</li><li>• Inline Display automatically shows reconstructed images. It offers immediate access to the results and opens automatically for e.g. interactive real-time scanning or CareBolus examinations</li><li>• Inline Movie automatically starts the cine image display</li></ul>

### **TimCT FastView**

TimCT FastView is the “one go” localizer for the whole body or large body regions such as the whole spine or the whole abdomen. It acquires the complete extended Field of View in one volume with isotropic resolution. Transverse, coronal and sagittal reformats of the volume are calculated Inline and displayed for planning subsequent exams.

- Inline reconstruction of the localizer images during the scan
- Localizing images in the three planes over the maximum Field of View available for subsequent planning in all orientations.
- TimCT FastView runs without laser light positioning to further streamline the workflow for several indications


<sup>1)</sup> Optional

# Tim Application Suite

The Tim Application Suite offers a complete range of clinically optimized examinations for all regions. The Tim Application Suite – allowing excellent head-to-toe imaging – is provided standard on MAGNETOM Skyra.

- Neuro Suite
- Angio Suite
- Cardiac Suite
- Body Suite
- Onco Suite
- Ortho Suite
- Breast Suite
- Scientific Suite
- Pediatric Suite<sup>1)</sup>

## Neuro Suite

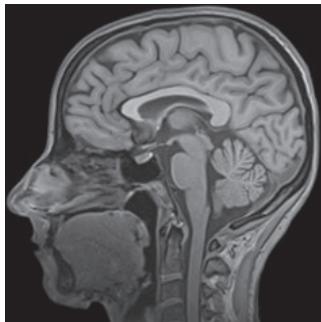

Comprehensive head and spine examinations can be performed with dedicated programs. High resolution protocols and fast protocols for uncooperative patients are provided. The Neuro Suite also includes protocols for e.g., diffusion imaging, or fMRI.

<sup>1)</sup> MR scanning has not been established as safe for imaging fetuses and infants under two years of age. The responsible physician must evaluate the benefit of the MRI examination in comparison to other imaging procedures.

## **Neuro Suite (Continued)**

General features	<ul style="list-style-type: none"><li>• Fast 2D imaging with SE, TSE, GRE protocols for high-resolution imaging in all orientations and all contrasts</li><li>• BLADE motion correction for TSE imaging in all orientations and contrasts</li><li>• EPI sequences and protocols for diffusion imaging, perfusion imaging, and fMRI for advanced neuro applications. Diffusion-weighted imaging is possible with up to 16 b-values in the orthogonal directions</li><li>• 3D TOF for non-contrast-enhanced angiography</li><li>• 3D isotropic resolution volume imaging using T1 3D MPRAGE/3D FLASH, SPACE DarkFluid, T1 and T2 SPACE and 3D TSE T2-weighted high resolution 3D Restore protocols optimized for inner ear examinations</li><li>• Double Inversion Recovery 3D protocols (DIR SPACE) with two user-selectable inversion pulses for the simultaneous suppression of e.g. cerebro-spinal fluid and white matter</li><li>• MP2RAGE (Magnetization Prepared 2 Rapid Acquisition Gradient Echoes) provides homogeneous tissue contrast for segmentation and applications such as voxel-based morphometry. In combination with MapIt<sup>1)</sup>, it also provides T1 mapping functionality</li><li>• Whole-spine protocols in multiple steps with software controlled table movement</li><li>• 2D and 3D MEDIC protocols for T2-weighted imaging, particularly for C-spine examinations in axial orientation where reproducibility is difficult due to CSF pulsations and blood flow artifacts</li><li>• 3D Myelo with 3D HASTE and 3D True-FISP for anatomical details</li><li>• Spine diffusion protocols with PSIF sequence</li><li>• Precision filter for high spatial accuracy e.g. for neuro intra-operative imaging and stereotactic planning</li><li>• 3D CISS (Constructive Interference in Steady State) for excellent visualization of fine structures such as cranial nerves. High resolution imaging of inner ear and spine</li><li>• TGSE sequence used primarily for T2-weighted imaging for shorter measurement time, decreased RF power deposition, improved visualization of hemorrhage, and high resolution imaging of brain and spine</li><li>• AutoAlign Head LS providing a fast, easy, standardized, and reproducible patient scanning supporting reading by delivering a higher and more standardized image quality</li></ul>
------------------	---

<sup>1)</sup> Option

## Angio Suite



Excellent MR Angiography can be performed to visualize arteries and veins  
• 3D MRA protocols for e.g. single step, dynamic, peripheral, whole body MRA with short TR and TE. The strong gradients make it possible to separate the arterial phase from the venous phase  
• Dynamic MRA for 3D imaging over time


### Non-contrast MRA and venography

- 2D or 3D Time-of-Flight (ToF) protocols for MRA for the Circle of Willis, carotids, neck vessels, and breath-hold protocols for abdominal vessels
- Triggered 2D ToF sequences for non-contrast MRA, particularly in the abdomen and the extremities
- 2D/3D Phase-Contrast
- MR venography with 2D/3D Time-of-Flight (ToF) and Phase-Contrast
- TONE (Tilted Optimized Non-saturating Excitation) and MTC (Magnetization Transfer Contrast) techniques for improved Contrast-to-Noise Ratio (CNR)

### Image processing tools

- MPR, MIP, MinIP, and 3D SSD
- Inline MIP for immediate results
- Inline subtraction
- Inline standard deviation maps of Phase-Contrast measurements for delineation of arteries and veins

## Cardiac Suite

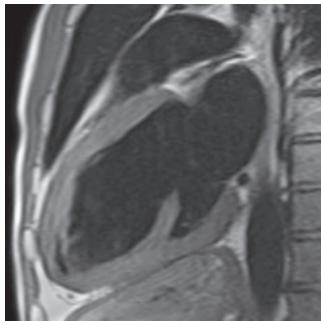

The cardiac suite covers comprehensive 2D routine cardiac applications, ranging from morphology and ventricular function to tissue characterization. Featuring BEAT 2D in conjunction with iPAT and T-PAT techniques

### Cardiac views

- Fast acquisition of the basic cardiac orientations for further examination planning
- Cardiac scouting provides users with a step-by-step procedure for the visualization and planning of typical cardiac views, e.g. based on TrueFISP or Dark Blood TurboFLASH: short-axis, 4-chamber, and 2-chamber views

### BEAT

- Unique tool for fast and easy cardiovascular MR imaging
- E.g. 1 click change from FLASH to TrueFISP for easy contrast optimization
- 1-click to switch arrhythmia rejection on/off
- 1-click change from Cartesian to radial sampling to increase effective image resolution (e.g. in pediatric patients)<sup>1)</sup> and avoid folding artifacts in large patients

### Visualization of structural cardiovascular pathologies with CMR – BEAT


- Breath-hold and free breathing techniques for strong contrast between the blood and vascular structures. Dark Blood TSE and HASTE imaging are available for the structural evaluation of the cardiothoracic anatomy, including vessels or heart valves. Cine techniques (FLASH & TrueFISP) for high-resolution valve evaluation
- Multiple contrasts such as T1- and T2-weighted imaging
- Dark-blood TSE with motion compensation for high-quality vessel wall imaging in small or large vessels

<sup>1)</sup> MR scanning has not been established as safe for imaging fetuses and infants under two years of age.  
The responsible physician must evaluate the benefit of the MRI examination in comparison to other imaging procedures.

### **Cardiac Suite (Continued)**

Tools for rapid evaluation of left or right ventricular function:	<ul style="list-style-type: none"><li>• Acquisition of a stack of short-axis slices (standard segmented FLASH, or advanced segmented TrueFISP)</li><li>• Automatic adjustment of the acquisition window to the current heart rate</li><li>• Use of the Inline ECG for graphical ECG triggering setup</li><li>• Retrospective gating with cine sequences (TrueFISP, FLASH)</li><li>• Protocols for whole-heart coverage</li><li>• iPAT integration for highest temporal and spatial resolution</li><li>• Real-time imaging in case the patient is not able to hold his breath</li></ul>
Imaging and tissue characterization with BEAT Protocols for high-contrast and high-resolution tissue characterization	<ul style="list-style-type: none"><li>• Protocols for stress and rest imaging with TrueFISP or TurboFLASH contrast support the acquisition of multiple slices with high resolution and arbitrarily adjustable slice orientation for each slice</li><li>• T-PAT with mSENSE and GRAPPA for advanced parallel imaging provides fast high-resolution dynamic imaging</li><li>• Segmented IR TrueFISP/FLASH with TI scout for optimization of tissue contrast</li><li>• Advanced tissue characterization with 2D phase-sensitive IR (PSIR) sequences TrueFISP and FLASH contrast. Magnitude and phase-sensitive images with one acquisition</li><li>• Simple: no adjustment of inversion time (TI) necessary with PSIR technique</li><li>• Ungated single-shot PSIR imaging for tissue characterization under difficult conditions: free-breathing technique that can be applied even in case of arrhythmia</li></ul>

## Body Suite

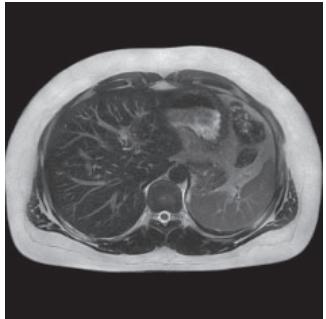

The Body Suite is dedicated to clinical body applications. Ultra-fast high resolution 2D and 3D protocols are provided for abdomen, pelvis, MR Colonography, MRCP, dynamic kidney, and MR Urography applications. 2D PACE technique makes body imaging easy, allowing for multi-breath-hold examinations as well as free breathing during the scans. Motion artifacts are greatly reduced with 2D PACE Inline technology.

This package includes:

- Free breathing 2D PACE applications with 2D/3D HASTE (RESTORE) and 2D/3D TSE (RESTORE) – it is possible to use a phase navigator, which measures respiratory induced off-resonance effects. The positioning can be done automatically for most protocols.
- Optimized fast single shot HASTE protocols and high-resolution 3D RESTORE protocols based on SPACE and TSE for MRCP and MR Urography examinations
- REVEAL: diffusion imaging for abdomen and whole body exams. In protocols with multiple b-values, a different number of averages may be specified for each b-value.

---

### Abdomen

2D:

- T1 (FLASH) breath-hold scans with and without FatSat (SPAIR, Quick FatSat, in-/opp-phase)
- T2 (HASTE, TSE/BLADE, EPI) breath-hold scans with and without FatSat (SPAIR, FatSat, STIR)
- 2D TSE with multiple averages – it is possible to acquire T2-weighted TSE images during shallow breathing in a time efficient manner
- T1 (TFL) triggered scans (2D PACE free breathing) in-/opp-phase
- T2 (HASTE, TSE/BLADE, EPI) triggered scans (2D PACE free breathing) with and without FatSat (SPAIR, FatSat, STIR) as well as HASTE- and TSE-multi-echo
- Optimized fast single shot HASTE protocols and high-resolution 3D RESTORE protocols based on SPACE and TSE for MRCP and MR urography examinations

3D:

- Dixon (VIBE 2pt-Dixon) breath-hold scans that provide the following contrasts: in-phase, opposed phase, fat and water image
- Dynamic (VIBE and Quick-FatSat) protocols with Inline motion correction for visualization of focal lesions with high spatial and temporal resolution
- Colonography dark lumen with T1-weighted VIBE

---

### Pelvis

- High-resolution T1, T2 pelvic imaging (prostate, cervix)
- Isotropic T2 SPACE 3D protocols for tumor search in the pelvis
- Dynamic volume examinations with 3D VIBE

## Onco Suite



MR imaging provides excellent soft-tissue differentiation, multi-planar capabilities, and the possibility of selectively suppressing specific tissue, e.g. fat or water. The Onco Suite features a collection of sequences as well as protocols and evaluation tools that may be used for a detailed assessment of a variety of oncological conditions.

### General features

- STIR TSE, HASTE, and FLASH in-phase and opposed-phase protocols for highly sensitive visualization of metastases
- Dynamic imaging protocols for assessment of the kinetic behavior as an aid for lesion visualization and characterization
- Quantitative evaluation and fast analysis of the data with colorized Wash-in, Wash-out, Time-To-Peak, Positive-Enhancement-Integral, MIP-time and combination maps with Inline technology or for offline calculation
- Display and analysis of the temporal behavior in selected regions of interest with the included MeanCurve postprocessing application. This includes the capability of using additional datasets as a guide for defining regions of interest even faster and easier than before
- REVEAL: diffusion imaging for liver and whole body exams. In protocols with multiple b-values, a different number of averages may be specified for each b-value.

### Prostate protocols

- Dedicated prostate protocols for detection, localization, and staging of tumors and recurrences
- REVEAL (diffusion-weighted imaging)
- Protocols with high temporal resolution allow time course evaluation based on pharmacokinetic modeling
- Prostate spectroscopy (3D CSI) with up to 8 sat bands supports tumor diagnosis<sup>1)</sup>

<sup>1)</sup> Option

## Ortho Suite



The Ortho Suite is a comprehensive collection of protocols for joint imaging including the spine. Also in case of tumors, infections, or vascular necrosis, a large amount of additional information can be acquired using the protocols provided as standard in this suite.

### General features

- 2D TSE protocols for PD, T1, and T2-weighted contrast with high in-plane resolution and thin slices
- 3D MEDIC, 3D TrueFISP protocols with water excitation for T2-weighted imaging with high in-plane resolution and thin slices
- High resolution 3D VIBE protocols for MR Arthrography (knee, shoulder, and hip)
- 3D MEDIC, 3D TrueFISP, 3D VIBE protocols with Water Excitation having high isotropic resolution optimized for 3D post-processing
- T1, T2, and PD SPACE, 3D imaging with high isotropic resolution optimized for post-processing
- Whole-spine, single-step, and multi-step protocols
- Excellent fat suppression in off-center positions, e.g. in the shoulder due to high magnet homogeneity
- Dynamic TMJ protocol (different joint positions)
- Multi Echo SE sequence with up to 32 echoes for T2 mapping
- High resolution 3D DESS (Double Echo Steady State): T2/T1-weighted imaging for excellent fluid-cartilage differentiation
- 2 point Dixon technique for fat and water separation – Turbo Spin Echo sequence
- WARP – 2D TSE sequence combining optimized high-bandwidth protocols and View Angle Tilting (VAT), tailored to reduce susceptibility artifacts caused by orthopedic MR-Conditional<sup>1)</sup> metal implants. This helps in the evaluation of soft tissue in proximity of the implants. Available protocols include T1-weighted, T2-weighted, proton density and STIR contrast.

<sup>1)</sup> MR imaging of patients with metallic implants brings specific risks. However, certain implants are approved by the governing regulatory bodies to be MR conditionally safe. For such implants, the previously mentioned warning may not be applicable. Please contact the implant manufacturer for the specific conditional information. The conditions for MR safety are the responsibility of the implant manufacturer, not of Siemens.

## Breast Suite



MR imaging provides excellent tissue contrast that may be useful in the evaluation of the breasts. Extremely high spatial and temporal resolution can be achieved in very short measuring times by using iPAT with GRAPPA. Excellent soft tissue differentiation, customized protocols (e.g. with fat saturation or water excitation or silicone excitation), as well as flexible multiplanar visualization allow for fast, simple and reproducible evaluation of MR breast examinations.

### General features

This package includes:

- High-resolution 2D protocols for morphology evaluation
- High-resolution 3D protocols covering both breasts simultaneously
- Protocols to support interventions (fine needle and vacuum biopsies, wire localization)
- Protocols for evaluating breasts with silicone implants
- Automatic and manual frequency adjustment, taking into account the silicone signal
- Detection of the silicone signal either to suppress the silicone signal, if the surrounding tissue is to be evaluated, or to suppress the tissue signal in order to detect an implant leakage
- SPAIR – robust fat sat (robust fat suppression using an adiabatic frequency selective inversion pulse)
- DIXON – 2-point Dixon with 3D VIBE; the following contrasts can be obtained: in-phase, opposed phase, fat and water image
- iPAT with GRAPPA for maximum resolution in short time
- iPAT Extension that allows state-of-the-art sagittal breast imaging
- Inline subtraction and MIP display
- Offline subtraction, MPR and MIP display
- REVEAL: diffusion imaging for breast exams. In protocols with multiple b-values, a different number of averages may be specified for each b-value.

### Including RADIANT (ultra-sound like reconstruction around the nipple)

Siemens Technique: VIEWS  
(Volume Imaging with Enhanced Water Signal)

- Bilateral – both breasts are examined simultaneously
- Axial – the milk ducts are directly displayed
- Fat-saturated or water-excited – fat complicates clinical evaluation and is suppressed
- Near-isotropic 3D measurement – the same voxel size in all three directions for reconstruction in any slice direction
- Submillimeter voxel – highest resolution for precise evaluation

## **Scientific Suite**

The Scientific Suite supports scientific users by providing easy access to application-specific data for further processing and advanced image calculus.

### General features

- Support of USB Memory sticks
- Access to file system via a secure and comfortable File Browser
- Anonymization of patient data
- Easy creation of AVIs and screen snapshots to include in presentations or teaching videos
- Export of tables, statistics and signal time courses to communal exchange formats like e.g. tabulated text files (MeanCurve, Spectroscopy evaluation, DTI evaluation)
- Advanced image calculus including T2 and T1 time calculation, addition, subtraction, multiplication, division, log, and integration of images

## **Pediatric Suite<sup>1)</sup>**

Tissue relaxation times in pediatrics are very different compared to those of adults. The reasons for these differences are: developing tissues, body size, faster heart rates, and compliance with breath-hold commands. Protocols can be easily adapted for imaging infants.

<sup>1)</sup> MR scanning has not been established as safe for imaging fetuses and infants under two years of age.  
The responsible physician must evaluate the benefit of the MRI examination in comparison to other imaging procedures.

# DotGO. Go for consistent results, efficiently

In 2009, Siemens set the benchmark in MR scanning and productivity by introducing Dot. Easily adapt to the patient's condition or clinical question, consistently achieve reproducible, high-quality results, and consequently reduce exam times and the number of rescans. From 2014 on, the newest generation of Dot – DotGO – is also setting the standard in protocol configuration. For true flexibility, consistency and efficiency in every aspect of MRI.

## **Flexibility. Intuitive protocol management.**

One central user-interface to configure any protocol and flexibly create your exam strategies. Intuitive, fast functionality results in 80%<sup>1)</sup> improved usability in exam configuration. DotGO empowers you to provide your MRI expertise for the entire department and to define a higher standard of care for more patients and referrers.

## **Consistency. Quality results for each exam.**

Every patient is different. Every referrer's and radiologist's requirement is different. But your results need to be consistent and of high quality. Your daily schedule has to be met. DotGO partners you in meeting all of these different needs with dedicated functionality for the clinical question at hand.

## **Efficiency. Stay on time with less than 1 minute exam-time variation.<sup>2)</sup>**

Time, quality and costs define the efficiency of your MRI exams. DotGO enables scheduling to be more predictable by reducing exam-time variations to less than a minute<sup>2)</sup>. Also time-consuming software interaction is reduced dramatically (by up to 46%<sup>3)</sup>). Standardized procedures support quality results for each exam and help to reduce rescans. All in all turnaround time to the referrer is quicker, quality higher, and MRI more efficient.

<sup>1)</sup> Compared to MR protocol configuration without Dot Cockpit, Usability Study, 2013

<sup>2)</sup> Zhongshang Hospital Fudan University, Fudan, CN, Abdomen Dot Engine Workflow Study

<sup>3)</sup> University Hospital Essen, GER, Brain Dot Engine Workflow Study

# Dot Cockpit

## Intuitive protocol management ...

by providing unprecedented flexibility in MRI configuration.

At the heart of this new flexibility is the Dot Cockpit. It is the central tool to continuously build your knowledge into standardized exam strategies and to make them available for every technician in your MRI department. Whether you are using a Dot engine or not, the Dot Cockpit is the new starting point for every exam.

MRI flexibility from the start:

- One central user-interface for every protocol
- Fast and intuitive protocol configuration
- User-friendly functionalities like drag & drop, AutoSearch
- Exam strategies created with one click
- Multiple strategies in one protocol
- Change protocols on the fly
- Changes in one sequence applied to all protocols – if you want to

Take the lead in defining the standard of MRI in your institution!

### Dot Cockpit



Designed to realize the full potential of the Dot engines. The new Dot Cockpit is your central interface for all protocol management tasks. This includes flexible configuration of all Dot engines, according to your standards of care. In the following, we introduce the most important features of the new Dot Cockpit.

**Dot Cockpit (Continued)**

Configure all protocols from one central interface	The Dot Cockpit enables you to configure MRI protocols – whether it is a Dot or non-Dot protocol – and all Dot engines.
Dot Explorer and Program Editor on one page	The Dot Cockpit offers two tasks: Dot Explorer and Program Editor. In the Dot Explorer, you browse through and organize your protocols, in the Program Editor, you modify them.
A new structogram view	With the new structogram view of the Dot Cockpit, you can see the whole exam workflow, the different strategies, decisions, the branches and protocols clearly layed out on the screen.
Dynamic search delivers highlighted results	In the Dot Explorer, searching for protocols is very quick. Just type in your search query, and results are highlighted instantly.
Editing protocols instantly	In order to modify a protocol opened in the Dot Explorer, you can immediately switch to the Program Editor with one click.
Adding a new Strategy	In the Program Editor, just drag & drop or click on the strategy button in the sidebar, and a new strategy is added to your exam workflow. This step automatically creates a new Dot engine.
Drag & drop from the sidebar	In the Program Editor, you can add protocols to a strategy by drag & drop from the sidebar.
User-friendly toolbar	Use the toolbar for opening and saving of programs, for Copy, Paste, Undo, Redo – in the same way as you are used to in Office programs.

## Brain Dot Engine



The Brain Dot Engine simplifies general brain examinations with guided and automated workflows customized to your standards of care. The Brain Dot Engine supports the user to achieve reproducible image quality with increased ease of use and time efficient exams.

### Patient View

Within the Patient View the user can easily tailor examinations to an individual patient. Dot Exam Strategies allow you to choose the most appropriate strategy with one mouse click, the complete scan setup is then automatically prepared.

### Guidance View

Step-by-step user guidance is seamlessly integrated. Sample images and guidance text are displayed for each individual step of the scanning workflow to ensure reproducible scanning. Both images and text are easily configurable by the user.

### Parameter View

The new streamlined Parameter View displays a user-defined subset of parameters which are available for manual protocol optimization. If desired, the user can switch to the conventional – fully loaded – parameter view at any time.

### AutoPosition

The head of the patient is automatically placed at the isocenter without any laser marking required.

### AutoAlign Head LS

Automated, positioning and alignment of slice groups to the anatomy, relying on multiple anatomical landmarks. Provides fast, easy, and reproducible patient scanning and facilitates the reading by consistently delivering high image quality with a standardized slice orientation, both for follow-ups and across patients. Besides basic brain positioning, AutoAlign Head LS computes reference position for several other brain structures such as the inner ear, the orbits and the optic nerve. It also delivers robust and consistent results independently of patient age, head position, disease or existing lesions.

### AutoCoverage

Maximizes the speed of the examination by automatically setting the number of slices and the FoV to fully cover the brain. This is performed based on the information delivered by AutoAlign, eliminating manual setting and the scanning of unnecessary slices.

### **Brain Dot Engine (Continued)**

Dot Exam Strategies	Examinations can be easily personalized to the individual patient condition and clinical need. The Brain Dot Engine comes with the following predefined examination strategies, which the user can select according to patient conditions or change at any time during the workflow, when conditions change: <ul style="list-style-type: none"><li>• Standard: Standard examination with 2D protocols</li><li>• Resolution focus: Examination with 3D protocols (with e.g. SPACE) for detailed views</li><li>• Speed focus: Examination with fast 2D protocols (with e.g. HASTE) for further speeding up the exam</li><li>• Motion-insensitive: Examination with BLADE protocols to minimize and correct for the effects of motion automatically</li></ul>
BLADE	Motion insensitive Turbo Spin Echo sequence. Improves image quality by correcting for the effects of motion during an MR acquisition. (Can be used in head, spine, and other body regions).
Rerun	An image inside the examination UI can be selected and a rerun of the corresponding series can be triggered with identical sequences or parameters.
Inline MPRs	Automatic multiplanar reconstruction for 3D datasets. The Multi Planar Reconstruction (MPR) tool can be easily configured to automatically generate any required 2D images from high resolution 3D acquisitions by using the position information from the AutoAlign algorithm.
Inline Diffusion	Automatic calculation of trace-weighted images and ADC maps with Inline Technology.
Customization	The Brain Dot Engine can be easily modified by the user to their individual standard of care. <ul style="list-style-type: none"><li>• Add/remove protocol steps</li><li>• Change guidance content (images and text)</li><li>• Change or add Dot exam strategies</li><li>• Add clinical decision points</li><li>• Add/remove parameters in the parameter viewing card</li><li>• User-defined offsets to the standard positions delivered by AutoAlign</li><li>• Customized inline MPR reconstructions</li></ul>

## Large Joint Dot Engine<sup>1)</sup>



The Large Joint Dot Engine ensures reproducible image quality and streamlines large joint examinations by bundling Knee, Hip and Shoulder Dot Engine. It optimizes image quality of knee, hip and shoulder scans by proposing the most appropriate protocols according to the examination strategy chosen for the specific patient.

The Large Joint Dot Engine features AutoAlign and AutoCoverage for knee, hip and shoulder. The WARP and advanced WARP techniques (including high bandwidth protocols, VAT and SEMAC) provide susceptibility artifact reduction functionality (e.g. from MR-Conditional<sup>2)</sup> metal implants), and include optimized protocols for knee and hip examinations. High resolution 3D imaging programs together with user-configurable automatic Inline MPR (Multi Planar Reconstruction) calculations provide increased efficiency, reproducibility and ease of use.

Patient View	Within the Patient View the user can easily tailor the exam to an individual patient. Dot Exam Strategies can be integrated. With one mouse-click you simply choose the most appropriate scan strategy, and then the queue is automatically loaded and filled with the complete scan setup.
Guidance View	Step-by-step user guidance is seamlessly integrated. Sample images and guidance text are displayed for each individual step of the scanning workflow. Both images and text are easily configurable by the user.
Parameter View	The new streamlined Parameter View displays a user-defined subset of parameters which are available for manual protocol optimization. If desired, the user can switch to the conventional – fully loaded – parameter view at any time.
Dot Exam Strategies	The workflow can be personalized to the individual patient condition and clinical need. The Large Joint Dot Engine comes with the following predefined strategies, which the user can select according to patient conditions or change at any time during the workflow, when conditions change: <ul style="list-style-type: none"><li>• Standard: Achieve highest image quality in a reasonable scan time with 2D and 3D protocols</li><li>• Speed focus: Examine patients quickly with protocols being accelerated to the maximal extend</li><li>• Motion Insensitive (BLADE): Compensate for the effects of motion with motion insensitive BLADE protocols</li><li>• High Bandwidth (WARP): Optimized strategy for the reduction of susceptibility artifacts.</li></ul>

<sup>1)</sup> Optional

<sup>2)</sup> MR imaging of patients with metallic implants brings specific risks. However, certain implants are approved by the governing regulatory bodies to be MR conditionally safe. For such implants, the previously mentioned warning may not be applicable. Please contact the implant manufacturer for the specific conditional information. The conditions for MR safety are the responsibility of the implant manufacturer, not of Siemens.

### **Large Joint Dot Engine (Continued)**

AutoAlign	Automated, localizer based positioning and alignment of slice groups to the anatomy, relying on anatomical landmarks. Providing fast, easy, and reproducible patient scanning and supporting the reading by consistently delivering high image quality with a standardized slice orientation.
AutoCoverage	Maximizes the speed of the examination by automatically setting the number of slices and the FoV to fully cover knee, hip or shoulder anatomy. This is performed based on the information delivered by AutoAlign, eliminating manual setting and the scanning of unnecessary slices. This feature is configurable.
Inline MPRs	Automatic multiplanar reconstruction for 3D datasets. The Multi Planar Reconstruction (MPR) tool uses the position information from the AutoAlign algorithm and can be easily configured to automatically generate any required 2D images from high resolution 3D acquisitions.
WARP Susceptibility Artifact Reduction	WARP and advanced WARP (SEMAC) integrates different techniques tailored to reduce susceptibility artifacts caused by orthopedic MR-Conditional <sup>1)</sup> metal implants. 2D TSE sequence combining optimized high-bandwidth protocols and View Angle Tilting (VAT) technique, helps in evaluation of soft tissue in proximity of the implant. SEMAC (Slice Encoding for Metal Artifact Correction) is a technique to correct through-plane distortions by means of additional phase encoding in slice direction. It is especially useful in the case of hip and knee joint replacements. Available protocols can be found in the library.
Customization	The Large Joint Dot Engine can be modified by the user to their individual standard of care. <ul style="list-style-type: none"><li>• Add/remove protocol steps</li><li>• Change guidance content (images and text)</li><li>• Change or add Dot exam strategies</li><li>• Add clinical decision points</li><li>• Add/remove parameters in the parameter viewing card</li></ul>

<sup>1)</sup> MR imaging of patients with metallic implants brings specific risks. However, certain implants are approved by the governing regulatory bodies to be MR conditionally safe. For such implants, the previously mentioned warning may not be applicable. Please contact the implant manufacturer for the specific conditional information. The conditions for MR safety are the responsibility of the implant manufacturer, not of Siemens.

## Abdomen Dot Engine<sup>1)</sup>



The Abdomen Dot Engine offers standardized, efficient, and comprehensive workflows for the upper abdomen with excellent image quality. The workflow covers liver, biliary and pancreatic system and, if slightly adapted, kidneys as well. The workflow is prepared for easy reading and reporting together with syngo.via.

### Patient View

Within the Patient View the user can easily tailor the exam to each individual patient. Several pre-defined Dot Exam Strategies can be integrated. The user just selects the appropriate strategy with one click, and the queue and the complete scan set-up are automatically updated. Furthermore protocols tailored for use of contrast media can be integrated.

### Guidance View

Step-by-step user guidance is seamlessly integrated. Sample images and guidance text are displayed for each individual step of the scanning workflow. Both images and text are easily configurable by the user

### Parameter View

The new streamlined Parameter View displays the parameters that are really needed for the scan set-up. If desired, the user can switch to the conventional – fully loaded – parameter view at any time.

### AutoPosition

After registration the patient is positioned automatically at the optimal scanning position.

### Automatic sequence scaling

According to physiological characteristic (AutoFoV, AutoNavigator, breath-hold adaptations)

### AutoNavigator

Automatic breathing pattern detection and scaling of triggered scans

### AutoFoV (automatic Field of View calculation)

Based on the localizer images the optimal FoV is automatically estimated. In case the patient moves during the examination, this step can be repeated at any time.

<sup>1)</sup> Optional

### **Abdomen Dot Engine (Continued)**

Dot Exam Strategies	The workflow can be personalized to the individual patient's condition and clinical need. The following predefined strategies are included. They can be changed at any time during the workflow: <ul style="list-style-type: none"><li>• Breathhold (fast with robust image quality)</li><li>• Respiratory synchronized (using PACE triggering, high image resolution)</li><li>• Motion-insensitive (fast, using BLADE and PACE triggering)</li></ul>
Dot Decisions	Your decisions can be seamlessly integrated into the scanning workflow. The user just selects the queue, and the appropriate protocol or set of protocols are automatically added. For the abdomen MRCP and Diffusion decision points are offered.
MRCP decision point	Dot provides comprehensive guidance, including positioning help. MRCP is measured and Inline Radial Ranges are generated in-line.
Timeline monitoring	For best overview of multi-phase breath-hold examinations. The contrast media enhancement curve is visualized.
Automatic Timing	Liver dynamics is done using the care bolus approach. Auto Bolus Detection enables the system to monitor the arrival of contrast agent in a user defined ROI. When "Auto Bolus Detection" is enabled, Auto ROI can be enabled in the patient view, which allows the system to perform an automatic ROI positioning on the descending aorta at the level of the diaphragm. The ROI positioning can be confirmed and adjusted by the user.
Bolus Timing	An alternative way of performing liver dynamics. The optimal time window for data acquisition is derived by the system after the application of a test bolus. Visual guidance and interactive evaluation during the setup provide ease-of-use.
AutoVoiceCommands	Seamlessly integrated into the scanning workflow. The system plays them automatically at the desired time point. This assists the user in providing the optimal timing of scanning, breathing and contrast media. The user can monitor which breathhold or pauses are actually played, and can add pauses between the automatic breath hold commands if necessary.
Inline Subtraction	Within the contrast-enhanced abdomen exam, multiple phases are acquired: native, arterial phase, portal-venous phase, and late-phase. The scanner automatically subtracts the native measurement from the arterial, portal-venous and late phase.
Abdomen Dot Library	StarVIBE <sup>1)</sup> and TWIST-VIBE <sup>1)</sup> protocols will be part of the Abdomen Dot library.

<sup>1)</sup> Optional

### **Abdomen Dot Engine (Continued)**

Inline Registration	For best visualization of potential lesions the system can be set to automatically perform a registration/alignment of the anatomy for the different dynamic phases. The importance of registration/correction can be seen when examining nodular enhancing pathologies.
Customization	Existing Dot Engines can be adapted by the user to their individual standard of care. <ul style="list-style-type: none"><li>• Add/remove protocol steps</li><li>• Change guidance content (images and text)</li><li>• Change or add Dot Exam Strategies and Decision Points</li><li>• Modify the Parameter View</li><li>• Dot Library – alternative protocols with preconfigured add-ins. Only simple drag &amp; drop needed.</li></ul>
LiverLab <sup>1)</sup>	<p>LiverLab is a system guided workflow to examine the hepatic fat and iron status, as part of the Abdomen Dot Engine.</p> <p>Main Features:</p> <p>The inline First look Dixon sequence gives the user a first overview of possible fat and/or iron overload in the whole liver. Based on the resulting images, liver segmentation runs without user interaction.</p> <p>If further evaluation is needed, the user can choose from two methods:</p> <ul style="list-style-type: none"><li>• HISTO is a push-button single breath-hold single voxel spectroscopy method to calculate fat signal fraction as well as water R2.</li><li>• Multi-echo Dixon VIBE is an image based method to calculate maps such as water, fat, fat signal fraction, and R2*.</li></ul>

<sup>1)</sup> Optionally available for Tim [204x48], [204x64], and [204x128] configurations

## TimCT Onco Dot Engine<sup>1)</sup>



TimCT Oncology employs the revolutionary TimCT Continuous Table move technology for large Field of View applications with smooth workflow and excellent image quality. TimCT Oncology is built on Tim technology as well as on a highly advanced patient table with high positioning accuracy and an RF shielded table drive. Simultaneous coverage of a large Field of View using local coils with a high signal-to-noise ratio enables excellent image quality and extremely fast imaging with iPAT.

TimCT Oncology allows a CT-like MR examination:

- Definition of start point and end point of scan area only
- No need to plan in multiple steps
- No need to plan overlapping areas
- No delay, no measurement pauses during table move
- No need for composing

TimCT Onco Dot Engine makes the easy workflow of TimCT even easier by customizable guidance throughout the exam.

### Guidance View

Step-by-step user guidance is seamlessly integrated. Sample images and guidance text are displayed for each individual step of the scanning workflow. Both images and text are easily configurable by the user.

### Parameter View

The new streamlined Parameter View displays the parameters that are really needed for the scan set-up. If desired, the user can switch to the conventional – fully loaded – parameter view at any time.

### iPAT compatibility

Enabled by Tim 4G

### Seamless scanning

Enables high image homogeneity and suppression of boundary artifacts

<sup>1)</sup> Optional; Prerequisite: Abdomen Dot Engine and either Tim[204x48], Tim[204x64], or Tim[204x128], Tim Whole Body Suite

**TimCT Onco Dot Engine (Continued)**

Special features	The possibility of shorter examination times, the BLADE technique and the suppression of boundary artifacts.
Liver dynamics	Key functionalities of the Abdomen Dot Engine are integrated.
Techniques	<p>The protocols are based on axial 2D T1-weighted FLASH- and T2-weighted imaging (TSE with and without BLADE and HASTE). This technique suits best as a complement to the primary tumor diagnosis done in stationary mode (e.g., in the upper abdomen) by providing comprehensive metastasis and lymph node evaluation in the body regions thorax-abdomen-pelvis.</p> <p>The following fat saturation techniques are available:</p> <ul style="list-style-type: none"><li>• T1 FLASH with FatSat, SPAIR or Dixon, 4 contrasts in one scan</li><li>• T2 HASTE with FatSat, SPAIR or Inversion Recovery</li><li>• T2 TSE (with and without BLADE) with FatSat, SPAIR or STIR</li></ul>
Customization	<p>Existing Dot Engines can be adapted by the user to their individual standard of care.</p> <ul style="list-style-type: none"><li>• Add/remove protocol steps</li><li>• Change guidance content (images and text)</li><li>• Change or add Dot Exam Strategies and Decision Points</li><li>• Modify the Parameter View</li><li>• Dot library (alternative sequences with preconfigured add-ins)</li></ul>

## Angio Dot Engine<sup>1)</sup>




The timing of contrast injection and scan is commonly indicated as the most challenging part of an angiographic exam. The Angio Dot Engine guides the user through angiographic single- or multi-station examinations by providing visualization of arterial and venous timing windows using a test bolus technique. This information is fed back into the next planning steps so scan parameters can be adapted to the individual patient and patient's condition. Where needed, automatic voice commands support the communication with the patient

Guidance View	Step-by-step user guidance is seamlessly integrated. Sample images and guidance text are displayed for each individual step of the scanning workflow. Both images and text are easily configurable by the user
Parameter View	The new streamlined Parameter View displays the parameters that are really needed for the scan set-up. If desired, the user can switch to the conventional – fully loaded – parameter view at any time.
Test bolus	Visual display of arterial/venous timing window
Feedback of bolus timing information	Timing information is fed back into planning steps and parameters can be adapted automatically
AutoVoiceCommands	Integrated into the scanning workflow. The system plays them automatically at the right point in time. This ensures optimal timing of scanning, breathing and contrast media. The user can monitor which breath hold or pauses are actually played, and could add pauses between the automatic breath hold commands if necessary
Customization	Existing Dot Engines can be modified by the user to their individual standard of care. <ul style="list-style-type: none"><li>• Add/remove protocol steps</li><li>• Change guidance content (images and text)</li><li>• Change or add Dot Exam Strategies and Decision Points</li><li>• Modify the Parameter View</li></ul>

<sup>1)</sup> Optional

## TimCT Angio Dot Engine<sup>1)</sup>

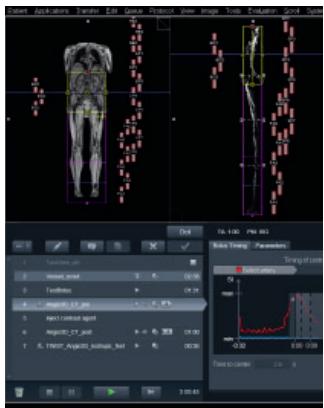

TimCT Angiography employs the revolutionary TimCT Continuous Table move technology for large Field of View angiographies with a smooth workflow and homogeneous image quality. TimCT Angiography is built on the Tim technology as well as on a highly advanced patient table with high positioning accuracy and an RF shielded table drive.

Dot TimCT Angio makes TimCT even easier with guidance throughout the exam and by providing a visual display of arterial and venous timing windows using a test bolus technique. This information is fed back into the next planning steps so scan parameters can be adapted to the individual patient and patient's condition. Where needed, automatic voice commands support the communication with the patient.

### Guidance View

Step-by-step user guidance is seamlessly integrated. Sample images and guidance text are displayed for each individual step of the scanning workflow. Both images and text are easily configurable by the user

### Parameter View

The new streamlined Parameter View displays the parameters that are really needed for the scan set-up. If desired, the user can switch to the conventional – fully loaded – parameter view at any time.

### AutoVoiceCommands

Integrated into the scanning workflow. The system plays them automatically at the right time point. This supports the synchronized timing of scanning, breathing and contrast media. The user can monitor which breath hold or pauses are actually played, and can add pauses between the automatic breath hold commands if necessary.

### Test bolus

Automatic detection of arterial/venous timing window

### Feedback of bolus timing information

Timing information is fed back into planning steps so parameters can be adapted automatically

<sup>1)</sup> Optional; Prerequisite: Angio Dot Engine and either Tim[204x48], Tim[204x64], or Tim[204x128]

### **TimCT Angio Dot Engine (Continued)**

iPAT compatibility utilizing Tim's Matrix coils capabilities

Inline subtraction and Inline MIP of complete peripheral run off images

High image homogeneity and no boundary artifacts thanks to seamless TimCT scanning

Max. FoV of TimCT (depending on the resolution)	205 cm (with Tim Whole Body Suite <sup>1)</sup> ) 140 cm (without Tim Whole Body Suite)
---	--

Table speed during angiographic measurements	Up to 5 cm/s with patient weight up to 250 kg (550 lbs)
--	---

Fast examination time for TimCT peripheral angiographic exam	40–70 s depending on resolution
--	---------------------------------

Customization	Existing Dot engines can be modified by the user to their individual standard of care. <ul style="list-style-type: none"><li>• Add/remove protocol steps</li><li>• Change guidance content (images and text)</li><li>• Change or add Dot Exam Strategies and Decision Points</li><li>• Modify the Parameter View</li></ul>
---------------	--

<sup>1)</sup> Optional

## Cardiac Dot Engine<sup>1)</sup>



Cardiac examinations used to be the most complex exams in MR. Now the Cardiac Dot Engine supports the user in many ways. Using anatomical landmarks, standard views of the heart, such as dedicated long axis and short-axis views are easily generated and can easily be reproduced using different scanning techniques. Scan parameters are adjusted to the patient's heart rate and automatic voice commands are given. All of this helps handle the complexity of CMR examinations with confidence and supports customized workflows that are easy to repeat.

Different workflows are supported:

- Functional evaluation
- Ischaemic Heart Disease

Patient View	Within the Patient View the user can easily tailor the exam to each individual patient (e.g. patient with arrhythmia, breath hold capability). Several pre-defined Dot Exam Strategies are integrated. The user just selects the appropriate strategy with one click and the queue and the complete scan set-up are automatically updated to the users pre-defined standard of care.
Guidance View	Step-by-step user guidance is seamlessly integrated. Sample images and guidance text are displayed for the individual steps of the scanning workflow. Both images and text are easily configurable by the user
AutoFoV (automatic Field of View calculation)	Based on the localizer images the optimal FoV is automatically estimated. In case the patient moves during the examination, this step can be repeated at any time
Automated parameter adaptation	Scan parameters are automatically adapted to the patient's condition (heart rate etc.)
AutoAlign Heart	Based on the localizer images, automatic detection of cardiac landmarks is obtained and used to optimally plan cardiac exams without user interaction. The fully automatic planning process results in 2-, 3- and 4-chamber view and a stack of short axis views. In case the patient moves during the examination, this step can be repeated at any time. The user can modify the AutoAlign result according to their needs.
Automated localization	Automated localization of short-axis views
Guided slice positioning	Easy way to match slice positions (short-axis) between cine, dynamic imaging, tissue characterization
Cardiac Views	Easy selection of cardiac views (e.g. 3 chamber view) during scan planning

<sup>1)</sup> Optional

### **Cardiac Dot Engine (Continued)**

Inline Ventricular Function Evaluation	Inline VF performs volumetric evaluation of cardiac cine data fully automatically right after image reconstruction. There is no user input necessary. If desired, inline calculated segmentation results can be loaded to 4D Ventricular Function Analysis for further review or processing
Cardiac specific layout for the Exam task	Automatically chosen layouts show the new physio display and are configured for every step of the exam
Automatic display of images	Automatic display of images in dedicated cardiac image orientations instead of the standard DICOM orientations.
Adaptive triggering	Acquisition adapts in realtime to heart rate variations for non-cine applications.
Automated Naming	Automated naming of series depending on cardiac views and image contrast.
AutoVoiceCommands	AutoVoiceCommands are seamlessly integrated into the scanning workflow. The system plays them automatically at the desired time point. This ensures synchronized timing of scanning and breathing. The user can monitor which breath-hold or pauses are actually played, and could add pauses between the automatic breath hold commands if necessary.
Dot Exam Strategies	The workflow can be personalized to the individual patient's condition and clinical need. The following predefined strategies are included. They can be changed at any time during the workflow: <ul style="list-style-type: none"><li>• Standard: Segmented acquisition</li><li>• Limited patient capabilities: switch to realtime and single shot imaging if breath-hold is not possible or arrhythmias occur</li></ul>
Customization	Existing Dot engines can be modified by the user to his individual standard of care. <ul style="list-style-type: none"><li>• Add/remove protocol steps</li><li>• Change guidance content (images and text)</li><li>• Change or add Dot Exam Strategies and Decision Points</li><li>• Modify the Parameter View</li></ul>

## Breast Dot Engine<sup>1)</sup>



The Breast Dot Engine provides optimized protocols for lesion evaluation and characterization as well as implant evaluation. For ease of use, different examination strategies (FatSat, non-FatSat, feet-first/head-first positioning, InterVIEWS) are available for both high-channel coils and the 4ch BI coil.

- High channel coils
- 4ch BI
- Biopsy Sentinelle 2ch medial
- Biopsy Sentinelle 10/4ch medial
- Biopsy 4ch BI

### Patient View

The user simply tailors the exam to the condition of each individual patient (e.g. patient with implants) and defines the examination approach (AutoCoverage, Frequency Adjustment Confirmation Mode, Silicone Protocols, Inline MPR).

### Implant situation

Based on an implant type identification scan, the user can visually select or modify the exam dependent on the actual implant type and laterality. The system automatically modifies the scan queue accordingly, and the frequency adjustment setting of the protocols is changed (assume dominant fat or silicone). The user may change these modifications.

### Guidance View

Sample images and a guidance text are displayed for each individual step of the scanning workflow. Both images and text are easily configurable by the user.

### Parameter View

This view displays at a glance the parameters that are really needed for the examination. The displayed parameters are easily configurable by the user. If desired, the user can switch to the conventional – fully loaded – parameter view at any time.

<sup>1)</sup> Optional

### Breast Dot Engine (Continued)

AutoCoverage: (Automatic Segmentation, AutoFoV, AutoSlice)	Based on the localizer data, an automatic segmentation is performed, which allows the estimation of the optimal FoV (entire FoV for both breasts, right or left breast, breast with chest) and which is used to automatically adapt the size of the adjust volume to the patient's anatomy. The user may modify this segmentation. The user can predefine for every protocol individually which parameters shall be automatically adjusted, e.g. whether time or slice thickness shall remain constant.
MPR Planning	For user-selected protocols, e.g. the high resolution "delayed VIEWS", adjustable MPRs are automatically calculated.
Biopsy support	Supporting interventions with the 2/4/8 ch and 2/10/16 ch Sentinel Breast and 4ch BI Breast coils. In case a Siemens or BreVis biopsy planning software is used, the target coordinates of the lesion are displayed on the Dot display at the scanner.
Single frequency adjust	The user can preselect to show the frequency adjustment dialogue only once for the exam queue. This preselection stays valid until a new coil combination or deviating z-position is used.
Customization	Existing Dot Engines can be modified by the user to their individual standard of care. <ul style="list-style-type: none"><li>• Add/remove protocol steps</li><li>• Change guidance content (images and text)</li><li>• Change or add Dot Exam Strategies and Decision Points</li><li>• Modify the Parameter View</li></ul>

## Spine Dot Engine<sup>1)</sup>



The Spine Dot Engine delivers optimized cervical, thoracic and lumbar spine imaging for all patients and provides guided and automated workflows customized to your standards of care. The Spine Dot Engine supports the user in achieving reproducible image quality with increased ease of use and time efficient exams.

### Patient View

Within the Patient View the user can easily tailor examinations to an individual patient. Dot Exam Strategies allow you to choose the most appropriate strategy with one mouse click, enabling automatic preparation of the complete MR examination.

### Guidance View

Step-by-step user guidance can be seamlessly integrated. Sample images and guidance text are then displayed for each individual step of the scanning workflow to ensure reproducible scanning. Both images and text are easily configurable by the user.

### Parameter View

The new streamlined Parameter View displays a user-defined subset of parameters which are available for manual protocol optimization. If desired, the user can switch to the conventional – fully loaded – parameter view at any time.

### AutoPosition

The C, T or L spine of the patient is automatically placed at the isocenter without any laser marking required.

### AutoAlign Spine LS

Automated and highly reliable positioning and alignment of slice groups to the spine anatomy, based on multiple anatomical landmarks. Provides fast, easy, and reproducible patient scanning and facilitates the reading by consistently delivering high image quality with a standardized slice orientation, both for follow-ups and across patients. AutoAlign Spine LS automatically detects and labels vertebra and body disks, suggests positioning for sagittal, coronal and double oblique axial slices in the spine, and automatically positions the saturation region, but also allowing the user to modify these suggestions at any time.

### AutoLabeling

Automatic labeling of vertebra for easier examination planning and faster reading

<sup>1)</sup> Optional

### **Spine Dot Engine (Continued)**

Interactive Snapping	Just drag the slide group over the sagittal plane. AutoAlign Spine LS delivers automatic double oblique positioning of axial slice groups to intervertebral disk layers.
AutoCoverage	Maximizes the speed of the examination by automatically setting the number of slices and the FoV to fully cover the C, T or L-spine. This is performed based on the information delivered by AutoAlign Spine LS, eliminating manual setting and the scanning of unnecessary slices.
Dot Exam Strategies	Examinations can be easily personalized to the individual patient condition and clinical need. The Brain Dot Engine comes with the following predefined examination strategies, which the user can select according to patient conditions or change at any time during the workflow, when conditions change: <ul style="list-style-type: none"><li>• Standard: for fast routine spine examinations</li><li>• Post surgery: for detailed evaluation of spine including fat saturation and DIXON techniques.</li><li>• High Bandwidth (WARP): Optimized strategy for the reduction of susceptibility artifacts.</li></ul>
WARP	Susceptibility artifact reduction techniques. 2D TSE sequences combining high bandwidth protocols and VAT (View Angle Tilting)-technique, tailored to reduce susceptibility artifacts (e.g. from MRI-Conditional <sup>1)</sup> implants). Available protocols include T1-weighted, T2-weighted, proton density and STIR contrast.
Rerun	An image inside the examination UI can be selected and a rerun of the corresponding series can be triggered with identical sequences or parameters.
Inline Curved reconstructions	Automatic curved reconstruction from 3D acquisitions by using the position information from the AutoAlign Spine LS algorithm.
Customization	The Spine Dot Engine can be easily modified by the user to their individual standard of care. <ul style="list-style-type: none"><li>• Add/remove protocol steps</li><li>• Change guidance content (images and text)</li><li>• Change or add Dot exam strategies</li><li>• Add clinical decision points</li><li>• Add/remove parameters in the parameter viewing card</li><li>• User-defined offsets to the standard positions delivered by AutoAlign Spine LS(also for the saturation region)</li><li>• Customized inline curved and MPR reconstructions</li></ul>

<sup>1)</sup> MR imaging of patients with metallic implants brings specific risks. However, certain implants are approved by the governing regulatory bodies to be MR conditionally safe. For such implants, the previously mentioned warning may not be applicable. Please contact the implant manufacturer for the specific conditional information. The conditions for MR safety are the responsibility of the implant manufacturer, not of Siemens.

# syngo MR Software

## syngo MR Examination

Exam Explorer	<ul style="list-style-type: none"><li>• Free and flexible programming of customized integrated exam programs</li><li>• Simple change of exam programs via drag &amp; drop</li><li>• Allows configuration of Dot: e.g. customization of image and text guidance, definition of strategies and decision points and to add sequences</li><li>• Automatic adjustment of frequency, transmitter power and 3D Shim</li><li>• Eliminates the need for receive adjustments through dynamic receiver gain control, significantly reducing scan time</li><li>• Allows for individual interactive adjustments</li><li>• No coil tuning necessary, also saving examination time</li></ul>
AutoScout	<ul style="list-style-type: none"><li>• Automatic start of localizer scan with very short acquisition time</li><li>• Allows for arbitrary orientations (multi-slice multi-angle)</li><li>• Automatically loads images into Graphical Slice Positioning</li></ul>
Graphical Slice Positioning	<p>Simultaneous use of three arbitrary localizer images from possibly different measurements for graphically positioning slices and sat regions. Interactive modification of measurement parameters (slice thickness, distance factor, oversampling etc.):</p> <ul style="list-style-type: none"><li>• Automatic selection of relevant coil elements</li><li>• Graphical selection of coil elements</li><li>• Off-center positioning (shift of FoV within the selected slice position)</li><li>• True multi-slice multi-angle, e.g. simultaneous measurement of multiple images (stacks with different orientation)</li><li>• Recall of previous slice and/or sat region positioning</li><li>• Paging through all images during graphical positioning</li><li>• Inline Movie, allowing positioning of slices on e.g. the beating heart</li><li>• Loads images immediately when they are available, e.g. during image reconstruction</li><li>• Allows quick overview via image stamps. Loads entire series of planning images with drag-and-drop</li><li>• Slice positioning (GSP) on 3D reconstructed images</li><li>• Slice positioning (GSP) on 2D and 3D distortion corrected images</li><li>• Slice positioning (GSP) on composed images</li></ul>

## **syngo MR Image Viewing and Filming**

Image Display	<ul style="list-style-type: none"><li>• Various display layouts selectable</li><li>• Up to 3 patients can be simultaneously active in the viewer</li><li>• Image annotation and labeling</li><li>• Non-interpolated display</li><li>• Fast paging through up to 500 images with 15 images/s for full screen display</li></ul>
Windowing	<ul style="list-style-type: none"><li>• Freely selectable window width and center</li><li>• Windowing on succeeding images</li><li>• Auto-windowing for optimized contrast</li><li>• Saves and sends window values</li></ul>
Automatic Movie for cine display	
Interactive movie paging by dragging the mouse or Automatic Movie mode by clicking the icon	
Evaluation	<p>Parallel evaluation of up to 40 regions of interest</p> <ul style="list-style-type: none"><li>• Circle</li><li>• Rectangle</li><li>• Freehand ROI</li><li>• Pixel lens with position marker</li><li>• Statistical evaluation</li><li>• Area</li><li>• Standard deviation</li><li>• Mean value</li><li>• Min/max values</li><li>• Image scrolling</li><li>• Magnification</li><li>• Distance</li><li>• Angle</li></ul>
2D Post-processing	<p>Image manipulations</p> <ul style="list-style-type: none"><li>• Reversal of gray-scale values</li><li>• Image rotation by 90° or by user-defined angle</li><li>• Flip horizontally/vertically</li><li>• Image zoom and pan</li><li>• Shutter</li><li>• Annotation</li></ul>
Position display	Displays measured slice positions on localizer image and selected series.

### **syngo MR Image Viewing and Filming (Continued)**

Argus Viewer	<p>Viewing software for cardiac MR studies and large data sets</p> <ul style="list-style-type: none"> <li>• Efficient cine review of cardiac and other dynamic data sets</li> <li>• Multiple sorting options</li> <li>• Single movie as well as 2, 4, or 8 simultaneous slices together in movie mode</li> <li>• Rapid AVI creation of 1 to 8 slices simultaneously</li> <li>• Creates and edits DICOM structured reports</li> </ul>				
Mean Curve	<p>Time-intensity analysis</p> <ul style="list-style-type: none"> <li>• Creates and edits DICOM structured reports</li> </ul>				
Filming	<ul style="list-style-type: none"> <li>• Connection via DICOM Basic Print</li> <li>• Interactive filming</li> <li>• Filming parallel to other activities</li> <li>• Independent scanning and documentation – no wait time due to camera delays</li> <li>• Freely selectable positioning of images onto virtual film sheet</li> <li>• Selectable various film layouts</li> <li>• Mother-in-Child display</li> <li>• Windowing, image zoom and pan on film sheet</li> <li>• Configurable image text</li> <li>• Simultaneous handling of multiple film jobs</li> <li>• Up to 100 virtual film sheets</li> </ul>				
Dynamic Analysis	<p>Arithmetic operations on images and series</p> <ul style="list-style-type: none"> <li>• Addition, subtraction, multiplication, division of single images and whole series</li> <li>• Arithmetic mean and standard deviation across a range of selected images</li> <li>• Calculation of T1 and T2, and logarithmic images</li> <li>• Differentiation/integration of selected images</li> <li>• Calculation of a mean slope image from a range of selected images</li> <li>• Calculation of z-score (t-test) images for evaluation of BOLD imaging data (Blood Oxygenation Level Dependent)</li> <li>• Time-to-peak evaluation (TTP)</li> <li>• ADC maps</li> </ul> <p>Several evaluation functions may be started consecutively in the background</p>				
Printing on Paper	<p>Interface and software for printing images on paper (laser printer not included)</p> <table style="width: 100%; border-collapse: collapse;"> <tr> <td style="width: 50%;">Supported printing</td><td style="width: 50%;">Grey levels and color</td></tr> <tr> <td>Data format</td><td>PostScript Level 2</td></tr> </table>	Supported printing	Grey levels and color	Data format	PostScript Level 2
Supported printing	Grey levels and color				
Data format	PostScript Level 2				

## **syngo MR 3D Post-processing**

MPR – Multi-Planar Reconstruction	Real-time multi-planar reformatting of secondary views <ul style="list-style-type: none"><li>• Viewing perspectives: sagittal, coronal, axial, oblique, double oblique, curved (freehand)</li><li>• Reconstruction along polygon and/or curved (freehand) cut lines</li><li>• Reconstruction based on reconstructed planes possible</li><li>• Reconstruction of user-defined ranges of parallel, radial or freehand cuts</li><li>• Selectable slice thickness and slice increment of reconstructed images</li><li>• Storing of post-processing protocols</li><li>• Annotations and 2D evaluations such as distance and ROI</li></ul>
MIP – Maximum Intensity Projection	3D reconstructions of vessels from a 3D data set, or a 2D sequential slice data set (acquired with dedicated MR Angiography sequences) <ul style="list-style-type: none"><li>• Volume of Interest (Vol) defined to increase reconstruction speed and to improve image quality</li><li>• Freehand MIP</li><li>• Arbitrary views along any direction can be defined interactively with mouse-driven virtual trackball</li><li>• Multiple view angles around any orthogonal axis</li><li>• Projections displayed as single images, as interactive movie or by fast paging</li><li>• MIP thin/MIP thick</li></ul>
MinIP – Minimum Intensity Projection	Similar to MIP but reconstructs the minimum intensity (e.g. for Dark Blood techniques)
SSD – Shaded Surface Display	Three-dimensional display of surfaces, such as vessels <ul style="list-style-type: none"><li>• Selectable variable threshold values</li><li>• Multiple view angles around any orthogonal axis</li></ul>
Volumes of Interest (Vol)	Rectangular and irregular Vol can be defined to improve image quality

## **syngo MR Network Communication**

DICOM Services (Digital Imaging and Communications in Medicine)	Interface for transmitting medical images and information in the DICOM 3.0 industrial standard. Allows for communication between devices from different manufacturers <ul style="list-style-type: none"><li>• DICOM Send/Receive</li><li>• DICOM Query/Retrieve</li><li>• DICOM SC Storage commitment</li><li>• DICOM Basic Print</li><li>• DICOM Modality Worklist</li><li>• DICOM MPPS Modality performed procedure steps. Communication back to information system</li><li>• DICOM Structured Reports</li><li>• DICOM Study Split</li></ul>
DICOM Study Split	<p>DICOM Study Split provides the mapping of one study acquired based on multiple requests to multiple studies directly at the scanner. For example, two requests for head and neck acquisition can be registered once, scanned once and immediately mapped to two separate studies for individual reading.</p> <p>Multiple requested procedures can be combined in a time saving manner by scanning a larger body region and then splitting them to individual billing relevant studies for separate reading.</p> <p>This package allows:</p> <ul style="list-style-type: none"><li>• Time saving simple mapping of multiple requested procedures to multiple acquired series with one scan</li><li>• Simple creation of studies with individual billing based on one scan workflow</li><li>• Improvement for departmental workflow by eliminating need to load/change and to request/execute splitting on a separate workstation after the scan</li><li>• Immediate visual selection, check and correction of images to study assignments.</li><li>• Overlapping region images can be copied to both studies</li></ul>

***syngo MR Network Communication (Continued)***

syngo MR Network Communication	Exchange Media Storage of images and additional data (e.g. AVI files) on CD/DVD	
DICOM Viewer	A viewing tool which can be stored together with images on a DICOM CD/DVD to be handed out to the patient	
Virus Protection	<ul style="list-style-type: none"><li>• Permanent scanning for malicious software in the background to provide maximum security</li><li>• Via Remote Access over secure network connection the latest virus scanner updates and operating system hotfixes are installed automatically</li><li>• Provided in conjunction with a service contract with Siemens (UPTIME Services)</li></ul>	
Image Transfer	Local network	Ethernet
	Data transfer rate	Max. 1 Gbit/s
	Transfer rate (256×256 image)	Approx. 60 images/s

# Computer System

## **syngo Acquisition Workplace**

General	Full multi-tasking for simultaneous functionality, e.g.: <ul style="list-style-type: none"><li>• Patient registration and pre-registration</li><li>• Scanning</li><li>• Reconstruction</li><li>• Viewing</li><li>• Post-processing</li><li>• Filming</li><li>• Data storage</li></ul>
Color LCD Monitor	High resolution flicker-free flat-screen monitor Horizontally tilttable, forward and backward Automatic backlight control for long-term brightness stability Optional second monitor
	Screen size (diagonal) 19"
	Horizontal frequency 30–100 kHz
	Vertical frequency 50–75 Hz
	Screen matrix 1280×1024
Host computer	Processor Intel Xeon ≥ E5-1620 Quad-Core
	Clock rate 3.6 GHz
	RAM 32 GB
	1 <sup>st</sup> hard disk (system SW) ≥300 GB SAS
	2 <sup>nd</sup> hard disk (data base) ≥300 GB SAS
	3 <sup>rd</sup> hard disk (images) ≥300 GB SAS
	CD-R writer Approx. 4000 images 256 <sup>2</sup> DICOM Standard, ISO 9660
	DVD-R writer Approx. 25 000 images 256 <sup>2</sup> DICOM Standard, ISO 9660
	Media drives CD/DVD drive

**syngo Acquisition Workplace (Continued)**

Measurement and reconstruction system	Processor	Intel ≥ E5-2620 (2×6-Core)
	Clock rate	2×2.0 GHz, or comparable
	Main memory (RAM)	48 GB
	Hard disk for raw data	≥300 GB
	Hard disk for system software	≥100 GB
	Parallel Scan & Recon	Simultaneous scan and reconstruction of up to 8 data sets
	Reconstruction speed	22 556 recons per second (256 <sup>2</sup> FFT, full FoV) 88 889 recons per second (256 <sup>2</sup> FFT, 25% recFoV)
Measurement and reconstruction system (optional with Tim [204x24] configuration)	Processor	Intel ≥ E3-1225
	Clock rate	3.2 GHz
	Main memory (RAM)	32 GB
	Hard disk for raw data	≥300 GB
	Hard disk for system software	≥100 GB
	Parallel Scan & Recon	Simultaneous scan and reconstruction of up to 8 data sets
	Reconstruction speed	12 987 recons per second (256 <sup>2</sup> FFT, full FoV) 57 971 recons per second (256 <sup>2</sup> FFT, 25% recFoV)

***syngo Acquisition Workplace* (Continued)**

Measurement and reconstruction system (optional with Tim [204x64] configuration)	Processor	Intel ≥ E5-2658 (2×8-Core)
	Clock Rate	≥2×2.1 GHz
	Main memory (RAM)	≥64 GB
	Hard disk for raw data	≥400 GB
	Hard disk for system software	≥100 GB
	Reconstruction speed	31 128 recons per second (256 <sup>2</sup> FFT, full FoV) 118 519 recons per second (256 <sup>2</sup> FFT, 25% recFoV)
	Parallel Scan & Recon	Simultaneous scan and reconstruction of up to 8 data sets
Measurement and reconstruction system (optional with Tim [204x128] configuration)	GPGPU	1x Tesla K10
	Processor	Intel ≥ E5-2690 (2×8-Core)
	Clock rate	≥ 2 × 2.9 GHz
	Main memory (RAM)	≥128 GB
	Hard disk for raw data	≥750 GB
	Hard disk for system software	≥100 GB
	Reconstruction speed	44 077 recons per second (256 <sup>2</sup> FFT, full FoV) 170 213 recons per second (256 <sup>2</sup> FFT, 25 % recFoV)
Parallel Scan & Recon	Simultaneous scan and reconstruction of up to 8 data sets	
	GPGPU	1x Tesla K10

***syngo MR Workplace*<sup>1)</sup>**Color LCD Monitor and host computer as for *syngo Acquisition Workplace*<sup>1)</sup> Optional

# Installation

## Siting and Installation

Short installation time due to integrated digital DirectRF technology

Typical installation time                           Less than 7 working days

## Radio Frequency Shielding

For shielding the examination room from external RF sources

RF attenuation factor                           >90 dB

Frequency range                                   15–128 MHz

## Magnetic Shielding

Room shielding                                   For additional reduction of the magnetic fringe field, suitable iron shielding can be installed in the walls of the examination room. The room shielding can be used to create a magnetic shielding enclosure

One-Floor Installation                           A combination of active shielding and a special shielding (installed on the ceiling of the magnet room or below it) will keep the 0.5 mT line within the same floor as the MRI scanner installation, even in case of very low room heights

## System Electronics Cabinets

Two cabinets which may be placed directly against the wall or even in a corner

Require service access only from the front, saving considerable space

Integrated water cooling cabinet may eliminate the need for a dedicated computer room

## Power Requirements

Line voltage	380, 400, 420, 440, 460, 480 V
Stability tolerances	±10%
Line frequency	50/60 Hz, ±1 Hz
Connection value	110 kVA

## Cooling

Two different customer specific cooling alternatives (Separator or Eco Chiller) available.

Separator option for connection to available cooling system	Water consumption Heat dissipation to water	90 l/min <sup>1)</sup> 60 kW
Eco Chiller option with automatic adaptation to the required cooling demands (e.g. different night/day mode) to decrease energy cost	GREEN Cooling Package <sup>2)</sup> : The Free Cooling Unit reduces energy consumption by up to 50%. It automatically starts if the surrounding temperature is 18 °C (64 °F) or less and reduces the chiller energy consumption. If the temperature is less than -10 °C (14 °F) the chiller is switched off <sup>3)</sup>	

## Power Consumption

System off	6.1 kW
System ready to measure <sup>4)</sup>	9.6 kW
Scan <sup>4)</sup>	25.4 kW

All values are typical values, applicable for 400V/50Hz

Consumption for optional separator pump and other options not included

<sup>1)</sup> Water temperature 12 °C/45 °F

<sup>2)</sup> Optional

<sup>3)</sup> In case of clinical routine measurement conditions

<sup>4)</sup> The power consumption described herein is based on results that were achieved in a setting according to the COCIR methodology MRI – Measurement of the energy consumption (<http://www.cocir.org/index.php?id=46>). Since many variables impact power consumption (e.g. sequences used for scanning and sequence parameters, scan time), there can be no guarantee that each customer will achieve the same values.

## Space Requirements

Min. total space requirement (for magnet, electronics,  
and console room)  $< 31 \text{ m}^2$



Dimensions		Width [cm]	Depth [cm]	Height [cm]	Weight [kg]
Examination Room	Magnet 3 Tesla AS (incl. Helium)	205	163	215	5755
	Magnet in operation, incl. gradient coil, body coil, Tim Table and covers	231	433 461 <sup>1)</sup>	219	7320
	Tim Table	76	249	52–102 <sup>2)</sup> +1.3 <sup>5)</sup>	
	Required min. room height clearance			240 <sup>3)</sup>	
Control Room	Min. transport dimensions	231	182	227	
	syngo Acquisition Workplace (table + monitor)	120	80	117 (72+45)	
	Host computer	22	46	47	
	syngo MR Workplace (optional)	120	80	117 (72+45)	
Equipment Room	Electronics cabinet, incl. system control, RF system, gradient power system, image processor	160	65	198 <sup>4)</sup>	1500
	Heat dissipation	$\leq 5 \text{ kW}$ , only ventilation might be required			
	Cooling system	65	65	189	500

<sup>1)</sup> With whole body option

<sup>2)</sup> Including Heightening Kit, if necessary

<sup>3)</sup> Finished floor to finished ceiling

<sup>4)</sup> Without attachments

<sup>5)</sup> Depending on the floor conditions

## System Cover

Different design variants are available for customer specific needs

Standard variant:

Pure White Design with  
brilliant front ring



Optional color and  
Illumination MoodLight™  
variants with brilliant front  
rings are available



Illumination MoodLight  
with or without Customized  
Logo with brilliant front ring



Light Green Design  
with brilliant front ring



Water Blue Design  
with brilliant front ring

On account of certain regional limitations of sales rights and service availability, we cannot guarantee that all products included in this brochure are available through the Siemens sales organization worldwide. Siemens reserves the right to modify the design, packaging, specifications, and options described herein without prior notice.

Any technical data contained in this document may vary within defined tolerances. Original images always lose a certain amount of detail when reproduced.

Please find fitting accessories:  
[www.siemens.com/medical-accessories](http://www.siemens.com/medical-accessories)

Please contact your local Siemens sales representative for the most current information.

#### Local Contact Information

##### In the USA

Siemens Medical Solutions USA, Inc.  
51 Valley Stream Parkway  
Malvern, PA 19355  
Phone: +1 888-826-9702  
Phone: +1 610-448-4500  
Fax: +1 610-448-2254

##### In Asia

Siemens Healthcare Sector  
Asia Pacific Headquarters  
The Siemens Center  
60 MacPherson Road  
Singapore 348615  
Phone: +65 6490 6000  
Fax: +65 6490 6001

##### In Japan

Siemens Japan K.K.  
Gate City Osaki West Tower  
1-11-1 Osaki, Shinagawa-ku  
Tokyo 141-8644  
Phone: +81 3 5423 8411

##### Global Business Unit

Siemens Healthcare Sector  
Magnetic Resonance  
Henkestr. 127  
DE-91052 Erlangen  
Germany  
Phone: +49 9131 84-0

##### Global Siemens Headquarters

Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

##### Global Siemens Healthcare

**Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

##### Legal Manufacturer

Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**SIEMENS**

**MAGNETOM Skyra**  
A Tim+Dot System

[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

Tim [204x24] XQ Gradients

Answers for life.

# Magnet System

## General


Superconducting Magnet

Short bore, patient-friendly design, high homogeneity  
3 Tesla with 70 cm Open Bore design

Easy siting due to AS (Active Shielding) and E.I.S. (External Interference Shielding) magnet technology

TrueForm Magnet Design

TrueForm magnet design produces a cylindrically optimized homogeneity volume that corresponds better to the true form of the human body. This results in better image quality as well as better fat saturation for the whole area covered in a scan. TrueForm reduces the overlap needed between steps for large virtual FoV exams and thus reduces the number of steps needed for a given scanning range

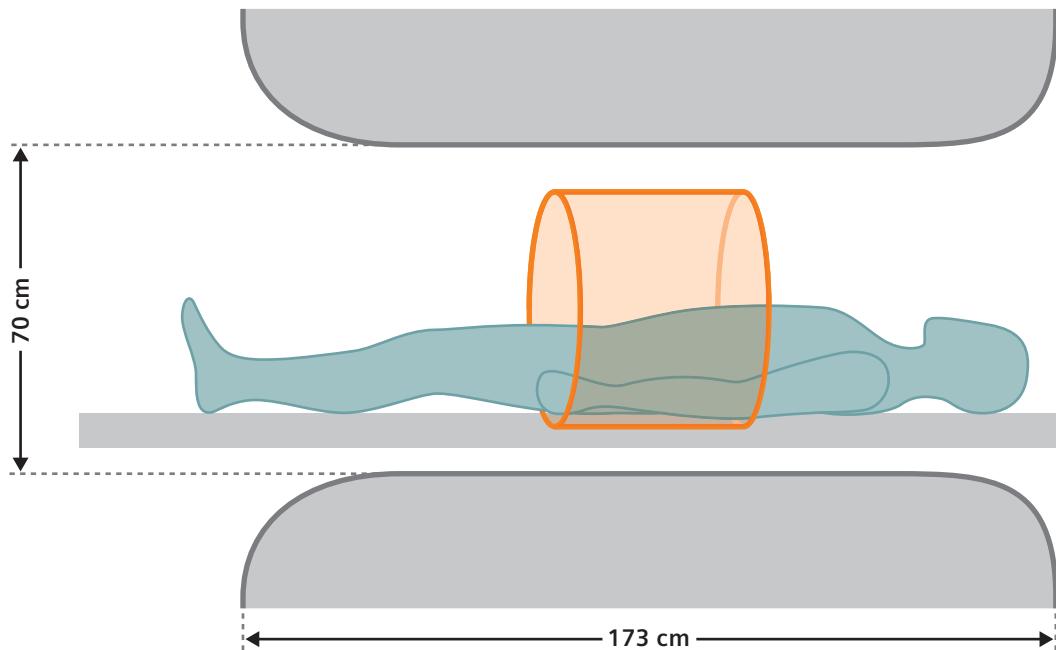

## Magnet Parameters

Operating field strength	3 Tesla
Magnet type	Superconductor
Field stability over time	<0.1 ppm/h
Weight (with cryogens)	5755 kg
Magnet length	1.63 m
Open Bore design <sup>1)</sup>	70 cm
System length cover to cover	1.73 m

## Homogeneity

### (based on highly accurate 24 plane plot)

TrueForm magnet design with a cylindrically optimized homogeneity volume for higher image quality

10 cm DSV	Guaranteed	0.01 ppm
	Typical	0.003 ppm
20 cm DSV	Guaranteed	0.05 ppm
	Typical	0.03 ppm
30 cm DSV	Guaranteed	0.3 ppm
	Typical	0.2 ppm
40 cm DSV	Guaranteed	1.4 ppm
	Typical	1.2 ppm
50×50×45 cm <sup>3</sup>	Guaranteed	4.0 ppm
DEV	Typical	3.6 ppm

In compliance with the German "Qualifikationsvereinbarung".

Standard deviation Vrms (volume root-mean square) measured with highly accurate 24 plane plot method (20 points per plane).

Standard active shim with 3 linear and 5 non-linear channels (2<sup>nd</sup> order).

DSV = Diameter spherical volume (x, y, and z direction);

DEV = Diameter elliptical volume.

<sup>1)</sup> Incl. shim coils, gradient coil, RF body coil

## Shimming

Both: passive and active shimming. Passive shimming during installation

Standard active shim with 3 linear channels (1st order) and 5 non linear channels (2nd order)

3D Shim	Patient-specific automated shim
	Time to shim Approx. 30 s

## Shielding

Active Shielding (AS)	5 <sup>th</sup> generation active shielding (AS) technology with counter coils	
Fringe field (axial × radial)	0.5 mT <sup>1)</sup>	4.6×2.6 m
	0.1 mT	6.8×3.9 m
External Interference Shield (E.I.S.)	Patented shielding system integrated into the magnet	
	Continuous compensation and automatic suppression of external magnetic field interferences during measurement (caused by moving ferromagnetic objects or nearby power lines)	

## Magnet Cooling System

Zero Helium boil-off technology	
Refill interval (typical) <sup>2)</sup>	Not applicable
Boil-off rate (typical) <sup>2)</sup>	0.0 l/year
Max. helium capacity	Approx. 1200 liters

<sup>1)</sup> Pacemaker safety limit

<sup>2)</sup> For typical clinical use, depending on sequences and operating time with running helium compressor. The system needs to be serviced at regular interval. Undisturbed magnet cooling for 24 hours and 7 days a week.

# Gradient System

## XQ Gradients: General Features

- Actively shielded (AS) whole-body gradient coil system
- Extremely low eddy currents
- Water-cooled coil and amplifier for maximum performance
- All axes force compensated

## Gradient Performance For Each Axis

Max. amplitude	45 mT/m
Min. rise time	225 µs
Max. slew rate	200 T/m/sec

## Vector Gradient Performance (vector addition of all 3 gradient axes)

Max. eff. amplitude	78 mT/m
Max. eff. slew rate	346 T/m/s
Gradient duty cycle	100%

## XQ Gradients: Amplifier

Water-cooled, highly compact, modular design	
Ultra-fast solid-state technology with very low switching losses	
Max. output voltage <sup>1)</sup>	2250 V
Max. output current <sup>1)</sup>	750 A

## XQ Gradients: Resolution Parameters

Min. FoV	5 mm
Max. FoV <sup>2)</sup>	500 mm
Slice thickness 2D	min. 0.1 mm max. 200 mm
Partition thickness 3D	min. 0.05 mm max. 20 mm
Slab thickness 3D	min. 5 mm max. 500 mm
Max. matrix	1024
Highest in-plane resolution	12 µm

<sup>1)</sup> Values for each of the 3 gradient axes

<sup>2)</sup> Depending on the application, the maximum FoV in the z-direction can be up to 45 cm

Sequences		Matrix			
		64	128	256	512
Spin Echo	min. TR [ms]	5	5	5.5	6.3
	min. TE [ms]	1.5	1.5	1.8	2.4
Inversion Recovery	min. TR [ms]	26	26	27	27
	min. TE [ms]	1.5	1.5	1.8	2.4
	min. TI [ms]	21	21	21	21
2D GRE	min. TR [ms]	0.59	0.7	1	1.22
	min. TE [ms]	0.22	0.22	0.22	0.22
3D GRE	min. TR [ms]	0.59	0.7	0.95	1.22
	min. TE [ms]	0.22	0.22	0.22	0.22
TrueFISP	min. TR [ms]	2.03	2.22	2.7	3.54
	min. TE [ms]	0.94	0.98	1.19	1.53
TSE (HASTE)	min. Echo Spacing [ms]	1.54	1.54	1.84	2.38
	min. TR [ms]	5	5	5.5	6.3
	min. TE [ms]	1.5	1.5	1.8	2.4
	max. Turbo Factor = 512				
Turbo GSE	min. Echo Spacing [ms]	0.7	0.94	0.94	1.38
	min. TR [ms]	7.5	7.8	8.1	9
	min. TE [ms]	4.5	4.5	5	5.5
max. Turbo Factor = 65					
max. EPI Factor = 21					
EPI (single-shot and multi-shot)	min. Echo Spacing [ms]	0.28	0.4	0.66	
	min. TR [ms]	10	10	10	
	min. TE [ms]	2.1	2.3	2.7	
	min. Measurement time	11	19	25	
	max. EPI Factor = 256				
Diffusion Imaging	Max. b-value [s/mm <sup>2</sup> ]	10 000	10 000	10 000	
	Min. TE [ms] with b = 1000 s/mm <sup>2</sup>	45	45	48	

All matrices without interpolation. Combinations of the stated parameters are not always possible; some parameters may require optional application packages.

# Coils

## Standard Integrated Whole-Body Coil

- No tune transmit/receive coil with 32 rungs
- Enabling TimTX TrueForm technology

## 3T Tim Matrix Coils

The Tim Matrix coils are designed for highest image quality in combination with easy handling. High element coils increase SNR and reduce examination times. DirectConnect® and SlideConnect® technology reduce patient set up time. Light weight, ergonomically designed coils enable highest patient comfort.

- No coil changing with multi-exam studies saves patient setup time
- All coils are time-saving "no-tune" coils
- Low-noise preamplifiers
- AutoCoilSelect for dynamic, automatic, or interactive selection of the coil elements within the Field of View

## Standard Coils

Head/Neck 16 (DirectConnect)	Application area	Head and neck
	Dimensions with look out mirror (L×W×H)	440 mm × 330 mm × 370 mm
	Weight	4.7 kg
Spine 24 (DirectConnect)	Application area	Spine
	Dimensions (L×W×H)	1200 mm × 489 mm × 63 mm
	Weight	11 kg
Body 6 (SlideConnect)	Application area	Thorax, Heart, Abdomen, Pelvis, Hip
	Dimensions (L×W×H)	322 mm × 520 mm × 70 mm
	Weight	1.6 kg
Flex Large 4	Application area	Multi purpose
	Dimensions (L×W)	516 mm × 224 mm
	Weight	550 g
Flex Small 4	Application area	Multi purpose
	Dimensions (L×W)	366 mm × 174 mm
	Weight	450 g
Accessories	• Flex Coil Interface 3T • Tim Coil Interface 3T	

Combination of all coils possible for large Field of View exams.

On account of certain regional limitations of sales rights and service availability, we cannot guarantee that all products included in this brochure are available through the Siemens sales organization worldwide. Siemens reserves the right to modify the design, packaging, specifications, and options described herein without prior notice.

Any technical data contained in this document may vary within defined tolerances. Original images always lose a certain amount of detail when reproduced.

Please find fitting accessories:  
[www.siemens.com/medical-accessories](http://www.siemens.com/medical-accessories)

Please contact your local Siemens sales representative for the most current information.

#### Local Contact Information

##### In the USA

Siemens Medical Solutions USA, Inc.  
51 Valley Stream Parkway  
Malvern, PA 19355  
Phone: +1 888-826-9702  
Phone: +1 610-448-4500  
Fax: +1 610-448-2254

##### In Asia

Siemens Healthcare Sector  
Asia Pacific Headquarters  
The Siemens Center  
60 MacPherson Road  
Singapore 348615  
Phone: +65 6490 6000  
Fax: +65 6490 6001

##### In Japan

Siemens Japan K.K.  
Gate City Osaki West Tower  
1-11-1 Osaki, Shinagawa-ku  
Tokyo 141-8644  
Phone: +81 3 5423 8411

##### Global Business Unit

Siemens Healthcare Sector  
Magnetic Resonance  
Henkestr. 127  
DE-91052 Erlangen  
Germany  
Phone: +49 9131 84-0

##### Global Siemens Headquarters

Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

##### Global Siemens Healthcare

**Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

##### Legal Manufacturer

Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**SIEMENS**

**MAGNETOM Skyra**  
A Tim+Dot System

[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

Tim [204x48] XQ Gradients  
Tim [204x64] XQ Gradients  
Tim [204x128] XQ Gradients

Answers for life.

# Magnet System

## General


Superconducting Magnet

Short bore, patient-friendly design, high homogeneity  
3 Tesla with 70 cm Open Bore design

Easy siting due to AS (Active Shielding) and E.I.S. (External Interference Shielding) magnet technology

TrueForm Magnet Design

TrueForm magnet design produces a cylindrically optimized homogeneity volume that corresponds better to the true form of the human body. This results in better image quality as well as better fat saturation for the whole area covered in a scan. TrueForm reduces the overlap needed between steps for large virtual FoV exams and thus reduces the number of steps needed for a given scanning range

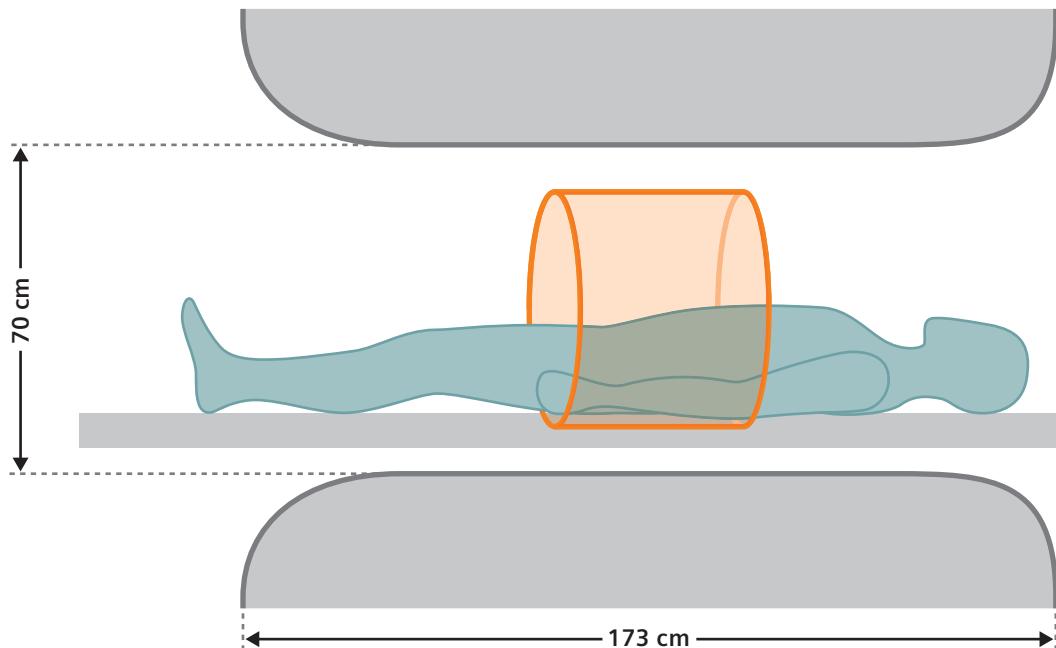

## Magnet Parameters

Operating field strength	3 Tesla
Magnet type	Superconductor
Field stability over time	<0.1 ppm/h
Weight (with cryogens)	5755 kg
Magnet length	1.63 m
Open Bore design <sup>1)</sup>	70 cm
System length cover to cover	1.73 m

## Homogeneity

### (based on highly accurate 24 plane plot)

TrueForm magnet design with a cylindrically optimized homogeneity volume for higher image quality

10 cm DSV	Guaranteed	0.01 ppm
	Typical	0.003 ppm
20 cm DSV	Guaranteed	0.05 ppm
	Typical	0.03 ppm
30 cm DSV	Guaranteed	0.3 ppm
	Typical	0.2 ppm
40 cm DSV	Guaranteed	1.4 ppm
	Typical	1.2 ppm
50×50×45 cm <sup>3</sup>	Guaranteed	4.0 ppm
DEV	Typical	3.6 ppm

In compliance with the German "Qualifikationsvereinbarung".

Standard deviation Vrms (volume root-mean square) measured with highly accurate 24 plane plot method (20 points per plane).

Standard active shim with 3 linear and 5 non-linear channels (2<sup>nd</sup> order).

DSV = Diameter spherical volume (x, y, and z direction);

DEV = Diameter elliptical volume.

<sup>1)</sup> Incl. shim coils, gradient coil, RF body coil

## Shimming

Both: passive and active shimming. Passive shimming during installation

Standard active shim with 3 linear channels (1st order) and 5 non linear channels (2nd order)

3D Shim	Patient-specific automated shim
	Time to shim Approx. 30 s

## Shielding

Active Shielding (AS)	5 <sup>th</sup> generation active shielding (AS) technology with counter coils	
Fringe field (axial × radial)	0.5 mT <sup>1)</sup>	4.6×2.6 m
	0.1 mT	6.8×3.9 m
External Interference Shield (E.I.S.)	Patented shielding system integrated into the magnet	
	Continuous compensation and automatic suppression of external magnetic field interferences during measurement (caused by moving ferromagnetic objects or nearby power lines)	

## Magnet Cooling System

Zero Helium boil-off technology	
Refill interval (typical) <sup>2)</sup>	Not applicable
Boil-off rate (typical) <sup>2)</sup>	0.0 l/year
Max. helium capacity	Approx. 1200 liters

<sup>1)</sup> Pacemaker safety limit

<sup>2)</sup> For typical clinical use, depending on sequences and operating time with running helium compressor. The system needs to be serviced at regular interval. Undisturbed magnet cooling for 24 hours and 7 days a week.

# Gradient System

## XQ Gradients: General Features

- Actively shielded (AS) whole-body gradient coil system
- Extremely low eddy currents
- Water-cooled coil and amplifier for maximum performance
- All axes force compensated

## Gradient Performance For Each Axis

Max. amplitude	45 mT/m
Min. rise time	225 µs
Max. slew rate	200 T/m/sec

## Vector Gradient Performance (vector addition of all 3 gradient axes)

Max. eff. amplitude	78 mT/m
Max. eff. slew rate	346 T/m/s
Gradient duty cycle	100%

## XQ Gradients: Amplifier

Water-cooled, highly compact, modular design	
Ultra-fast solid-state technology with very low switching losses	
Max. output voltage <sup>1)</sup>	2250 V
Max. output current <sup>1)</sup>	750 A

## XQ Gradients: Resolution Parameters

Min. FoV	5 mm
Max. FoV <sup>2)</sup>	500 mm
Slice thickness 2D	min. 0.1 mm max. 200 mm
Partition thickness 3D	min. 0.05 mm max. 20 mm
Slab thickness 3D	min. 5 mm max. 500 mm
Max. matrix	1024
Highest in-plane resolution	12 µm

<sup>1)</sup> Values for each of the 3 gradient axes

<sup>2)</sup> Depending on the application, the maximum FoV in the z-direction can be up to 45 cm

Sequences		Matrix			
		64	128	256	512
Spin Echo	min. TR [ms]	5	5	5.5	6.3
	min. TE [ms]	1.5	1.5	1.8	2.4
Inversion Recovery	min. TR [ms]	26	26	27	27
	min. TE [ms]	1.5	1.5	1.8	2.4
	min. TI [ms]	21	21	21	21
2D GRE	min. TR [ms]	0.59	0.7	1	1.22
	min. TE [ms]	0.22	0.22	0.22	0.22
3D GRE	min. TR [ms]	0.59	0.7	0.95	1.22
	min. TE [ms]	0.22	0.22	0.22	0.22
TrueFISP	min. TR [ms]	2.03	2.22	2.7	3.54
	min. TE [ms]	0.94	0.98	1.19	1.53
TSE (HASTE)	min. Echo Spacing [ms]	1.54	1.54	1.84	2.38
	min. TR [ms]	5	5	5.5	6.3
	min. TE [ms]	1.5	1.5	1.8	2.4
	max. Turbo Factor = 512				
Turbo GSE	min. Echo Spacing [ms]	0.7	0.94	0.94	1.38
	min. TR [ms]	7.5	7.8	8.1	9
	min. TE [ms]	4.5	4.5	5	5.5
max. Turbo Factor = 65					
max. EPI Factor = 21					
EPI (single-shot and multi-shot)	min. Echo Spacing [ms]	0.28	0.4	0.66	
	min. TR [ms]	10	10	10	
	min. TE [ms]	2.1	2.3	2.7	
	min. Measurement time	11	19	25	
	max. EPI Factor = 256				
Diffusion Imaging	Max. b-value [s/mm <sup>2</sup> ]	10 000	10 000	10 000	
	Min. TE [ms] with b = 1000 s/mm <sup>2</sup>	45	45	48	

All matrices without interpolation. Combinations of the stated parameters are not always possible; some parameters may require optional application packages.

# Coils

## Standard Integrated Whole-Body Coil

- No tune transmit/receive coil with 32 rungs
- Enabling TimTX TrueForm technology

## 3T Tim Matrix Coils

The Tim Matrix coils are designed for highest image quality in combination with easy handling. High element coils increase SNR and reduce examination times. DirectConnect® and SlideConnect® technology reduce patient set up time. Light weight, ergonomically designed coils enable highest patient comfort.

- No coil changing with multi-exam studies saves patient setup time
- All coils are time-saving "no-tune" coils
- Low-noise preamplifiers
- AutoCoilSelect for dynamic, automatic, or interactive selection of the coil elements within the Field of View

## Standard Coils

Head/Neck 20 (DirectConnect)	Application area	Head and neck
	Dimensions with look out mirror (L×W×H)	440 mm × 330 mm × 370 mm
	Weight	4.7 kg
Spine 32 (DirectConnect)	Application area	Spine
	Dimensions (L×W×H)	1200 mm × 489 mm × 63 mm
	Weight	11 kg
Body 18 (SlideConnect)	Application area	<ul style="list-style-type: none"><li>• Thorax</li><li>• Heart</li><li>• Abdomen</li><li>• Pelvis</li><li>• Hip</li></ul>
	Dimensions (L×W×H)	385 mm × 590 mm × 65 mm
	Weight	1.6 kg
Flex Large 4	Application area	Multi purpose
	Dimensions (L×W)	516 mm × 224 mm
	Weight	550 g
Flex Small 4	Application area	Multi purpose
	Dimensions (L×W)	366 mm × 174 mm
	Weight	450 g
Accessories	<ul style="list-style-type: none"><li>• Flex Coil Interface 3T</li><li>• Tim Coil Interface 3T</li></ul>	

Combination of all coils possible for large Field of View exams.

On account of certain regional limitations of sales rights and service availability, we cannot guarantee that all products included in this brochure are available through the Siemens sales organization worldwide. Siemens reserves the right to modify the design, packaging, specifications, and options described herein without prior notice.

Any technical data contained in this document may vary within defined tolerances. Original images always lose a certain amount of detail when reproduced.

Please find fitting accessories:  
[www.siemens.com/medical-accessories](http://www.siemens.com/medical-accessories)

Please contact your local Siemens sales representative for the most current information.

#### Local Contact Information

##### In the USA

Siemens Medical Solutions USA, Inc.  
51 Valley Stream Parkway  
Malvern, PA 19355  
Phone: +1 888-826-9702  
Phone: +1 610-448-4500  
Fax: +1 610-448-2254

##### In Asia

Siemens Healthcare Sector  
Asia Pacific Headquarters  
The Siemens Center  
60 MacPherson Road  
Singapore 348615  
Phone: +65 6490 6000  
Fax: +65 6490 6001

##### In Japan

Siemens Japan K.K.  
Gate City Osaki West Tower  
1-11-1 Osaki, Shinagawa-ku  
Tokyo 141-8644  
Phone: +81 3 5423 8411

##### Global Business Unit

Siemens Healthcare Sector  
Magnetic Resonance  
Henkestr. 127  
DE-91052 Erlangen  
Germany  
Phone: +49 9131 84-0

##### Global Siemens Headquarters

Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

##### Global Siemens Healthcare

**Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

##### Legal Manufacturer

Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**SIEMENS**

**MAGNETOM Skyra**  
A Tim+Dot System




[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

TimTX TrueShape enabling ZOOMit

Answers for life.

# TimTX True Shape

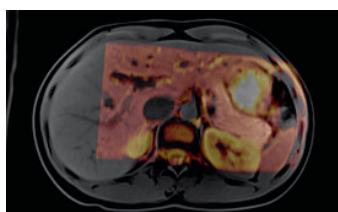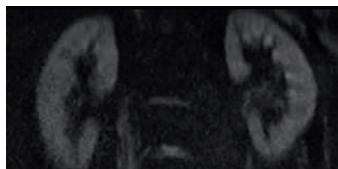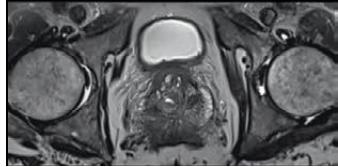

## General

TimTX TrueShape is Siemens' architecture for parallel transmit (pTx) technology and an option for MAGNETOM Skyra. It uses two independent transmit channels for fully dynamic RF excitation. TimTX TrueShape together with ZOOMit provides selective excitation within a user specified FoV. MRI applications benefit from shorter scan times, decreased image distortions, and optimized image homogeneity due to volume-selective B1 shimming<sup>1)</sup>.

TimTX TrueShape is designed to break ground for a broad range of new MRI applications. ZOOMit is the first TrueShape application.

## Direct Transmit Technology

Frequency stability (5 min)	$\pm 2 \times 10^{-10}$
Frequency control	32 bits (0.03 Hz)
Phase control	16 bits (0.006 degrees)
Body coil	Integrated whole body no-tune transmit / receive coil with 32 rungs and two independent RF transmit channels Optimized RF efficiency and signal-to-noise ratio (SNR)
Transmitter path	Real-time Feedback loop for unmatched RF stabilization
	Transmit amplitude 16 bit control 25 ns resolution
	Gain stability (after first minute) < 0.05 dB (1 s) < 0.2 dB (5 min)
Transmit amplifier	Extremely compact, water-cooled solid state amplifiers, fully integrated at the magnet as part of DirectRF technology
	Transmit amplifier bandwidth 800 kHz
	Peak power 43.2 kW

<sup>1)</sup> Prerequisite: Tim [204x48], [204x64], or [204x128] configurations.


## ZOOMit

ZOOMit is a unique application using selective excitation. Volume and shape of the excitation can be adjusted to zoom into the anatomy of interest and enable the highlighting of regions, organs, or sub-structures of an organ.

ZOOMit enables improved image quality and less distortions due to shorter echo trains, a suppression of aliasing artifacts, and shorter scan time due to fewer phase encoding steps.

With the option to accelerate the pulse by a factor of 2, higher SNR can be achieved with zoomed imaging.

- ZOOMit EPI for fMRI and DWI/DTI and ZOOMit SPACE T2 sequences are supported.  
For clinical applications, ZOOMit offers protocols for neurology, musculoskeletal, and oncology.

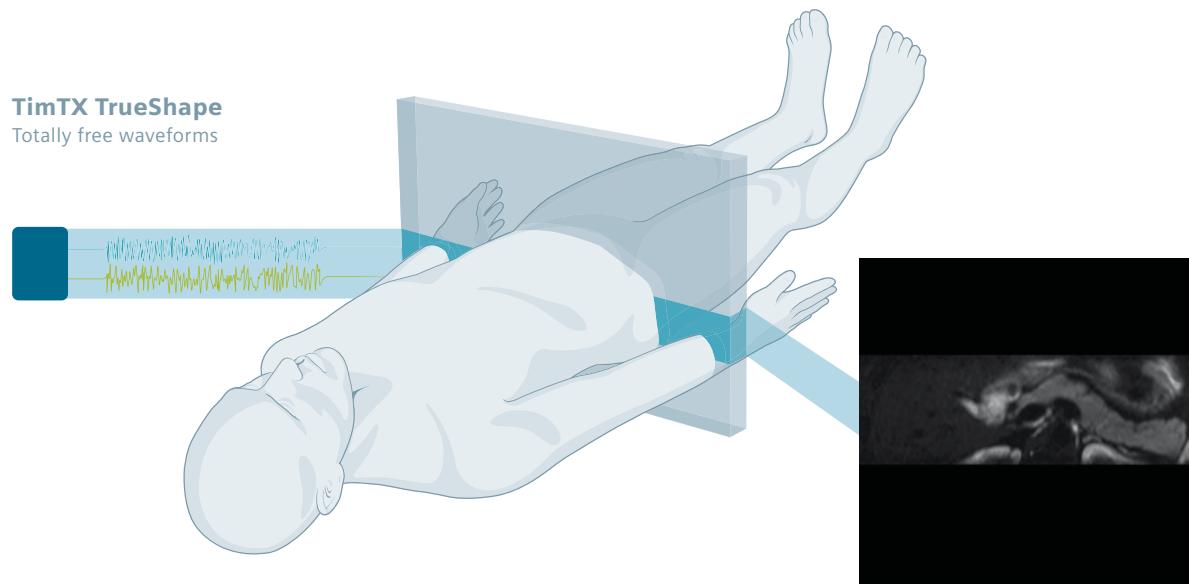

On account of certain regional limitations of sales rights and service availability, we cannot guarantee that all products included in this brochure are available through the Siemens sales organization worldwide. Siemens reserves the right to modify the design, packaging, specifications, and options described herein without prior notice.

Any technical data contained in this document may vary within defined tolerances. Original images always lose a certain amount of detail when reproduced.

Please find fitting accessories:  
[www.siemens.com/medical-accessories](http://www.siemens.com/medical-accessories)

Please contact your local Siemens sales representative for the most current information.

#### Local Contact Information

##### In the USA

Siemens Medical Solutions USA, Inc.  
51 Valley Stream Parkway  
Malvern, PA 19355  
Phone: +1 888-826-9702  
Phone: +1 610-448-4500  
Fax: +1 610-448-2254

##### In Asia

Siemens Healthcare Sector  
Asia Pacific Headquarters  
The Siemens Center  
60 MacPherson Road  
Singapore 348615  
Phone: +65 6490 6000  
Fax: +65 6490 6001

##### In Japan

Siemens Japan K.K.  
Gate City Osaki West Tower  
1-11-1 Osaki, Shinagawa-ku  
Tokyo 141-8644  
Phone: +81 3 5423 8411

##### Global Business Unit

Siemens Healthcare Sector  
Magnetic Resonance  
Henkestr. 127  
DE-91052 Erlangen  
Germany  
Phone: +49 9131 84-0

##### Global Siemens Headquarters

Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

##### Global Siemens Healthcare

**Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

##### Legal Manufacturer

Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**SIEMENS**



[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

**Tim Dockable Table**

**Answers for life.**

# Tim Dockable Table



## General

Comfortable patient table fitting the needs for patients up to 250 kg/550 lb.

- Integrated coils for fast patient preparation and enhanced user comfort
- Integrated arm boards for IV injection
- Integrated infusion stand

## General (Continued)

- 360° maneuverability with integrated navigation wheel
- Fast dock/undock functionality
- Integrated safety rails
- Compatible with TimCT
- Compatible with available Tim 4G coils

## Technical Data

Max. patient weight for vertical and horizontal table movement 250 kg (550 lbs)

Max. scan range 140 cm  
205 cm<sup>1)</sup>

User can adjust the table speed with two predefined speed mode buttons or accelerate continuously with the wheel on the Dot Control Centers

Vertical table movement	Range	56–106 cm <sup>2)</sup> +13 mm <sup>3)</sup>
	Speed	60 mm/s; one click table up
Horizontal table movement	Max. range	2750 mm
	Max. speed	200 mm/s
Position accuracy		±0.5 mm
Continuous table movement during scan capable		

<sup>1)</sup> With Tim Whole Body option

<sup>2)</sup> Including Heightening Kit, if necessary

<sup>3)</sup> Depending on the floor conditions

**Global Siemens Headquarters**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**Global Siemens Healthcare Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

**Legal Manufacturer**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**SIEMENS**

MAGNETOM Skyra  
A Tim+Dot System

**SIEMENS**



[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

Head/Neck 16

Answers for life.

# Head/Neck 16<sup>1)</sup>



## General

The Head/Neck 16 is part of the standard system configuration of the Tim [204x24] configuration.

- 16-channel design with 16 integrated pre-amplifiers, two rings of 6 elements each and one ring with 4 elements
- Cable-less coil with DirectConnect™ technology
- Combined coil for head and neck examination for optimized workflow
- Upper coil part removable
- Lower coil part usable without upper part for highly claustrophobic patients
- Lower coil part may stay on the patient table for most of the examinations
- Smoothly integrated into the patient table with Spine 24

## General (Continued)

- Open patient-friendly design
- Cushioned head stabilizers (removable)
- No coil tuning
- iPAT-compatible in all directions
- Dual-Density Signal Transfer enables ultra-high density coil designs by integrating key RF components into the local coil
- Detachable double mirror

## Applications

- Head examination
- Neck examination
- MR Head/Neck Angiography
- Combined head/neck examination
- TMJ (temporomandibular joints)

## Typically combined with

- Spine 24
- Body 6
- Peripheral Angio 36 (optional)
- Flex Large 4
- Flex Small 4

## Weight

Total	4.7 kg
Anterior part	1.7 kg

## Dimensions (L × W × H)

440 mm × 330 mm × 370 mm

<sup>1)</sup> Prerequisite: Tim [204x24]

**Global Siemens Headquarters**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**Global Siemens Healthcare Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

**Legal Manufacturer**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**SIEMENS**



[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

Head/Neck 20

Answers for life.

# Head/Neck 20<sup>1)</sup>



## General

The Head/Neck 20 is part of the standard system configuration of the Tim [204x48], [204x64], and [204x128] configurations.

- 20-channel design with 20 integrated pre-amplifiers, two rings of 8 elements each and one ring with 4 elements
- Cable-less coil with DirectConnect® technology
- Combined coil for head and neck examination for optimized workflow
- Upper coil part removable
- Lower coil part usable without upper part for highly claustrophobic patients
- Lower coil part may stay on the patient table for most of the examinations
- Smoothly integrated into the patient table with Spine 32

## General (Continued)

- Open patient-friendly design
- Cushioned head stabilizers (removable)
- No coil tuning
- iPAT-compatible in all directions
- Dual-Density Signal Transfer enables ultra-high density coil designs by integrating key RF components into the local coil
- Detachable double mirror

## Applications

- Head examination
- Neck examination
- MR Head/Neck Angiography
- Combined head/neck examination
- TMJ (temporomandibular joints)

## Typically combined with

- Spine 32
- Body 18
- Peripheral Angio 36 (optional)
- Flex Large 4
- Flex Small 4
- Loop 3T coils (optional)

## Weight

Total	4.7 kg
Anterior part	1.7 kg

## Dimensions (L × W × H)

440 mm × 330 mm × 370 mm

<sup>1)</sup> Prerequisite: Tim [204x48], Tim [204x64], Tim [204x128]

**Global Siemens Headquarters**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**Global Siemens Healthcare Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

**Legal Manufacturer**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**SIEMENS**



[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

Head/Neck 64

Answers for life.

# Head/Neck 64<sup>1)</sup>



## General

- 64-channel design with 64 integrated pre-amplifiers
- Dual-Density Signal Transfer enables ultra-high density coil designs by integrating key RF components into the local coil
- Combined coil for head and neck examination for optimized workflow
- Upper coil part removable, designed with 24 elements
- Lower coil part usable without upper part for highly claustrophobic patients, designed with 40 elements
- Cable-less lower part with DirectConnect™ technology

## General (Continued)

- Lower coil part may stay on the patient table for most of the examinations
- Cushioned head stabilizers (removable)
- No coil tuning
- iPAT-compatible
- Detachable double mirror
- One SlideConnect plug

## Applications

- High resolution head/neck proton imaging
- MR angiography of the head/neck
- Functional imaging of the brain/neck

## Typically combined with

- Spine 32
- Body 18
- Peripheral Angio 36 (optional)
- Flex Large 4
- Flex Small 4
- Loop 3T coils (optional)

## Weight

Total 5.2 kg

## Dimensions (L × W × H)

435 mm × 395 mm × 350 mm

<sup>1)</sup> Prerequisite: Tim [204x64], or [204x128] configuration.

**Global Siemens Headquarters**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**Global Siemens Healthcare Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

**Legal Manufacturer**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**SIEMENS**



[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

Spine 24

Answers for life.

# Spine 24<sup>1)</sup>



## General

The Spine 24 is part of the standard system configuration of the Tim [204x24] configuration.

- 24-channel design with 24 integrated pre-amplifiers, 8 rows of 3 elements each
- Cable-less coil with DirectConnect™ technology
- Smoothly integrated into the patient table and streamlined with Head/Neck 16
- May remain on the patient table for nearly all exams

## General (Continued)

- No coil tuning
- iPAT-compatible in all directions
- Dual-Density Signal Transfer enables ultra-high density coil designs by integrating key RF components into the local coil

## Applications

- High resolution imaging of the whole spine
- Various applications in combination with additional coils

## Typically combined with

- Head/Neck 16
- Body 6
- Peripheral Angio 36 (optional)
- Flex Large 4
- Flex Small 4

## Weight

11 kg

## Dimensions (L × W × H)

1200 mm × 489 mm × 63 mm

<sup>1)</sup> Prerequisite: Tim [204x24]

**Global Siemens Headquarters**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**Global Siemens Healthcare Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

**Legal Manufacturer**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**SIEMENS**



[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

Spine 32

Answers for life.

# Spine 32<sup>1)</sup>



## General

The Spine 32 is part of the standard system configuration of the Tim [204x48], [204x64], and [204x128] configurations.

- 32-channel design with 32 integrated pre-amplifiers, 8 rows of 4 elements each
- Cable-less coil with DirectConnect® technology
- Smoothly integrated into the patient table and streamlined with Head/Neck 20
- May remain on the patient table for nearly all exams
- No coil tuning

## General (Continued)

- iPAT-compatible in all directions
- Dual-Density Signal Transfer enables ultra-high density coil designs by integrating key RF components into the local coil

## Applications

- High resolution imaging of the whole spine
- Various applications in combination with additional coils

## Typically combined with

- Head/Neck 20
- Body 18
- Peripheral Angio 36 (optional)
- Flex Large 4
- Flex Small 4
- Loop 3T coils (optional)

## Weight

11 kg

## Dimensions (L × W × H)

1200 mm × 489 mm × 63 mm

<sup>1)</sup> Prerequisite: Tim [204x48], Tim [204x64], Tim [204x128]

**Global Siemens Headquarters**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**Global Siemens Healthcare Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

**Legal Manufacturer**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**SIEMENS**



[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

Body 6

Answers for life.

# Body 6<sup>1)</sup>



## General

The Body 6 is part of the standard system configuration of the Tim [204x24] configuration.

- 6-channel design with 6 integrated preamplifiers, with 2 rows of 3 elements each
- Operates in an integrated fashion with the Spine 24 (8 rows of 3 elements each)
- Can be combined with further Body 6 coils for larger coverage
- No coil tuning
- iPAT-compatible in all directions
- Dual-Density Signal Transfer enables ultra-high density coil designs by integrating key RF components into the local coil
- SlideConnect® technology for easy coil set up

## Applications

- Thorax
- Heart
- Abdomen
- Pelvis
- Hip
- Vascular

## Typically combined with

- Head/Neck 16
- Spine 24
- Additional Body 6 coils (optional)
- Peripheral Angio 36 (optional)
- Flex Large 4
- Flex Small 4
- Endorectal coil (optional)

## Weight

1.6 kg

"patient-felt" weight of coil only – 1.1 kg

## Dimensions (L × W × H)

322 mm × 520 mm × 70 mm

<sup>1)</sup> Prerequisite: Tim [204x24]

**Global Siemens Headquarters**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**Global Siemens Healthcare Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

**Legal Manufacturer**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**SIEMENS**



[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

Body 18

Answers for life.

# Body 18<sup>1)</sup>



## General

The Body 18 is part of the standard system configuration of the Tim [204x48], [204x64], and [204x128] configurations.

- 18-channel design with 18 integrated pre-amplifiers, with 3 rows of 6 elements each
- Operates in an integrated fashion with the Spine 32 (8 rows of 4 elements each)

## General (Continued)

- Can be combined with further Body 18 coils for larger coverage
- No coil tuning
- iPAT-compatible in all directions
- Dual-Density Signal Transfer enables ultra-high density coil designs by integrating key RF components into the local coil.
- SlideConnect® technology for easy coil set up

## Applications

- Thorax
- Heart
- Abdomen
- Pelvis
- Hip
- Vascular

## Typically combined with

- Head/Neck 20
- Spine 32
- Additional Body 18 coils
- Peripheral Angio 36 (optional)
- Flex Large 4
- Flex Small 4
- Loop 3T coils (optional)
- Endorectal coil (optional)

## Weight

1.6 kg  
“patient-felt” weight of coil only – 1.1 kg

## Dimensions (L × W × H)

385 mm × 590 mm × 65 mm

<sup>1)</sup> Prerequisite: Tim [204x48], Tim [204x64], Tim [204x128]

**Global Siemens Headquarters**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**Global Siemens Healthcare Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

**Legal Manufacturer**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**SIEMENS**



[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

Body 18 Long

Answers for life.

# Body 18 Long<sup>1)</sup>



## General

Body 18 coil with extended cable, especially suitable for therapy image guidance.

- 18-channel design with 18 integrated pre-amplifiers, with 3 rows of 6 elements each
- Operates in an integrated fashion with the Spine 32 as 30 channel body coil
- Can be combined with further Body 18 or Body 18 Long coils for larger coverage
- No coil tuning
- iPAT-compatible in all directions
- Dual-Density Signal Transfer enables ultra-high density coil design by integrating key RF components into the local coil.
- SlideConnect® technology for easy coil set up

## Applications

- MRI for RT image guidance
- MRI in the context of neuro- and cardiovascular interventions
- all Body 18 applications:  
Thorax; Heart; Abdomen; Pelvis; Hip; Vascular

## Typically combined with

- for Radiation Therapy imaging purposes:
  - Flex 4 coil(s)
  - Body 18 coil(s)
  - Spine 32 coil
- for imaging in the context of neuro- and cardiovascular interventions:
  - Body 18 coil(s)
  - Combi Coil Base (only in combination with the Combi Dockable Table; allows to combine the Body 18 Long with Body 18 and to use the combination as spine coil in situations where the patient is positioned on a transfer board so that the Spine 32 cannot be used)

## Weight

2 kg

"patient-perceived" weight of coil only – 1.1 kg

## Dimensions (L × W × H)

385 mm × 590 mm × 65 mm

## Cable length

168 cm (70 cm longer compared to the Body 18)

<sup>1)</sup> Prerequisite: Tim [204x48], Tim [204x64], or Tim [204x128] configuration

**Global Siemens Headquarters**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**Global Siemens Healthcare Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

**Legal Manufacturer**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**SIEMENS**



[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

**Flex Large 4  
Flex Small 4**

**Answers for life.**

# Flex Large 4 and Flex Small 4



## General

The Flex Large 4 and Flex Small 4 are part of the standard system configuration.

- Four integrated low-noise preamplifiers
- Allows flexible coil positioning
- Only one interface necessary for all Flex coils
- Several Flex Coil Interfaces can be used simultaneously
- Dual-Density Signal Transfer enables ultra-high density coil designs by integrating key RF components into the local coil
- Connection via Flex Coil Interface

## Features

- Wrap-around coil made from soft and flexible material
- 4-channel design
- iPAT-compatible
- No coil tuning

## Flex Large 4

### Applications

Imaging of large regions such as medium to large shoulder, hip, and knee

## FlexSmall 4

Imaging of small regions such as small to medium shoulder, wrist, elbow, and ankle

### Typically combined with

- |                                  |                                  |
|----------------------------------|----------------------------------|
| • Head/Neck 16/20                | • Head/Neck 16/20                |
| • Body 6/18                      | • Body 6/18                      |
| • Peripheral Angio 36 (optional) | • Peripheral Angio 36 (optional) |
| • Flex Small 4 <sup>1)</sup>     | • Flex Large 4 <sup>1)</sup>     |
| • Loop 3T coils <sup>1)</sup>    | • Loop 3T coils <sup>1)</sup>    |
| • Endorectal coil (optional)     | • Endorectal coil (optional)     |

### Weight

550 g                          450 g

### Dimensions (L × W × H)

516 mm × 224 mm                          366 mm × 174 mm

<sup>1)</sup> Second Flex Coil Interface 3T required (option)

**Global Siemens Headquarters**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**Global Siemens Healthcare Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

**Legal Manufacturer**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**SIEMENS**



[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

Peripheral Angio 36

Answers for life.

# Peripheral Angio 36<sup>1)</sup>



## General

- 36-channel design with 36 integrated pre-amplifiers, distributed over 6 planes with 6 elements each
- Operates in an integrated fashion with Body 18 coils and with the Spine 32 and for whole-body examinations also with the Head/Neck 20
- Can be utilized head and feet first
- Both legs are independently covered with coil elements, maximizing the coil filling factor and the signal-to-noise ratio

## General (Continued)

- No coil tuning
- iPAT-compatible in all directions
- Dual-Density Signal Transfer enables ultra-high density coil designs by integrating key RF components into the local coil
- SlideConnect® technology for easy coil set up
- One cable only for easy handling

## Applications

- High resolution angiography of both legs with high signal-to-noise ratio
- Bilateral examinations of long bones of the legs

## Typically combined with

- Head/Neck 16/20
- Body 6/18
- Spine 24/32
- Flex Large 4
- Flex Small 4

## Weight

8 kg

## Dimensions (L × W × H)

860 mm × 300–640 mm × 280 mm

<sup>1)</sup> Prerequisite: Tim [204x48], Tim [204x64], Tim [204x128]

**Global Siemens Headquarters**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**Global Siemens Healthcare Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

**Legal Manufacturer**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**SIEMENS**



[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

Hand/Wrist 16

Answers for life.

# Hand/Wrist 16



## General

- 16-channel coil with 16 integrated preamplifiers
- iPAT-compatible in all directions
- Hinged design of the upper part for quick and easy patient positioning
- Stabilization pads for comfortable positioning
- Holder allows off-center positioning to ensure a comfortable position for the patient
- No coil tuning
- Dual-Density Signal Transfer enables ultra-high density coil designs by integrating key RF components into the local coil
- SlideConnect™ technology for easy coil set up

## Applications

High resolution hand and wrist imaging

## Typically combined with

- Body 6/18
- Flex Large 4
- Flex Small 4
- Loop 3T coils (optional)

## Weight

Coil	approx. 2.8 kg
------	----------------

Base plate	approx. 1.6 kg
------------	----------------

## Dimensions (L × W × H)

Coil	approx. 332 mm × 215 mm × 115 mm
------	-------------------------------------

Base plate	approx. 524 mm × 313 mm × 30.5 mm
------------	--------------------------------------

**Global Siemens Headquarters**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**Global Siemens Healthcare  
Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

**Legal Manufacturer**  
Siemens Shenzhen Magnetic  
Resonance Ltd. (SSMR)  
Siemens MRI Center, Gaoxin C. Ave.  
2nd, Hi-Tech Industrial Park  
Shenzhen 518057  
P.R. China  
Phone: + 86 755-26525421  
Fax: + 86 755-26549253

**SIEMENS**

MAGNETOM Skyra  
A Total MRI System

**SIEMENS**



[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

Foot/Ankle 16

Answers for life.

# Foot/Ankle 16



## Applications

High resolution foot and ankle imaging

## Weight

Coil	3.2 kg
Base plate	7.1 kg

## Dimensions (L × W × H)

Coil	410 mm × 330 mm × 390 mm
Base plate	427 mm × 333 mm × 383 mm

## General

- 16-channel coil with 16 integrated preamplifiers
- iPAT-compatible in all directions
- Boot-like coil design
- Cable-less coil with DirectConnect® technology
- Stabilization pads for comfortable patient positioning
- No coil tuning
- Dual-Density Signal Transfer enables ultra-high density coil designs by integrating key RF components into the local coil

**Global Siemens Headquarters**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**Global Siemens Healthcare Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

**Legal Manufacturer**  
Siemens Shenzhen Magnetic Resonance Ltd. (SSMR)  
Siemens MRI Center, Gaoxin C. Ave.  
2nd, Hi-Tech Industrial Park  
Shenzhen 518057  
P.R. China  
Phone: + 86 755-26525421  
Fax: + 86 755-26549253

**SIEMENS**



[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

Shoulder Large 16  
Shoulder Small 16

Answers for life.

# Shoulder Large and Shoulder Small 16



## General

- Two 16-channel coils to cover small and large shoulder anatomy, – each with 16-channel coil design with 16 integrated preamplifiers
- For narrow or wide shoulders the coil can be attached at different positions on the base plate
- Includes one base plate pad for high patient comfort
- No coil tuning
- iPAT-compatible in all directions
- Dual-Density Signal Transfer enables ultra-high density coil designs by integrating key RF components into the local coil
- SlideConnect® technology for easy coil set up

## Applications

- Excellent visualization of small anatomical structures (e.g. labrum)
- High SNR and high field homogeneity
- Reduced slice thickness and measurement times

## Technical Data

Shoulder Large 16	Opening	200 mm
	Weight	2.3 kg
Shoulder Small 16	Opening	165 mm
	Weight	2.2 kg
Base plate	Dimensions (L × W)	445 mm × 490 mm
	Weight	5 kg

**Global Siemens Headquarters**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**Global Siemens Healthcare Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

**Legal Manufacturer**  
Siemens Shenzhen Magnetic Resonance Ltd. (SSMR)  
Siemens MRI Center, Gaoxin C. Ave.  
2nd, Hi-Tech Industrial Park  
Shenzhen 518057  
P.R. China  
Phone: + 86 755-26525421  
Fax: + 86 755-26549253

**SIEMENS**



[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

CP Extremity Coil

Answers for life.

# CP Extremity Coil



## General

- Transmit/receive coil
- Upper coil part removable
- Holder allows off-center positioning to keep knee or foot which is not under examination in a comfortable position
- No coil tuning
- Connection via Tim Coil Interface 3T

## Applications

- Knee
- Ankle
- Peripheral MR Angiography
- Pediatric imaging<sup>1)</sup>

## Weight

5.7 kg

## Dimensions (L × W × H)

265 mm × 360 mm × 310 mm

## Minimum inner dimension

154 mm

<sup>1)</sup> MR scanning has not been established as safe for imaging fetuses and infants under two years of age. The responsible physician must evaluate the benefit of the MRI examination in comparison to other imaging procedures.

**Global Siemens Headquarters**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**Global Siemens Healthcare Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

**Legal Manufacturer**  
Quality Electrodynamics LLC  
700 Beta Drive, Suite 100  
44143 Mayfield Village  
USA  
Phone: +1 440-484-2228

**SIEMENS**

MAGNETOM Skyra  
A Timedot System

SIE



[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

Tx/Rx 15-Channel Knee Coil

Answers for life.

# Tx/Rx 15-Channel Knee Coil<sup>1)</sup>



## Applications

- Examinations of joints in the area of the lower extremities
- High resolution knee imaging

## Weight

6.6 kg

## Dimensions (L × W × H)

256 mm × 360 mm × 310 mm

## Minimum inner dimension

154 mm

## General

- 15 channel transmit/receive coil
- 15-channel coil with 15 integrated preamplifiers, elements arranged in 3 rungs by 5 elements
- iPAT-compatible in all directions
- Upper coil part removable
- Holder allows off-center positioning to ensure a comfortable position for the patient
- Cushions for patient comfort and stabilization of the anatomy
- No coil tuning
- One plug only
- SlideConnect® technology for easy coil set up

<sup>1)</sup> Alternative name: Tx/Rx Knee 15

**Global Siemens Headquarters**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**Global Siemens Healthcare Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

**Legal Manufacturer**  
Quality Electrodynamics LLC  
700 Beta Drive, Suite 100  
44143 Mayfield Village  
USA  
Phone: +1 440-484-2228

**SIEMENS**

MAGNETOM Aera  
A Tim+Dot System

**SIEMENS**




[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

4-Channel BI Breast Coil

Answers for life.

# 4-Channel BI Breast Coil

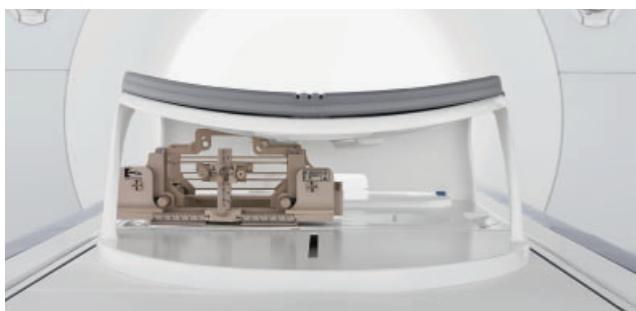

## General

- Frame
- 2-channel insert plate coil
- 2-channel patient pad coil
- Positioning cushion
- Head rest
- Biopsy plate

## General (Continued)

- Biopsy set: biopsy box; 2 fixation units (grid and post/pillar); positioning system including 2 needle adapter tubes and oil marker
- Tim Coil Interface 3T needed to connect coil with scanner
- Spine 24/32 can remain on the table

## Applications

- Simultaneous basic imaging of both breasts in all directions
- Uni- or bi-lateral basic imaging of the breasts in sagittal direction
- Biopsy imaging for lateral, medial, and crano-caudal access

## Can be combined with

- Flex Large 4
- Flex Small 4
- Loop 3T coils (optional)

## Weight (Coil and frame)

10 kg

## Dimensions (L × W × H)

880 mm × 470 mm × 210 mm

**Global Siemens Headquarters**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**Global Siemens Healthcare Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

**Legal Manufacturer**  
Noras MRI products GmbH  
Leibnizstr. 4  
97204 Hoechberg  
Germany  
Phone: +49 931/29 92 7-0  
Fax: +49 931/29 92 7-20  
[www.noras.de](http://www.noras.de)

**SIEMENS**



[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

16-Channel AI Breast Coil

Answers for life.

# 16-Channel AI Breast Coil



## Applications

- Simultaneous imaging of both breasts in all directions
- Uni- or bi-lateral imaging of the breasts in sagittal direction
- High-resolution 2D and 3D MR breast imaging
- Unmatched iPAT capabilities, iPAT factors up to 4

## Weight

11 kg

## Dimensions (L × W × H)

710 mm × 470 mm × 200 mm

## General

- The coil consists of a 16-channel design with 16 integrated preamplifiers. The coil elements are arranged in arrays of 6 elements, plus an axilla element and a cup design element on each side.
- Frame
- Positioning cushion
- Head rest
- iPAT compatible
- Two Tim Coil Interfaces 3T needed to connect coil with scanner (one optional)
- Spine 24/32 can remain on the table

**Global Siemens Headquarters**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**Global Siemens Healthcare Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

**Legal Manufacturer**  
RAPID Biomedical GmbH  
Technology Park Würzburg-Rimpar  
Kettelerstrasse 3-11  
97222 Rimpar  
Germany  
Phone: +49 93 65 / 88 26-0  
Fax: +49 93 65 / 88 26-99  
[www.rapidbiomed.de](http://www.rapidbiomed.de)

**SIEMENS**

MAGNETOM Skyra  
A Tim+Dot system

**SIEMENS**



[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

2-/4-/8-Channel Sentinelle Breast Coil

Answers for life.

# 2-/4-/8-Channel Sentinelle Breast Coil



## General

- Patient frame
- Immobilization plate
- Slider
- Two 3-channel diagnostic insert coils,  
two 1-channel biopsy insert coils,  
one 2-channel medial coil
- The coil can be used in the following configurations:  
8-channel diagnostic imaging,  
4-channel biopsy (bilateral/lateral),  
2-channel biopsy (unilateral/medial)

## General (Continued)

- Breast cushion set
- Height adjustable head rest
- Contra-lateral support plate for use in unilateral biopsy
- Tim Coil Interface 3T needed to connect coil with scanner
- Biopsy set for training purposes (grid, marker and training needle kit)

## Applications

- Simultaneous imaging of both breasts in all directions
- Uni- or bi-lateral imaging of the breasts in sagittal direction
- Biopsy imaging for lateral and medial access
- High-resolution 2D and 3D imaging
- iPAT factors up to 3
- For quantitative spectroscopy (GRACE<sup>1)</sup>) a reference bottle can be inserted

## Can be combined with

- Flex Large 4
- Flex Small 4
- Body 6/18

## Weight

16 kg without riser  
22 kg with riser

## Dimensions (L × W × H)

1097 mm × 582 mm × 279 mm

<sup>1)</sup> Optional

**Global Siemens Headquarters**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**Global Siemens Healthcare Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

**Legal Manufacturer**  
Sentinelle Medical Inc.  
555 Richmond St. West Suite 800  
Toronto, Ontario, M5V 3B1  
Canada  
Phone: +1 416-366-4994  
Fax: +1 416-594-9696  
[www.sentinelomedical.com](http://www.sentinelomedical.com)

**SIEMENS**




[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

8-Channel Sentinel Breast Coil/  
Upgrade to Biopsy Configuration

Answers for life.

# 8-Channel Sentinelle Breast Coil

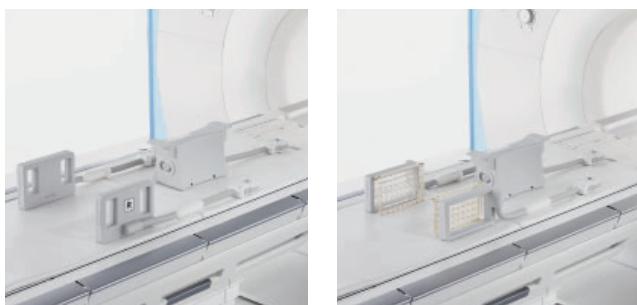

## Sentinelle Breast Coil (Imaging Configuration)

### General

- Patient frame
- Immobilization plate
- Slider
- Two 3-channel diagnostic insert coils, one 2-channel medial coil
- The coil can be used for 8-channel diagnostic imaging
- Breast cushion set
- Height adjustable head rest
- Tim Coil Interface 3T needed to connect coil with scanner
- Coil configuration functionally upgradable for biopsy (optional)

### Applications

- Simultaneous imaging of both breasts in all directions
- Uni- or bi-lateral imaging of the breasts in sagittal direction
- High-resolution 2D and 3D imaging
- iPAT factors up to 3
- For quantitative spectroscopy (GRACE<sup>1)</sup>) a reference bottle can be inserted.

### Can be combined with

Flex Large 4; Flex Small 4; Body 6/18

### Weight

16 kg without riser; 22 kg with riser

### Dimensions (L × W × H)

1097 mm × 582 mm × 279 mm

## Sentinelle Breast Coil Upgrade to Biopsy Configuration<sup>2)</sup>

### General

- Two 1-channel biopsy insert coils, one 2-channel medial coil
- The coil can be used in the following configurations: 4-channel biopsy (bilateral/lateral), 2-channel biopsy (unilateral/medial)
- Contra-lateral support plate for use in uni lateral biopsy needle kit)
- Biopsy set for training purposes (grid, marker and training needle kit)

### Applications

Biopsy imaging for lateral and medial access

### Weight

16 kg without riser; 22 kg with riser

### Dimensions (L × W × H)

1097 mm × 582 mm × 279 mm

<sup>1)</sup> Optional

<sup>2)</sup> Prerequisite: 8-Channel Imaging Configuration

**Global Siemens Headquarters**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**Global Siemens Healthcare Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

**Legal Manufacturer**  
Sentinelle Medical Inc.  
555 Richmond St. West Suite 800  
Toronto, Ontario, M5V 3B1  
Canada  
Phone: +1 416-366-4994  
Fax: +1 416-594-9696  
[www.sentinelomedical.com](http://www.sentinelomedical.com)

**SIEMENS**



[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

2-/10-/16-Channel Sentinelle Breast Coil

Answers for life.

# 2-/10-/16-Channel Sentinelle Breast Coil



## General

- Patient frame
- Immobilization plate
- Slider
- Two 4-channel diagnostic insert coils,  
two 1-channel biopsy insert coils,  
one 8-channel medial coil
- The coil can be used in the following configurations:  
16-channel diagnostic imaging,  
10-channel biopsy (bilateral/lateral),  
2-channel biopsy (unilateral/medial)
- Breast cushion set
- Height adjustable head rest

## General (Continued)

- Contra-lateral support plate for use in unilateral biopsy
- Biopsy set for training purposes (grid, marker and training needle kit)
- Connection with two Tim Coil Interfaces 3T (one optional)

## Applications

- Simultaneous imaging of both breasts in all directions
- Uni- or bi-lateral imaging of the breasts in sagittal direction
- Biopsy imaging for lateral and medial access
- High-resolution 2D and 3D imaging
- iPAT factors up to 5
- For quantitative spectroscopy (GRACE<sup>1)</sup>) a reference bottle can be inserted.

## Can be combined with

Flex Large 4; Flex Small 4; Body 6/18

## Weight

16 kg without riser; 22 kg with riser

## Dimensions (L × W × H)

1097 mm × 582 mm × 279 mm

<sup>1)</sup> Optional

<sup>2)</sup> Prerequisite: Tim [204x48], Tim [204x64], or Tim [204x128] configuration

**Global Siemens Headquarters**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**Global Siemens Healthcare Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

**Legal Manufacturer**  
Sentinelle Medical Inc.  
555 Richmond St. West Suite 800  
Toronto, Ontario, M5V 3B1  
Canada  
Phone: +1 416-366-4994  
Fax: +1 416-594-9696  
[www.sentinelomedical.com](http://www.sentinelomedical.com)

**SIEMENS**



[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

16-Channel Sentinelle Breast Coil/  
Upgrade to Biopsy Configuration

Answers for life.

# 16-Channel Sentinelle Breast Coil



## 16-Channel Sentinelle Breast Coil (Imaging Configuration)

### General

- Patient frame
- Immobilization plate
- Slider
- Two 4-channel diagnostic insert coils, one 8-channel medial coil
- The coil can be used in the following configurations:  
16-channel diagnostic imaging
- Breast cushion set
- Height adjustable head rest

### Applications

- Simultaneous imaging of both breasts in all directions
- Uni- or bi-lateral imaging of the breasts in sagittal direction
- High-resolution 2D and 3D imaging
- iPAT factors up to 5
- For quantitative spectroscopy (GRACE<sup>1)</sup>) a reference bottle can be inserted

### Can be combined with

Flex Large 4; Flex Small 4; Body 6/18

### Weight

16 kg without riser; 22 kg with riser

### Dimensions (L × W × H)

1097 mm × 582 mm × 279 mm

## 16-Channel Sentinelle Breast Coil / Upgrade to Biopsy Configuration<sup>2)</sup>

### General

- Two 1-channel biopsy insert coils, one 8-channel medial coil
- The coil can be used in the following configurations:  
10-channel biopsy (bilateral/lateral), 2-channel biopsy (unilateral/medial)
- Contra-lateral support plate for use in unilateral biopsy needle kit
- Biopsy set for training purposes (grid, marker and training needle kit) Applications

### Applications

Biopsy imaging for lateral and medial access

### Weight

16 kg without riser; 22 kg with riser

### Dimensions (L × W × H)

1097 mm × 582 mm × 279 mm

<sup>1)</sup> Optional

<sup>3)</sup> Prerequisite: 8-Channel Imaging Configuration

**Global Siemens Headquarters**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**Global Siemens Healthcare  
Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

**Legal Manufacturer**  
Sentinelle Medical Inc.  
555 Richmond St. West Suite 800  
Toronto, Ontario, M5V 3B1  
Canada  
Phone: +1 416-366-4994  
Fax: +1 416-594-9696  
[www.sentinelomedical.com](http://www.sentinelomedical.com)

**SIEMENS**



[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

Breast 18

Answers for life.

# Breast 18



## General

- 18 channels with 4 frontal elements, 4 elements around the breast and 1 axillary element, for each breast
- Height adjustable head rest
- Compact design
- Plug parking position
- Single plug connect
- Head or feet first measurement possible
- Support cushion with mechanical lock to coil
- Volume per breast 2200ml

## Applications

- Simultaneous imaging of both breasts in all directions
- Uni- or bi-lateral imaging of the breasts in sagittal direction
- Axillary imaging elements
- High-resolution 2D and 3D imaging
- For quantitative imaging spectroscopy (GRACE<sup>1)</sup>) a reference bottle can be inserted

## Can be combined with

- Flex Large 4
- Flex Small 4
- Body 18

## Weight

5.5 kg

## Dimensions (L x W x H)

575 mm x 410 mm x 205 mm

<sup>1)</sup> Optional

**Global Siemens Headquarters**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**Global Siemens Healthcare Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

**Legal Manufacturer**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**SIEMENS**



[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

Loop Coils

Answers for life.



**SIEMENS**



[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

MEDRAD Endorectal Coil Kit

Answers for life.

# MEDRAD Endorectal Coil Kit



## General

- The MEDRAD Endorectal Coil Kit includes the MEDRAD Endo Interface 3T\* and the Endo Adapter 3T, and connects to the Tim Coil Interface 3T that is available separately
- Interface device for connecting the disposable endorectal coil (to be ordered separately)
- No coil tuning

## Applications

- Excellent visualization of the prostate
- Non-invasive preoperative diagnostic evaluation and treatment planning

## Typically combined with

- Body 6/18
- Spine 24/32
- All flexible coils (second, optional Flex Coil Interface 3T required)

## Weight of the disposable coil

200 g


\* Legal Manufacturer:  
Bayer Medical Care Inc.  
1 Bayer Drive  
Indianola, PA 15051-0780  
U.S.A.  
Phone: +1 412-767-2400  
Fax: +1 416-594-9696  
[www.medrad.com](http://www.medrad.com)

**Global Siemens Headquarters**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**Global Siemens Healthcare  
Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

**Legal Manufacturer**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**SIEMENS**

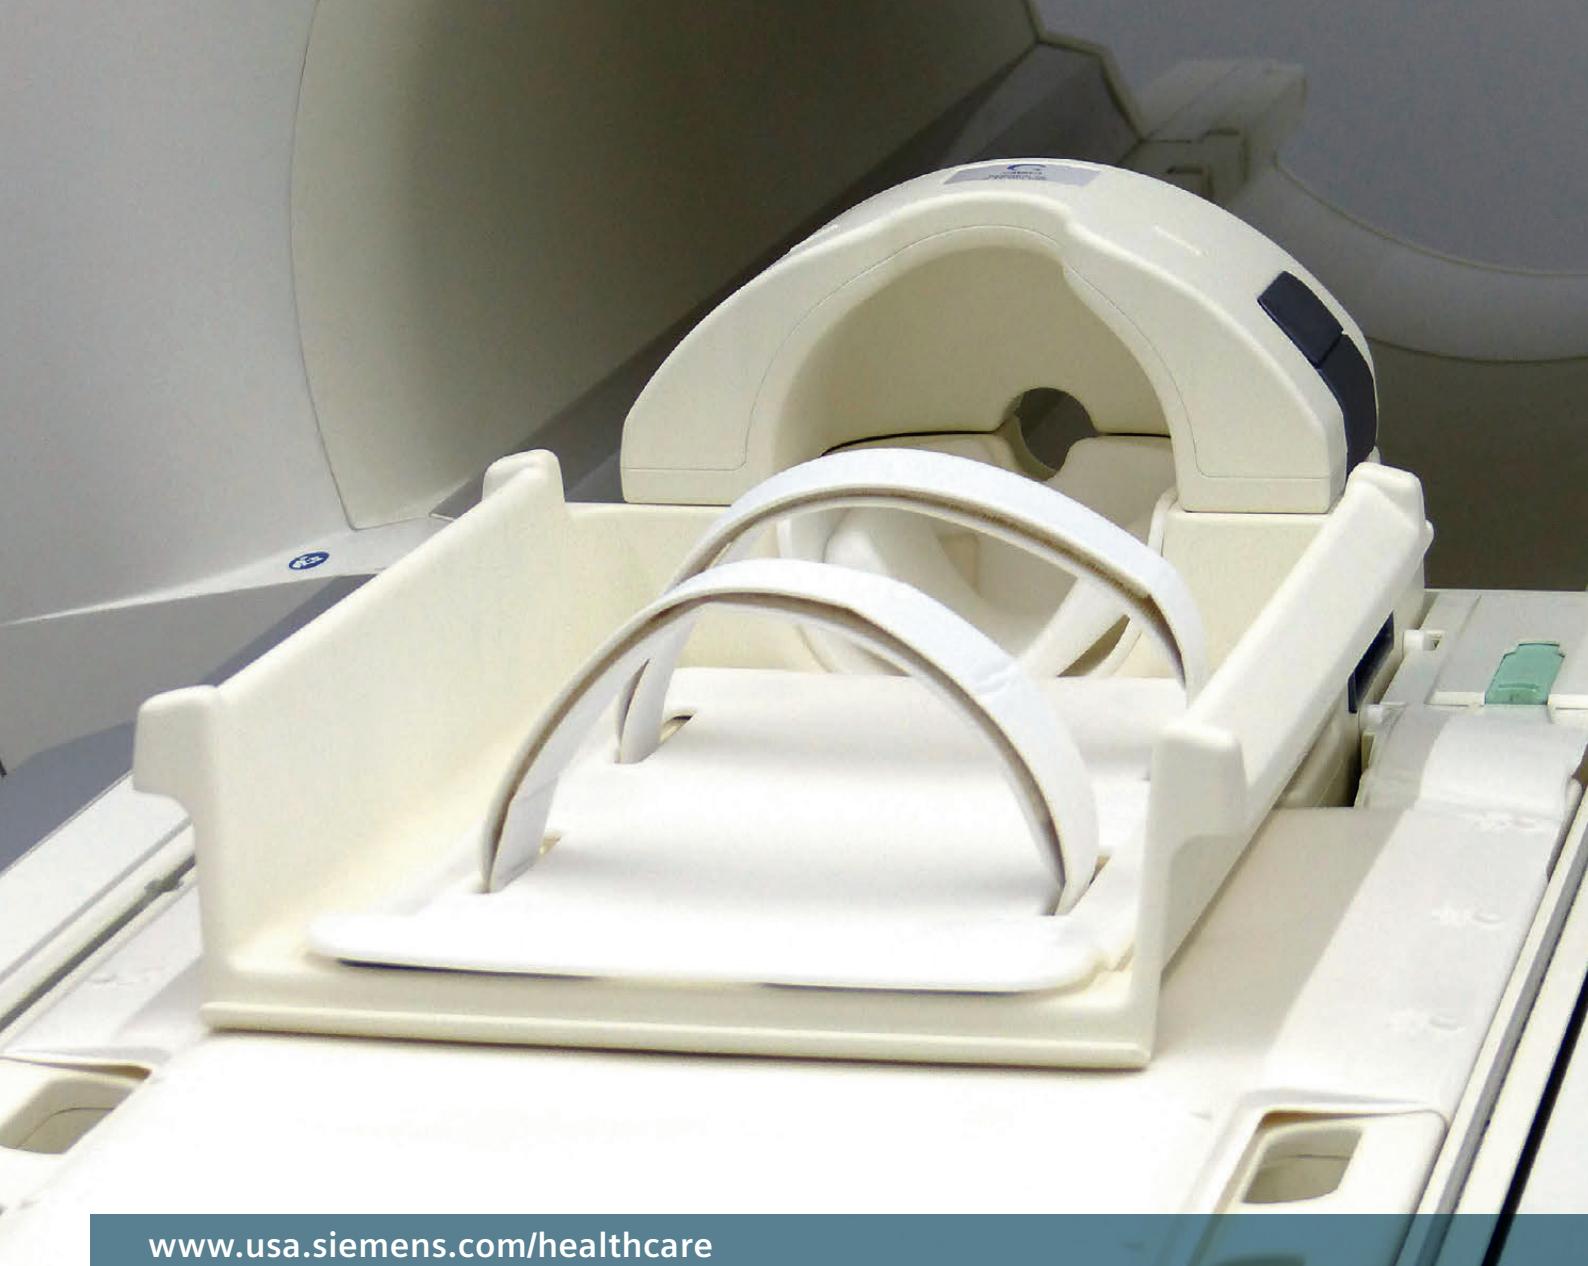

[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

Pediatric 16

Answers for life.

# Pediatric 16<sup>1)</sup>



## General

- 16-channel Head/Neck design with 16 integrated pre-amplifiers, with 13 elements for head imaging (a ring of 7 and a ring of 6 elements) and 3 elements for neck imaging
- Head and neck elements can be used separately for head-only and neck-only imaging
- Neck elements can be switched off when only scanning the brain
- Smooth integration into the table with the Spine coil
- Can be used in combination with other Tim 4G coils (eg Spine and Body) for whole body imaging
- Cable-less with DirectConnect™ technology
- Upper coil part easily removable
- Cushioned head stabilizers (removable)
- No coil tuning required
- iPAT compatible in all directions

## General (Continued)

- Dual-Density Signal Transfer technology with key RF components integrated into the coil
- Comes with a cradle (optional for imaging) which can be used to safely and efficiently transport and position children up to 5 months of age and 10 kgs in weight.
- Features a recess at the bottom of the anterior coil for easier, better positioning of intubation tubes
- 4 cm aperture at the top of the coil to ensure good ventilation

## Applications

- For head and neck examinations of children up to 18 months of age
- Can be combined with other Tim 4G coils for whole body imaging

## Can be combined with

- Spine32
- Body 18
- Flex Large 4
- Flex Small 4
- Special Purpose 4

## Weight

Total Coil	4.4 kg
Anterior Coil	1.4 kg
Cradle	2.3 kg

## Dimensions (L x W x H)

Coil	371 mm x 318 mm x 269 mm
Cradle	685 mm x 319 mm x 123 mm

<sup>1)</sup> MR scanning has not been established as safe for imaging fetuses and infants under two years of age. The responsible physician must evaluate the benefit of the MRI examination in comparison to other imaging procedures

**Global Siemens Headquarters**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**Global Siemens Healthcare Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

**Legal Manufacturer**  
Quality Electrodynamics LLC  
700 Beta Drive, Suite 100  
44143 Mayfield Village  
USA  
Phone: +1 440-484-2228

**SIEMENS**




[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

Head 32

Answers for life.

# Head 32<sup>1)</sup>

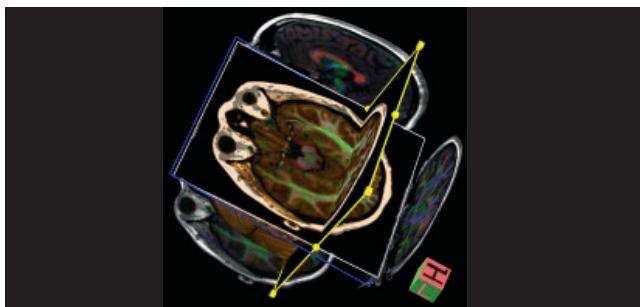

## General (Continued)

- Lower coil part usable without upper part (e.g. for highly claustrophobic patients), designed with 20 elements
- Coil design with comfortable open view for visual stimulation experiments and reduction of claustrophobic response
- Cushions (removable) for head stabilization
- No coil tuning
- iPAT-compatible
- Detachable double mirror assembly

## Applications

- High resolution head proton imaging
- MR angiography of the head
- Functional imaging of the brain

## Lower part can be combined with

- Loop Coils

## Weight

5.6 kg

## Dimensions (L × W × H)

300 mm × 390 mm × 315 mm

## General

- 32-element design with 32 integrated preamplifiers
- Dual-Density Signal Transfer enables ultra-high density coil design by integrating key RF components into the local coil.
- Upper coil part removable, designed with 12 elements

<sup>1)</sup> Prerequisite: Tim [204x48], Tim [204x64], or Tim [204x128] configuration

**Global Siemens Headquarters**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**Global Siemens Healthcare Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

**Legal Manufacturer**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**SIEMENS**



[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

Tx/Rx CP Head Coil

Answers for life.

# Tx/Rx CP Head Coil



## General

- CP Send/Receive head coil with integrated preamplifier
- Upper coil part removable
- Open patient-friendly design
- No coil tuning
- Cushions for patient comfort and stabilization of the head
- Detachable double mirror
- SlideConnect® technology for easy coil set up

## Applications

- Head examinations
- High resolution brain spectroscopy

## Weight

5.2 kg

## Dimensions (L × W × H)

315 mm × 475 mm × 360 mm

**Global Siemens Headquarters**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**Global Siemens Healthcare Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

**Legal Manufacturer**  
Quality Electrodynamics LLC  
700 Beta Drive, Suite 100  
44143 Mayfield Village,  
USA  
Phone: +1 440-484-2228

**SIEMENS**



[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

## 4-Channel Special-Purpose Coil

\*MR scanning has not been established as safe for imaging fetuses and infants under two years of age.  
The responsible physician must evaluate the benefit of the MRI examination in comparison to other imaging procedures.

Answers for life.

# 4-Channel Special-Purpose Coil



## Applications

- Carotids
- Examinations with small Field-of-Views
- Small structures near the surface

## Weight

200 g

## Dimensions (L × W × H)<sup>1)</sup>

90 mm × 143 mm × 20 mm

## General

- 4-channel
- iPAT compatible
- No coil tuning

<sup>1)</sup> without cable

**Global Siemens Headquarters**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**Global Siemens Healthcare  
Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

## Legal Manufacturer

Siemens Shenzhen Magnetic  
Resonance Ltd. (SSMR)  
Siemens MRI Center, Gaoxin C. Ave.  
2nd, Hi-Tech Industrial Park  
Shenzhen 518057  
P.R. China  
Phone: + 86 755-26525421  
Fax: + 86 755-26549253

**SIEMENS**



[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

Sentinelle Endorectal Coil

Answers for life.

# Sentinelle Endorectal Coil<sup>1)</sup>



## General

- Reusable
- Improved coil handling (no inflation necessary)
- Reduced form factor (comparable to endorectal ultrasound probe) vs. conventional inflatable coil
- Reduced prostate deformation through smaller coil diameter
- 2 channels
- Parallel imaging capabilities
- Includes comfortable patient support that provides optimum access
- Held by stable, easily positioned arm (one-knob multi-axis fixation)

## Applications

- Excellent visualization of the prostate, outstanding spectroscopy performance
- Non-invasive preoperative diagnostic evaluation and treatment planning

## Typically combined with

- Body 6/18
- Flex Large 4
- Flex Small 4
- Spine 24/32 (depending on patient positioning) for optimum imaging results

## Technical Data

2 channels

<sup>1)</sup> Alternative name: Prostate 2

**Global Siemens Headquarters**  
Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**Global Siemens Healthcare Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

**Legal Manufacturer**  
Sentinelle Medical Inc.  
555 Richmond St. West Suite 800  
Toronto, Ontario, M5V 3B1  
Canada  
Phone: +1 416-366-4994  
Fax: +1 416-594-9696  
[www.sentinelomedical.com](http://www.sentinelomedical.com)

**SIEMENS**



[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

Application Packages

Answers for life.

# Application Packages

## **Quiet Suite**

Quiet Suite enables complete, quiet examinations of the brain and large joints. Quiet Suite includes QuietX, an algorithm which enables intelligent gradient optimization to substantially reduce noise without significant compromise to image quality or scan time.

In addition, Quiet Suite includes PETRA, a 3D T1-weighted sequence which is barely audible above background noise. When used with a Tx/Rx coil, PETRA is inaudible.

- Quiet prescan normalize and quiet localizers
- QuietX TSE, SE and GRE sequences for T1, T2, and DarkFluid contrasts
- QuietX SWI<sup>1)</sup>
- PETRA (Pointwise Encoding Time reduction with Radial Acquisition) for inaudible 3D T1-weighted imaging
- Optimized Quiet protocols for the brain, spine and large joints

## **FREEZEit**

FREEZEit combines the two applications TWIST-VIBE and StarVIBE.

FREEZEit facilitates high quality diagnostic MR imaging of the liver. Based on the excellent soft tissue contrast that MRI inherently offers, FREEZEit now adds imaging speed and motion compensation to liver MRI. This allows imaging the entire arterial phase of the liver with multiple 3D datasets within seconds while maintaining a high spatial image resolution. Furthermore, the motion compensation of FREEZEit enables contrast-enhanced liver imaging during free breathing.

### StarVIBE

StarVIBE is a motion insensitive VIBE sequence using a stack-of-stars trajectory. It allows body imaging in free breathing mode, providing a solution for patients without breath hold capabilities.

### TWIST-VIBE

TWIST VIBE is a new fast, high-resolution 4D imaging sequence for multi-arterial liver imaging. It is a VIBE sequence with CAIPIRINHA capability providing high spatial resolution. The view-sharing mode provides temporal information to ensure the right contrast timing for different lesions. Dixon is used for fat-water separation.

## **LiverLab<sup>2)</sup>**

Within the Abdomen Dot Engine, LiverLab is a system guided workflow to examine the hepatic fat and iron status. The Inline First look Dixon sequence gives the user a first overview of possible fat and/or iron overload in the whole liver. Based on the resulting images, liver segmentation runs without user interaction. If further evaluation is needed, the user can choose from two methods: HISTO is a push-button single breath-hold single voxel spectroscopy method to calculate fat signal fraction as well as water R2; Multi-echo Dixon VIBE is an image based method to calculate maps such as water, fat, fat signal fraction, and R2\*.

<sup>1)</sup> Precondition syngo SWI

<sup>2)</sup> Prerequisite: Abdomen Dot Engine

### **Advanced WARP<sup>1)</sup>**

Advanced WARP enables the reduction of gross metal artifacts (i.e. through-plane artifacts) caused by large orthopedic implants. It contains the 2D TSE based SEMAC technique and is especially useful in the case of hip and knee joint replacements. Available protocols include T1-weighted, T2-weighted, proton density and STIR contrast.

### **RESOLVE**

RESOLVE (Readout Segmentation Of Long Variable Echo-trains) delivers high resolution diffusion-weighted imaging (DWI) for visualizing the diffusion properties of fine anatomical structures. Additionally, this technique is largely insensitive to susceptibility effects, providing detailed anatomy-true diffusion imaging for brain, spine, breast and prostate. In combination with the DTI Tractography package, RESOLVE enables excellent white-matter tract imaging even in the most challenging areas, such as the cervical spine.

- Diffusion-weighted, readout-segmented (multi shot) EPI sequence for high-resolution susceptibility-insensitive DWI
- Variable number of readout segments for greater flexibility
- 2D navigator-based phase correction for pulsation artifact reduction and automatic reacquisition of corrupted data
- Inline calculation of diffusion tensor (DTI) and diffusion parameter maps

### **Tim Planning Suite**

Easy planning of extended Field of View examinations in an efficient way using Set-n-Go protocols. It allows planning of several stations at once e.g. on composed localizer images. The overlap of slice groups can be adjusted. All stations can have independent parameter settings although they are displayed together. A special coupling mode allows easy positioning of all stations at once according to the patient's anatomy. Fully supports scan@center and Phoenix functionality.

- Tim Planning UI with optimized layout for slice positioning
- Ready to use Set-n-Go protocols for different clinical questions
- Integrated toolbar for fast advanced slice planning: FoV-Plus, FoV-Minus, AlignParallel, AlignFieldOfViews

### **Tim Whole Body Suite**

MAGNETOM Skyra features a full effective Field of View of 205 cm. Table movement to its full extent can be controlled from the syngo Acquisition Workplace. The large FoV helps in imaging potential metastases with sequences such as TIRM (Turbo Inversion Recovery Magnitude). Whole body MR Angiography is possible on the entire volume with iPAT.

- Max. scan range of 205 cm
- Protocols and programs for whole body MR Angiography and metastases detection

<sup>1)</sup> MR imaging of patients with metallic implants brings specific risks. However, certain implants are approved by the governing regulatory bodies to be MR conditionally safe. For such implants, the previously mentioned warning may not be applicable. Please contact the implant manufacturer for the specific conditional information. The conditions for MR safety are the responsibility of the implant manufacturer, not of Siemens.

### **MapIt**

MapIt provides protocols and Inline calculation functionality to obtain parametric maps of T1, T2, T2\*, R2 and R2\* properties of the imaged tissue. The application range includes cartilage evaluation of joints and also the evaluation of other organs such as liver, kidney or prostate.

In particular, MapIt may aid the user in the diagnosis of joint disorders, based on the T1, T2, and T2\* properties of the cartilage.

- 3D VIBE sequence for Inline T1 mapping
- Multi-echo spin echo sequence for Inline T2/R2 mapping
- Multi-echo gradient echo sequence for Inline T2\*/R2\* mapping
- Protocols for fully automated Inline parametric mapping

### **SWI (Susceptibility Weighted Imaging)**

Siemens-unique sequence technique for Susceptibility Weighted Imaging

- Visualization of local changes of the magnetic field due to tissue properties in general and due to the presence of deoxygenated blood or blood decomposition products
- 3D GRE sequence with full flow compensation to support venous angiography
- Enhanced susceptibility weighting of the magnitude images by phase images

### **Inline BOLD Imaging (Blood Oxygen Level Dependent)**

Examination of intrinsic susceptibility changes in different areas of the brain, induced by external stimulation (e.g. motor or visual). Automatic real-time calculation of z-score (t-test) maps with Inline Technology, for variable paradigms.

- Compatible with single-shot EPI with high susceptibility contrast for fast multi-slice imaging
- ART (Advanced Retrospective Technique) for fully automatic 3D retrospective motion correction, for 6 degrees of freedom (3 translations and 3 rotations)
- Mosaic images for efficient storage and transfer of large data sets
- 3D spatial filtering
- Inline calculation of t-statistics (t-maps) based on a general linear model (GLM) including the hemodynamic response function and correcting for slow drifts
- Overlay of inline calculated statistical results on the EPI images

### **Inline Perfusion**

Automatic real-time calculation of Global Bolus Plot (GBP), Percentage of Baseline at Peak map (PPB) and Time-to-Peak map (TTP) with Inline technology

### **3D PACE**

3D PACE (Prospective Acquisition CorrEction) enhances Inline BOLD imaging with motion correction during the acquisition of a BOLD exam.

In contrast to a retrospective motion correction that corrects previously acquired data, the unique 3D PACE tracks the head of the patient, correcting for motion in real time during the acquisition. This increases the data quality beyond what can be achieved with a retrospective motion correction. As a result the sensitivity and specificity of BOLD experiments are increased.

- Fully automatic 3D prospective motion correction during data acquisition, for 6 degrees of freedom (3 translations and 3 rotations)
- Motion correction covering the complete 3D volume
- Provides high accuracy
- Substantially reduced motion-related artifacts in t-test calculations
- Significantly increased signal changes in the activated neuronal volume
- Increased functional MRI (fMRI) sensitivity and specificity

### **DTI (Diffusion Tensor Imaging)**

Acquisition of data sets with multi-directional diffusion weighting to assess anisotropic diffusion properties of brain tissue

- Measurement of up to 256 directions of diffusion weighting with up to 16 different b-values
- Inline calculation of the diffusion tensor
- Inline calculation of Fractional Anisotropy (FA) maps (grey-scale as well as color-coded for principle diffusion direction), Apparent Diffusion Coefficient (ADC) maps and trace-weighted images based on the tensor
- Measurement of user defined diffusion directions (Free Mode)

Diffusion Spectrum Imaging (DSI) is a type of diffusion weighted imaging. This technique allows for more accurate fiber tracking than conventional diffusion techniques due to a higher sensitivity to intra-voxel diffusion caused by crossing fiber tracks. The DSI acquisition technique comes as part of the DTI package.

- Cartesian sampling approach performed in q-space
- Measure multiple directions with independent b-values
- Up to 514 different directions
- Up to 514 different directions

### **Inline Composing**

Automatic anatomical or angiographic composing of multiple adjacent coronal or sagittal images for presentation and further evaluation.

Composed images can be automatically loaded into Graphical Slice Positioning for planning purposes.

## **TWIST**

This package contains a Siemens-unique sequence and protocols for advanced time-resolved (4D) MR angiography and dynamic imaging in general with high spatial and temporal resolution. It offers temporal information of vessel filling in addition to conventional static MR angiography. TWIST can be combined with water excitation.

New reconstruction algorithms for iPAT<sup>2</sup> enable highly efficient multi-directional parallel imaging

## **NATIVE**

Integrated software package with sequences and protocols for non-contrast enhanced 3D MRA with high spatial resolution. NATIVE particularly enables imaging of abdominal and peripheral vessel

NATIVE offers:

- Non-contrast MRA
- Separate imaging of arteries and veins
- Visualization of – e.g. – renal arteries or peripheral vessels

The syngo NATIVE package comprises:

- NATIVE TrueFISP
- NATIVE SPACE

## **ASL (Arterial Spin Labeling) 2D**

Arterial Spin Labeling (ASL) is an MR technique using the water in arterial blood as an endogenous contrast agent to evaluate perfusion noninvasively. ASL assists in the evaluation of human brain perfusion and function physiology by giving information on relative cerebral blood flow.

ASL is capable of high spatial resolution perfusion imaging.

ASL may also be useful in basic neuroscience, e.g. for studies of functional CBF changes.

- iPAT compatible
- Includes 3D PACE motion correction for increased reliability
- Fully automated Inline calculation of relCBF color maps
- Supports the “Pulsed Arterial Spin Labeling” – technique (PASL)

## **ASL (Arterial Spin Labeling) 3D**

Arterial Spin Labeling (ASL) is an MR technique using the water in arterial blood as an endogenous contrast agent to evaluate perfusion noninvasively. ASL 3D enables the physician to qualitatively assess perfusion throughout the whole brain without the use of a contrast agent.

ASL 3D is a tool to acquire high spatial resolution brain perfusion-weighted images.

- Based on a 3D TGSE sequence for minimal low susceptibility and full brain coverage
- Higher SNR, optimized contrast uniformity and reduced motion sensitivity.
- Perfusion maps can be easily fused with anatomical images for detail evaluation in Neuro 3D<sup>1)</sup>.

<sup>1)</sup> Optional

## Advanced Cardiac

This package contains special sequences and protocols for advanced cardiac imaging including 3D and 4D BEAT functionalities. It supports advanced techniques for ventricular function imaging, dynamic imaging, tissue characterization, coronary imaging, and more.

BEAT is a unique tool for fast and easy cardiovascular MR imaging. It provides 1-click switch from cine imaging to tagging for wall motion evaluation and 1-click switch from 2D to 3D imaging. BEAT automatically adjusts all parameters associated with the changes.

Cardiac and vessel morphology	<ul style="list-style-type: none"><li>• Multi echo technique thalassemia assessment</li><li>• 3D aortopathy imaging with free breathing (SPACE)</li></ul>
Morphology and global or regional ventricular wall motion analysis with BEAT	<ul style="list-style-type: none"><li>• 3D cine acquisition for full CT-like heart coverage</li><li>• 2D segmented FLASH for visualization of the regional wall motion using various tagging techniques (grid or stripes)</li></ul>
Dynamic myocardial imaging with BEAT	<ul style="list-style-type: none"><li>• Ultra-fast, high-SNR sequence for imaging with GRE EPI contrast for stress and rest exams</li></ul>
Tissue characterization with BEAT	<ul style="list-style-type: none"><li>• Robust myocardial tissue characterization with 3D PSIR (phase-sensitive inversion recovery)</li><li>• Fast and complete coverage of the myocardium with IR 3D FLASH and TrueFISP</li></ul>
Coronary imaging with BEAT	<ul style="list-style-type: none"><li>• 3D whole heart non-contrast coronary MRA</li><li>• 3D whole heart MRA with advanced free-breathing navigator compensating diaphragm shifts during the acquisition (motion-adaptive respiratory gating)</li></ul>

## MyoMaps<sup>1)</sup>

On the basis of fully system guided HeartFreeze Inline Motion Correction, MyoMaps provides pixel-based T1 and T2 myocardial tissue quantification. Results are presented in fully system guided inline colored parametric maps of the heart.

T1 Map	<ul style="list-style-type: none"><li>– based on Modified Look-Locker Inversion Recovery T1 mapping for e.g. detection of global, diffuse and sometimes subtle myocardial pathologies.</li></ul>
T2 Map	<ul style="list-style-type: none"><li>– based on T2-prepared single shot TrueFISP T2 mapping for e.g. depiction of cardiac edema.</li></ul>

<sup>1)</sup> Prerequisite: Tim [204x64], or [204x128] configuration

## Flow Quantification

Special sequences for quantitative flow determination studies

- Non-invasive blood/CSF flow quantification
- ECG Triggered 2D phase contrast with iPAT support
- Retrospective reconstruction algorithms for full R-R interval coverage

## Interactive Realtime

Sequences for interactive real-time scanning

Uses ultra-fast Gradient Echo sequences for high image contrast

Real-time reconstruction of the acquired data

The user can navigate in all planes on-the-fly during data acquisition

- Real-time cardiac examinations
- Real-time interactive slice positioning and slice angulation for scan planning

## Single Voxel Spectroscopy

Integrated software package with sequences and protocols for proton spectroscopy. Streamlined for easy push-button operation

- Matrix Spectroscopy – phase-coherent signal combination from several coil elements for maximum SNR based on the Head/Neck 20
- Spectral suppression (user definable parameter) to avoid lipid superposition
- Spectroscopy can be combined with Free-Breath Prospective Acquisition Correction (2D-Phase navigator) when needed
- Up to 8 regional saturation (RSat) bands for outer volume suppression can be defined by the user.
- Automatic reference scan for inline correction
- Physiological triggering (ECG, pulse, respiratory or external trigger) in order to avoid e.g. breathing artifacts.
- Spectroscopy relevant GRE-based shim protocols provided
- Clinical applications: brain, breast, prostate

## SVS Techniques SE and STEAM

- Short TE's available
- Fully automated adjustments including localized shimming and adjustment of water suppression pulses
- Also available: Interactive adjustments and control of adjustments
- Optimized protocols for brain applications

## **CSI 2D: Chemical Shift Imaging**

Integrated software package with sequences and protocols for Chemical Shift Imaging (CSI)

Extension of the Single Voxel Spectroscopy (SVS) package, offering the same level of user-friendliness and automation

- Matrix Spectroscopy – phase-coherent signal combination from several coil elements for maximum SNR with configurable prescan-based normalization for optimal homogeneity
- 2D Chemical Shift Imaging
- Hybrid CSI with combined volume selection and Field of View (FoV) encoding
- Short TEs available (30 ms for SE, 20 ms for STEAM)
- Automated shimming of the higher order shimming channels for optimal homogeneity of the larger CSI volumes
- Weighted acquisition, leading to a reduced examination time compared to full k-space coverage while keeping SNR and spatial resolution
- Outer Volume Suppression
- Spectral Suppression
- Semi-LASER sequence available for CSI examination of the brain

## **CSI 3D: Chemical Shift Imaging (Continued)**

Integrated hardware and system software package to prepare the MAGNETOM system for imaging and spectroscopy with nuclei other than  $^1\text{H}$ . Coils, pre-amplifiers and optimized pulse sequences are not included.

- Matrix Spectroscopy – phase-coherent signal combination from several coil elements for maximum SNR with configurable prescan-based normalization for optimal homogeneity
- 3D Chemical Shift Imaging
- Hybrid CSI with combined volume selection and Field of View (FoV) encoding
- Short TEs available (30 ms for SE, 20 ms for STEAM)
- Automated shimming of the higher order shimming channels for optimal homogeneity of the larger CSI volumes
- Weighted acquisition, leading to a reduced examination time compared to full k-space coverage while keeping SNR and spatial resolution
- Outer Volume Suppression
- Spectral Suppression
- Protocols for prostate spectroscopy

## **M multinuclear Support<sup>1)</sup>**

Integrated software package with sequences and protocols for Chemical Shift Imaging (CSI)  
Extension of the SVS package, offering the same level of user-friendliness and automation

- Supports the generation of RF pulses for  $^3\text{He}$ ,  $^7\text{Li}$ ,  $^{13}\text{C}$ ,  $^{17}\text{O}$ ,  $^{19}\text{F}$ ,  $^{23}\text{Na}$ ,  $^{31}\text{P}$  and  $^{129}\text{Xe}$  and allows to receive signals at the respective frequencies
- Supports mono and double resonant send/receive coils ( $^1\text{H}/x$ -nucleus)
- Imaging with the nuclei  $^3\text{He}$ ,  $^7\text{Li}$ ,  $^{13}\text{C}$ ,  $^{17}\text{O}$ ,  $^{19}\text{F}$ ,  $^{23}\text{Na}$ ,  $^{31}\text{P}$  and  $^{129}\text{Xe}$  and spectroscopy with the nuclei  $^7\text{Li}$ ,  $^{13}\text{C}$ ,  $^{19}\text{F}$ , and  $^{31}\text{P}$
- Spectroscopic and imaging experiments using the  $^1\text{H}$  Nuclear Overhauser Effect (NOE) and using  $^1\text{H}$  decoupling
- A basic pulse sequence serves as a starting point for flexible design of x-nucleus sequences using the development environment IDEA

<sup>1)</sup> Prerequisite: Tim [204x48], Tim [204x64], and Tim [204x128]

## Multinuclear Spectroscopy<sup>1)</sup>

CSI spectroscopy sequence and protocols for x-nuclei

- The CSI sequence supports measurements with all frequencies supported by the hardware
- Basic measurement and post-processing protocols for <sup>7</sup>Li, <sup>13</sup>C, <sup>17</sup>O, <sup>19</sup>F and <sup>31</sup>P
- The sequence supports NOE (Nuclear Overhauser Effect) and <sup>1</sup>H decoupling
- ECG triggering available
- Weighted acquisition available

## GRACE (GeneRALized breast speCtroscopy Exam)

SVS technique (spin echo sequence) optimized for breast spectroscopy.

The technique contains a special spectral lipid suppression pulse (user definable) for lipid signal reduction.

Siemens unique water reference detection to visualize the normalized choline ratio.

Online frequency shift correction for reduction of breathing related artifacts, Inline implementation – no additional user interaction is required.

Clinical applications:

- GRACE may assist the physician to improve the specificity of tumor diagnoses
- GRACE may be a helpful tool for therapy monitoring

## syngo Security

Security package for general regulatory security rules

The option supports customers to achieve compliance with HIPAA (Health Insurance and Accountability Act)

- User authentication
- Restricts access to functions and data through privileges and permissions
- Logs relevant data security information in audit trail

## MR Elastography

MR Elastography is a tool that helps the physician to non-invasively assess relative stiffness of liver tissue.

MR Elastography includes pulse sequence and processing software.\*

- Sequence and protocols with 2D gradient-echo sequences with cyclic motion-encoding gradients (MEG)

Advanced Siemens implementation

- iPAT enables shortened breath-hold time
- Fully integrated processing of the elastogram at the scanner
- Completely automated calculation of wave images and corresponding elastograms
- Confidence map for reliability

\* Please note that this functionality can only be used in combination with a dedicated hardware, which is not part of the MR Elastography package

### **syngo Expert-i<sup>1)</sup>**

Interactive real-time access to imaging data and exam information from any PC within the hospital network during the MR exam.

Until now, radiologists or other experts had to stop what they were doing and go to the MR scanner to see the acquired images, help with the scan set-up, or answer an open question.

Now, questions can be addressed quickly and efficiently via remote PC.

---

#### Benefits of syngo Expert-i

- Excellent results right from the first examination
- Streamlined workflow and faster patient throughput
- Reduced repeat rates with a check on images while the patient is still in the examination room
- Reduced training effort by enabling expert assistance for specialized procedure

### **syngo Remote Assist**

Direct computer link to the local Siemens service department or the Siemens service centers (via router with telephone connection)

---

#### Image transfer for further evaluation

- Image and file transfer in batch mode
- Reading of entries in the error logbook
- Remote trouble shooting
- Remote access to service manuals written in easy-to-use HTML format
- Remote access to Service Site Database
- Start of preventive maintenance and quality assurance routines.  
Provided in conjunction with a service contract with Siemens (UPTIME Services)
- Remote access granted only with permission of the institution
- Data security is ensured by secure access

### **IDEA (Integrated Development Environment for Applications)**

Extensive programming environment used to create and modify pulse sequences, offering a maximum of flexibility

---

Based on C++ for Windows 7. Sequences and RF pulses are displayed in a visual interface

---

#### Features

- Allows direct access to the Image Calculation Environment (ICE), and to all protocols
- Testing the generated code is extensively supported by the debugger and the simulation program
- IDEA is also usable on any standard PC with operating system Windows XP making developments independent of the MR system

---

#### Processing plug-ins

- For development or modification of user-defined image processing steps which may be integrated into the measurement protocols
  - Individual processing is secured by a number of functions (e.g. TTP and MTT), useful for neuro or perfusion imaging

---

#### Prerequisite

- IDEA training course

<sup>1)</sup> Within hospital enterprise

On account of certain regional limitations of sales rights and service availability, we cannot guarantee that all products included in this brochure are available through the Siemens sales organization worldwide. Siemens reserves the right to modify the design, packaging, specifications, and options described herein without prior notice.

Any technical data contained in this document may vary within defined tolerances. Original images always lose a certain amount of detail when reproduced.

Please find fitting accessories:  
[www.siemens.com/medical-accessories](http://www.siemens.com/medical-accessories)

Please contact your local Siemens sales representative for the most current information.

#### Local Contact Information

##### In the USA

Siemens Medical Solutions USA, Inc.  
51 Valley Stream Parkway  
Malvern, PA 19355  
Phone: +1 888-826-9702  
Phone: +1 610-448-4500  
Fax: +1 610-448-2254

##### In Asia

Siemens Healthcare Sector  
Asia Pacific Headquarters  
The Siemens Center  
60 MacPherson Road  
Singapore 348615  
Phone: +65 6490 6000  
Fax: +65 6490 6001

##### In Japan

Siemens Japan K.K.  
Gate City Osaki West Tower  
1-11-1 Osaki, Shinagawa-ku  
Tokyo 141-8644  
Phone: +81 3 5423 8411

##### Global Business Unit

Siemens Healthcare Sector  
Magnetic Resonance  
Henkestr. 127  
DE-91052 Erlangen  
Germany  
Phone: +49 9131 84-0

##### Global Siemens Headquarters

Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

##### Global Siemens Healthcare

**Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

##### Legal Manufacturer

Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**SIEMENS**



[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

Post-processing Packages

Answers for life.

# Post-processing Packages

All post-processing packages are separately available for the **syngo** Acquisition Workplace or the **syngo** MR Workplace.

## **syngo Argus 4D Ventricular Function**

**syngo Argus 4D VF** software processes MR cine images of the heart and generates quantitative results for physicians in the diagnostic process. It provides volumetric cardiac data of a given patient very quickly and easily. Parametric results and volume-time curves are being calculated upon automatic creation and adaptation of a 4D model of the left ventricle. The resulting 4D model of the patient's heart can be visualized superimposed to anatomical images as reference.

**syngo Argus 4D VF** includes the well-known functionalities of Argus Function, the automated tool for cardiac function evaluation.

- Fully automatic left ventricle and semi-automatic right ventricle segmentation
- Easy user guidance with graphical selection of ED, ES, basal and apical slices
- Volumetric and regional wall motion analysis (e.g. stroke volume and bull's-eye plots)

## **Argus Flow**

Automated tool for analysis of blood and CSF flow.

- Semi-automatic detection of regions of interest over time
- Color-coded display of velocity values
- Calculation of flow and velocity parameters (e.g. peak velocity, average velocity, flow, integral flow)

## **Vessel View**

Interactive analysis of vessel disease using MR or CT angiography data.

Viewing with VRT, MPR, or MIP mode.

- Semi-automatic detection of vessel segments
- Quantification of changes in vessel size
- Protocol-based software for workflow support
- Creates and edits DICOM structured reports

## **Vessel View Artery-Vein-Separation**

This package allows semi-automated segmentation and separation of arteries and veins, as well as suppression of surrounding tissue. Supports modes allowing the display of only arteries or only veins, or arteries and veins together in different colors.  
(Prerequisite: Vessel View)

## **3D VRT Volume Rendering Technique**

3D visualization for clearer depiction of complex anatomy and relationship of anatomy in 3D for e.g. VIBE imaging.

More productive surgical planning and discussion with referring physicians.

- Integrated with other 3D functionality
- Color image creation
- Color gallery of icon presets
- Additional threshold-based segmentation of 3D objects
- Volume measurements

### **syngo BOLD 3D Evaluation**

Comprehensive processing and visualization package for BOLD fMRI. It provides a full set of features for clinical fMRI, as well as advanced features for more research oriented applications.

This package provides statistical map calculations from BOLD datasets and enables the visualization of task-related areas of activation with 2D or 3D anatomical data.

On the syngo Acquisition Workplace the unique Inline function of BOLD 3D Evaluation merges, in real time, the results of ongoing BOLD imaging measurements with 3D anatomical data. Additionally, evolving signal time courses in task-related areas of activation can be displayed and monitored.

Functional and anatomical image data can be exported for surgical planning as DICOM datasets, additionally all color fused images and results can be stored or printed.

- Statistical map generation: paradigm definition, calculation of t-value map with General Linear Model or t-test
- 3D Visualization: fused display of fMRI results, color t-value maps on anatomical datasets
- Inline 3D real time monitoring of the fMRI acquisition
- On-the-Fly Adjustment for t-value thresholding, 3D clustering, and opacity control
- Data export to neurosurgical planning software
- Fly Through the Volume: Zoom, pan, rotate, cut planes
- Analysis of Signal Time Curves
- Data Quality Monitoring: B0 field map, cine display of the BOLD time series
- Archiving & Distribution of results and views as colored DICOM images and bit maps
- If the respective options are available, results from Diffusion Tensor Imaging and DTI Tractography can be displayed together with fMRI results and anatomy

## DTI Evaluation

Offline post-processing to generate and visualize parametric maps derived from the diffusion tensor in order to assess anisotropic diffusion properties of brain tissue

- Generation of diffusion maps based on tensor including: Fractional Anisotropy (FA), Volume Ratio (VR), trace-weighted, ADC, E1–E3, E1, linear, planar, tensor maps
- Display of maps in scalar mode (grey scale), vectorized mode (directions color coded) and tensorized mode (using tensor graphics like ellipsoid or cuboids); overlay of maps onto anatomical images
- Side by side display of several maps (e.g. ADC, FA, and trace-weighted) and anatomy for simultaneous ROI based evaluation; generation of a results table in order to support the assessment of diseases of the white matter
- Integrated into Neuro 3D taskcard: display of DTI maps in the context of an anatomical 3D data set; arbitrary oriented clip planes allow to explore the 3D volume
- Fused display with white matter tracts if the "DTI Tractography" option is present.
- Export of reformatted images for neuro navigation
- Together with the "BOLD 3D Evaluation" option: simultaneous display of anatomical, fMRI, and DTI data

## syngo DTI Tractography

syngo DTI Tractography allows the visualization of multiple white matter tracts based on diffusion tensor imaging data. DTI Tractography is optimized to support the presurgical planning and to allow for neuro physiological research with respect to connectivity and white matter pathology.

- Advanced 3D visualization of white matter tracts in the context of 2D or 3D anatomical and DTI datasets
- Texture Diffusion, a highly versatile in-plane visualization of white matter tracts, allows to display and read DTI Tractography results on PACS reading stations and in the OR
- Seed points for tracking with single ROI and with multiple ROIs to assess connectivity
- Tract and seeding ROI statistics (mean / max FA value, min / mean / max ADC value, and more)
- DICOM export of views, HTML export of Tract, and seeding ROI statistics
- Interactive QuickTracking displays the tract originating from the mouse pointer position while moving over the DTI data set

## **Neuro Perfusion Evaluation**

Dedicated task card for quantitative processing of neuro perfusion data.

- Color display of relative Mean Transit Time (relMTT), relative Cerebral Blood Volume (relCBV), and relative Cerebral Blood Flow (relCBF)
- Flexible selection of Arterial Input Function (AIF) for reliable analysis

## **Composing**

Composing of images from different table positions.

- Automatic and manual composing of sagittal and coronal images
- Dedicated algorithms for spine, angiography, and adaptive composing algorithms
- Measurement on composed images (angle, distance)

## **Fly Through**

Simulated endoscopic views of the inside of bronchi, vessels, colon, and any other hollow structures.

Multi-modality application for CT, MR, and 3D AX data.

Fully integrated into the familiar 3D workflow and user interface.

- Ready-to-use from day one
- One click to action

## **Spectroscopy Evaluation**

Integrated software package with extensive graphical display functionality

Comprehensive and user-friendly evaluation of spectroscopy data

Display of CSI data as colored metabolite images or spectral overview maps, overlayed on anatomical images

- Export of spectroscopy data to a user-accessible file format
- Relative quantification of spectra, compilation of the data to result table

Peak normalization tissue, water or reference

Dedicated Single Voxel Spectroscopy breast evaluation protocols

## **Image Fusion**

Image fusion of multiple 3D data sets with alpha blending, i.e. overlay of two images with manual setting of the opacity

- Multiple 3D data sets from different modalities (MR, CT, Nuclear Medicine, PET)
- Visual alignment, automatic registration, or landmark based registration

### **syngo BreVis\***

syngo BreVis is easy-to-use, fast, and reliable. Quick preprocessing, which includes elastic motion correction in case of patient movement, enables efficient breast reading and reporting.

This flexible tool provides various functionalities such as:

- Intelligent visualization of 2D-, 3D- and 4D-datasets according to customized layouts, e.g. dedicated layouts for intervention, multiple time point follow-up
- Elastic Motion Correction
- Multi-modality viewing capabilities
- Reporting according to BI-RADS\*\* standard
- On-the-fly reconstruction of subtracted images
- Auto-MultiPlanar Reformatted images (MPR) and auto-Maximum Intensity Projection (MIP)
- Real-time display and analysis of kinetic parameters (timecourse evaluation, color overlay maps to visualize angiogenesis or curve types)
- Graphical volume statistics of lesion enhancement
- Calculation of lesion volumes

\* Not available on AQWP

\*\* Breast Imaging Reporting and Data System

### **syngo BreVis Biopsy**

syngo BreVis Biopsy is a professional solution for a fast and accurate MR biopsy workflow with automatic calculation of target coordinates.

The easy-to-handle workflow enables shorter examination times for both patient and operator. The user interface offers a guide for MR breast interventional planning, supporting following biopsy system:

- For example Sentinel Breast coils, 4-channel BI Breast Coil
- Related accessories including the post-pillar and grid method syngo BreVis Biopsy enables path planning directly at the scanner – no sending of data over the network required.

### **syngo Breast Biopsy Software**

Easy to use syngo-based post-processing software helps finding the coordinates for needle insertion for biopsy or localization of potential breast lesions detected by MR

Allows calculation of the coordinates after clicking the center of the potential lesion and the 0 marker of a third party breast biopsy device

- Printout of working sheet
- Multi-lesion calculation

Prerequisites:

- 4-channel BI breast coil or Large Loop Flex coil

### **Soft Tissue Motion Correction**

3D elastic motion correction, for offline 3D correction in all directions over entire 2D and 3D data sets suitable for e.g. soft tissue MR exams

Allows higher conspicuity and accuracy especially for multi-focal lesion detection

New image data is reconstructed and saved in a separate series within the patient browser. It can be combined with the original non-corrected image data

## **syngo Tissue 4D**

syngo Tissue 4D is a tool to aid in the detection of tumor tissues in organs such as the liver.  
It is an application card for visualizing and post-processing dynamic 3D datasets.

Evaluation options	<ul style="list-style-type: none"><li>• Standard curve evaluation</li><li>• Curve evaluation according to a pharmacokinetic model</li></ul>
Visualization features	<p>4D visualization (3D and over time)</p> <p>Color display of parametric maps describing the contrast media kinetics such as:</p> <ul style="list-style-type: none"><li>• Transfer constant (Ktrans)</li><li>• Reflux constant (Kep)</li><li>• Extra vascular extra cellular volume fraction (Ve)</li><li>• Plasma volume fraction (Vp)</li><li>• Initial Area-Under-Curve (iAUC) for the first 60 seconds</li></ul>
	<p>Additional visualization of 2D or 3D morphological dataset</p>
Post-processing features	<p>Elastic 3D motion correction</p> <p>Fully automatic calculation of subtracted images</p>
Kinetic model	<p>Kinetic calculation on a pixel-by-pixel basis using a 2-compartment model.</p> <p>Calculation is based on the Tofts model. Various model functions are available.</p> <p>Manual segmentation and calculation on the resulting images.</p> <p>The following resulting images can be saved as DICOM images:</p> <ul style="list-style-type: none"><li>• 3D motion-corrected, dynamic images</li><li>• Colored images</li><li>• Storage of calculated results</li><li>• Export of results in the relevant layout format</li></ul>

On account of certain regional limitations of sales rights and service availability, we cannot guarantee that all products included in this brochure are available through the Siemens sales organization worldwide. Siemens reserves the right to modify the design, packaging, specifications, and options described herein without prior notice.

Any technical data contained in this document may vary within defined tolerances. Original images always lose a certain amount of detail when reproduced.

Please find fitting accessories:  
[www.siemens.com/medical-accessories](http://www.siemens.com/medical-accessories)

Please contact your local Siemens sales representative for the most current information.

#### Local Contact Information

##### In the USA

Siemens Medical Solutions USA, Inc.  
51 Valley Stream Parkway  
Malvern, PA 19355  
Phone: +1 888-826-9702  
Phone: +1 610-448-4500  
Fax: +1 610-448-2254

##### In Asia

Siemens Healthcare Sector  
Asia Pacific Headquarters  
The Siemens Center  
60 MacPherson Road  
Singapore 348615  
Phone: +65 6490 6000  
Fax: +65 6490 6001

##### In Japan

Siemens Japan K.K.  
Gate City Osaki West Tower  
1-11-1 Osaki, Shinagawa-ku  
Tokyo 141-8644  
Phone: +81 3 5423 8411

##### Global Business Unit

Siemens Healthcare Sector  
Magnetic Resonance  
Henkestr. 127  
DE-91052 Erlangen  
Germany  
Phone: +49 9131 84-0

##### Global Siemens Headquarters

Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

##### Global Siemens Healthcare

**Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

##### Legal Manufacturer

Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**SIEMENS**



[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

*syngo.via* and MAGNETOM Skyra

Answers for life.

# syngo.via and MAGNETOM Skyra

syngo.via is our advanced software, creating an exciting experience in efficiency and ease of use – across the enterprise<sup>1)</sup>. syngo.via is your agent for productivity throughout your radiology workflow – from scanning to result sharing.

## Integrated Engine concept

The Engine concept integrates the scanning and reading processes into one holistic workflow and enables you to maximize your scanner and application investment.

Key features	The Dot (Day optimizing throughput) Engines optimize the performance of MAGNETOM Skyra and offer patient personalization, user guidance, and exam automation.  syngo.via offers reading workflows, which are optimally adjusted to the Dot Engines for the best reading outcomes
Key benefits	The scanning and reading workflows are easily customizable to the user's standards of care.  Results from the scanner are optimally displayed in the reading workflows.

---

Key benefits	Guidance, standardization and flexibility is offered for every step of the workflow, reducing the need for further inquiry
	Increasing throughput, minimizing recalls, and enhancing quality of care.

<sup>1)</sup> Prerequisites include: internet connection to clinical network, DICOM compliance, meeting of minimum hardware requirements and adherence to local data security regulations

### **Direct Image Transfer (DIT)**

After completion of a series of images, they are transferred automatically to *syngo.via*. Easily view the images with any *syngo.via* client immediately after they were acquired.

Key features	This data will be automatically transferred to the <i>syngo.via</i> data base and loaded into the related workflow. Enhanced DICOM MR enables to transfer fMRI data and spectroscopy raw data in new DICOM standard format. In <i>syngo.via</i> and in any PACS supporting this standard, these data can be handled.
Key benefits	Images are immediately available throughout the institution. This enables fast and convenient feedback from everywhere.
Direct Image Transfer Pro	The MAGNETOM scanner and <i>syngo.via</i> server are directly connected, enabling image transfer.

### **Seamless workstation integration**

*syngo.via* integrates smoothly with *syngo MultiModality Workstation* (MMWP). Open MMWP directly out of *syngo.via*, and vice versa.

Key features	Remotely open the same patient at the MMWP easily with <i>syngo Expert-i</i> The MMWP results can then be easily integrated into the <i>syngo.via</i> report <i>syngo.via</i> client can be opened from any MMWP with one click
Key benefits	Remote and easy access of all MMWP applications Smooth integration of results into <i>syngo.via</i>

On account of certain regional limitations of sales rights and service availability, we cannot guarantee that all products included in this brochure are available through the Siemens sales organization worldwide. Siemens reserves the right to modify the design, packaging, specifications, and options described herein without prior notice.

Any technical data contained in this document may vary within defined tolerances. Original images always lose a certain amount of detail when reproduced.

Please find fitting accessories:  
[www.siemens.com/medical-accessories](http://www.siemens.com/medical-accessories)

Please contact your local Siemens sales representative for the most current information.

#### Local Contact Information

##### In the USA

Siemens Medical Solutions USA, Inc.  
51 Valley Stream Parkway  
Malvern, PA 19355  
Phone: +1 888-826-9702  
Phone: +1 610-448-4500  
Fax: +1 610-448-2254

##### In Asia

Siemens Healthcare Sector  
Asia Pacific Headquarters  
The Siemens Center  
60 MacPherson Road  
Singapore 348615  
Phone: +65 6490 6000  
Fax: +65 6490 6001

##### In Japan

Siemens Japan K.K.  
Gate City Osaki West Tower  
1-11-1 Osaki, Shinagawa-ku  
Tokyo 141-8644  
Phone: +81 3 5423 8411

##### Global Business Unit

Siemens Healthcare Sector  
Magnetic Resonance  
Henkestr. 127  
DE-91052 Erlangen  
Germany  
Phone: +49 9131 84-0

##### Global Siemens Headquarters

Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

##### Global Siemens Healthcare

**Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

##### Legal Manufacturer

Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**SIEMENS**



[www.usa.siemens.com/healthcare](http://www.usa.siemens.com/healthcare)

# MAGNETOM Skyra

Parts & Accessories

Answers for life.

# Parts & Accessories

## Patient Video Monitoring

Dedicated MAGNETOM Skyra video camera for comprehensive patient observation in the examination room and waiting room observation.

- Up to two in-room cameras for optimized patient observation from front end and rear-end
- Up to two waiting room cameras for observing the situation in the waiting room
- Color 640×480 pixel LCD monitor may be positioned at the syngo Acquisition Workplace or at a convenient wall location
- Possibility to switch between 4 camera layout and single camera layout

## Remote Viewing Monitor

Color LCD monitor (1280×1024) to be connected in parallel to the Workplace monitor.

Data transfer via ethernet for high signal quality over a long distance allows the computer and user to be located anywhere on the 100 or 1000 Mbps network with full routing of data across routers, switches and subnets (1 Gbit/s recommended).

The system supports SSL (Secure Sockets Layer) via a TCP/IP connection. All media streams transferred in the network are encrypted.

## Additional Dot Control Center Rear

Additional Dot Display and Dot Control Center Rear, e.g. for interventional procedures. Located at the rear end of the system.

## Foot Switch

In-room foot switch with two pneumatic buttons for start and stop of a preset MR sequence. The foot switch is MR compatible and is positioned near the patient table on the examination room floor.

## syngo MR Workplace

Additional integrated Workplace with host computer for post-processing and image evaluation.

Same user interface as the syngo Acquisition Workplace, except for scan control.

Shared database with syngo Acquisition Workplace, therefore eliminating image copy time.

➤ Host Computer and LCD Monitor technical data: refer to "Computer System" section of the main data sheet.

## Workplace Table

Ergonomically designed table for:

- Color monitor
- Keyboard
- Mouse
- Patient communication unit
- Patient supervision display

## Patient Transport Stretcher

MR-compatible design on wheels for transporting a patient into the examination room.

Useful when the removable tabletop and trolley option are not purchased

- Non-ferromagnetic, height-adjustable design
- Trendelenburg positioning possible

Max. patient weight	160 kg (350 lbs)
---------------------	------------------

### **Comfort Kit**

Vacuum cushions for stable and comfortable positioning of the patient during the examination

Vacuum pump connection at the Tim Table

3 anatomically shaped cushions of different size for patient stabilization and comfort (spine, head, multi-purpose)

May significantly reduce patient set-up times and improve image quality by minimizing the occurrence of motion artifacts

### **Coil Storage Cart**

Specially designed non-ferromagnetic cart for easy storage of some of the most commonly used coils and accessories

May be rolled to convenient locations in the examination room

Additional storage space on the inside of the doors when doors are opened

Coil storage	Width	cart closed	140 cm (4'7")
		cart opened	280 cm (9'2")
	Depth		54 cm (1'9")
	Height		121 cm (3'12")
Upper drawer	Height		13.3 cm
Tray	Height		9.0 cm
Lower drawer	Height		24.0 cm

Additional optional accessories and consumables for MR: [www.usa.siemens.com/healthcare-accessories](http://www.usa.siemens.com/healthcare-accessories)



On account of certain regional limitations of sales rights and service availability, we cannot guarantee that all products included in this brochure are available through the Siemens sales organization worldwide. Siemens reserves the right to modify the design, packaging, specifications, and options described herein without prior notice.

Any technical data contained in this document may vary within defined tolerances. Original images always lose a certain amount of detail when reproduced.

Please find fitting accessories:  
[www.siemens.com/medical-accessories](http://www.siemens.com/medical-accessories)

Please contact your local Siemens sales representative for the most current information.

#### Local Contact Information

##### In the USA

Siemens Medical Solutions USA, Inc.  
51 Valley Stream Parkway  
Malvern, PA 19355  
Phone: +1 888-826-9702  
Phone: +1 610-448-4500  
Fax: +1 610-448-2254

##### In Asia

Siemens Healthcare Sector  
Asia Pacific Headquarters  
The Siemens Center  
60 MacPherson Road  
Singapore 348615  
Phone: +65 6490 6000  
Fax: +65 6490 6001

##### In Japan

Siemens Japan K.K.  
Gate City Osaki West Tower  
1-11-1 Osaki, Shinagawa-ku  
Tokyo 141-8644  
Phone: +81 3 5423 8411

##### Global Business Unit

Siemens Healthcare Sector  
Magnetic Resonance  
Henkestr. 127  
DE-91052 Erlangen  
Germany  
Phone: +49 9131 84-0

##### Global Siemens Headquarters

Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

##### Global Siemens Healthcare

**Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

##### Legal Manufacturer

Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

**MAGNETOM Skyra**  
**Datasheet-Box Content**  
**syngo MR E11**

**Sales Project / Customer**

Part of Tender	Document/TITLE	Legal Manufacturer	Printkey / Document ID
<input type="checkbox"/>	MAGNETOM Skyra – A Tim+Dot System – Data Sheet	Siemens	Order No. A91MR-9013-51-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra – Tim [204x24] XQ Gradients	Siemens	Order No. A91MR-9013-52-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra – Tim [204x48] XQ Gradients, Tim [204x64] XQ Gradients, Tim [204x128] XQ Gradients	Siemens	Order No. A91MR-9013-53-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra – A Tim+Dot System – TimTX TrueShape enabling ZOOMit	Siemens	Order No. A91MR-9013-54-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, Tim Dockable Table	Siemens	Order No. A91MR-9013-55-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, Head/Neck 16	Siemens	Order No. A91MR-9013-A501-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, Head/Neck 20	Siemens	Order No. A91MR-9013-A502-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, Head/Neck 64 <sup>1)</sup>	Siemens	Order No. A91MR-9013-A503-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, Spine 24	Siemens	Order No. A91MR-9013-A504-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, Spine 32 <sup>2)</sup>	Siemens	Order No. A91MR-9013-A505-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, Body 6	Siemens	Order No. A91MR-9013-A506-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, Body 18	Siemens	Order No. A91MR-9013-A507-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, Body 18 Long	Siemens	Order No. A91MR-9013-A508-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, Flex Large 4 / Flex Small 4	Siemens	Order No. A91MR-9013-A509-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, Peripheral Angio 36	Siemens	Order No. A91MR-9013-A510-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, Hand/Wrist 16	Siemens	Order No. A91MR-9013-A511-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, Foot/Ankle 16	Siemens	Order No. A91MR-9013-A512-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, Shoulder Large 16 Shoulder Small 16	Siemens	Order No. A91MR-9013-A513-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, CP Extremity Coil	QED	Order No. A91MR-9013-A514-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, Tx/Rx 15-Channel Knee Coil <sup>3)</sup>	QED	Order No. A91MR-9013-A515-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, 4-Channel BI Breast Coil	Noras	Order No. A91MR-9013-A516-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, 16-Channel AI Breast Coil	RAPID	Order No. A91MR-9013-A517-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, 2-/4-/8-Channel Sentinelle Breast Coil	Sentinelle	Order No. A91MR-9013-A518-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, 8-Channel Sentinelle Breast Coil/ Upgrade to Biopsy Configuration	Sentinelle	Order No. A91MR-9013-A519-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, 2-/10-/16-Channel Sentinelle Breast Coil	Sentinelle	Order No. A91MR-9013-A520-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, 16-Channel Sentinelle Breast Coil/ Upgrade to Biopsy Configuration	Sentinelle	Order No. A91MR-9013-A521-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, Breast 18	Siemens	Order No. A91MR-9013-A522-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, Loop Coils	Siemens	Order No. A91MR-9013-A523-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, MEDRAD Endorectal Coil Kit	Bayer	Order No. A91MR-9013-A524-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, Pediatric 16	QED	Order No. A91MR-9013-A525-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, Head 32 <sup>2)</sup>	Siemens	Order No. A91MR-9013-A526-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, Tx/Rx CP Head Coil	QED	Order No. A91MR-9013-A527-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, 4-Channel Special-Purpose Coil	SSMR	Order No. A91MR-9013-A528-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, Sentinelle Endorectal Coil <sup>4)</sup>	Sentinelle	Order No. A91MR-9013-A529-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, Application Packages	Siemens	Order No. A91MR-9013-B5-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, Post-processing Packages	Siemens	Order No. A91MR-9013-C5-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, syngo.via and MAGNETOM Skyra	Siemens	Order No. A91MR-9013-D5-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
<input type="checkbox"/>	MAGNETOM Skyra, Parts & Accessories	Siemens	Order No. A91MR-9013-E5-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG
	Backpage (Printnumber of Package)	Siemens	Order No. A91MR-9013-F5-4A00   Printed in Germany   MC.MR-00901 PA 0714 POD   © 01.2015, Siemens AG

<sup>1)</sup> Prerequisites: Tim [204x64] or Tim [204x128]

<sup>2)</sup> Prerequisites: Tim [204x48]; Tim [204x64] or Tim [204x128]

<sup>3)</sup> Alternative name: Tx/Rx Knee 15

<sup>4)</sup> Alternative name: Prostate 2

On account of certain regional limitations of sales rights and service availability, we cannot guarantee that all products included in this brochure are available through the Siemens sales organization worldwide. Siemens reserves the right to modify the design, packaging, specifications, and options described herein without prior notice.

Any technical data contained in this document may vary within defined tolerances. Original images always lose a certain amount of detail when reproduced.

Please find fitting accessories:  
[www.siemens.com/medical-accessories](http://www.siemens.com/medical-accessories)

Please contact your local Siemens sales representative for the most current information.

#### Local Contact Information

##### In the USA

Siemens Medical Solutions USA, Inc.  
51 Valley Stream Parkway  
Malvern, PA 19355  
Phone: +1 888-826-9702  
Phone: +1 610-448-4500  
Fax: +1 610-448-2254

##### In Asia

Siemens Healthcare Sector  
Asia Pacific Headquarters  
The Siemens Center  
60 MacPherson Road  
Singapore 348615  
Phone: +65 6490 6000  
Fax: +65 6490 6001

##### In Japan

Siemens Japan K.K.  
Gate City Osaki West Tower  
1-11-1 Osaki, Shinagawa-ku  
Tokyo 141-8644  
Phone: +81 3 5423 8411

##### Global Business Unit

Siemens Healthcare Sector  
Magnetic Resonance  
Henkestr. 127  
DE-91052 Erlangen  
Germany  
Phone: +49 9131 84-0

##### Global Siemens Headquarters

Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany

##### Global Siemens Healthcare

**Headquarters**  
Siemens AG  
Healthcare Sector  
Henkestrasse 127  
91052 Erlangen  
Telephone: +49 9131 84-0  
Germany  
[www.siemens.com/healthcare](http://www.siemens.com/healthcare)

##### Legal Manufacturer

Siemens AG  
Wittelsbacherplatz 2  
80333 Muenchen  
Germany