
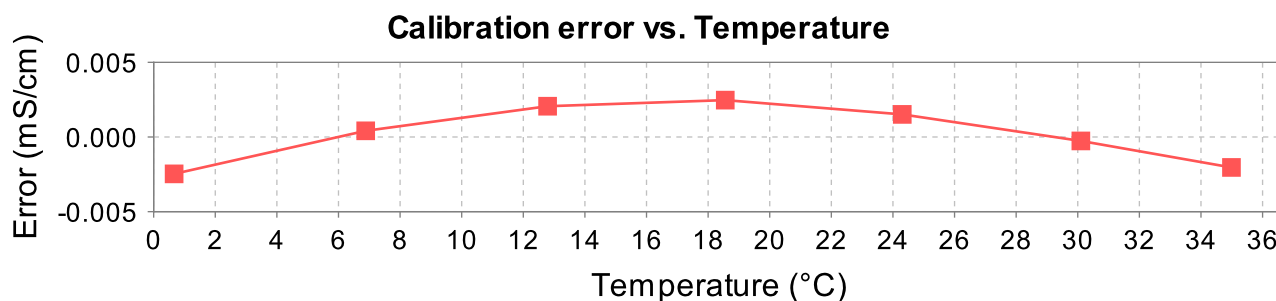


RBRlegato³ C.T.D, UWG Seaglider, wet bay (1000dbar) s/n: 238230
 References: Autosal8400B#66289, MS-315#15506, SSW P168, RC#002

Reference Resistance (ohm)	Reference Conductivity (mS/cm)	Voltage Ratio, V	Measured Conductivity (mS/cm)	Calibration Error (mS/cm)	Coefficients	
open	0.0000	-0.000138	0.0011	0.0011	C0:	26.10363E-3
693.9963	7.0965	0.038916	7.0969	0.0004	C1:	181.6952
331.9147	14.8381	0.081519	14.8378	-0.0003	(K) C2:	1.00113
150.0111	32.8308	0.180542	32.8297	-0.0011	X0:	429.67018E-6
100.0117	49.2440	0.270876	49.2429	-0.0011	X1:	-12.756421E-6
75.0207	65.6483	0.361165	65.6480	-0.0003	X2:	1.1797E-6
55.5183	88.7091	0.488093	88.7103	0.0012	X3:	-199.1314E-12
Bath	Voltage Ratio	Temperature (ITS-90)	Salinity (PSS-78)	Conductivity (mS/cm)	X4:	-124.2382E-15
T15S35	0.2362043	15.03476	34.9923	42.9433	X5:	15.034758
T25S35	0.2911416	24.87880	34.9874	52.9275	X6:	10


Cell Constant @T15S35 = 4.92498 1/cm

$$C_c = \frac{C_0 + C_1 * C_2 * V - X_0 * (T - X_5)}{1 + X_1 * (T - X_5) + X_2 * (P - X_6) + X_3 * (P - X_6)^2 + X_4 * (P - X_6)^3}$$

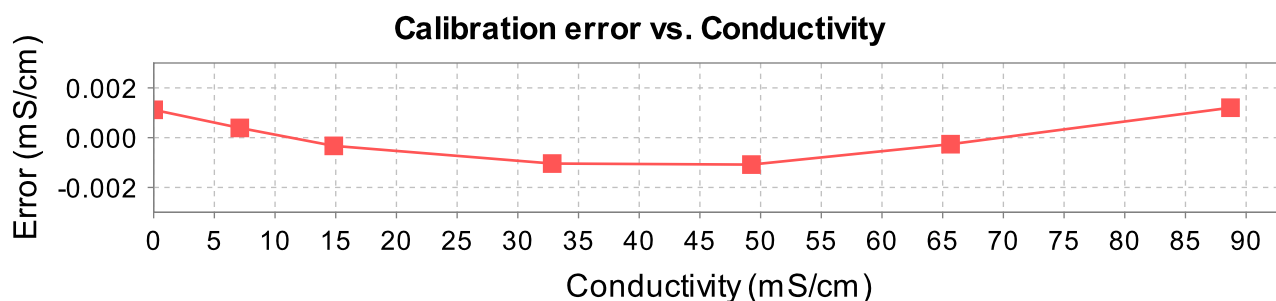

Calibration Date: 2025-03-18
 Issue Date: 2025-03-20
 File Name: 238230_20250318_1457fCcal.rsk

Operator: 
 kbelgaid

Approver: 
 ytouba