



Pressure Calibration Certificate



RBRlegato³ C.T.D, UWG Seaglider, wet bay (1000dbar) s/n: 238230
Instrument rating: 1000
Nominal accuracy: 0.05%FS (0.5 dbar)
Reference instrument: Mensor CPC6050 s/n: 41000CAM

Applied pressure, P _{app} (dbar)	Voltage ratio, V	Measured pressure, P _c (dbar)	Calibration error (dbar)	Coefficients
10.389	0.0210523	10.424	0.035	C0: -37.226616
110.285	0.0652210	110.335	0.050	C1: 2.2603774E3
210.283	0.1093751	210.319	0.036	C2: 27.122137
310.284	0.1534833	310.283	-0.001	C3: -19.49778
410.285	0.1975759	410.283	-0.002	X0: 10.1034
510.286	0.2416368	510.274	-0.012	X1: 71.86447E-3
610.283	0.2856829	610.281	-0.002	X2: 17.299133E-6
710.291	0.3297119	710.294	0.003	X3: -476.72287E-9
810.286	0.3737208	810.294	0.008	X4: -134.51188E-6
910.284	0.4177225	910.298	0.014	X5: 20.808868
1010.275	0.4617055	1010.273	-0.002	

Head (mm) = 285

$$P_c = X_0 + \frac{P_m - X_0 - X_1(T - X_5) - X_2(T - X_5)^2 - X_3(T - X_5)^3}{1 + X_4(T - X_5)}$$

$$P_m = C_0 + C_1V + C_2V^2 + C_3V^3$$

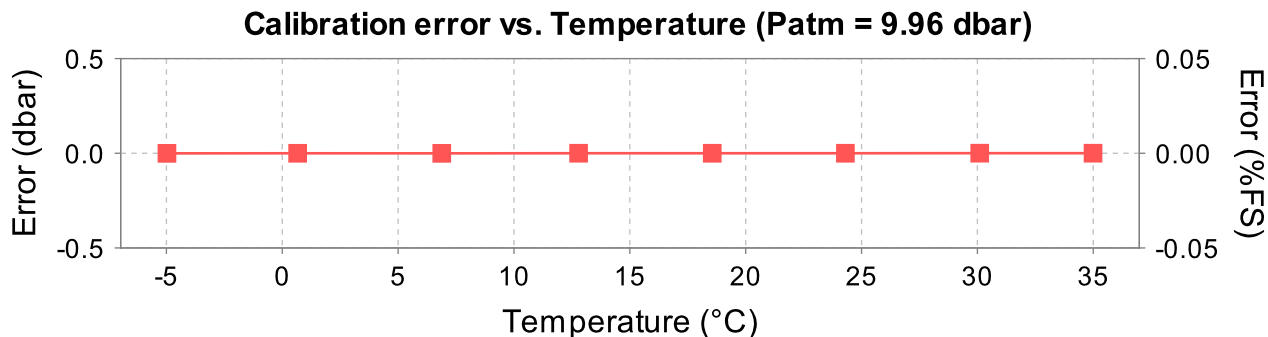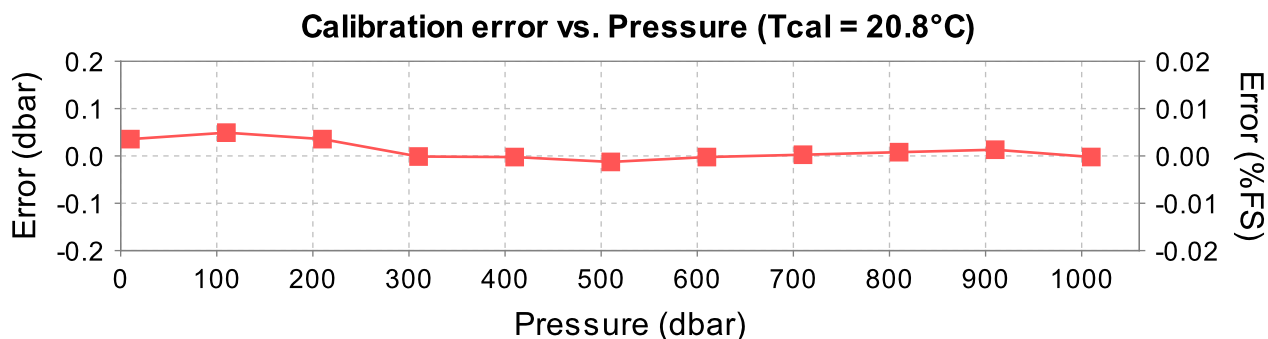

Calibration Date: 2025-03-18
Issue Date: 2025-03-18
File Name: 238230_20250318_1148P.rsk

Operator: P. J. Shah
pshah

Approver: A. Weinerth
aweinerth