


Reference Temperature, ITS-90	Voltage ratio, V	Measured Temperature, ITS-90	Calibration error	Coefficients	
-4.97588	0.7294837	-4.97583	0.00005	C0:	3.4746116E-3
0.66404	0.6669584	0.66394	-0.00010	C1:	-253.88267E-6
6.88359	0.5934580	6.88360	0.00001	C2:	2.4168662E-6
12.78886	0.5222584	12.78897	0.00011	C3:	-79.2018E-9
18.55636	0.4542535	18.55634	-0.00002		
24.30257	0.3903378	24.30257	0.00000		
30.10047	0.3314182	30.10037	-0.00010		
34.98971	0.2868036	34.98978	0.00007		

$$T_m = \ln\left(\left(\frac{1}{V}\right) - 1\right)$$

$$T_c = \frac{1}{(C_0 + C_1 T_m + C_2 T_m^2 + C_3 T_m^3)} - 273.15$$

Calibration error vs. Temperature

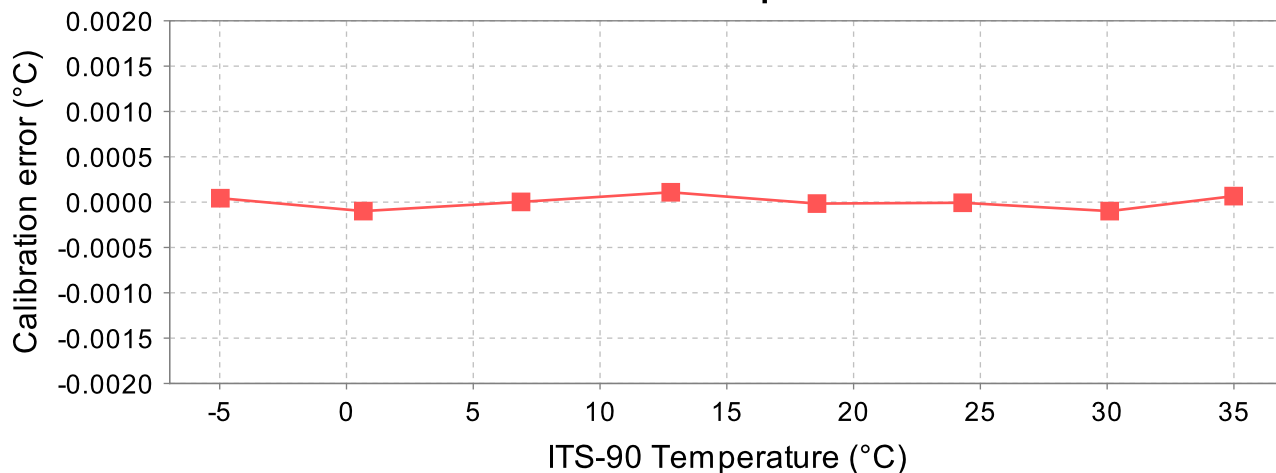

Calibration Date: 2025-03-17
Issue Date: 2025-03-17
Calibration ID: 84011

Operator:

ksong

Approver:

jwang