
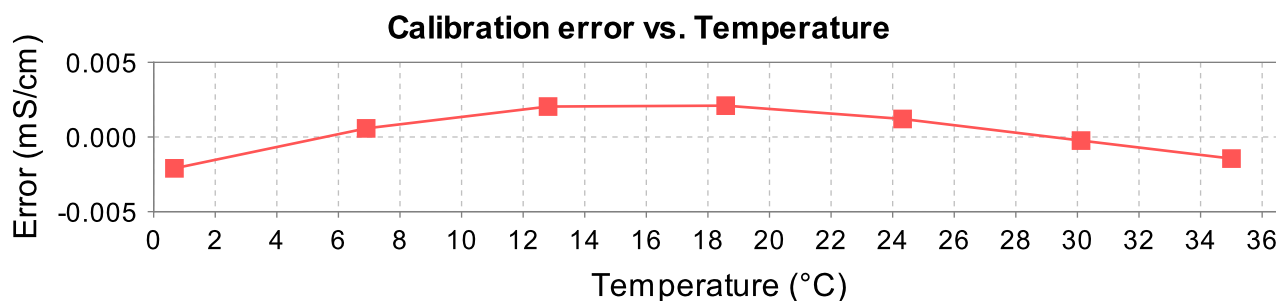


RBRlegato<sup>3</sup> C.T.D, UWG Seaglider, wet bay (1000dbar) s/n: 238232  
 References: Autosal8400B#66289, MS-315#15506, SSW P168, RC#002

| Reference Resistance (ohm) | Reference Conductivity (mS/cm) | Voltage Ratio, V     | Measured Conductivity (mS/cm) | Calibration Error (mS/cm) | Coefficients |               |
|----------------------------|--------------------------------|----------------------|-------------------------------|---------------------------|--------------|---------------|
| open                       | 0.0000                         | -0.000123            | 0.0013                        | 0.0013                    | C0:          | 23.642417E-3  |
| 693.9963                   | 7.0943                         | 0.038926             | 7.0944                        | 0.0001                    | C1:          | 181.6431      |
| 331.9147                   | 14.8334                        | 0.081530             | 14.8330                       | -0.0004                   | (K) C2:      | 1.00113       |
| 150.0111                   | 32.8204                        | 0.180553             | 32.8198                       | -0.0006                   | X0:          | 227.02076E-6  |
| 100.0117                   | 49.2284                        | 0.270881             | 49.2272                       | -0.0012                   | X1:          | -9.460689E-6  |
| 75.0207                    | 65.6275                        | 0.361166             | 65.6269                       | -0.0006                   | X2:          | 557.4669E-9   |
| 55.5183                    | 88.6810                        | 0.488093             | 88.6824                       | 0.0014                    | X3:          | 464.8872E-12  |
| Bath                       | Voltage Ratio                  | Temperature (ITS-90) | Salinity (PSS-78)             | Conductivity (mS/cm)      | X4:          | -436.4245E-15 |
| T15S35                     | 0.2362915                      | 15.03462             | 34.9934                       | 42.9444                   | X5:          | 15.034621     |
| T25S35                     | 0.2913938                      | 24.91021             | 34.9842                       | 52.9560                   | X6:          | 10            |


Cell Constant @T15S35 = 4.92342 1/cm

$$C_c = \frac{C_0 + C_1 * C_2 * V - X_0 * (T - X_5)}{1 + X_1 * (T - X_5) + X_2 * (P - X_6) + X_3 * (P - X_6)^2 + X_4 * (P - X_6)^3}$$

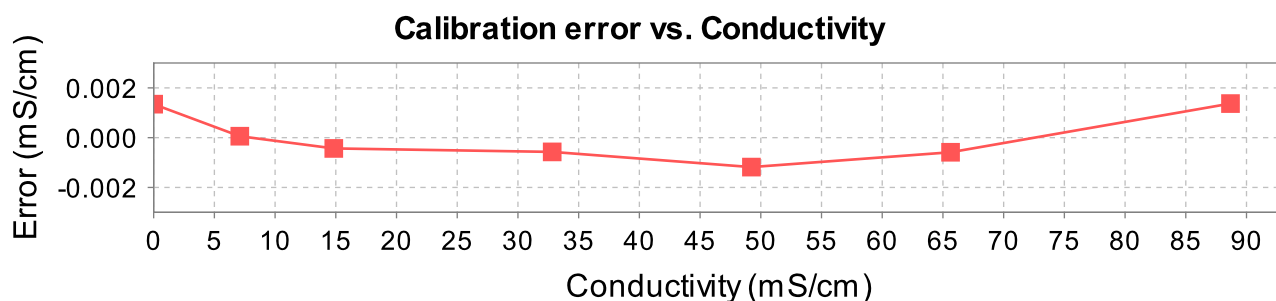

Calibration Date: 2025-03-18  
 Issue Date: 2025-03-20  
 File Name: 238232\_20250318\_1540fCcal.rsk

Operator:   
 kbelgaid

Approver:   
 ytouba