



Pressure Calibration Certificate

RBRlegato³ C.T.D, UWG Seaglider, wet bay (1000dbar) s/n: 238232

Instrument rating: 1000

Nominal accuracy: 0.05%FS (0.5 dbar)



Reference instrument: Mensor CPC6050 s/n: 41000CAM

Applied pressure, P _{app} (dbar)	Voltage ratio, V	Measured pressure, P _c (dbar)	Calibration error (dbar)	Coefficients
10.354	0.0175243	10.365	0.011	C0: -28.898691
110.267	0.0620934	110.280	0.013	C1: 2.238776E3
210.266	0.1066320	210.278	0.012	C2: 42.56222
310.266	0.1511085	310.268	0.002	C3: -30.017004
410.266	0.1955375	410.268	0.002	X0: 10.0867
510.266	0.2399153	510.251	-0.015	X1: 46.965655E-3
610.270	0.2842666	610.262	-0.008	X2: -47.71985E-6
710.270	0.3285894	710.271	0.001	X3: -647.81887E-9
810.271	0.3728906	810.284	0.013	X4: -134.47269E-6
910.270	0.4171711	910.286	0.016	X5: 21.105999
1010.257	0.4614271	1010.255	-0.002	

Head (mm) = 266

$$P_c = X_0 + \frac{P_m - X_0 - X_1(T - X_5) - X_2(T - X_5)^2 - X_3(T - X_5)^3}{1 + X_4(T - X_5)}$$

$$P_m = C_0 + C_1V + C_2V^2 + C_3V^3$$

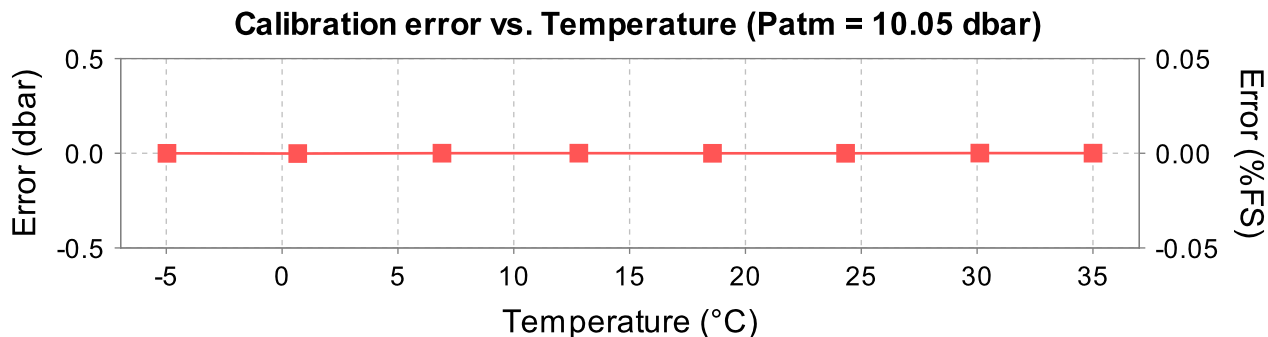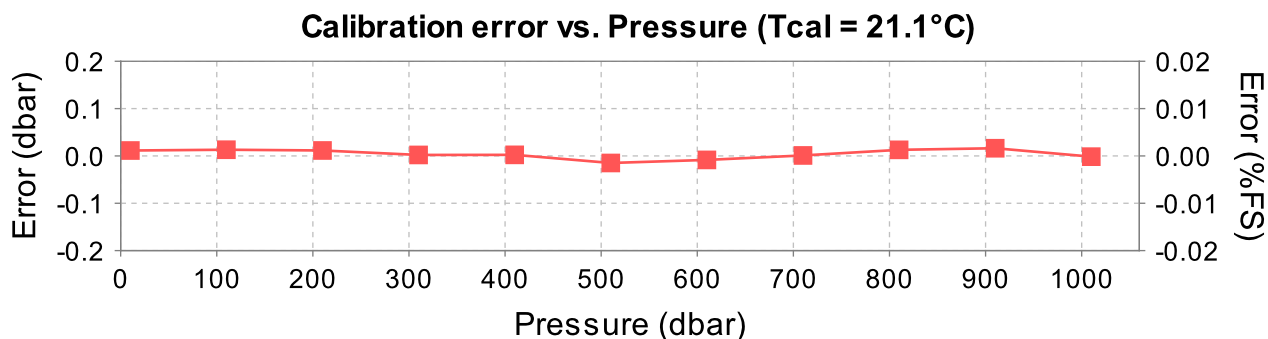

Calibration Date: 2025-03-17

Issue Date: 2025-03-17

File Name: 238232_20250317_1545P.rsk

Operator:

dluong

Approver:

aweinerth