



Reference Temperature, ITS-90	Voltage ratio, V	Measured Temperature, ITS-90	Calibration error	Coefficients	
-4.97046	0.7315480	-4.97048	-0.00002	C0:	3.4724032E-3
0.67470	0.6690981	0.67475	0.00005	C1:	-253.25155E-6
6.90077	0.5955566	6.90072	-0.00005	C2:	2.4669962E-6
12.80856	0.5242486	12.80859	0.00003	C3:	-79.989185E-9
18.57722	0.4560671	18.57720	-0.00002		
24.32261	0.3919410	24.32260	-0.00001		
30.11746	0.3327980	30.11751	0.00005		
35.00341	0.2879956	35.00338	-0.00003		

$$T_m = \ln \left(\left(\frac{1}{V} \right) - 1 \right)$$

$$T_c = \frac{1}{(C_0 + C_1 T_m + C_2 T_m^2 + C_3 T_m^3)} - 273.15$$

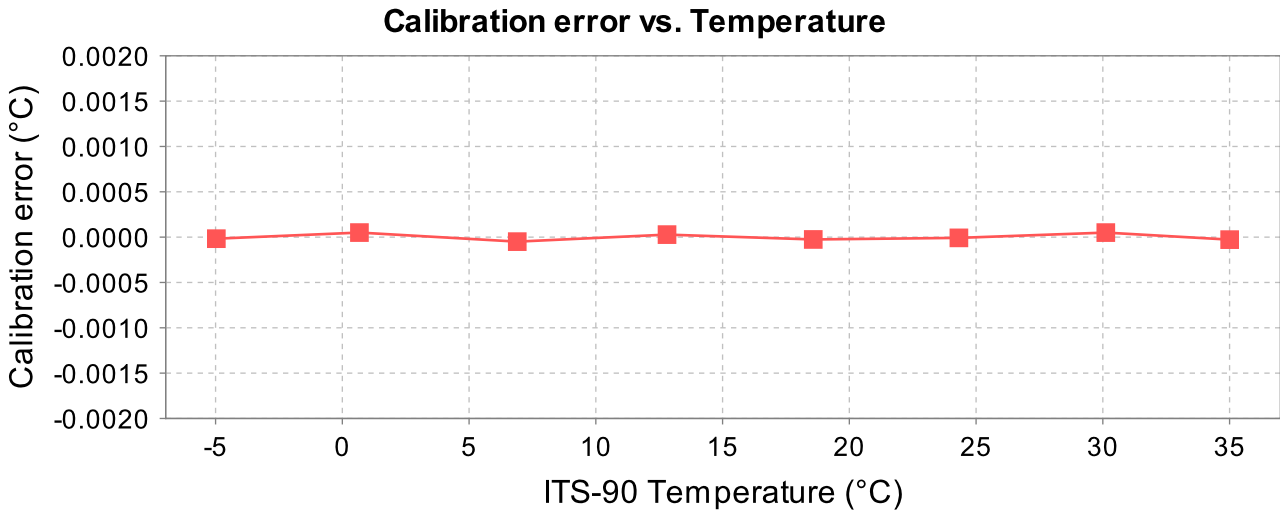

Calibration Date: 2025-03-17
 Issue Date: 2025-03-17
 Calibration ID: 83999

Operator: 
 ksong

Approver: 
 jwang