



a xylem brand

CALIBRATION CERTIFICATE

Form No 830, March 2021

Certificate no: 4831_1300_00246676
Foil batch no: 2519WM

Product: 4831
Calibration date: 15.10.2025

Serial no: 1300
Page 1 of 2

Index	Temperature reference(°C)	[O2] Reference(μM)	Temperature raw data(mV)	Phase reading(°)
0	30.672	0.98	-91.140	61.98
1	20.466	0.44	218.323	62.89
2	10.423	-0.10	524.807	63.66
3	1.424	-0.65	782.403	64.30
4	1.430	60.81	782.273	56.47
5	1.433	106.08	782.173	52.09
6	1.439	147.77	782.000	48.81
7	1.441	220.28	781.987	44.29
8	1.495	303.63	780.500	40.43
9	1.551	401.28	778.993	36.97
10	1.556	531.00	778.827	33.57
11	10.465	52.89	523.513	54.56
12	10.432	84.44	524.500	50.54
13	10.421	119.71	524.820	46.92
14	10.418	174.19	524.900	42.59
15	10.418	241.61	524.933	38.66
16	10.420	321.36	524.853	35.20
17	10.419	426.67	524.893	31.89
18	20.342	42.43	222.113	53.10
19	20.334	68.67	222.387	48.72
20	20.318	95.26	222.867	45.22
21	20.303	139.87	223.347	40.74
22	20.315	195.00	222.967	36.78
23	20.331	256.48	222.500	33.55
24	20.335	334.78	222.360	30.56
25	30.508	34.68	-86.307	51.63
26	30.514	54.75	-86.500	47.35
27	30.518	78.85	-86.607	43.38
28	30.523	111.53	-86.767	39.33
29	30.542	159.48	-87.340	35.15
30	30.556	212.15	-87.733	31.91
31	30.559	275.69	-87.800	29.12

Giving these coefficients


Index	0	1	2	3	4	5	6
SVUFoilCoef	2.85325E-03	1.19166E-04	1.98484E-06	1.81158E02	-2.22285E-01	-5.08205E01	3.65814E00
TempCoef	2.76096E01	-3.32456E-02	3.43986E-06	-4.75791E-09	0.00000E00	0.00000E00	

Certificate no: 4831_1300_00246676
Foil batch no: 2519WM


Product: 4831
Calibration date: 15.10.2025

Serial no: 1300
Page 2 of 2

Oxygen validation

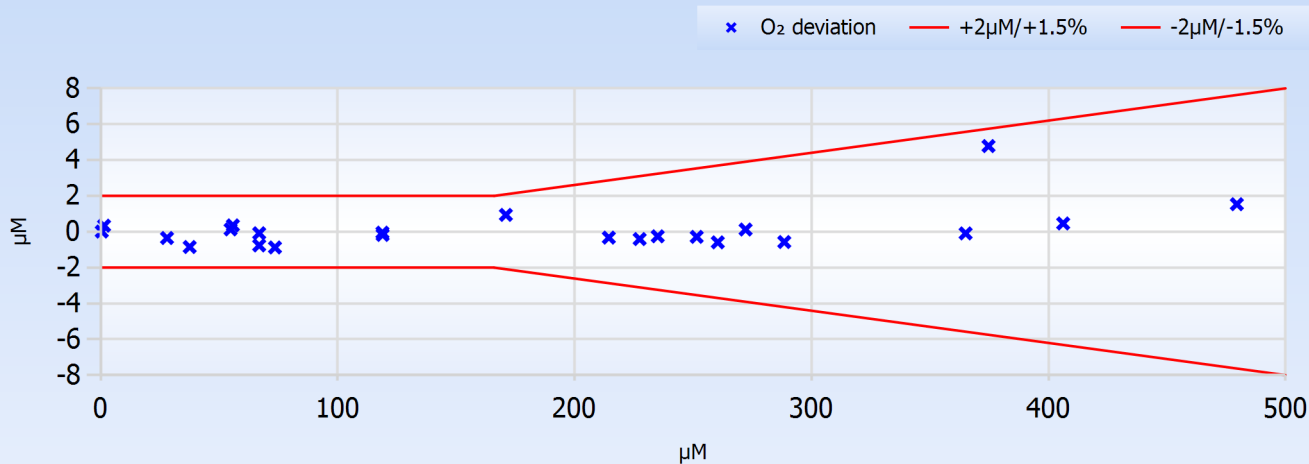

Temperature validation

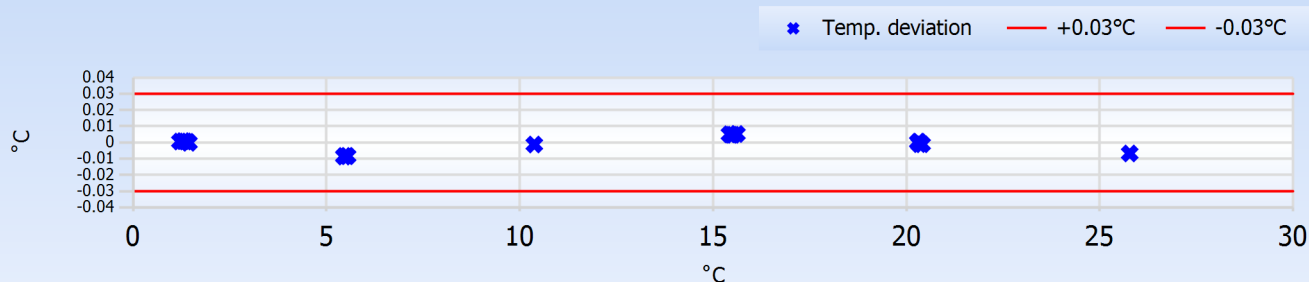

With following settings

Index	0	1	2	3
PhaseCoef	-7.94000E-01	1.00000E00	0.00000E00	0.00000E00

Index	0 (Offset)	1 (Slope)
ConcCoef	0.00000E00	1.00000E00

Salinity	0.00
----------	------

Firmware Version	5.3.1
------------------	-------

Date:15.10.2025

Astrid Fjeldtvedt

Astrid Fjeldtvedt, Production Engineer



a xylem brand

CALIBRATION CERTIFICATE

Form No 830, March 2021

Certificate no: 4831_1301_00246932
Foil batch no: 2519WM

Product: 4831
Calibration date: 22.10.2025

Serial no: 1301
Page 1 of 2

Index	Temperature reference(°C)	[O2] Reference(μM)	Temperature raw data(mV)	Phase reading(°)
0	30.855	0.92	-181.853	61.15
1	20.209	0.41	142.440	62.02
2	10.272	-0.17	452.947	62.75
3	0.857	-0.72	732.847	63.37
4	0.924	24.66	730.967	59.76
5	0.961	45.26	729.907	57.28
6	0.993	66.40	729.000	55.00
7	1.020	106.98	728.247	51.20
8	1.035	151.91	727.833	47.71
9	1.051	216.21	727.373	43.72
10	1.120	312.29	725.400	39.28
11	1.124	414.06	725.300	35.80
12	1.124	527.50	725.293	32.85
13	10.647	15.90	441.340	59.47
14	10.553	36.46	444.267	55.92
15	10.494	53.40	446.100	53.40
16	10.449	84.72	447.467	49.47
17	10.415	116.73	448.547	46.18
18	10.386	169.44	449.433	41.92
19	10.359	244.68	450.293	37.53
20	10.382	324.17	449.567	34.13
21	10.385	404.85	449.500	31.54
22	20.342	12.82	138.273	58.58
23	20.321	28.65	138.900	54.84
24	20.309	42.06	139.300	52.14
25	20.289	66.78	139.927	48.04
26	20.277	92.31	140.300	44.64
27	20.272	134.18	140.473	40.28
28	20.272	195.02	140.440	35.84
29	20.278	258.97	140.300	32.51
30	20.277	324.94	140.300	29.98
31	30.471	10.63	-170.553	57.60
32	30.458	23.51	-170.200	53.60
33	30.454	34.16	-170.100	50.82
34	30.448	54.58	-169.900	46.50
35	30.451	75.42	-169.980	43.02
36	30.453	108.55	-170.013	38.77
37	30.446	158.91	-169.827	34.33
38	30.451	211.85	-169.993	31.07
39	30.455	267.01	-170.100	28.61

Certificate no: 4831_1301_00246932
Foil batch no: 2519WM


Product: 4831
Calibration date: 22.10.2025

Serial no: 1301
Page 2 of 2


Giving these coefficients

Index	0	1	2	3	4	5	6
SVUFoilCoef	2.86906E-03	1.20043E-04	1.87264E-06	1.85613E02	-2.36489E-01	-5.22333E01	3.74837E00
TempCoef	2.47991E01	-3.25851E-02	3.14696E-06	-4.44860E-09	0.00000E00	0.00000E00	

Oxygen validation

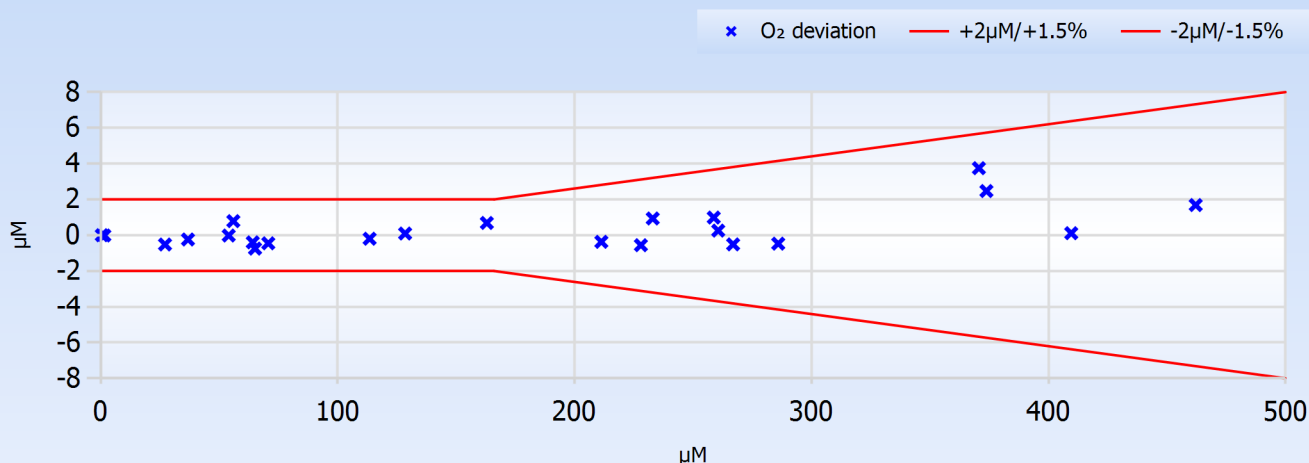

Temperature validation

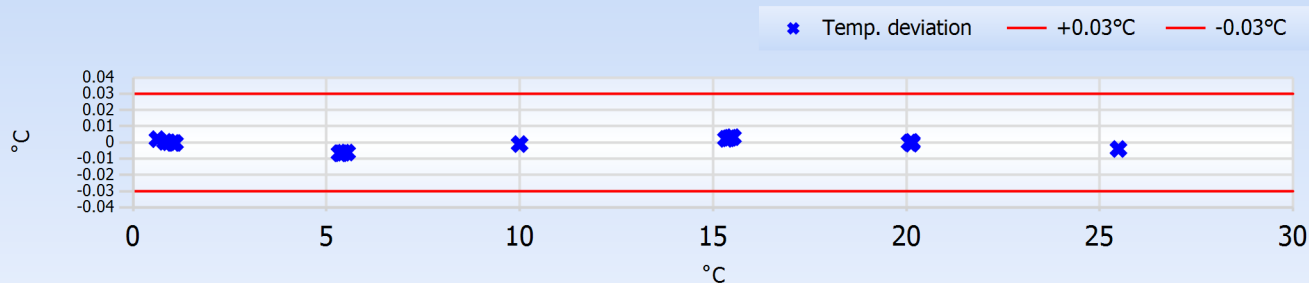

With following settings

Index	0	1	2	3
PhaseCoef	1.88000E-01	1.00000E00	0.00000E00	0.00000E00

Index	0 (Offset)	1 (Slope)
ConcCoef	0.00000E00	1.00000E00
Salinity	0.00	

Firmware Version	5.3.1
------------------	-------

Date:22.10.2025

Tor-Ove Kvalvaag
Tor-Ove Kvalvaag, Calibration Engineer