

Piezoresistive Pressure Sensor Calibration

Type 4260M099
Serial Number 6341354
Manufacturer Kistler
Pressure Range 0 to 1500 PSI
Reference Absolute
Test Condition New

Certificate ID # 6341354-241218T0714
Calibration Technician Jason Griswold
Date/Time 12/18/2024 7:14:24 AM
Span mV/V 9.944
Offset mV/V 1.068
Supply Voltage V 9.998

Non-Linearity, Hysteresis, and Repeatability (NLHR)

P (PSI)	Output (mV/V)	BFSL Error (%)
0.0	1.0675	0.017
375.0	3.5507	-0.014
750.0	6.0370	-0.013
1125.0	8.5240	-0.002
1500.0	11.0115	0.012
750.0*	6.0362	-0.007
0.0*	1.0677	0.001

* Decreasing Pressure

Summary:


Environmental Conditions

Temperature	°C	22 ± 4
Relative Humidity	%	30 ± 30

Temperature Performance

Temperature (°C)	Span Error (%)	Offset Error (%)
-11.2	-0.221	-0.028
-0.3	-0.156	-0.024
25.0	0.000	0.000
40.5	0.086	0.026

Error Calculation	Unit
NLHR limits are based on	% span
Temperature Performance limits are based on	% span
Span & Offset limits are based on	% span

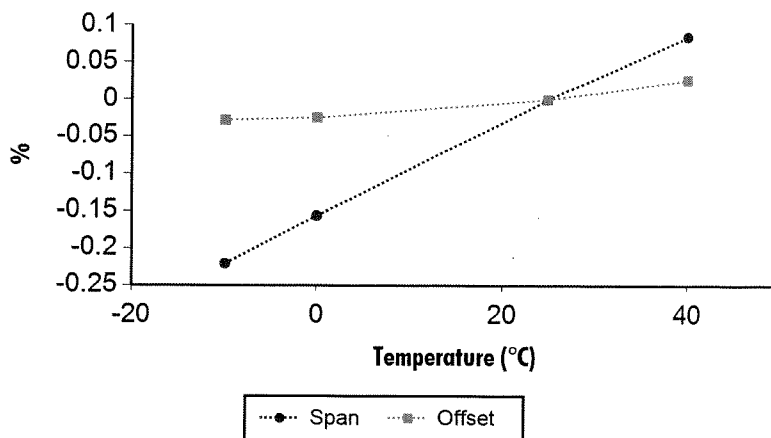

Reference Equipment

Type	S/N
Agilent 34970A	MY44021689
Mensor 750/1500 psi	830472
Mensor APC600	610322
Mensor Barometer	680141

This sensor was calibrated per Kistler test procedure 300.002.750 using a comparison technique against a Kistler working standard. Kistler working standards are periodically calibrated against a primary standard system, which in turn is periodically recertified to the National Institute of Standards and Technology (NIST) or another recognized national standard. Measurements are derived from accepted values of natural physical constants according to the International System of Units (SI). This calibration meets or exceeds the requirements of ISO 9001:2015, ANSI/NCSL Z540-1-1994 (R2002) and is accredited to ISO/IEC 17025:2017 as verified by the ANSI-ASQ National Accreditation Board/ANAB. Refer to certificate and Scope of Accreditation AC-1117. Estimated uncertainty of this calibration is ±0.25% of pressure reading with respect to the primary standard. Certificates are on file at Kistler and may be requested in writing. This certificate shall not be reproduced, except in full, without written approval of Kistler Instrument Corporation.