

Piezoresistive Pressure Sensor Calibration

Type	4260M099	Certificate ID #	6341357-241218T0714
Serial Number	6341357	Calibration Technician	Jason Griswold
Manufacturer	Kistler	Date/Time	12/18/2024 7:14:24 AM
Pressure Range	0 to 1500 PSI	Span	mV/V 9.941
Reference	Absolute	Offset	mV/V 1.118
Test Condition	New	Supply Voltage	V 9.998

Non-Linearity, Hysteresis, and Repeatability (NLHR)

P (PSI)	Output (mV/V)	BFSL Error (%)
0.0	1.1180	0.016
375.0	3.6009	-0.010
750.0	6.0857	-0.016
1125.0	8.5724	-0.001
1500.0	11.0589	0.011
750.0*	6.0851	-0.005
0.0*	1.1180	0.000

* Decreasing Pressure

Summary:


Environmental Conditions

Temperature	°C	22 ± 4
Relative Humidity	%	30 ± 30

Temperature Performance

Temperature (°C)	Span Error (%)	Offset Error (%)
-11.2	-0.194	-0.038
-0.3	-0.129	-0.033
25.0	0.000	0.000
40.5	0.083	0.030

Error Calculation	Unit
NLHR limits are based on	% span
Temperature Performance limits are based on	% span
Span & Offset limits are based on	% span

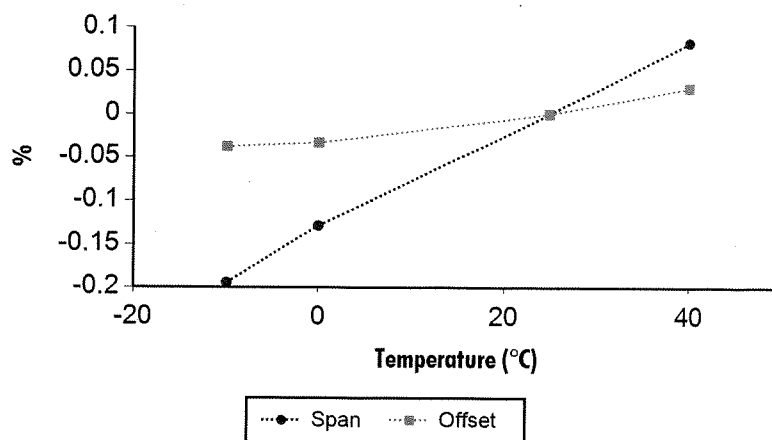

Reference Equipment

Type	S/N
Agilent 34970A	MY44021689
Mensor 750/1500 psi	830472
Mensor APC600	610322
Mensor Barometer	680141

This sensor was calibrated per Kistler test procedure 300.002.750 using a comparison technique against a Kistler working standard. Kistler working standards are periodically calibrated against a primary standard system, which in turn is periodically recertified to the National Institute of Standards and Technology (NIST) or another recognized national standard. Measurements are derived from accepted values of natural physical constants according to the International System of Units (SI). This calibration meets or exceeds the requirements of ISO 9001:2015, ANSI/NCSL Z540-1-1994 (R2002) and is accredited to ISO/IEC 17025:2017 as verified by the ANSI-ASQ National Accreditation Board/ANAB. Refer to certificate and Scope of Accreditation AC-1117. Estimated uncertainty of this calibration is ±0.25% of pressure reading with respect to the primary standard. Certificates are on file at Kistler and may be requested in writing. This certificate shall not be reproduced, except in full, without written approval of Kistler Instrument Corporation.