




(a) seno, 100 kHz

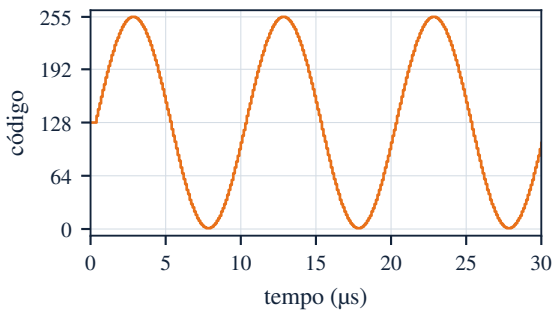


(b) troca de 100 kHz para 262 kHz, sem salto de fase

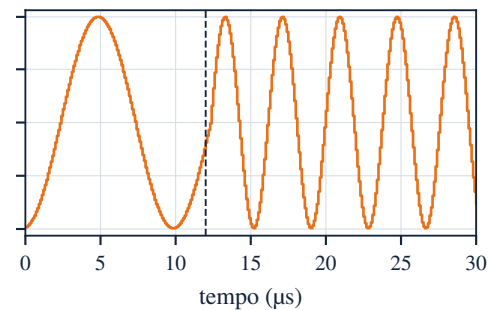


(c) rampa, 7 919 Hz

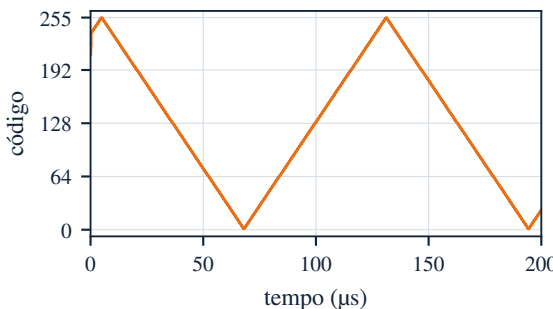

(d) sinc, 7 919 Hz

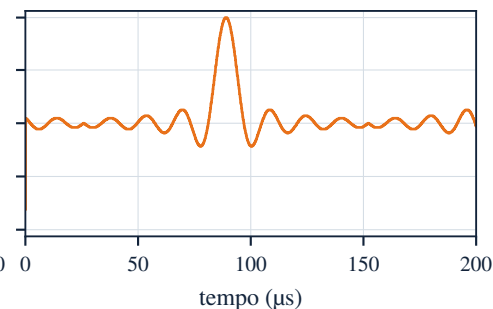

(e) arbitrária, ECG inicial, 100 kHz

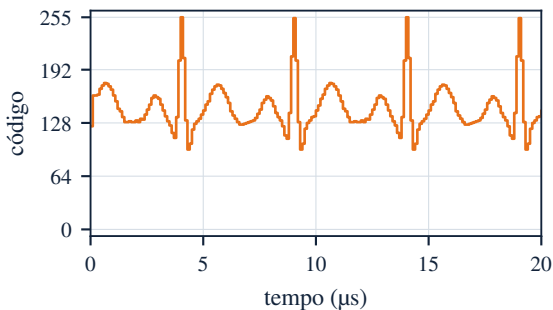

(f) dente de serra escrito na RAM, 100 kHz

