


FEB1 Chan0 Calibration

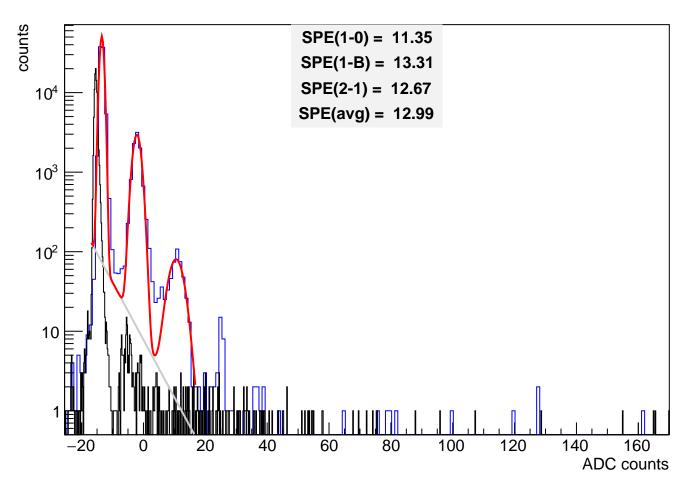


FEB1 Chan1 Calibration

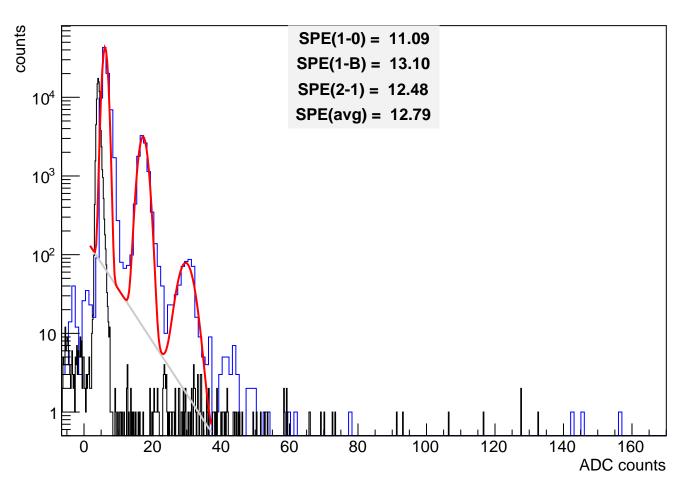


FEB1 Chan2 Calibration

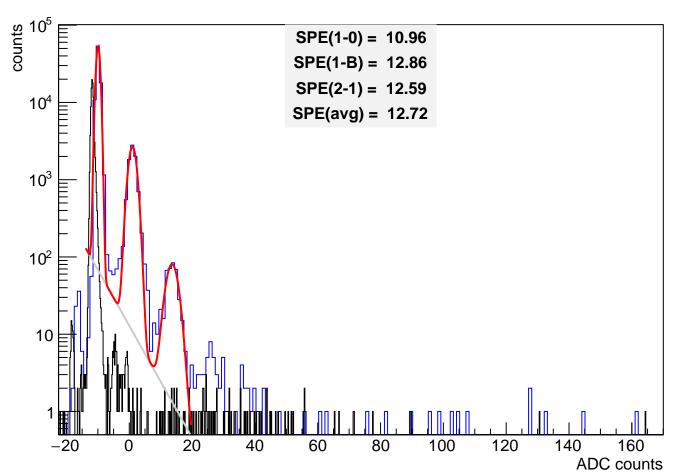


FEB1 Chan3 Calibration

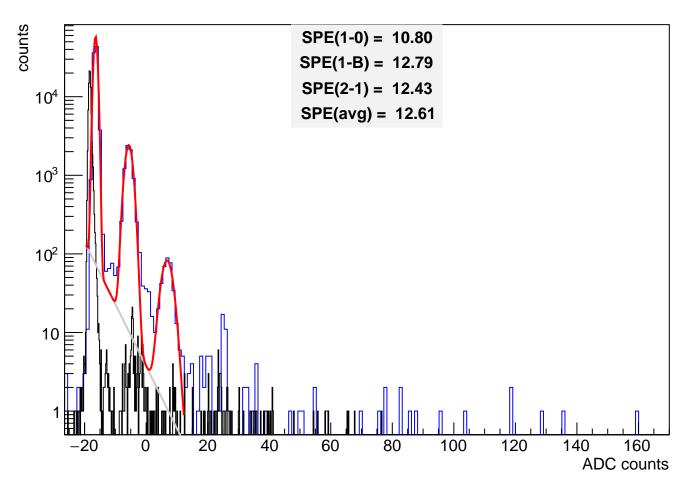


FEB1 Chan4 Calibration

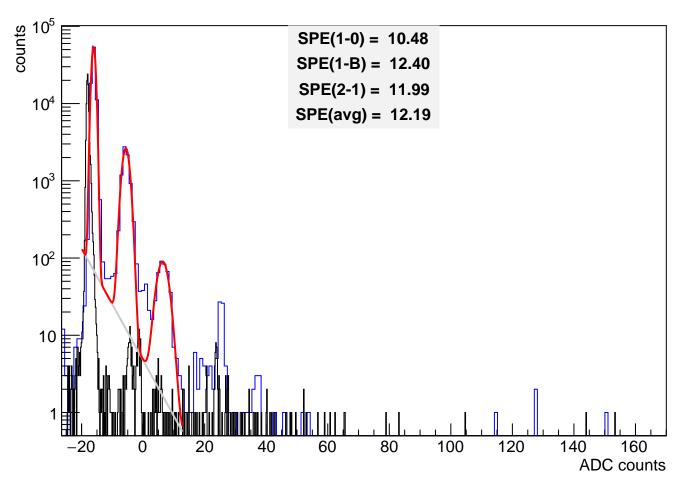


FEB1 Chan5 Calibration

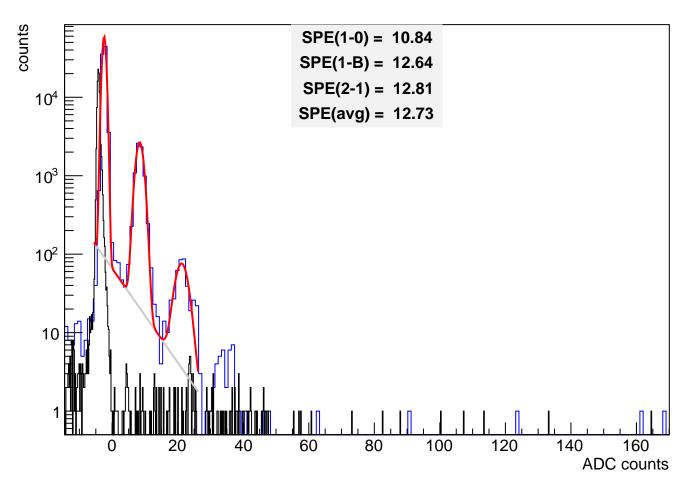


FEB1 Chan6 Calibration

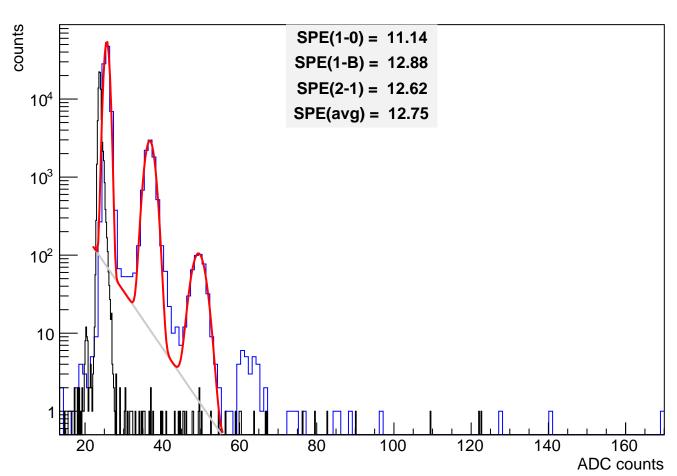


FEB1 Chan7 Calibration

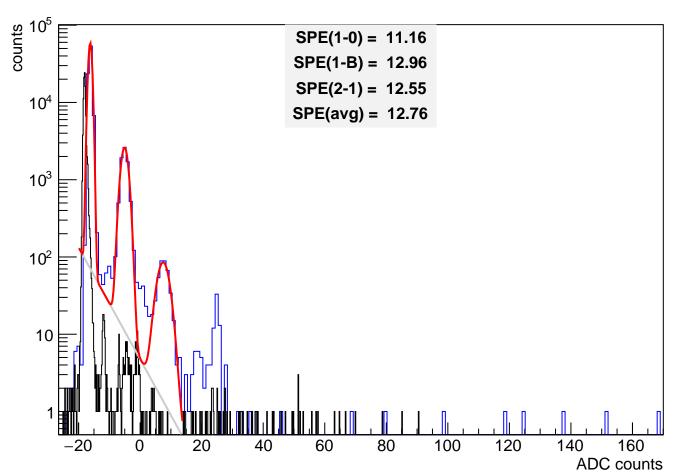


FEB1 Chan8 Calibration

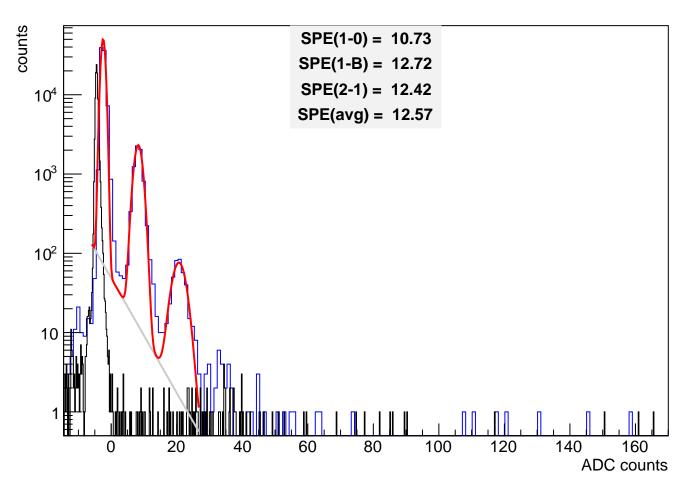


FEB1 Chan9 Calibration

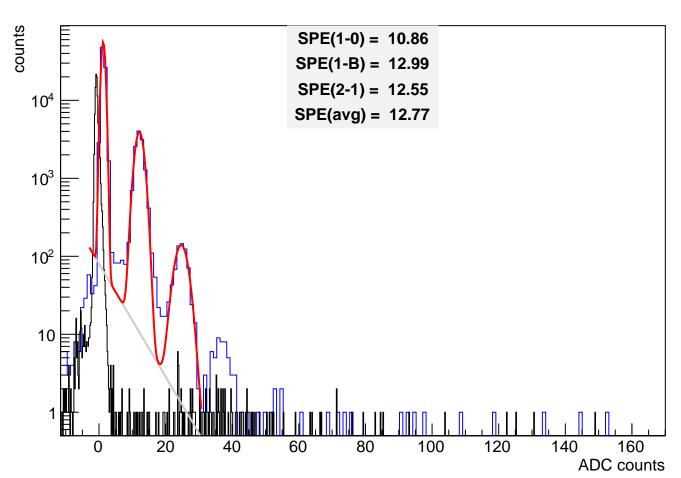


FEB1 Chan10 Calibration

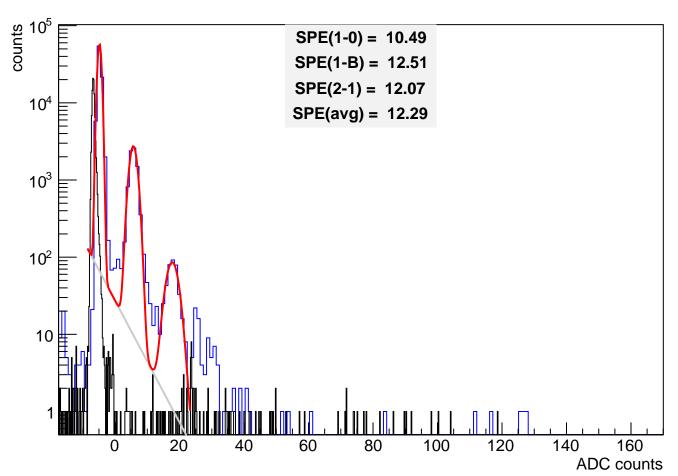


FEB1 Chan11 Calibration

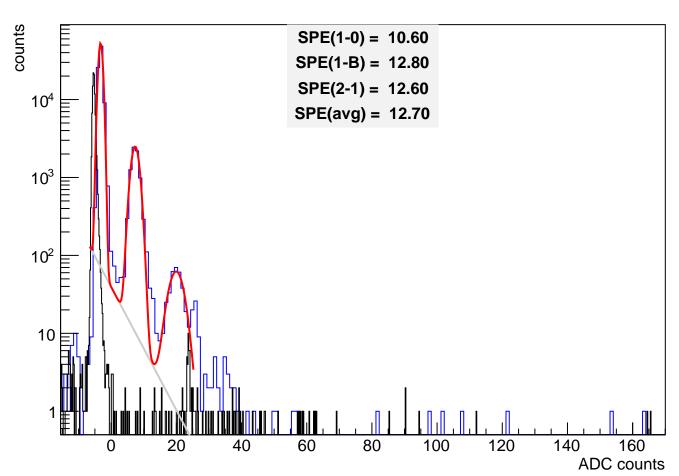


FEB1 Chan12 Calibration

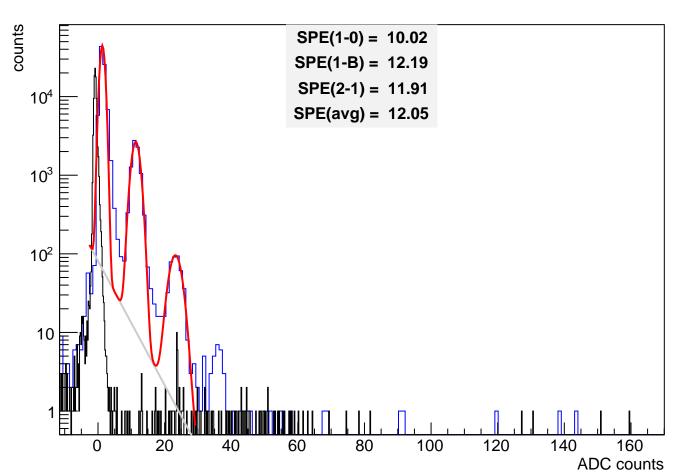


FEB1 Chan13 Calibration

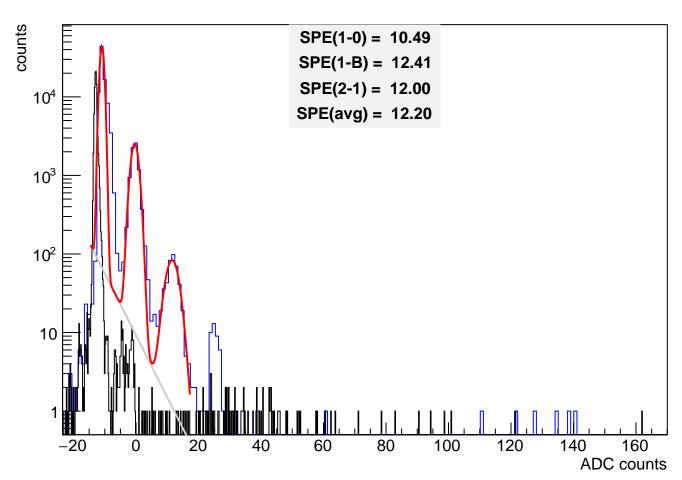


FEB1 Chan14 Calibration

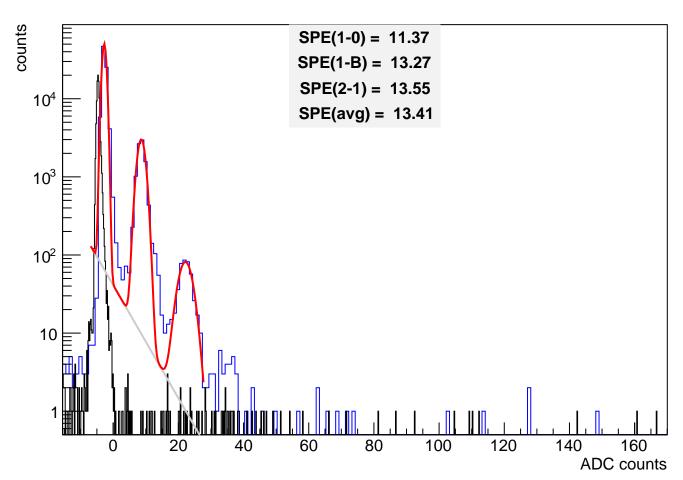


FEB1 Chan15 Calibration

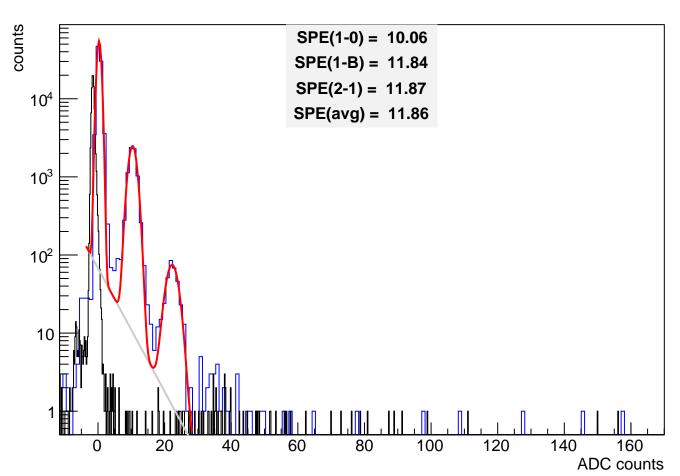


FEB2 Chan0 Calibration

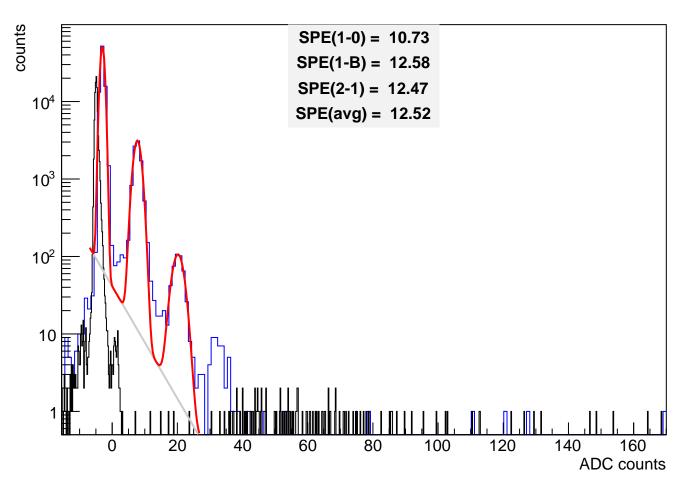


FEB2 Chan1 Calibration

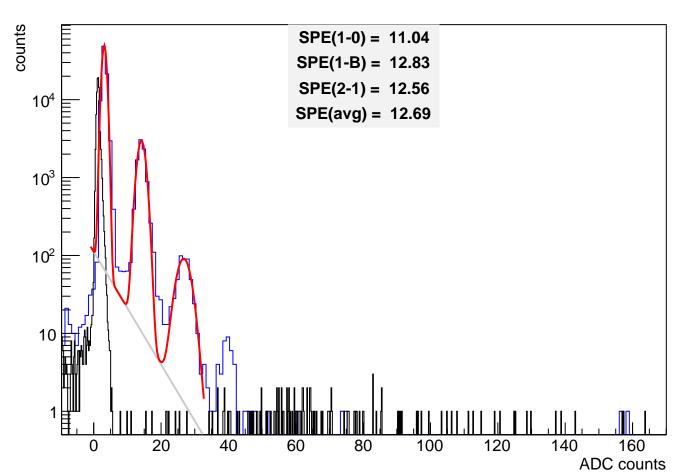


FEB2 Chan2 Calibration

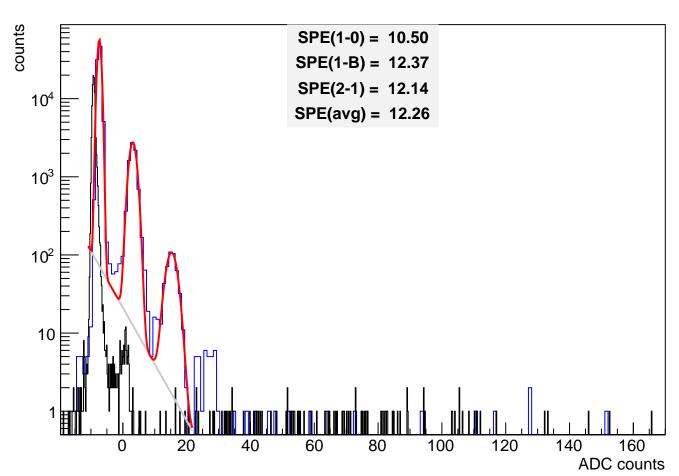


FEB2 Chan3 Calibration

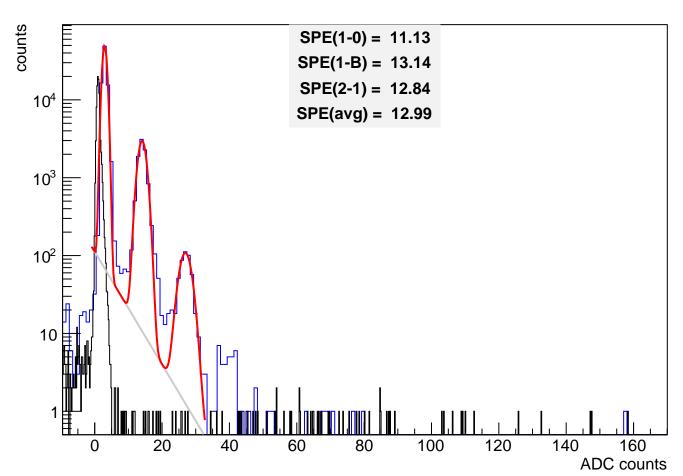


FEB2 Chan4 Calibration

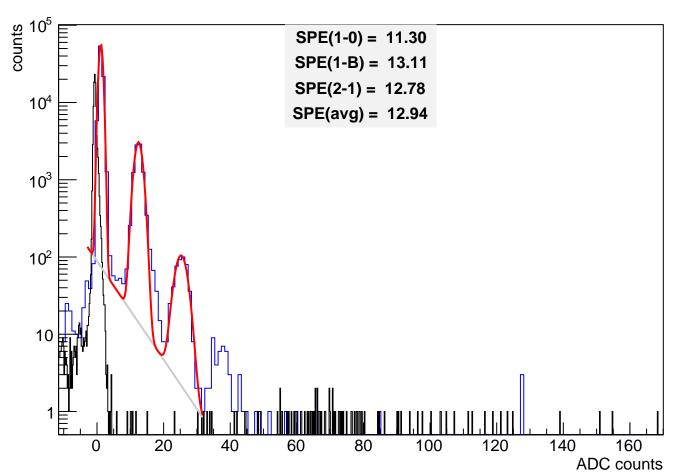


FEB2 Chan5 Calibration

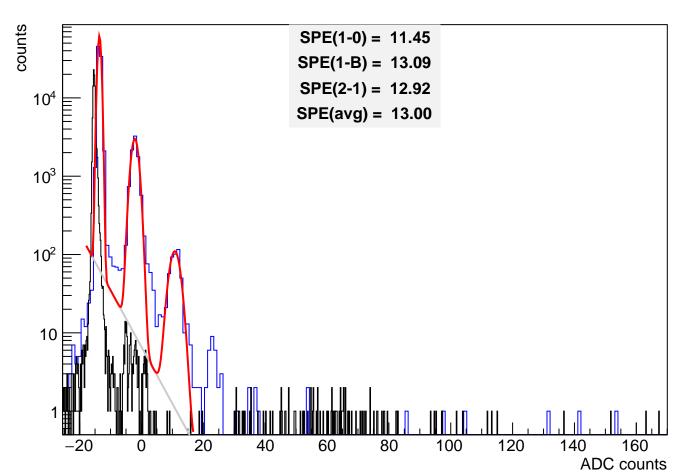


FEB2 Chan6 Calibration

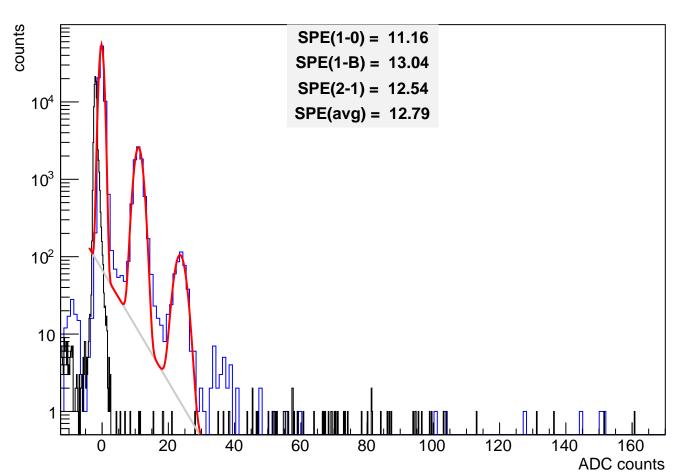


FEB2 Chan7 Calibration

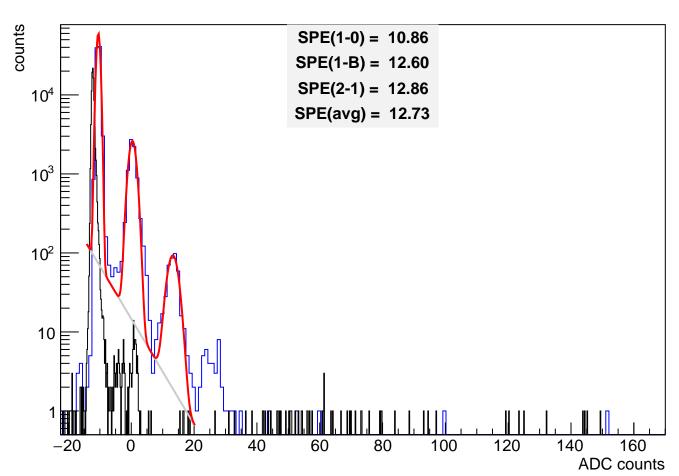


FEB2 Chan8 Calibration

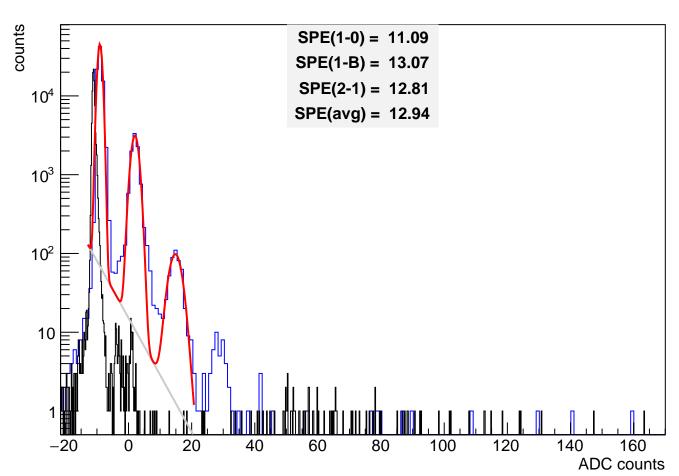


FEB2 Chan9 Calibration

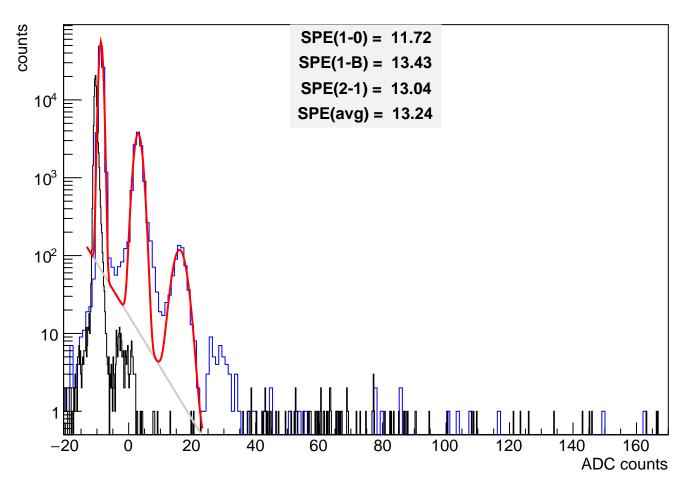


FEB2 Chan10 Calibration

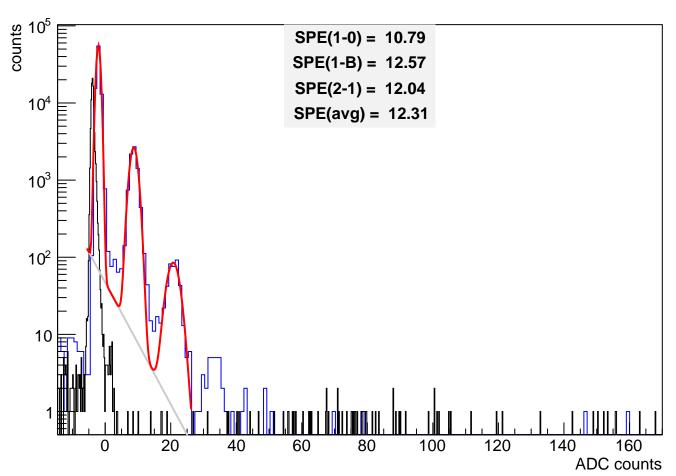


FEB2 Chan11 Calibration

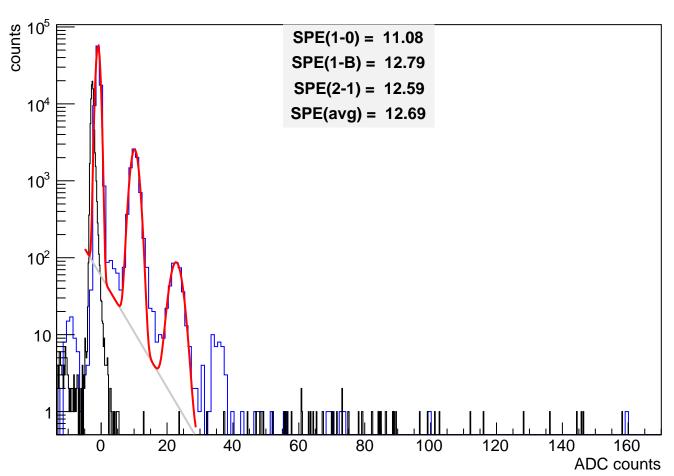


FEB2 Chan12 Calibration

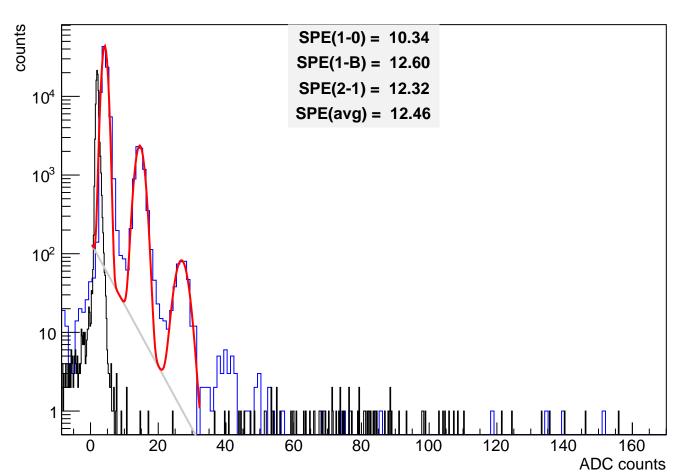

FEB2 Chan13 Calibration

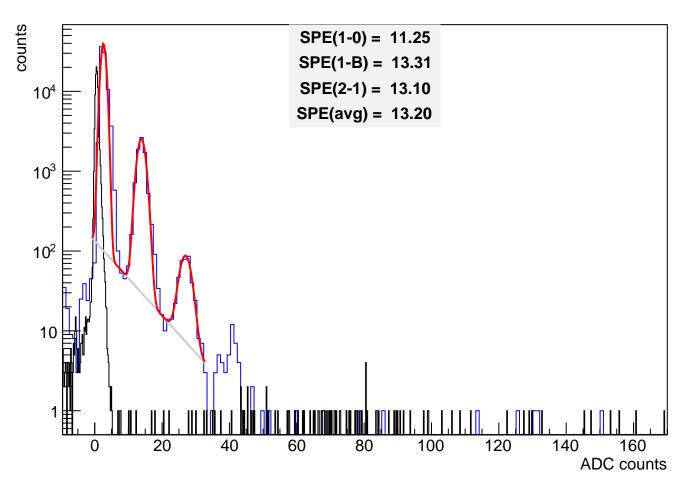

FEB2 Chan14 Calibration

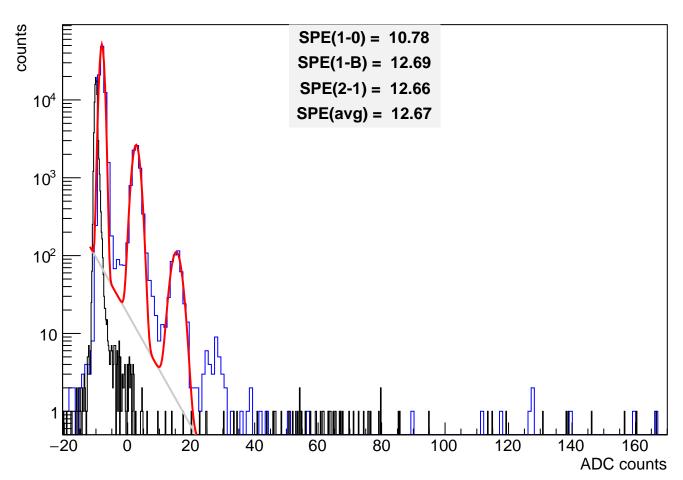

FEB2 Chan15 Calibration

