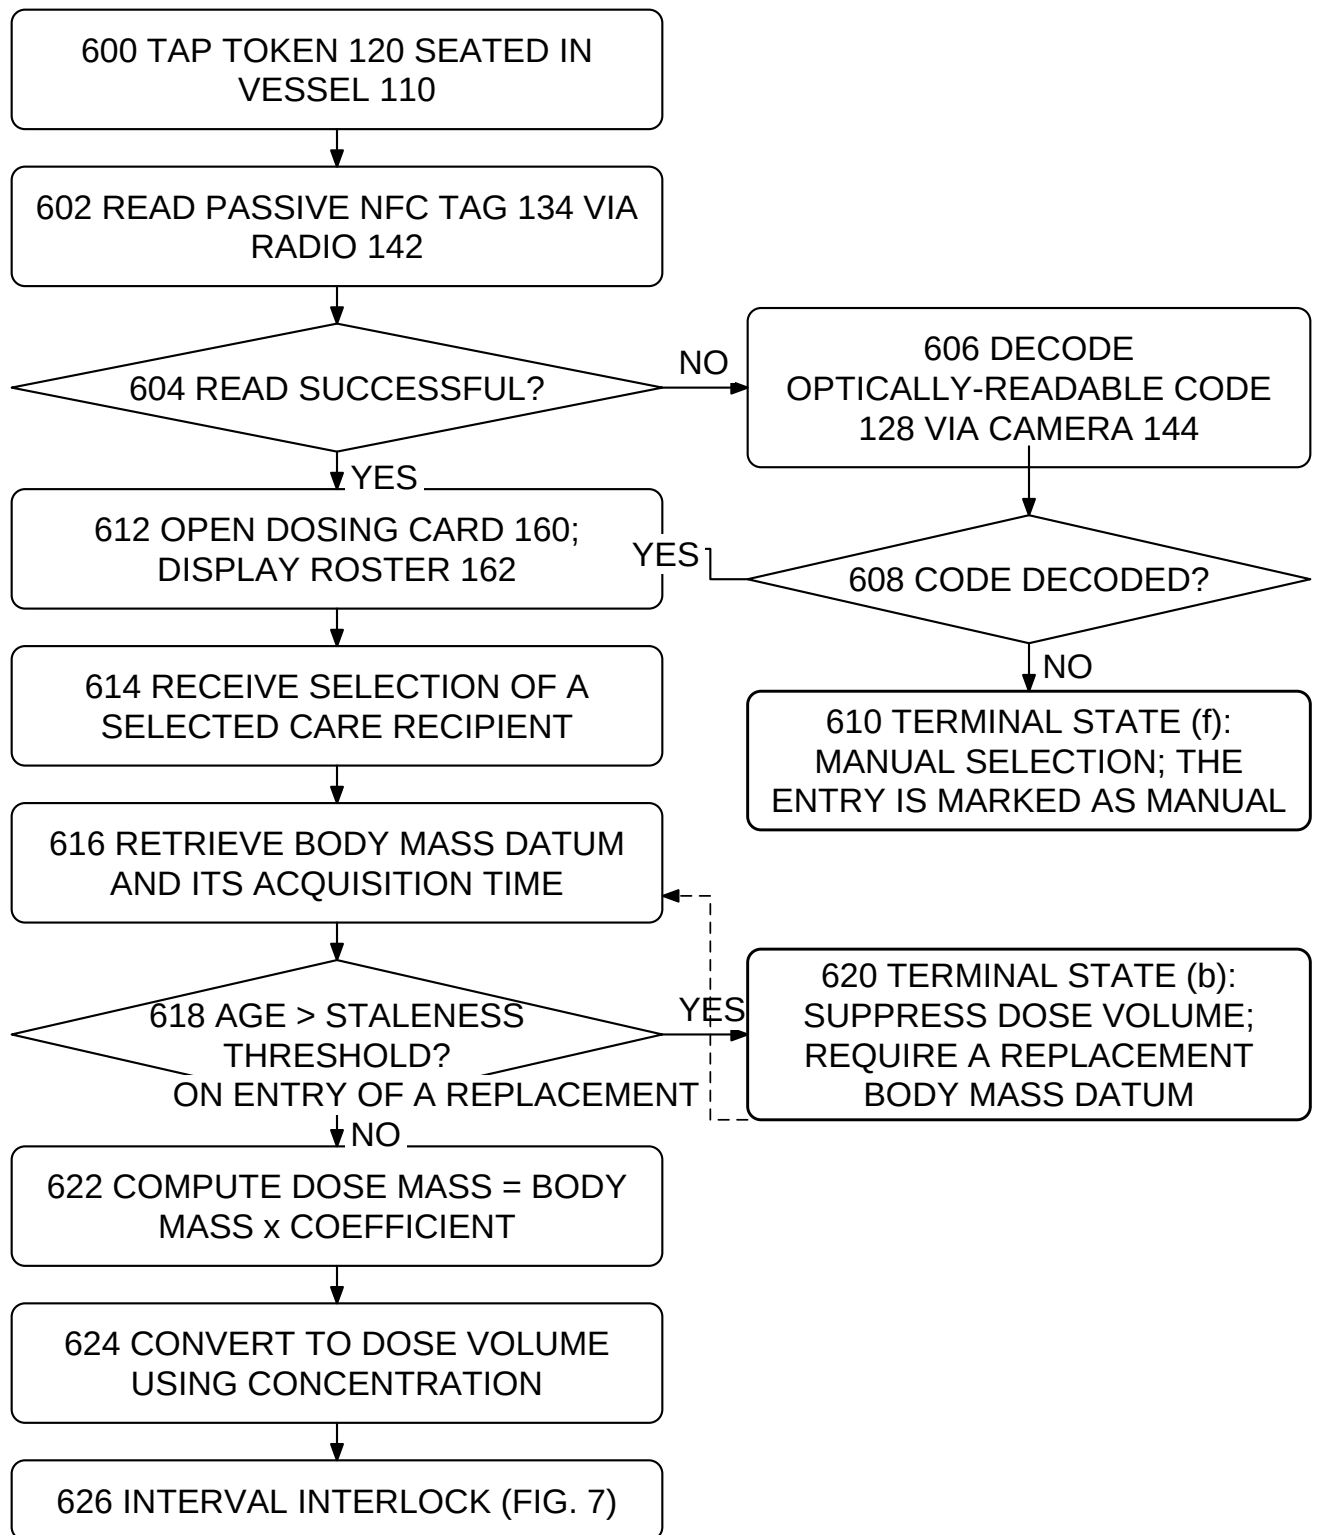


**FIG. 6**

DOSE VOLUME DETERMINATION WITH BODY MASS FRESHNESS GATE