


EXPLODED PERSPECTIVE VIEW — VESSEL 110 AND TOKEN 120.
DRAWN TO A SINGLE TRUE SCALE: TOKEN 120 AND RECESS 116
SPAN 90.2% OF BASE 114.

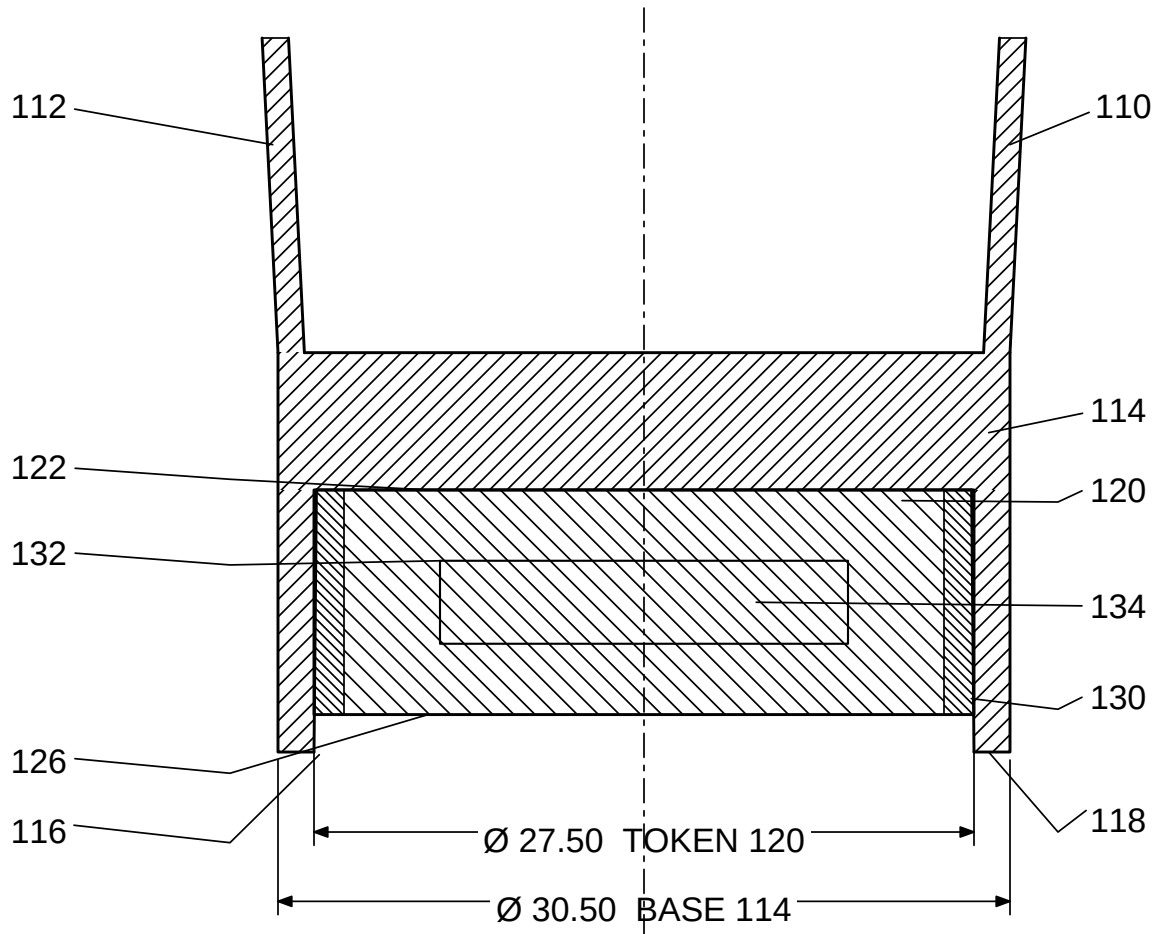

TOKEN 120 OCCUPIES 90.2% OF THE BASE DIAMETER; ONLY 1.50 mm OF BASE WALL REMAINS OUTBOARD OF RECESS 116.

FIG. 2

SECTIONAL VIEW — TOKEN 120 SEATED IN RECESS 116. RADIAL SCALE TRUE; AXIAL SCALE EXAGGERATED. SECOND FACE 126 LIES 0.30 mm INSIDE LOWERMOST SURFACE 118, AND PERIPHERAL SIDEWALL 130 BEARS ON THE RECESS WALL.

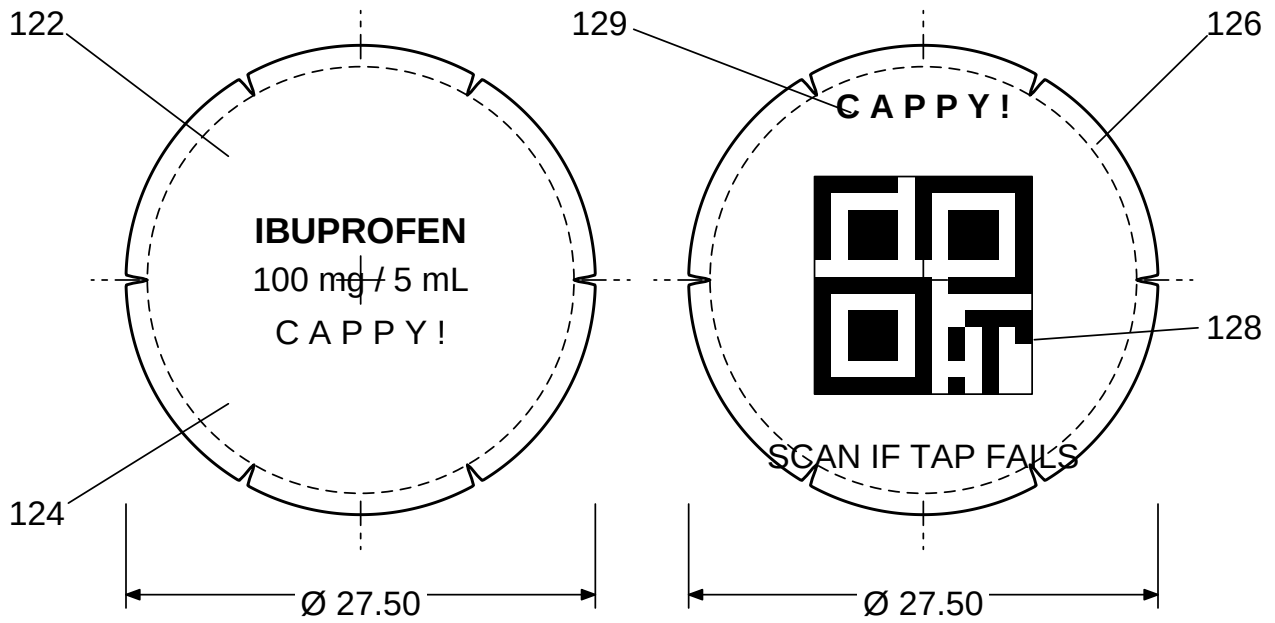


FIG. 3

PLAN VIEW — FIRST FACE 122. FACES UPWARD INTO BASE 114 AND IS READ THROUGH THE TRANSPARENT BASE.

FIG. 4

PLAN VIEW — SECOND FACE 126. FACES DOWNWARD AND IS EXPOSED AT BASE 114; NFC TAG 134 LIES WITHIN, ON THE OPPOSED SIDE.

BOTH FACES ARE SHOWN AT THE SAME SCALE. THE LOBED OUTLINE IS THE Ø 27.50 mm FREE PAD ENVELOPE; THE BROKEN CIRCLE IS THE Ø 25.00 mm RIGID CORE. FACE 122 CARRIES THE MEDICATION INDICIA AND FACE 126 CARRIES THE OPTICALLY-READABLE CODE.

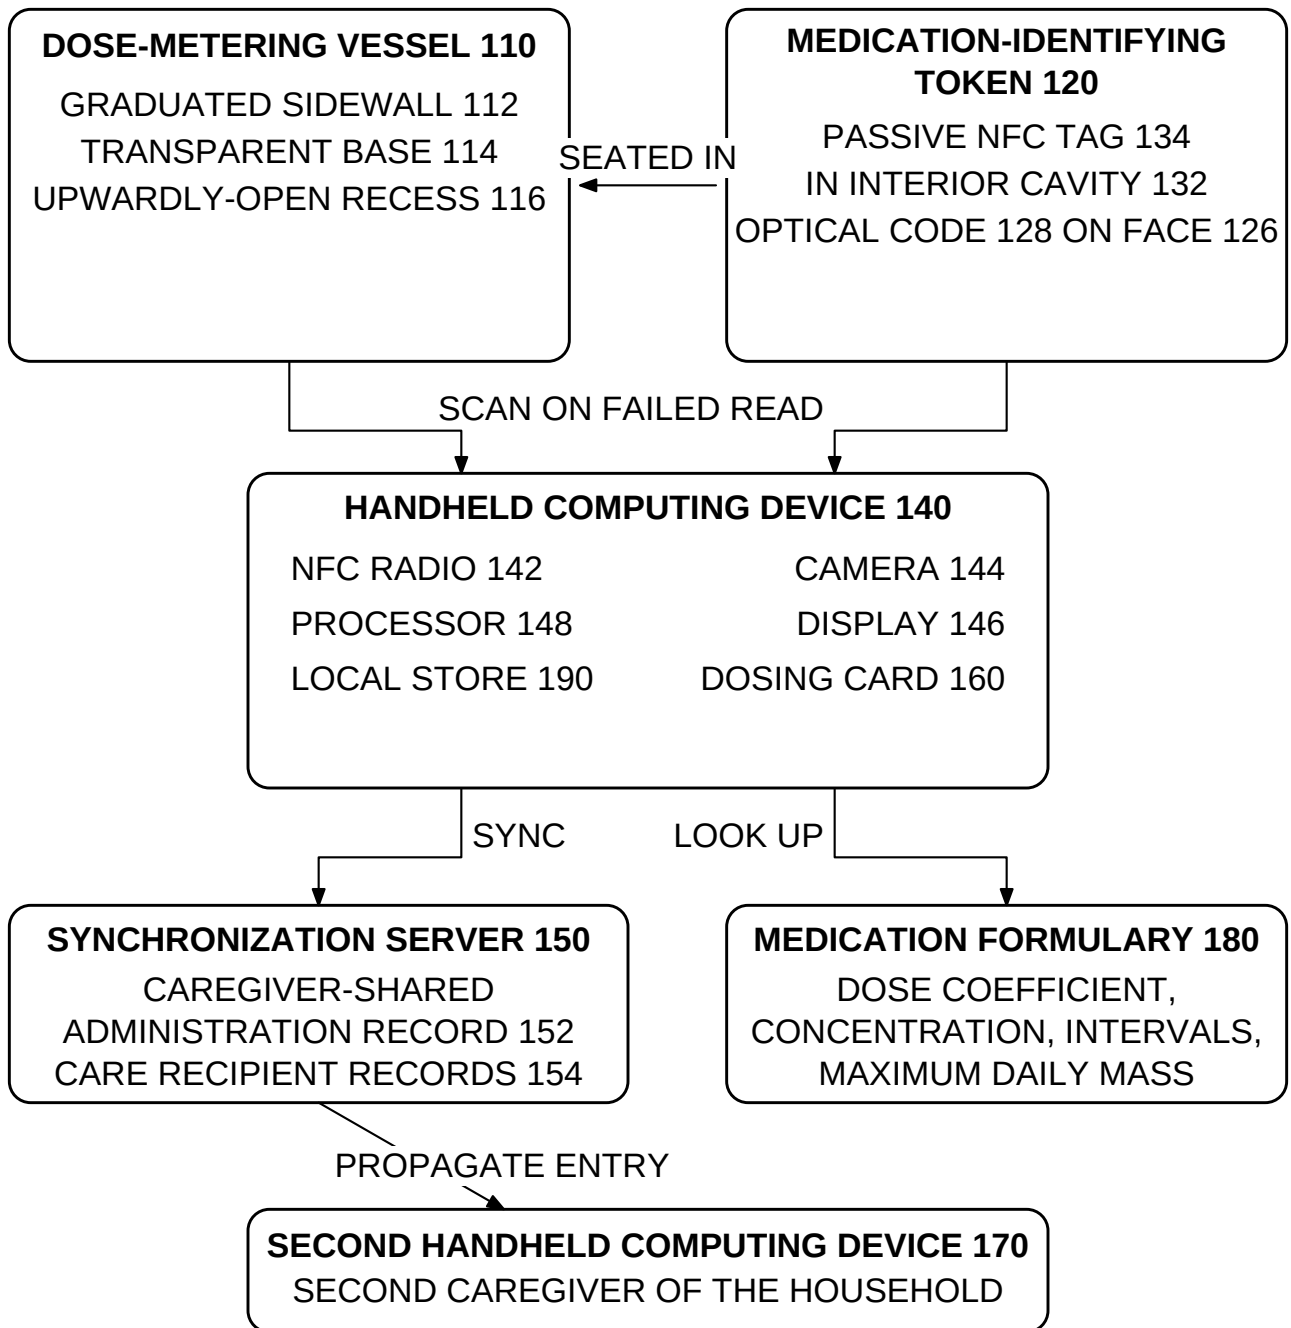
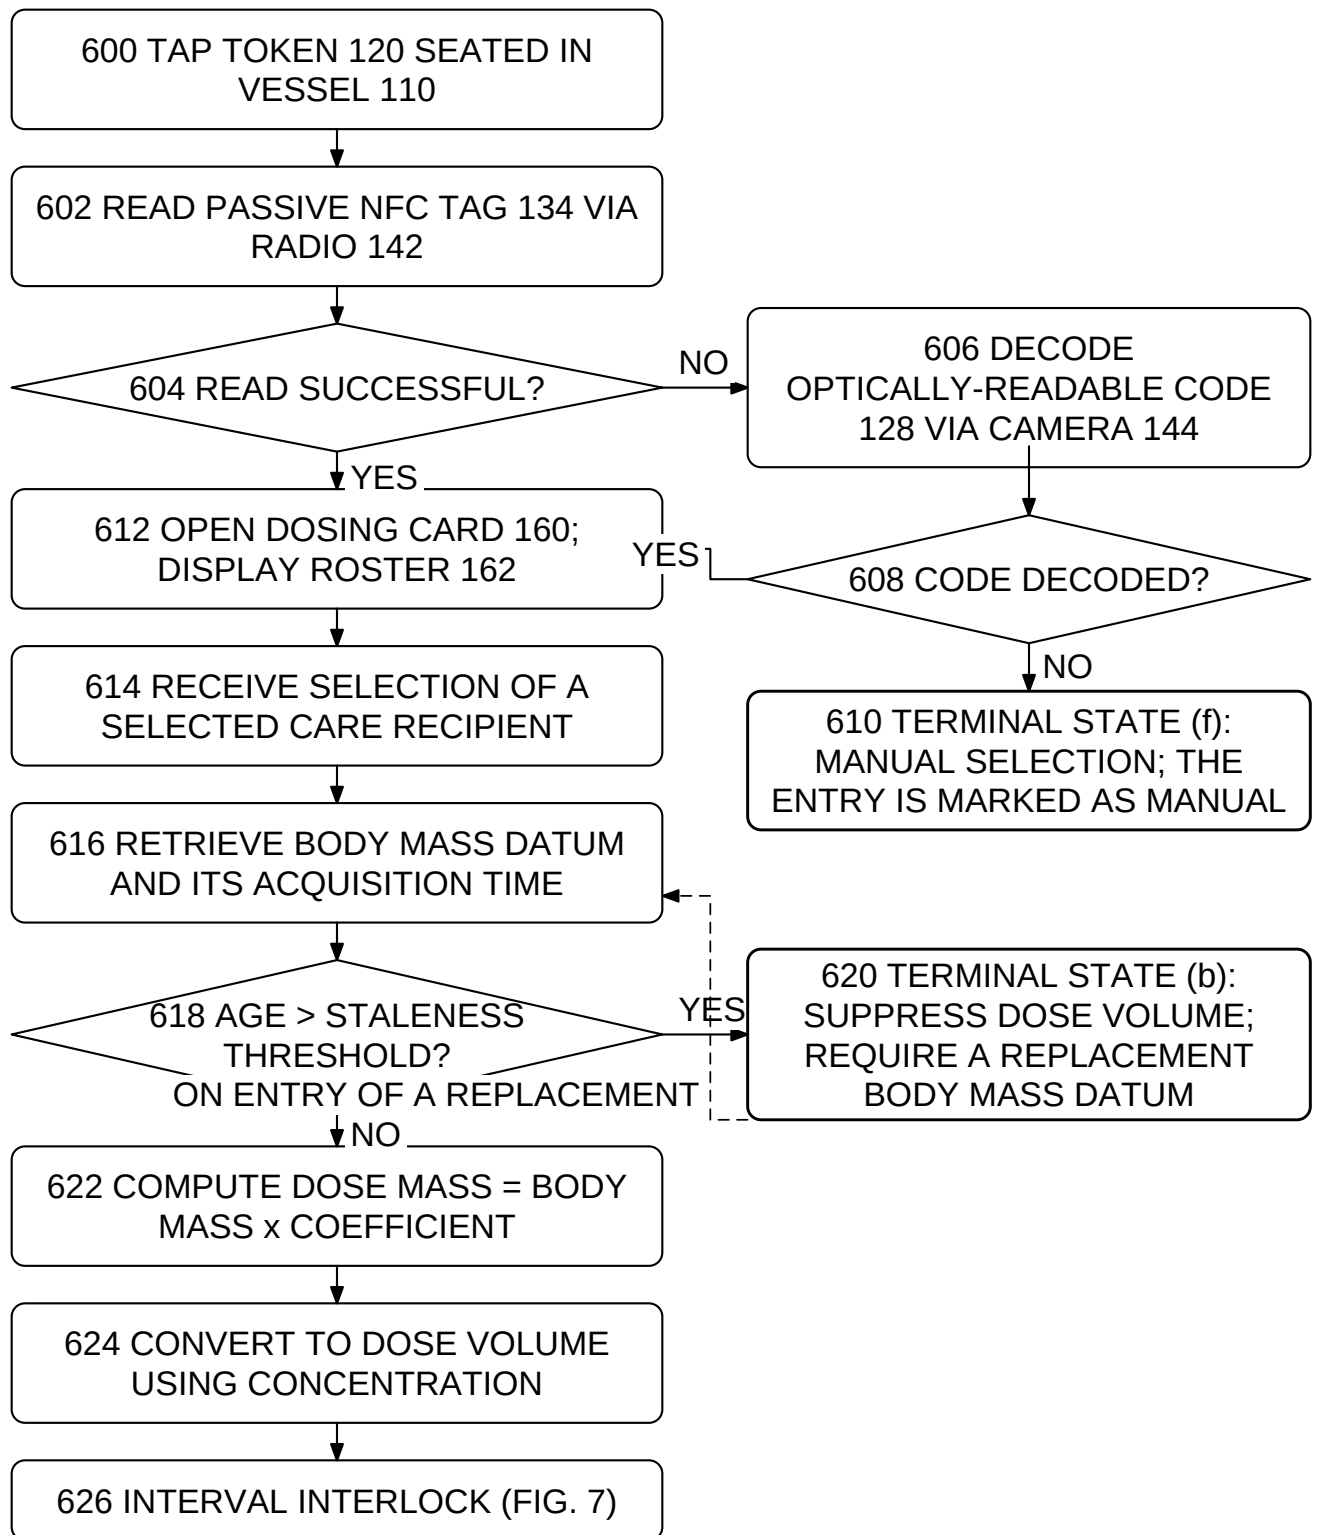
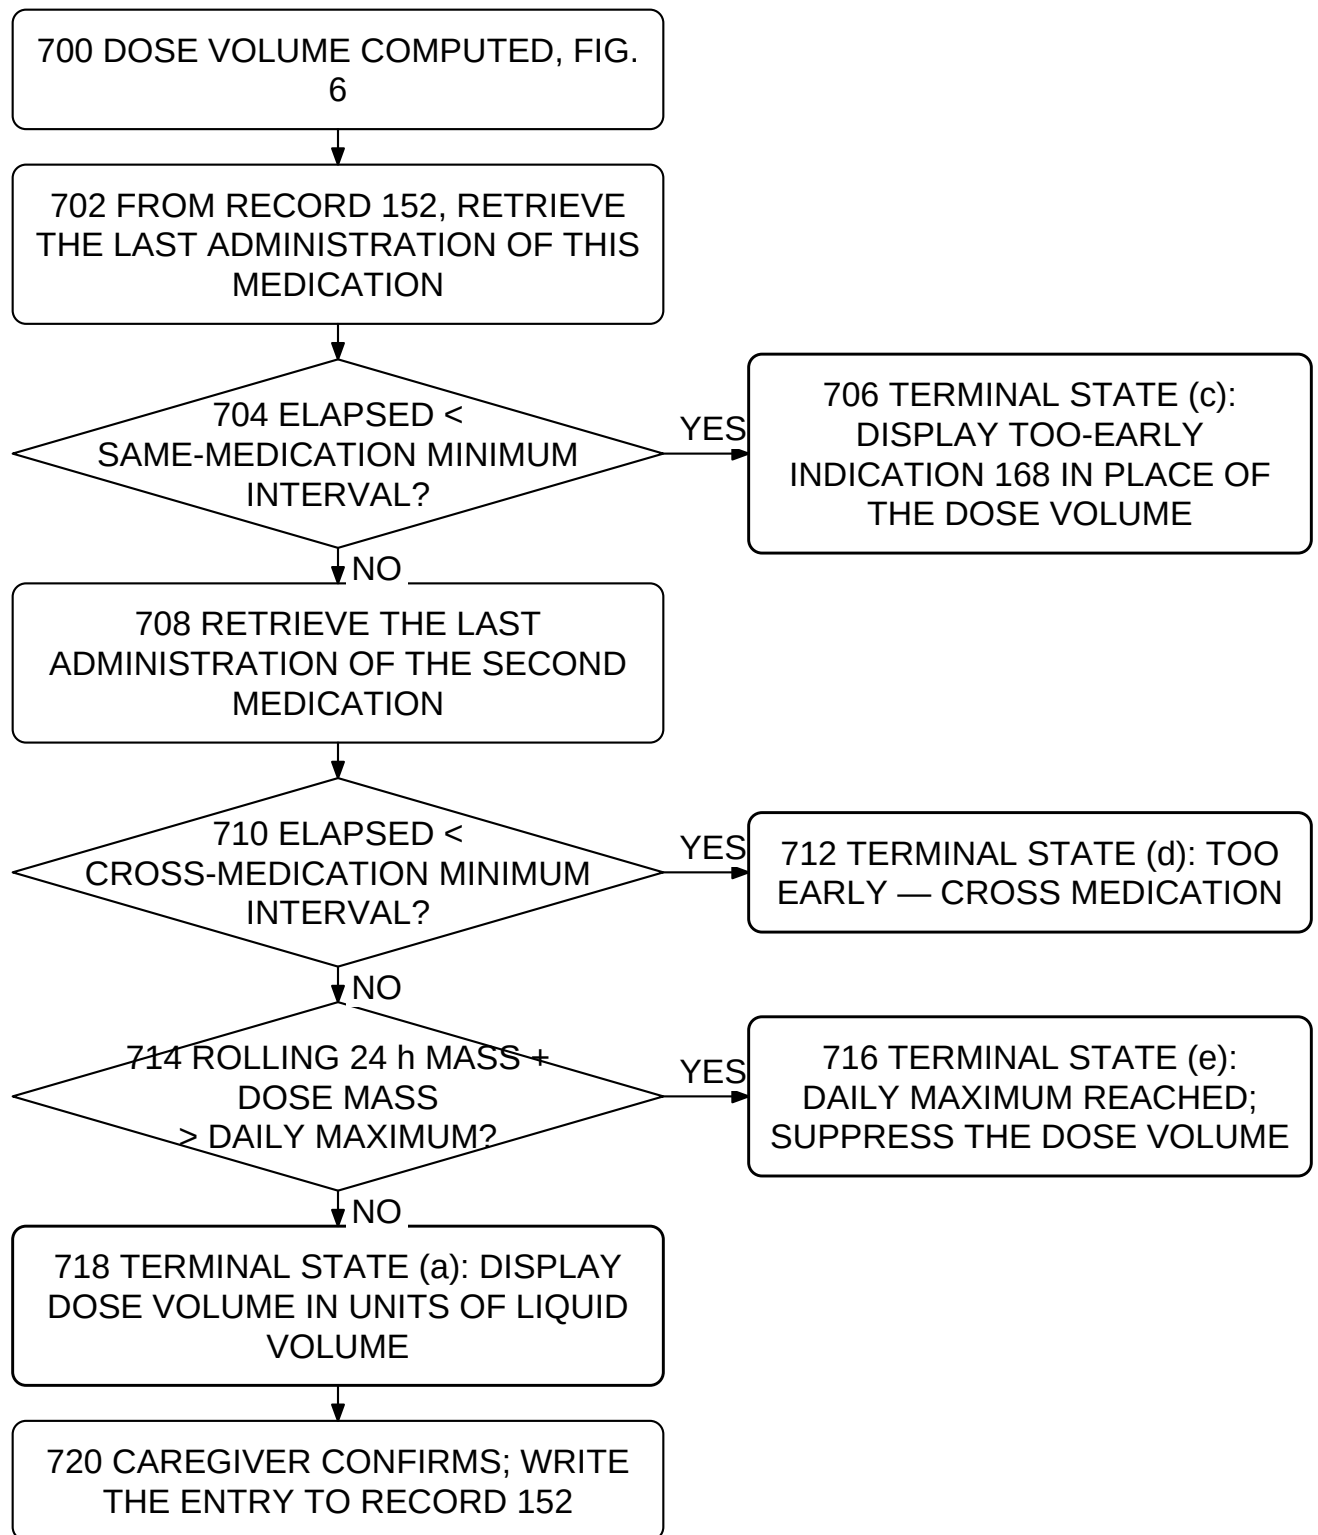



FIG. 5
MEDICATION DOSING SYSTEM 100

**FIG. 6**

DOSE VOLUME DETERMINATION WITH BODY MASS FRESHNESS GATE

**FIG. 7**

SAME-MEDICATION AND CROSS-MEDICATION INTERVAL INTERLOCK

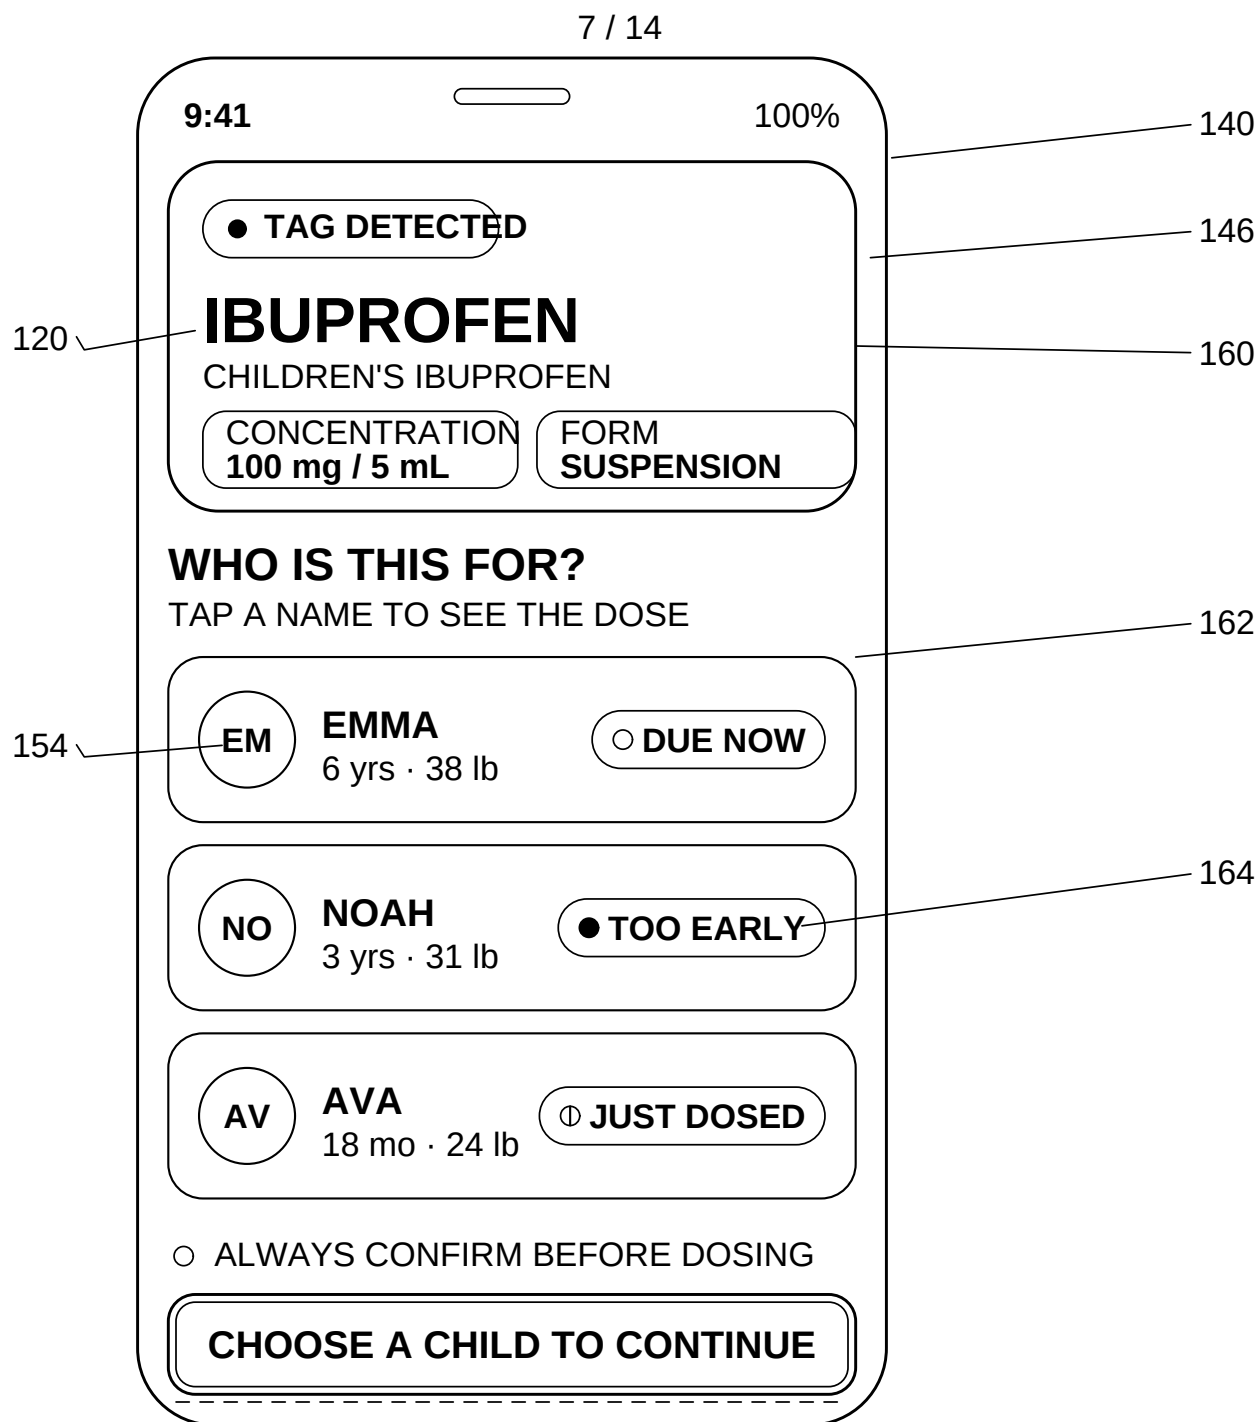

DOSING CARD 160 IS POPULATED FROM TOKEN 120. STATUS INDICIUM 164 CARRIES AN OPEN MARKER FOR A DOSE THAT MAY BE GIVEN, A SOLID MARKER FOR TOO EARLY, AND A DIVIDED MARKER FOR A DOSE JUST GIVEN; THE INTERFACE ITSELF SEPARATES THESE STATES BY COLOUR.

FIG. 8

DOSING CARD 160 — ROSTER 162 WITH STATUS INDICIA 164


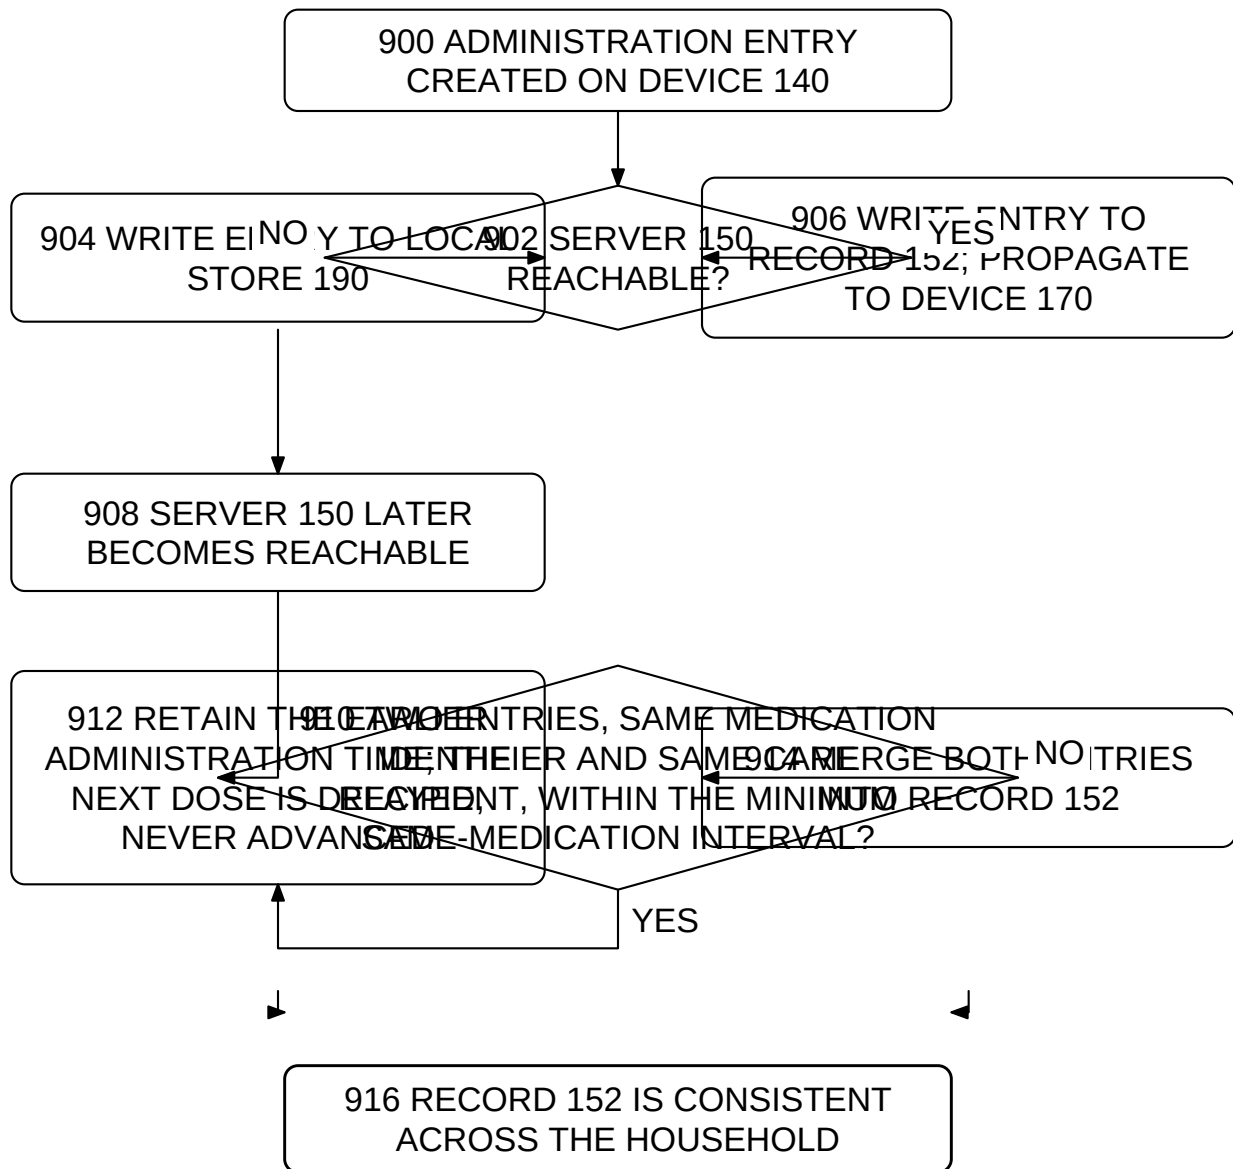



FIG. 9
OFFLINE RECONCILIATION OF ADMINISTRATION ENTRIES

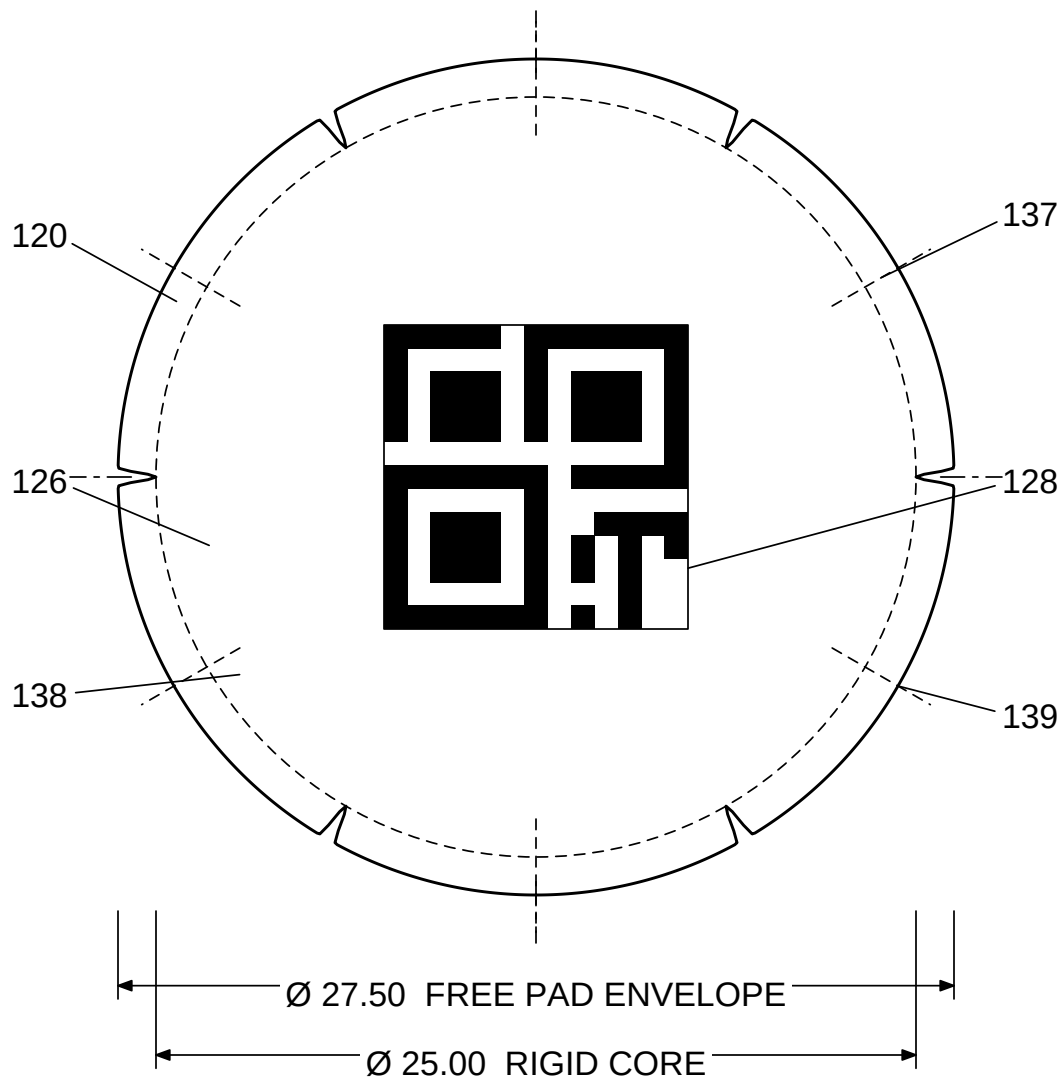

6 PADS ON 60° CENTRES · 1.25 mm RADIAL PROJECTION · 12.00 mm
 ROOT CHORD (57.37° SPAN). SIX PAD ROOTS COVER 95.6% OF THE
 CORE PERIMETER; NOMINAL GAP BETWEEN ROOTS IS 2.63° .

FIG. 10


PLAN VIEW — SECOND FACE 126 AND PAD GEOMETRY

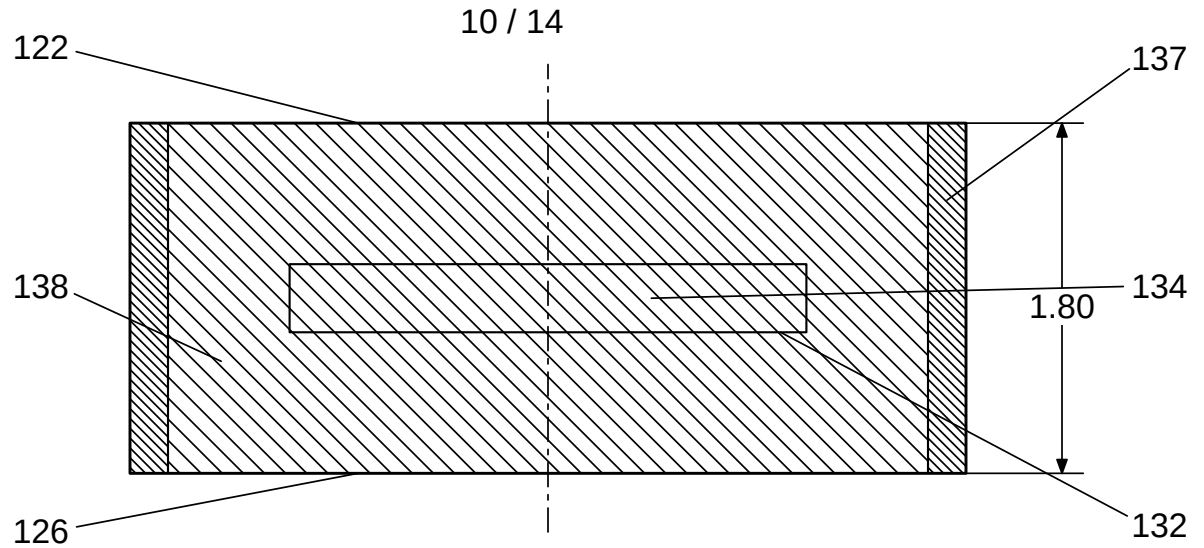

PADS EXTEND THROUGH THE FULL 1.80 mm AXIAL THICKNESS.
PAD MATERIAL AND DUROMETER ARE NOT LIMITING; THE NFC
INLAY IS SEALED WITHIN THE CORE.

FIG. 11


SECTION A-A THROUGH OPPOSING PADS — FREE STATE. RADIAL
SCALE TRUE; AXIAL SCALE ENLARGED FOR CLARITY.

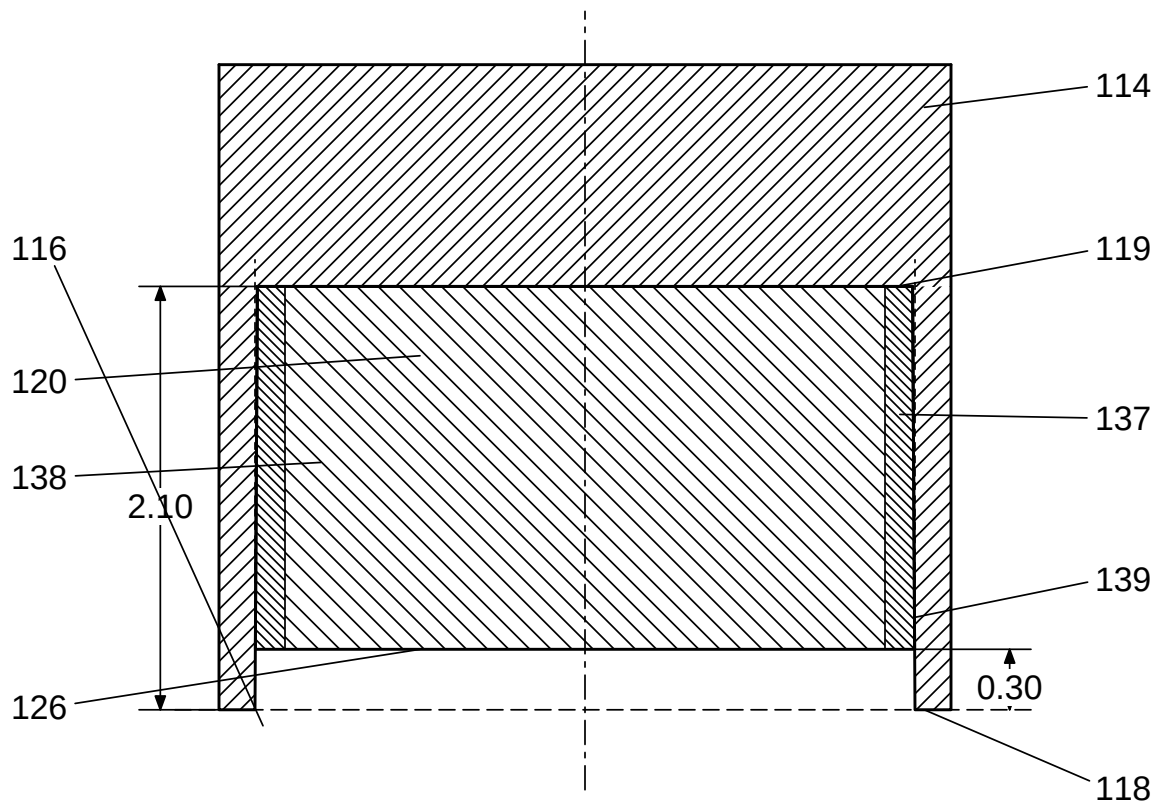

RECESS 116 TAPERS FROM $\varnothing 27.50$ AT LOWERMOST SURFACE 118 TO $\varnothing 27.30$ AT DEEPEST PLANE 119, A WALL HALF-ANGLE OF 2.73° . THE LOCAL CAVITY DIAMETER AT THE EXTERNAL TOKEN FACE IS $\varnothing 27.471$, SO PAD 137 DEFLECTS RADially BETWEEN 0.014 mm AND 0.10 mm. NO LIP OR POSITIVE SNAP FEATURE IS ASSUMED; RETENTION IS BY INTERFERENCE AT THE PADS.


FIG. 12

ENLARGED DETAIL — TOKEN 120 INSTALLED IN RECESS 116. RADIAL SCALE TRUE; AXIAL SCALE AND WALL TAPER EXAGGERATED.

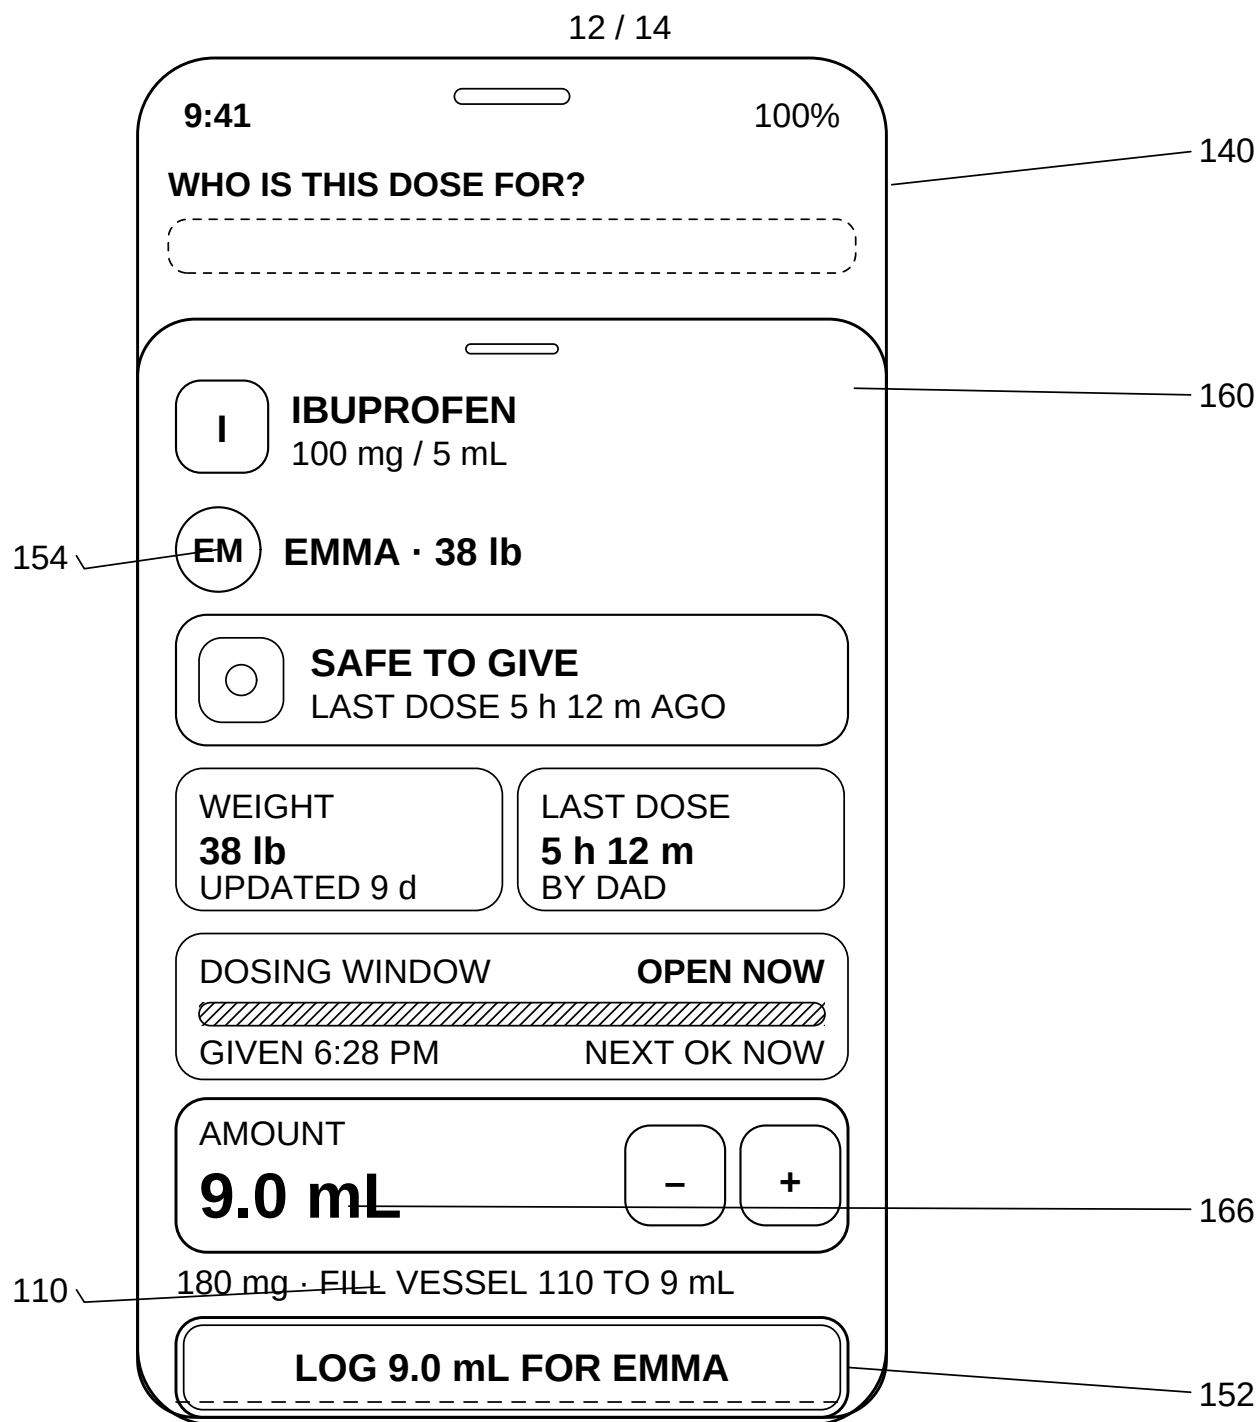

TERMINAL STATE (a) OF FIG. 7. DOSE VOLUME 166 IS GIVEN IN UNITS OF LIQUID VOLUME AND REFERRED TO A GRADUATION ON SIDEWALL 112, SO THE CAREGIVER NEVER CONVERTS A MASS INTO A VOLUME. CONFIRMING WRITES AN ENTRY TO RECORD 152.


FIG. 13
DOSING CARD 160 — DOSE VOLUME 166

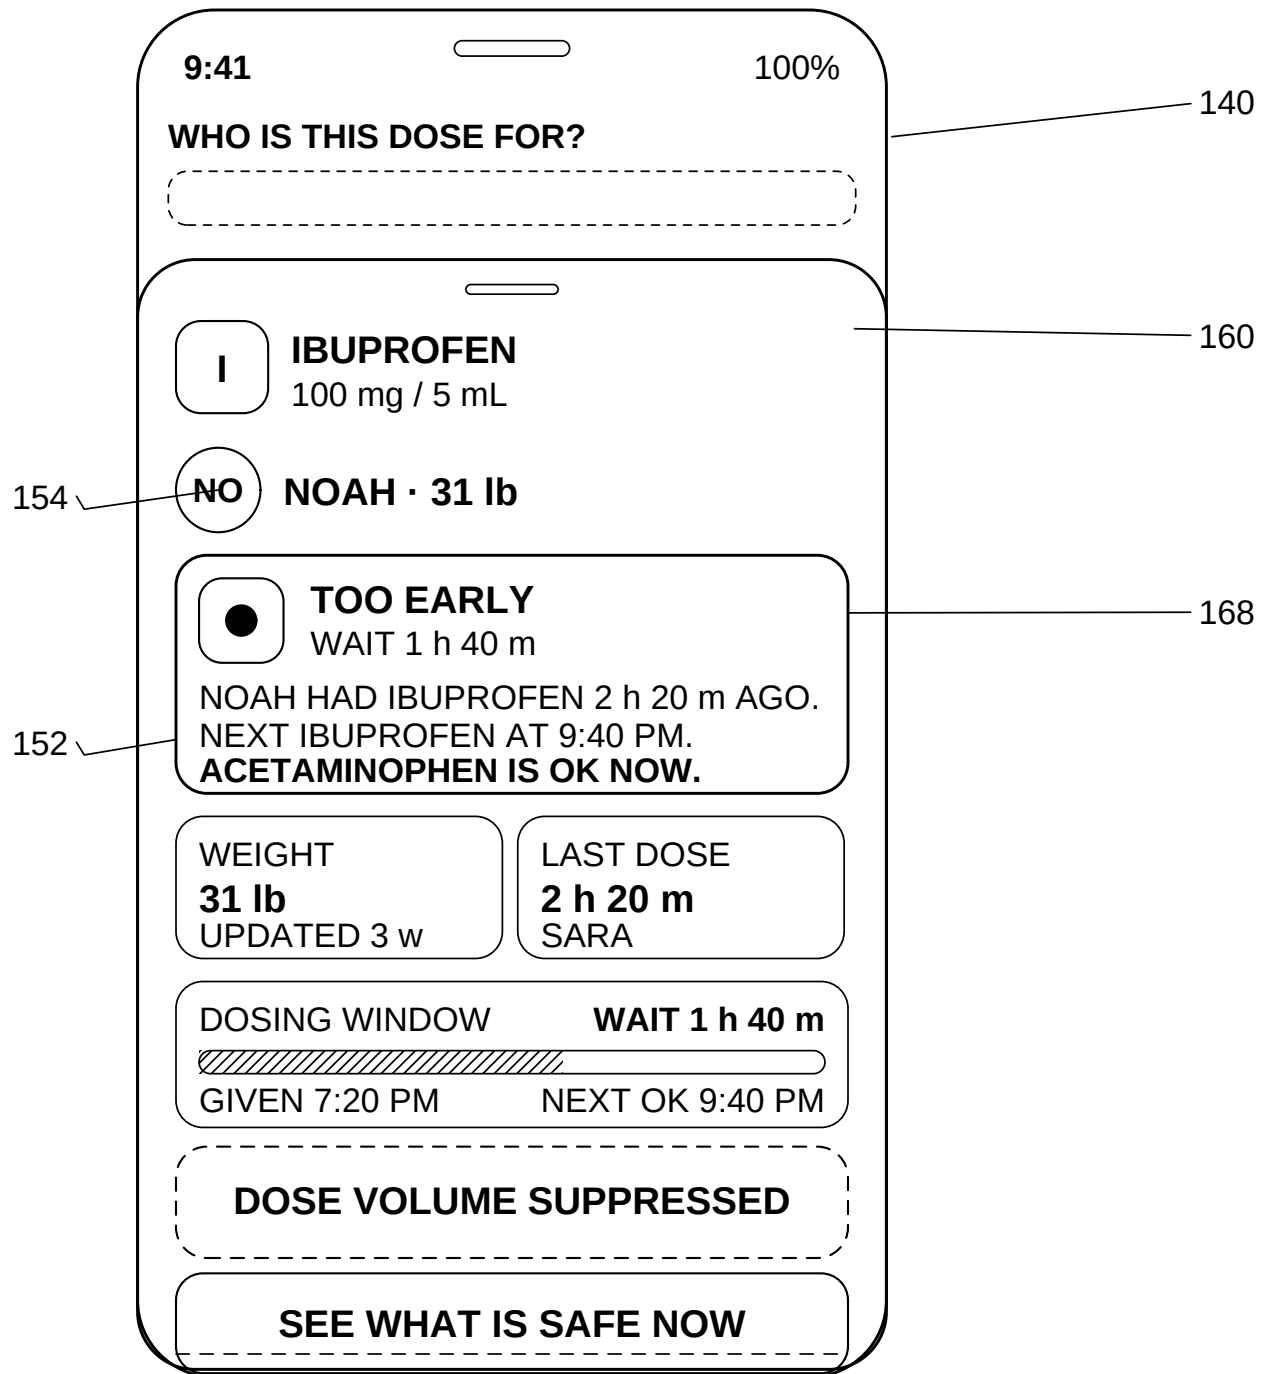

TERMINAL STATE (c) OF FIG. 7. TOO-EARLY INDICATION 168 REPLACES THE DOSE VOLUME, NAMES THE REMAINING INTERVAL, AND OFFERS THE SECOND MEDICATION WHERE THE CROSS-MEDICATION INTERVAL PERMITS.

FIG. 14

DOSING CARD 160 — TOO-EARLY INDICATION 168 IN PLACE OF THE DOSE VOLUME

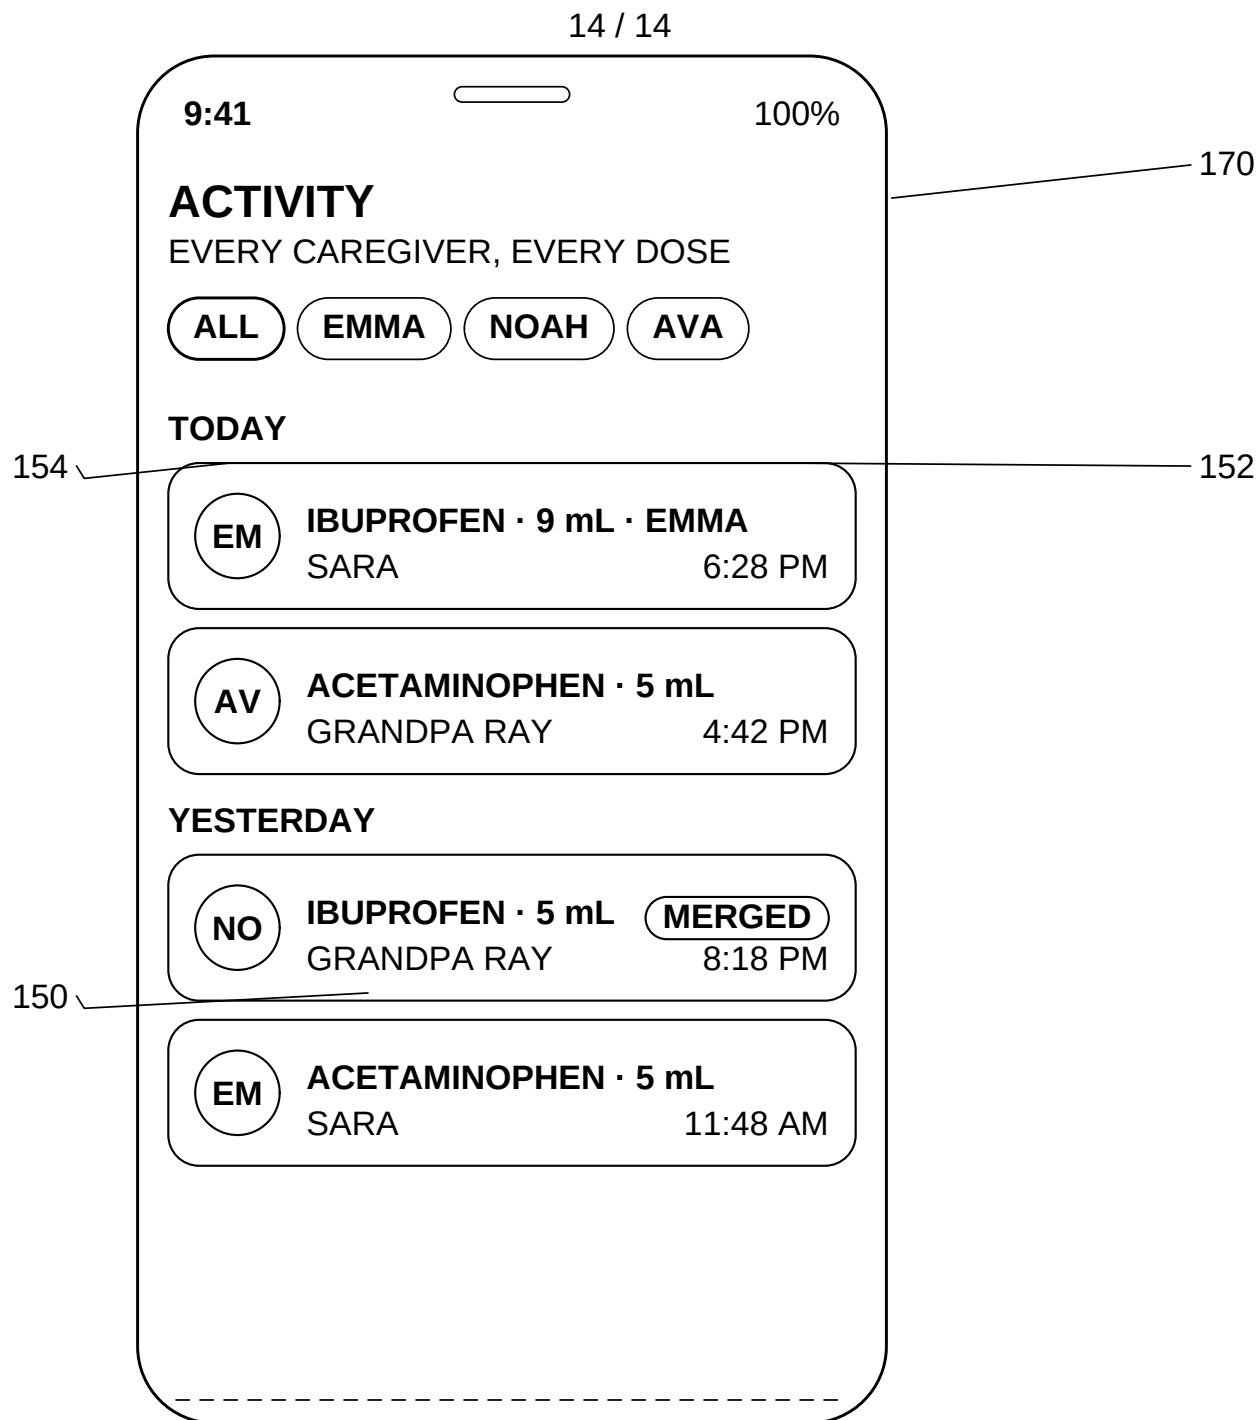

CAREGIVER-SHARED ADMINISTRATION RECORD 152 AS IT REACHES SECOND HANDHELD COMPUTING DEVICE 170. AN ENTRY RECONCILED BY THE PROCESS OF FIG. 9 IS MARKED MERGED AND CARRIES THE EARLIER OF THE TWO ADMINISTRATION TIMES.

FIG. 15
ADMINISTRATION RECORD 152 ON SECOND DEVICE 170