


Calibration (Brier = 0.000)

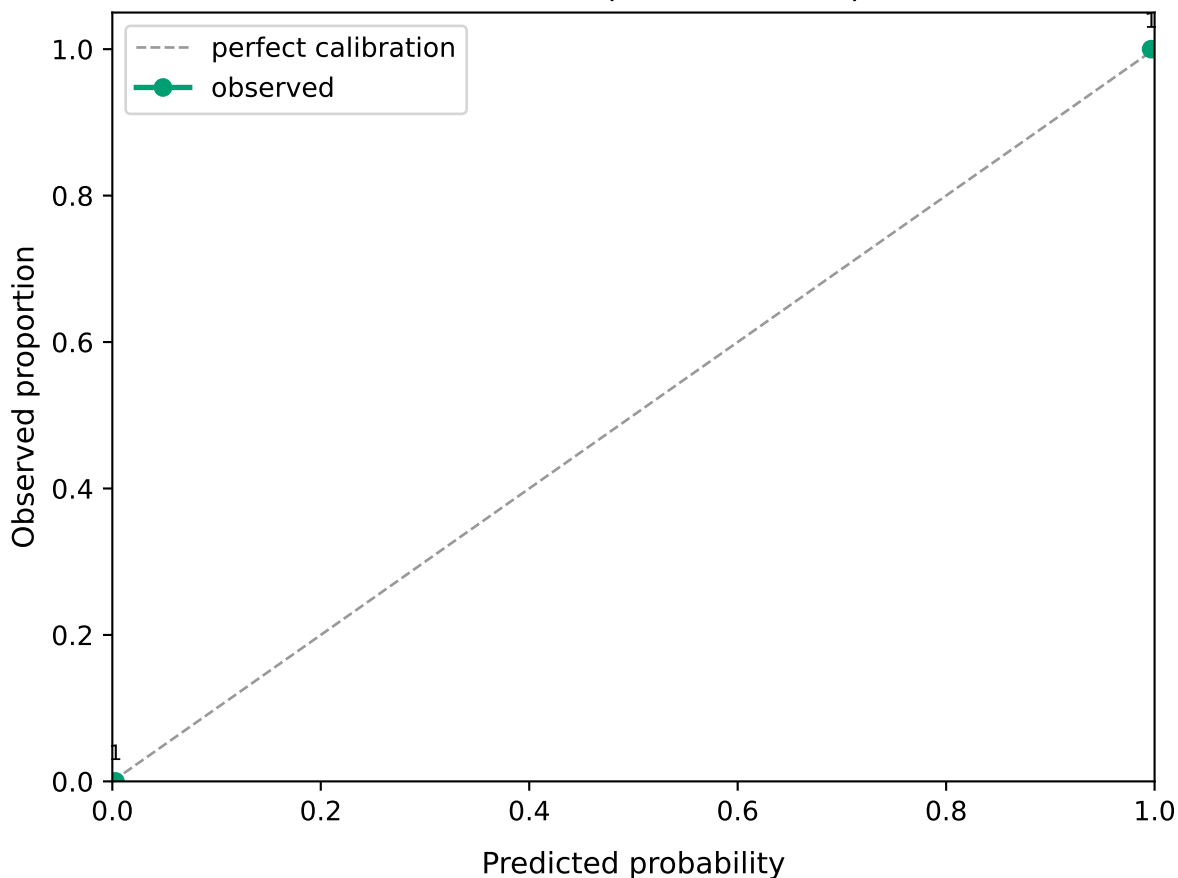

split=validation | bins=10 | source hash=51673c6282a8...

DEMO / simulated data - not for clinical/publication use