GlycoTwin architecture

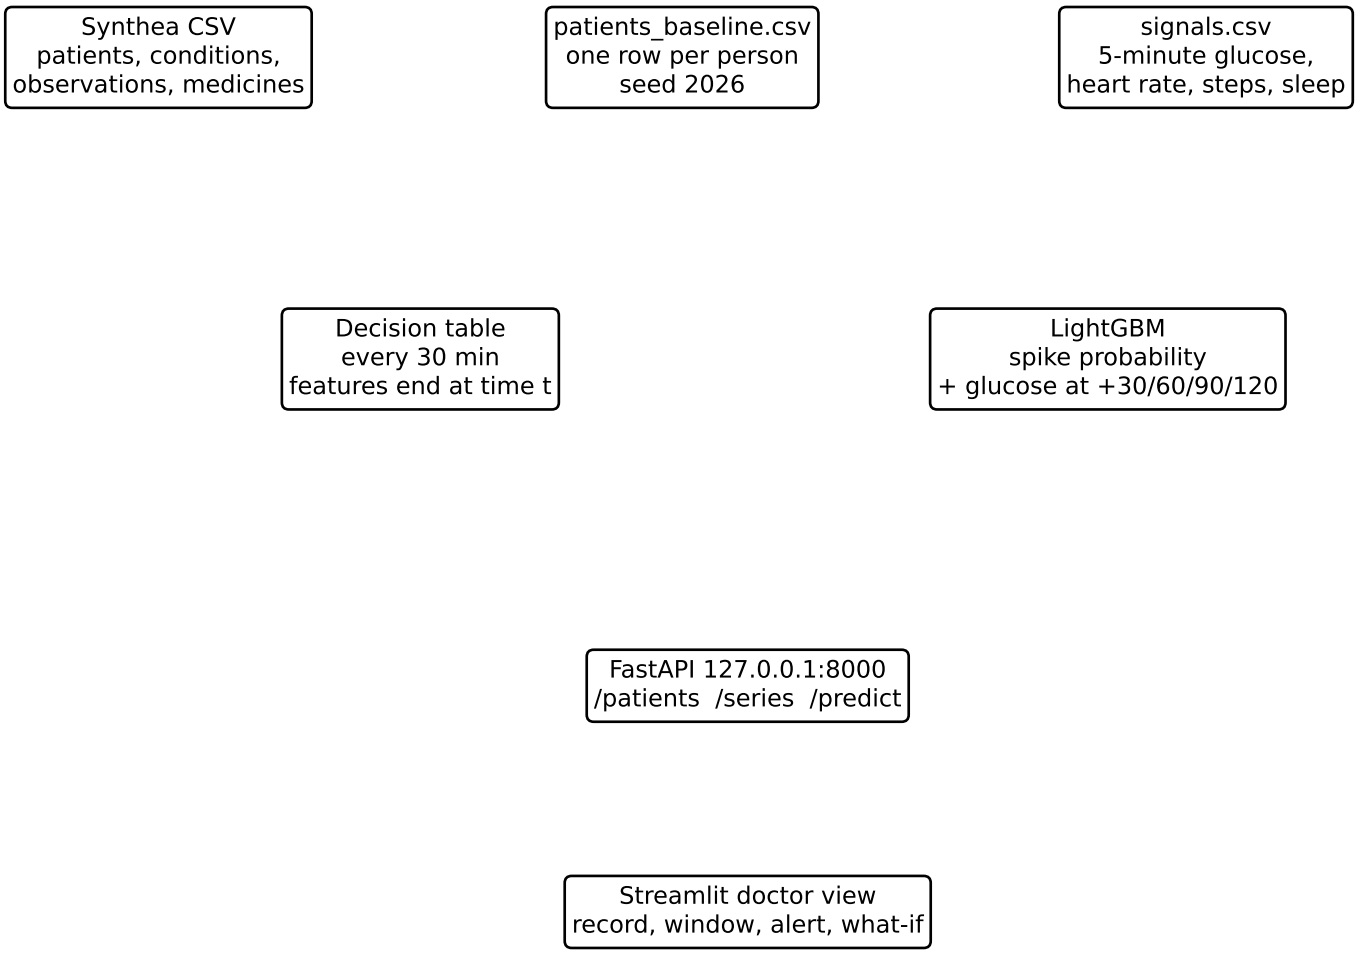

Same patient_id on the record and the wearable series. Synthetic glucose is not a watch recording.