



Pupil position





Corneal reflex (CR)




Pupil minus CR



Maximum power

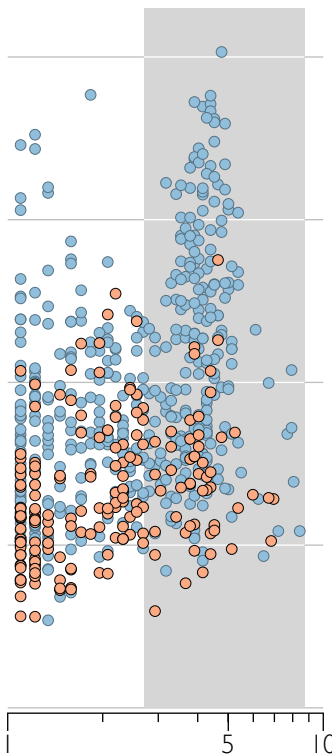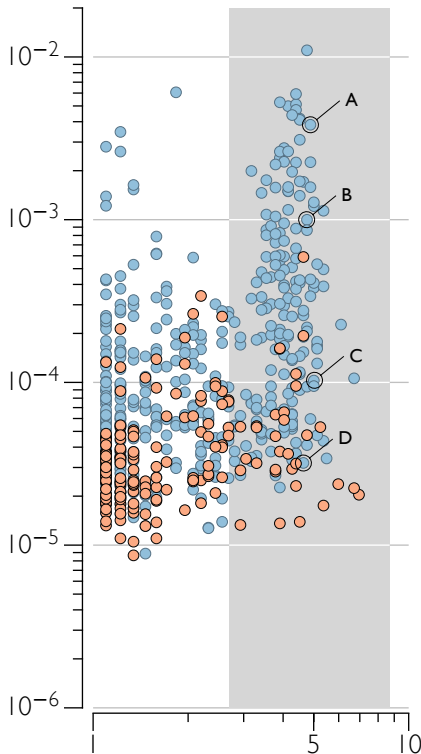

● PD  
● Control

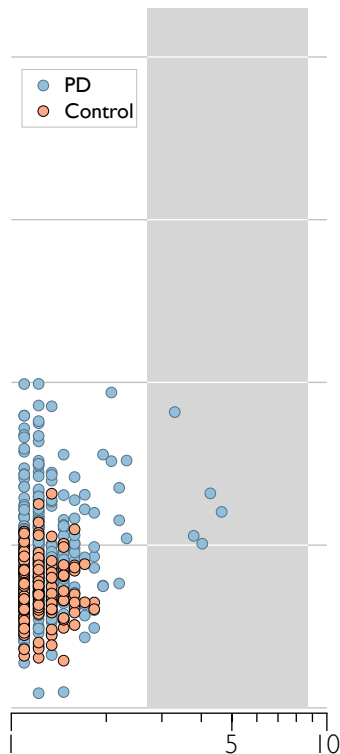

Frequency at which maximum power occurs (Hz)