OIML Certification System	CMI	V 3112

OIML Member State	**OIML Certificate No.**
Czech Republic	R76/2006-A-CZ1-26.03

OIML CERTIFICATE ISSUED UNDER SCHEME A

OIML Issuing Authority

Name: Czech Metrology Institute
Address: Okružní 31
638 00 Brno
Czech Republic

Person responsible: Jan Kalandra

Applicant

Name: CAS Corporation
Address: #262, Geurugogae-ro, Gwangjeok-myeon
Yangju-si, Gyeonggi-do
Republic of Korea

Manufacturer

Name: CAS Corporation
Address: #262, Geurugogae-ro, Gwangjeok-myeon
Yangju-si, Gyeonggi-do
Republic of Korea

Identification of the certified type *(the detailed characteristics will be defined in the additional pages)*

Non-automatic weighing instrument, dual interval, intended to be used for variable applications as portable bench scale
type PB Series

Designation of the module *(if applicable)*

-

This OIML Certificate attests the conformity of the above identified type (represented by the sample(s) identified in the OIML type evaluation report) with the requirements of the following Recommendation of the International Organization of Legal Metrology (OIML):

OIML R 76 Edition (year): 2006

For accuracy class: III

Český metrologický institut
-3-

This OIML Certificate relates only to metrological and technical characteristics of the type of measuring instrument covered by the relevant OIML Recommendation identified above.

This OIML Certificate does not bestow any form of legal international approval.

The conformity was established by the results of tests and examinations provided in the associated reports:

Test report No. 6012-PT-R0005-26 dated 19.09.2026 that includes 53 pages.
Test report No. 8551-PT-E0338-26 dated 20.08.2026 that includes 30 pages.

OIML type evaluation report No. 0511-ER-N116-25 dated 21.09.2026 that includes 11 pages.

The technical documentation relating to the identified type is contained in documentation file:

0511-UL-N116-25

OIML Certificate History

Revision No.	Date	Description of the modification
-	22 September 2026	Issuing of certificate

The OIML Issuing Authority
RNDr. Pavel Klenovský
Director of Certification Body

Date: 22 September 2026


Český metrologický institut
-3-

Important note: Apart from the mention of the Certificate's reference number and the name of the OIML Member State in which the Certificate is issued, partial quotation of the Certificate and of the associated OIML type evaluation report(s) is not permitted, although either may be reproduced in full.

1 Characteristics of the instrument

The PB series is a non-automatic electronic weighing instrument for general-purpose bench weighing. It comprises a load receptor, single-point strain-gauge load cell, mechanical base with overload protection, detachable indicator, main electronic board, six-digit LCD, four keys, and battery/external-adaptor power facilities. The instrument is designed as a dual-interval Class III weighing instrument.

The name of the instruments may be followed by alphanumeric characters for technical, legally or commercial characterisation of the instrument.

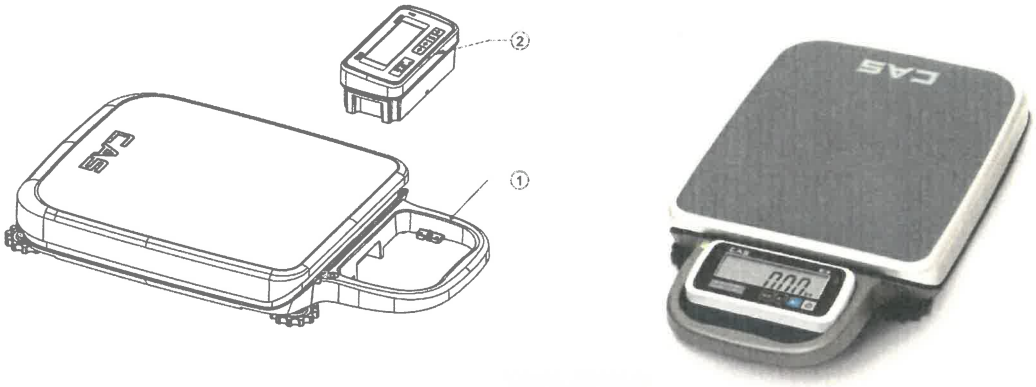

Picture 1 PB series overview

2 Metrological characteristics

Type	**PB series**			
Ingres protection rating	IP52			
Display	LCD			
Operating temperature	-10°C … 40 °C			
Accuracy class OIML R76	III			
The applied error fraction p_i	1			
Weighing software version	The **legally relevant software version is V 5xx or yy5xx**(The „xx“ represent sub version number reflecting non-legally relevant changes. “yy” represent country code. Both parameters can be number from 00 to 99)			
Application software version	N/A			
Operating system	Embedded			
Primary indication unit	kg			
Weighing range configuration	Dual interval	Dual interval	Dual interval	Dual interval
Max	**15 / 30 kg**	**30/60 kg**	**60/150 kg**	**100/200 kg**
Min	100 g	200 g	400 g	1000 g
Verification Scale interval e =	5/10 g	10/20 g	20/50 g	50/100 g
Actual Scale interval d =	e			
Maximum number of Verification Scale Intervals (per Weighing Range) n =	2 x 3000			
Maximum subtractive Tare effect	-14,995 kg	-29,99 kg	-59,98 kg	-99,950 kg
Load cell	CAS Corporation BCS-PB-1K			
E_{max}	50 kg	100 kg	200 kg	250 kg
Power supply, voltage	external 12 V AC/DC, 1.25 A adaptor; four 1.5 V C-size dry batteries; optional 6 V, 1.3 Ah rechargeable lead-acid battery			

Český metrologický institut
-3-

3 Devices and functions

- Determination of stability of equilibrium.
- Initial zero setting device (≤ 20% of Max).
- Zero indication.
- Semi-automatic zero setting device (≤ 4% of Max).
- Automatic zero tracking (≤ 4% of Max).
- Semi-automatic tare balancing device. The net indicator is on, when a tare is active.
- Net indicator.
- Weight hold/averaging. Pressing HOLD during unstable indication initiates averaging. "HOLD" appears twice, followed by the average; the function then cancels automatically.
- Gravity compensation.
- Low battery indication.

3.1 Additional Instrument Functions

No additional functionality available.

4 Interfaces

On the main board are UART interfaces without access for users used for software updates, peripheral devices and service features.
Optional Bluetooth interface. Communication and data are not protected and cannot be used for legal purposes.

Český metrologický institut
-3-