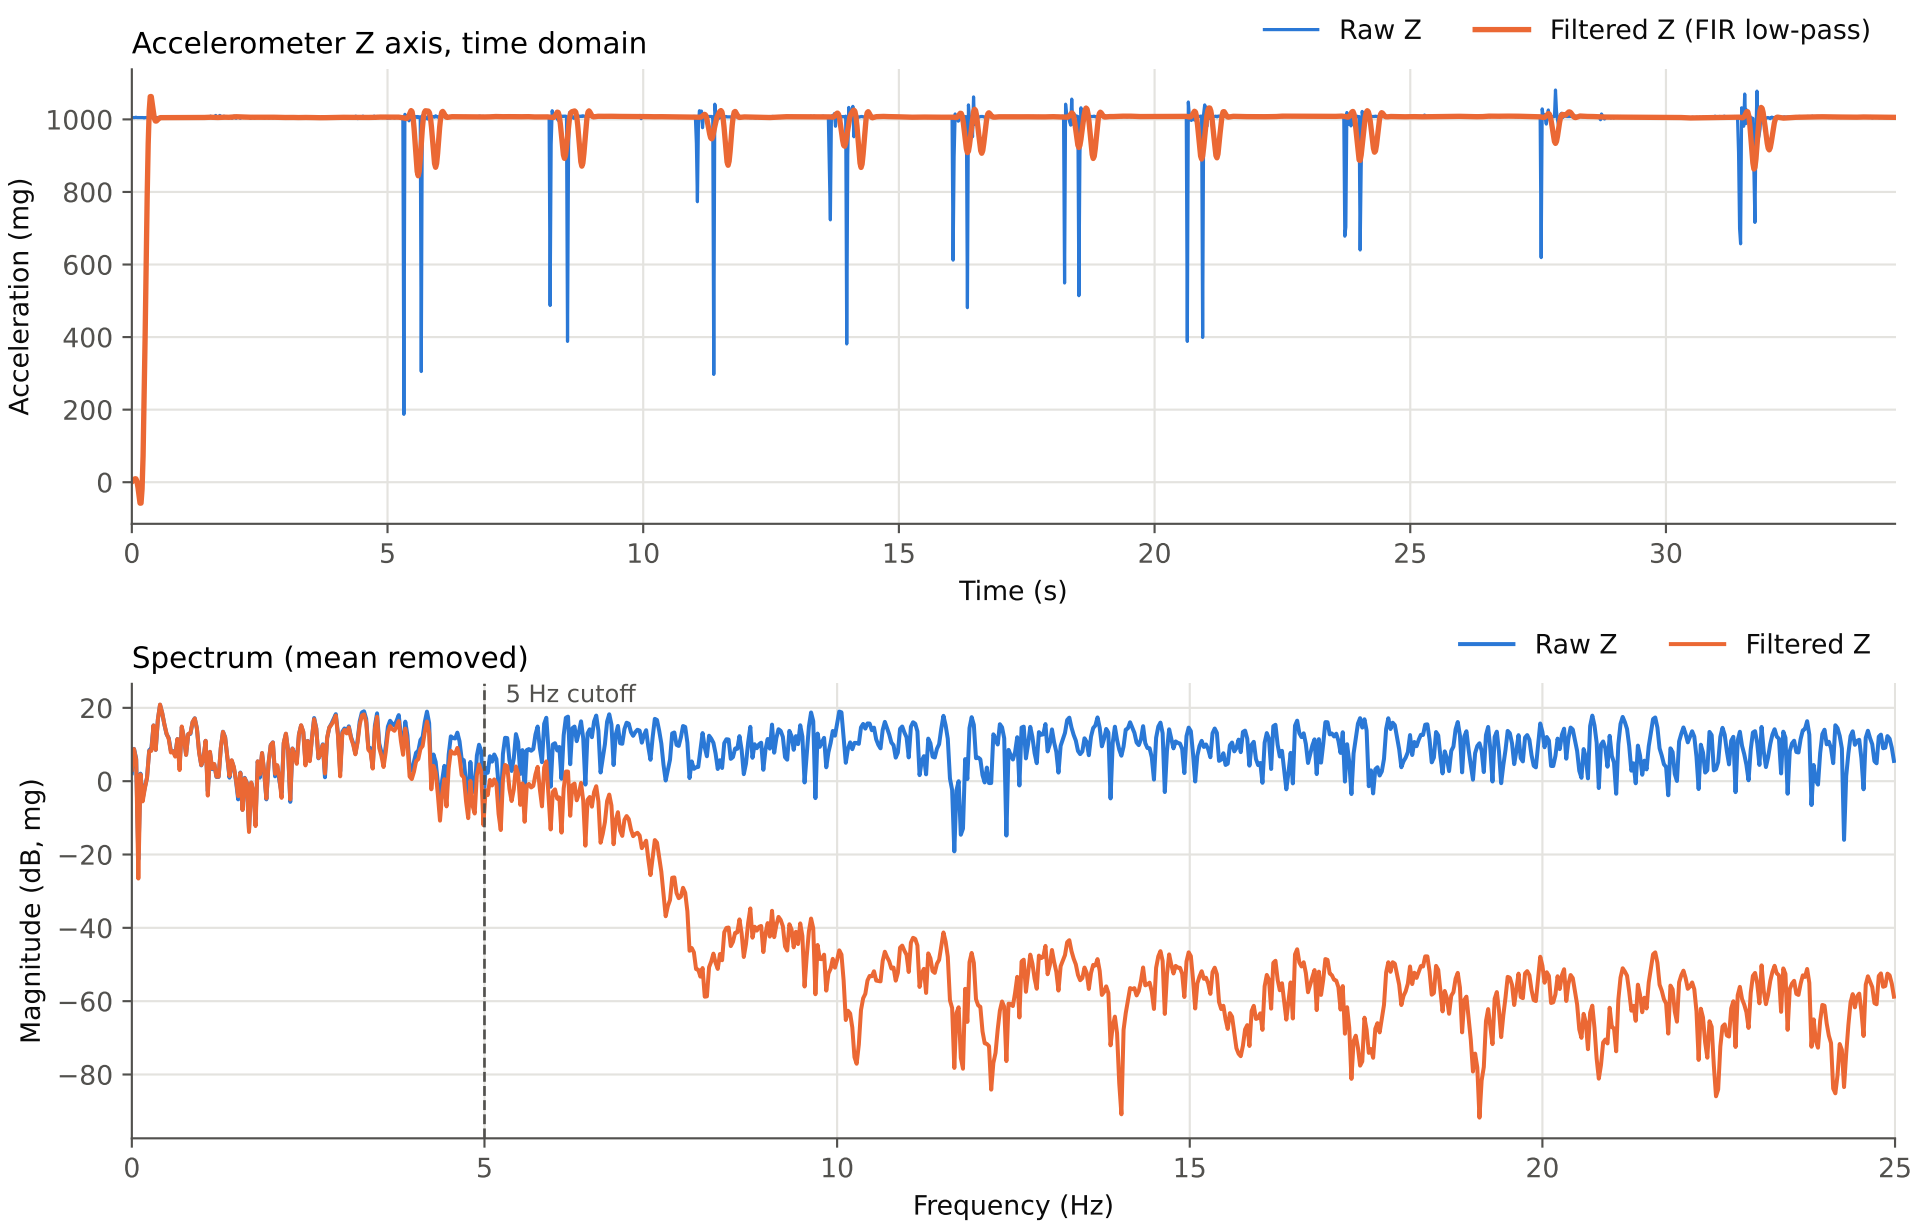
Accelerometer Z axis, time domain
Raw Z
Filtered Z (FIR low-pass)
Acceleration (mg)
1000
800
600
400
200
0
0
5
10
15
20
25
30
Time (s)
Spectrum (mean removed)
Raw Z
Filtered Z
5 Hz cutoff
Magnitude (dB, mg)
20
0
−20
−40
−60
−80
0
5
10
15
20
25
Frequency (Hz)