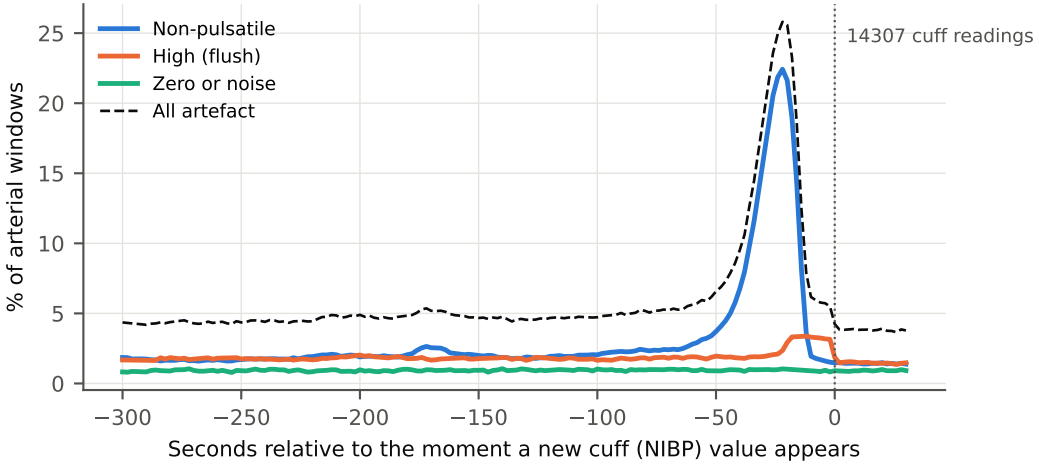
Non-pulsatile
High (flush)
Zero or noise
All artefact
14307 cuff readings
% of arterial windows
25
20
15
10
5
0
−300
−250
−200
−150
−100
−50
0
Seconds relative to the moment a new cuff (NIBP) value appears