


Spooky²

Cancer Protocols x 4

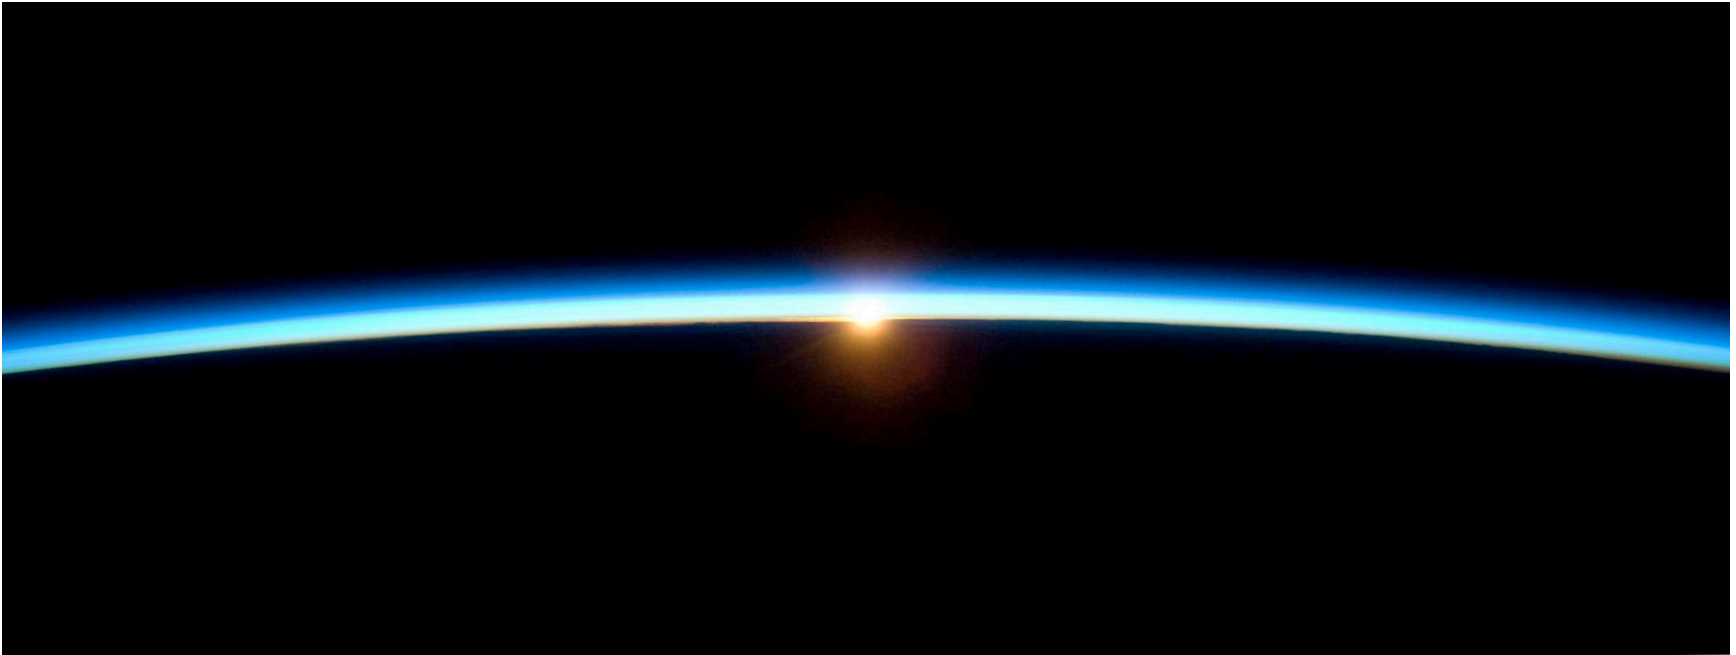

March 2020

By the Spooky Team

Table of contents

The problem with cancer	3
Three tasks	5
Biofeedback scanning	5
Editing Presets	12
Editing Plasma Presets	22
Building Presets	32
Plasma Plus	41
Phase I – Terrain	44
Phase II – Target	45
Scalar Plus	46
Phase I – Terrain	48
Phase II – Target	49
Contact Plus 4	50
Phase I – Terrain	51
Phase II – Target	52
Contact Plus 2	53
Phase I – Terrain	55
Phase II – Target	55
Extras:	56
Protocol history	57

Click on a section to go there.

The problem with cancer

Using Rife technology to deal with cancer isn't simply a matter of killing cancer cells. There's much more to it than that. Cancer cells produce many poisonous byproducts as they furiously reproduce. When you kill a cancer cell, it's likely to rupture and release its toxic contents. At best, it may retain cell wall integrity until nature and time take over. Then it spills its poisons.

So, depending on the extent of the cancer, and the rate at which you kill it, you're going to have countless dead cancer cells in your body, all of them carrying – or leaking – poison. While our healthy cells are constantly dying and being replaced, these are not filled with toxins, and they're not all dying at the same time, so our body systems can deal with this natural process without problems.

Dr. Royal Raymond Rife treated his cancer patients for five minutes a day every third day. He limited his treatments in this way so as not to overwhelm patients with toxins from killed cells, and to allow their body systems and organs enough time to deal with the cleanup of the destruction his treatment had achieved.

There's a very good reason for what he did: toxic overload can shut down the liver and kidneys very quickly, and can even kill. At that time, only killing frequencies existed – detox and support frequencies came later.

So you have to get all this dangerous rubble out of the body as quickly as possible. And you do that by using detox frequencies. Doing this prevents the pollutants from settling, and keeps them moving so that they enter the bloodstream, the lymphatic system, and the intestines. And this is where the next problem arises.

The eliminatory system consists of the liver, the kidneys, the intestines, the lungs, and the skin, but only the first two need concern us here. Even a healthy body would find it difficult and damaging to try to cope with an internal tidal wave of toxins like this, so a body weakened by cancer and the ravages of certain other treatments would be brought under great strain – unless the liver, kidneys, and intestines were actively supported.

IMPORTANT: this document outlines four Spooky² methods to deal with cancer. Since these methods have many things in common, we won't repeat them all four times. Instead, we ask you to read this document in its entirety so that you miss nothing.

And then there's the problem of managing the pain of cancer without further poisoning the body. So dealing effectively with cancer isn't just one single job of killing cancer cells. It's actually four tasks, all vital – killing, detox, support, and pain control.

Prior to the introduction of the Spooky² Rife System, you'd have had to tackle each of these jobs separately. So you would have been sitting next to a machine holding electrodes, not just for a couple of hours as you perhaps believed, but for anything up to eight hours every day, depending on your condition.

But, uniquely, Spooky² offers the extraordinary ability to perform parallel processing. This allows multiple jobs to be performed by multiple systems operating at the same time, often in different transmission modes. So for certain conditions like late-stage cancers, Lyme Disease, Morgellons Disease, and other synergistic multi-system multi-pathogen illnesses, we strongly recommend using parallel processing.

The Spooky² Rife System offers two main routes to tackle cancer. The first uses Plasma Mode as its principal weapon, and the second uses Contact Mode. Both of these are adjuncted by Remote Mode.

Because there are many different types of cancer, this document gives necessarily broad outlines of how I would personally approach dealing with late-stage cancer in both modes. I've further subdivided contact mode into two plans, one for four Spooky²-XM frequency generators, and one for two.

For the purposes of this document, I'll call these four approaches **Plasma Plus**, **Scalar Plus**, **Contact Plus 4**, and **Contact Plus 2**. Plasma Plus requires a Spooky Central/Plasma Essential Kit, Scalar Plus requires Spooky² Scalar, Contact Plus 4 requires a Spooky² Advanced Kit, and Contact Plus 2 requires a Spooky² Essential Kit.

The main difference between them is speed of efficacy. Plasma Plus is fastest, then Contact Plus 4, followed by Contact Plus 2. It's been authoritatively estimated that to produce the same effectiveness as one Contact Mode session, you would need to apply the same frequencies between 10 and 20 times in a row in Remote Mode. It's also been estimated that to produce the same effectiveness as one Plasma Mode session, you would need to do 5-10 Contact Mode sessions. However, until the results of our studies are in, we're going to err on the side of caution for now.

Three tasks

After you've run the first five presets, there are three jobs you must learn to perform for yourself – biofeedback scanning, preset editing, and preset creation. Although they may look tricky, they're actually quite easy, as I'll show you now.


Biofeedback scanning

Where indicated in the treatment timetables for each plan, you will do two biofeedback scans – the first for cancer viruses, and the second for all other problems. Do both in the morning, one after another, preferably in Contact Mode. **All other generators should be stopped.**

Choose one of the following biofeedback presets depending on which Biofeedback hardware you are using:


Biofeedback Hardware	Preset
Spooky Pulse	\Biofeedback\Spooky Pulse\General\General Purpose Full System Scan - JW
GeneratorX	\Biofeedback\GeneratorX\GX General Biofeedback Scan (C) - JW
Scalar Digitizer	\Biofeedback\Scalar Digitizer\Spooky2 Scalar Digitizer Master (GX) - JW <i>and</i> \Biofeedback\Scalar Digitizer\Spooky2 Scalar Digitizer Slave (GX) - JW
Sample Digitizer	\Biofeedback\Sample Digitizer\General Biofeedback Scan (SD) - JW

Note: Because the Sample Digitizer scan results only reflect the bacteria, virus, and parasites found in the sample, and not the whole body, if you are to use the Sample Digitizer scan results, these result ought to be used in conjunction with one of the scan results of one of the other three biofeedback hardware (Spooky Pulse, GeneratorX, or Scalar Digitizer).

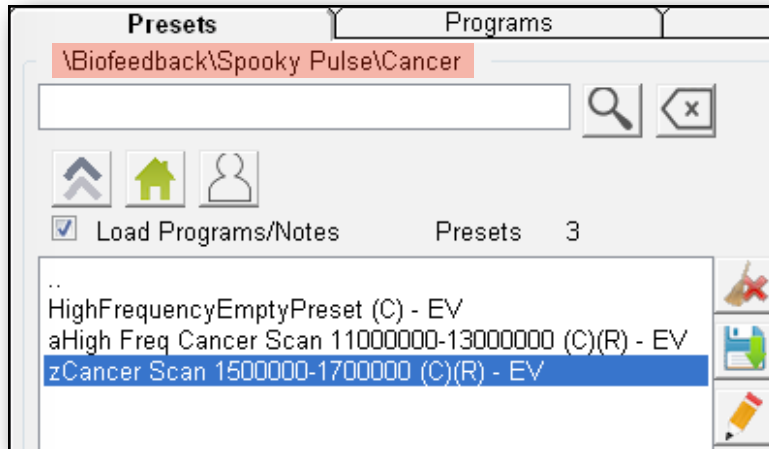

1. Select the >*Biofeedback* preset collection at the top of the *Presets* column on the left. The column's contents change. Then select >*Spooky Pulse*.
2. Select >*Cancer*, and you'll now see the cancer scan preset (above). Select it to load the correct parameter values into the *Settings* and *Control* tabs.
3. Select *zCancer Scan 1500000-1700000*. Now go to *Control*, tick *Overwrite Generator*, then click the scan generator.


For Spooky Pulse, set up biofeedback as follows:

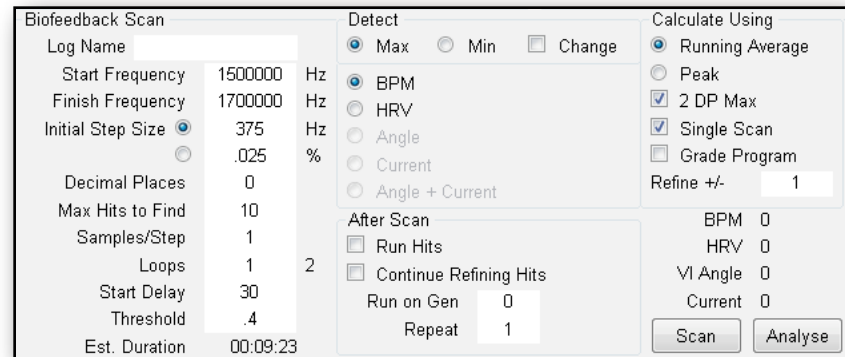


Above are the *Biofeedback Scan* settings loaded into the *Control* tab for the cancer scan. This sweeps the frequency range of the BX, BY, and HPV cancer viruses, and its results can be used to kill these.

It's set to find 10 such frequencies, and to start recording the results 30 heartbeats after you click the *Scan* button. This gives you a chance to prepare, and you may increase this number of heartbeats if you wish. When ready, click the *Scan* button to initiate the process.

Now here's the general scan:

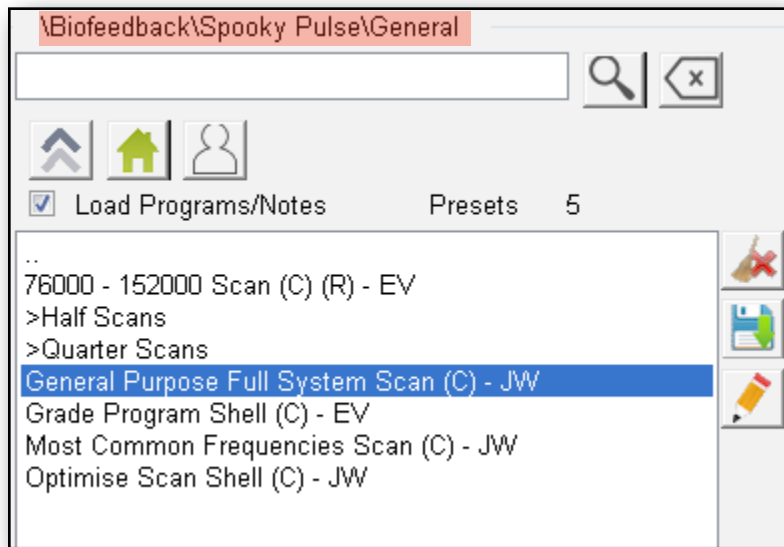


1. Select the >Biofeedback preset collection at the top of the *Presets* column on the left. The column's contents change. Then select >Spooky Pulse.
2. Select >General, and you'll now see the full system scan preset (above). Select it to load the correct parameter values into the *Settings* and *Control* tabs.
3. Select *General Purpose Full System Scan - JW*. Now go to *Control*, tick *Overwrite Generator*, then click the scan generator.

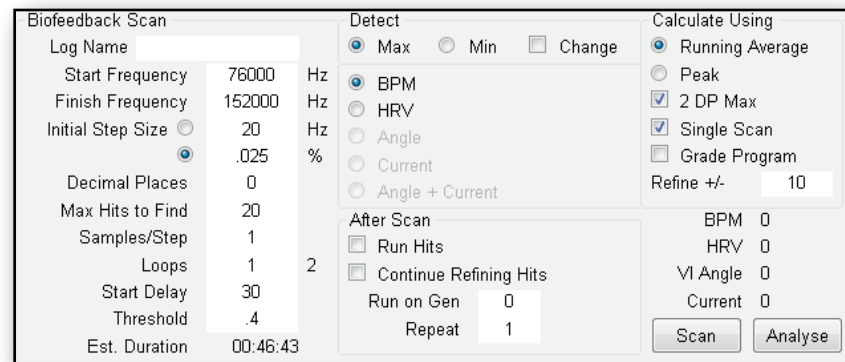

Above are the *Biofeedback Scan* settings loaded into the *Control* tab for the full system scan. This sweeps the entire frequency range of the vast majority of pathogenic organisms, and its results can be used to kill these.

This scan is set to find 20 such frequencies, and to start recording the results 30 heartbeats after you click the *Scan* button. This gives you a chance to prepare, and you may increase this number of heartbeats if you wish.

Now click the *Scan* button to start scanning.

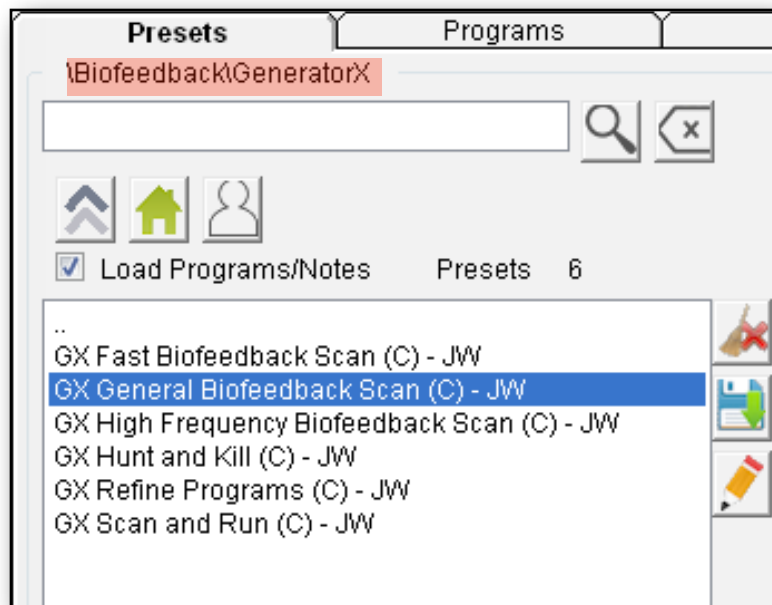

For GeneratorX biofeedback scanning, do the following:

1. Select the >*Biofeedback* preset collection at the top of the *Presets* column on the left. The column's contents change. Then select >*GeneratorX*.
2. Select *GX General Biofeedback Scan (C) - JW*. Now go to *Control*, tick *Overwrite Generator*, then click the scan generator.
3. Now click the *Scan* button to start scanning.


Note: For GeneratorX biofeedback scans, you use the same biofeedback preset for both the system and cancer scan. For the system scan, place the TENS pads on the sides of your torso at belly level. For the cancer scan, place the TENS pads

around your tumor.


When your scan finishes, you will be presented with a window listing the top 10/20 problem frequencies found by each scan. Click the *Save* button to save these to your personal custom database. The window will disappear and the *Create Program* screen appears in its place, with your found frequencies already entered.

Name your scan results program. I strongly recommend naming it “BFB Cancer” or “BFB System” as appropriate, followed by Your Initials, then the date in reverse format – year, month, date. As in, “*BFB Cancer YI 20190103*.” For clarity, you can enter the long form of the date in the *Program Description* box, and any other notes you wish. When you click the *Save* button, your new program will be written to your custom database and loaded into Spooky².


The biofeedback setting for Scalar Digitizer (master):

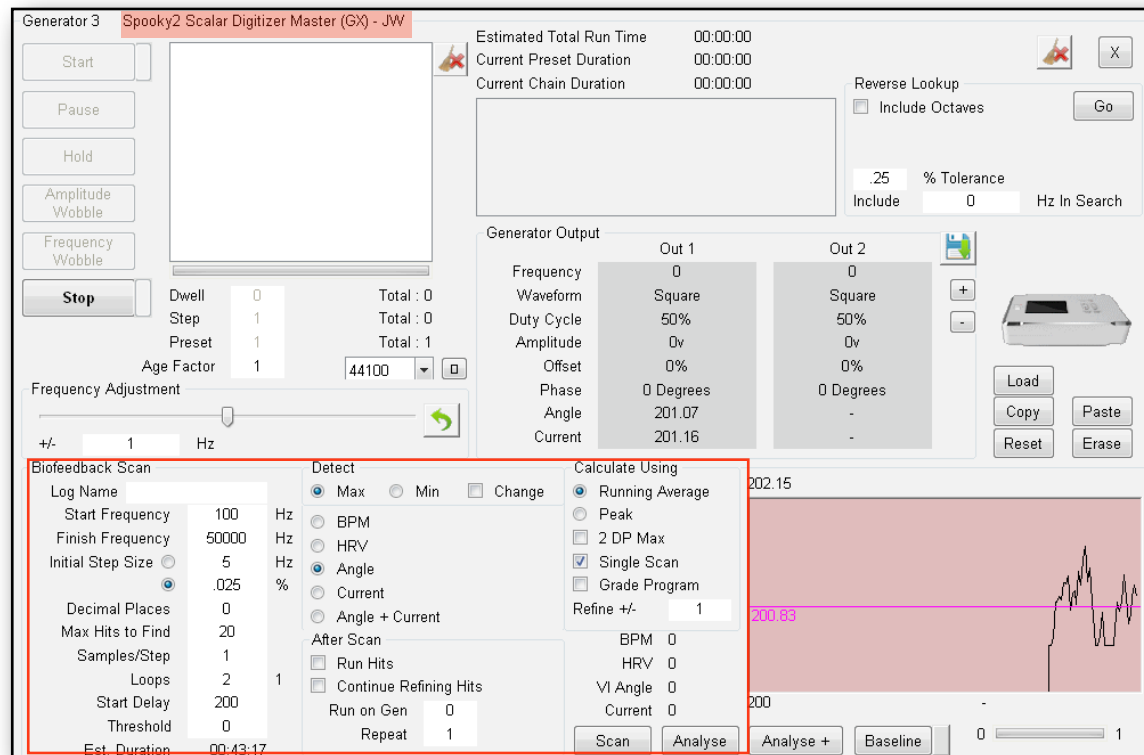


Before you load up the slave generator for Scalar Digitizer, you must set the master generator number:

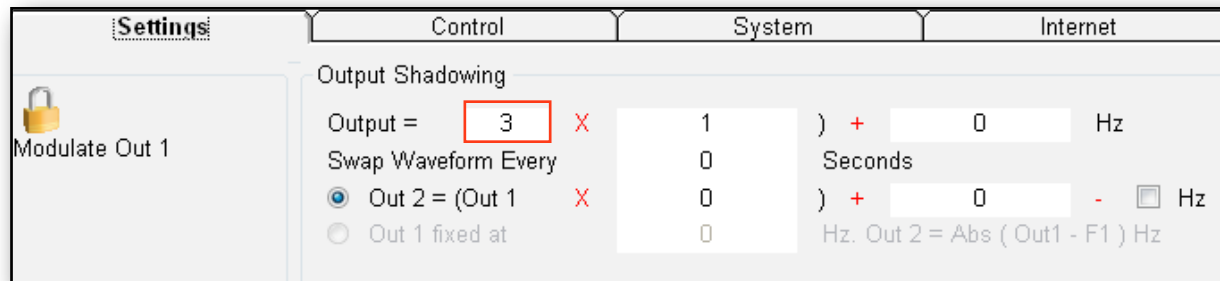

The biofeedback setting for Scalar Digitizer (slave):

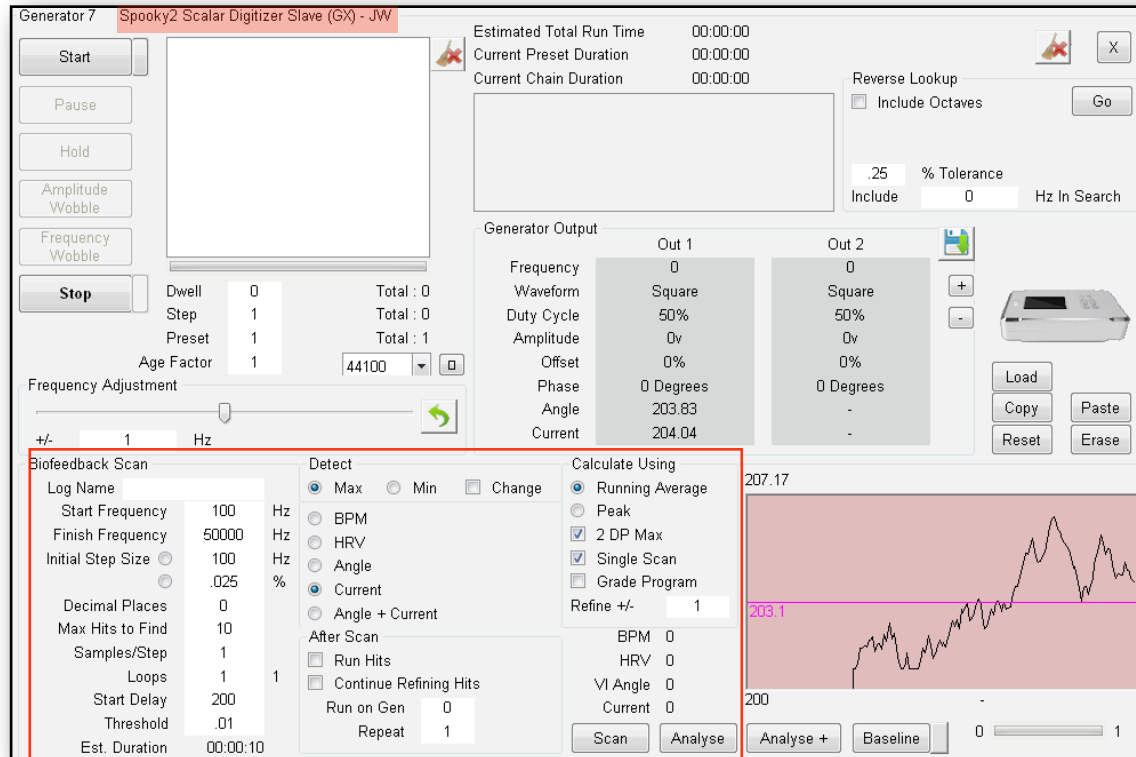


The biofeedback setting for Sample Digitizer:

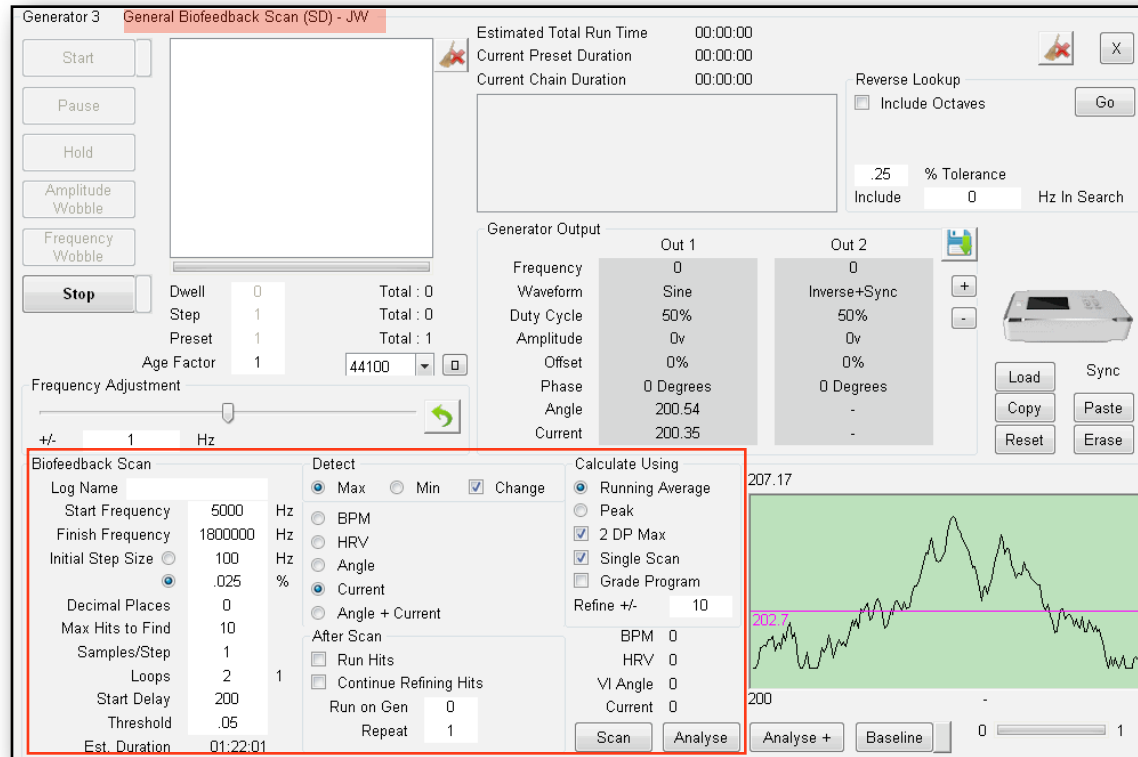

Note: Because the Sample Digitizer scan results only reflect the bacteria, virus, and parasites found in the sample, and not the whole body, if you are to use the Sample Digitizer scan results, these result ought to be used in conjunction with one of the scan results of one of the other three biofeedback hardware (Spooky Pulse, GeneratorX, or Scalar Digitizer).


Editing Presets

After you've finished and saved your two scans, you now need to substitute them for the placeholder dummy programs in the sixth preset – Cancer A. You will also choose your cancer type program and insert it, too. Let's assume we're dealing with pancreatic cancer, and we're following a Contact Plus timetable (this same process is

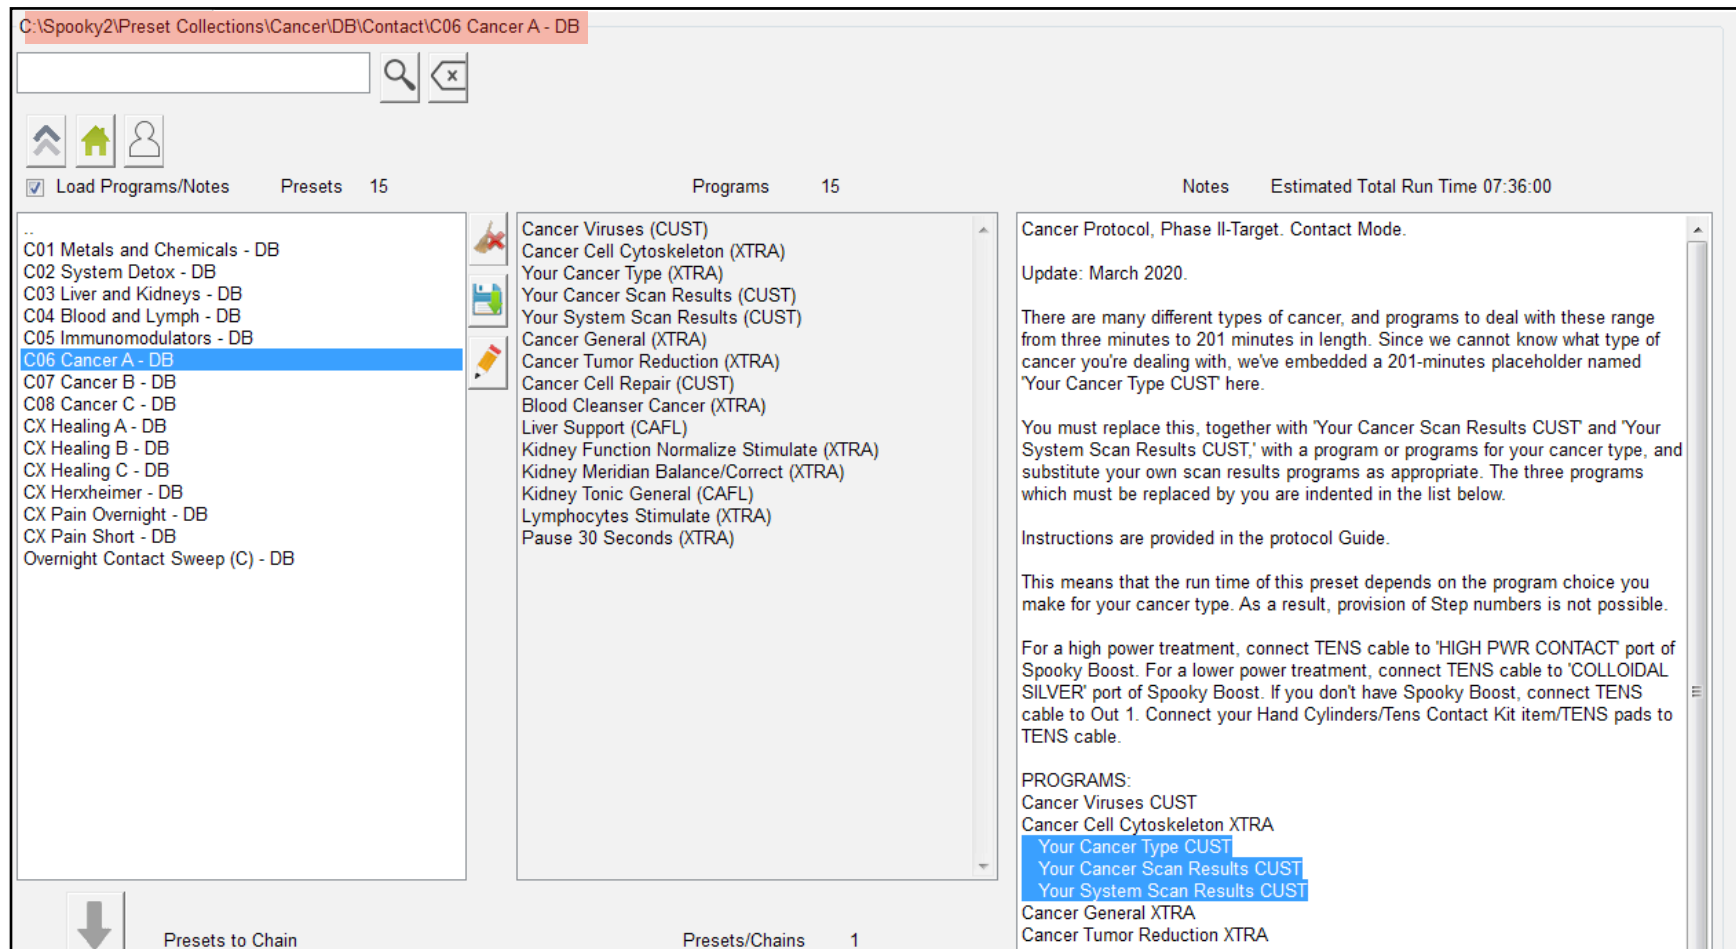

used for Scalar, Remote, and Coil Mode presets. See the next section for [Plasma presets](#)). Start by selecting the *>Cancer* collection in the *Presets* tab, then *>DB*, then *>Contact*, then *C06 Cancer A - DB*:

The text highlighted red top left shows the file path I followed to get here – I first selected the *Cancer* collection, then *DB*, then the *Contact* sub-collection. Finally, I chose *C06 Cancer A – DB*. The central *Programs Column* shows the 23 (red) programs this preset contains, and in the rightmost *Notes* column, I’ve highlighted in blue the programs we’re going to replace.

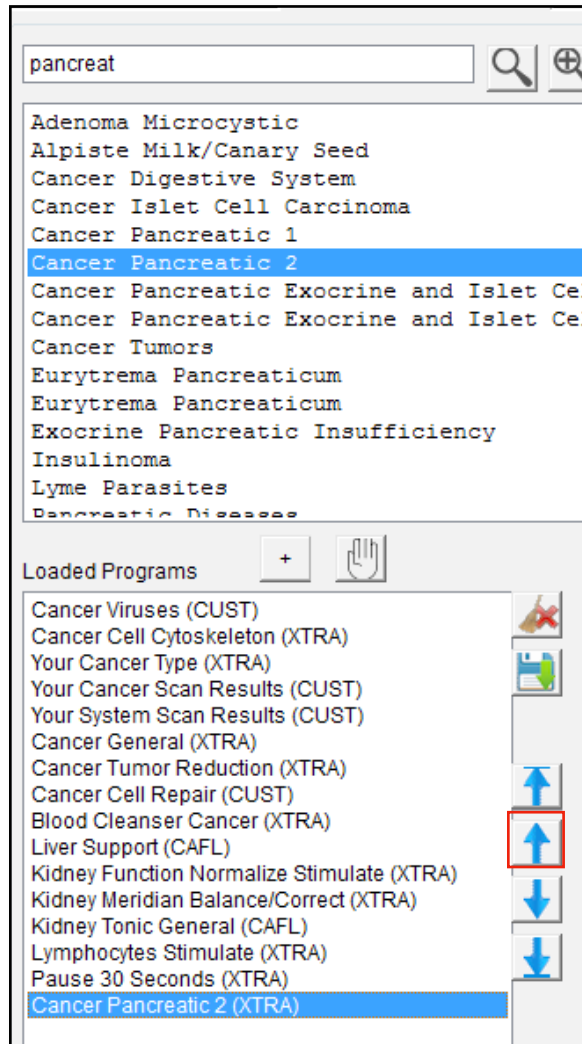


To find a program for pancreatic cancer, I go to the *Programs* tab and enter “pancrea” into the *Search* field. The reason I do this is because if I entered “pancreatic” instead, it wouldn’t find any programs named “Pancreas” – and I’d like to see all the options available.

For this reason, it’s often better to enter a partial name for a search.

I choose *Cancer Pancreatic 2 XTRA*. This is going to replace the program I’ve highlighted in the *Loaded Programs* column – *Your Cancer Type XTRA*.


So I double click it to load it into the column.

And here it is at the bottom of the list.

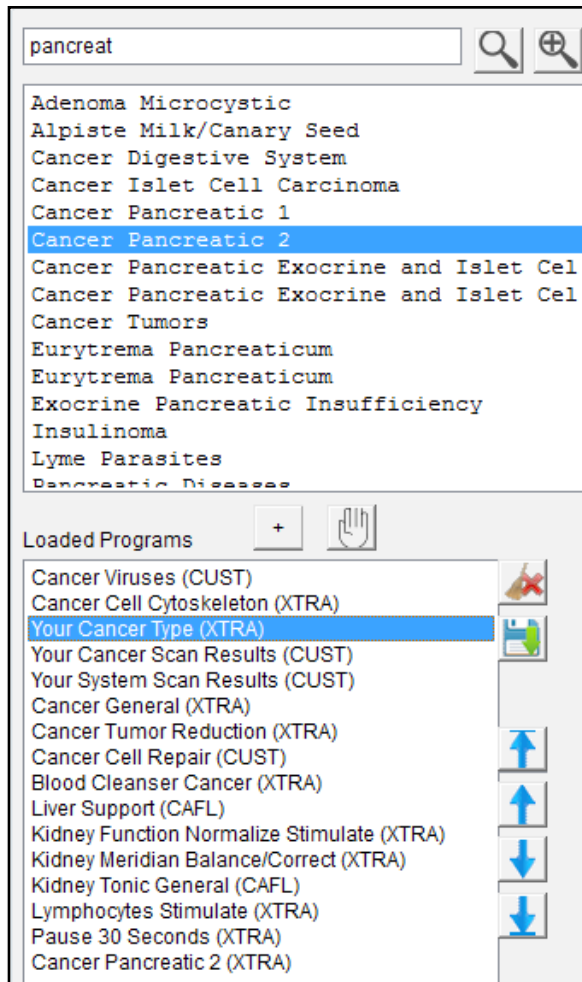


Now I have to move it into the correct position.

To do this, I select it, then click the *Move Up Arrow* (outlined red) repeatedly until my program sits above the one it's going to replace.

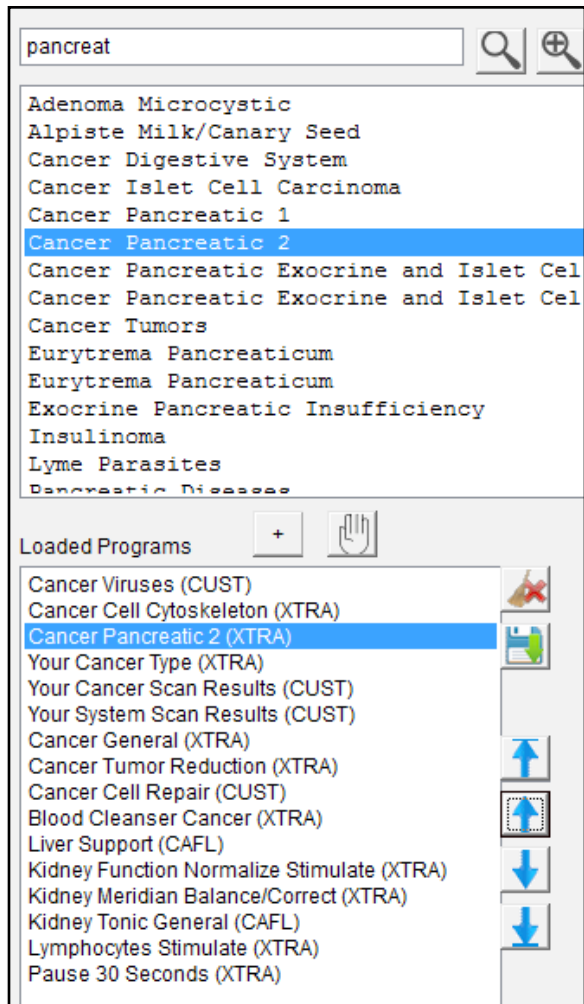


Now I have it where I want it.

I no longer need the placeholder dummy program, so I double click it to delete it from *Loaded Programs*.

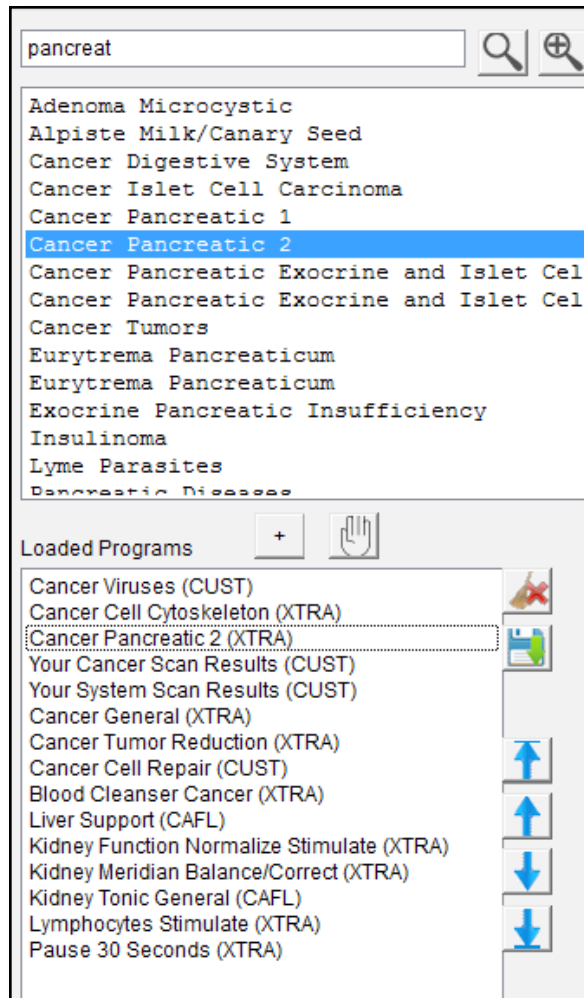

The placeholder program is now gone, and my replacement for it occupies its slot.

Next, I have to replace the two placeholder scan dummy programs with my own. So I enter “bfb” into the *Search* field:

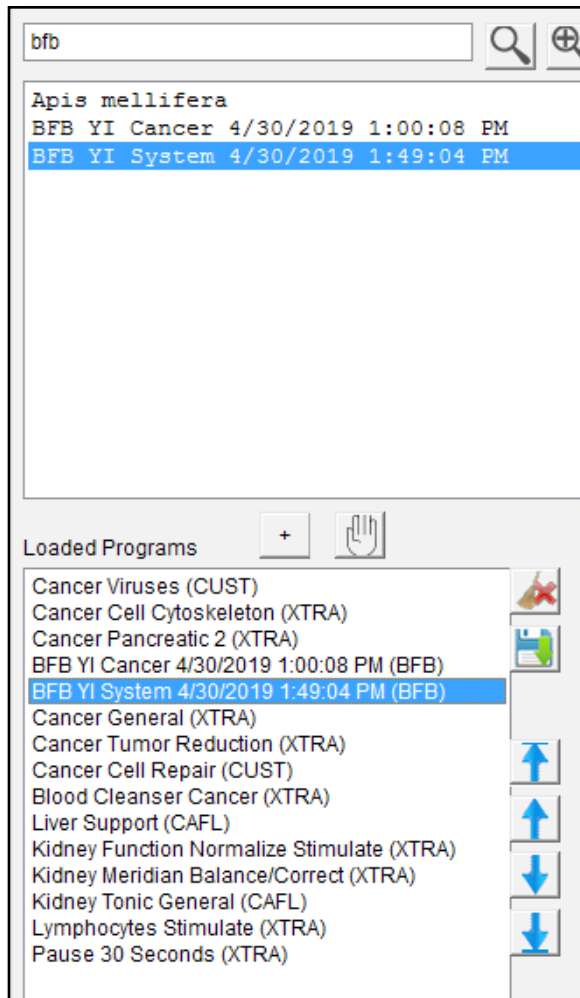

As you can see, this finds all my cancer and system scans, grouped together in date order.

I double click *BFB YI Cancer 4/30/2019 1:00:08 PM* to load it, then do the same for *BFB YI System 4/30/2019 1:49:04 PM*. For GeneratorX users, you will use the same BFB preset to create the System and Cancer scan, but you will place the TENS pads on the sides of the torso for the System scan, and around your tumor for the Cancer scan.

Once again, I select *BFB YI Cancer 4/30/2019 1:00:08 PM*, then click the *Move Up Arrow* repeatedly until it's above the placeholder dummy *Your Cancer Scan Results CUST*, then double click the dummy to delete it.

I do the same for *BFB YI System 4/30/2019 1:49:04 PM*, then delete its placeholder program *Your System Scan Results CUST*.

On the left, you see what I end up with:


My own three programs are now in their correct spots, and the three placeholder programs are gone.

Notice that the original preset we started with had an *Estimated Total Run Time* of 07:40:40, and this has now reduced to 05:54:40. This is because the placeholder program *Your Cancer Type XTRA* must be equal in


duration to the longest targeted cancer program in the database, which is 201 minutes.

We replaced it with *Cancer Pancreatic 2 XTRA*, which runs for 95 minutes, shaving 106 minutes off the *Estimated Total Run Time*.

Now we must save our edited preset:

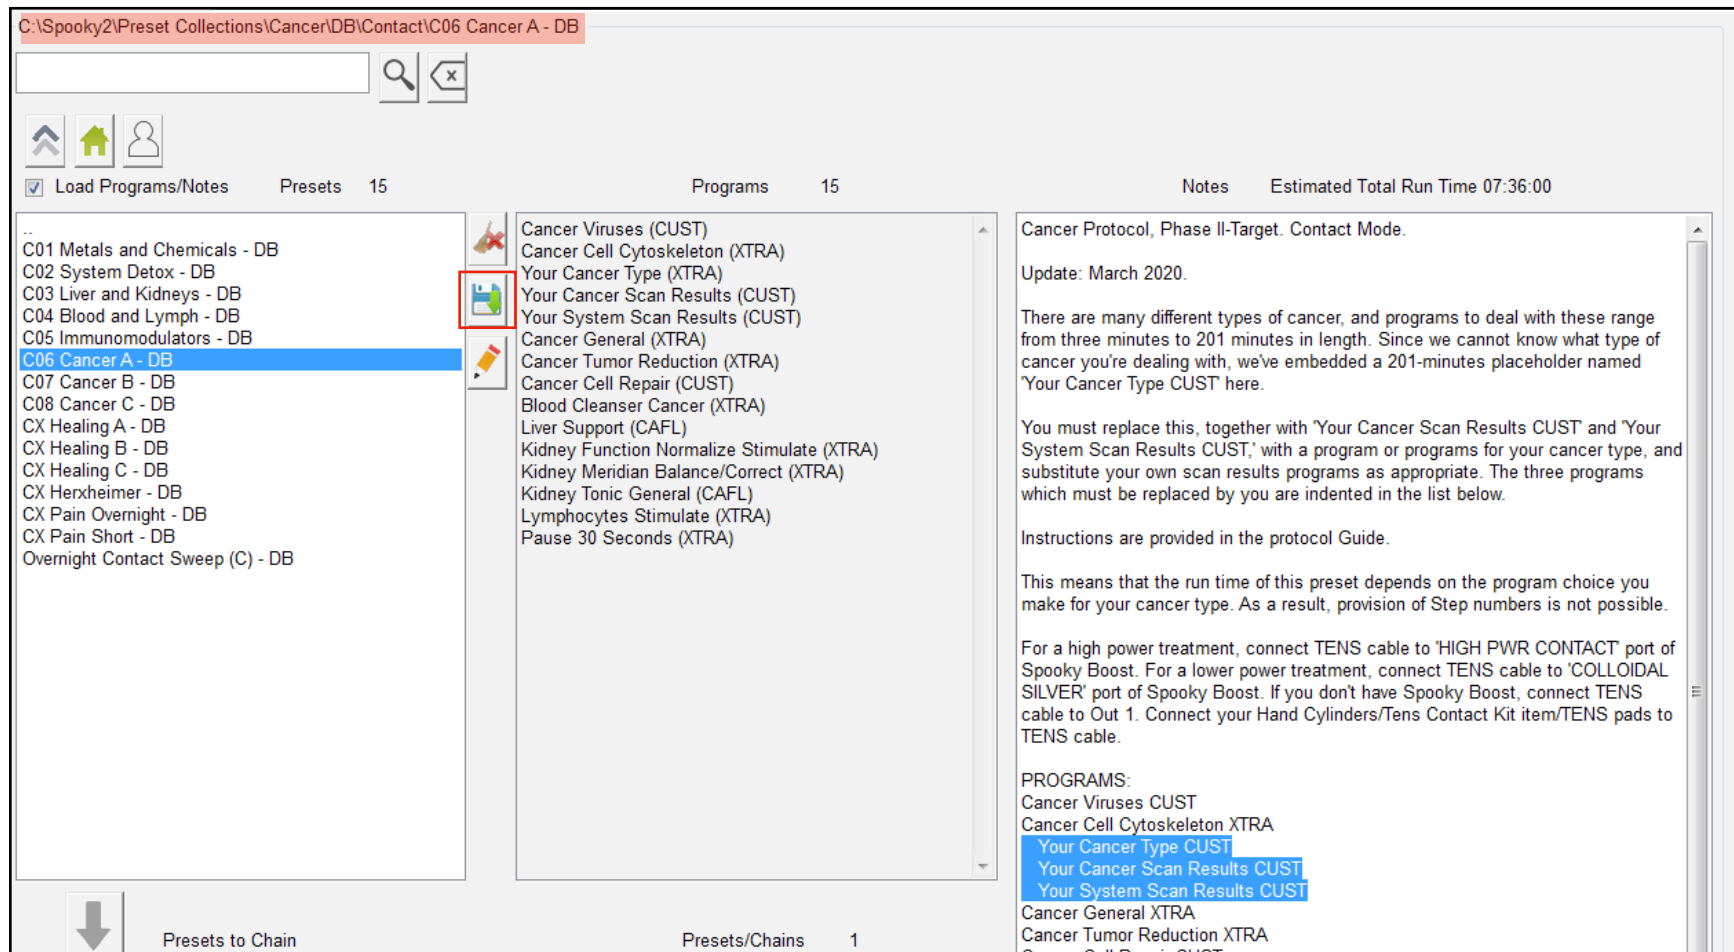


1. Click the *Presets* tab. I'm back where I started – the *Contact* sub-collection inside the *DB* sub-collection in the *Cancer* collection. You can see the file path highlighted in red top left above.
2. I select the names of the placeholder dummy programs in the *Notes* at the right and, to prevent any possible confusion later, I type the names of my own programs (highlighted blue).
3. I click the *Save* button – outlined in red above – and the following file dialog window appears:

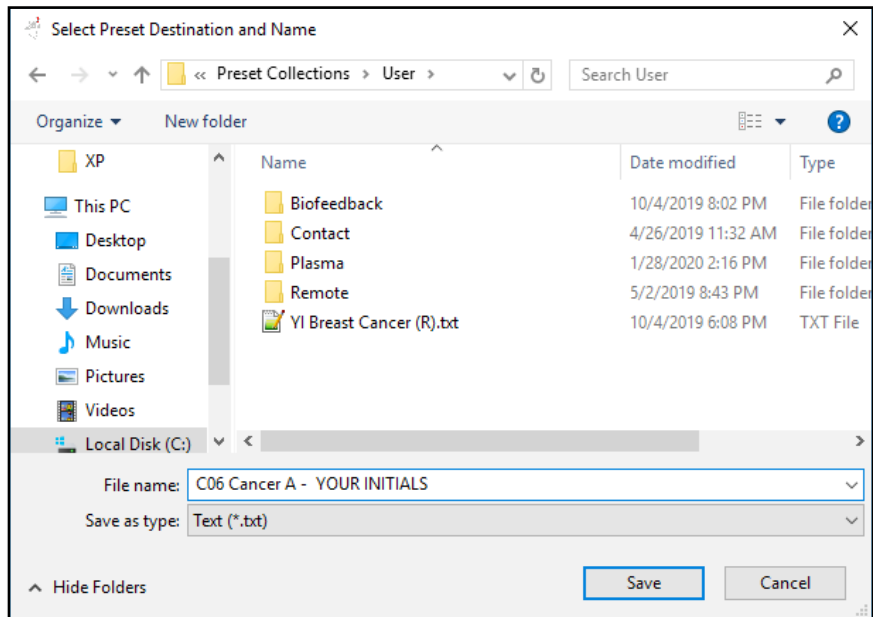

You should be brought to your *User* preset collection. If not, navigate through the file system to find it using the up arrow outlined in red (left), or by clicking locations in the red file path field.

Here, I've already created three new folders to store presets for each mode. This is a Contact Mode preset I'm saving, so I want it to go inside the *Contact* collection.

I double click the *Contact* folder, and this is what I see:

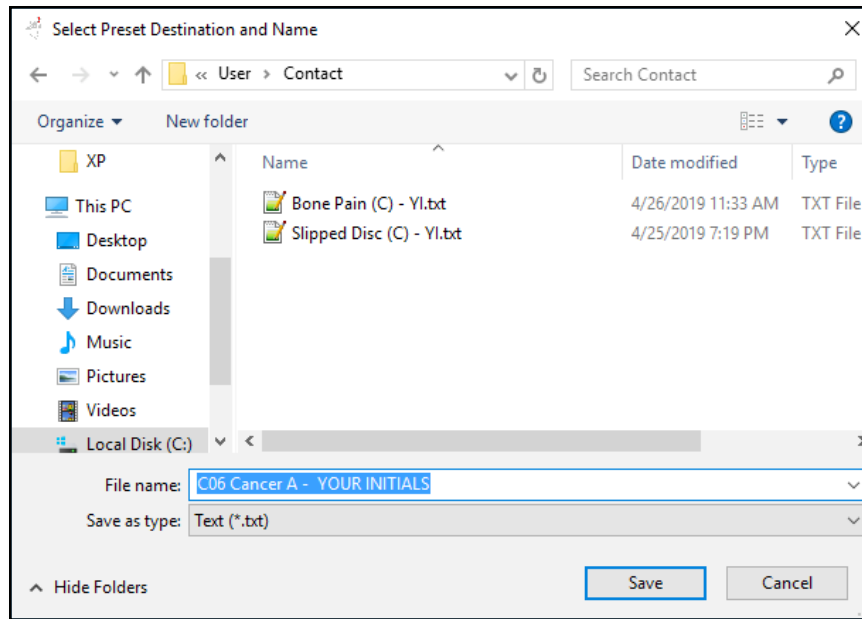


Nothing. The folder is empty because this is the first Contact Mode preset I'm saving.

It's best to save it using its original name, so you should type "C06 Cancer A," then add your own initials.

Now click the *Save* button, or press the Return key on your keyboard.

My edited preset is now saved to my *Contact* preset collection inside my *User* preset collection:

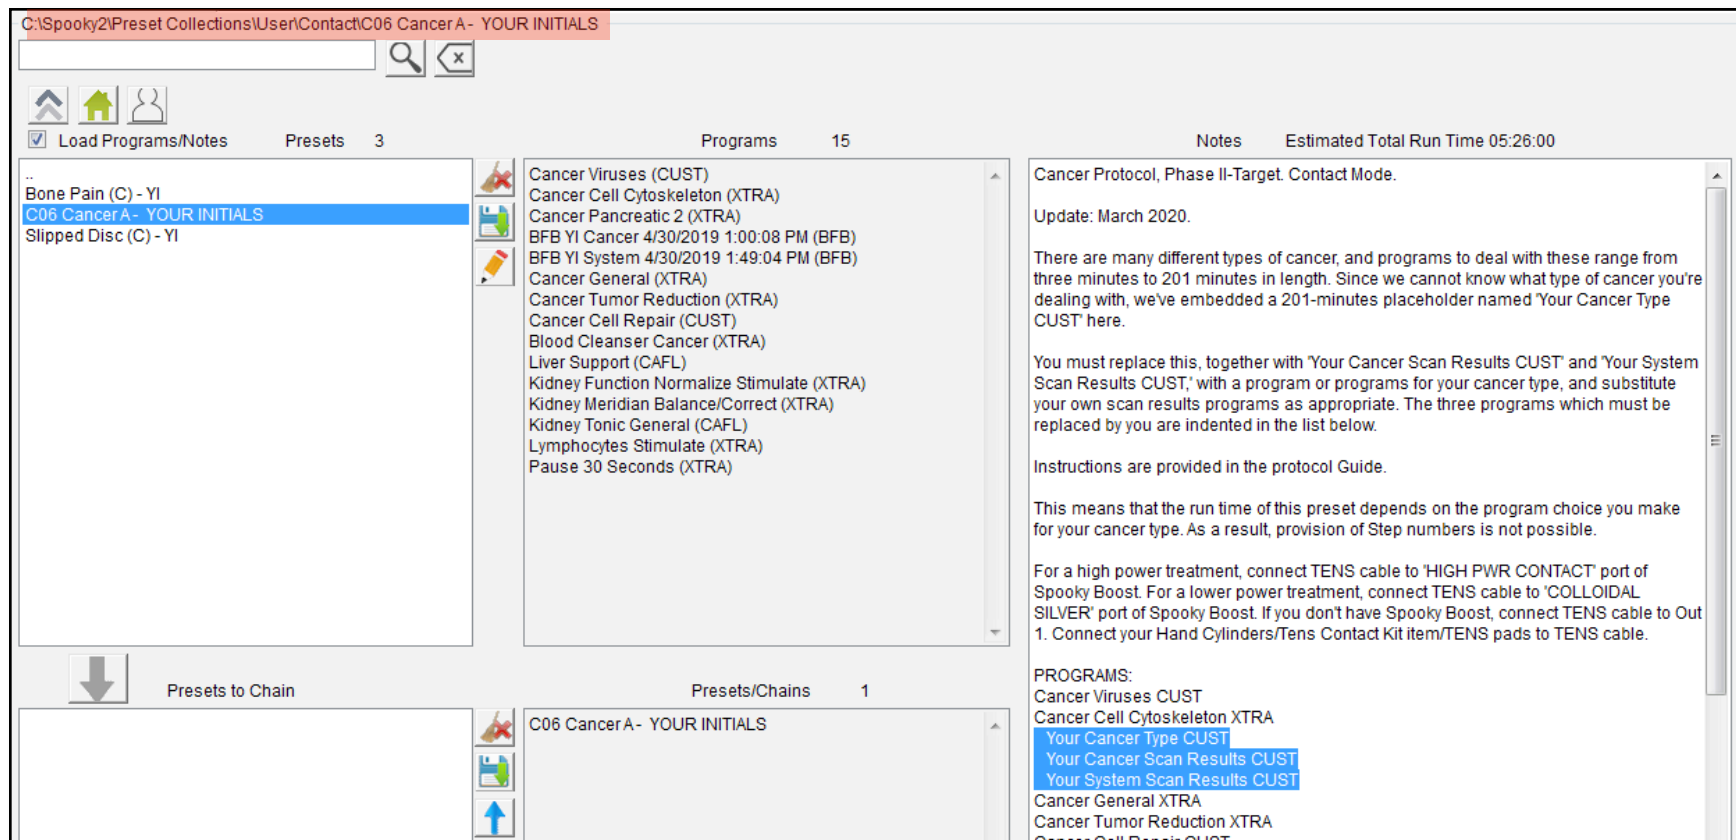


And here it is, right where I saved it – you can see the file path highlighted in red top left above.

This process is identical for plasma and remote presets. You will perform this operation for all the modes you use after every scan session, and edit your new programs into the Cancer A, Cancer B, and Cancer C presets in turn before you run them.


Finally, I'm going to show you [here](#) how easy it is to build your own preset. As you become familiar with Spooky², you will doubtless come across a few programs you'd like to try out. This simple process will allow you to do just that.

Editing Plasma Presets

The procedure for editing Plasma presets is the same as other preset, but the screen will look different because Plasma uses chained presets. After you've finished and saved your two scans, you now need to substitute them for the placeholder dummy programs in the sixth preset – Cancer A. You will also choose your cancer type program and insert it, too. Let's assume we're dealing with pancreatic cancer, and we're following a Plasma Plus timetable. Start by selecting the >*Cancer* collection in the *Presets* tab, then >*DB*, then >*Plasma*, then *P06 Cancer A - DB*:

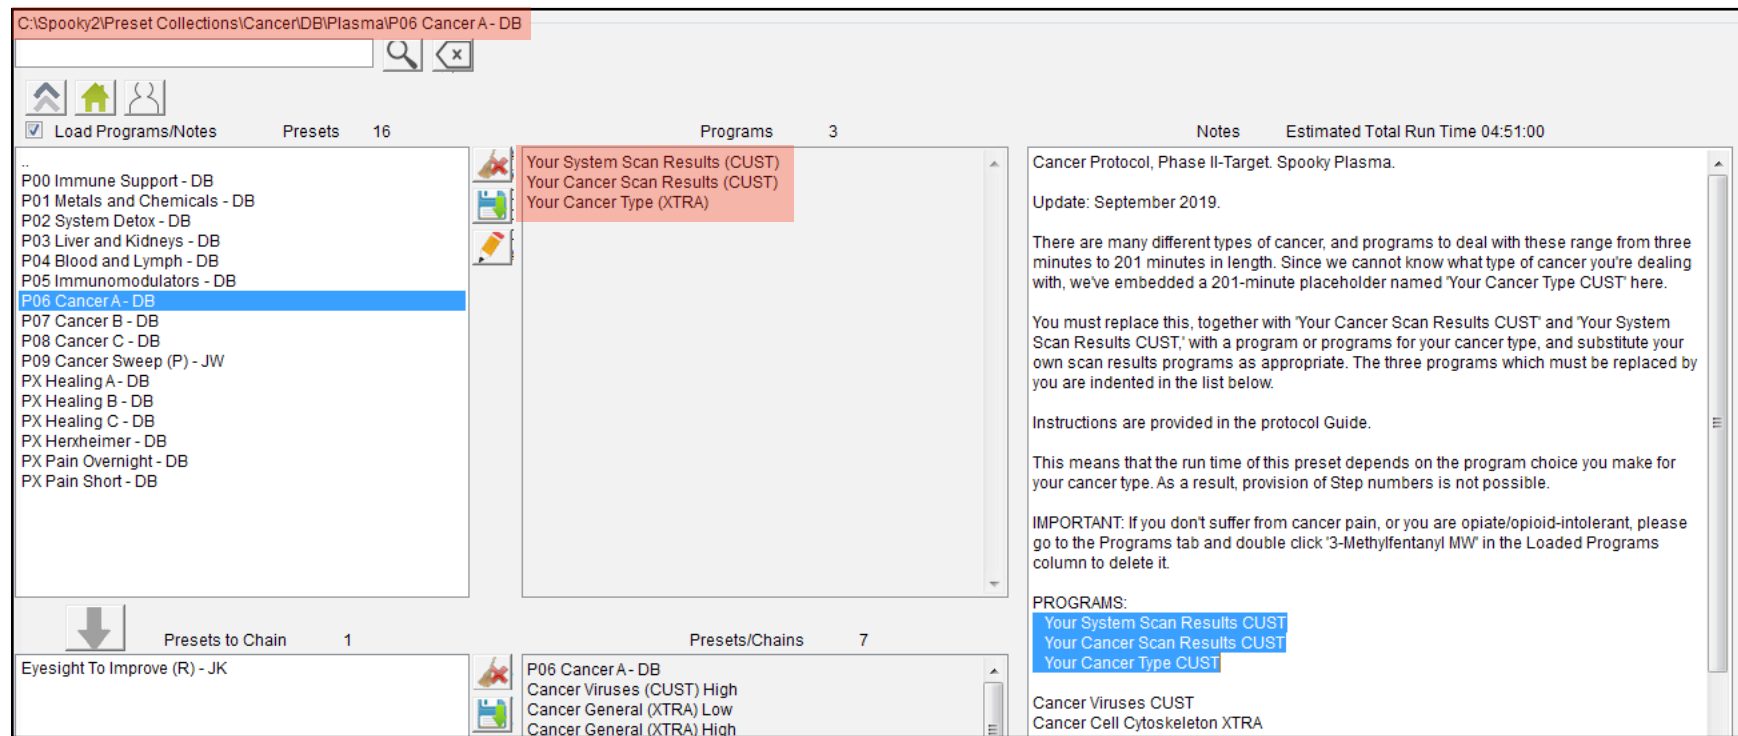

The text highlighted red top left shows the file path I followed to get here – I first selected the *Cancer* collection, then *DB*, then the *Contact* sub-collection. Finally, I chose *P06 Cancer A – DB*. The central *Programs Column* shows the 3 (red) programs this preset contains, and in the rightmost *Notes* column, I've highlighted in blue the programs we're going to replace.

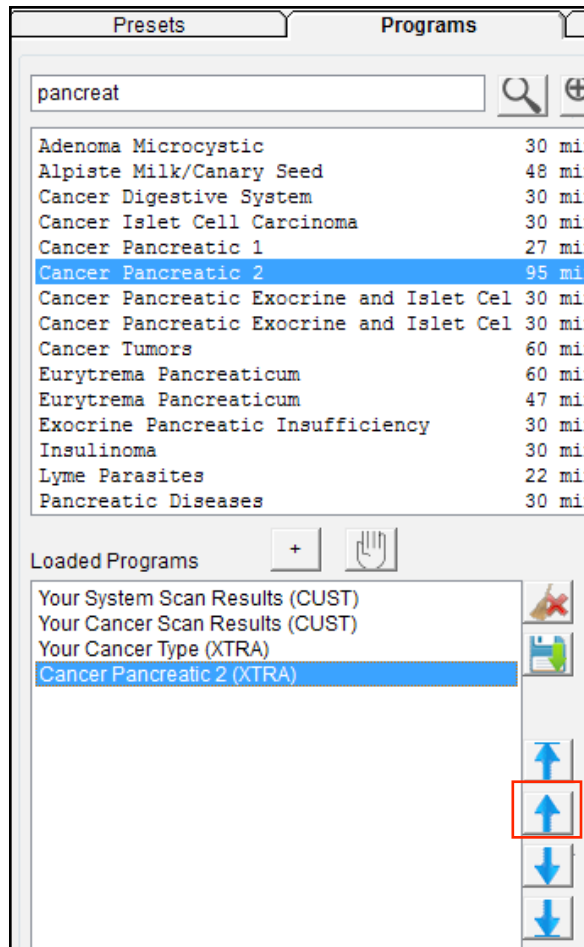


To find a program for pancreatic cancer, I go to the *Programs* tab and enter “pancrea” into the *Search* field. The reason I do this is because if I entered “pancreatic” instead, it wouldn’t find any programs named “Pancreas” – and I’d like to see all the options available.

For this reason, it’s often better to enter a partial name for a search.

I choose *Cancer Pancreatic 2 XTRA*. This is going to replace the program I’ve highlighted in the *Loaded Programs* column – *Your Cancer Type XTRA*.


So I double click it to load it into the column.

And here it is at the bottom of the list.

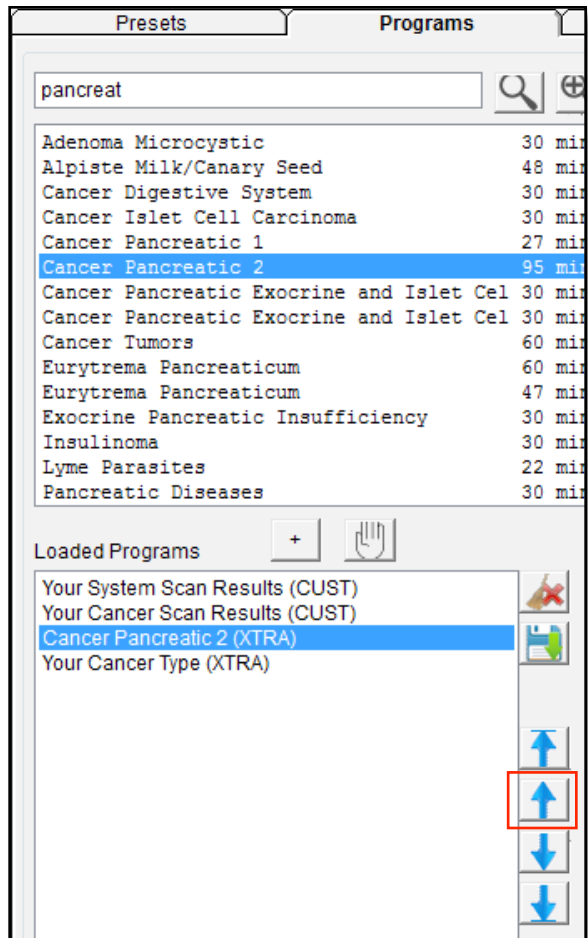


Now I have to move it into the correct position.

To do this, I select it, then click the *Move Up Arrow* (outlined red) repeatedly until my program sits above the one it's going to replace.

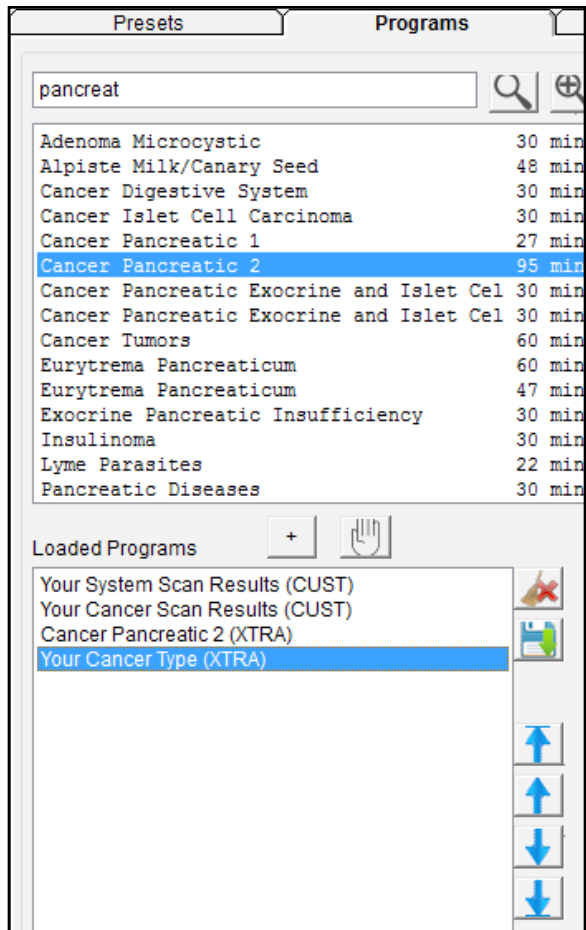


Now I have it where I want it.

I no longer need the placeholder dummy program, so I double click it to delete it from *Loaded Programs*.

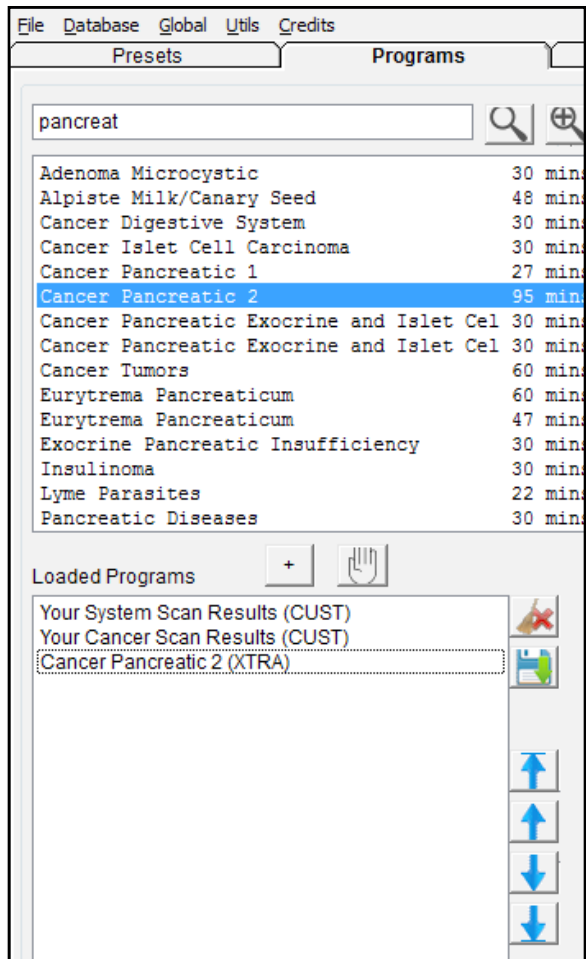

The placeholder program is now gone, and my replacement for it occupies its slot.

Next, I have to replace the two placeholder scan dummy programs with my own. So I enter “bfb” into the *Search* field:

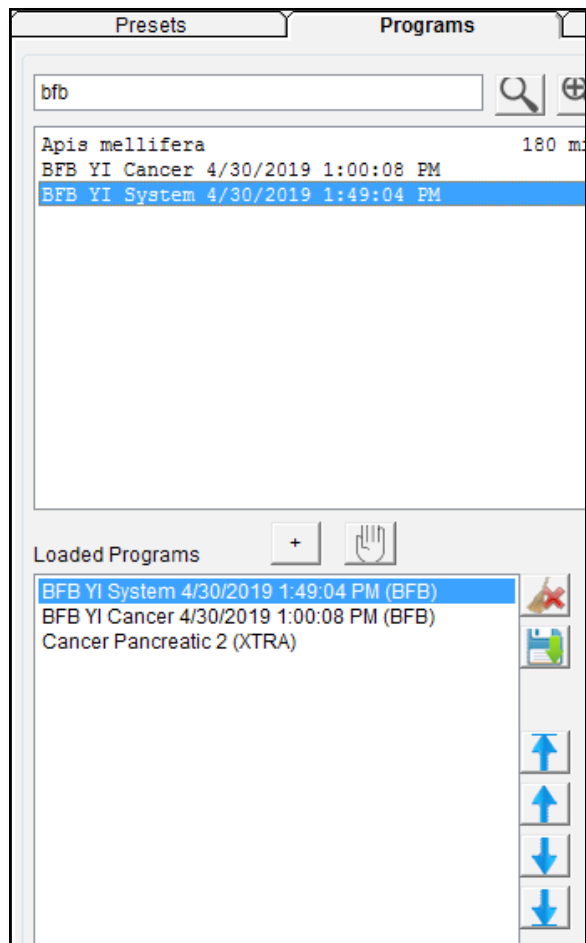

As you can see, this finds all my cancer and system scans, grouped together in date order.

I double click *BFB YI Cancer 4/30/2019* to load it, then do the same for *BFB YI System 4/30/2019*.


Once again, I select *BFB YI Cancer 4/30/2019* below, then click the *Move Up Arrow* repeatedly until it's above the placeholder dummy *Your Cancer Scan Results CUST*, then double click the dummy to delete it.

I do the same for *BFB YI System 4/30/2019*, then delete its placeholder program *Your System Scan Results CUST*.


On the left, you see what I end up with:

My own three programs are now in their correct spots, and the three placeholder programs are gone.

Now we must save our edited preset:

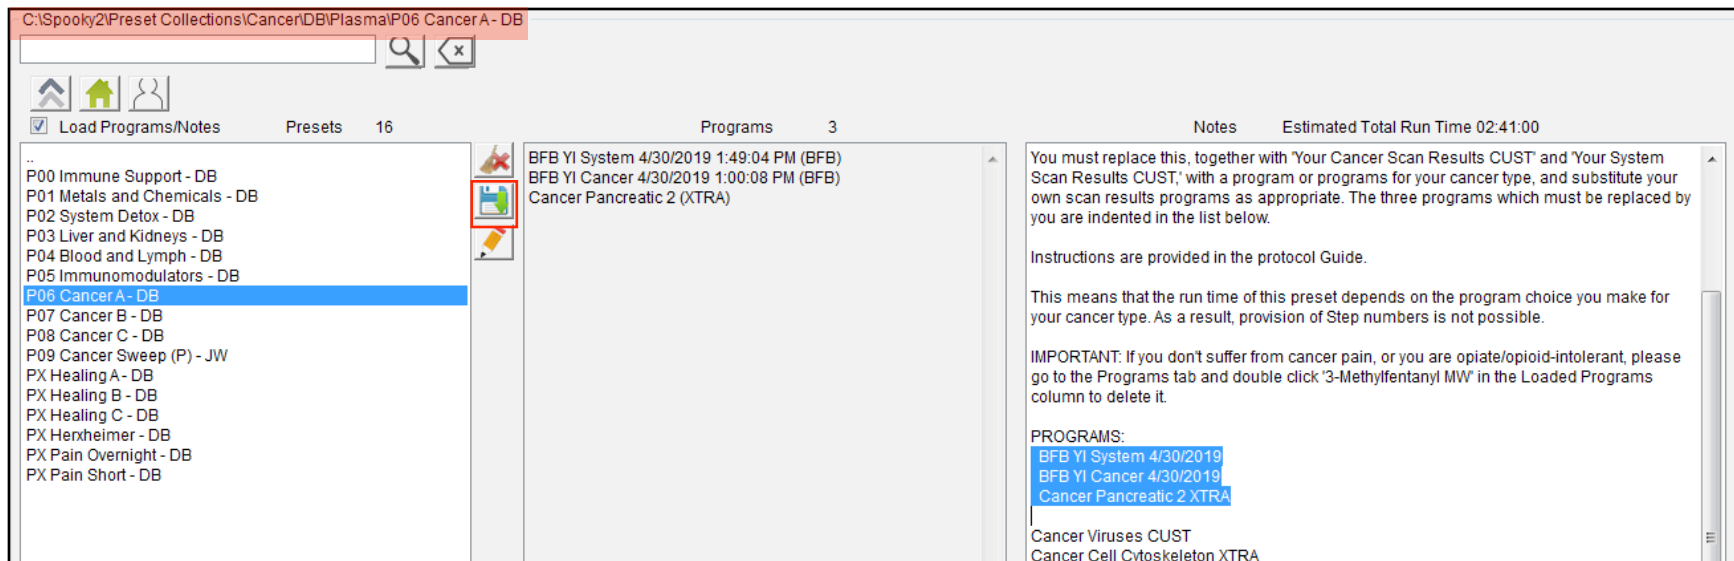


1. Click the *Presets* tab. I'm back where I started – the *Contact* sub-collection inside the *DB* sub-collection in the *Cancer* collection. You can see the file path highlighted in red top left above.
2. I select the names of the placeholder dummy programs in the *Notes* at the right and, to prevent any possible confusion later, I type the names of my own programs (highlighted blue).
3. I click the *Save* button – outlined in red above – and the following file dialog window appears:

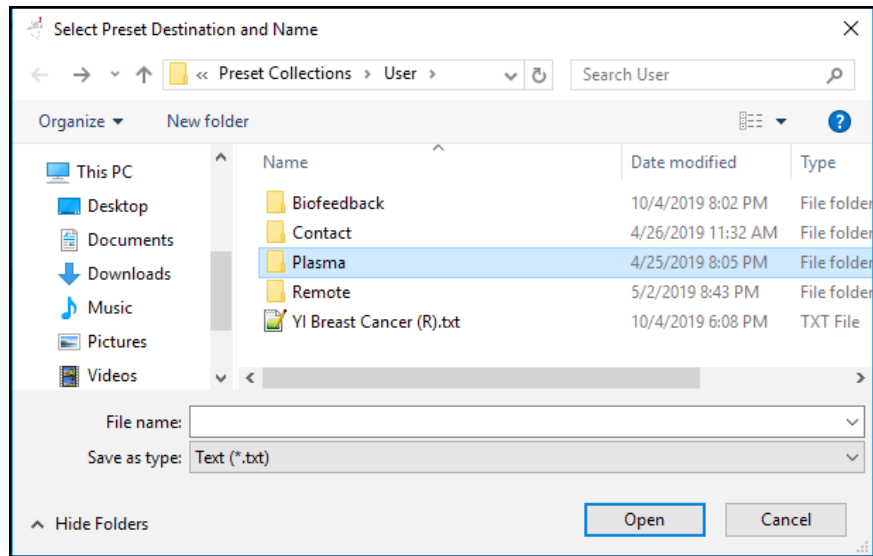

You should be brought to your *User* preset collection. If not, navigate through the file system to find it using the up arrow outlined in red (left), or by clicking locations in the red file path field.

Here, I've already created three new folders to store presets for each mode. This is a Contact Mode preset I'm saving, so I want it to go inside the *Contact* collection.

I double click the *Plasma* folder, and this is what I see:

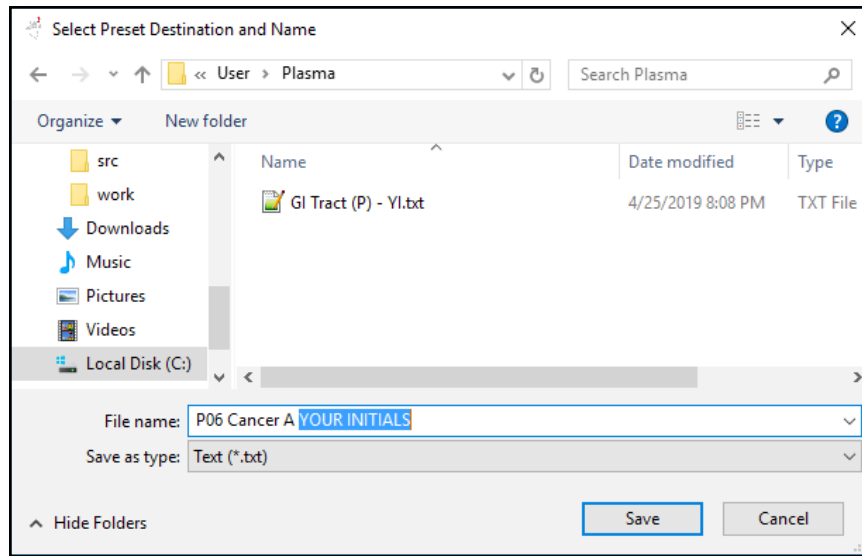


It's best to save it using its original name, so you should type "P06 Cancer A," then add your own initials.

Now click the *Save* button, or press the Return key on your keyboard.

My edited preset is now saved to my *Contact* preset collection inside my *User* preset collection:

And here it is, right where I saved it – you can see the file path highlighted in red top left above.

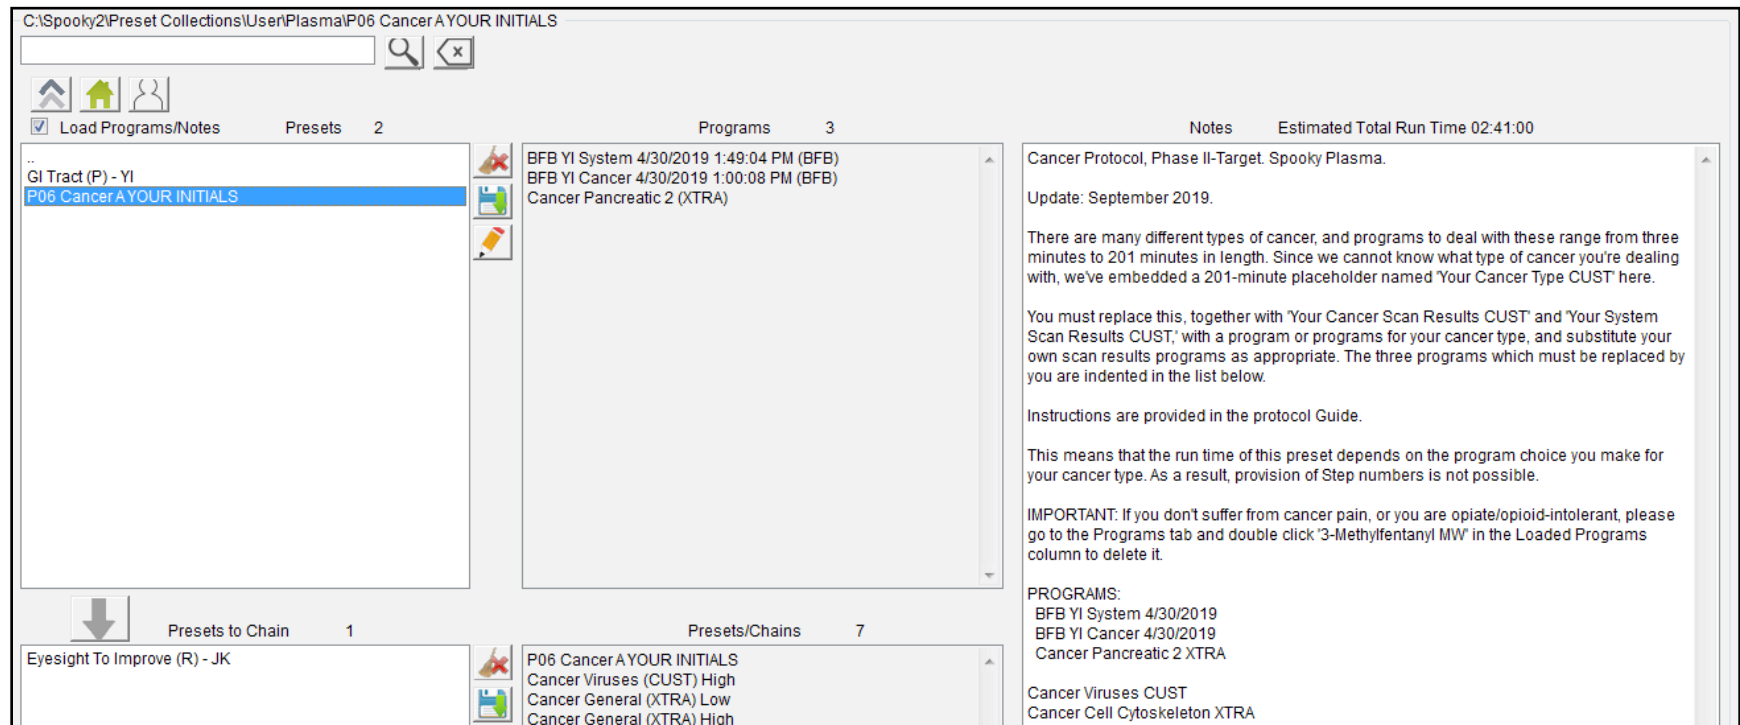

You will perform this operation for all the modes you use after every scan session, and edit your new programs into the Cancer A, Cancer B, and Cancer C presets in turn before you run them.

Finally, I'm going to show you how easy it is to build your own preset. As you become familiar with Spooky², you will doubtless come across a few programs you'd like to try out. This simple process will allow you to do just that.

Building Presets

Building any preset starts with two decisions:

1. Is it for Plasma, Contact, Remote, or Coil?
2. Is it for killing or healing?

Plasma: for killing OR for healing, you start in the *Presets* tab by selecting each step in the following path:

Shell (Empty) Presets > Plasma > Spooky Plasma Entrainment and Healing (P) – JW

Contact: here are the navigation paths to build Contact Mode presets for killing or healing:

Shell (Empty) Presets > Contact > Killing – JW

Shell (Empty) Presets > Contact > Healing – JW

Remote: here are the paths to follow for killing or healing remote presets:

Shell (Empty) Presets > Remote > Killing – JW

Shell (Empty) Presets > Remote > Healing – JW

Coil: for killing OR for healing, start in the *Presets* tab and select each step in the following path:

Shell (Empty) Presets > Spooky Coil (XM direct) – JW

Scalar: for killing OR for healing, start in the *Presets* tab and select each step in the following path:

Shell (Empty) Presets > Scalar > Spooky Scalar General (SS) – JW

In all cases, you are loading a collection of settings optimised for the task at hand and for the transmission mode you're using. Unlike most other presets in Spooky², shell presets contain no programs or frequencies. This allows you to add your own choice from the database, and be sure that your preset will work effectively. So go to the *Programs* tab, search for the condition you wish to deal with, then double click to load each program you want. Always keep an eye on the *Estimated Total Run Time* beneath the *Loaded Programs* column so you know how long your preset will run for, and when you're building remote presets, always keep your presets to a maximum of four to four and a half hours at most.

The right time?

Cancer never sleeps – but you do. For that reason, this Protocol has been designed so that it may be used while you sleep, or during the day, broken up into as many sessions as you like. Depending on your cancer type, and the length of the programs you choose to deal with it, the presets will vary in duration from four to 7.5 hours. The third preset, which addresses liver and kidney functions, runs for eight hours and 42 minutes, but you will likely only use this on two successive days or nights. If you suffer from known liver and kidney problems, double the number of days you run it for.

Note that Remote presets have a different structure, and are built in blocks of about four hours which repeat.

For Plasma Plus and for Contact Plus, there are different important considerations for both night and day use.

A. Plasma Plus night:

1. Placement: when you run plasma for long periods, the tube can get very hot. To prevent this, don't put it under the covers but on top of them. Doing this means the tube stays relatively cool – but can fall off the bed. So I've pushed my bed up against the wall. I place the tube close to the wall, and fall asleep with my back against it. The best and most secure way I've found so far to use the Ultrasonic transmitter is to place it between my thighs with its diaphragm directly against my perineum. If you move around the bed a lot while you sleep, you may have to find another way – in the armpit may be more viable. Spooky Central/Plasma's fan is very like white noise, but if it bothers you, use wax earplugs. And a sleeping mask if you find the light troublesome.

I put one TENS pad for SC Contact Mode on my left foot just below the outside ankle, and the other on the back of my right hand to ensure total body coverage. It may be a good idea to wear a bed-sock and a glove to keep the pads secure. Don't use a leather or latex glove.

2. Bathroom needs: when you wake, you must remember that you are connected by wires to Spooky Central/Plasma, hand and foot. And you must never disconnect the TENS pad cable while the machine is switched on. So the first thing to do is to switch off Spooky Central/Plasma. Then you can peel off the TENS pads, go to the the PC and click *Pause*. On your return, click *Pause* again and select the frequency above the one currently selected. Then reapply the TENS pads and turn Spooky Central/Plasma on again.

Personally, I found all this too disruptive. So...I bought myself a chamber pot. A bucket or a commode would be fine, too. There's nothing odd about this – urine's been used many times in battleground emergency surgeries as a substitute for blood plasma, and for cleaning wounds. You did it as a child, and if you were in a hospital, and sick

Run	SC Near-field/Far-field (day or night as desired)	Remarks	Generator 1 (if not running SC far-field)	Generator 2
Scan		Biofeedback scans x 2		Edit P06 & R06 presets
x4	P06 Cancer A – DB	+ SC Contact and Ultrasonic for near-field only	> R06 Cancer A – DB	ALL Detox (R) – DB (Run non-stop till protocol is done)
Scan		Biofeedback scans x 2		Edit P07 & R07 presets
x4	P07 Cancer B – DB	+ SC Contact and Ultrasonic for near-field only	> R07 Cancer B – DB	
Scan		Biofeedback scans x 2		Edit P08 & R08 presets
x4	P08 Cancer C – DB	+ SC Contact and Ultrasonic for near-field only	> R08 Cancer C – DB	
x2	P09 Cancer Sweep (P) – JW	+ SC Contact and Ultrasonic for near-field only	> Spectrum Cancer Sweep – DB (SC off & disconnect)	

enough, you'd be handed a bottle or a bedpan.

3. Herxing: this should not be a problem because one of your generators will be running a detox program non-stop remotely. In the event that it does happen, load and run the *RX Herxheimer - DB* preset remotely, then continue your plasma treatment. If your herx is bad, run the *PX Herxheimer - DB* version in place of the plasma preset you

were running. Keep a notebook by your PC and record the *Step* number you'd reached (below the *Frequency Column*), then complete the session next day, or next night.

B. Contact Plus night:

1. Placement: no rearrangement of furniture is required, but it's a good idea to keep the PC within reach of your bed with its screen set to sleep after three minutes. Attach one TENS pad to your left foot just below the outside ankle, and another to the back of your right hand. You may wish to use a woollen or silk bed-sock and a glove to keep the pads secure – not leather or latex.

Contact Plus 4 users who own a Spooky Coil can also use one generator with the coil taped to the skin, or beneath the body, instead of using a Spooky Remote. If you do this, you **must** ensure that the “BN” side of the coil is next to the skin.


2. Bathroom needs: when you wake, remember you're connected by wires to a generator which can be damaged if you inadvertently drag it off your bedside table. First, click the *Pause* button, then peel off both pads. When you return, reapply the pads, get into bed, and click *Pause* again. Please see the section on this topic above for an alternative strategy.

3. Herxing: this should not be a problem because one of your remote generators will be running a detox program non-stop. If it does happen, Contact Plus 4 users can load and run the *RX Herxheimer - DB* preset on one of their remote generators, then continue with treatment if possible. If not, run the *CX Herxheimer - DB* preset on the contact machine instead of the one you were running. Contact Plus 2 users will have to load the *CX Herxheimer - DB* preset on the contact machine in place of the preset that caused the herx. Keep a notebook and pen handy so you can note down the Step number you'd reached.

4. Voltage: most of the presets contain high-frequency programs which won't be a problem. But some contain low frequencies which may. All of these have damping and ramping set. If they're still too much, connect to the Colloidal Silver output.


C. Plasma Plus & Contact Plus day:

1. Treatment timings: all presets except for Remote start with a 60-second pause to allow you to get ready after you click *Start*. Between each program is a 10-second pause. In the first five presets, each program after a pause has a colon and two *Step* numbers after its name in the *Notes* to help you identify where pauses are located. If you intend to break up daytime treatments, it's best to do so after a pause. You can set Spooky² to sound an alert at each one. You enable this in the *Global* and *Settings* tabs:




Tick this box for use during the day. There's one more step before we're done.

Spooky² allows audio alerts for each individual generator. So for every one you wish to use this feature on, you must first click the *Control* tab, open a *Generator Control* panel, then click the *Settings* tab, go to the *Audio Options* pane top right, and tick *Notify when Zero Hz*.

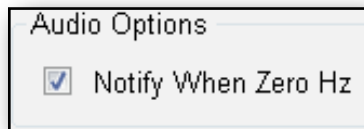


To save this setting for each of your presets, click the *Presets* tab, then click the *Save* button.



Untick this box for use while sleeping. You don't want any alerts to sound while you sleep.

So it's a good idea to check the *Audio Options* pane in the *Settings* tab for each of your generators to make sure that the *Notify when Zero Hz* checkbox is unticked. Go to the *Control* tab, open a *Generator Control* panel, then click the *Settings* tab to check.

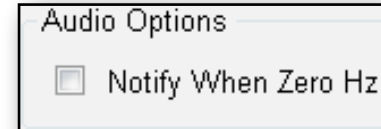

To save this setting for each of your presets, click the *Presets* tab, then click the *Save* button.

2. General: every time you need to visit the bathroom, answer the phone, cook or eat, you will have to click *Pause* in Spooky², and remove TENS pads if using Contact Plus. When you're ready to resume, reapply the pads and click *Pause* again. If your absence will be fairly long, you can also switch off Spooky Central/Plasma if using it – but don't switch off generators or quit Spooky².

In either plan, if you don't get enough time during the day to complete the preset, you can stop the generator, then use the *Resume* button next day to restart where you left off. Leave your remote generators running their current presets until you finish that contact or plasma preset.

Do not turn off any generators unless you're going to turn them all off. Switching off individual generators in a rig will cause Spooky² to report communications errors at a prodigious rate which can affect the smooth operation of

the other generators. Leaving unused generators switched on doesn't use very much electricity - less than a night-light. However, Spooky Central/Plasma can safely be switched off without affecting the rest of the rig.

Plasma, PEMF, and Ultrasonic are all safe to use on the head and neck. However, both SC Contact Mode and standard Contact Mode should not be used in these areas. Place a TENS pad on each shoulder close to the base of

Run	Spooky Scalar Treatment (day or night as desired)	Remarks	Generator 1 (if not running Spooky Scalar)	Generator 2
Scan		Biofeedback scans x 2		Edit S06 & R06 presets
x4	S06 Cancer A – DB		> R06 Cancer A – DB	ALL Detox (R) – DB (Run non-stop till protocol is done)
Scan		Biofeedback scans x 2		Edit S07 & R07 presets
x4	S07 Cancer B – DB		> R07 Cancer B – DB	
Scan		Biofeedback scans x 2		Edit S08 & R08 presets
x4	S08 Cancer C – DB		> R08 Cancer C – DB	
x2	S09 Cancer Sweep (P) – JW		> Spectrum Cancer Sweep – DB (SS off & disconnect)	

the neck instead.

SC Contact Mode, standard Contact Mode, or PEMF should **never** be used by people with pacemakers or electronic implants.

How I Use Spooky Central:

I use Plasma Plus while sleeping. Plasma tubes emit two fields – near-field and far-field. The first extends about six inches in all directions from the tube, and it's very powerful. After six inches, it becomes far-field. This is not as powerful as near-field, although it's far more effective than standard Contact Mode. This means that my feet are not receiving the same plasma energy intensity as my trunk.

Adding SC Contact Mode and Ultrasonic solves this problem. And since SC Contact Mode delivers the PEMF signal as

well, I can leave any localised PEMF treatments I may need for daytime administration if necessary.

Because I use Spooky Central for near-field treatment while sleeping, I have a choice in how I use its generator during the day: because Spooky Central only requires 5 volts, and no Remote preset uses more than 10 volts, I can safely leave a white BN Remote permanently connected to the Boost BN socket, then turn off Spooky Central, load the remote version of the preset, and run it until the next plasma session. This allows me to leave my home and go anywhere.

OR: I can simply run Spooky Central's plasma tube on its own during the day, using the same preset. As long as I remain within my home, I receive far-field treatment which will vary in power depending on how near I am to the tube. I've killed mould on fruit placed 10 feet away from the tube in less than 16 hours, so this is powerful stuff.

And because plasma tubes also emit scalar energy, I place a tape containing my fingernail beneath the tube. Doing this allows me to leave my home and still receive remote treatment *from the plasma tube*.

This is the method we recommend.

In emergency situations where time is of the essence, you can skip Phase I–Terrain and proceed directly to Phase II–Target if you must. However, doing Phase I is enormously beneficial because you will remove many burdens on your immune system, and prepare your eliminatory system for the war that is to come. Remember that your immune system is your most powerful weapon.

Before You Start

- You must actively assist in the detox process by drinking at least three litres of pure water daily, half of it before noon. This will help flush out the kidneys, and increase electrical conductivity in the body, especially if you add a tiny pinch of sea salt or Himalayan Pink Salt to your daily water ration.
- In any battle, the more weapons that are brought to bear on the enemy, the more likely it is that victory will be achieved. Don't neglect other modalities, especially diet, naturopathic, homeopathic, and herbal.
- The work of Dr. Bradley Nelson and others has clearly demonstrated that emotional trauma lies at the root of almost every cancer. His ground-breaking book "The Emotion Code" demonstrates a way to resolve this, and a PDF of this is free [here](#).

Schedule					
Run From	Midnight	▼	to	Midnight	▼
	<input type="checkbox"/> Stop When Complete				
Run For	48	Hours			
Start In	0	Days	0	Hours	0 Minutes

settings.

Some presets in the timetables say "*Run For* = xx hours." To program this, click the *Settings* tab, then enter the number into the *Run For* field as shown left (highlighted red). Save the preset if desired. This control overrides all *Repeat*

Plasma Plus



This requires a Spooky Central/Plasma Essential Kit.

Back in the 1930s, Dr. Royal Raymond Rife cured 14 terminal cancers and two terminal TBs using plasma.

The machine he used was very different to the crippled units that came later.

Today, Spooky Central/Plasma is the only machine on Earth that can replicate – and even vastly improve upon – his method and results.

Plasma: frequencies of up to 3.5MHz can be transmitted – the next best available today is 0.6MHz. Note that the fundamental frequency of the cancer BX

virus is 1.60745MHz. Most effective

when the tube is positioned close to the body or organ – the powerhouse near-field extends six inches in all directions from the tube, then drops off to become far-field (still very powerful, but much less so), so near-field use is recommended. Plasma can be wide-spectrum or directly targeted.

SC Contact: this is a form of Contact Mode unique to Spooky Central. It's wide-spectrum and non-targetable, so it should be used with plasma for maximum effect. It delivers a 320 volt energy spike at the end of each PEMF pulse. This reverses the electrical charge of every cell in the body for half of one-millionth of a second, opening its “doors” so that lethal plasma frequencies gain direct access. This is called reversible cell electroporation, and for

cancer cells and pathogens, it means execution. Can also be used with the plasma tube disconnected (**see warning on page 2 of your SC User's Guide**).

Ultrasonic: sound is frequency, and sound conducts far better in water and solids than it does in air. Since the human body is about 70% water and 30% solids, this means that Ultrasonic can hit just about every cell in the body. Place the metal diaphragm of the wand against bare skin. It can be wide-spectrum using linear sweeps (not Spectrum sweeps), or directly targeted. Ultrasonic can be used together with plasma, or with the tube disconnected.

PEMF: Pulsed ElectroMagnetic Field. Use a Spooky PEMF Coil where the location of the cancer is known – place it directly over the site, or as close to it as possible. Produces a wide-spectrum of high frequencies, each with a 29 volt energy spike. This is non-targetable, so it's best used in conjunction with plasma. It may also, however, be used with the plasma tube disconnected. PEMF is also particularly useful and effective for localised pain.

Spooky Central's four subsystems may be used together in any combination.

Spooky² Essential Kit

This comes with two Spooky²-XM generators, two Spooky Boost 2.0 signal processors, two white Bio North Spooky Remotes (plus a black Magnetic North model - not used here), the Spooky Pulse biofeedback detection system, plus a bunch of other stuff.

Generator 1: this is used to provide frequency input for Spooky Central/Plasma. Connect a Spooky Boost 2.0 to the generator first, then, using the two Dick ring BNC cables provided, connect its Out 1 to Spooky Central/Plasma's Input, and its Out 2 to Modulation. We strongly recommend marking the Out 1 > Input cable with tape to avoid inadvertently reversing these connections.


Generator 2: this is used to provide non-stop Remote Mode detox and support, also using a fingernail clipping as a DNA sample. Connect a Spooky Boost 2.0/3.0 first, then a Bio North (white v1.1) Remote, or a v2.0 Remote to its BN port. **Do NOT use a black MN v1.1 Remote.**

Spooky Pulse: after you've completed the Phase I–Terrain section, you should do your two biofeedback scans in standard Contact Mode using a generator directly. This is what we recommend, but you can also do the scan in Remote Mode if necessary.

GeneratorX: alternatively, if you have GeneratorX, you can do your biofeedback scans using GeneratorX.

Sample Digitizer: alternatively, if you have GeneratorX and Sample Digitizer, you can do your biofeedback scans using the Sample Digitizer biofeedback scan.

You cannot use Spooky Central/Plasma to supply the frequency sweep because the very powerful energy from the plasma tube will prevent Spooky Pulse from accurately reading your heart rate.

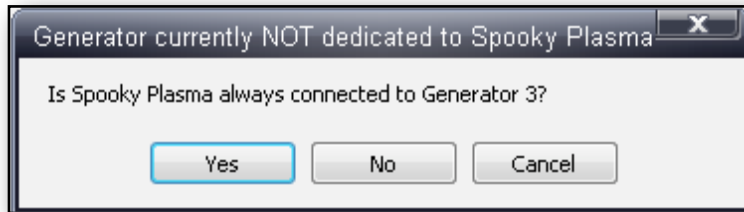

Before we start, we must first make a vital setting. To run any SC plasma preset, you must first right click the *Generator Button* to which Spooky Central/Plasma is connected. The dialog on left will appear. Click *Yes*. This ensures you cannot damage Spooky Central/Plasma with incorrect settings.

To use Remote or Contact Mode, do this again, and click *No*. **IMPORTANT:** do **NOT** tick *Remove Duplicate Frequencies*.

Phase I – Terrain

Run	SC Near-field/Far-field (day or night as desired)	Remarks	Generator 1 (if not running SC far-field)	Generator 2
x2	P01 Metals & Chemicals – DB	+ SC Contact and Ultrasonic for near-field only	> R01 Metals & Chemicals – DB	R01 Metals & Chemicals – DB (Run For = 48 hours)
x2	P02 System Detox – DB	+ SC Contact and Ultrasonic for near-field only	> R02 System Detox – DB	R02 System Detox – DB (Run For = 48 hours)
x2	P03 Liver & Kidneys – DB	+ SC Contact and Ultrasonic for near-field only	> R03 Liver & Kidneys – DB	R03 Liver & Kidneys – DB (Run For = 48 hours)
x2	P04 Blood & Lymph – DB	+ SC Contact and Ultrasonic for near-field only	> R04 Blood & Lymph – DB	R04 Blood & Lymph – DB (Run For = 48 hours)
x2	P05 Immunomodulators – DB	+ SC Contact and Ultrasonic for near-field only	> R05 Immunomodulators – DB	ALL Detox (R) – DB (Run For = 0, so runs non-stop)

Tables Key:

P = Spooky Central/Plasma Plasma preset. **Red** = standard Contact Mode scanning sessions, or **R** = Spooky²-XM generator Remote preset. important notes and directions.

> = switch from far-field to Remote Mode if desired.

This concludes Phase I–Terrain. The Spooky Central/Plasma Presets above are all pretty long, and so they lend themselves to sleep-time treatment. However, if you prefer to do your plasma treatments during the day, go right ahead. Start in the morning and go for as long as you can. When you feel you’ve done enough for the time being, open Spooky Central/Plasma’s *Generator Control Panel* and take a note of the *Step* number you’ve reached (below the *Frequency Column*).

Now you have a choice. You can simply place a fingernail specimen tape beneath the plasma tube, then get up and walk away, leaving Spooky Central/Plasma to continue transmitting in far-field plus remote. When it’s time for more near-field plasma, click *Pause*, then enter the *Step* number you noted, and hit *Pause* again.

If you don’t want to use Spooky Central/Plasma far-field, you can click *Stop*, switch off Spooky Central/Plasma, then load the corresponding Remote preset and use a Bio North Remote until your next plasma session. When that time comes, click *Stop*, reload the Plasma preset, switch Spooky Central/Plasma on, then click *Start*, followed by

Pause. Enter the *Step* number you noted earlier, then hit *Pause* again to resume where you left off in near-field. In this way, you can split a long session into two or three shorter sessions. In all cases, however, you should only do what your body will tolerate, then stop until you feel able to continue. At such times, if you are able, you should try to do one session using Ultrasonic only each day. You should also try to leave Spooky Central/Plasma far-field and Remote programs running until you've completed that particular Spooky Central/Plasma preset in full near-field mode. If you can't manage it, don't worry too much – Dr. Rife treated his terminal cancer and TB subjects every third day.

Phase II – Target

First, do your two biofeedback scans back-to-back in the morning. Spooky Central/Plasma should be turned off, and only the generator that's being used for the scan should be running. Save both sets of scan results into your custom database and edit the programs into P06 Cancer A – DB. For instructions, see pages 3-14.

Now repeat Phase II–Target for as long as necessary. Use the healing presets when you need a break from killing cancer.

Scalar Plus



This requires Spooky² Scalar.

This version of the protocol is very similar to the Plasma version of the protocol, where the plasma presets are replaced by the scalar versions of the same programs.

The Spooky² Scalar is potentially the most useful in terms of receiving treatments, as the Spooky² Scalar

Spooky² Essential Kit

This comes with two Spooky²-XM generators, two Spooky Boost 2.0 signal processors, two white Bio North Spooky Remotes (plus a black Magnetic North model - not used here), the Spooky Pulse biofeedback detection system, plus a bunch of other stuff.

Generator 1: this is used to provide frequency input for Spooky Scalar. Connect Out 1 to Spooky Scalar's BNC Input.

Generator 2: this is used to provide non-stop Remote Mode detox and support, also using a fingernail clipping as a DNA sample. Connect a Spooky Boost 2.0/3.0 first, then a Bio North (white v1.1) Remote, or a v2.0 Remote to its BN port. **Do NOT use a black MN v1.1 Remote.**

Spooky Pulse: after you've completed the Phase I–Terrain section, you should do your two biofeedback scans in standard Contact Mode using a generator directly. This is what we recommend, but you can also do the scan in Remote Mode if necessary.

GeneratorX: alternatively, if you have GeneratorX, you can do your biofeedback scans using GeneratorX.

Sample Digitizer: alternatively, if you have GeneratorX and Sample Digitizer, you can do your biofeedback scans using the Sample Digitizer biofeedback scan.

You cannot use Spooky Central/Plasma to supply the frequency sweep because the very powerful energy from the plasma tube will prevent Spooky Pulse from accurately reading your heart rate.

To use Remote or Contact Mode, do this again, and click *No*.

IMPORTANT: do NOT tick *Remove Duplicate Frequencies*.

Phase I – Terrain

Run	Spooky Scalar Treatment (day or night as desired)	Generator 1 (if not running Spooky Scalar)	Generator 2
x2	S01 Metals & Chemicals – DB	> R01 Metals & Chemicals – DB	R01 Metals & Chemicals – DB (Run For = 48 hours)
x2	S02 System Detox – DB	> R02 System Detox – DB	R02 System Detox – DB (Run For = 48 hours)
x2	S03 Liver & Kidneys – DB	> R03 Liver & Kidneys – DB	R03 Liver & Kidneys – DB (Run For = 48 hours)
x2	S04 Blood & Lymph – DB	> R04 Blood & Lymph – DB	R04 Blood & Lymph – DB (Run For = 48 hours)
x2	S05 Immunomodulators – DB	> R05 Immunomodulators – DB	ALL Detox (R) – DB (Run For = 0, so runs non-stop)

Tables Key:

S = Spooky Scalar preset. **Red** = standard Contact Mode scanning sessions, or **R** = Spooky²-XM generator Remote preset. important notes and directions.

> = switch from far-field to Remote Mode if desired.

This concludes Phase I–Terrain. The Scalar Presets above are all pretty long, and so they lend themselves to sleep-time treatment. However, if you prefer to do your scalar treatments during the day, go right ahead. Start in the morning and go for as long as you can. When you feel you’ve done enough for the time being, open Spooky Scalar’s *Generator Control Panel* and take a note of the *Step* number you’ve reached (below the *Frequency Column*).

Phase II – Target

First, do your two biofeedback scans back-to-back in the morning. Spooky Scalar should be turned off, and only the generator that's being used for the scan should be running. Save both sets of scan results into your custom database and edit the programs into S06 Cancer A – DB. For instructions, see pages 3-14.

Now repeat Phase II–Target for as long as necessary. Use the healing presets when you need a break from killing cancer.

Contact Plus 4



The Contact Plus 4 method requires a Spooky² Advanced Kit. This comes with four Spooky²-XM generators, four Spooky Remote v1.1 Bio North scalar transmitters, two Spooky Cold Lasers, the Spooky Pulse biofeedback detection system, plus a bunch of other stuff.

It uses Contact Mode and Remote Mode. Contact Mode isn't any more powerful than Remote Mode, but it produces beneficial effects quicker.

It's been authoritatively estimated that to produce the same effectiveness as one Contact Mode session, you need to apply the same frequencies between 10-20 times in a row in Remote Mode. So a contact session Program that takes 30 minutes would take 5-10 hours to produce the same effect remotely.

NB: in all cases, please ensure that the Remove Duplicate Frequencies checkbox is UNTICKED.

A Word on Amplitude: because frequencies lower than about 10,000Hz can “bite” in Contact Mode, the *Reduce Amplitude* box is ticked to reduce the voltage/*Amplitude* for both killing and healing. However, if you use a Spooky Boost 2.0/3.0 signal processor, you can connect your electrodes to its Colloidal Silver output and untick this box

because the signal from this output has a lower Amplitude that's eminently suitable for use with hand cylinder or TENS pad electrodes.

If you use the older Spooky Boost cable, you may need to either tick this box, or enter a lower *Amplitude* (14-16 volts suggested).

Phase I – Terrain

Run	Generator 1 – Contact & Remote (day or night as desired)	Generator 2 – Remote/day, Coil/night if desired	Generator 3 – Remote (start 5 mins after Generator 2)	Generator 4 – Remote (start 5 mins after Generator 3)
x3	C01 Metals & Chemicals – DB > R01 Metals & Chemicals – DB	R01 Metals & Chemicals – DB OR M01 Metals & Chemicals (Coil) – DB	R01 Metals & Chemicals – DB (Run For = 72 hours)	R01 Metals & Chemicals – DB (Run For = 72 hours)
x3	C02 System Detox – DB > R02 System Detox – DB	R02 System Detox – DB OR M02 System Detox (Coil) – DB	R02 System Detox – DB (Run For = 72 hours)	R02 System Detox – DB (Run For = 72 hours)
x3	C03 Liver & Kidneys – DB > R03 Liver & Kidneys – DB	R03 Liver & Kidneys – DB OR M03 Liver & Kidneys (Coil) – DB	R03 Liver & Kidneys – DB (Run For = 72 hours)	R03 Liver & Kidneys – DB (Run For = 72 hours)
x3	C04 Blood & Lymph – DB > R04 Blood & Lymph – DB	R04 Blood & Lymph – DB OR M04 Blood & Lymph (Coil) – DB	R04 Blood & Lymph – DB (Run For = 72 hours)	R04 Blood & Lymph – DB (Run For = 72 hours)
x3	C05 Immunomodulators – DB > R05 Immunomodulators – DB	R05 Immunomodulators – DB OR M05 Immuno-modulators (Coil) – DB	R05 Immunomodulators – DB (Run For = 72 hours)	ALL Detox (R) – DB (Run For = 0 hours, so this runs non-stop till protocol is done)

This concludes Phase I–Terrain.

Phase II – Target

First do two back-to-back biofeedback scans in Contact Mode and save their results. For details, please see pages 5 and 6.

Run	Generator 1 – Contact & Remote (day or night as desired)	Generator 2 – Remote/day, Coil/night if desired	Generator 3 – Remote (start 5 mins after Generator 2)	Generator 4/Notes (run as directed)
Scan	Biofeedback scans x 2			Edit C06 & R06 presets
x6	C06 Cancer A – DB > R06 Cancer A – DB	> R06 Cancer A – DB OR M06 Cancer A (Coil) – DB	> R06 Cancer A – DB (Run For = 144 hours)	ALL Detox (R) – DB (Run non- stop till protocol is done)
Scan	Biofeedback scans x 2			Edit C07 & R07 presets
x6	C07 Cancer B – DB > R07 Cancer B – DB	> R07 Cancer B – DB OR M07 Cancer A (Coil) – DB	> R07 Cancer B – DB (Run For = 144 hours)	
Scan	Biofeedback scans x 2			Edit C08 & R08 presets
x6	C08 Cancer C – DB > R08 Cancer C – DB	> R08 Cancer C – DB OR M08 Cancer A (Coil) – DB	> R08 Cancer C – DB (Run For = 144 hours)	
x3	Overnight Contact Sweep (C) – DB > Spectrum Cancer Sweep (R) – DB	Spectrum Cancer Sweep (R) – DB OR Immune Support (Coil) – DB	> Spectrum Cancer Sweep – DB (Run For = 72 hours)	

Now repeat Phase II–Target for as long as necessary. Use the healing presets when you need a break from killing cancer.

Tables Key: C = Contact Mode preset. R = Remote Mode preset.

M = Spooky Coil preset

> (Blue) = switch from Contact to Remote **OR** Coil.

Red = biofeedback scanning sessions and important notes.

Contact Plus 2



The Contact Plus 2 method requires a Spooky² Essential Kit. This comes with two Spooky²-XM generators, two Spooky Remote v1.1 Bio North scalar transmitters, two Spooky Cold Lasers, the Spooky Pulse biofeedback detection system, plus a bunch of other goodies.

It uses Contact Mode and Remote Mode in exactly the same way as Contact Plus 4, except it is done to a different – and necessarily longer – schedule. Because it features two generators rather than four, more Contact Mode sessions are required.

Please see the Plasma Plus and Contact Plus 4 sections for extra information.

NB: in all cases, please ensure that the Remove Duplicate Frequencies checkbox is UNTICKED.

A Word on Amplitude: because frequencies lower than about 10,000Hz can “bite” in Contact Mode, the *Reduce Amplitude* box is ticked to reduce the voltage/**Amplitude** for both killing and healing. However, if you use a Spooky Boost 2.0/3.0 signal processor, you can connect your electrodes to its Colloidal Silver output and untick this box because the signal from this output has a lower Amplitude that’s eminently suitable for use with hand cylinder or TENS pad electrodes.

If you use the older Spooky Boost cable, you may need to either tick this box, or enter a lower **Amplitude** value (14-16 volts is suggested).

Phase I – Terrain

Run	Generator 1 – Contact & Remote (day or night as desired)	Generator 2 – Remote
x3	C01 Metals & Chemicals – DB > R01 Metals & Chemicals – DB	R01 Metals & Chemicals – DB (Run For = 72 hours)
x3	C02 System Detox – DB > R02 System Detox – DB	R02 System Detox – DB (Run For = 72 hours)
x3	C03 Liver & Kidneys – DB > R03 Liver & Kidneys – DB	R03 Liver & Kidneys – DB (Run For = 72 hours)
x3	C04 Blood & Lymph – DB > R04 Blood & Lymph – DB	R04 Blood & Lymph – DB (Run For = 72 hours)
x3	C05 Immunomodulators – DB > R05 Immunomodulators – DB	ALL Detox (R) – DB (Run For = 0 hours, so this runs non-stop till protocol is done)

This concludes Phase I–Terrain.

Phase II – Target

First do two back-to-back biofeedback scans in Contact Mode and save their results. For details, please see pages 5 and 6.

Run	Generator 1 – Contact & Remote (day or night as desired)	Generator 2 – Remote
Scan	Biofeedback scans x 2	Edit C06 & R06 presets
x7	C06 Cancer A – DB > R06 Cancer A – DB	ALL Detox (R) – DB (Run non-stop till protocol is done)
Scan	Biofeedback scans x 2	Edit C07 & R07 presets
x7	C07 Cancer B – DB > R07 Cancer B – DB	
Scan	Biofeedback scans x 2	Edit C08 & R08 presets
x7	C08 Cancer C – DB > R08 Cancer C – DB	
x4	Overnight Contact Sweep (C) – DB > Spectrum Cancer Sweep (R) – DB	

Now repeat Phase II–Target for as long as necessary. Use the healing presets when you need a break from killing cancer.

Tables Key:

C = Contact Mode preset. **R** = Remote Mode preset.

> (Blue) = switch from Contact to Remote Mode. **Red** = scanning sessions and important notes.

Extras:

A number of extra presets are included for each transmission mode. Here's what they do:

Preset	Aim
Healing A – DB	All modes. Addresses endocrine/hormonal system, DNA, organs, bones, ligaments, muscles, nerves, tissues (including scars), and overall physical healing. Delivers energy signatures of five healing herbs.
Healing B – DB	All modes. Addresses deficiencies of important vitamins and minerals.
Healing C – DB	All modes. Addresses collagen and skin toning, mental function, and emotions. Delivers the energy signatures of 17 essential oils aimed at physical, mental, and emotional issues.
Herxheimer – DB	All modes. A Jarisch-Herxheimer reaction is a reaction to toxins released by the die-off of large numbers of pathogens and cancer cells. Common symptoms are lower back pain, joint pain, severe headache, nausea, and sometimes diarrhoea. Running this preset will address it quickly.
Pain Overnight – DB	Plasma & Contact Modes. Dr. Hulda Clark found that almost all cancer pain was caused by infection with <i>Streptococcus pneumoniae</i> . This preset addresses this. Run detox remotely while using it.
Pain Long – DB	Remote Mode only. Dr. Hulda Clark found that almost all cancer pain was caused by infection with <i>Streptococcus pneumoniae</i> . This preset addresses this. Run detox remotely while using it.
Pain Short – DB	All modes. This is a short version of the overnight treatment that can be run during the day if required.

Use the first three presets above for a couple of days when you want to take a break from dealing with cancer, and the last four as required.

Protocol history

28 January 2020: Removed the 3 minute *3-Methylfentanyl MW* program. Also removed Laser presets.

22 September 2019: The Contact presets have been enhanced to have a dynamic carrier wave on Out 2. This means it is possible to use the High Power port of Spooky Boost with Contact treatments and have the treatment be bearable. The Plasma presets have been enhanced to use the shell preset *Spooky Plasma Entrainment and Healing (P) - JW* for low frequencies, while using *Spooky Plasma Advanced (P) - JW* for the high frequencies. The plasma presets will now often be chained presets to accomodate better the low and high frequencies.

16 January 2019: Added Cancer presets for Spooky Scalar and Spooky Laser. The Spooky Scalar and Laser may be used if you don't have Spooky Plasma.

1 July 2017: Graphics update. Plasma presets changed.

17 March 2017: Graphics-only update.

17 February 2017: Removed *Nagalase XTRA* from all *Immunomodulators* presets. Removed *Glyphosate XTRA* from all *Metals and Chemicals* presets. Our research now shows that the so-called Disintegrative Factor does not actually disintegrate anything. Rather, it converts open air frequencies so that they may be used in tissue. The effects of the substance may still be applied – not a good idea for these two.

30 December 2016: Added 15 new presets for Spooky Coil to *Contact Plus 4* timetable. These may be used instead of Remote Mode presets.

25 November 2016: Added two new programs to *Cancer A – DB* presets for all modes. These are *Cancer General XTRA*, and *Cancer Tumor Reduction XTRA*. Both contain frequencies to reduce tumours. Added three new presets to Extras to address pain issues.

The Spooky team wishes you Godspeed on your journey back to health.

September 2019