


a

Standard negative controls: Field DNA reads

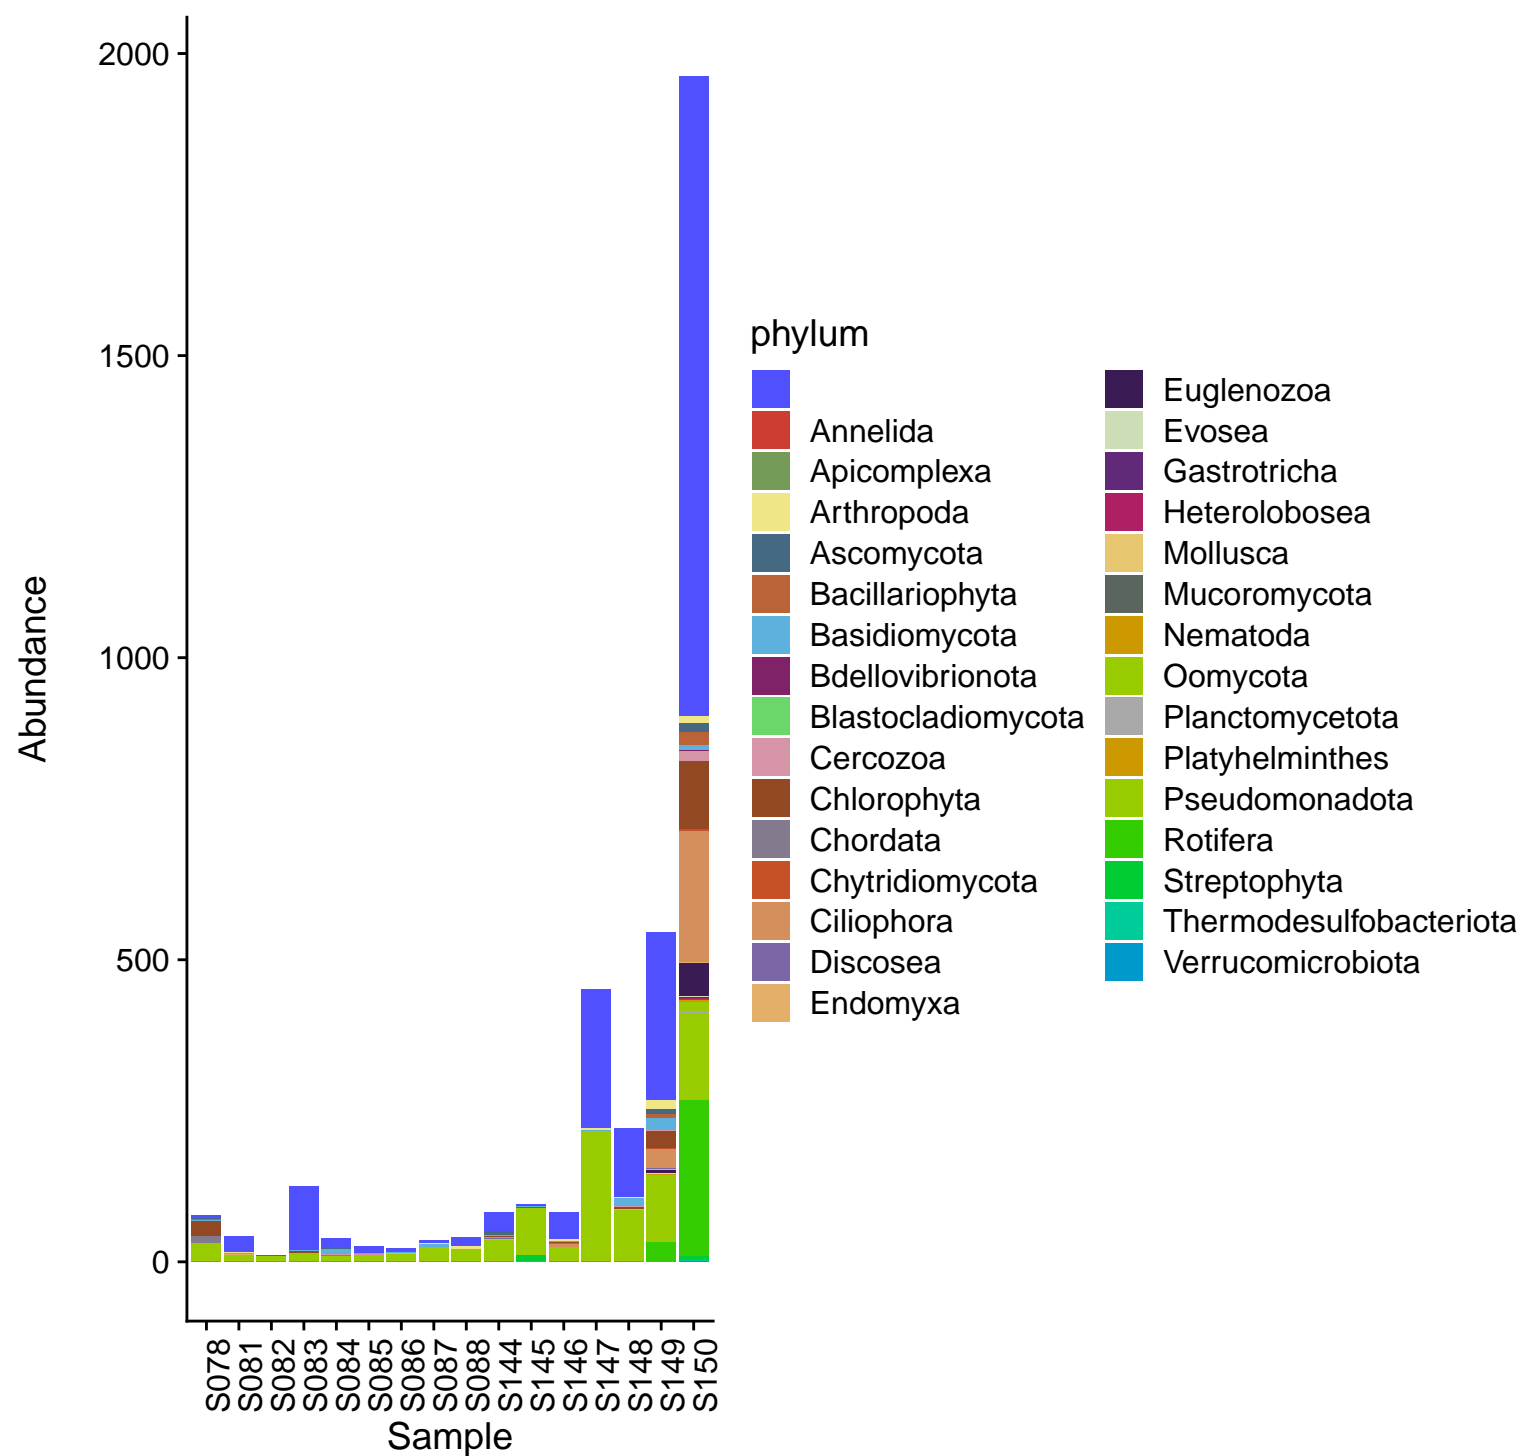

b

Standard negative controls: Standard DNA reads

